


Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...nt\2100 bioanalyzer\2100 expert\data\2023-11-01\AVT0072.xad

Created: 11/1/2023 2:33:50 PM  
Modified: 11/1/2023 3:20:40 PM

**Electrophoresis File Run Summary**

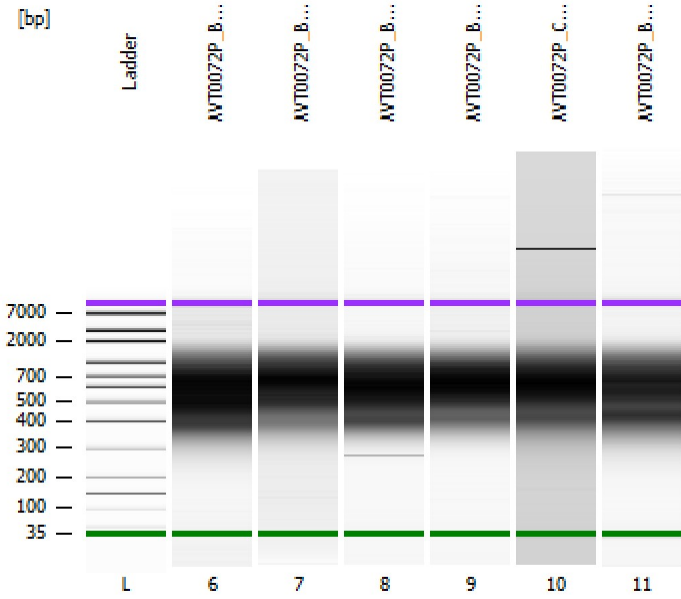

Instrument Information:

Instrument Name: DE34903152      Firmware: C.01.069  
Serial#: DE34903152      Type: G2938C

Assay Information:

Assay Origin Path: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy  
Assay Class: High Sensitivity DNA Assay  
Version: 1.03  
Assay Comments: Copyright © 2003-2010 Agilent Technologies




Chip Information:

Chip Lot #:  
Reagent Kit Lot #:  
Chip Comments:

AVT0072P\_B\_0.7X BC

AVT0072P\_B\_0.7X BC




AVT0072P\_B\_0.7X BC

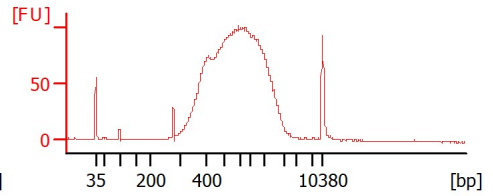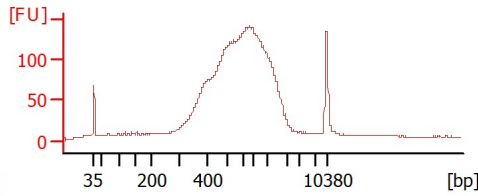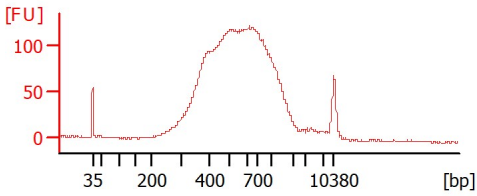

AVT0072P\_B\_0.7X BC

AVT0072P\_C (1:3)

AVT0072P\_B (1:2)

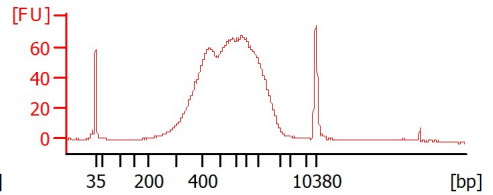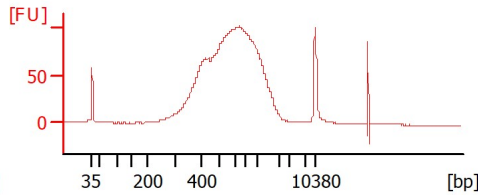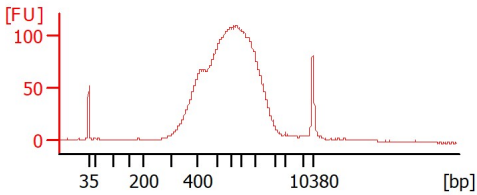

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...nt\2100 bioanalyzer\2100 expert\data\2023-11-01\AVT0072.xad

Created: 11/1/2023 2:33:50 PM  
 Modified: 11/1/2023 3:20:40 PM

**Electrophoresis File Run Summary (Chip Summary)**

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
AVT0072P_B_0.7X BC		<input type="checkbox"/>	✓			
AVT0072P_B_0.7X BC		<input type="checkbox"/>	✓			
AVT0072P_B_0.7X BC		<input type="checkbox"/>	✓			
AVT0072P_B_0.7X BC		<input type="checkbox"/>	✓			
AVT0072P_C (1:3)		<input type="checkbox"/>	✓			
AVT0072P_B (1:2)		<input type="checkbox"/>	✓			
Ladder		<input type="checkbox"/>	✓			

Chip Lot #

Reagent Kit Lot #

Chip Comments :

Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...nt\2100 bioanalyzer\2100 expert\data\2023-11-01\AVT0072.xad

Created: 11/1/2023 2:33:50 PM  
Modified: 11/1/2023 3:20:40 PM

## Electrophoresis Assay Details

### General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12  
Minimum Visible Range [s] : 32  
Maximum Visible Range [s] : 138  
Start Analysis Time Range [s] : 33  
End Analysis Time Range [s] : 137.5  
Ladder Concentration [pg/ $\mu$ l] : 1950  
Uses Standard Area for Ladder Fragments  
Lower Marker Concentration [pg/ $\mu$ l] : 125  
Upper Marker Concentration [pg/ $\mu$ l] : 75  
Used Upper Marker for Quantitation  
Standard Curve Fit is Point to Point  
Show Data Aligned to Lower and Upper Marker

### Integrator Settings

Integration Start Time [s] : 33.05  
Integration End Time [s] : 137  
Slope Threshold : 0.8  
Height Threshold [FU] : 5  
Area Threshold : 0.1  
Width Threshold [s] : 0.6  
Baseline Plateau [s] : 0.5

### Filter Settings

Filter Width [s] : 0.5  
Polynomial Order : 4


### Ladder

Ladder Peak	Size	Area
1	35	160
2	50	210
3	100	208
4	150	221
5	200	242
6	300	270
7	400	305
8	500	306
9	600	336
10	700	321
11	1000	366
12	2000	413
13	3000	411
14	7000	400
15	10380	214

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...nt\2100 bioanalyzer\2100 expert\data\2023-11-01\AVT0072.xad

Created: 11/1/2023 2:33:50 PM  
 Modified: 11/1/2023 3:20:40 PM

**Electropherogram Summary**

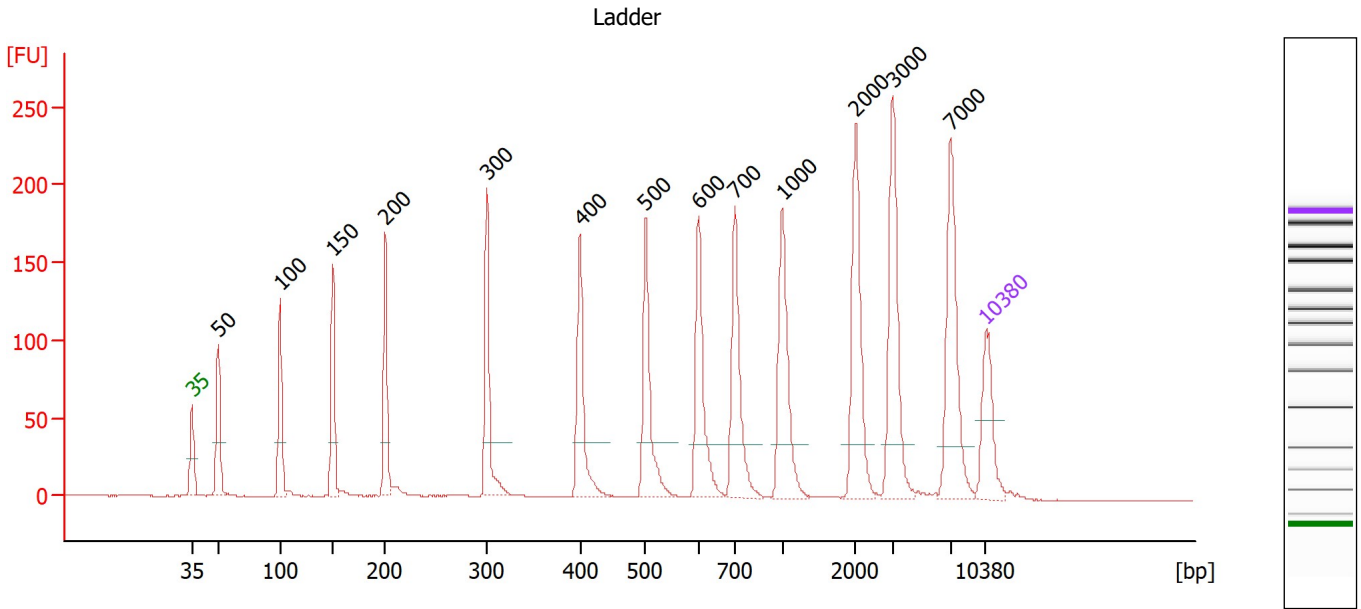

**Overall Results for Ladder**

Noise: 0.1


**Peak table for Ladder**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	50	150.00	4,545.5	Ladder Peak
3	100	150.00	2,272.7	Ladder Peak
4	150	150.00	1,515.2	Ladder Peak
5	200	150.00	1,136.4	Ladder Peak
6	300	150.00	757.6	Ladder Peak
7	400	150.00	568.2	Ladder Peak
8	500	150.00	454.5	Ladder Peak
9	600	150.00	378.8	Ladder Peak
10	700	150.00	324.7	Ladder Peak
11	1,000	150.00	227.3	Ladder Peak
12	2,000	150.00	113.6	Ladder Peak
13	3,000	150.00	75.8	Ladder Peak
14	7,000	150.00	32.5	Ladder Peak
15	10,380	75.00	10.9	Upper Marker

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...nt\2100 bioanalyzer\2100 expert\data\2023-11-01\AVT0072.xad

Created: 11/1/2023 2:33:50 PM  
 Modified: 11/1/2023 3:20:40 PM

**Electropherogram Summary Continued ...**

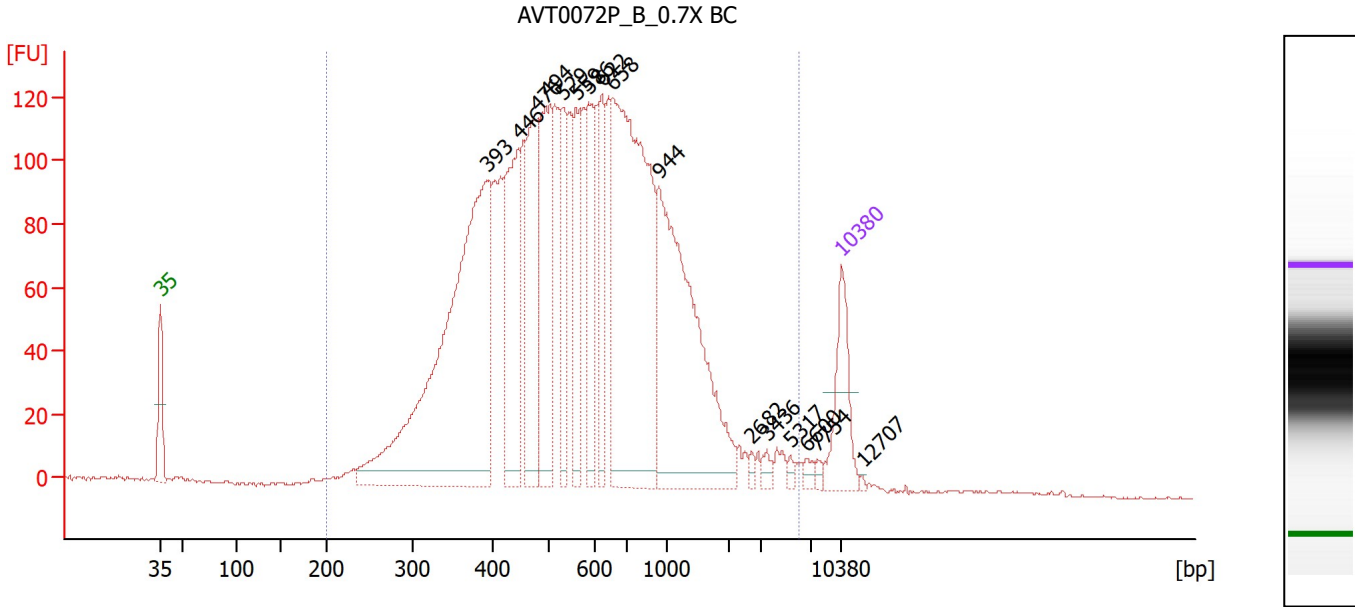

**Overall Results for sample 6 : AVT0072P B 0.7X BC**

Number of peaks found: 16                      Corr. Area 1: 3,421.4  
 Noise: 0.4

**Peak table for sample 6 : AVT0072P B 0.7X BC**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	393	774.39	2,987.6	
3	446	223.54	760.2	
4	476	204.01	649.5	
5	494	217.81	668.2	
6	529	104.24	298.8	
7	559	122.13	331.1	
8	586	126.89	328.3	
9	622	96.44	235.0	
10	658	568.42	1,309.3	
11	944	427.40	686.2	
12	2,682	5.93	3.4	
13	3,436	9.74	4.3	
14	5,317	6.14	1.7	
15	6,600	8.19	1.9	
16	7,754	4.62	0.9	
17	10,380	75.00	10.9	Upper Marker
18	12,707	0.00	0.0	


**Region table for sample 6 : AVT0072P B 0.7X BC**

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	5,962	3,421.4	99	716	81.2	3,584.00	10,578.3	Blue

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...nt\2100 bioanalyzer\2100 expert\data\2023-11-01\AVT0072.xad

Created: 11/1/2023 2:33:50 PM  
 Modified: 11/1/2023 3:20:40 PM

**Electropherogram Summary Continued ...**

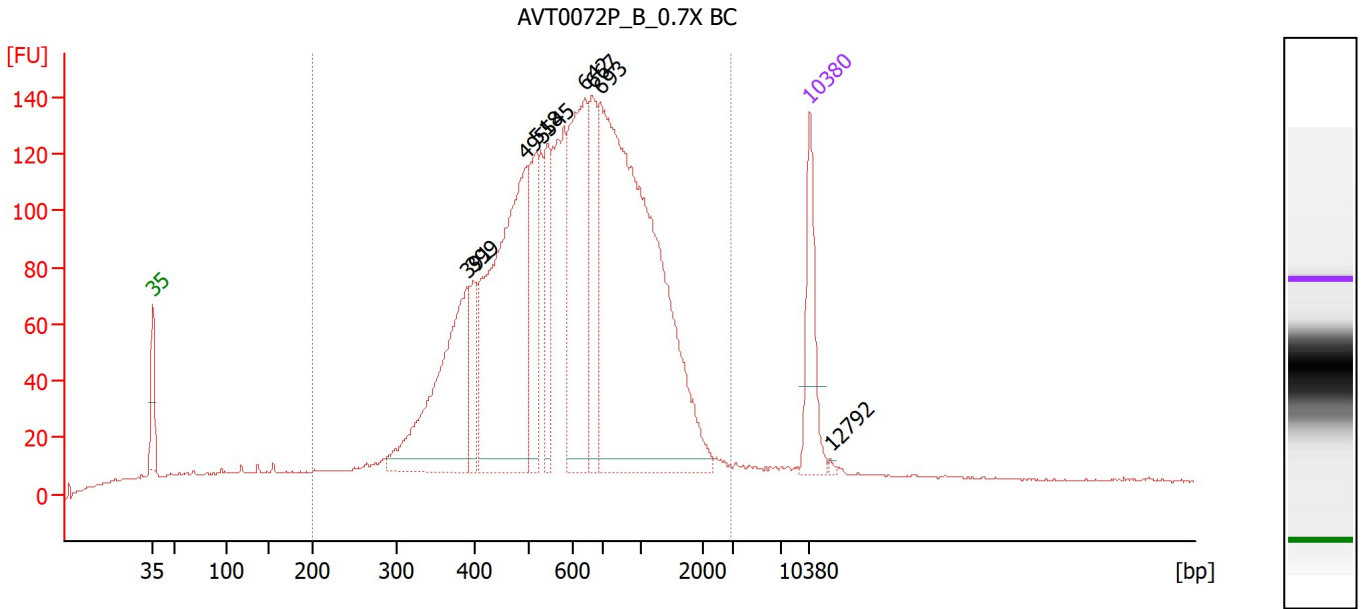

**Overall Results for sample 7 : AVT0072P B 0.7X BC**

Number of peaks found: 9                      Corr. Area 1: 3,217.8  
 Noise: 0.3

**Peak table for sample 7 : AVT0072P B 0.7X BC**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	391	293.79	1,138.2	
3	399	62.48	237.0	
4	495	456.16	1,395.4	
5	518	124.48	363.8	
6	545	80.40	223.5	
7	642	248.53	586.9	
8	667	119.03	270.6	
9	693	814.27	1,779.9	
10	10,380	75.00	10.9	Upper Marker
11	12,792	0.00	0.0	


**Region table for sample 7 : AVT0072P B 0.7X BC**

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	2,942	3,217.8	90	706	54.2	2,678.01	7,565.8	Blue

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...nt\2100 bioanalyzer\2100 expert\data\2023-11-01\AVT0072.xad

Created: 11/1/2023 2:33:50 PM  
 Modified: 11/1/2023 3:20:40 PM

**Electropherogram Summary Continued ...**

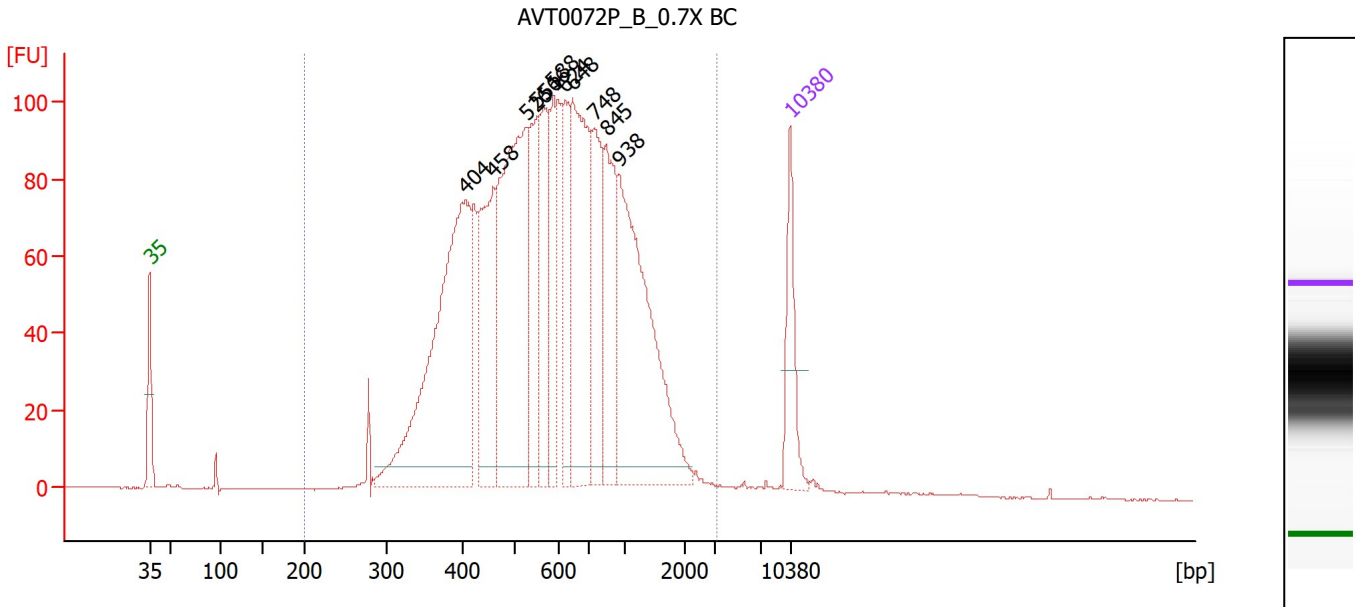

**Overall Results for sample 8 : AVT0072P B 0.7X BC**

Number of peaks found: 11                      Corr. Area 1: 2,442.9  
 Noise: 0.1

**Peak table for sample 8 : AVT0072P B 0.7X BC**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	404	578.86	2,169.6	
3	458	224.20	742.3	
4	526	446.42	1,286.1	
5	551	164.33	452.1	
6	566	142.38	381.4	
7	588	101.39	261.3	
8	624	107.79	261.7	
9	648	282.98	661.9	
10	748	165.45	335.2	
11	845	152.23	272.9	
12	938	383.80	620.0	
13	10,380	75.00	10.9	Upper Marker


**Region table for sample 8 : AVT0072P B 0.7X BC**

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	3,184	2,442.9	98	679	51.2	3,087.00	8,632.6	Blue

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...nt\2100 bioanalyzer\2100 expert\data\2023-11-01\AVT0072.xad

Created: 11/1/2023 2:33:50 PM  
 Modified: 11/1/2023 3:20:40 PM

**Electropherogram Summary Continued ...**

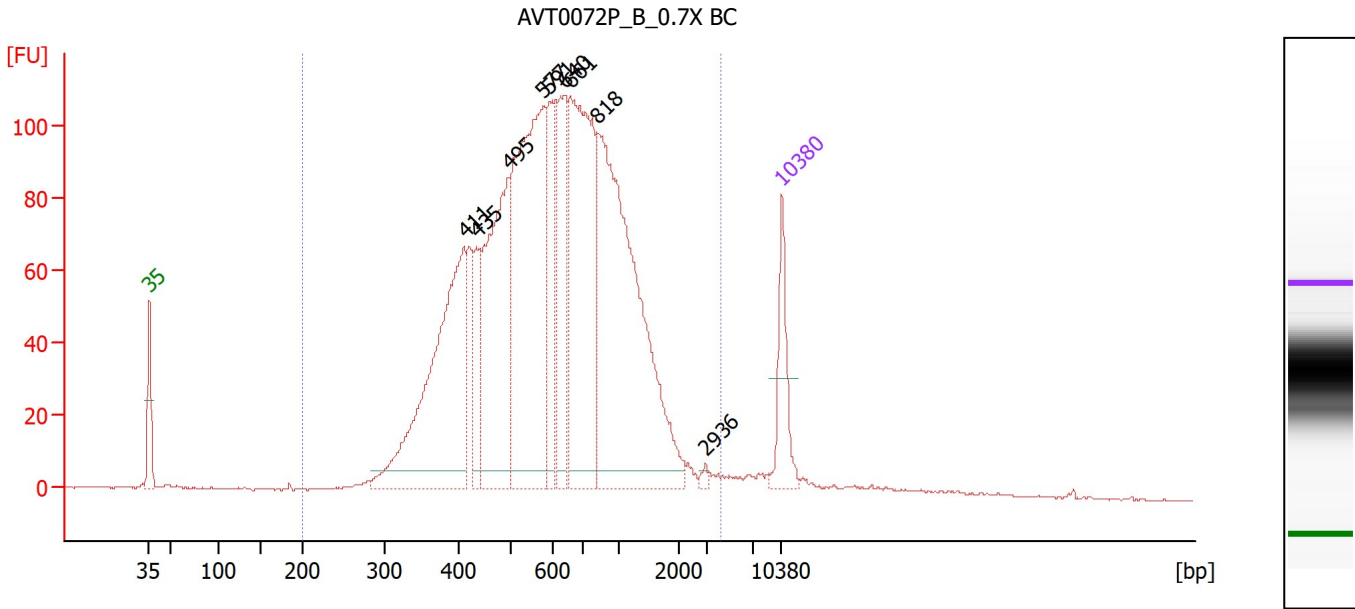

**Overall Results for sample 9 : AVT0072P B 0.7X BC**

Number of peaks found: 9                      Corr. Area 1: 2,437.2  
 Noise: 0.2

**Peak table for sample 9 : AVT0072P B 0.7X BC**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	411	512.03	1,888.7	
3	435	93.48	325.4	
4	495	391.58	1,197.6	
5	577	563.04	1,478.0	
6	591	152.95	392.1	
7	640	189.76	449.1	
8	661	453.75	1,040.8	
9	818	694.85	1,286.9	
10	2,936	5.85	3.0	
11	10,380	75.00	10.9	Upper Marker

**Region table for sample 9 : AVT0072P B 0.7X BC**


From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	4,184	2,437.2	97	718	56.9	3,273.47	8,818.6	Blue



Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...nt\2100 bioanalyzer\2100 expert\data\2023-11-01\AVT0072.xad

Created: 11/1/2023 2:33:50 PM  
 Modified: 11/1/2023 3:20:40 PM

**Electropherogram Summary Continued ...**

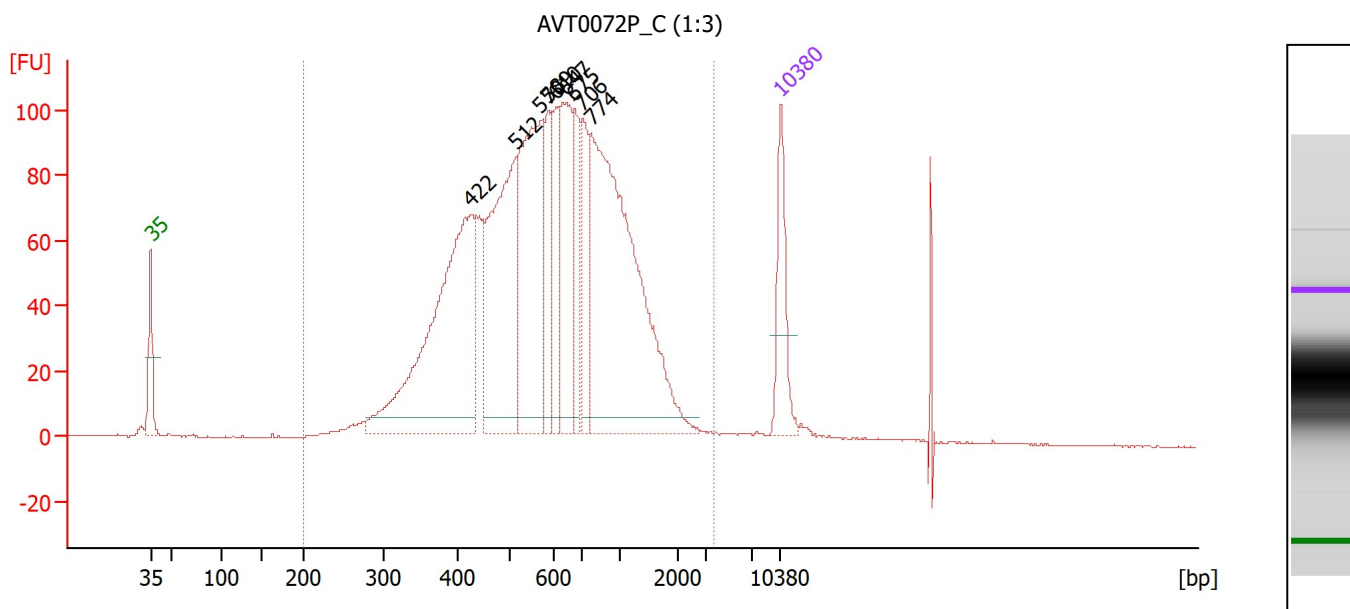

**Overall Results for sample 10 : AVT0072P\_C (1:3)**

Number of peaks found: 9                      Corr. Area 1: 2,355.0  
 Noise: 0.2

**Peak table for sample 10 : AVT0072P\_C (1:3)**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	422	512.75	1,840.9	
3	512	333.35	985.8	
4	570	324.83	863.1	
5	589	84.16	216.4	
6	610	84.42	209.7	
7	647	171.30	401.2	
8	675	90.10	202.3	
9	706	86.67	186.1	
10	774	567.37	1,110.0	
11	10,380	75.00	10.9	Upper Marker


**Region table for sample 10 : AVT0072P\_C (1:3)**

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	3,631	2,355.0	97	693	53.2	2,480.79	6,919.0	Blue

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...nt\2100 bioanalyzer\2100 expert\data\2023-11-01\AVT0072.xad

Created: 11/1/2023 2:33:50 PM  
 Modified: 11/1/2023 3:20:40 PM

**Electropherogram Summary Continued ...**

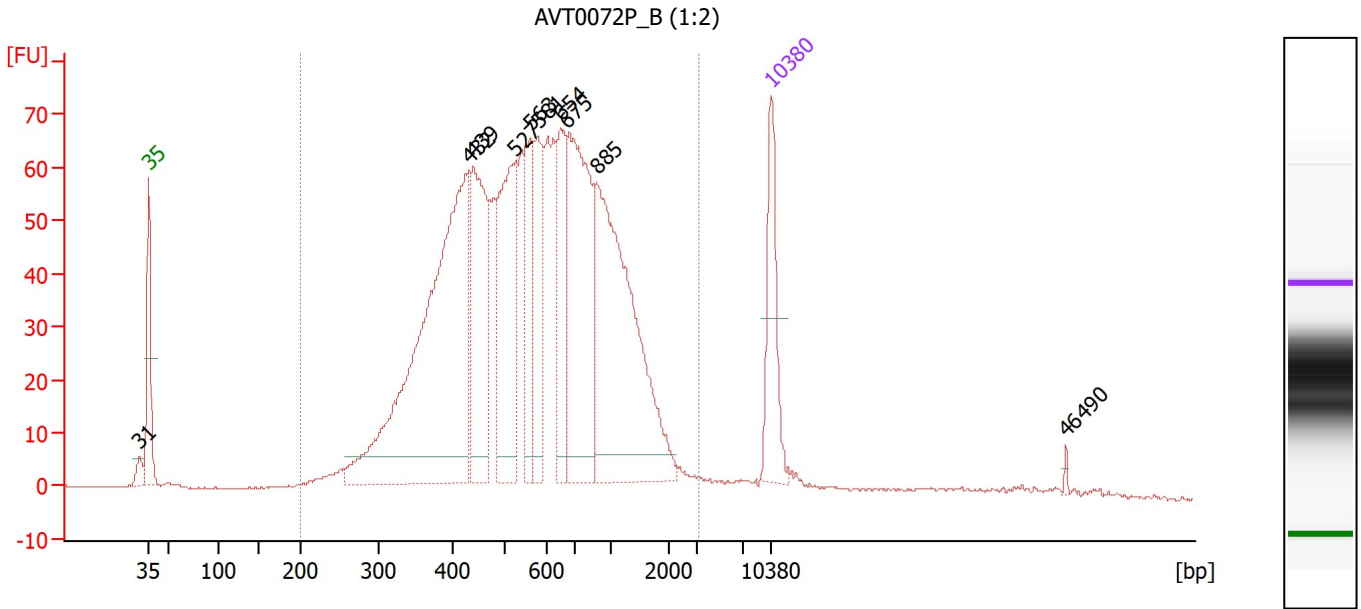

**Overall Results for sample 11 : AVT0072P B (1:2)**

Number of peaks found: 10      Corr. Area 1: 1,744.2  
 Noise: 0.1

**Peak table for sample 11 : AVT0072P B (1:2)**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	31	0.00	0.0	
2	35	125.00	5,411.3	Lower Marker
3	432	585.13	2,052.4	
4	439	190.91	658.6	
5	527	198.03	569.1	
6	563	93.31	251.1	
7	581	91.86	239.6	
8	654	102.71	237.8	
9	675	258.86	581.2	
10	885	354.75	607.2	
11	10,380	75.00	10.9	Upper Marker
12	46,490	0.00	0.0	


**Region table for sample 11 : AVT0072P B (1:2)**

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	3,122	1,744.2	96	673	54.9	2,316.00	6,771.6	Blue

Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...nt\2100 bioanalyzer\2100 expert\data\2023-11-01\AVT0072.xad

Created: 11/1/2023 2:33:50 PM  
Modified: 11/1/2023 3:20:40 PM

**Gel Image**

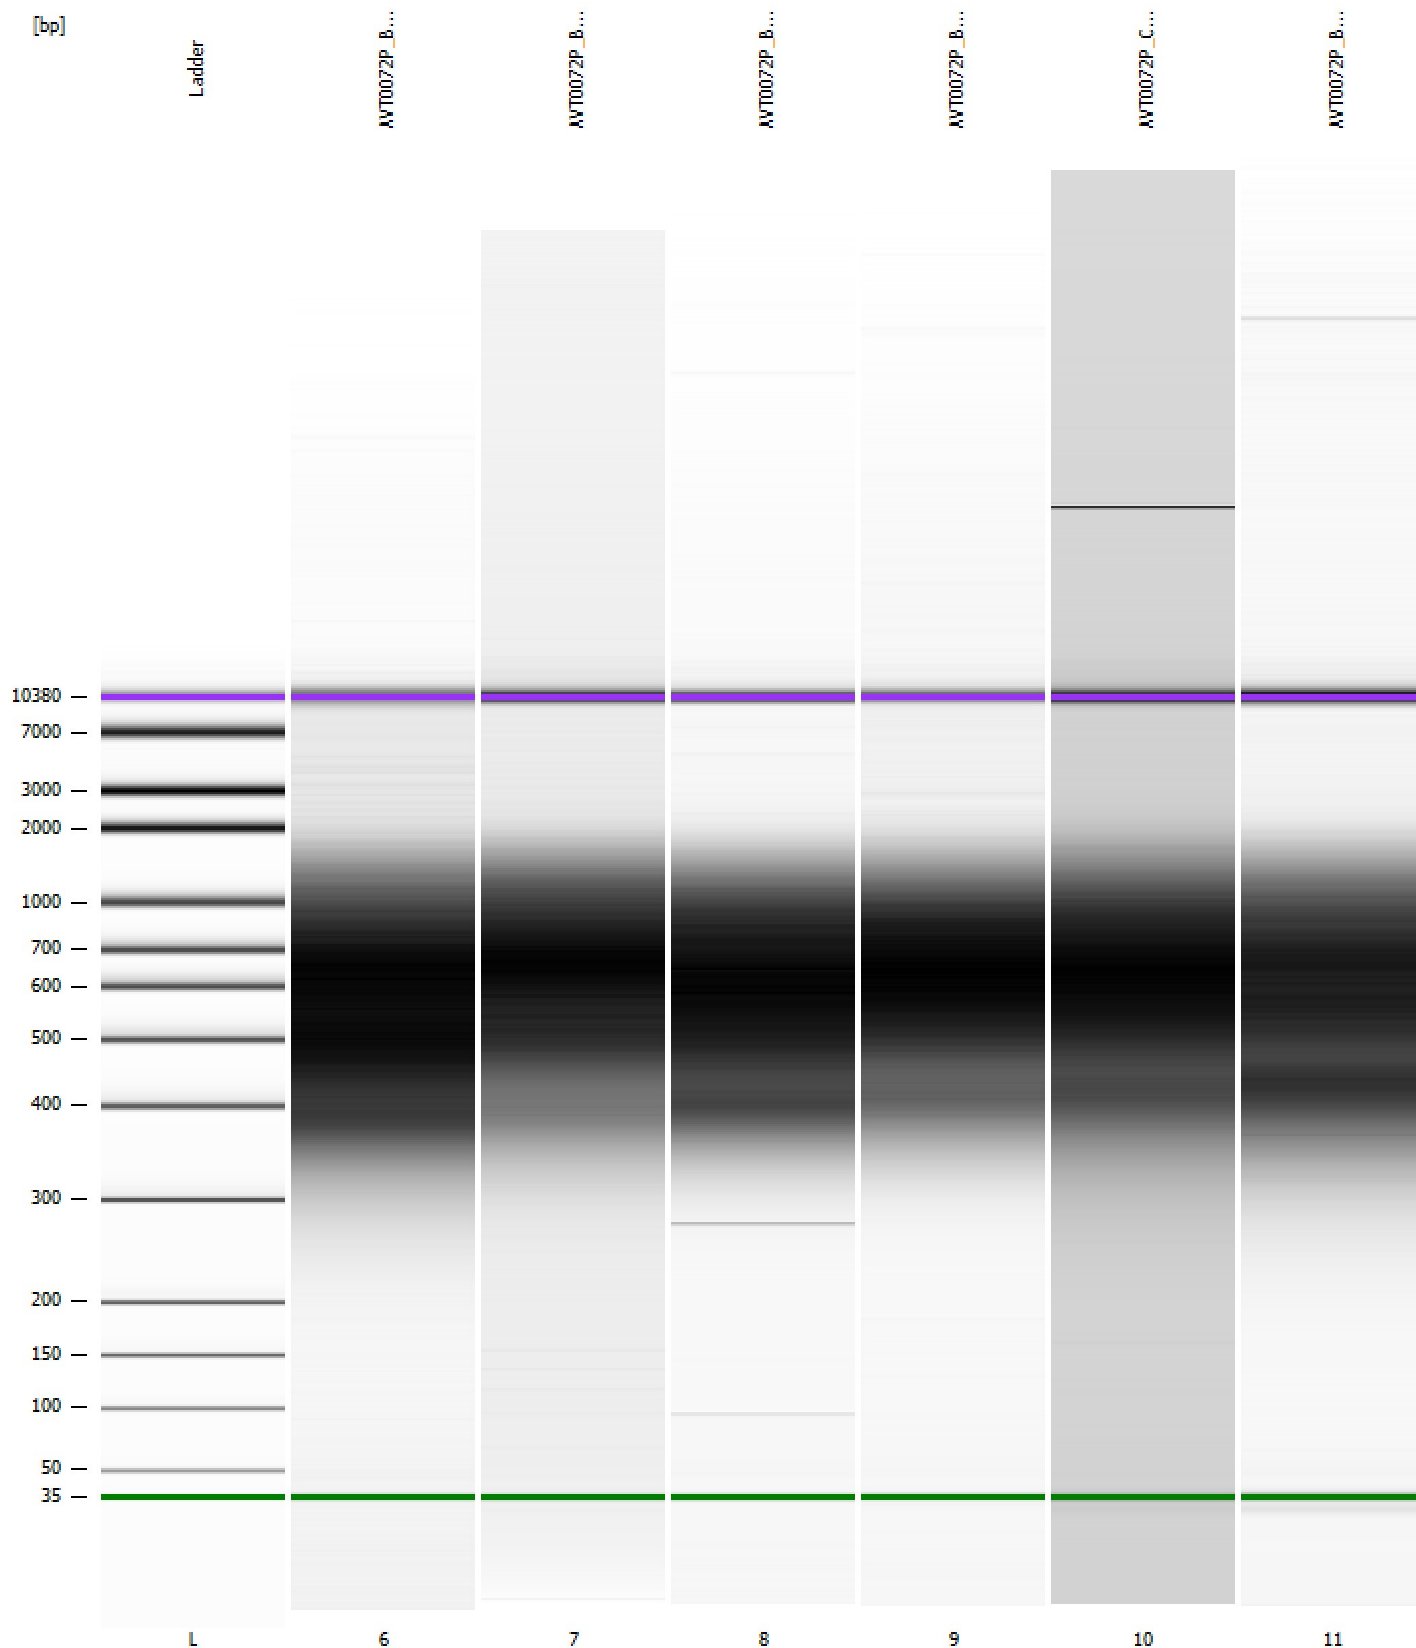


Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...nt\2100 bioanalyzer\2100 expert\data\2023-11-01\AVT0072.xad

Created: 11/1/2023 2:33:50 PM  
Modified: 11/1/2023 3:20:40 PM

**Curves**

**Standard Curve**

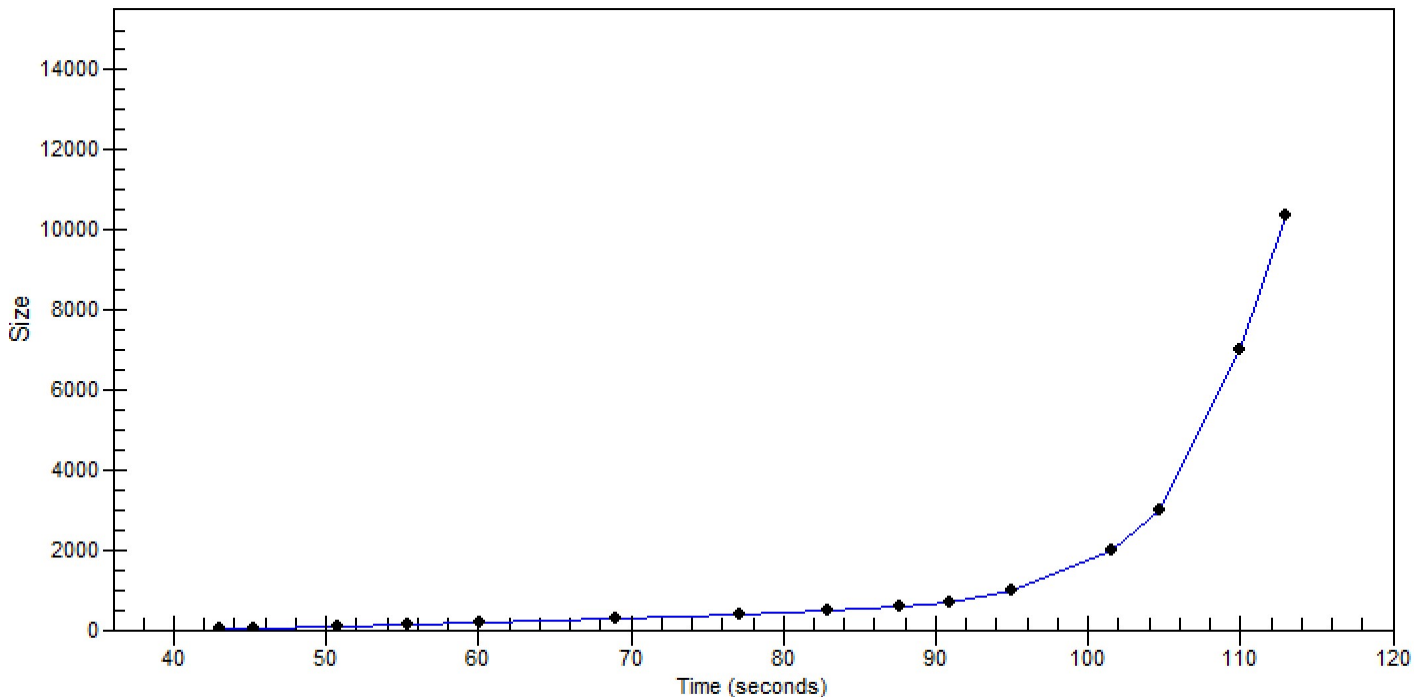

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...nt\2100 bioanalyzer\2100 expert\data\2023-11-01\AVT0072.xad

Created: 11/1/2023 2:33:50 PM  
 Modified: 11/1/2023 3:20:40 PM

**Run Logbook**

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 12)		Instrument	Run		11/1/2023 3:15:10 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Run started on port 1 (File: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\data\2023-11-01\Bioanalyzer1_High Sensitivity DNA Assay_DE34903152_2023-11-01_002.xad)		Instrument	Run		11/1/2023 2:33:57 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Product Number : G2938C		Instrument	Run		11/1/2023 2:33:57 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Name :		Instrument	Run		11/1/2023 2:33:57 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Vendor : Agilent Technologies		Instrument	Run		11/1/2023 2:33:57 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Serial# : DE34903152		Instrument	Run		11/1/2023 2:33:57 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Firmware : C.01.069		Instrument	Run		11/1/2023 2:33:57 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Cartridge : Electrode		Instrument	Run		11/1/2023 2:33:57 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB