


Assay Class: Eukaryote Total RNA Pico  
Data Path: C:\...zer1\_Eukaryote Total RNA Pico\_2023-06-12\_002\_NOVA873-23.xad

Created: 6/12/2023 12:47:18 PM  
Modified: 6/12/2023 1:16:25 PM

**Electrophoresis File Run Summary**

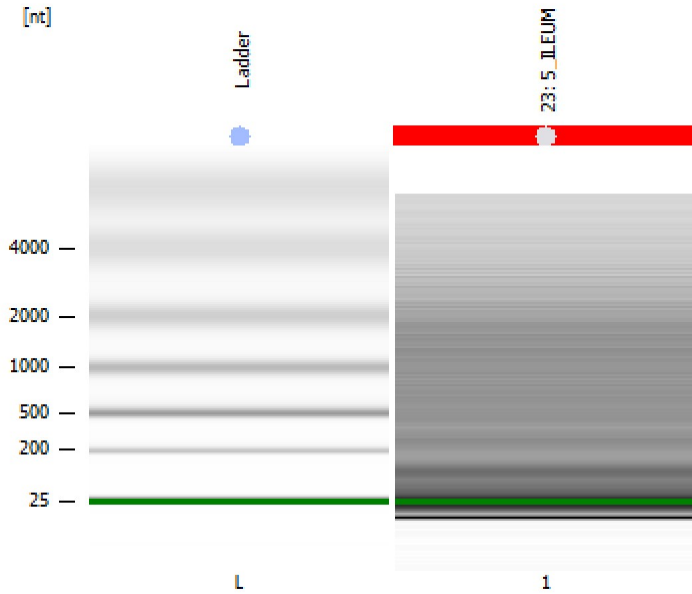

Instrument Information:

Instrument Name: DE34903152      Firmware: C.01.069  
Serial#: DE34903152      Type: G2938C

Assay Information:

Assay Origin Path: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\assays\RNA\Eukaryote Total RNA Pico Series II.xsy


Assay Class: Eukaryote Total RNA Pico  
Version: 2.6  
Assay Comments: Total RNA Analysis pg sensitivity (Eukaryote)

© Copyright 2003 - 2009 Agilent Technologies, Inc.

Chip Information:

Chip Lot #:  
Reagent Kit Lot #:  
Chip Comments:

NOVA0873      **23: 5\_ILEUM**  
RIN N/A

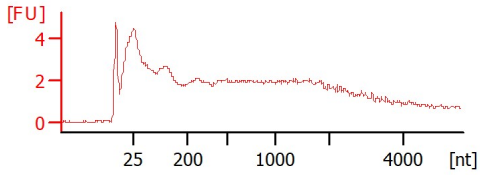

Assay Class: Eukaryote Total RNA Pico  
Data Path: C:\...zer1\_Eukaryote Total RNA Pico\_2023-06-12\_002\_NOVA873-23.xad

Created: 6/12/2023 12:47:18 PM  
Modified: 6/12/2023 1:16:25 PM

**Electrophoresis File Run Summary (Chip Summary)**

Sample Name	Sample Comment	Status	Result Label	Result Color
23: 5_ILEUM Ladder	NOVA0873	✓	RIN N/A	
		✓	All Other Samples	

Chip Lot #

Reagent Kit Lot #

Chip Comments :

Assay Class: Eukaryote Total RNA Pico  
 Data Path: C:\...zer1\_Eukaryote Total RNA Pico\_2023-06-12\_002\_NOVA873-23.xad

Created: 6/12/2023 12:47:18 PM  
 Modified: 6/12/2023 1:16:25 PM

**Electrophoresis Assay Details**

**General Analysis Settings**

Number of Available Sample and Ladder Wells (Max.) : 12  
 Minimum Visible Range [s] : 17  
 Maximum Visible Range [s] : 70  
 Start Analysis Time Range [s] : 18  
 End Analysis Time Range [s] : 69  
 Ladder Concentration [pg/μl] : 1000  
 Lower Marker Concentration [pg/μl] : 0  
 Upper Marker Concentration [pg/μl] : 0  
 Used Lower Marker for Quantitation  
 Standard Curve Fit is Logarithmic  
 Show Data Aligned to Lower Marker

**Integrator Settings**

Integration Start Time [s] : 18  
 Integration End Time [s] : 69  
 Slope Threshold : 0.6  
 Height Threshold [FU] : 0.5  
 Area Threshold : 0.2  
 Width Threshold [s] : 0.3  
 Baseline Plateau [s] : 6

**Filter Settings**

Filter Width [s] : 0.5  
 Polynomial Order : 4


**Ladder**

Ladder Peak	Size
1	25
2	200
3	500
4	1000
5	2000
6	4000

Assay Class: Eukaryote Total RNA Pico  
Data Path: C:\...zer1\_Eukaryote Total RNA Pico\_2023-06-12\_002\_NOVA873-23.xad

Created: 6/12/2023 12:47:18 PM  
Modified: 6/12/2023 1:16:25 PM

**Electropherogram Summary**

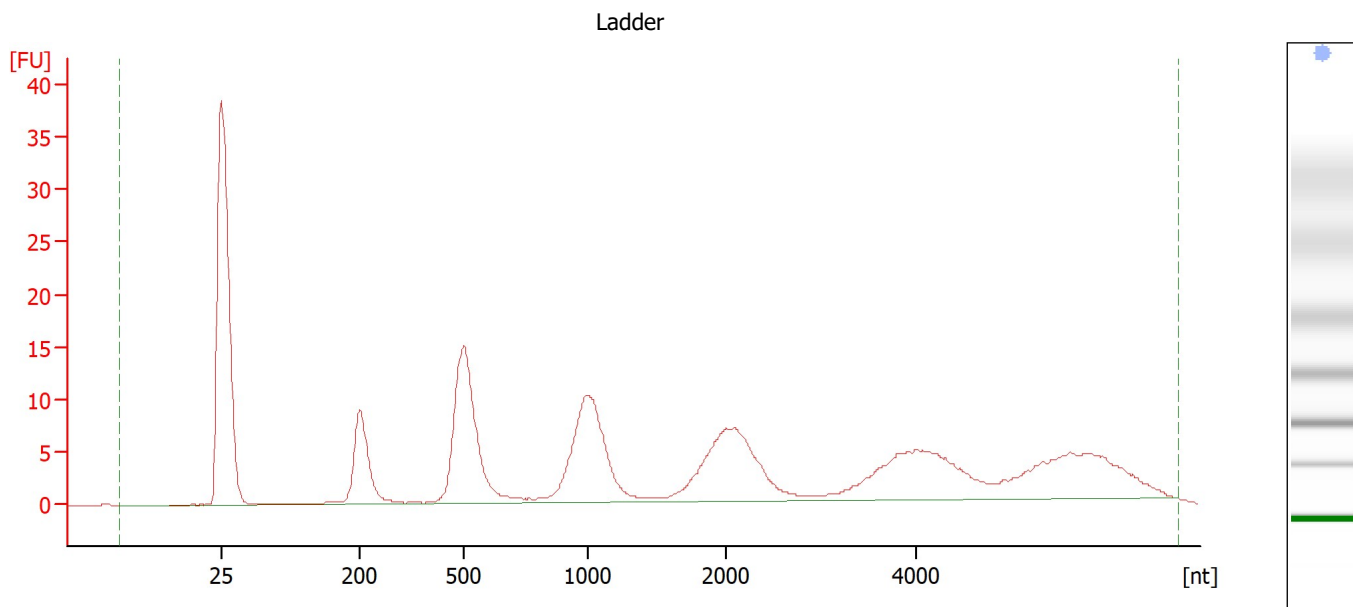


**Overall Results for Ladder**

RNA Area:	233.8	Result Flagging Color:	<span style="background-color: #ADD8E6; border: 1px solid black; display: inline-block; width: 20px; height: 10px;"></span>
RNA Concentration:	1,000 pg/μl	Result Flagging Label:	All Other Samples

Assay Class: Eukaryote Total RNA Pico  
 Data Path: C:\...zer1\_Eukaryote Total RNA Pico\_2023-06-12\_002\_NOVA873-23.xad

Created: 6/12/2023 12:47:18 PM  
 Modified: 6/12/2023 1:16:25 PM

**Electropherogram Summary Continued ...**

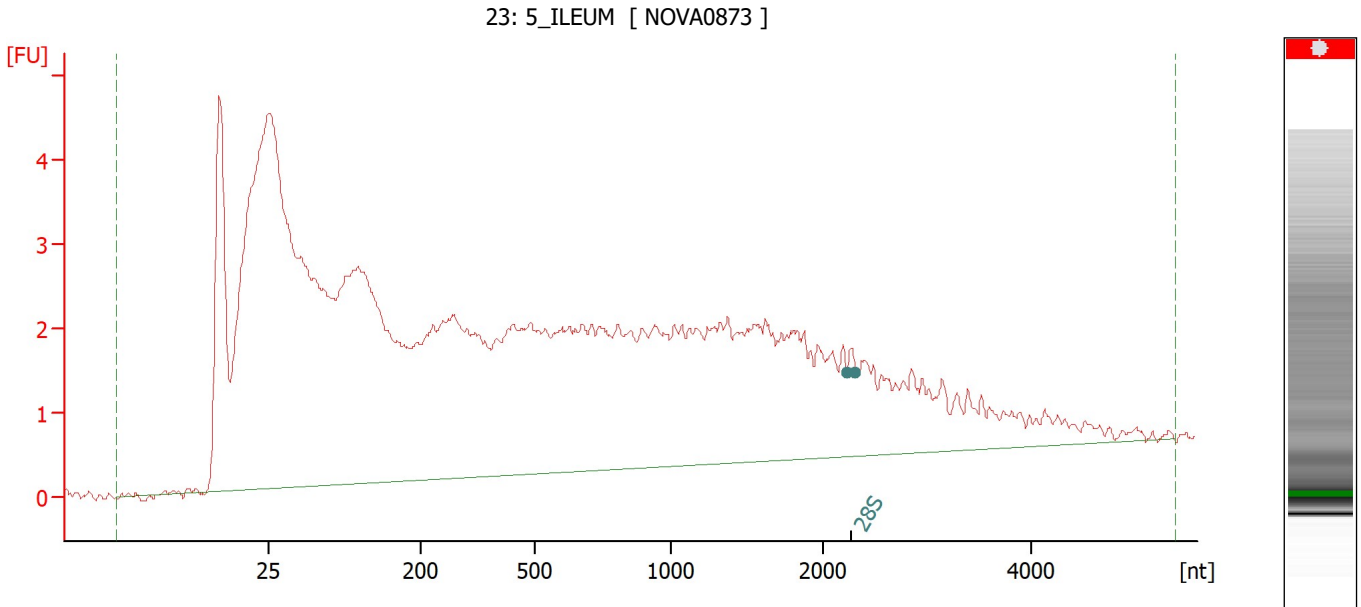

**Overall Results for sample 1 : 23: 5 ILEUM**

RNA Area:	139.4	RNA Integrity Number (RIN):	N/A (B.02.10)
RNA Concentration:	596 µg/µl	Result Flagging Color:	<span style="background-color: #cccccc; border: 1px solid black; display: inline-block; width: 20px; height: 10px;"></span>
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN N/A


**Fragment table for sample 1 : 23: 5 ILEUM**

Name	Start Size [nt]	End Size [nt]	Area	% of total Area
28S	2,228	2,310	0.1	0.1

Assay Class: Eukaryote Total RNA Pico  
Data Path: C:\...zer1\_Eukaryote Total RNA Pico\_2023-06-12\_002\_NOVA873-23.xad

Created: 6/12/2023 12:47:18 PM  
Modified: 6/12/2023 1:16:25 PM

**Gel Image**

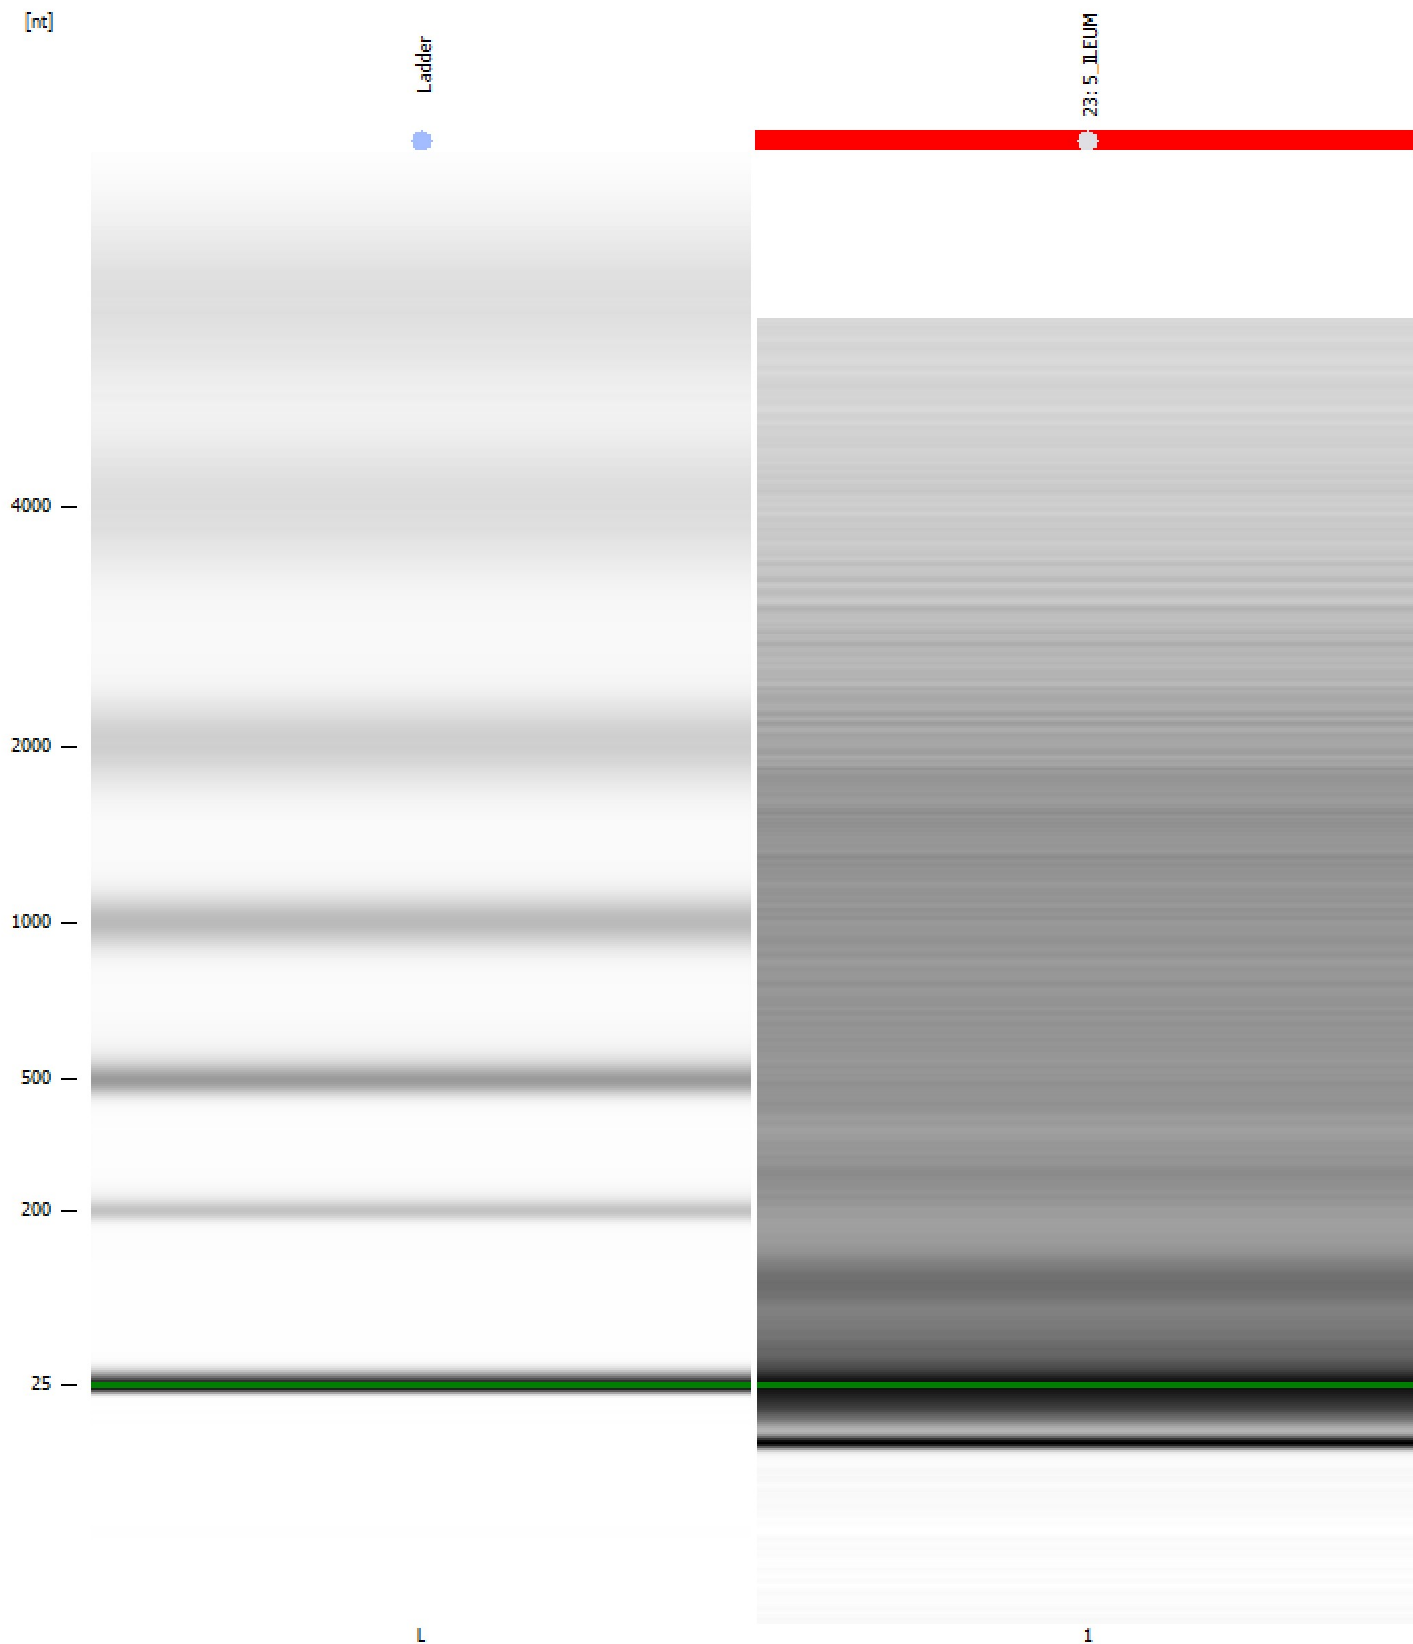


Assay Class: Eukaryote Total RNA Pico  
Data Path: C:\...zer1\_Eukaryote Total RNA Pico\_2023-06-12\_002\_NOVA873-23.xad

Created: 6/12/2023 12:47:18 PM  
Modified: 6/12/2023 1:16:25 PM

**Curves**

**Standard Curve**

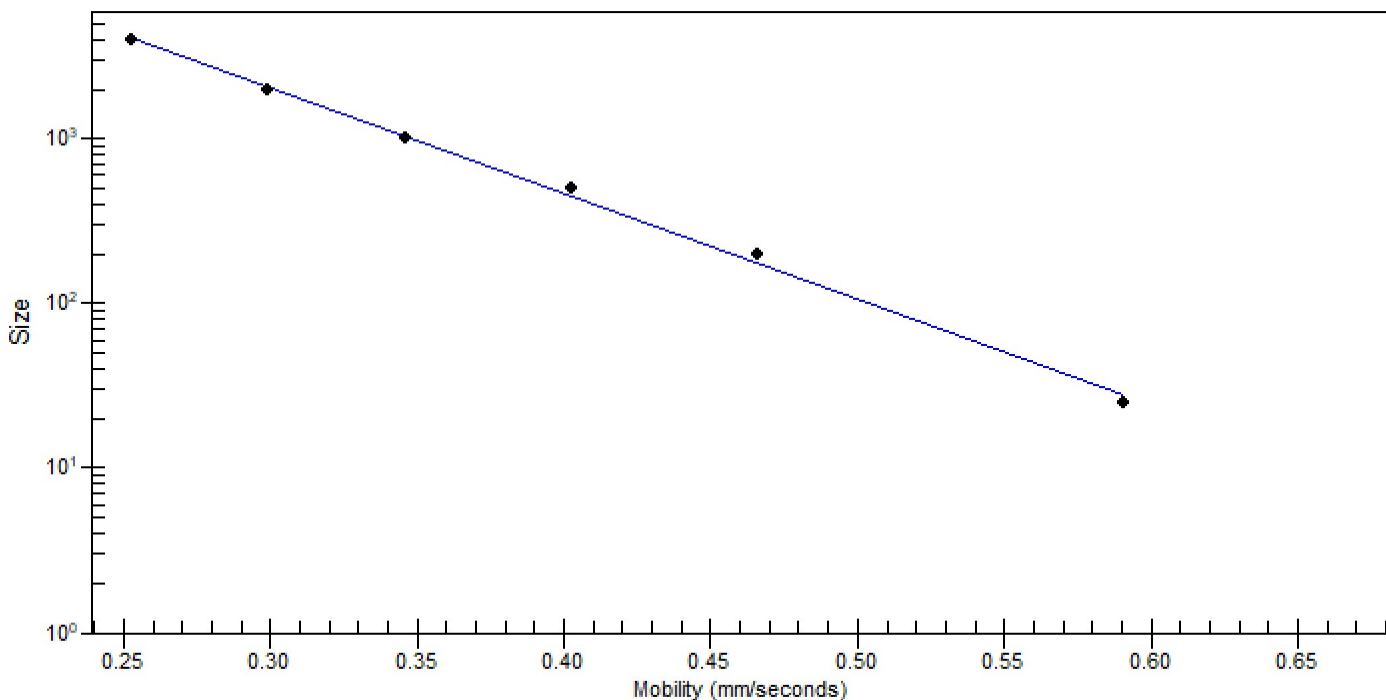

Assay Class: Eukaryote Total RNA Pico  
 Data Path: C:\...zer1\_Eukaryote Total RNA Pico\_2023-06-12\_002\_NOVA873-23.xad

Created: 6/12/2023 12:47:18 PM  
 Modified: 6/12/2023 1:16:25 PM

**Run Logbook**

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 12)		Instrument	Run		6/12/2023 1:09:19 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Run started on port 1 (File: C:\Users\sbsuser\Desktop\2023-06-12\Bioanalyzer1_Eukaryote Total RNA Pico_2023-06-12_002.xad)		Instrument	Run		6/12/2023 12:47:24 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Product Number : G2938C		Instrument	Run		6/12/2023 12:47:24 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Name :		Instrument	Run		6/12/2023 12:47:24 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Vendor : Agilent Technologies		Instrument	Run		6/12/2023 12:47:24 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Serial# : DE34903152		Instrument	Run		6/12/2023 12:47:24 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Firmware : C.01.069		Instrument	Run		6/12/2023 12:47:24 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Cartridge : Electrode		Instrument	Run		6/12/2023 12:47:23 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB