


Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...\_High Sensitivity DNA Assay\_2023-06-14\_001\_QC1497\_36-43.xad

Created: 6/14/2023 12:28:35 PM  
Modified: 6/14/2023 1:46:16 PM

**Electrophoresis File Run Summary**

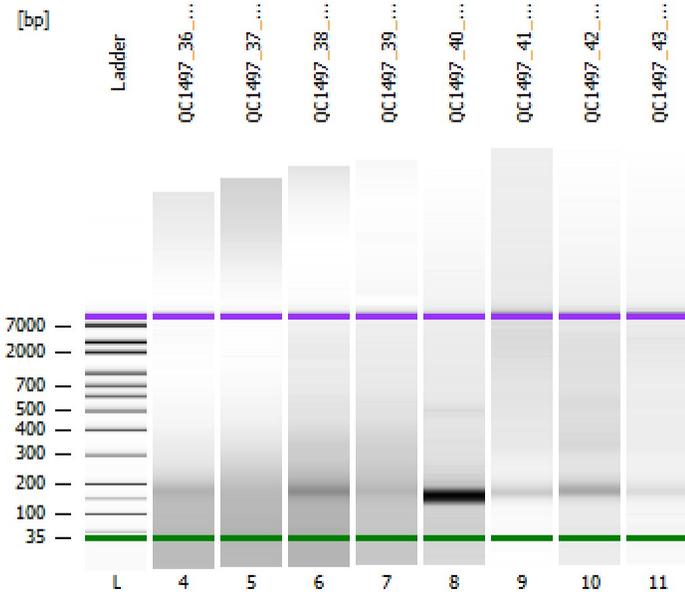

Instrument Information:

Instrument Name: DE34903152      Firmware: C.01.069  
Serial#: DE34903152      Type: G2938C

Assay Information:

Assay Origin Path: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy  
Assay Class: High Sensitivity DNA Assay  
Version: 1.03  
Assay Comments: Copyright © 2003-2010 Agilent Technologies




Chip Information:

Chip Lot #:        
Reagent Kit Lot #:        
Chip Comments:

QC1497\_36\_LWB36

QC1497\_37\_LWB37




QC1497\_38\_LWB38

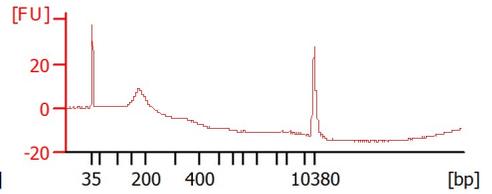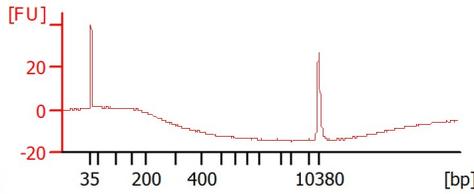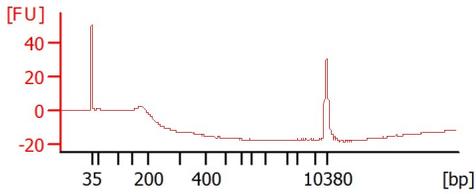

QC1497\_39\_LWB39



QC1497\_40\_LWB40

QC1497\_41\_LWB41

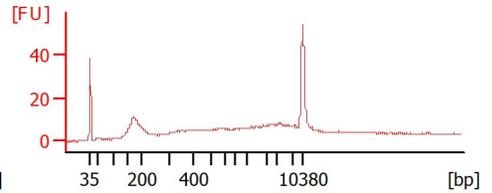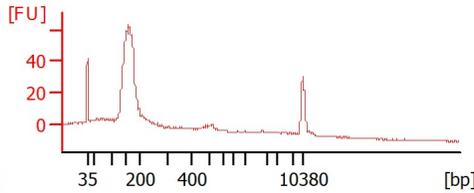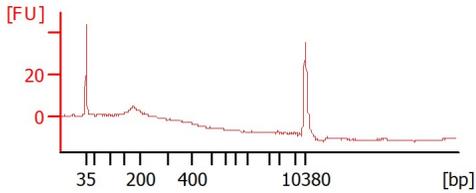

QC1497\_42\_LWB42

QC1497\_43\_LWB43

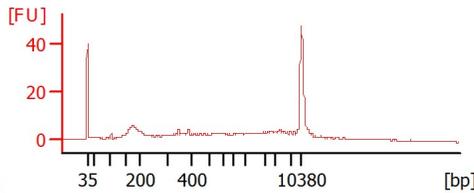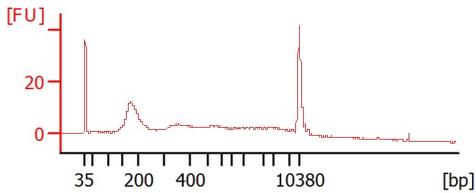

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...\High Sensitivity DNA Assay\_2023-06-14\_001\_QC1497\_36-43.xad

Created: 6/14/2023 12:28:35 PM  
 Modified: 6/14/2023 1:46:16 PM

**Electrophoresis File Run Summary (Chip Summary)**

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
QC1497_36_LWB36		<input type="checkbox"/>		✓		
QC1497_37_LWB37		<input type="checkbox"/>		✓		
QC1497_38_LWB38		<input type="checkbox"/>		✓		
QC1497_39_LWB39		<input type="checkbox"/>		✓		
QC1497_40_LWB40		<input type="checkbox"/>		✓		
QC1497_41_LWB41		<input type="checkbox"/>		✓		
QC1497_42_LWB42		<input type="checkbox"/>		✓		
QC1497_43_LWB43		<input type="checkbox"/>		✓		
Ladder		<input type="checkbox"/>		✓		

Chip Lot #

Reagent Kit Lot #

Chip Comments :

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...\_High Sensitivity DNA Assay\_2023-06-14\_001\_QC1497\_36-43.xad

Created: 6/14/2023 12:28:35 PM  
 Modified: 6/14/2023 1:46:16 PM

**Electrophoresis Assay Details**

**General Analysis Settings**

Number of Available Sample and Ladder Wells (Max.) : 12  
 Minimum Visible Range [s] : 32  
 Maximum Visible Range [s] : 138  
 Start Analysis Time Range [s] : 33  
 End Analysis Time Range [s] : 137.5  
 Ladder Concentration [pg/μl] : 1950  
 Uses Standard Area for Ladder Fragments  
 Lower Marker Concentration [pg/μl] : 125  
 Upper Marker Concentration [pg/μl] : 75  
 Used Upper Marker for Quantitation  
 Standard Curve Fit is Point to Point  
 Show Data Aligned to Lower and Upper Marker

**Integrator Settings**

Integration Start Time [s] : 33.05  
 Integration End Time [s] : 137  
 Slope Threshold : 0.8  
 Height Threshold [FU] : 5  
 Area Threshold : 0.1  
 Width Threshold [s] : 0.6  
 Baseline Plateau [s] : 0.5

**Filter Settings**

Filter Width [s] : 0.5  
 Polynomial Order : 4


**Ladder**

Ladder Peak	Size	Area
1	35	160
2	50	210
3	100	208
4	150	221
5	200	242
6	300	270
7	400	305
8	500	306
9	600	336
10	700	321
11	1000	366
12	2000	413
13	3000	411
14	7000	400
15	10380	214

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...\_High Sensitivity DNA Assay\_2023-06-14\_001\_QC1497\_36-43.xad

Created: 6/14/2023 12:28:35 PM  
 Modified: 6/14/2023 1:46:16 PM

**Electropherogram Summary**

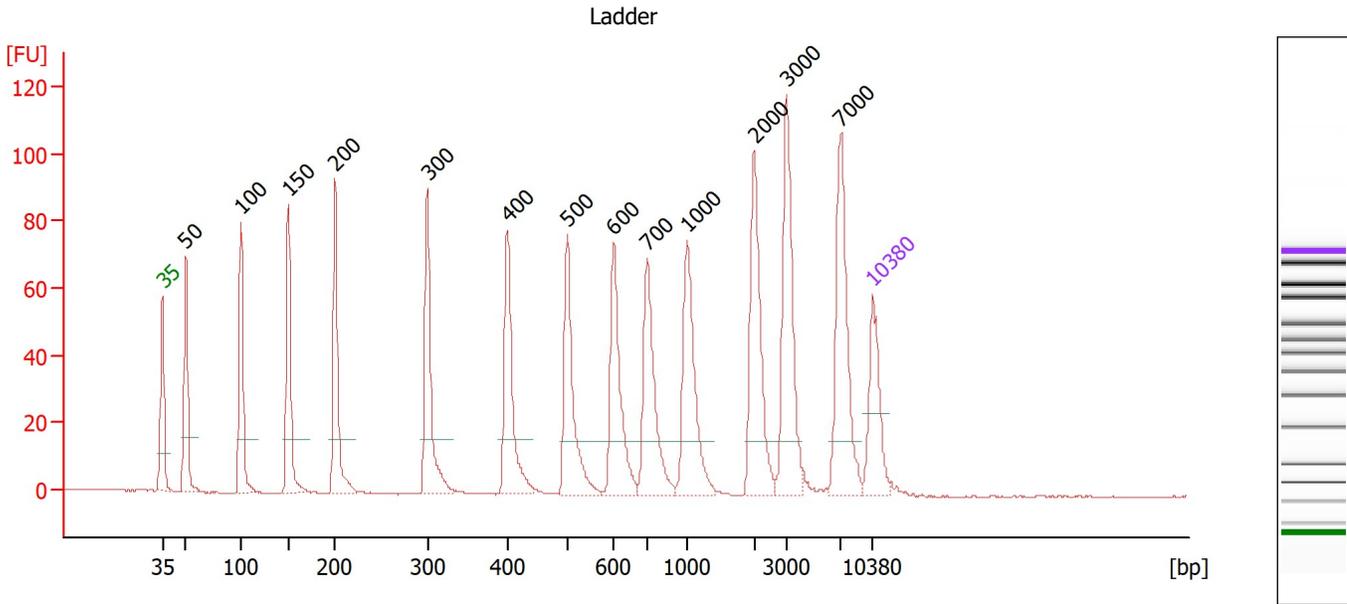

**Overall Results for Ladder**

Noise: 0.2


**Peak table for Ladder**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	50	150.00	4,545.5	Ladder Peak
3	100	150.00	2,272.7	Ladder Peak
4	150	150.00	1,515.2	Ladder Peak
5	200	150.00	1,136.4	Ladder Peak
6	300	150.00	757.6	Ladder Peak
7	400	150.00	568.2	Ladder Peak
8	500	150.00	454.5	Ladder Peak
9	600	150.00	378.8	Ladder Peak
10	700	150.00	324.7	Ladder Peak
11	1,000	150.00	227.3	Ladder Peak
12	2,000	150.00	113.6	Ladder Peak
13	3,000	150.00	75.8	Ladder Peak
14	7,000	150.00	32.5	Ladder Peak
15	10,380	75.00	10.9	Upper Marker

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...\_High Sensitivity DNA Assay\_2023-06-14\_001\_QC1497\_36-43.xad

Created: 6/14/2023 12:28:35 PM  
 Modified: 6/14/2023 1:46:16 PM

**Electropherogram Summary Continued ...**

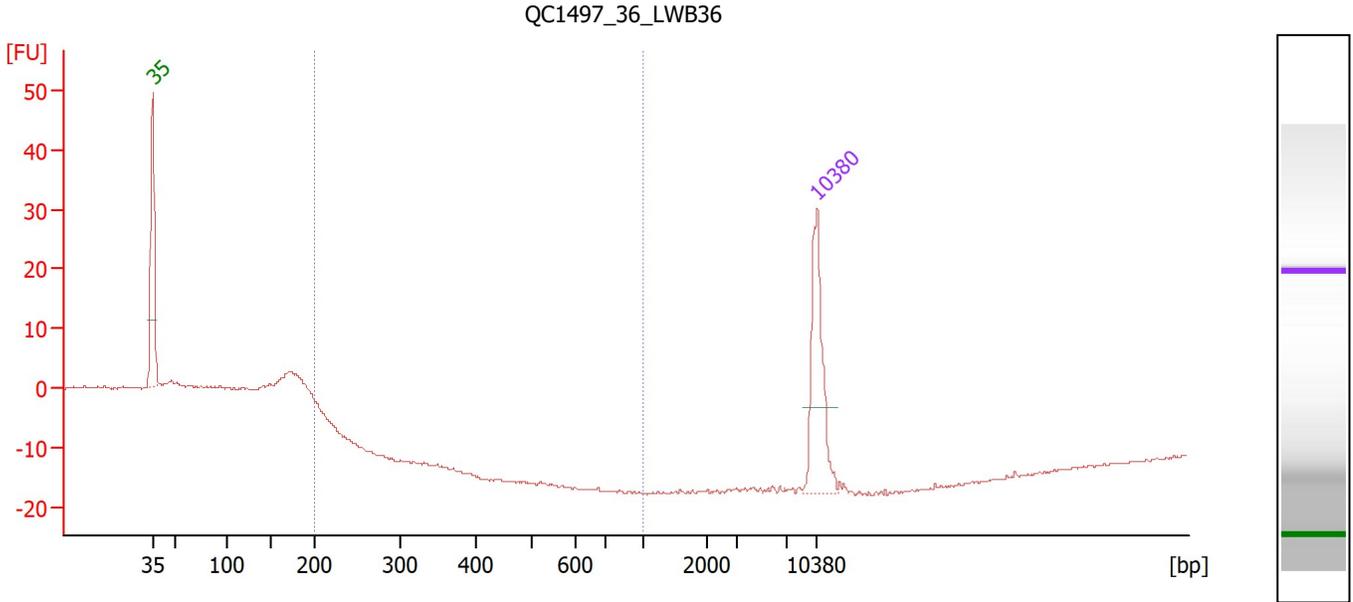

**Overall Results for sample 4 : QC1497 36 LWB36**

Number of peaks found: 0                      Corr. Area 1: 0.0  
 Noise: 0.2

**Peak table for sample 4 : QC1497 36 LWB36**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	10,380	75.00	10.9	Upper Marker


**Region table for sample 4 : QC1497 36 LWB36**

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	0.0	0	200	0.1	0.09	0.7	Blue

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...\_High Sensitivity DNA Assay\_2023-06-14\_001\_QC1497\_36-43.xad

Created: 6/14/2023 12:28:35 PM  
 Modified: 6/14/2023 1:46:16 PM

**Electropherogram Summary Continued ...**

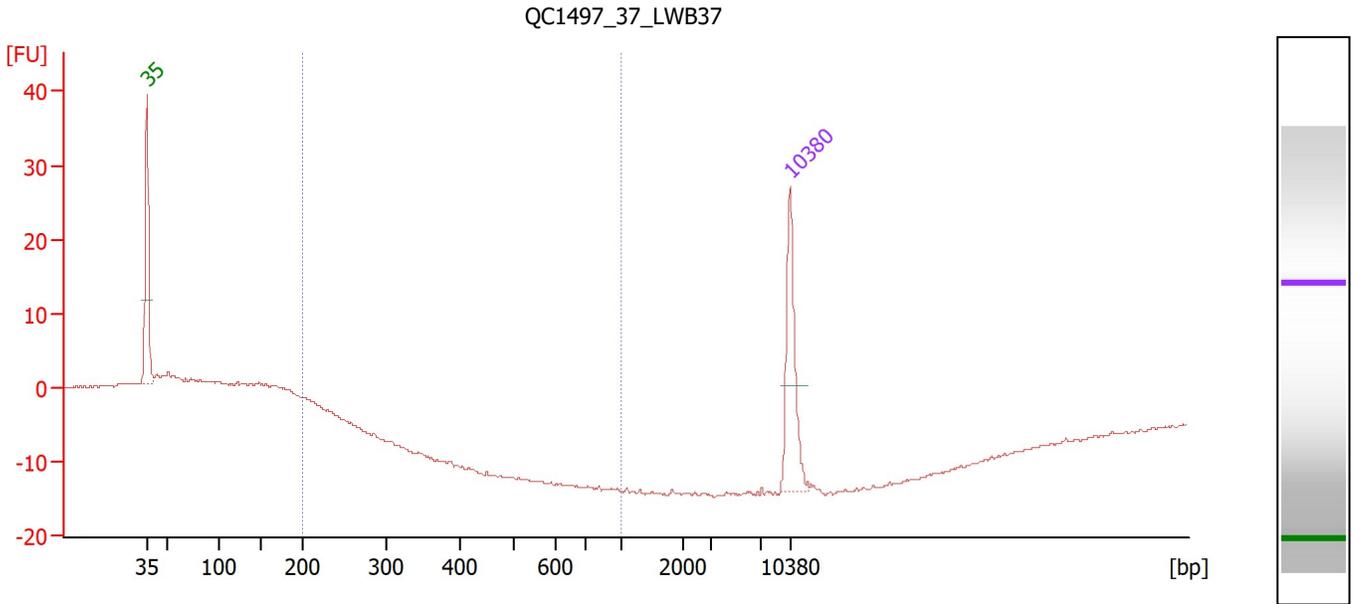

**Overall Results for sample 5 : QC1497 37 LWB37**

Number of peaks found: 0                      Corr. Area 1: 0.0  
 Noise: 0.2

**Peak table for sample 5 : QC1497 37 LWB37**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	10,380	75.00	10.9	Upper Marker


**Region table for sample 5 : QC1497 37 LWB37**

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	0.0	0	0	0.0	0.00	0.0	Blue

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...\_High Sensitivity DNA Assay\_2023-06-14\_001\_QC1497\_36-43.xad

Created: 6/14/2023 12:28:35 PM  
 Modified: 6/14/2023 1:46:16 PM

**Electropherogram Summary Continued ...**

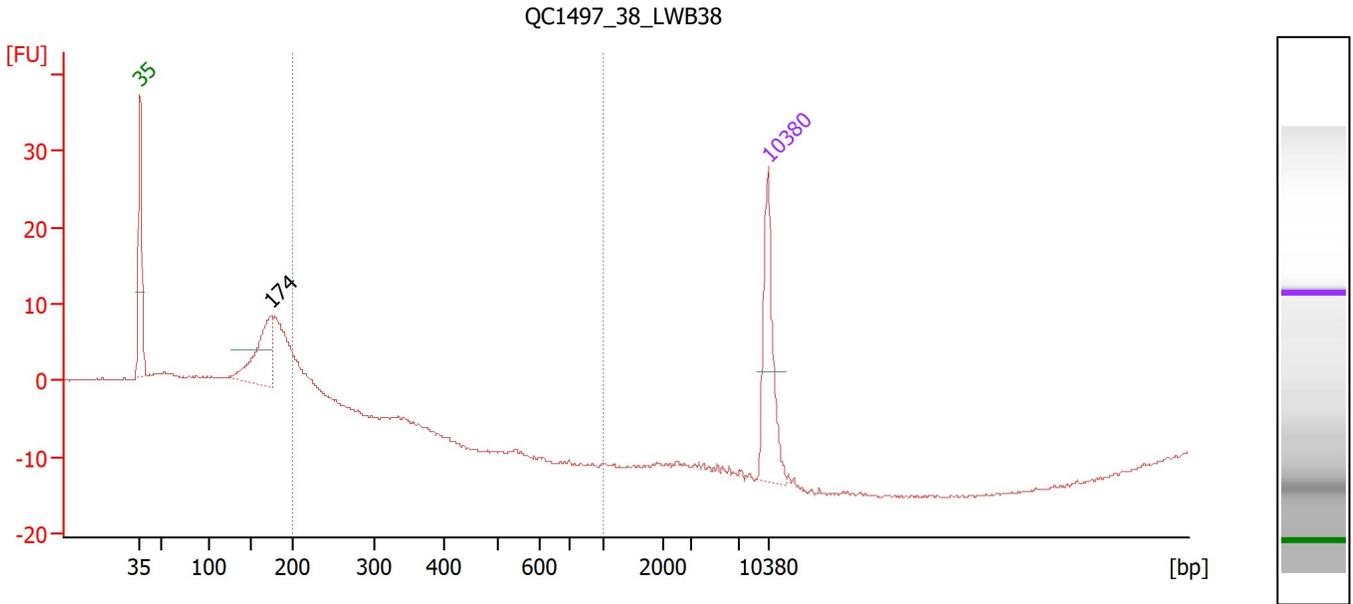

**Overall Results for sample 6 : QC1497 38 LWB38**

Number of peaks found: 1                      Corr. Area 1: 14.2  
 Noise: 0.2

**Peak table for sample 6 : QC1497 38 LWB38**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	174	102.10	889.5	
3	10,380	75.00	10.9	Upper Marker


**Region table for sample 6 : QC1497 38 LWB38**

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	14.2	12	213	4.8	43.70	311.1	Blue

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...\_High Sensitivity DNA Assay\_2023-06-14\_001\_QC1497\_36-43.xad

Created: 6/14/2023 12:28:35 PM  
 Modified: 6/14/2023 1:46:16 PM

**Electropherogram Summary Continued ...**

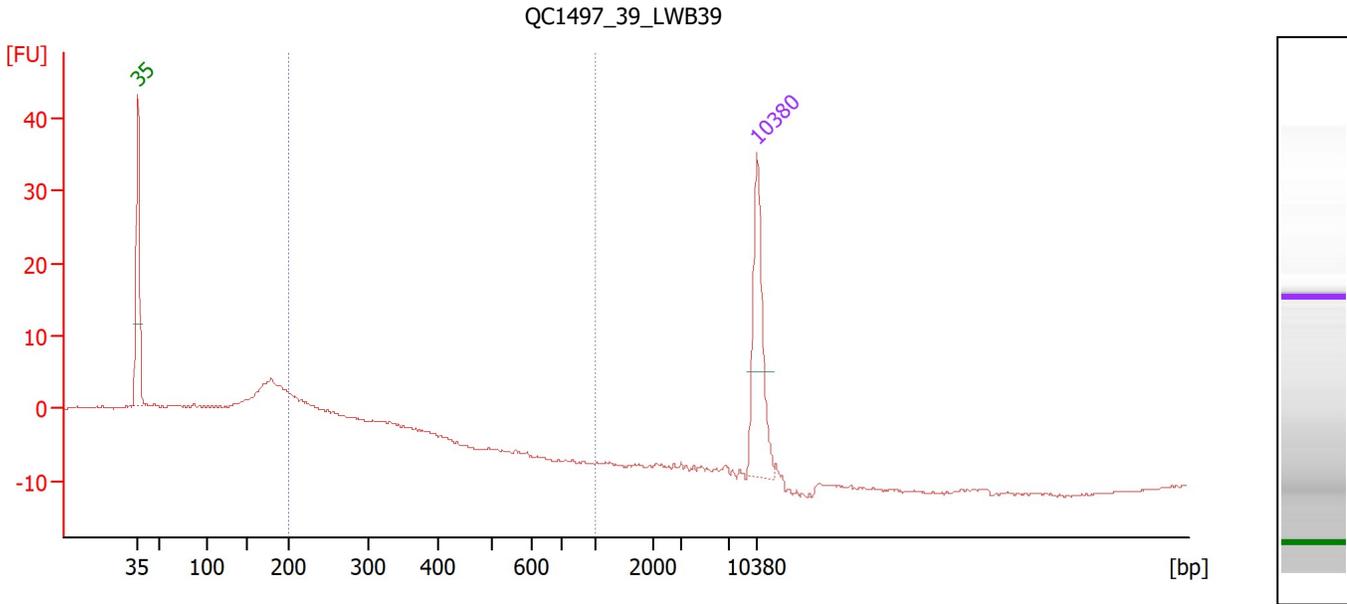

**Overall Results for sample 7 : QC1497 39 LWB39**

Number of peaks found: 0                      Corr. Area 1: 35.9  
 Noise: 0.2

**Peak table for sample 7 : QC1497 39 LWB39**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	10,380	75.00	10.9	Upper Marker


**Region table for sample 7 : QC1497 39 LWB39**

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	35.9	33	256	17.9	93.61	569.0	Blue

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...\_High Sensitivity DNA Assay\_2023-06-14\_001\_QC1497\_36-43.xad

Created: 6/14/2023 12:28:35 PM  
 Modified: 6/14/2023 1:46:16 PM

**Electropherogram Summary Continued ...**

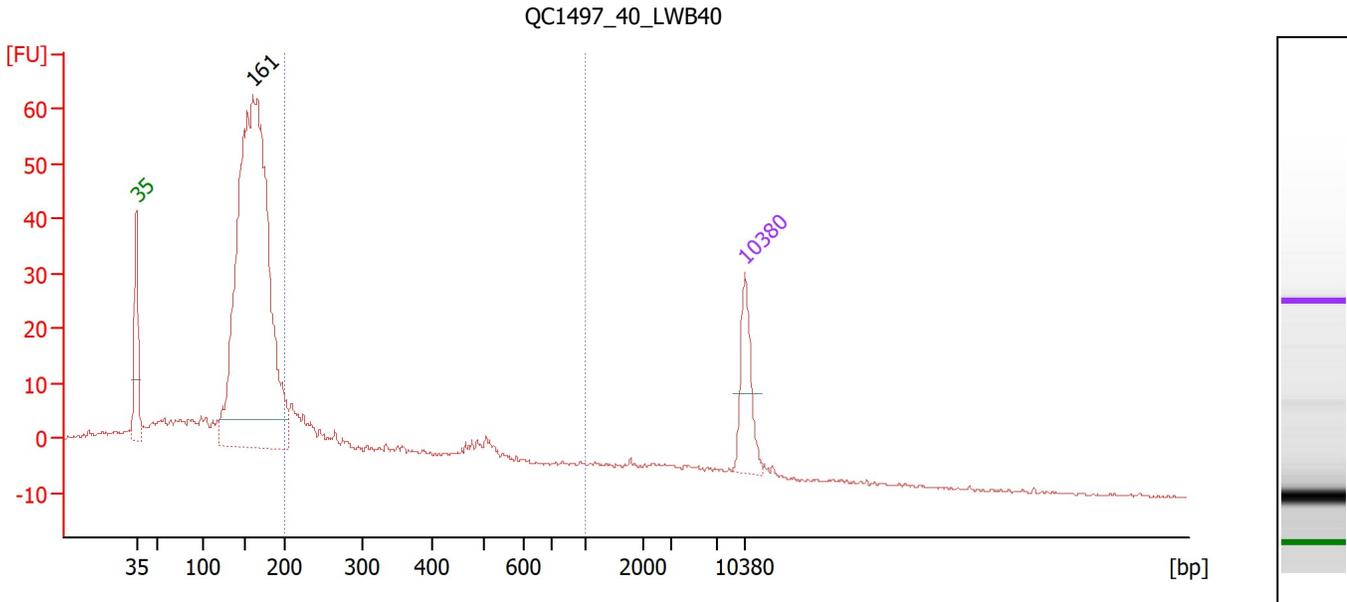

**Overall Results for sample 8 : QC1497 40 LWB40**

Number of peaks found: 1                      Corr. Area 1: 73.8  
 Noise: 0.2

**Peak table for sample 8 : QC1497 40 LWB40**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	161	1,479.44	13,910.9	
3	10,380	75.00	10.9	Upper Marker


**Region table for sample 8 : QC1497 40 LWB40**

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	73.8	12	320	39.9	206.61	1,163.4	Blue

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...\_High Sensitivity DNA Assay\_2023-06-14\_001\_QC1497\_36-43.xad

Created: 6/14/2023 12:28:35 PM  
 Modified: 6/14/2023 1:46:16 PM

**Electropherogram Summary Continued ...**

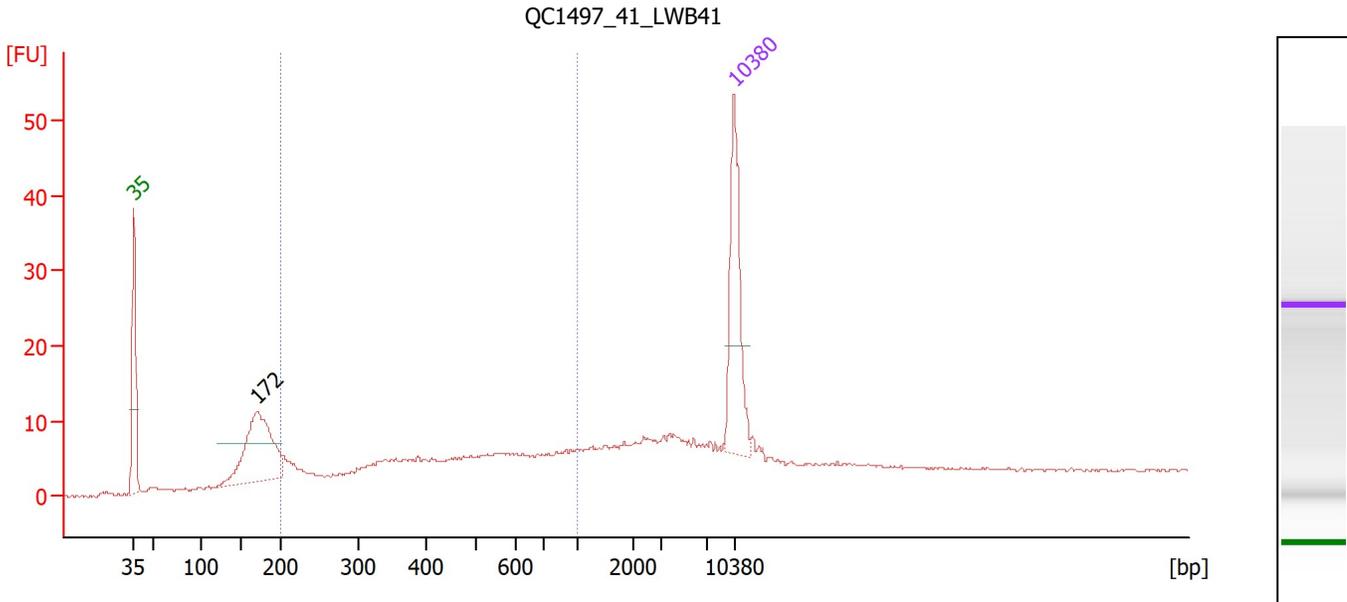

**Overall Results for sample 9 : QC1497 41 LWB41**

Number of peaks found: 1                      Corr. Area 1: 149.9  
 Noise: 0.2

**Peak table for sample 9 : QC1497 41 LWB41**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	172	139.29	1,229.3	
3	10,380	75.00	10.9	Upper Marker


**Region table for sample 9 : QC1497 41 LWB41**

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	149.9	42	478	41.3	304.20	1,233.6	Blue

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...\_High Sensitivity DNA Assay\_2023-06-14\_001\_QC1497\_36-43.xad

Created: 6/14/2023 12:28:35 PM  
 Modified: 6/14/2023 1:46:16 PM

**Electropherogram Summary Continued ...**

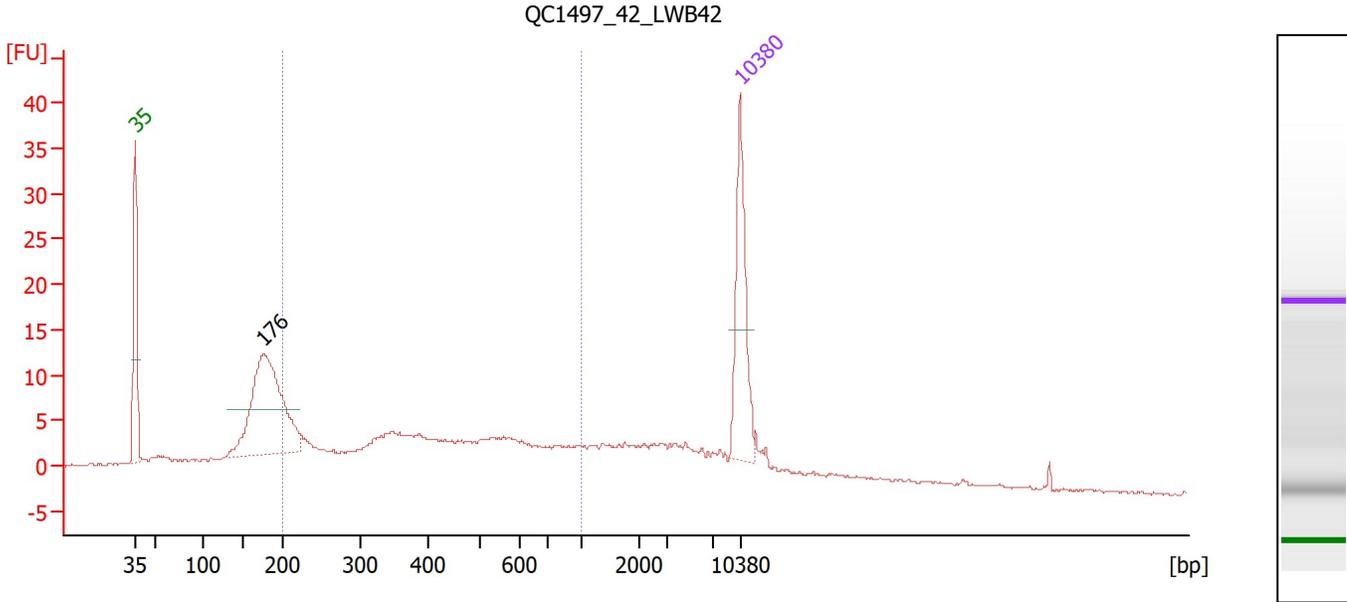

**Overall Results for sample 10 : QC1497 42 LWB42**

Number of peaks found: 1                      Corr. Area 1: 159.6  
 Noise: 0.2

**Peak table for sample 10 : QC1497 42 LWB42**

Peak	Size [bp]	Conc. [pg/µl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	176	238.38	2,053.5	
3	10,380	75.00	10.9	Upper Marker

**Region table for sample 10 : QC1497 42 LWB42**


From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/µl]	Molarity [pmol/l]	Color
200	1,000	159.6	46	451	42.3	412.16	1,771.3	Blue



Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...\_High Sensitivity DNA Assay\_2023-06-14\_001\_QC1497\_36-43.xad

Created: 6/14/2023 12:28:35 PM  
Modified: 6/14/2023 1:46:16 PM

Gel Image

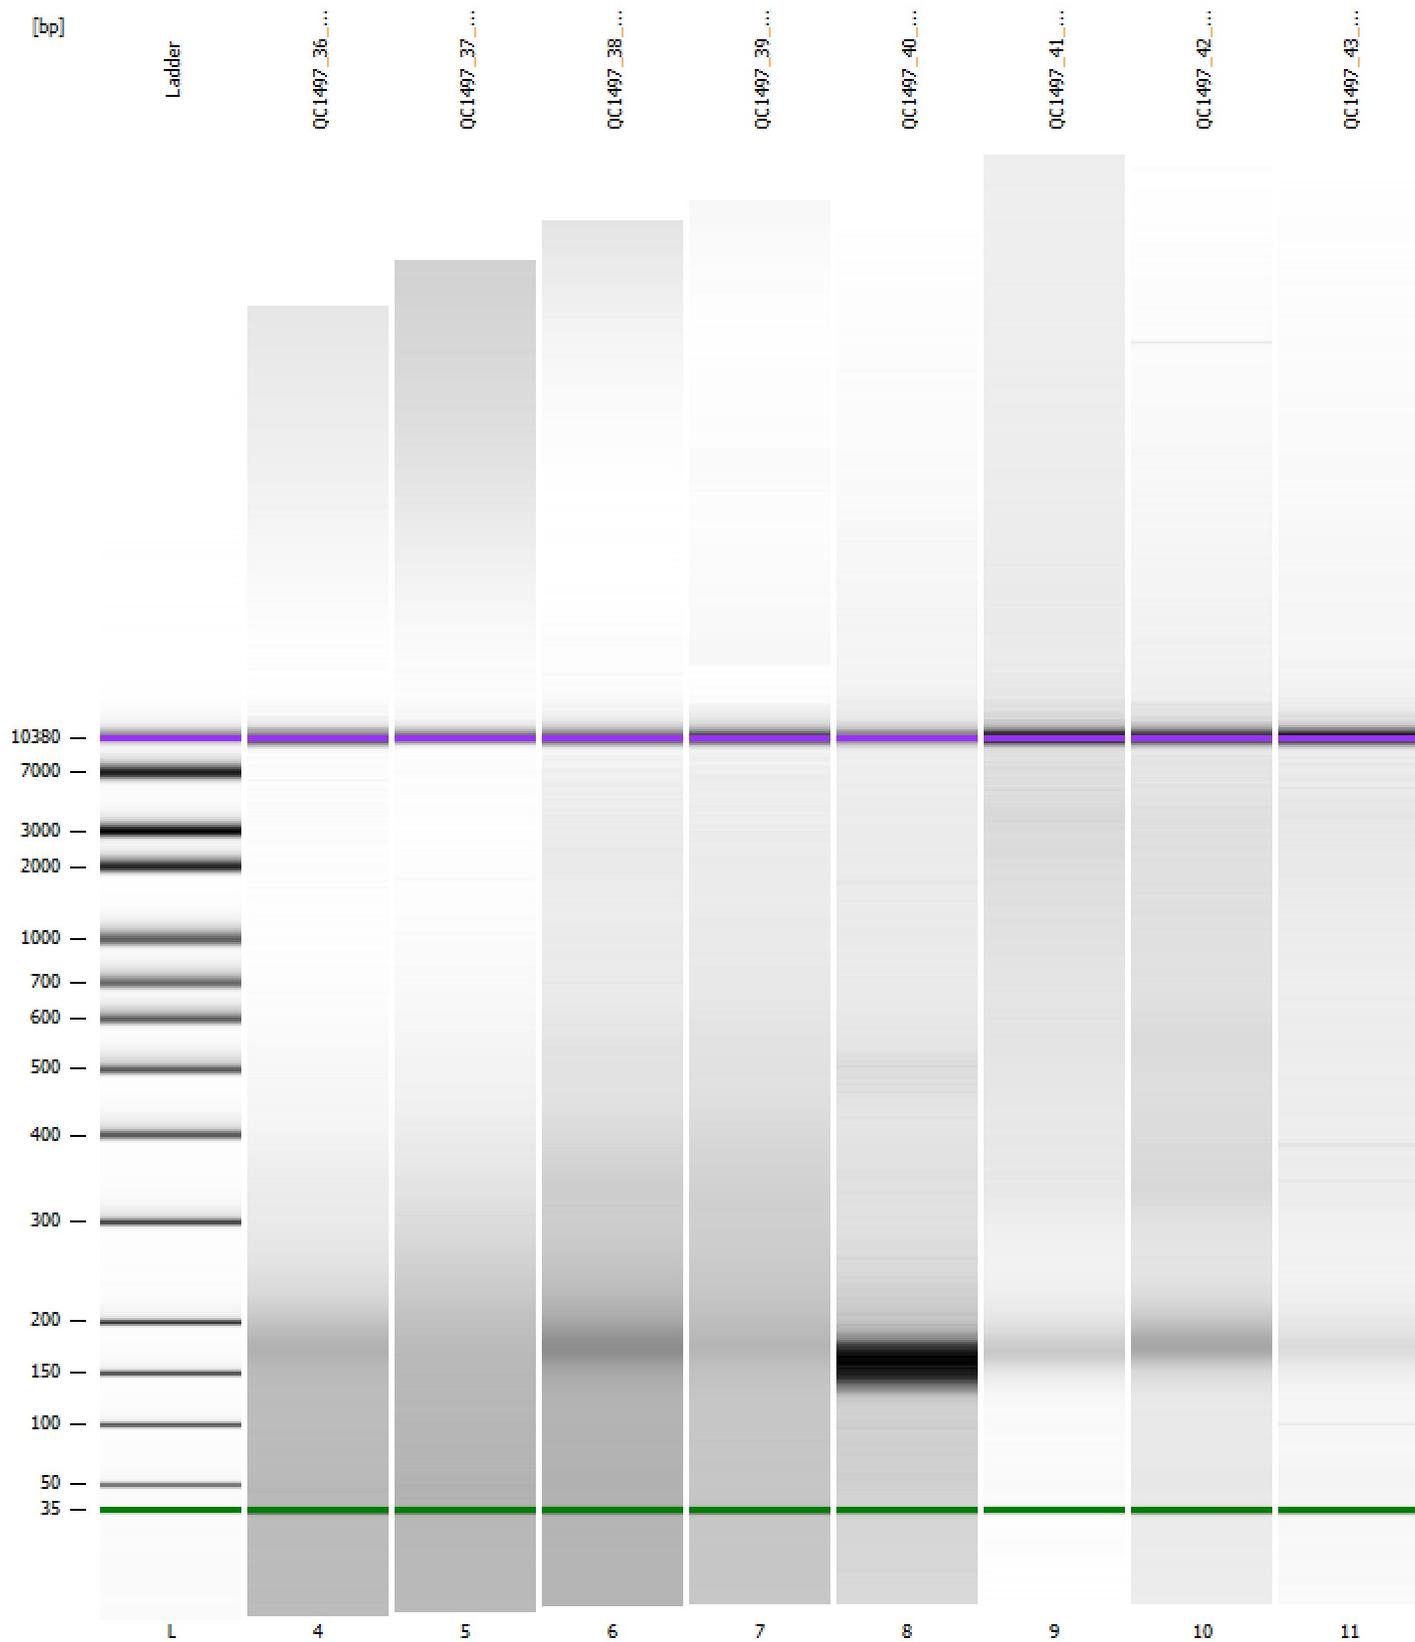


Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...\_High Sensitivity DNA Assay\_2023-06-14\_001\_QC1497\_36-43.xad

Created: 6/14/2023 12:28:35 PM  
Modified: 6/14/2023 1:46:16 PM

**Curves**

**Standard Curve**

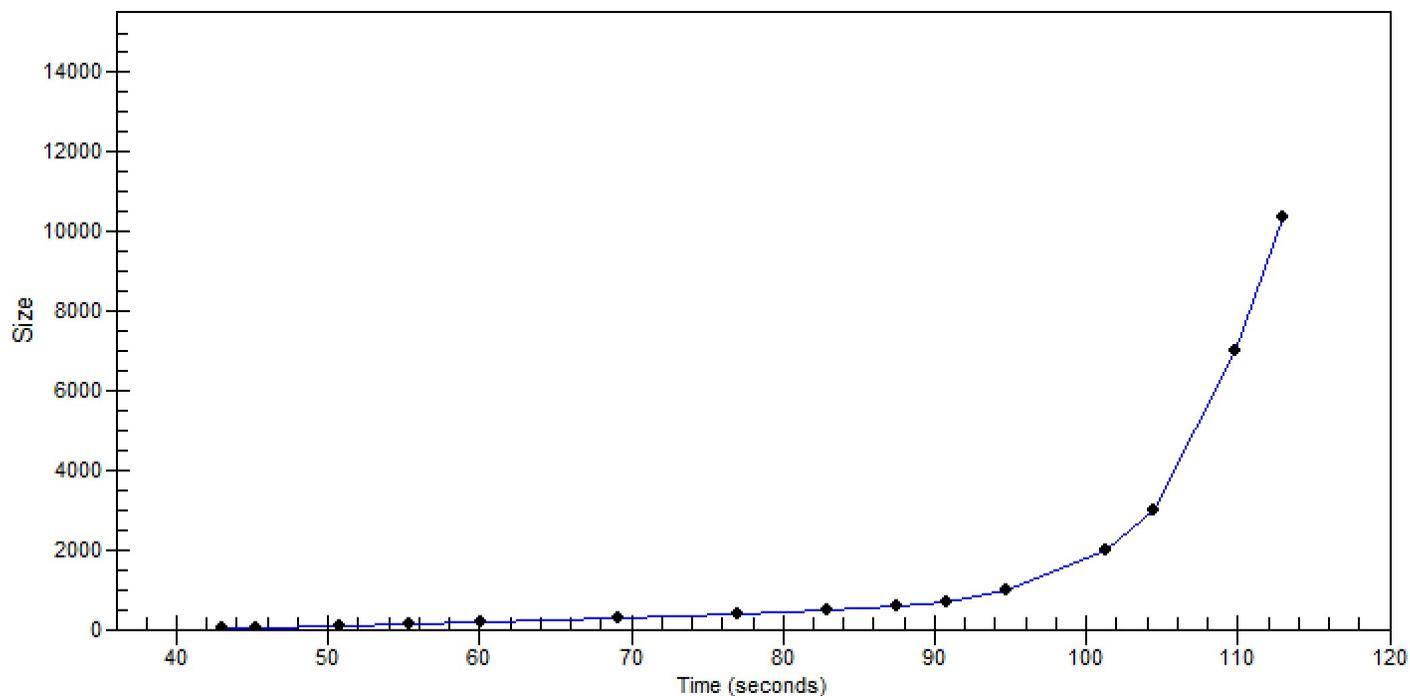

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...\High Sensitivity DNA Assay\_2023-06-14\_001\_QC1497\_36-43.xad

Created: 6/14/2023 12:28:35 PM  
 Modified: 6/14/2023 1:46:16 PM

**Run Logbook**

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 12)		Instrument	Run		6/14/2023 1:09:55 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Run started on port 1 (File: C:\Users\sbsuser\Desktop\2023-06-14\Bioanalyzer1_High Sensitivity DNA Assay_2023-06-14_001.xad)		Instrument	Run		6/14/2023 12:28:41 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Product Number : G2938C		Instrument	Run		6/14/2023 12:28:41 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Name :		Instrument	Run		6/14/2023 12:28:41 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Vendor : Agilent Technologies		Instrument	Run		6/14/2023 12:28:41 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Serial# : DE34903152		Instrument	Run		6/14/2023 12:28:41 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Firmware : C.01.069		Instrument	Run		6/14/2023 12:28:41 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Cartridge : Electrode		Instrument	Run		6/14/2023 12:28:41 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB