


Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...sitivity DNA Assay_DE34903152_2023-08-14_001_PB972_Libs.xad

Created: 8/14/2023 10:10:19 AM
 Modified: 8/14/2023 10:55:09 AM

Electrophoresis File Run Summary

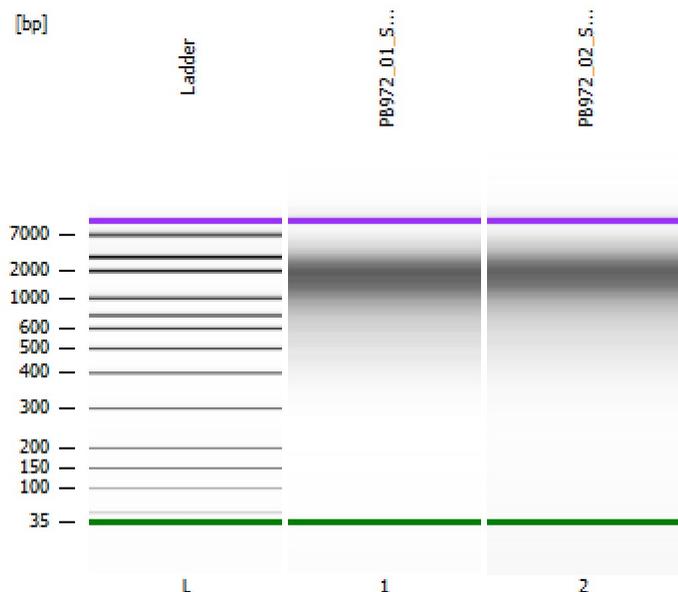

Instrument Information:

Instrument Name: DE34903152 Firmware: C.01.069
 Serial#: DE34903152 Type: G2938C

Assay Information:



Assay Origin Path: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy
 Assay Class: High Sensitivity DNA Assay
 Version: 1.03
 Assay Comments: Copyright © 2003-2010 Agilent Technologies

Chip Information:

Chip Lot #:
 Reagent Kit Lot #:
 Chip Comments:

PB972_01_SubLib1_10XSc-Split-Seq/Ampli...

PB972_02_SubLib2_10XSc-Split-SeqAmpli...

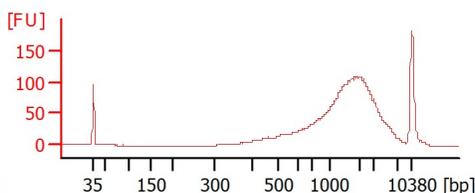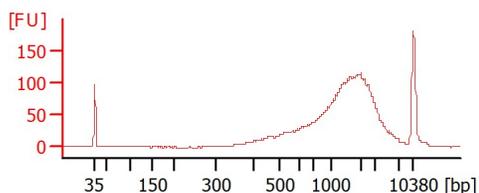

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...sitivity DNA Assay_DE34903152_2023-08-14_001_PB972_Libs.xad

Created: 8/14/2023 10:10:19 AM
 Modified: 8/14/2023 10:55:09 AM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
PB972_01_SubLib1_10XS		<input type="checkbox"/>	✓			
c-Split-Seq/Amplicon_Lib						
PB972_02_SubLib2_10XS		<input type="checkbox"/>	✓			
c-Split-SeqAmplicon_Lib						
Ladder		<input type="checkbox"/>	✓			

Chip Lot #

Reagent Kit Lot #

Chip Comments :

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...sitivity DNA Assay_DE34903152_2023-08-14_001_PB972_Libs.xad

Created: 8/14/2023 10:10:19 AM
 Modified: 8/14/2023 10:55:09 AM

Electrophoresis Assay Details

General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12
 Minimum Visible Range [s] : 32
 Maximum Visible Range [s] : 138
 Start Analysis Time Range [s] : 33
 End Analysis Time Range [s] : 137.5
 Ladder Concentration [pg/μl] : 1950
 Uses Standard Area for Ladder Fragments
 Lower Marker Concentration [pg/μl] : 125
 Upper Marker Concentration [pg/μl] : 75
 Used Upper Marker for Quantitation
 Standard Curve Fit is Point to Point
 Show Data Aligned to Lower and Upper Marker

Integrator Settings

Integration Start Time [s] : 33.05
 Integration End Time [s] : 137
 Slope Threshold : 0.8
 Height Threshold [FU] : 5
 Area Threshold : 0.1
 Width Threshold [s] : 0.6
 Baseline Plateau [s] : 0.5

Filter Settings

Filter Width [s] : 0.5
 Polynomial Order : 4


Ladder

Ladder Peak	Size	Area
1	35	160
2	50	210
3	100	208
4	150	221
5	200	242
6	300	270
7	400	305
8	500	306
9	600	336
10	700	321
11	1000	366
12	2000	413
13	3000	411
14	7000	400
15	10380	214

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...sitivity DNA Assay_DE34903152_2023-08-14_001_PB972_Libs.xad

Created: 8/14/2023 10:10:19 AM
 Modified: 8/14/2023 10:55:09 AM

Electropherogram Summary

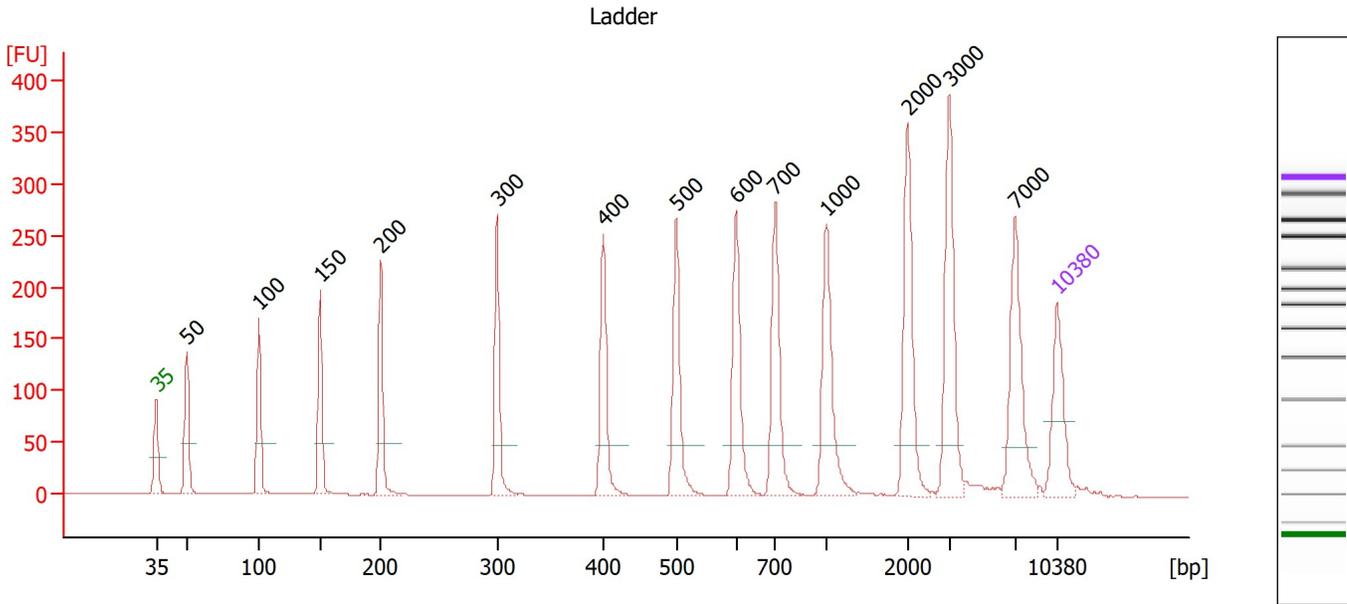

Overall Results for Ladder

Noise: 0.2

Peak table for Ladder


Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	50	150.00	4,545.5	Ladder Peak
3	100	150.00	2,272.7	Ladder Peak
4	150	150.00	1,515.2	Ladder Peak
5	200	150.00	1,136.4	Ladder Peak
6	300	150.00	757.6	Ladder Peak
7	400	150.00	568.2	Ladder Peak
8	500	150.00	454.5	Ladder Peak
9	600	150.00	378.8	Ladder Peak
10	700	150.00	324.7	Ladder Peak
11	1,000	150.00	227.3	Ladder Peak
12	2,000	150.00	113.6	Ladder Peak
13	3,000	150.00	75.8	Ladder Peak
14	7,000	150.00	32.5	Ladder Peak
15	10,380	75.00	10.9	Upper Marker

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...sitivity DNA Assay_DE34903152_2023-08-14_001_PB972_Libs.xad

Created: 8/14/2023 10:10:19 AM
 Modified: 8/14/2023 10:55:09 AM

Electropherogram Summary Continued ...

PB972_01_SubLib1_10XSc-Split-Seq/Amplicon_Lib

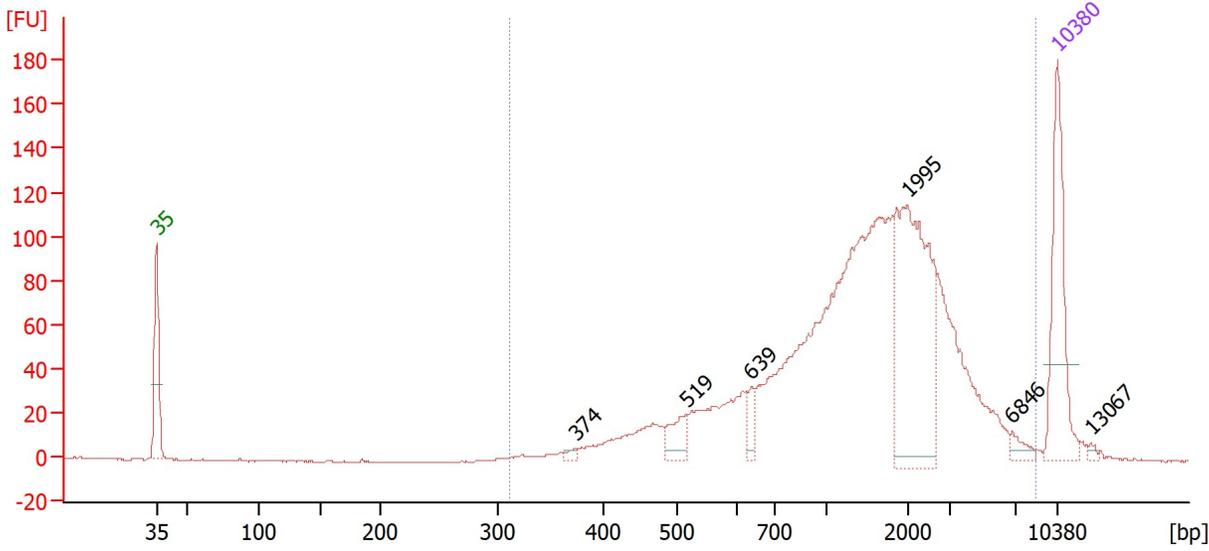

Overall Results for sample 1 : PB972_01_SubLib1_10XSc-Split-Seq/Amplicon_Lib

Number of peaks found: 6 Corr. Area 1: 1,706.7
 Noise: 0.2

Peak table for sample 1 : PB972_01_SubLib1_10XSc-Split-Seq/Amplicon_Lib

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	374	4.39	17.8	
3	519	23.78	69.4	
4	639	12.79	30.3	
5	1,995	161.00	122.3	
6	6,846	7.38	1.6	
7	10,380	75.00	10.9	Upper Marker
8	13,067	0.00	0.0	


Region table for sample 1 : PB972_01_SubLib1_10XSc-Split-Seq/Amplicon_Lib

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
312	8,648	1,706.7	99	1,768	72.4	875.03	1,276.7	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...sitivity DNA Assay_DE34903152_2023-08-14_001_PB972_Libs.xad

Created: 8/14/2023 10:10:19 AM
 Modified: 8/14/2023 10:55:09 AM

Electropherogram Summary Continued ...

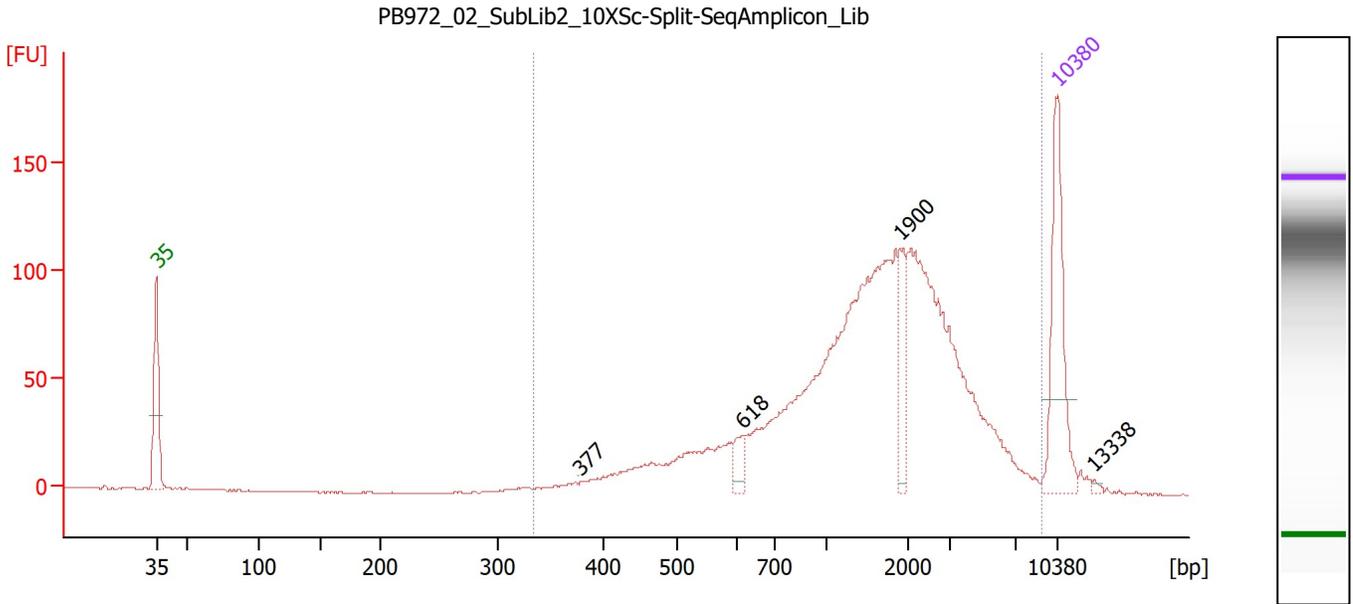

Overall Results for sample 2 : PB972_02_SubLib2_10XSc-Split-SeqAmplicon_Lib

Number of peaks found: 4 Corr. Area 1: 1,633.7
 Noise: 0.3

Peak table for sample 2 : PB972_02_SubLib2_10XSc-Split-SeqAmplicon_Lib

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	377	0.17	0.7	
3	618	14.71	36.1	
4	1,900	32.55	26.0	
5	10,380	75.00	10.9	Upper Marker
6	13,338	0.00	0.0	


Region table for sample 2 : PB972_02_SubLib2_10XSc-Split-SeqAmplicon_Lib

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
334	9,050	1,633.7	99	1,942	73.3	793.52	1,075.5	Blue

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...sitivity DNA Assay_DE34903152_2023-08-14_001_PB972_Libs.xad

Created: 8/14/2023 10:10:19 AM
Modified: 8/14/2023 10:55:09 AM

Gel Image

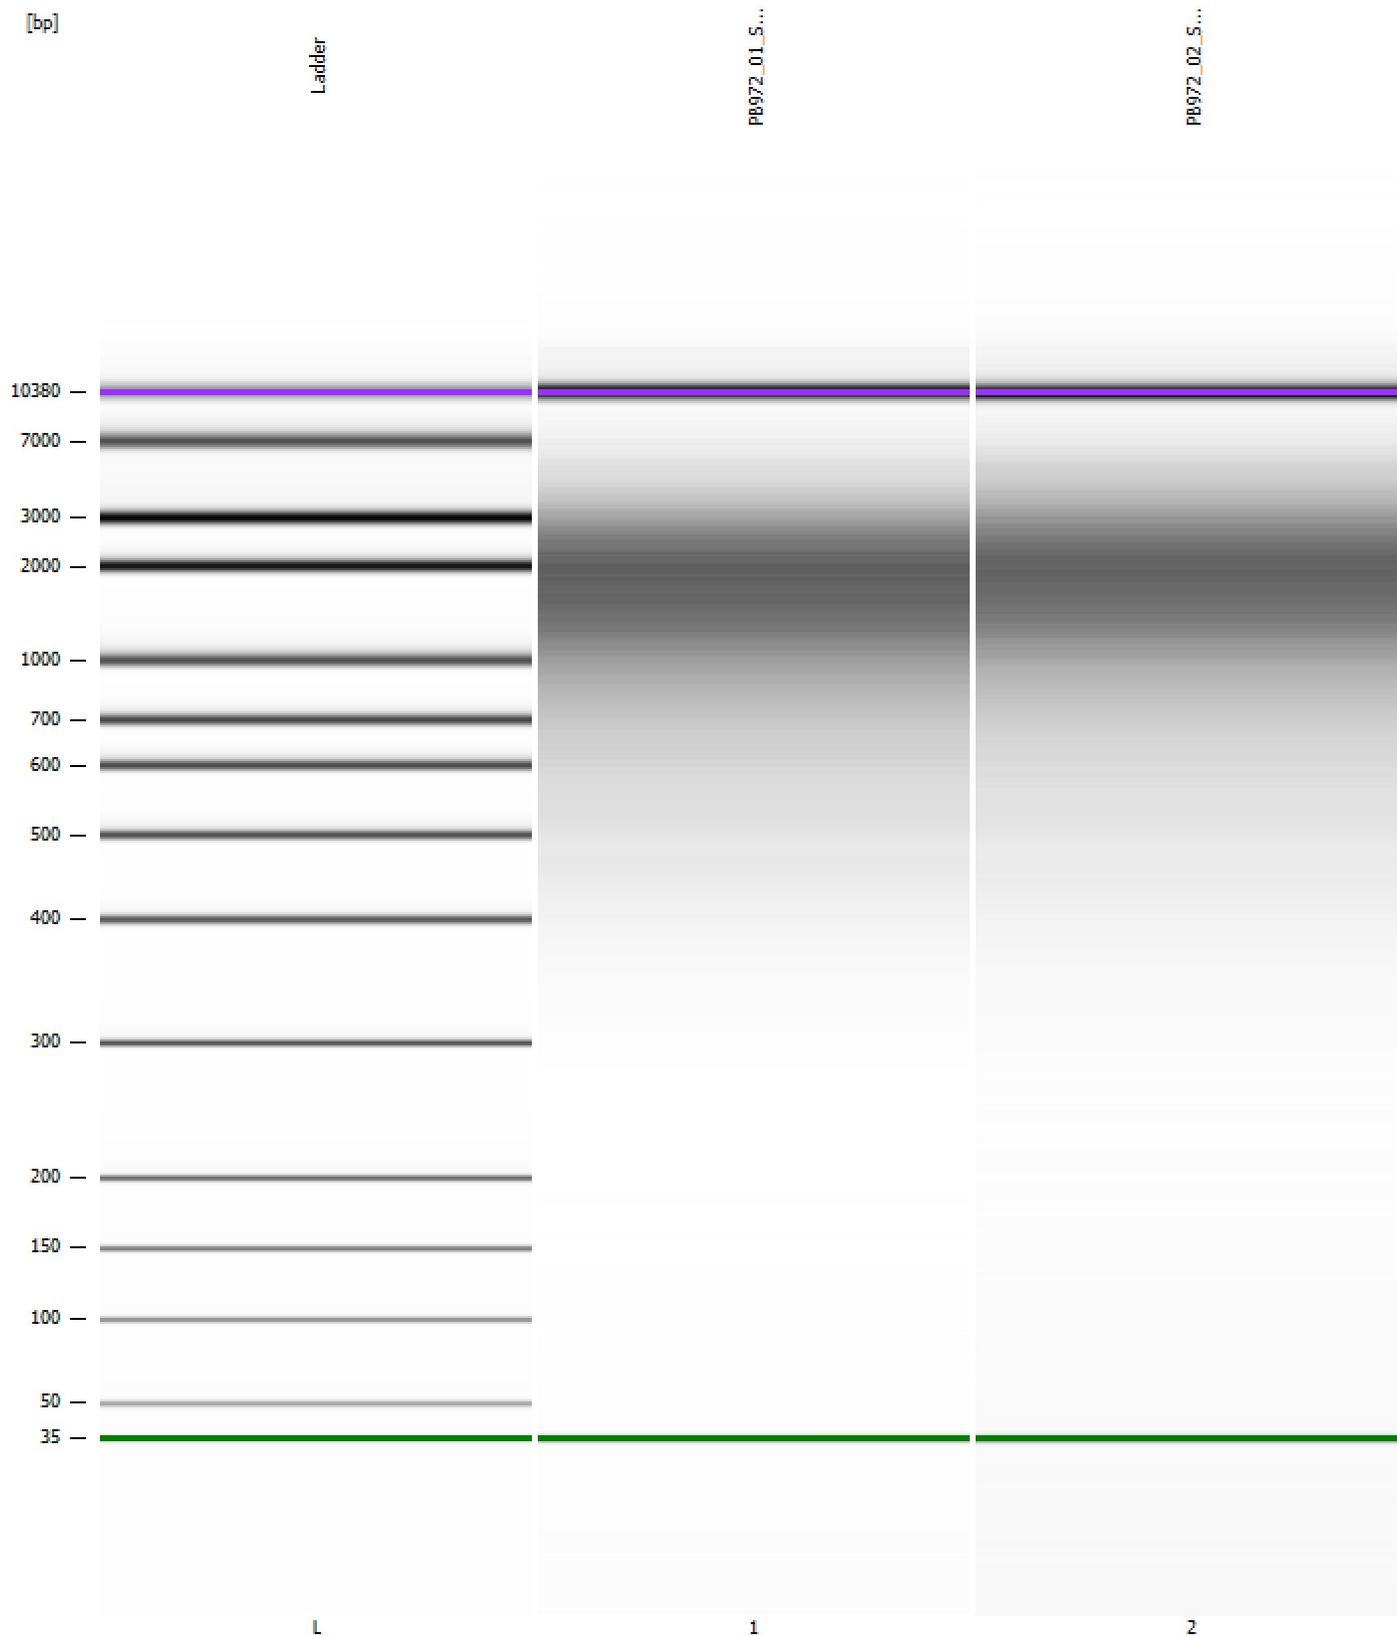


Assay Class: High Sensitivity DNA Assay
Data Path: C:\...sitivity DNA Assay_DE34903152_2023-08-14_001_PB972_Libs.xad

Created: 8/14/2023 10:10:19 AM
Modified: 8/14/2023 10:55:09 AM

Curves

Standard Curve

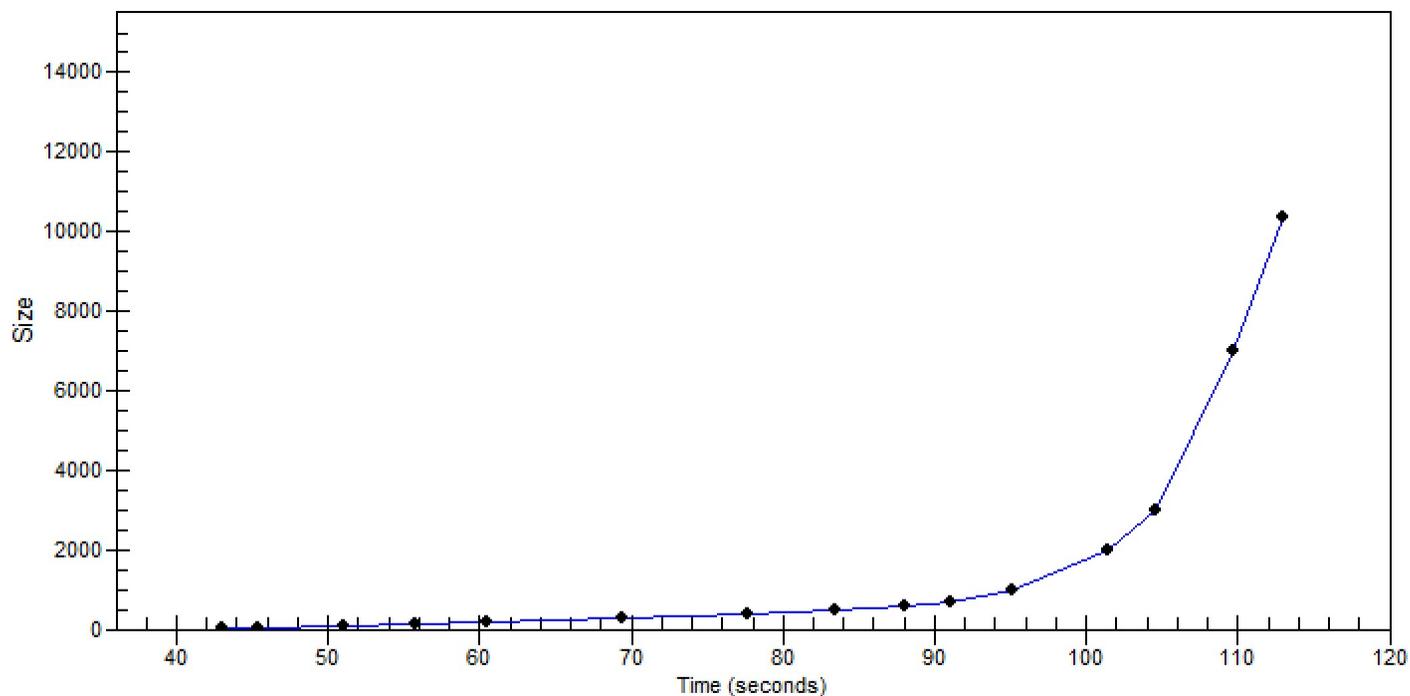

Assay Class: High Sensitivity DNA Assay Created: 8/14/2023 10:10:19 AM
 Data Path: C:\...sitivity DNA Assay_DE34903152_2023-08-14_001_PB972_Libs.xad Modified: 8/14/2023 10:55:09 AM

Run Logbook

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 8)		Instrument	Run		8/14/2023 10:40:15 AM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Run started on port 1 (File: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\data\2023-08-14\Bioanalyzer1_High Sensitivity DNA Assay_DE34903152_2023-08-14_001.xad)		Instrument	Run		8/14/2023 10:10:26 AM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Product Number : G2938C		Instrument	Run		8/14/2023 10:10:26 AM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Name :		Instrument	Run		8/14/2023 10:10:26 AM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Vendor : Agilent Technologies		Instrument	Run		8/14/2023 10:10:26 AM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Serial# : DE34903152		Instrument	Run		8/14/2023 10:10:26 AM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Firmware : C.01.069		Instrument	Run		8/14/2023 10:10:26 AM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Cartridge : Electrode		Instrument	Run		8/14/2023 10:10:26 AM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB