


Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-01-08_002.xad

Created: 1/8/2025 3:38:39 PM
 Modified: 1/8/2025 4:31:37 PM


Electrophoresis File Run Summary

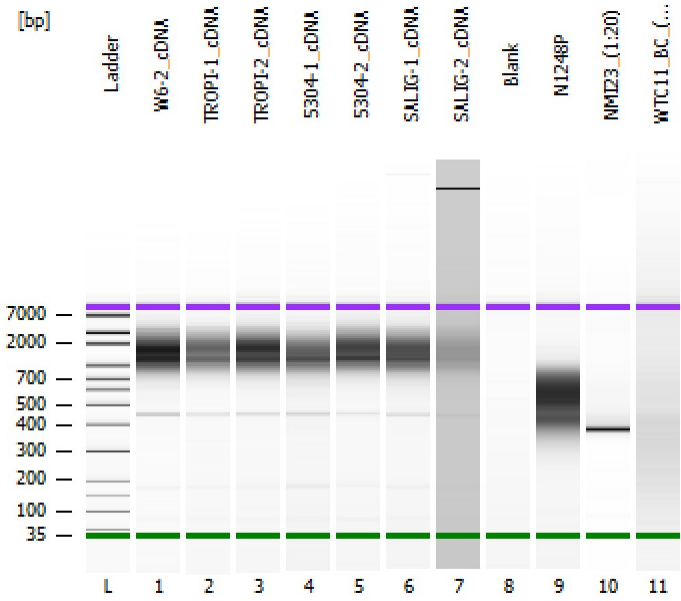

Instrument Information:
 Instrument Name: DE34903152 Firmware: C.01.069
 Serial#: DE34903152 Type: G2938C

Assay Information:
 Assay Origin Path: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy
 Assay Class: High Sensitivity DNA Assay
 Version: 1.03
 Assay Comments: Copyright © 2003-2010 Agilent Technologies

Chip Information:
 Chip Lot #:
 Reagent Kit Lot #:
 Chip Comments:

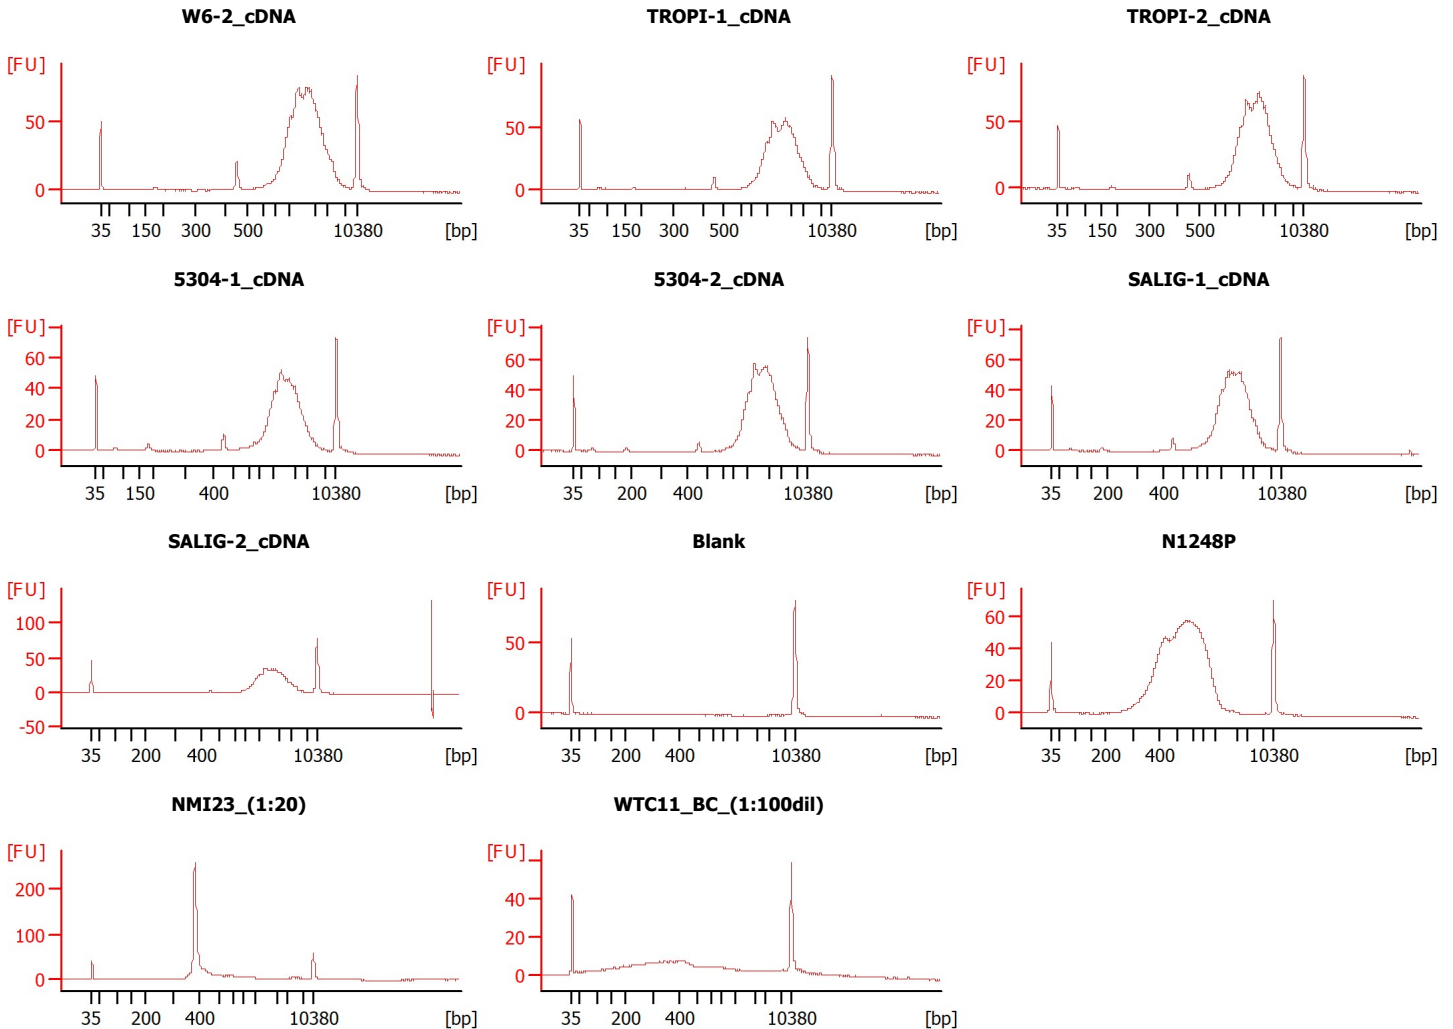

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-01-08_002.xad

Created: 1/8/2025 3:38:39 PM
 Modified: 1/8/2025 4:31:37 PM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
W6-2_cDNA		<input type="checkbox"/>		✓		
TROPI-1_cDNA		<input type="checkbox"/>		✓		
TROPI-2_cDNA		<input type="checkbox"/>		✓		
5304-1_cDNA		<input type="checkbox"/>		✓		
5304-2_cDNA		<input type="checkbox"/>		✓		
SALIG-1_cDNA		<input type="checkbox"/>		✓		
SALIG-2_cDNA		<input type="checkbox"/>		✓		
Blank		<input type="checkbox"/>		✓		
N1248P		<input type="checkbox"/>		✓		
NMI23_(1:20)		<input type="checkbox"/>		✓		
WTC11_BC_(1:100dil)		<input type="checkbox"/>		✓		
Ladder		<input type="checkbox"/>		✓		

Chip Lot #

Reagent Kit Lot #

Chip Comments :

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-01-08_002.xad

Created: 1/8/2025 3:38:39 PM
 Modified: 1/8/2025 4:31:37 PM

Electrophoresis Assay Details

General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12
 Minimum Visible Range [s] : 32
 Maximum Visible Range [s] : 138
 Start Analysis Time Range [s] : 33
 End Analysis Time Range [s] : 137.5
 Ladder Concentration [pg/μl] : 1950
 Uses Standard Area for Ladder Fragments
 Lower Marker Concentration [pg/μl] : 125
 Upper Marker Concentration [pg/μl] : 75
 Used Upper Marker for Quantitation
 Standard Curve Fit is Point to Point
 Show Data Aligned to Lower and Upper Marker

Integrator Settings

Integration Start Time [s] : 33.05
 Integration End Time [s] : 137
 Slope Threshold : 0.8
 Height Threshold [FU] : 5
 Area Threshold : 0.1
 Width Threshold [s] : 0.6
 Baseline Plateau [s] : 0.5

Filter Settings

Filter Width [s] : 0.5
 Polynomial Order : 4


Ladder

Ladder Peak	Size	Area
1	35	160
2	50	210
3	100	208
4	150	221
5	200	242
6	300	270
7	400	305
8	500	306
9	600	336
10	700	321
11	1000	366
12	2000	413
13	3000	411
14	7000	400
15	10380	214

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-01-08_002.xad

Created: 1/8/2025 3:38:39 PM
 Modified: 1/8/2025 4:31:37 PM

Electropherogram Summary

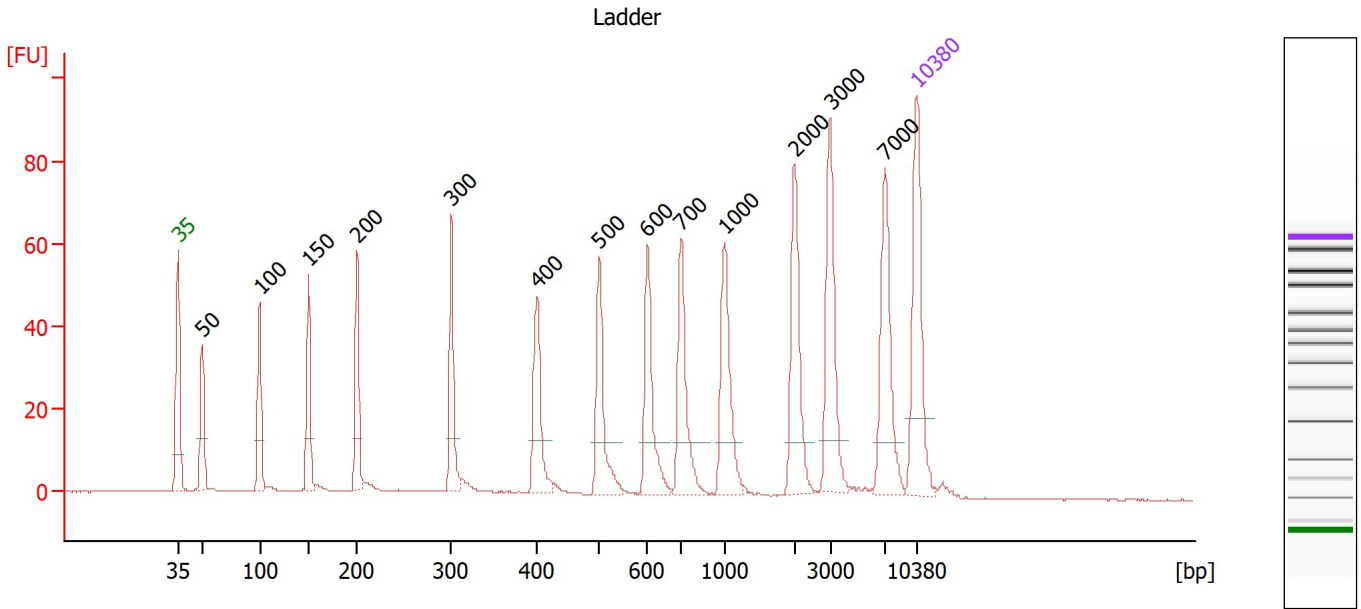

Overall Results for Ladder

Noise: 0.2


Peak table for Ladder

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	50	150.00	4,545.5	Ladder Peak
3	100	150.00	2,272.7	Ladder Peak
4	150	150.00	1,515.2	Ladder Peak
5	200	150.00	1,136.4	Ladder Peak
6	300	150.00	757.6	Ladder Peak
7	400	150.00	568.2	Ladder Peak
8	500	150.00	454.5	Ladder Peak
9	600	150.00	378.8	Ladder Peak
10	700	150.00	324.7	Ladder Peak
11	1,000	150.00	227.3	Ladder Peak
12	2,000	150.00	113.6	Ladder Peak
13	3,000	150.00	75.8	Ladder Peak
14	7,000	150.00	32.5	Ladder Peak
15	10,380	75.00	10.9	Upper Marker

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-01-08_002.xad

Created: 1/8/2025 3:38:39 PM
 Modified: 1/8/2025 4:31:37 PM

Electropherogram Summary Continued ...

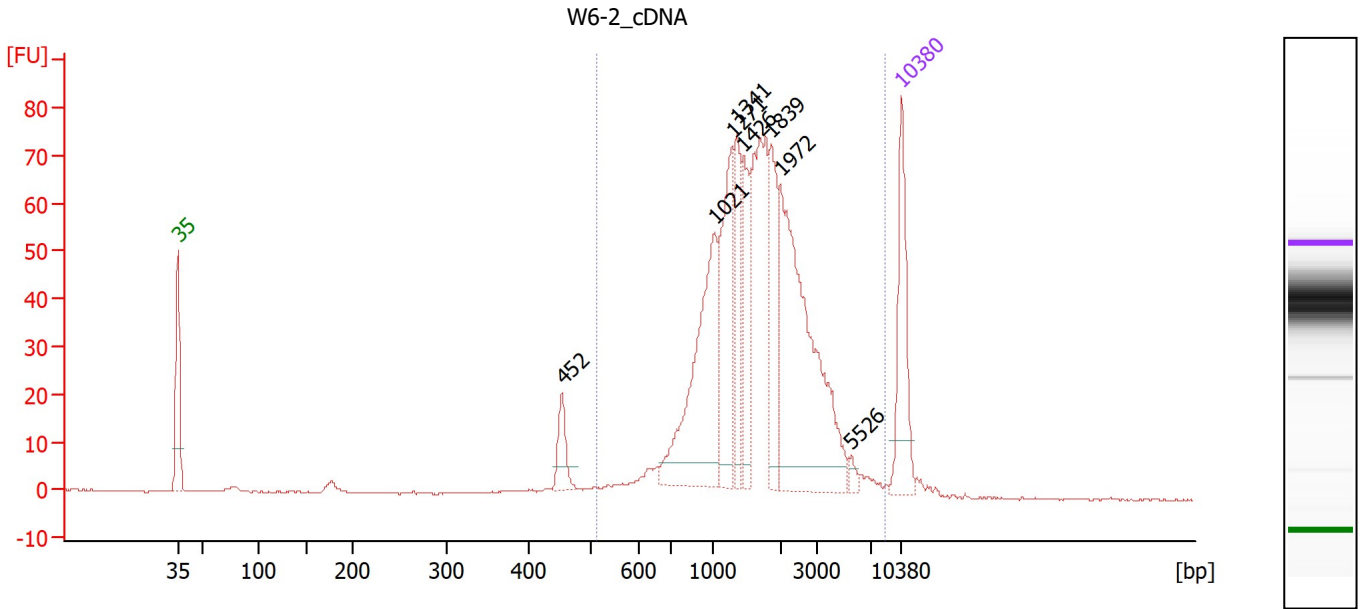

Overall Results for sample 1 : W6-2_cDNA

Number of peaks found: 8 Corr. Area 1: 818.5
 Noise: 0.2

Peak table for sample 1 : W6-2_cDNA

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	452	33.61	112.6	
3	1,021	185.40	275.1	
4	1,271	118.47	141.3	
5	1,341	60.98	68.9	
6	1,426	65.13	69.2	
7	1,839	73.60	60.6	
8	1,972	254.53	195.6	
9	5,526	6.25	1.7	
10	10,380	75.00	10.9	Upper Marker


Region table for sample 1 : W6-2_cDNA

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
513	8,496	818.5	95	1,831	56.9	1,006.79	1,066.8	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-01-08_002.xad

Created: 1/8/2025 3:38:39 PM
 Modified: 1/8/2025 4:31:37 PM

Electropherogram Summary Continued ...

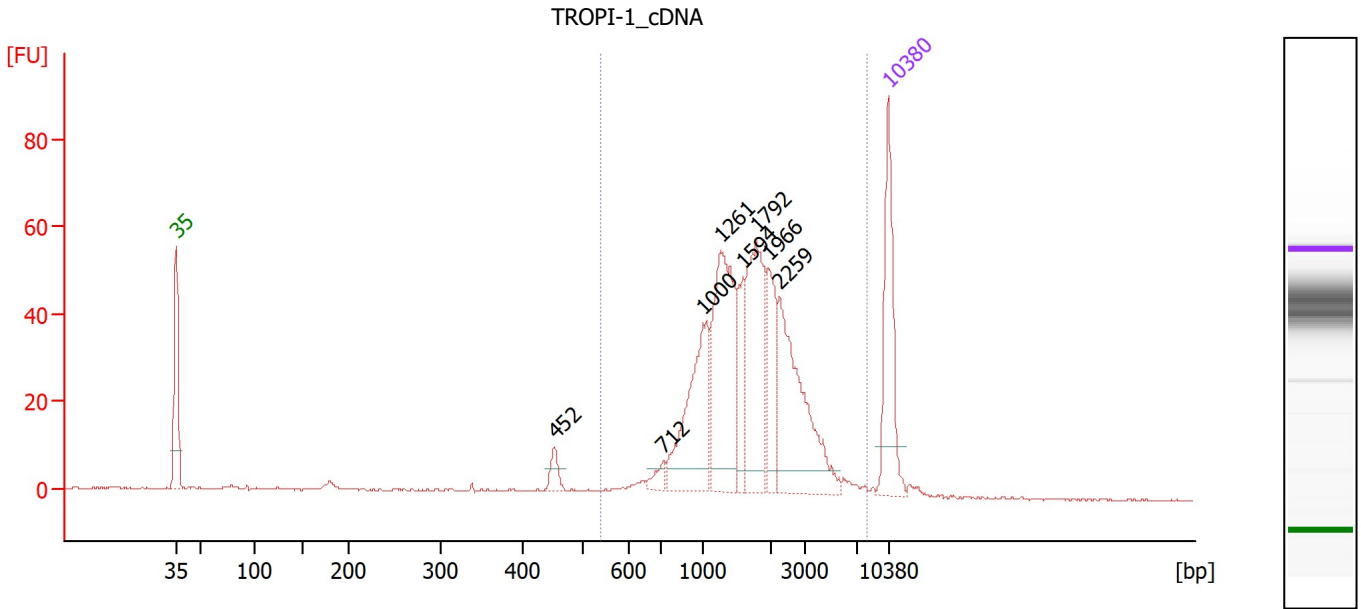

Overall Results for sample 2 : TROPI-1 cDNA

Number of peaks found: 8 Corr. Area 1: 589.3
 Noise: 0.2

Peak table for sample 2 : TROPI-1 cDNA

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	452	14.09	47.2	
3	712	10.62	22.6	
4	1,000	110.15	166.9	
5	1,261	142.69	171.4	
6	1,594	34.04	32.4	
7	1,792	110.06	93.1	
8	1,966	49.91	38.5	
9	2,259	122.08	81.9	
10	10,380	75.00	10.9	Upper Marker


Region table for sample 2 : TROPI-1 cDNA

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
538	7,961	589.3	93	1,838	53.4	628.66	646.4	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-01-08_002.xad

Created: 1/8/2025 3:38:39 PM
 Modified: 1/8/2025 4:31:37 PM

Electropherogram Summary Continued ...

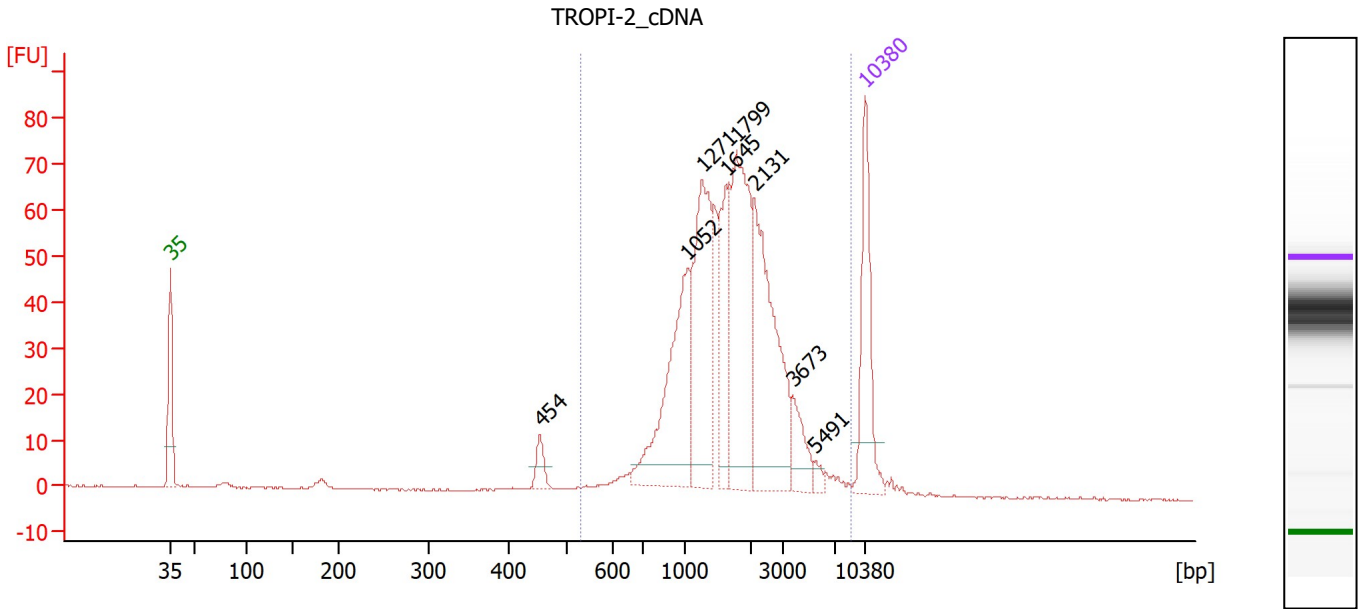

Overall Results for sample 3 : TROPI-2_cDNA

Number of peaks found: 8 Corr. Area 1: 757.9
 Noise: 0.2

Peak table for sample 3 : TROPI-2_cDNA

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	454	17.22	57.4	
3	1,052	141.47	203.7	
4	1,271	144.67	172.4	
5	1,645	73.19	67.4	
6	1,799	154.22	129.9	
7	2,131	156.60	111.3	
8	3,673	28.64	11.8	
9	5,491	5.64	1.6	
10	10,380	75.00	10.9	Upper Marker


Region table for sample 3 : TROPI-2_cDNA

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
531	8,912	757.9	94	1,891	57.5	807.19	824.1	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-01-08_002.xad

Created: 1/8/2025 3:38:39 PM
 Modified: 1/8/2025 4:31:37 PM

Electropherogram Summary Continued ...

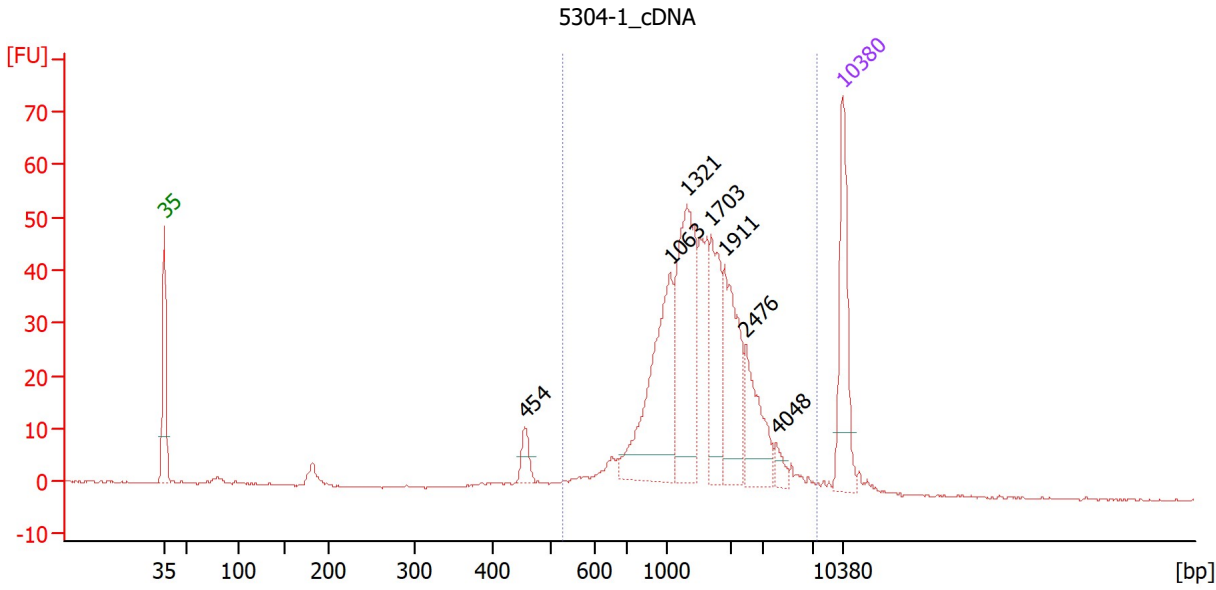

Overall Results for sample 4 : 5304-1 cDNA

Number of peaks found: 7 Corr. Area 1: 528.8
 Noise: 0.2

Peak table for sample 4 : 5304-1 cDNA

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	454	19.27	64.3	
3	1,063	151.51	215.9	
4	1,321	156.47	179.5	
5	1,703	75.57	67.2	
6	1,911	91.05	72.2	
7	2,476	57.69	35.3	
8	4,048	10.12	3.8	
9	10,380	75.00	10.9	Upper Marker


Region table for sample 4 : 5304-1 cDNA

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
526	7,512	528.8	91	1,704	55.1	701.66	788.9	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-01-08_002.xad

Created: 1/8/2025 3:38:39 PM
 Modified: 1/8/2025 4:31:37 PM

Electropherogram Summary Continued ...

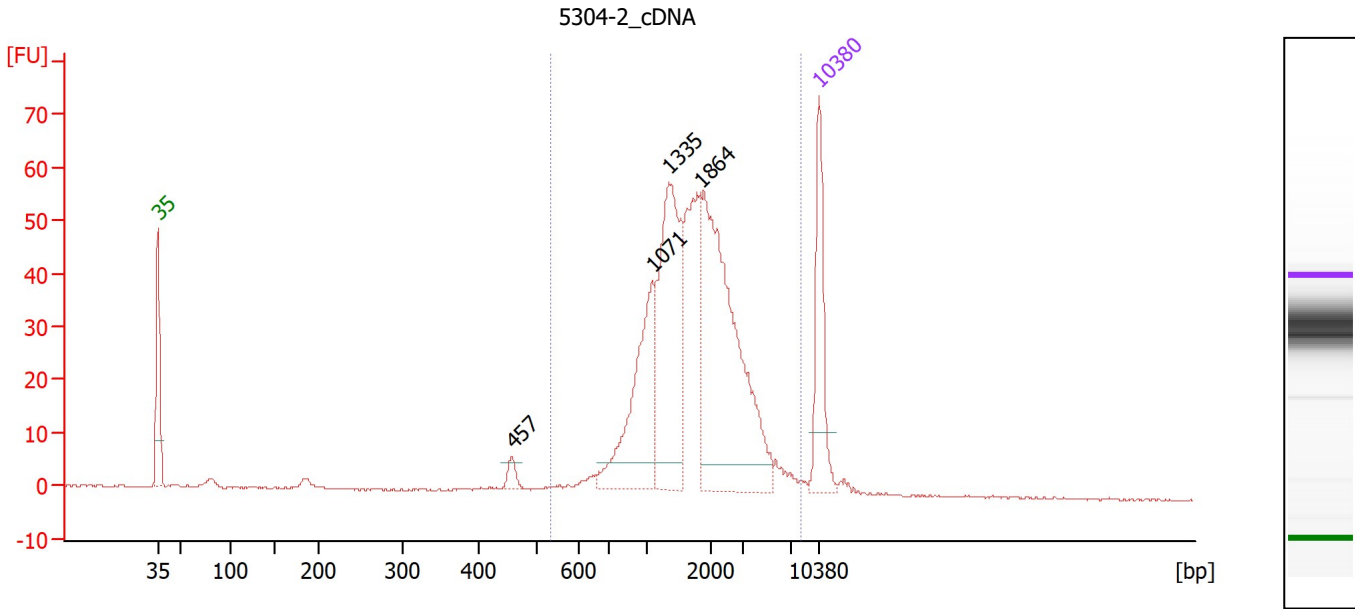

Overall Results for sample 5 : 5304-2_cDNA

Number of peaks found: 4 Corr. Area 1: 605.6
 Noise: 0.2

Peak table for sample 5 : 5304-2_cDNA

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	457	11.90	39.4	
3	1,071	139.29	197.1	
4	1,335	186.52	211.7	
5	1,864	282.46	229.6	
6	10,380	75.00	10.9	Upper Marker


Region table for sample 5 : 5304-2_cDNA

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
533	8,242	605.6	95	1,939	56.3	790.06	784.3	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-01-08_002.xad

Created: 1/8/2025 3:38:39 PM
 Modified: 1/8/2025 4:31:37 PM

Electropherogram Summary Continued ...

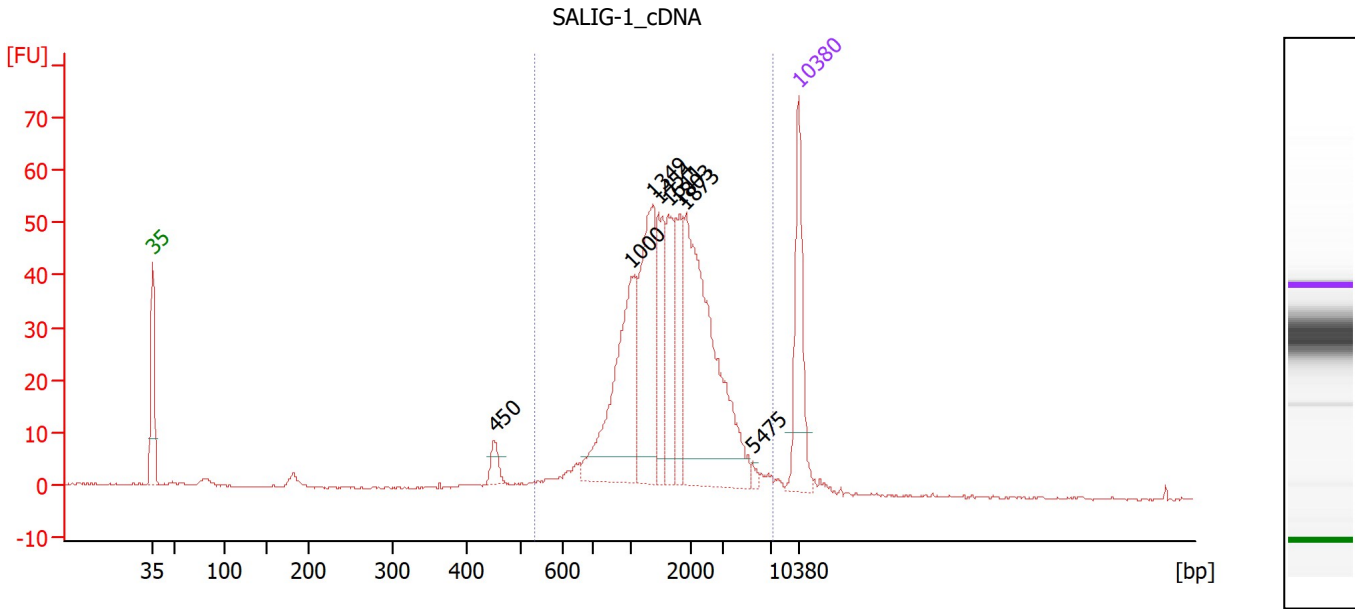

Overall Results for sample 6 : SALIG-1_cDNA

Number of peaks found: 8 Corr. Area 1: 597.8
 Noise: 0.2

Peak table for sample 6 : SALIG-1_cDNA

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	450	15.71	52.9	
3	1,000	163.88	248.2	
4	1,349	128.80	144.6	
5	1,454	65.21	68.0	
6	1,611	59.84	56.3	
7	1,803	54.46	45.8	
8	1,873	237.93	192.5	
9	5,475	4.12	1.1	
10	10,380	75.00	10.9	Upper Marker


Region table for sample 6 : SALIG-1_cDNA

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
530	7,160	597.8	93	1,798	54.5	798.18	858.9	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-01-08_002.xad

Created: 1/8/2025 3:38:39 PM
 Modified: 1/8/2025 4:31:37 PM

Electropherogram Summary Continued ...

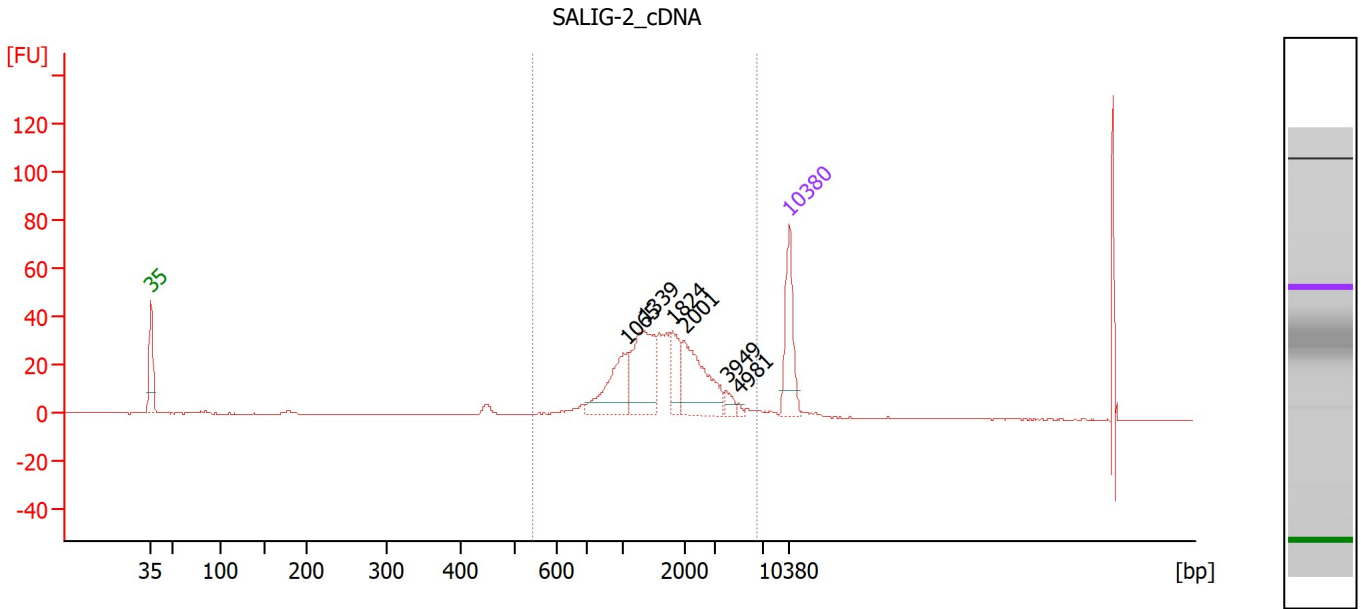

Overall Results for sample 7 : SALIG-2_cDNA

Number of peaks found: 6 Corr. Area 1: 381.9
 Noise: 0.2

Peak table for sample 7 : SALIG-2_cDNA

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	1,065	91.52	130.2	
3	1,339	117.10	132.5	
4	1,824	46.18	38.4	
5	2,001	105.15	79.6	
6	3,949	12.54	4.8	
7	4,981	3.16	1.0	
8	10,380	75.00	10.9	Upper Marker


Region table for sample 7 : SALIG-2_cDNA

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
540	6,616	381.9	89	1,810	52.9	477.34	503.5	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-01-08_002.xad

Created: 1/8/2025 3:38:39 PM
 Modified: 1/8/2025 4:31:37 PM

Gel Image

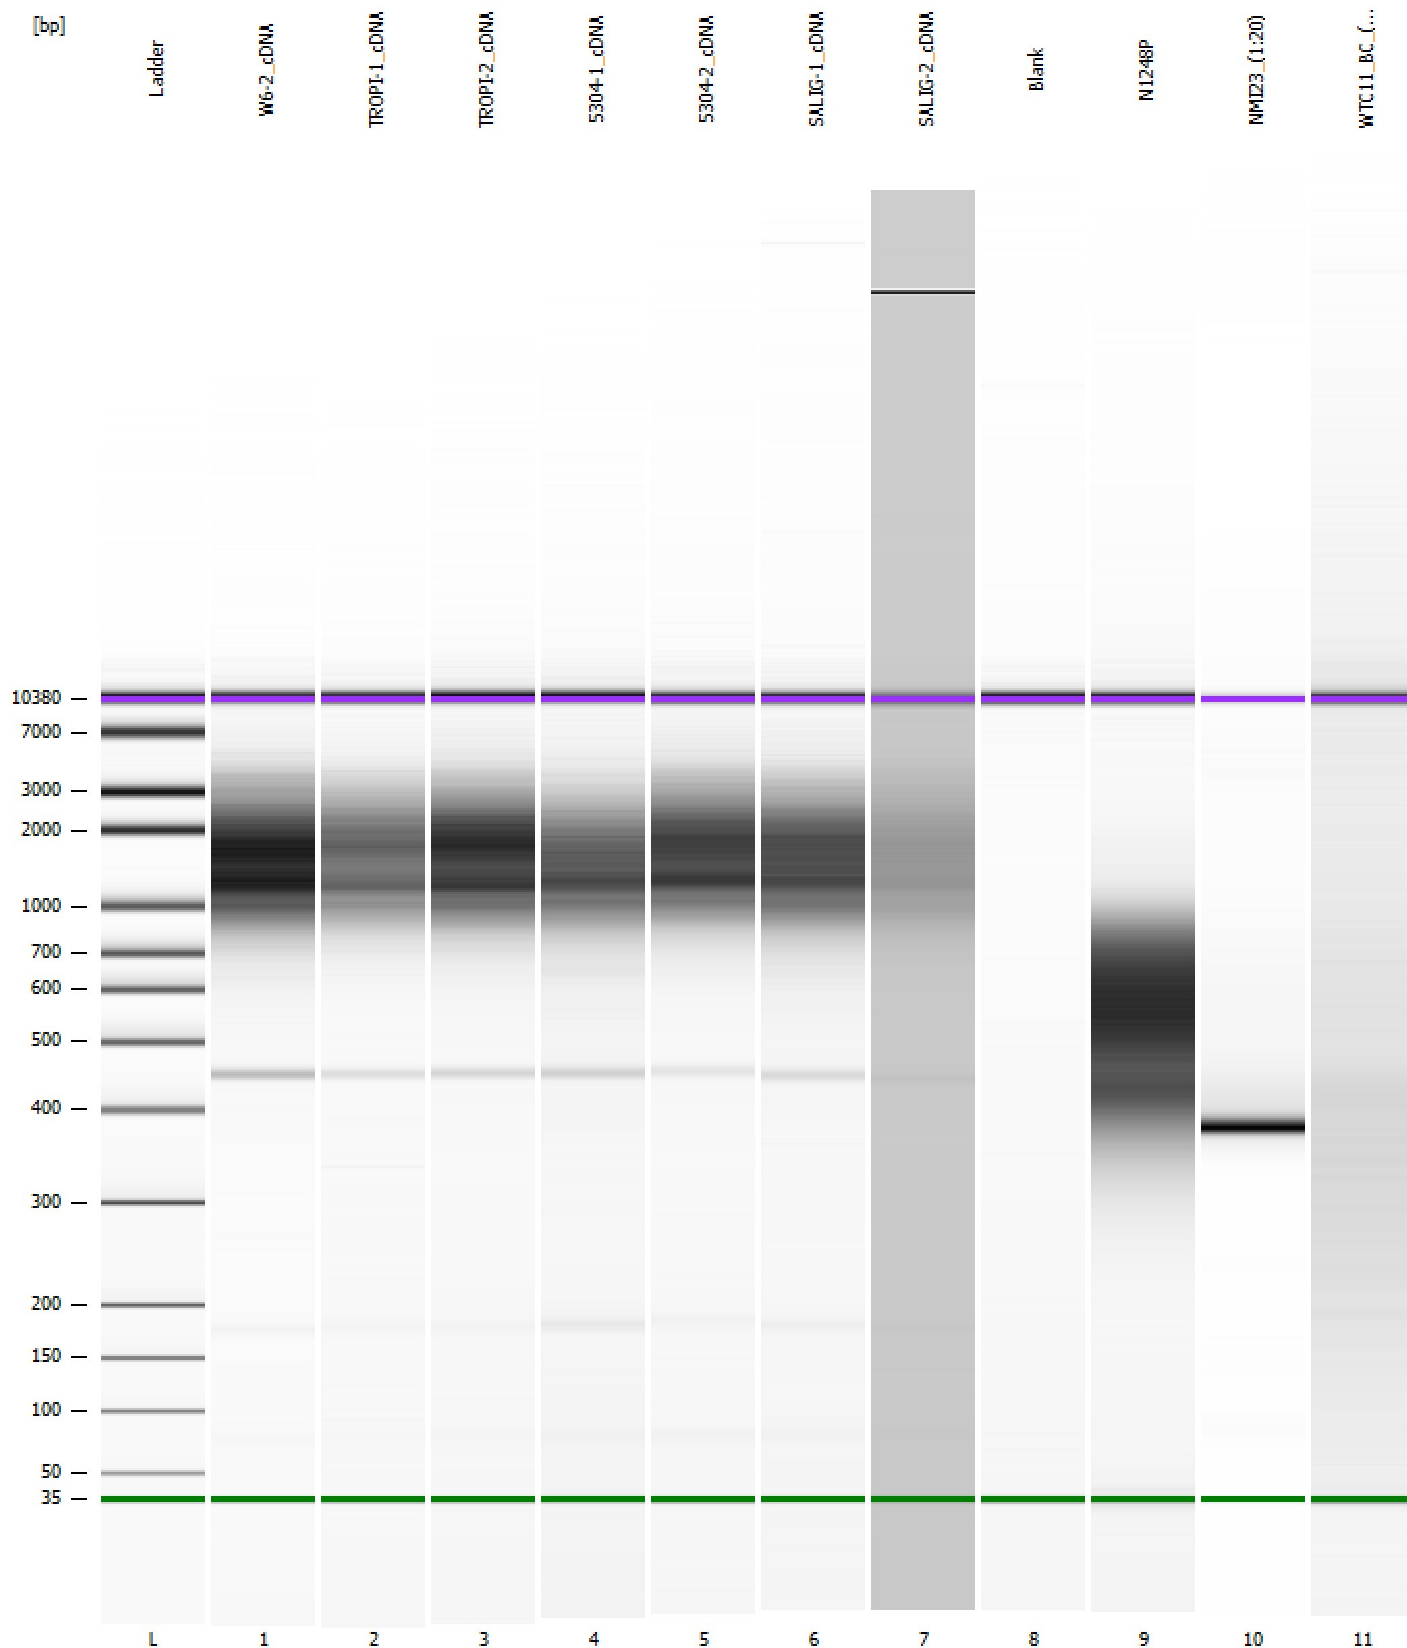

Assay Class: High Sensitivity DNA Assay Created: 1/8/2025 3:38:39 PM
 Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-01-08_002.xad Modified: 1/8/2025 4:31:37 PM

Run Logbook

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 12)		Instrument	Run		1/8/2025 4:19:08 PM	(GMT --08:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Run started on port 1 (File: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\data\2025-01-08\Bioanalyzer1_High Sensitivity DNA Assay_DE34903152_2025-01-08_002.xad)		Instrument	Run		1/8/2025 3:38:45 PM	(GMT --08:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Product Number : G2938C		Instrument	Run		1/8/2025 3:38:45 PM	(GMT --08:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Name :		Instrument	Run		1/8/2025 3:38:45 PM	(GMT --08:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Vendor : Agilent Technologies		Instrument	Run		1/8/2025 3:38:45 PM	(GMT --08:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Serial# : DE34903152		Instrument	Run		1/8/2025 3:38:45 PM	(GMT --08:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Firmware : C.01.069		Instrument	Run		1/8/2025 3:38:45 PM	(GMT --08:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Cartridge : Electrode		Instrument	Run		1/8/2025 3:38:45 PM	(GMT --08:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB