


Assay Class: High Sensitivity DNA Assay
Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-10-20_003.xad

Created: 10/20/2025 5:00:25 PM
Modified: 10/20/2025 5:43:24 PM

Electrophoresis File Run Summary

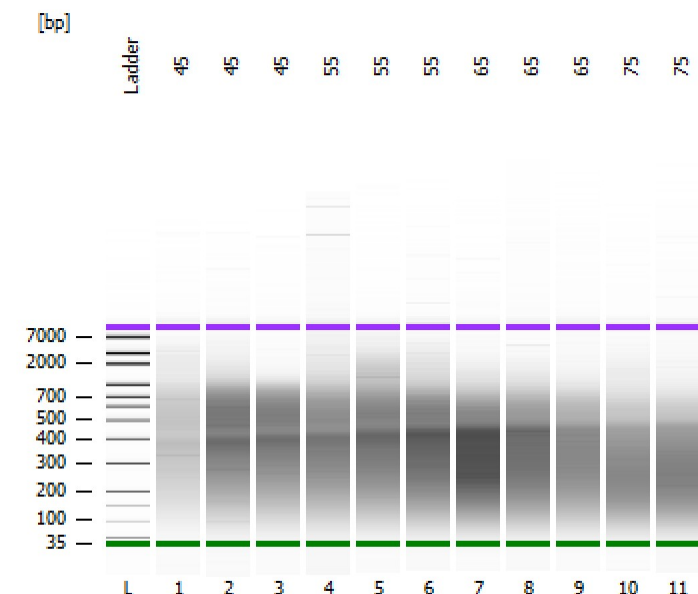

Instrument Information:


Instrument Name: DE34903152
Serial#: DE34903152
Firmware: C.01.069
Type: G2938C

Assay Information:

Assay Origin Path: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy
Assay Class: High Sensitivity DNA Assay
Version: 1.03
Assay Comments: Copyright © 2003-2010 Agilent Technologies

Chip Information:

Chip Lot #:
Reagent Kit Lot #:
Chip Comments:

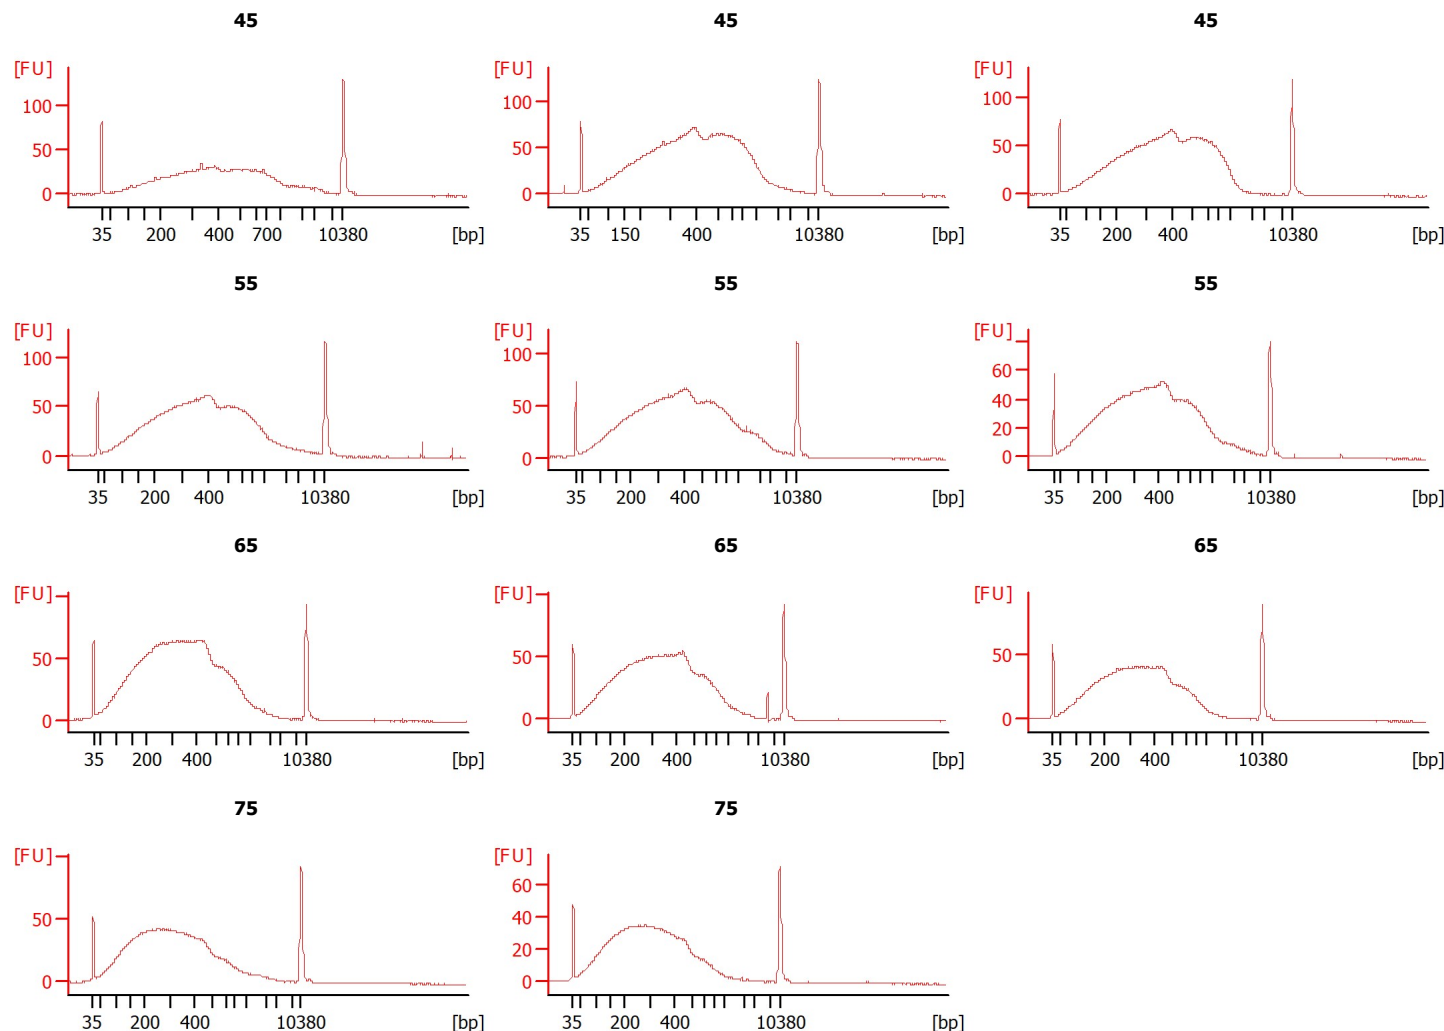

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-10-20_003.xad

Created: 10/20/2025 5:00:25 PM
 Modified: 10/20/2025 5:43:24 PM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
45		☐	✓			
45		☐	✓			
45		☐	✓			
55		☐	✓			
55		☐	✓			
55		☐	✓			
65		☐	✓			
65		☐	✓			
65		☐	✓			
75		☐	✓			
75		☐	✓			
Ladder		☐	✓			

Chip Lot #

Reagent Kit Lot #

Chip Comments :

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-10-20_003.xad

Created: 10/20/2025 5:00:25 PM
 Modified: 10/20/2025 5:43:24 PM

Electrophoresis Assay Details

General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12
 Minimum Visible Range [s] : 32
 Maximum Visible Range [s] : 138
 Start Analysis Time Range [s] : 33
 End Analysis Time Range [s] : 137.5
 Ladder Concentration [pg/μl] : 1950
 Uses Standard Area for Ladder Fragments
 Lower Marker Concentration [pg/μl] : 125
 Upper Marker Concentration [pg/μl] : 75
 Used Upper Marker for Quantitation
 Standard Curve Fit is Point to Point
 Show Data Aligned to Lower and Upper Marker

Integrator Settings

Integration Start Time [s] : 33.05
 Integration End Time [s] : 137
 Slope Threshold : 0.8
 Height Threshold [FU] : 5
 Area Threshold : 0.1
 Width Threshold [s] : 0.6
 Baseline Plateau [s] : 0.5

Filter Settings

Filter Width [s] : 0.5
 Polynomial Order : 4


Ladder

Ladder Peak	Size	Area
1	35	160
2	50	210
3	100	208
4	150	221
5	200	242
6	300	270
7	400	305
8	500	306
9	600	336
10	700	321
11	1000	366
12	2000	413
13	3000	411
14	7000	400
15	10380	214

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-10-20_003.xad

Created: 10/20/2025 5:00:25 PM
 Modified: 10/20/2025 5:43:24 PM

Electropherogram Summary

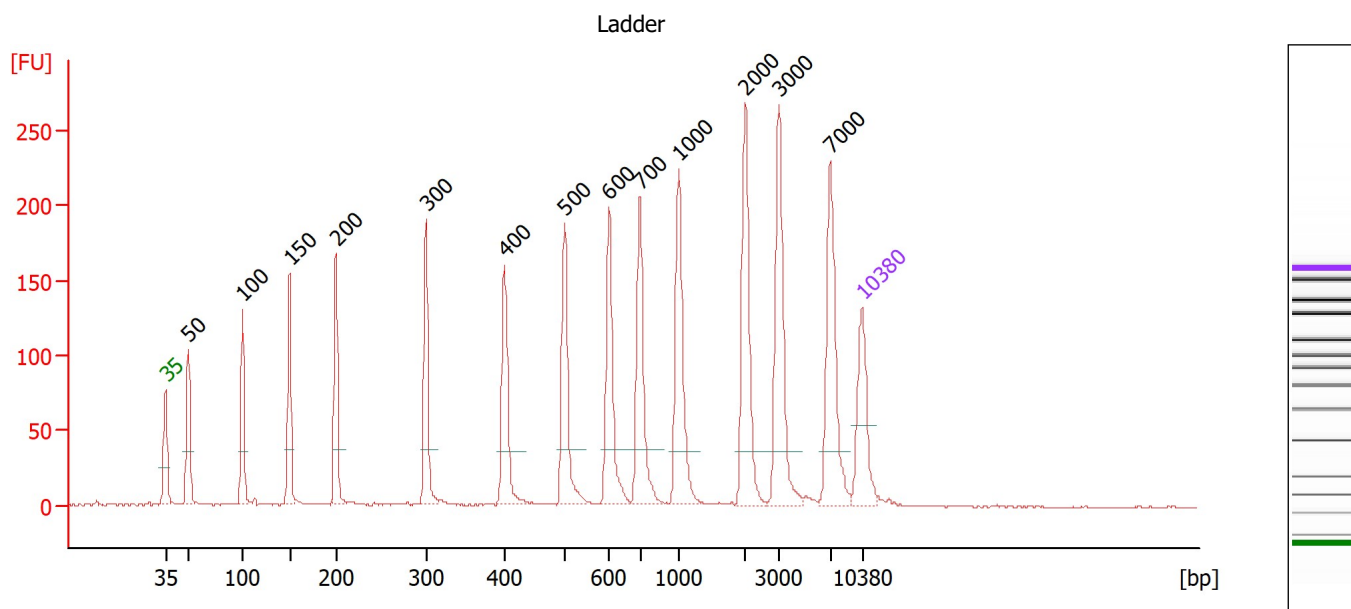

Overall Results for Ladder

Noise: 0.3


Peak table for Ladder

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	50	150.00	4,545.5	Ladder Peak
3	100	150.00	2,272.7	Ladder Peak
4	150	150.00	1,515.2	Ladder Peak
5	200	150.00	1,136.4	Ladder Peak
6	300	150.00	757.6	Ladder Peak
7	400	150.00	568.2	Ladder Peak
8	500	150.00	454.5	Ladder Peak
9	600	150.00	378.8	Ladder Peak
10	700	150.00	324.7	Ladder Peak
11	1,000	150.00	227.3	Ladder Peak
12	2,000	150.00	113.6	Ladder Peak
13	3,000	150.00	75.8	Ladder Peak
14	7,000	150.00	32.5	Ladder Peak
15	10,380	75.00	10.9	Upper Marker

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-10-20_003.xad

Created: 10/20/2025 5:00:25 PM
 Modified: 10/20/2025 5:43:24 PM

Electropherogram Summary Continued ...

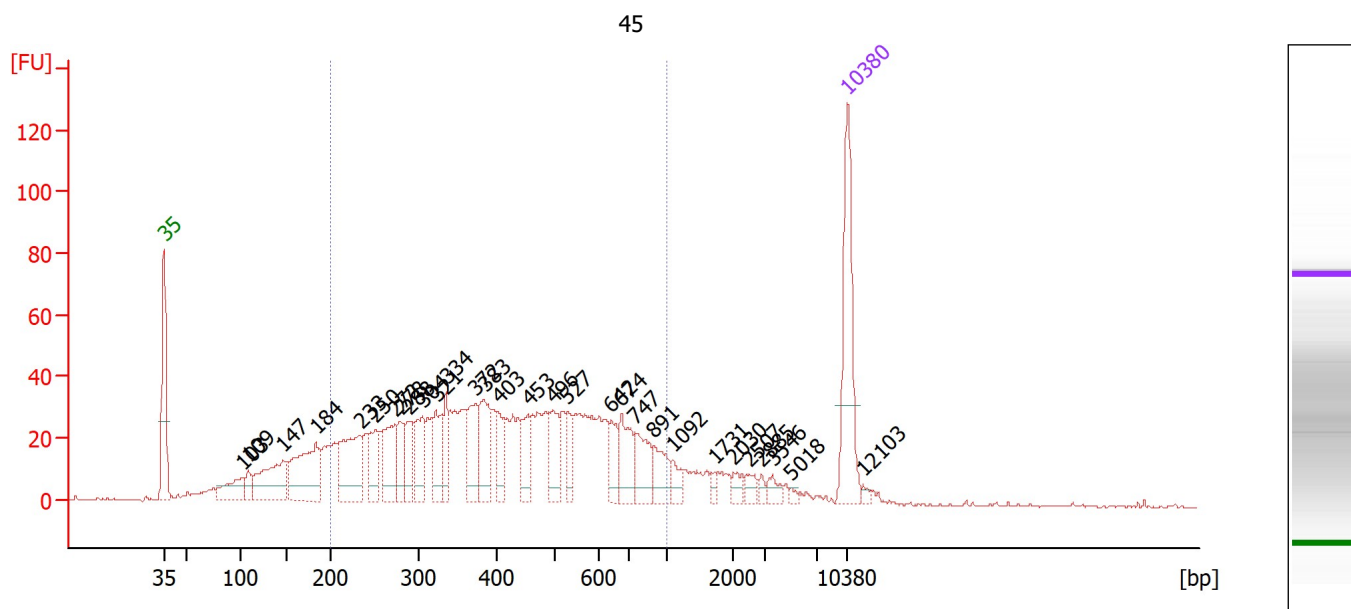

Overall Results for sample 1 : 45

Number of peaks found: 30 Corr. Area 1: 1,151.3
 Noise: 0.4

Peak table for sample 1 : 45

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	103	38.75	571.3	
3	109	14.50	201.3	
4	147	76.83	793.0	
5	184	95.45	787.4	
6	233	83.39	543.1	
7	250	36.89	223.5	
8	272	52.62	292.6	
9	278	28.64	156.1	
10	288	30.37	160.0	
11	304	40.40	201.5	
12	321	36.87	174.0	
13	334	28.52	129.3	
14	372	42.51	173.0	
15	383	44.25	174.8	
16	403	22.43	84.4	
17	453	27.47	91.8	
18	496	34.66	105.9	
19	527	20.38	58.5	
20	642	21.46	50.6	
21	674	36.56	82.2	
22	747	33.77	68.5	
23	891	23.40	39.8	
24	1,092	11.48	15.9	
25	1,731	5.13	4.5	
26	2,030	7.40	5.5	

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-10-20_003.xad

Created: 10/20/2025 5:00:25 PM
 Modified: 10/20/2025 5:43:24 PM

Electropherogram Summary Continued ...

... Peak table for sample 1 : 45

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
27	2,507	7.36	4.5	
28	2,885	3.99	2.1	
29	3,546	7.24	3.1	
30	5,018	2.41	0.7	
31	10,380	75.00	10.9	Upper Marker
32	12,103	0.00	0.0	


Region table for sample 1 : 45

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	1,151.3	74	444	39.5	1,061.03	4,452.4	

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-10-20_003.xad

Created: 10/20/2025 5:00:25 PM
 Modified: 10/20/2025 5:43:24 PM

Electropherogram Summary Continued ...

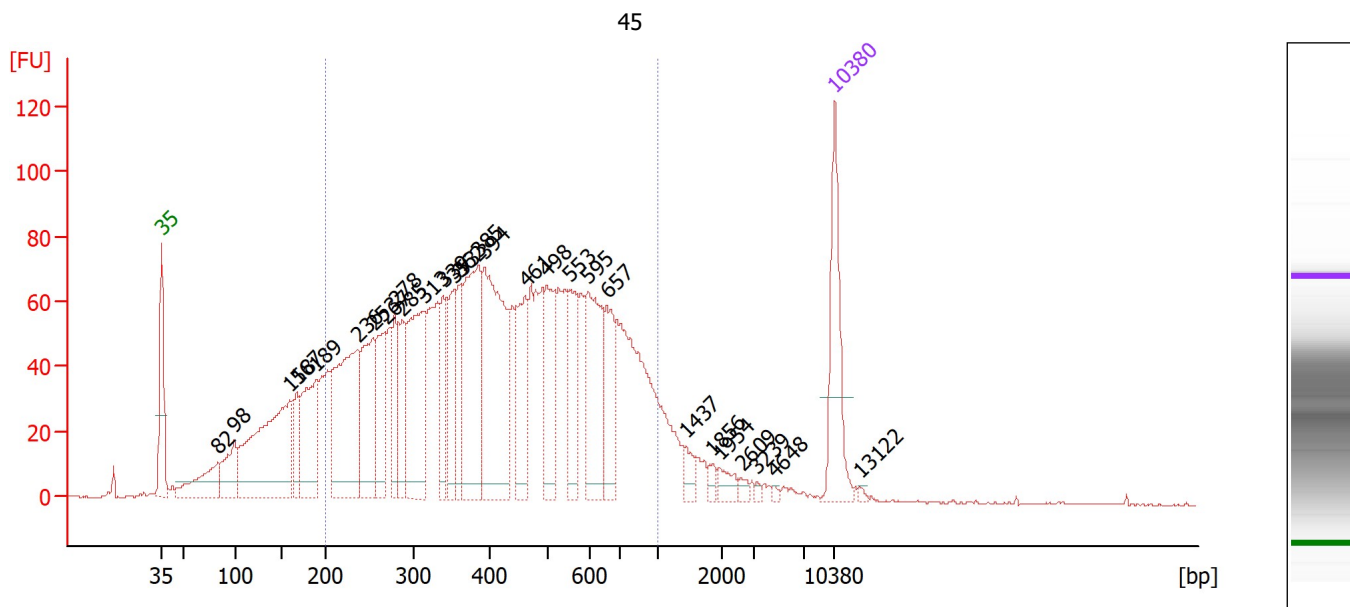

Overall Results for sample 2 : 45

Number of peaks found: 28 Corr. Area 1: 2,467.2
 Noise: 0.2

Peak table for sample 2 : 45

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	82	72.28	1,331.9	
3	98	59.84	925.5	
4	158	265.91	2,544.4	
5	167	45.97	417.9	
6	189	121.35	974.4	
7	236	212.88	1,369.3	
8	253	117.86	704.9	
9	267	82.06	466.0	
10	278	58.78	319.9	
11	285	57.92	307.7	
12	313	168.81	816.5	
13	339	58.14	260.1	
14	353	62.13	266.9	
15	362	58.38	244.4	
16	385	167.34	658.3	
17	394	215.19	828.4	
18	461	80.66	264.9	
19	498	76.02	231.3	
20	553	62.36	170.8	
21	595	112.71	287.2	
22	657	59.14	136.5	
23	1,437	13.25	14.0	
24	1,856	6.75	5.5	
25	1,954	12.18	9.4	
26	2,609	4.92	2.9	

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-10-20_003.xad

Created: 10/20/2025 5:00:25 PM
 Modified: 10/20/2025 5:43:24 PM

Electropherogram Summary Continued ...

... Peak table for sample 2 : 45

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
27	3,239	2.47	1.2	
28	4,648	2.02	0.7	
29	10,380	75.00	10.9	Upper Marker
30	13,122	0.00	0.0	


Region table for sample 2 : 45

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	2,467.2	78	447	39.1	2,338.10	9,728.2	

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-10-20_003.xad

Created: 10/20/2025 5:00:25 PM
Modified: 10/20/2025 5:43:24 PM

Electropherogram Summary Continued ...

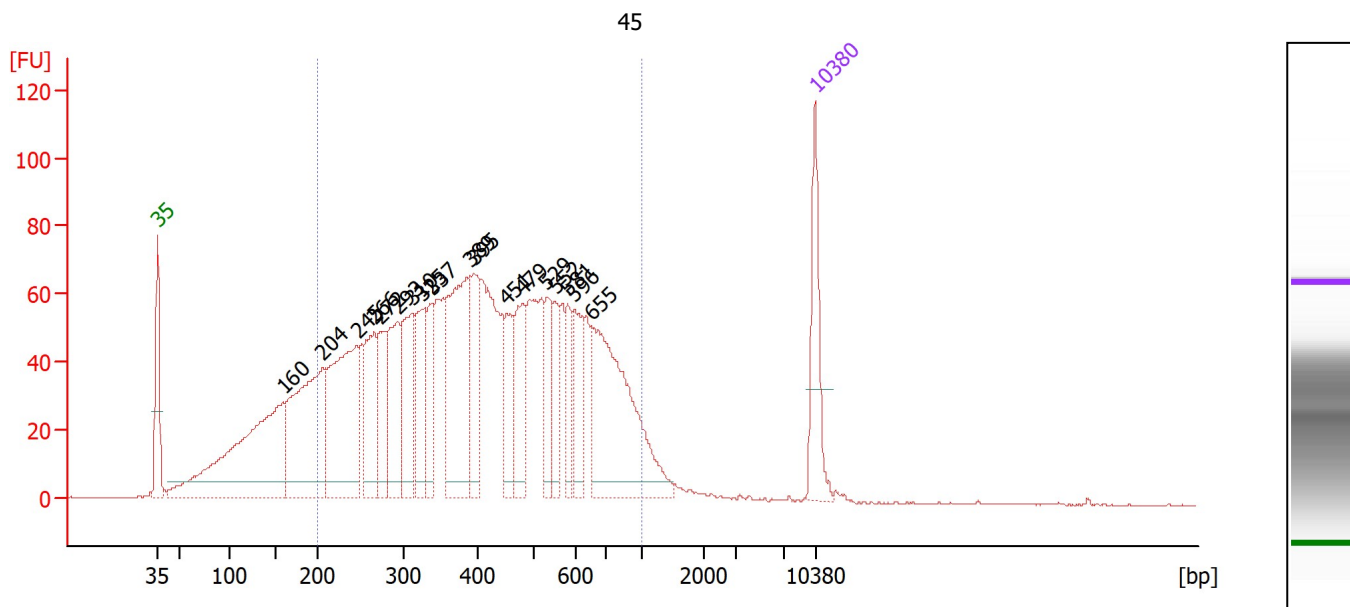

Overall Results for sample 3 : 45

Number of peaks found: 18 Corr. Area 1: 2,266.2
Noise: 0.1

Peak table for sample 3 : 45


Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	160	437.19	4,127.8	
3	204	310.38	2,300.1	
4	245	287.73	1,777.7	
5	266	130.24	742.1	
6	272	92.12	512.8	
7	293	126.38	653.7	
8	310	132.40	647.4	
9	325	107.16	499.5	
10	337	71.47	321.1	
11	389	224.04	872.2	
12	395	98.28	377.0	
13	451	64.88	218.1	
14	479	94.86	300.2	
15	529	61.00	174.8	
16	552	50.22	138.0	
17	581	47.01	122.6	
18	596	68.48	174.0	
19	655	271.98	629.1	
20	10,380	75.00	10.9	Upper Marker

Region table for sample 3 : 45

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	2,266.2	79	441	38.8	2,627.65	11,041.2	Blue

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-10-20_003.xad

Created: 10/20/2025 5:00:25 PM
Modified: 10/20/2025 5:43:24 PM

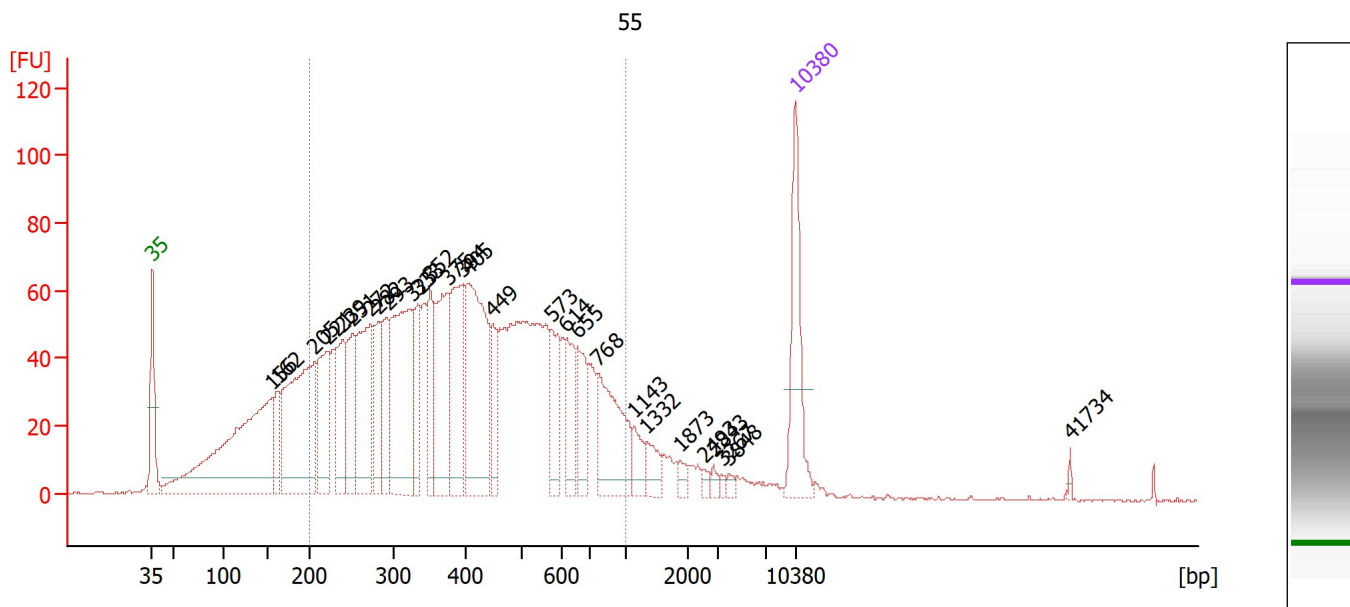Electropherogram Summary Continued ...**Overall Results for sample 4 : 55**

Number of peaks found: 28 Corr. Area 1: 2,110.8
Noise: 0.2

Peak table for sample 4 : 55

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	156	357.59	3,470.5	
3	162	47.25	441.0	
4	205	249.57	1,840.7	
5	221	101.21	692.5	
6	239	83.15	526.3	
7	251	84.50	510.2	
8	272	132.44	737.5	
9	282	67.29	361.1	
10	293	67.26	348.3	
11	325	189.89	886.3	
12	333	56.94	258.7	
13	352	61.42	264.5	
14	375	117.51	475.2	
15	394	114.43	440.2	
16	405	180.00	672.7	
17	449	42.42	143.3	
18	573	54.23	143.3	
19	614	44.62	110.1	
20	655	48.23	111.5	
21	768	95.52	188.4	
22	1,143	19.73	26.2	
23	1,332	18.98	21.6	
24	1,873	7.18	5.8	
25	2,493	4.34	2.6	
26	2,843	4.61	2.5	

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-10-20_003.xad

Created: 10/20/2025 5:00:25 PM
 Modified: 10/20/2025 5:43:24 PM

Electropherogram Summary Continued ...

... Peak table for sample 4 : 55


Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
27	3,267	3.15	1.5	
28	3,848	3.84	1.5	
29	10,380	75.00	10.9	Upper Marker
30	41,734	0.00	0.0	

Region table for sample 4 : 55

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	2,110.8	76	430	39.2	2,096.18	8,995.7	

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-10-20_003.xad

Created: 10/20/2025 5:00:25 PM
Modified: 10/20/2025 5:43:24 PM

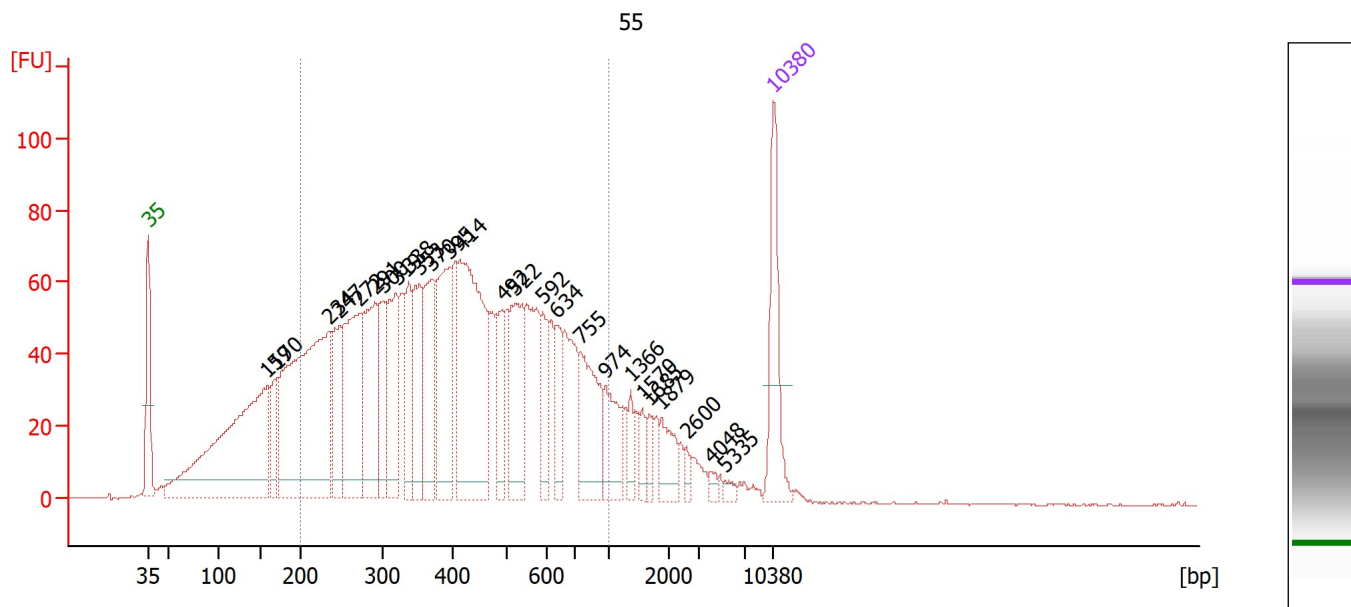Electropherogram Summary Continued ...**Overall Results for sample 5 : 55**

Number of peaks found: 26 Corr. Area 1: 2,227.2
Noise: 0.2

Peak table for sample 5 : 55

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	159	432.36	4,119.7	
3	170	59.21	528.0	
4	234	438.30	2,833.8	
5	247	89.66	550.2	
6	272	178.70	995.6	
7	291	155.52	809.5	
8	300	76.04	383.6	
9	319	109.02	517.3	
10	338	64.89	291.3	
11	353	87.40	375.4	
12	370	105.04	429.9	
13	395	142.37	545.8	
14	414	266.55	976.7	
15	492	57.96	178.3	
16	522	97.26	282.3	
17	592	46.11	118.0	
18	634	43.09	102.9	
19	755	95.01	190.6	
20	974	52.63	81.9	
21	1,366	16.64	18.5	
22	1,570	14.42	13.9	
23	1,685	13.63	12.3	
24	1,879	29.37	23.7	
25	2,600	7.33	4.3	
26	4,048	5.59	2.1	

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-10-20_003.xad

Created: 10/20/2025 5:00:25 PM
 Modified: 10/20/2025 5:43:24 PM

Electropherogram Summary Continued ...

... Peak table for sample 5 : 55

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
27	5,335	5.06	1.4	
28	10,380	75.00	10.9	Upper Marker


Region table for sample 5 : 55

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	2,227.2	73	435	39.7	2,378.19	10,138.5	

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-10-20_003.xad

Created: 10/20/2025 5:00:25 PM
Modified: 10/20/2025 5:43:24 PM

Electropherogram Summary Continued ...

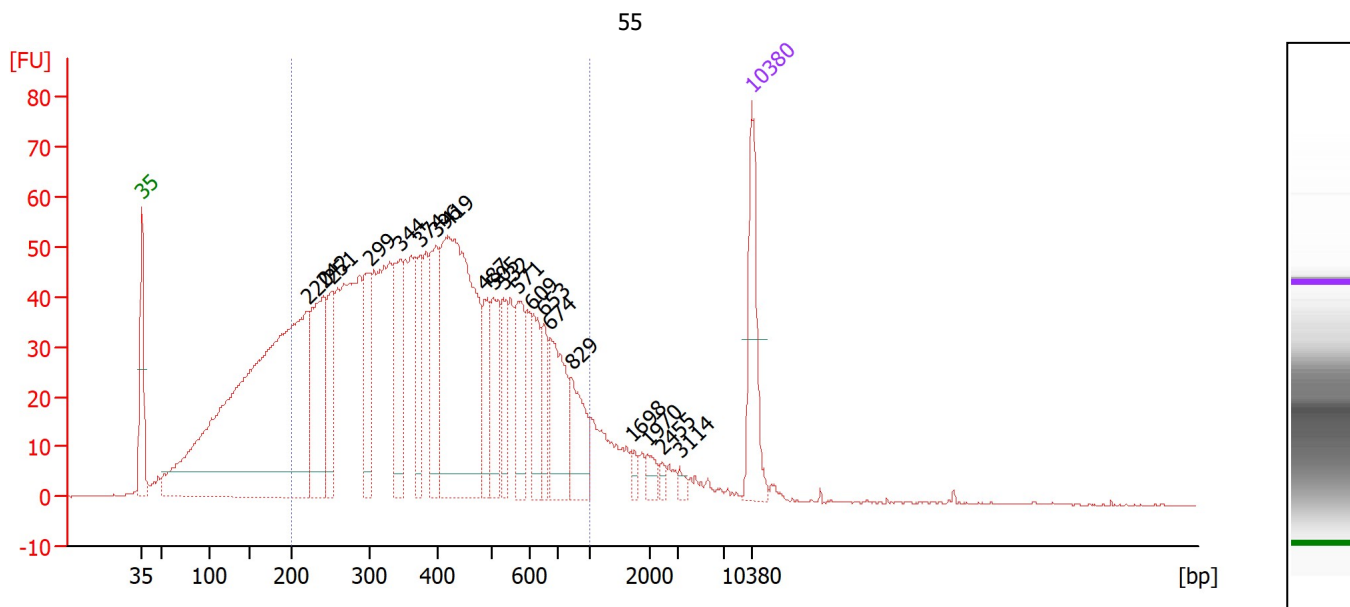

Overall Results for sample 6 : 55

Number of peaks found: 20 Corr. Area 1: 1,742.1
Noise: 0.2

Peak table for sample 6 : 55

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	220	920.36	6,332.3	
3	242	181.79	1,138.9	
4	251	90.31	544.4	
5	299	88.63	448.6	
6	344	101.32	445.9	
7	374	70.02	283.8	
8	396	100.60	384.6	
9	419	396.07	1,433.9	
10	487	54.69	170.1	
11	505	69.40	208.3	
12	532	48.17	137.1	
13	571	68.59	182.1	
14	609	51.79	128.8	
15	653	40.40	93.8	
16	674	93.89	211.0	
17	829	63.71	116.5	
18	1,698	8.34	7.4	
19	1,970	12.47	9.6	
20	2,455	5.97	3.7	
21	3,114	6.30	3.1	
22	10,380	75.00	10.9	Upper Marker


Region table for sample 6 : 55

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	1,742.1	74	422	39.0	2,602.51	11,325.2	Blue

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-10-20_003.xad

Created: 10/20/2025 5:00:25 PM
Modified: 10/20/2025 5:43:24 PM

Electropherogram Summary Continued ...

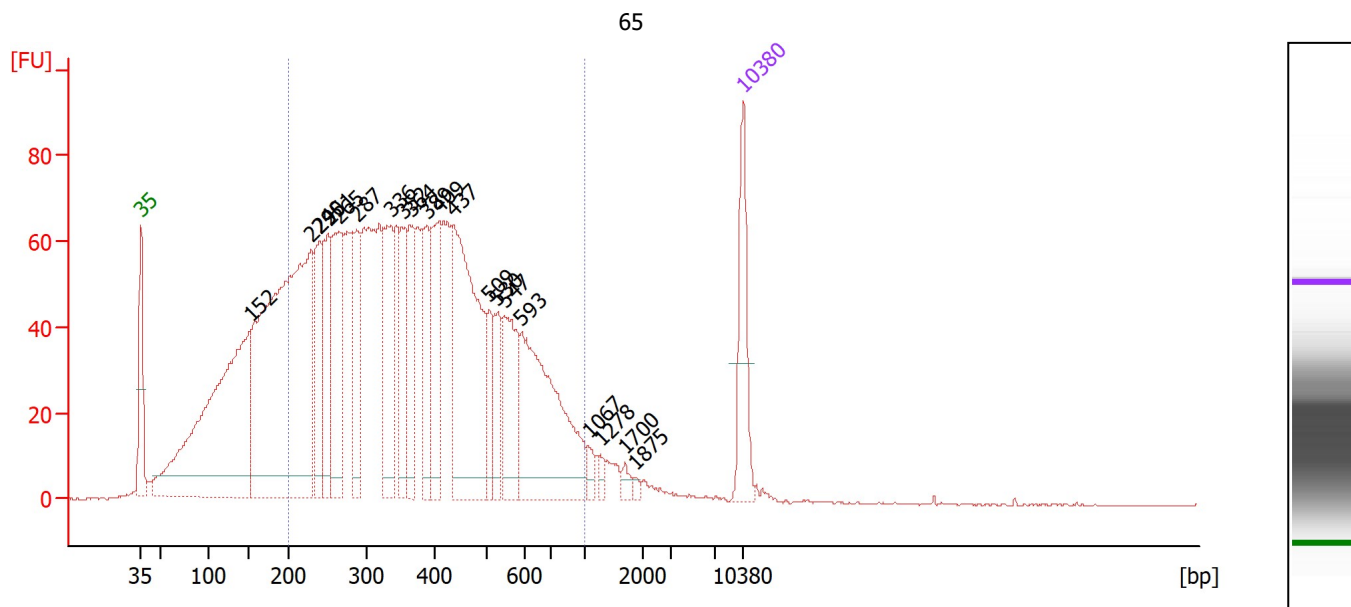

Overall Results for sample 7 : 65

Number of peaks found: 20 Corr. Area 1: 2,215.6
Noise: 0.1

Peak table for sample 7 : 65

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	152	645.58	6,419.9	
3	229	793.65	5,251.7	
4	240	120.35	760.0	
5	251	120.67	728.8	
6	265	166.20	951.8	
7	287	128.61	678.6	
8	336	131.03	591.6	
9	352	92.69	398.8	
10	364	84.28	350.9	
11	389	91.73	357.2	
12	409	114.35	423.3	
13	437	317.48	1,100.8	
14	509	48.91	145.6	
15	530	54.27	155.2	
16	547	111.59	309.3	
17	593	250.67	640.9	
18	1,067	11.22	15.9	
19	1,278	8.11	9.6	
20	1,700	8.30	7.4	
21	1,875	4.13	3.3	
22	10,380	75.00	10.9	Upper Marker


Region table for sample 7 : 65

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	2,215.6	73	398	38.3	2,986.66	13,552.2	Blue

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-10-20_003.xad

Created: 10/20/2025 5:00:25 PM
Modified: 10/20/2025 5:43:24 PM

Electropherogram Summary Continued ...

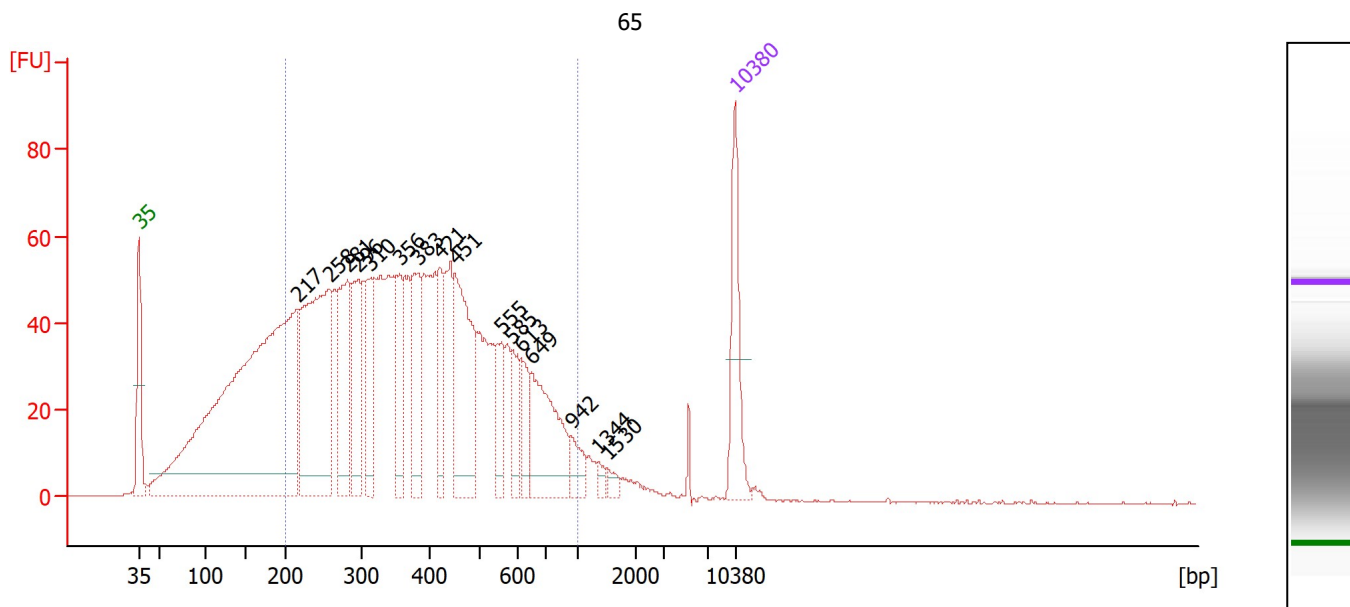

Overall Results for sample 8 : 65

Number of peaks found: 16 Corr. Area 1: 1,790.6
Noise: 0.2

Peak table for sample 8 : 65

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	217	985.70	6,889.0	
3	258	360.47	2,114.5	
4	281	158.08	852.0	
5	296	118.39	606.7	
6	310	97.50	476.4	
7	356	83.62	355.6	
8	383	100.68	398.0	
9	421	66.62	239.9	
10	451	180.15	605.7	
11	555	48.30	131.8	
12	585	45.65	118.2	
13	613	39.24	97.0	
14	649	132.37	309.0	
15	942	25.09	40.3	
16	1,344	8.33	9.4	
17	1,530	8.72	8.6	
18	10,380	75.00	10.9	Upper Marker


Region table for sample 8 : 65

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	1,790.6	73	405	38.4	2,511.93	11,266.5	Blue

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-10-20_003.xad

Created: 10/20/2025 5:00:25 PM
Modified: 10/20/2025 5:43:24 PM

Electropherogram Summary Continued ...

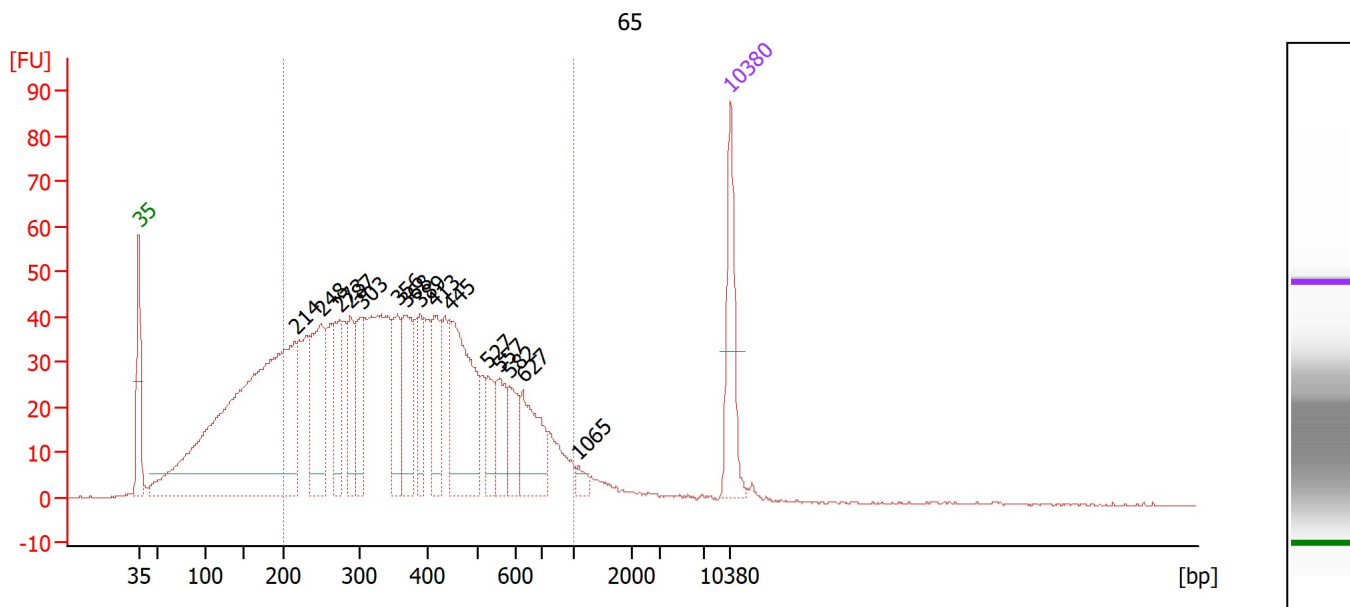

Overall Results for sample 9 : 65

Number of peaks found: 15
Noise: 0.2
Corr. Area 1: 1,387.7

Peak table for sample 9 : 65

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	214	784.46	5,551.6	
3	248	150.61	919.3	
4	273	82.32	456.3	
5	287	70.58	372.3	
6	303	63.61	318.1	
7	356	74.64	317.8	
8	368	98.23	404.6	
9	389	52.99	206.1	
10	413	78.69	288.4	
11	445	183.35	624.7	
12	527	39.56	113.8	
13	557	51.90	141.3	
14	582	40.56	105.6	
15	627	78.15	188.8	
16	1,065	8.57	12.2	
17	10,380	75.00	10.9	Upper Marker


Region table for sample 9 : 65

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	1,387.7	73	398	37.9	1,974.11	8,947.8	Blue

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-10-20_003.xad

Created: 10/20/2025 5:00:25 PM
Modified: 10/20/2025 5:43:24 PM

Electropherogram Summary Continued ...

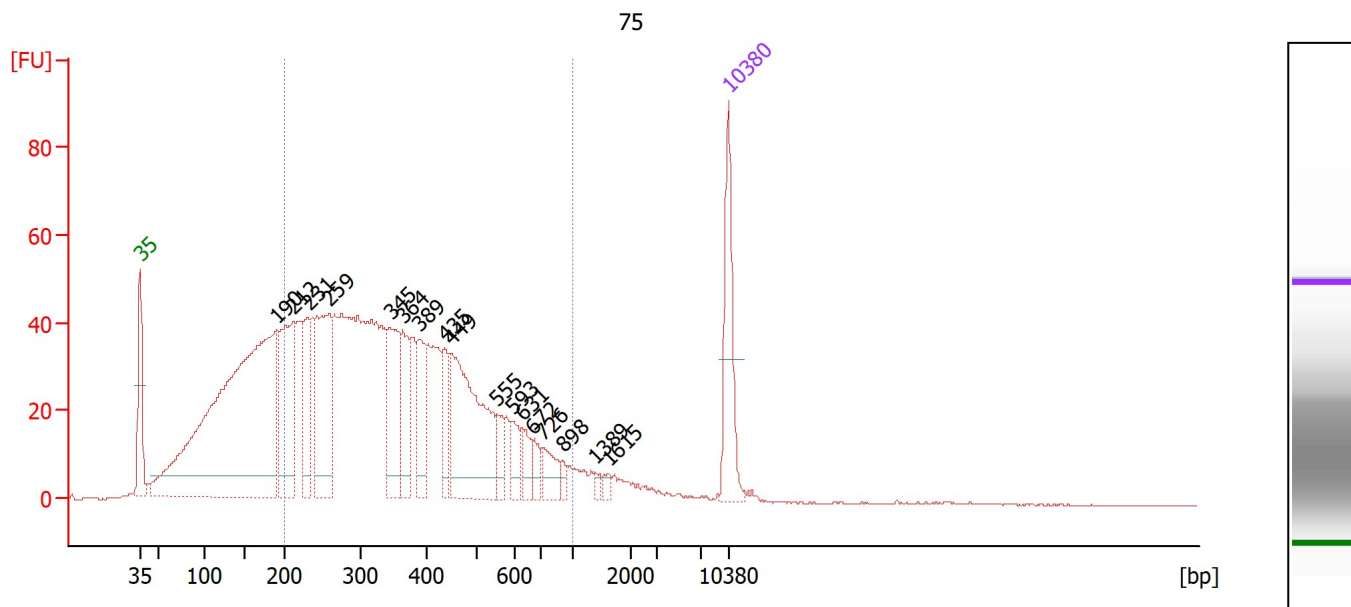

Overall Results for sample 10 : 75

Number of peaks found: 17 Corr. Area 1: 1,331.5
Noise: 0.1

Peak table for sample 10 : 75

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	190	797.36	6,349.4	
3	212	181.96	1,302.3	
4	231	87.64	574.0	
5	259	177.92	1,039.5	
6	345	106.46	467.4	
7	364	67.28	280.4	
8	389	61.31	239.1	
9	435	42.02	146.2	
10	449	205.49	693.4	
11	555	24.02	65.6	
12	593	25.78	65.8	
13	631	21.43	51.4	
14	672	16.17	36.5	
15	726	27.59	57.6	
16	898	7.82	13.2	
17	1,389	5.34	5.8	
18	1,615	5.27	4.9	
19	10,380	75.00	10.9	Upper Marker


Region table for sample 10 : 75

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	1,331.5	67	379	38.6	1,864.76	8,821.2	Blue

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-10-20_003.xad

Created: 10/20/2025 5:00:25 PM
Modified: 10/20/2025 5:43:24 PM

Electropherogram Summary Continued ...

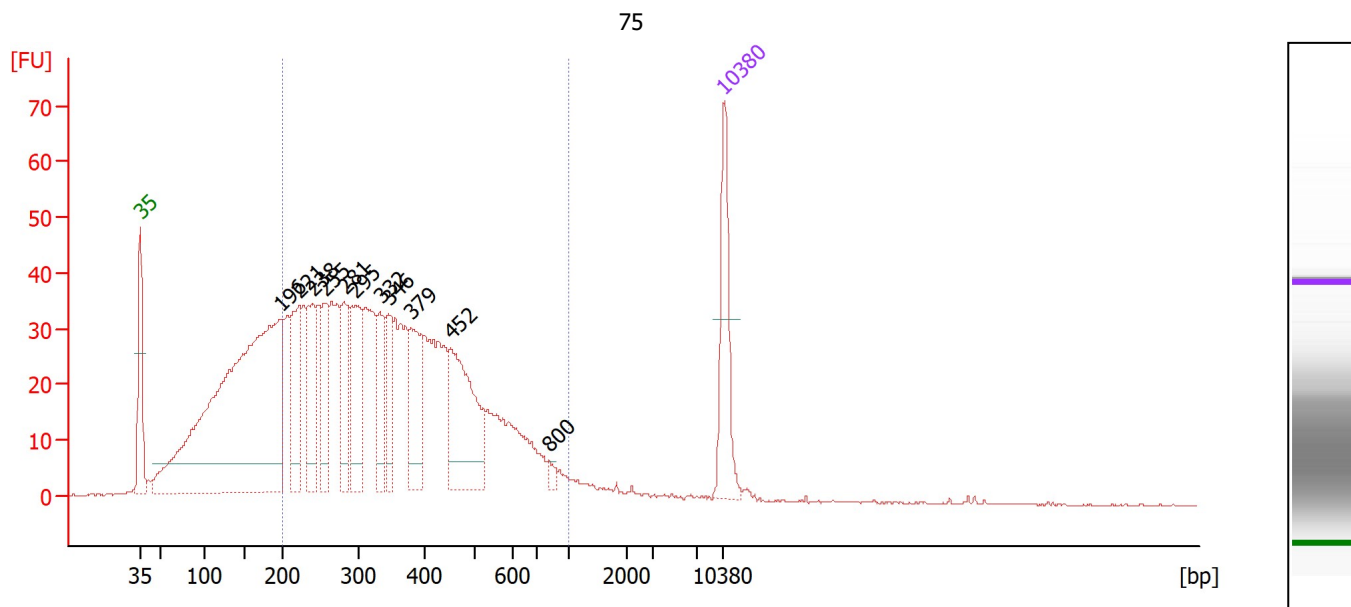

Overall Results for sample 11 : 75

Number of peaks found: 11 Corr. Area 1: 1,069.0
Noise: 0.1

Peak table for sample 11 : 75

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	196	798.21	6,171.0	
3	221	107.23	736.5	
4	238	94.30	601.4	
5	255	75.22	447.8	
6	281	75.49	407.5	
7	295	101.42	521.2	
8	332	63.30	288.7	
9	346	52.92	231.7	
10	379	82.63	330.0	
11	452	153.55	514.2	
12	800	6.93	13.1	
13	10,380	75.00	10.9	Upper Marker


Region table for sample 11 : 75

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	1,069.0	67	372	37.1	1,752.63	8,356.4	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-10-20_003.xad

Created: 10/20/2025 5:00:25 PM
 Modified: 10/20/2025 5:43:24 PM

Gel Image

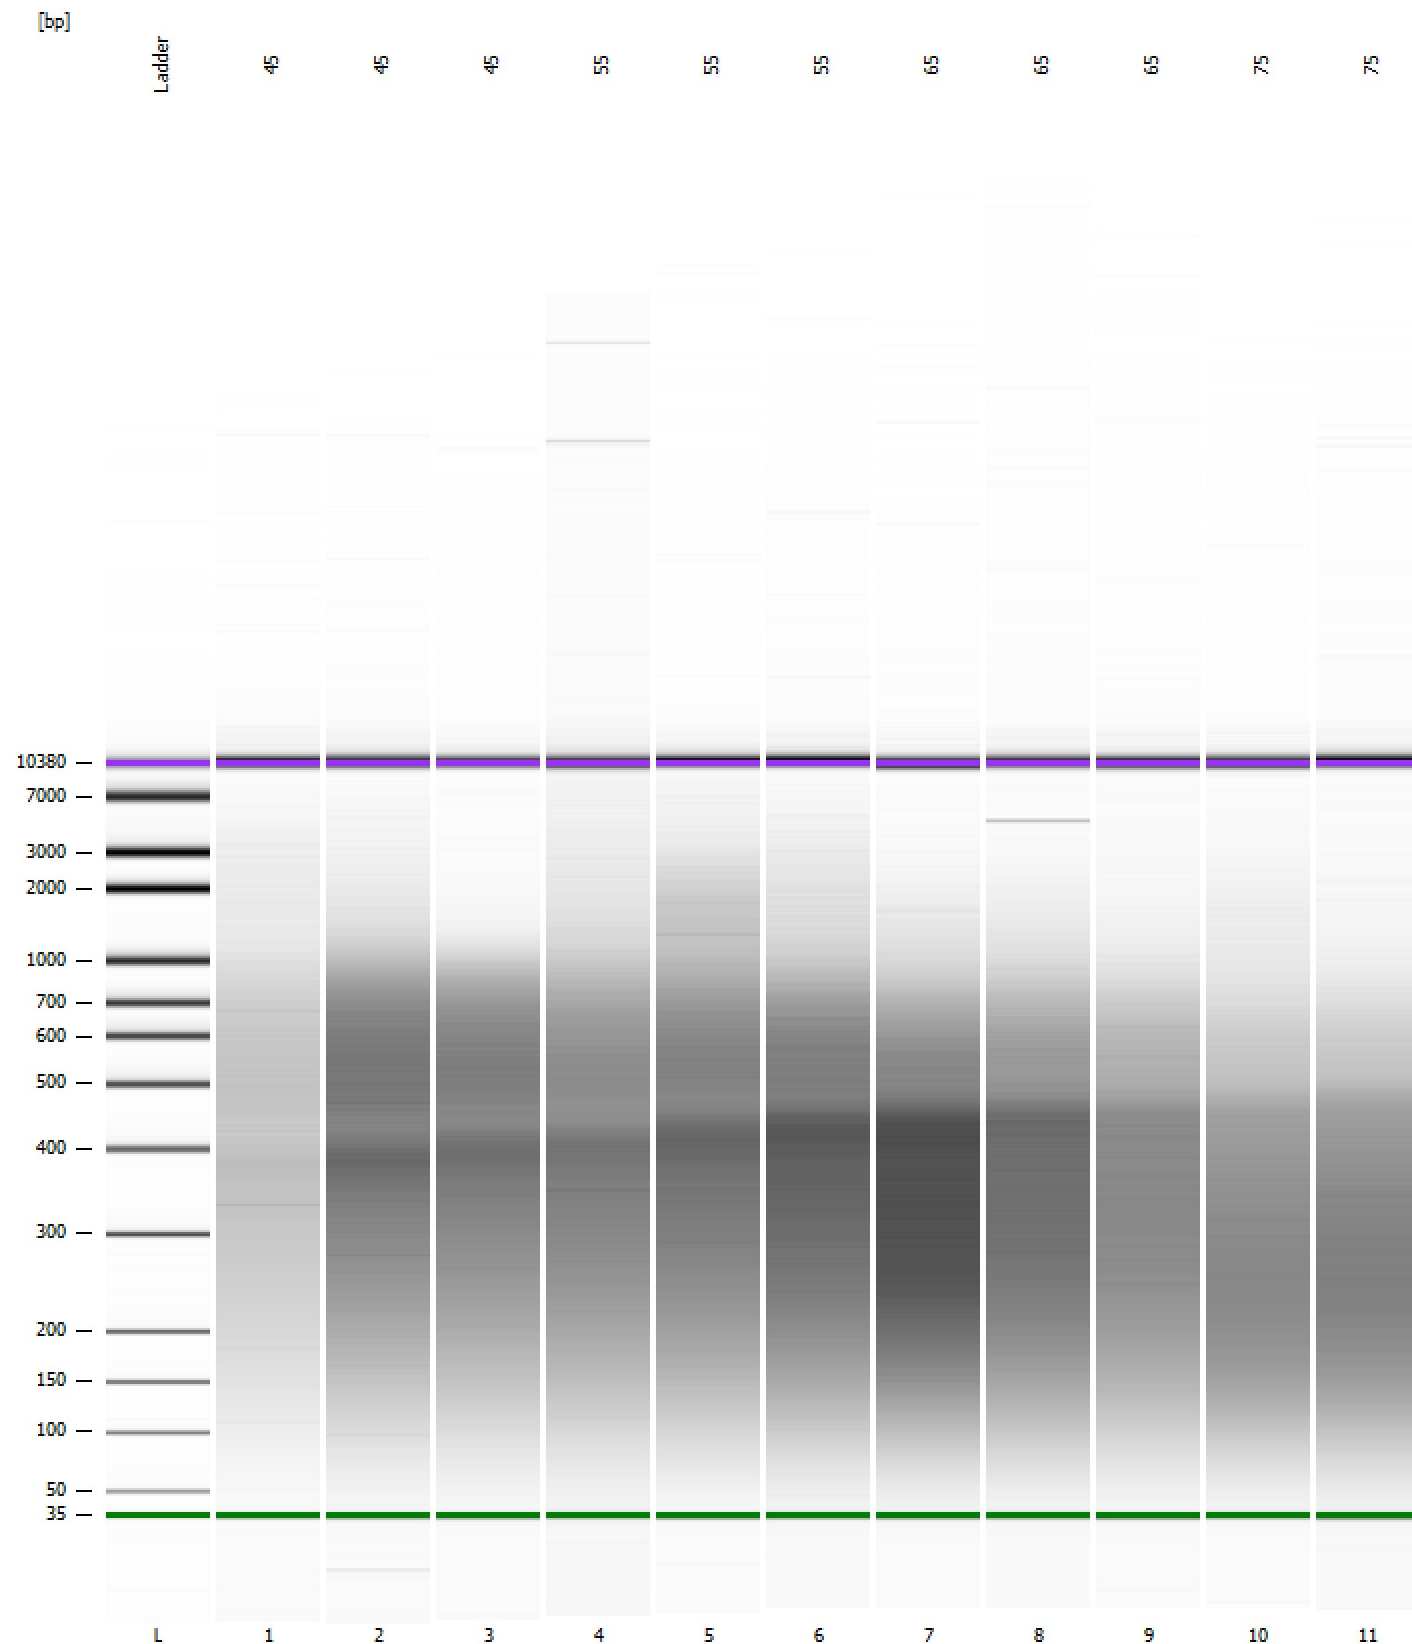

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...r1_High Sensitivity DNA Assay_DE34903152_2025-10-20_003.xad

Created: 10/20/2025 5:00:25 PM
 Modified: 10/20/2025 5:43:24 PM

Run Logbook

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 12)		Instrument	Run		10/20/2025 5:41:45 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Run started on port 1 (File: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\data\2025-10-20\Bioanalyzer1_High Sensitivity DNA Assay_DE34903152_2025-10-20_003.xad)		Instrument	Run		10/20/2025 5:00:30 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Product Number : G2938C		Instrument	Run		10/20/2025 5:00:30 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Name :		Instrument	Run		10/20/2025 5:00:30 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Vendor : Agilent Technologies		Instrument	Run		10/20/2025 5:00:30 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Serial# : DE34903152		Instrument	Run		10/20/2025 5:00:30 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Firmware : C.01.069		Instrument	Run		10/20/2025 5:00:30 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Cartridge : Electrode		Instrument	Run		10/20/2025 5:00:30 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB