


Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...yzer\2100 expert\data\2024-04-17\Lemay_Pippin_4-17-2024.xad

Created: 4/17/2024 1:08:44 PM
 Modified: 4/17/2024 3:08:31 PM

Electrophoresis File Run Summary

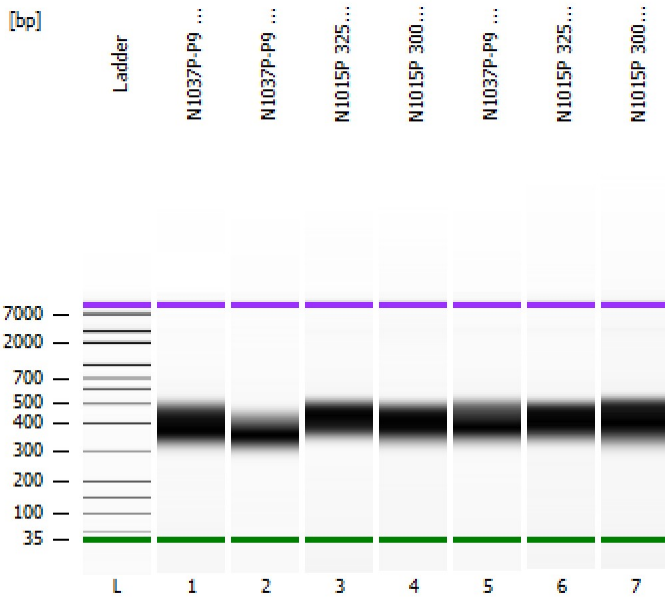

Instrument Information:

Instrument Name: DE34903152 Firmware: C.01.069
 Serial#: DE34903152 Type: G2938C

Assay Information:

Assay Origin Path: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy
 Assay Class: High Sensitivity DNA Assay
 Version: 1.03
 Assay Comments: Copyright © 2003-2010 Agilent Technologies




Chip Information:

Chip Lot #:
 Reagent Kit Lot #:
 Chip Comments:

N1037P-P9 325-600bp

N1037P-P9 300-550bp




N1015P 325-600bp 4/17

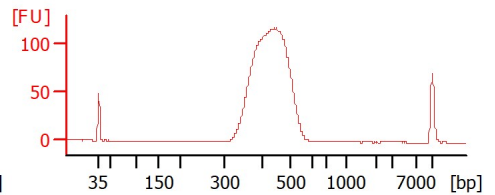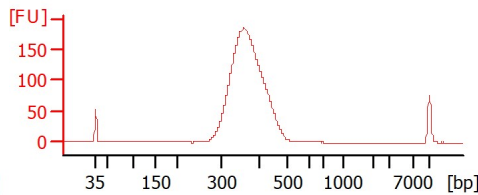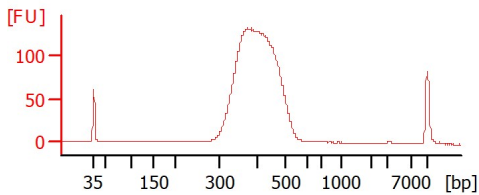


N1015P 300-550bp

N1037P-P9 325-600bp 4/16

N1015P 325-600bp

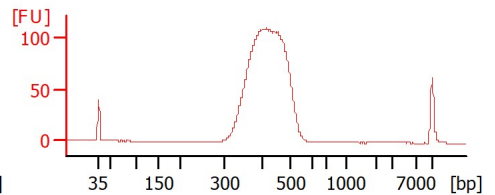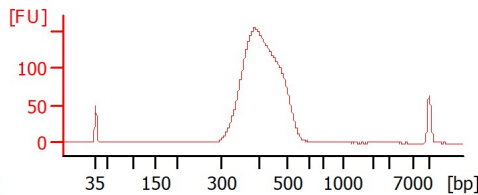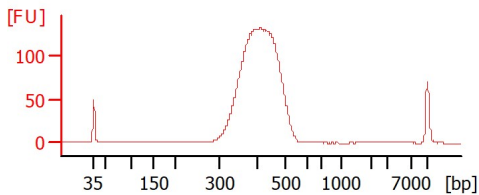

N1015P 300-625bp

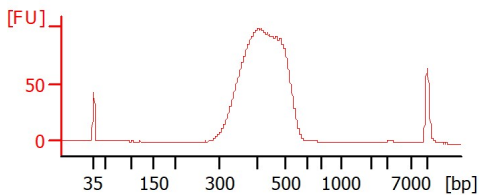

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...yzer\2100 expert\data\2024-04-17\Lemay_Pippin_4-17-2024.xad

Created: 4/17/2024 1:08:44 PM
 Modified: 4/17/2024 3:08:31 PM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
N1037P-P9 325-600bp		<input type="checkbox"/>	✓			
N1037P-P9 300-550bp		<input type="checkbox"/>	✓			
N1015P 325-600bp 4/17		<input type="checkbox"/>	✓			
N1015P 300-550bp		<input type="checkbox"/>	✓			
N1037P-P9 325-600bp 4/16		<input type="checkbox"/>	✓			
N1015P 325-600bp		<input type="checkbox"/>	✓			
N1015P 300-625bp		<input type="checkbox"/>	✓			
Ladder		<input type="checkbox"/>	✓			

Chip Lot #

Reagent Kit Lot #

Chip Comments :

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...yzer\2100 expert\data\2024-04-17\Lemay_Pippin_4-17-2024.xad

Created: 4/17/2024 1:08:44 PM
Modified: 4/17/2024 3:08:31 PM

Electrophoresis Assay Details

General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12
Minimum Visible Range [s] : 32
Maximum Visible Range [s] : 138
Start Analysis Time Range [s] : 33
End Analysis Time Range [s] : 137.5
Ladder Concentration [pg/ μ l] : 1950
Uses Standard Area for Ladder Fragments
Lower Marker Concentration [pg/ μ l] : 125
Upper Marker Concentration [pg/ μ l] : 75
Used Upper Marker for Quantitation
Standard Curve Fit is Point to Point
Show Data Aligned to Lower and Upper Marker

Integrator Settings

Integration Start Time [s] : 33.05
Integration End Time [s] : 137
Slope Threshold : 0.8
Height Threshold [FU] : 5
Area Threshold : 0.1
Width Threshold [s] : 0.6
Baseline Plateau [s] : 0.5

Filter Settings

Filter Width [s] : 0.5
Polynomial Order : 4


Ladder

Ladder Peak	Size	Area
1	35	160
2	50	210
3	100	208
4	150	221
5	200	242
6	300	270
7	400	305
8	500	306
9	600	336
10	700	321
11	1000	366
12	2000	413
13	3000	411
14	7000	400
15	10380	214

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...yzer\2100 expert\data\2024-04-17\Lemay_Pippin_4-17-2024.xad

Created: 4/17/2024 1:08:44 PM
 Modified: 4/17/2024 3:08:31 PM

Electropherogram Summary

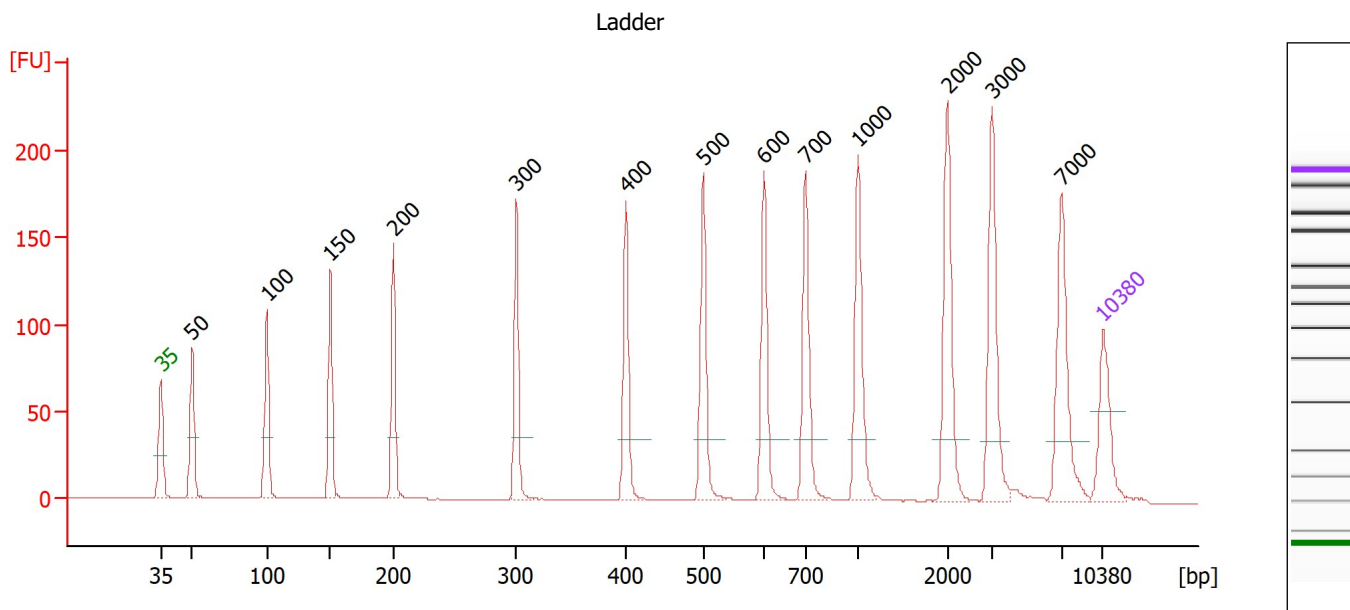

Overall Results for Ladder

Noise: 0.1


Peak table for Ladder

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	50	150.00	4,545.5	Ladder Peak
3	100	150.00	2,272.7	Ladder Peak
4	150	150.00	1,515.2	Ladder Peak
5	200	150.00	1,136.4	Ladder Peak
6	300	150.00	757.6	Ladder Peak
7	400	150.00	568.2	Ladder Peak
8	500	150.00	454.5	Ladder Peak
9	600	150.00	378.8	Ladder Peak
10	700	150.00	324.7	Ladder Peak
11	1,000	150.00	227.3	Ladder Peak
12	2,000	150.00	113.6	Ladder Peak
13	3,000	150.00	75.8	Ladder Peak
14	7,000	150.00	32.5	Ladder Peak
15	10,380	75.00	10.9	Upper Marker

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...yzer\2100 expert\data\2024-04-17\Lemay_Pippin_4-17-2024.xad

Created: 4/17/2024 1:08:44 PM
 Modified: 4/17/2024 3:08:31 PM

Electropherogram Summary Continued ...

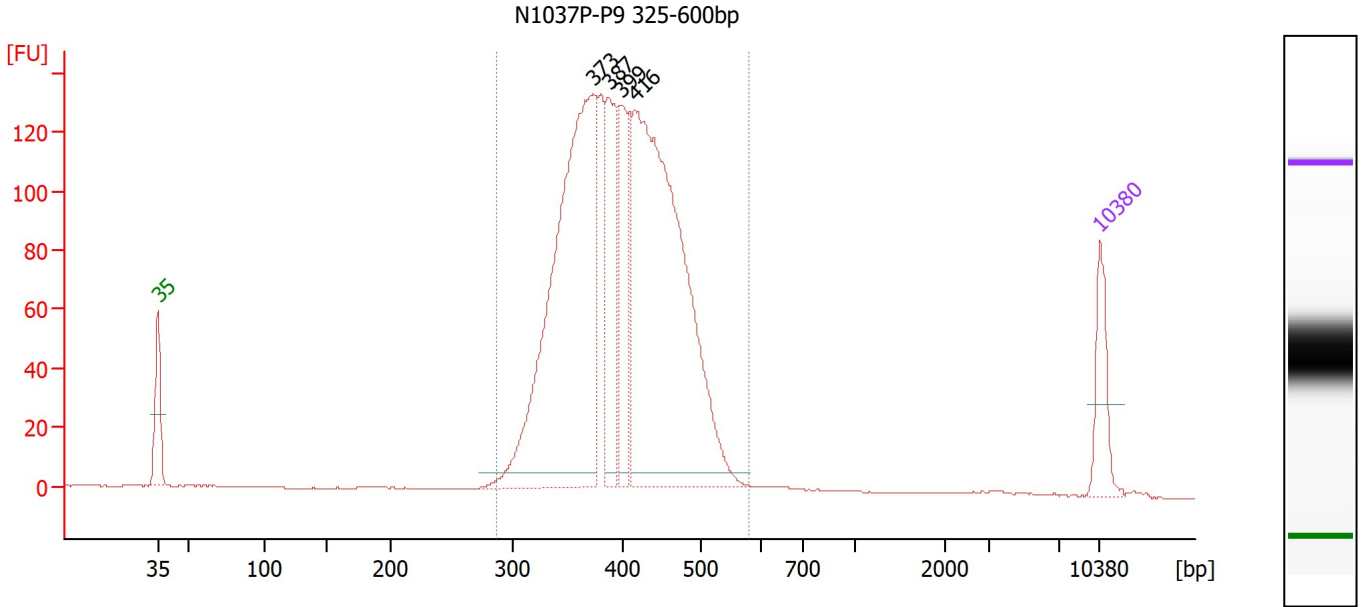

Overall Results for sample 1 : N1037P-P9 325-600bp

Number of peaks found: 4 Corr. Area 1: 1,819.4
 Noise: 0.2

Peak table for sample 1 : N1037P-P9 325-600bp

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	373	1,016.55	4,129.9	
3	387	229.93	900.1	
4	399	194.21	737.1	
5	416	1,096.36	3,991.9	
6	10,380	75.00	10.9	Upper Marker


Region table for sample 1 : N1037P-P9 325-600bp

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
287	580	1,819.4	98	404	13.2	2,795.63	10,703.4	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...yzer\2100 expert\data\2024-04-17\Lemay_Pippin_4-17-2024.xad

Created: 4/17/2024 1:08:44 PM
 Modified: 4/17/2024 3:08:31 PM

Electropherogram Summary Continued ...

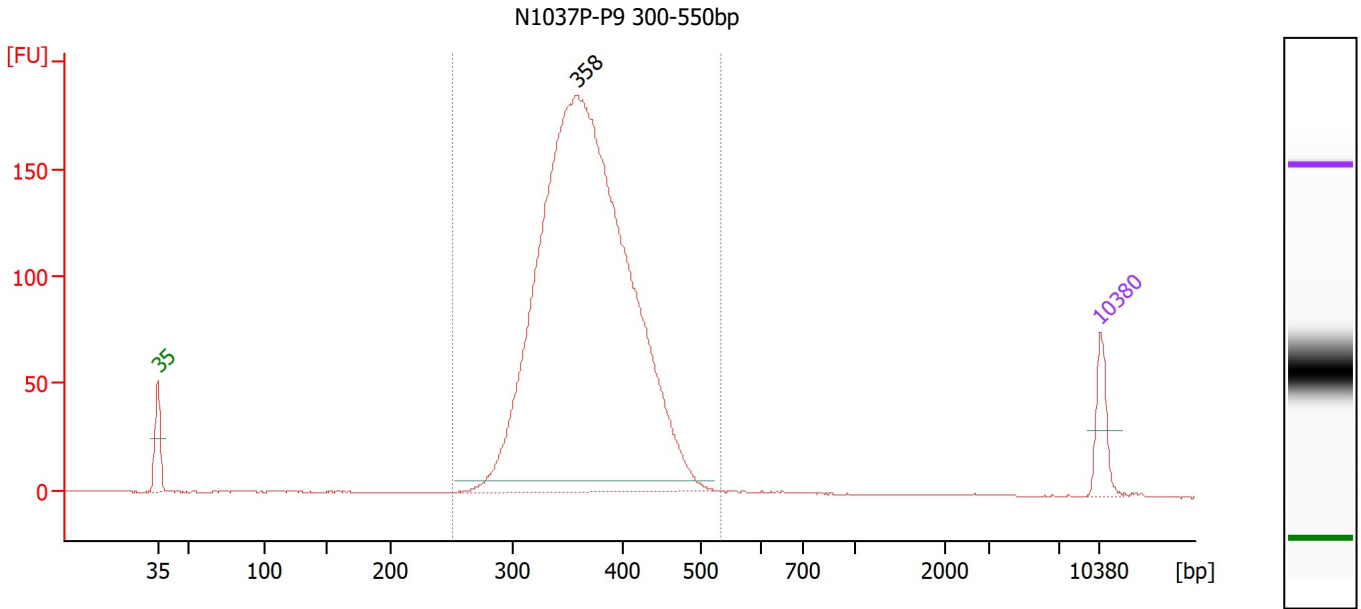

Overall Results for sample 2 : N1037P-P9 300-550bp

Number of peaks found: 1 Corr. Area 1: 1,970.0
 Noise: 0.2

Peak table for sample 2 : N1037P-P9 300-550bp

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	358	3,593.37	15,199.1	
3	10,380	75.00	10.9	Upper Marker


Region table for sample 2 : N1037P-P9 300-550bp

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
250	534	1,970.0	97	369	11.5	3,612.07	15,027.3	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...yzer\2100 expert\data\2024-04-17\Lemay_Pippin_4-17-2024.xad

Created: 4/17/2024 1:08:44 PM
 Modified: 4/17/2024 3:08:31 PM

Electropherogram Summary Continued ...

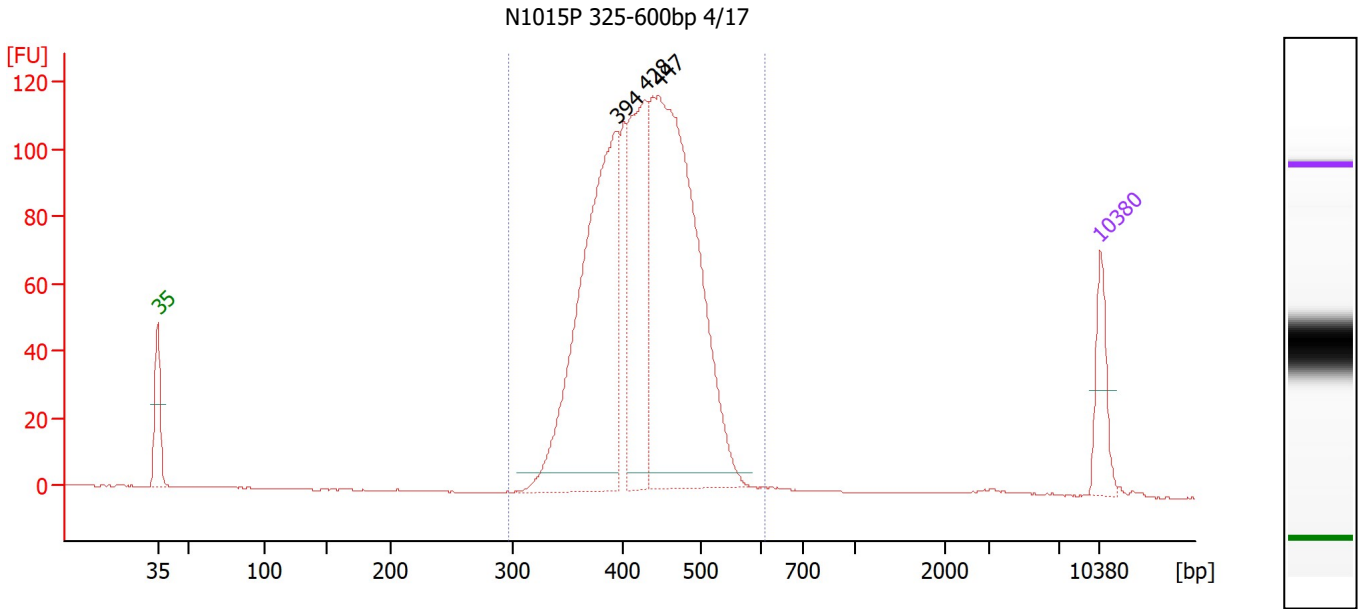

Overall Results for sample 3 : N1015P 325-600bp 4/17

Number of peaks found: 3 Corr. Area 1: 1,361.4
 Noise: 0.1

Peak table for sample 3 : N1015P 325-600bp 4/17

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	394	808.58	3,109.1	
3	428	397.88	1,408.1	
4	447	1,074.13	3,642.0	
5	10,380	75.00	10.9	Upper Marker


Region table for sample 3 : N1015P 325-600bp 4/17

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
296	610	1,361.4	98	429	11.9	2,483.52	8,914.7	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...yzer\2100 expert\data\2024-04-17\Lemay_Pippin_4-17-2024.xad

Created: 4/17/2024 1:08:44 PM
 Modified: 4/17/2024 3:08:31 PM

Electropherogram Summary Continued ...

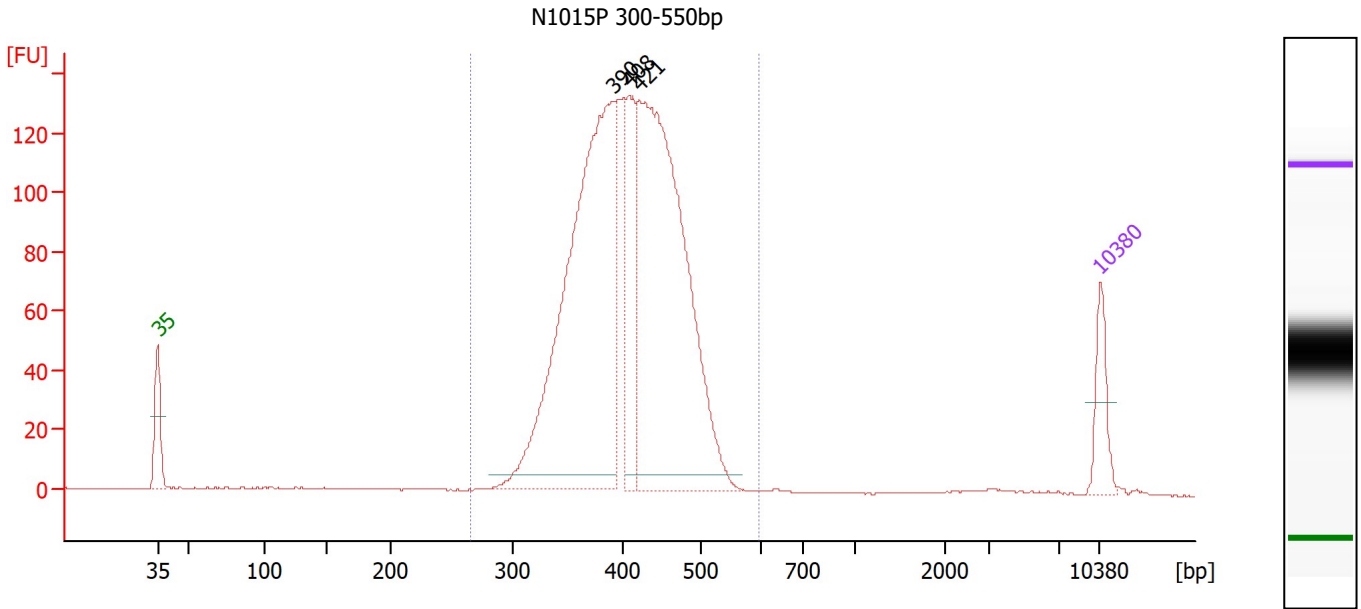

Overall Results for sample 4 : N1015P 300-550bp

Number of peaks found: 3 Corr. Area 1: 1,650.2
 Noise: 0.1

Peak table for sample 4 : N1015P 300-550bp

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	390	1,270.74	4,931.7	
3	408	285.41	1,058.8	
4	421	1,247.07	4,489.2	
5	10,380	75.00	10.9	Upper Marker


Region table for sample 4 : N1015P 300-550bp

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
265	597	1,650.2	96	411	12.4	3,084.56	11,583.6	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...yzer\2100 expert\data\2024-04-17\Lemay_Pippin_4-17-2024.xad

Created: 4/17/2024 1:08:44 PM
 Modified: 4/17/2024 3:08:31 PM

Electropherogram Summary Continued ...

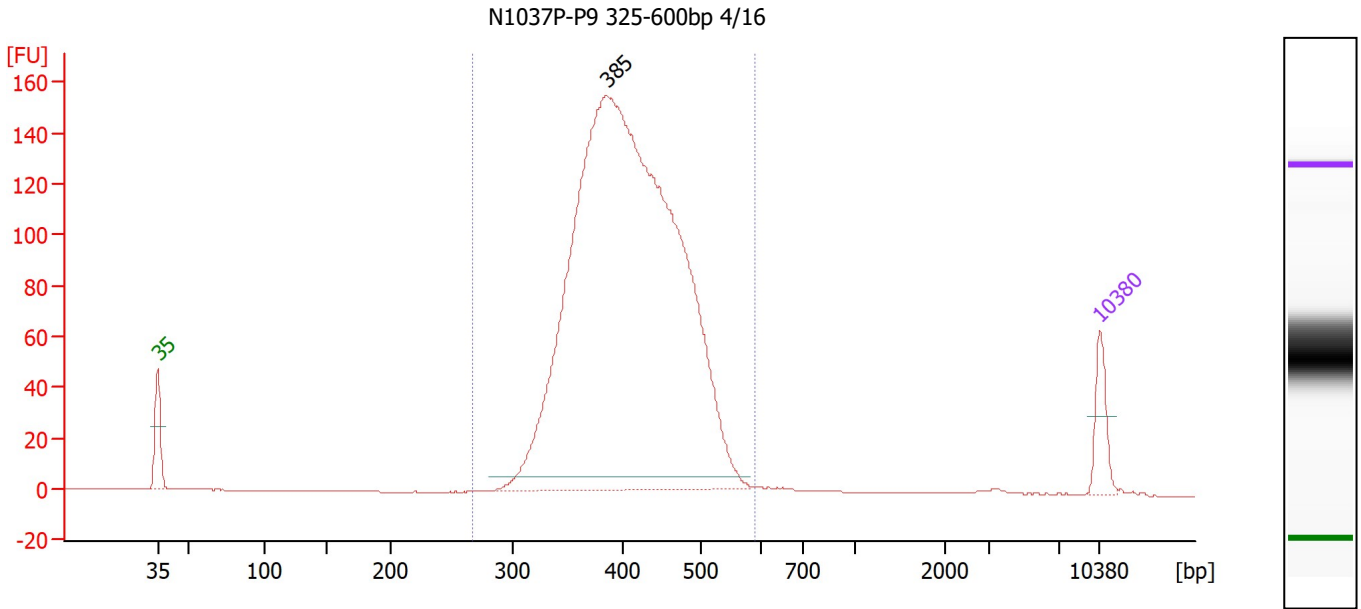

Overall Results for sample 5 : N1037P-P9 325-600bp 4/16

Number of peaks found: 1 Corr. Area 1: 1,843.8
 Noise: 0.2

Peak table for sample 5 : N1037P-P9 325-600bp 4/16

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	385	3,758.82	14,800.8	
3	10,380	75.00	10.9	Upper Marker


Region table for sample 5 : N1037P-P9 325-600bp 4/16

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
267	592	1,843.8	97	413	13.1	3,768.41	14,095.5	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...yzer\2100 expert\data\2024-04-17\Lemay_Pippin_4-17-2024.xad

Created: 4/17/2024 1:08:44 PM
 Modified: 4/17/2024 3:08:31 PM

Electropherogram Summary Continued ...

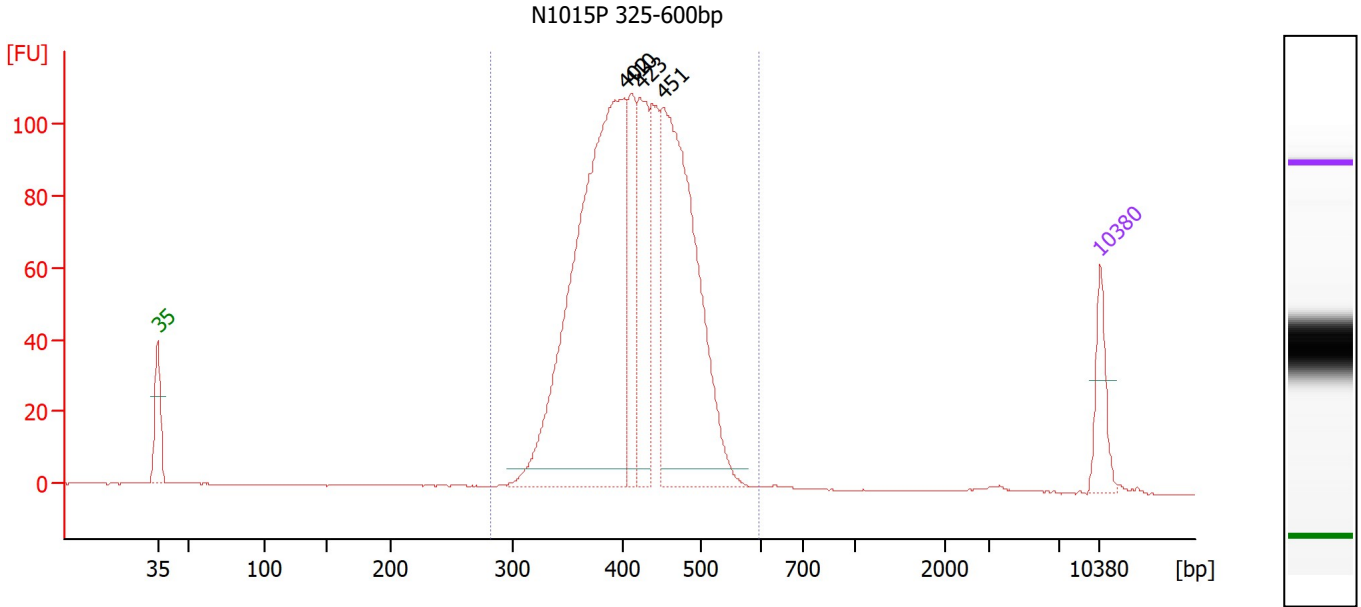

Overall Results for sample 6 : N1015P 325-600bp

Number of peaks found: 4 Corr. Area 1: 1,337.8
 Noise: 0.1

Peak table for sample 6 : N1015P 325-600bp

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	402	1,327.75	4,999.0	
3	410	229.33	846.5	
4	423	293.44	1,052.2	
5	451	899.98	3,025.1	
6	10,380	75.00	10.9	Upper Marker


Region table for sample 6 : N1015P 325-600bp

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
282	598	1,337.8	98	420	12.3	3,093.14	11,363.4	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...yzer\2100 expert\data\2024-04-17\Lemay_Pippin_4-17-2024.xad

Created: 4/17/2024 1:08:44 PM
 Modified: 4/17/2024 3:08:31 PM

Electropherogram Summary Continued ...

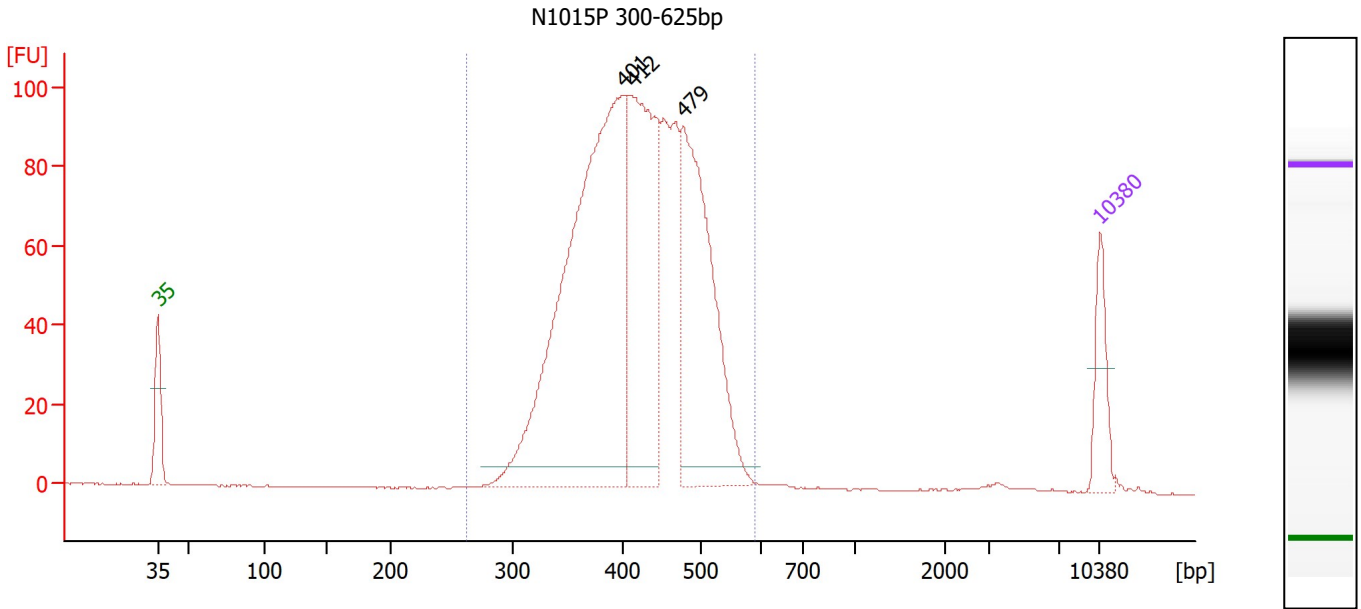

Overall Results for sample 7 : N1015P 300-625bp

Number of peaks found: 3 Corr. Area 1: 1,392.7
 Noise: 0.1

Peak table for sample 7 : N1015P 300-625bp

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	401	1,234.52	4,666.9	
3	412	573.35	2,108.2	
4	479	577.19	1,827.4	
5	10,380	75.00	10.9	Upper Marker


Region table for sample 7 : N1015P 300-625bp

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
262	592	1,392.7	98	422	14.3	2,858.64	10,516.9	Blue

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...yzer\2100 expert\data\2024-04-17\Lemay_Pippin_4-17-2024.xad

Created: 4/17/2024 1:08:44 PM
Modified: 4/17/2024 3:08:31 PM

Gel Image

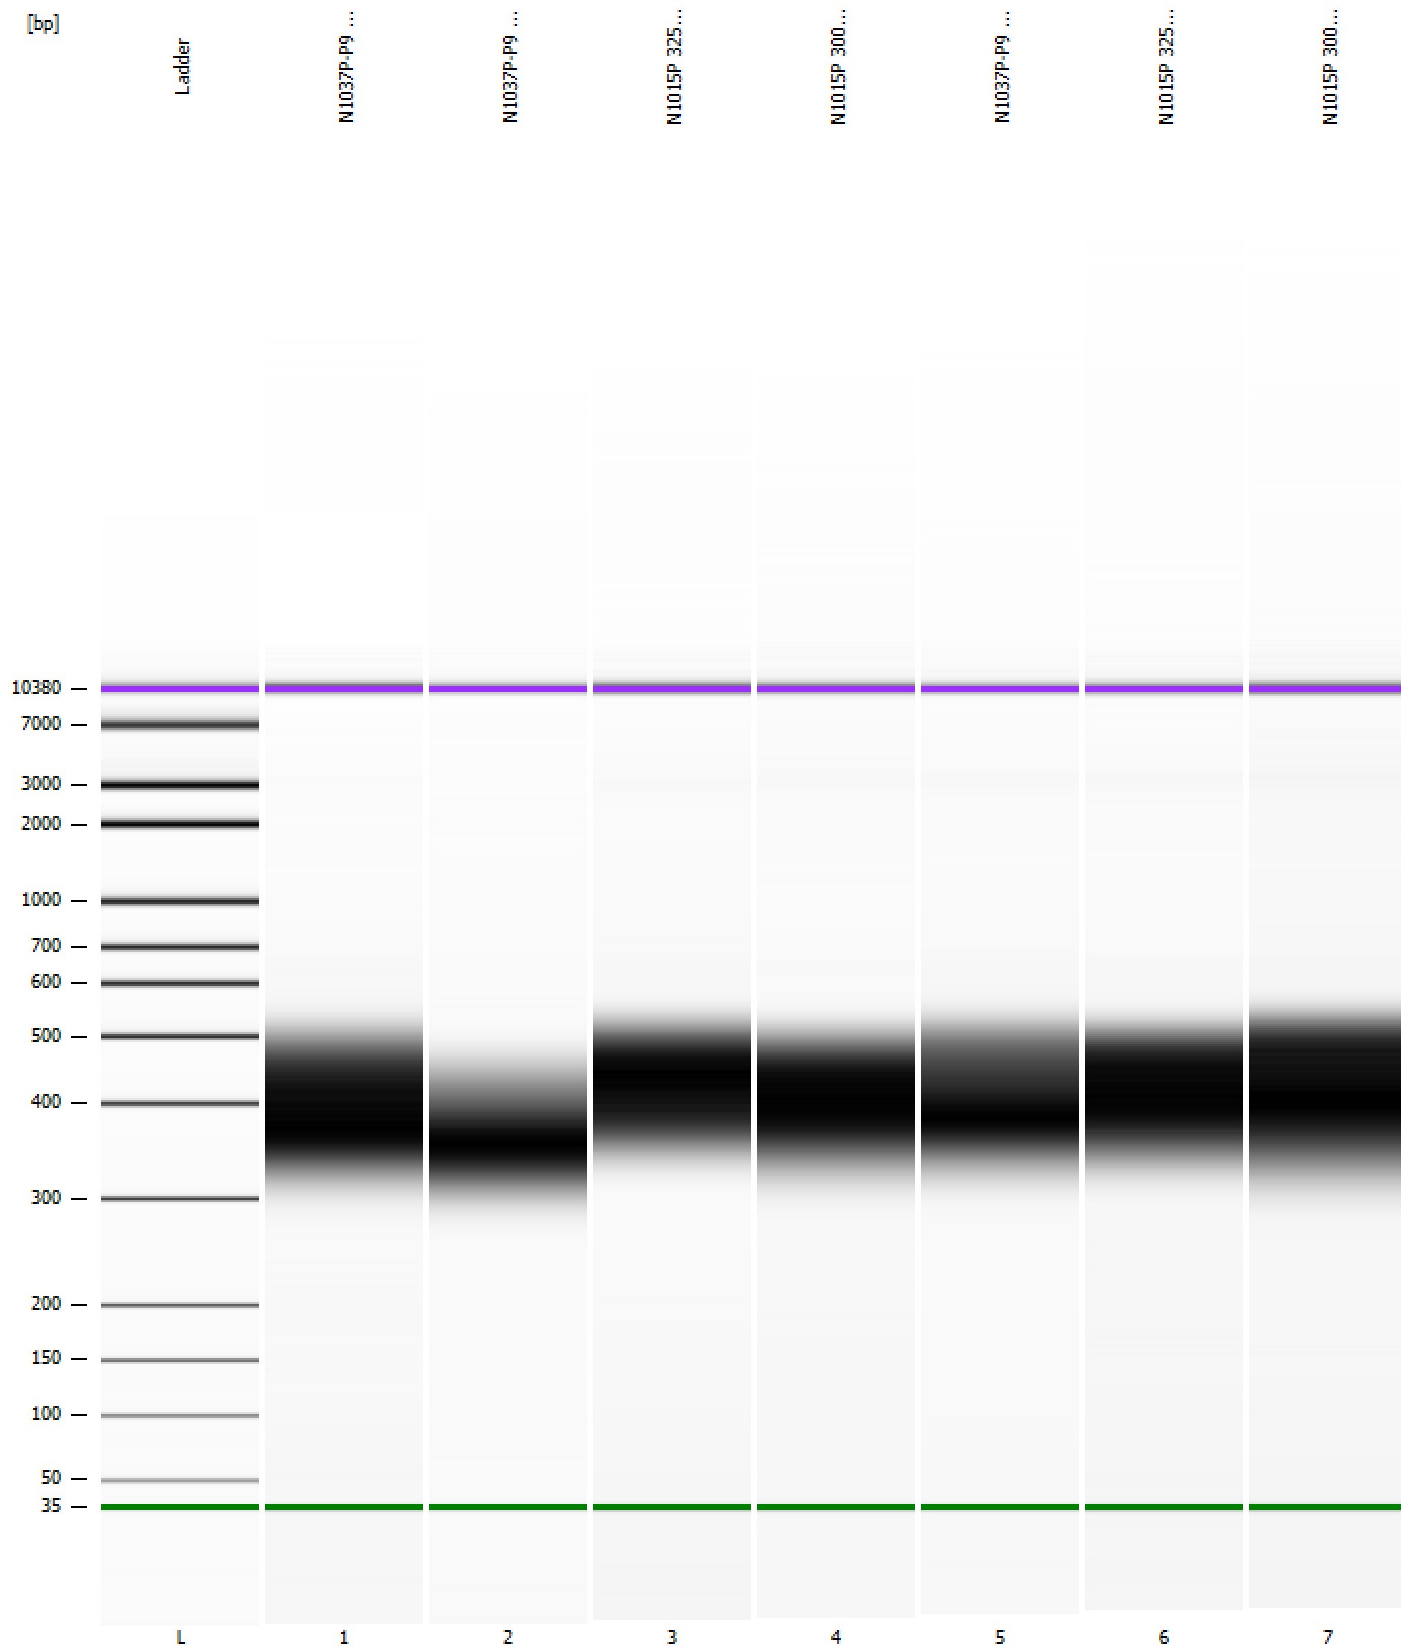

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...yzer\2100 expert\data\2024-04-17\Lemay_Pippin_4-17-2024.xad

Created: 4/17/2024 1:08:44 PM
 Modified: 4/17/2024 3:08:31 PM

Run Logbook

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 12)		Instrument	Run		4/17/2024 1:50:03 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Run started on port 1 (File: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\data\2024-04-17\Bioanalyzer1_High Sensitivity DNA Assay_DE34903152_2024-04-17_004.xad)		Instrument	Run		4/17/2024 1:08:49 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Product Number : G2938C		Instrument	Run		4/17/2024 1:08:49 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Name :		Instrument	Run		4/17/2024 1:08:49 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Vendor : Agilent Technologies		Instrument	Run		4/17/2024 1:08:49 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Serial# : DE34903152		Instrument	Run		4/17/2024 1:08:49 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Firmware : C.01.069		Instrument	Run		4/17/2024 1:08:49 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Cartridge : Electrode		Instrument	Run		4/17/2024 1:08:49 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB