


Assay Class: High Sensitivity DNA Assay
Data Path: C:\...zer\2100 expert\data\2024-04-02\Nova1036_PippinSS_Pools.xad

Created: 4/2/2024 8:50:20 AM
Modified: 4/2/2024 10:29:08 AM

Electrophoresis File Run Summary

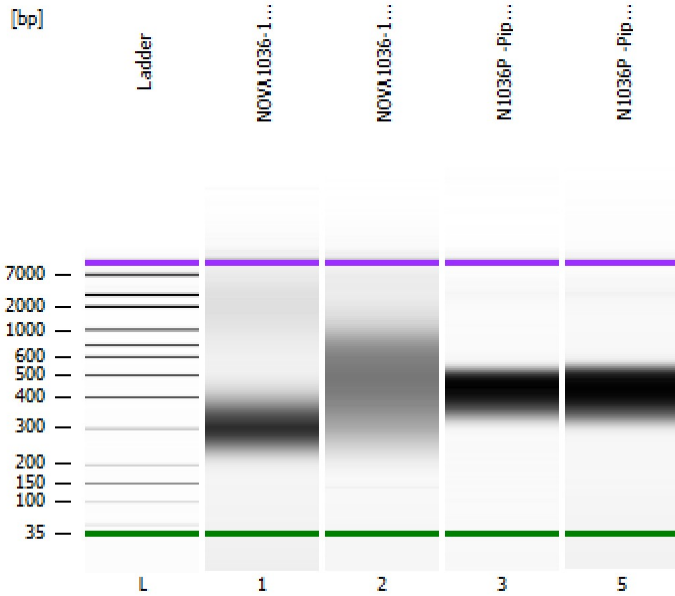

Instrument Information:

Instrument Name: DE34903152 Firmware: C.01.069
Serial#: DE34903152 Type: G2938C


Assay Information:

Assay Origin Path: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy
Assay Class: High Sensitivity DNA Assay
Version: 1.03
Assay Comments: Copyright © 2003-2010 Agilent Technologies


Chip Information:

Chip Lot #:
Reagent Kit Lot #:
Chip Comments:


NOVA1036-133 - F5 repeat SS Lib (1:4)

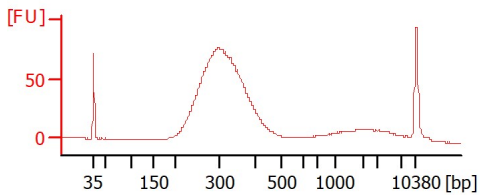


NOVA1036-133 - F5 repeat Lib (1:10)

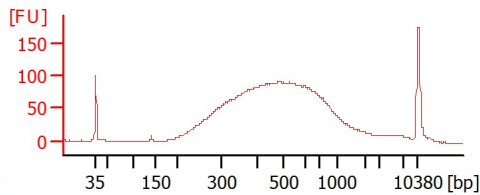

N1036P -Pippin SS 325-625

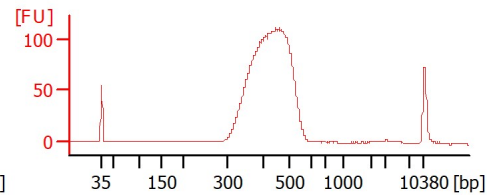

N1036P -Pippin SS 300-625

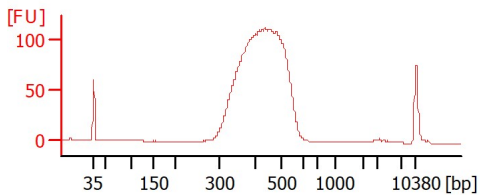

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...zer\2100 expert\data\2024-04-02\Nova1036_PippinSS_Pools.xad

Created: 4/2/2024 8:50:20 AM
 Modified: 4/2/2024 10:29:08 AM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
NOVA1036-133 - F5 repeat SS Lib (1:4)		<input type="checkbox"/>	✓			
NOVA1036-133 - F5 repeat Lib (1:10)		<input type="checkbox"/>	✓			
N1036P -Pippin SS 325-625		<input type="checkbox"/>	✓			
N1036P -Pippin SS 300-625		<input type="checkbox"/>	✓			
Ladder		<input type="checkbox"/>	✓			

Chip Lot #

Reagent Kit Lot #

Chip Comments :

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...zer\2100 expert\data\2024-04-02\Nova1036_PippinSS_Pools.xad

Created: 4/2/2024 8:50:20 AM
Modified: 4/2/2024 10:29:08 AM

Electrophoresis Assay Details

General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12
Minimum Visible Range [s] : 32
Maximum Visible Range [s] : 138
Start Analysis Time Range [s] : 33
End Analysis Time Range [s] : 137.5
Ladder Concentration [pg/ μ l] : 1950
Uses Standard Area for Ladder Fragments
Lower Marker Concentration [pg/ μ l] : 125
Upper Marker Concentration [pg/ μ l] : 75
Used Upper Marker for Quantitation
Standard Curve Fit is Point to Point
Show Data Aligned to Lower and Upper Marker

Integrator Settings

Integration Start Time [s] : 33.05
Integration End Time [s] : 137
Slope Threshold : 0.8
Height Threshold [FU] : 5
Area Threshold : 0.1
Width Threshold [s] : 0.6
Baseline Plateau [s] : 0.5

Filter Settings

Filter Width [s] : 0.5
Polynomial Order : 4


Ladder

Ladder Peak	Size	Area
1	35	160
2	50	210
3	100	208
4	150	221
5	200	242
6	300	270
7	400	305
8	500	306
9	600	336
10	700	321
11	1000	366
12	2000	413
13	3000	411
14	7000	400
15	10380	214

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...zer\2100 expert\data\2024-04-02\Nova1036_PippinSS_Pools.xad

Created: 4/2/2024 8:50:20 AM
 Modified: 4/2/2024 10:29:08 AM

Electropherogram Summary

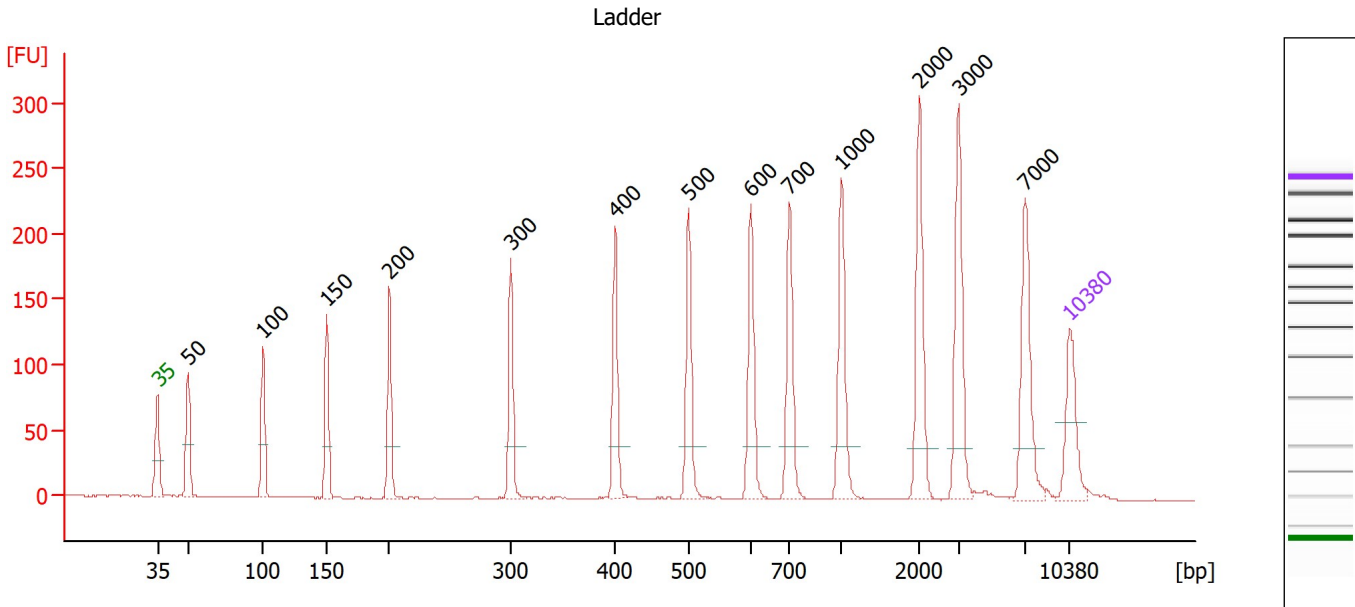

Overall Results for Ladder

Noise: 0.1


Peak table for Ladder

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	50	150.00	4,545.5	Ladder Peak
3	100	150.00	2,272.7	Ladder Peak
4	150	150.00	1,515.2	Ladder Peak
5	200	150.00	1,136.4	Ladder Peak
6	300	150.00	757.6	Ladder Peak
7	400	150.00	568.2	Ladder Peak
8	500	150.00	454.5	Ladder Peak
9	600	150.00	378.8	Ladder Peak
10	700	150.00	324.7	Ladder Peak
11	1,000	150.00	227.3	Ladder Peak
12	2,000	150.00	113.6	Ladder Peak
13	3,000	150.00	75.8	Ladder Peak
14	7,000	150.00	32.5	Ladder Peak
15	10,380	75.00	10.9	Upper Marker

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...zer\2100 expert\data\2024-04-02\Nova1036_PippinSS_Pools.xad

Created: 4/2/2024 8:50:20 AM
 Modified: 4/2/2024 10:29:08 AM

Electropherogram Summary Continued ...

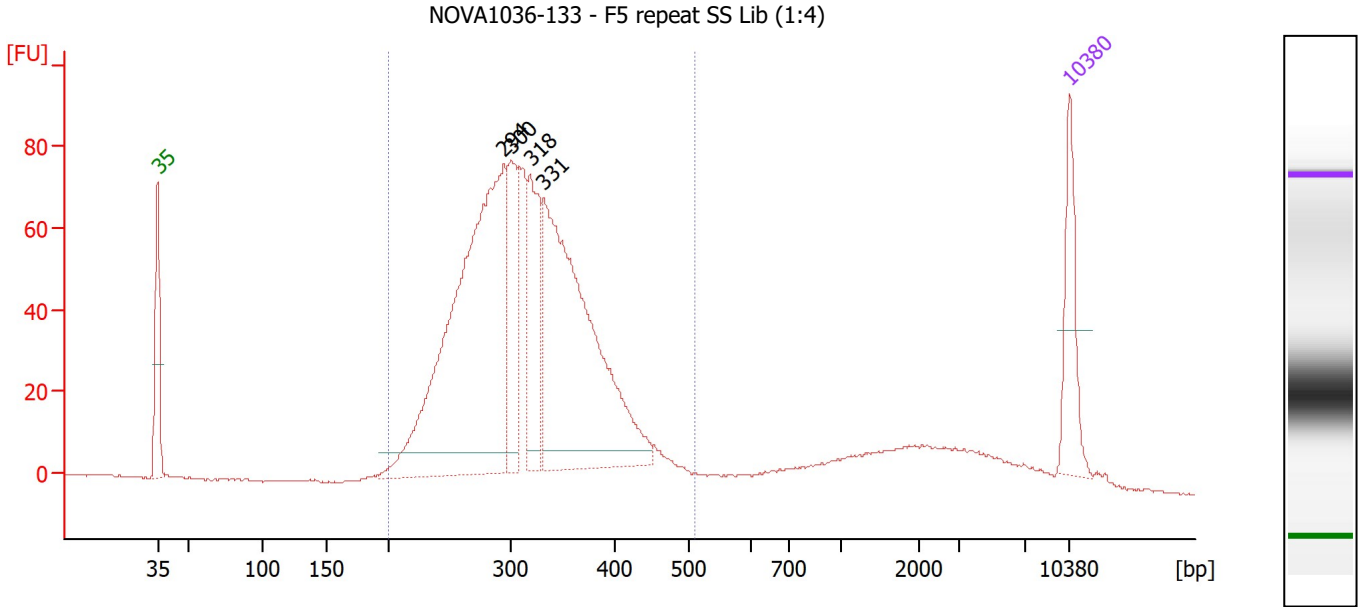

Overall Results for sample 1 : NOVA1036-133 - F5 repeat SS Lib (1:4)

Number of peaks found: 4 Corr. Area 1: 1,313.2
 Noise: 0.2

Peak table for sample 1 : NOVA1036-133 - F5 repeat SS Lib (1:4)

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	294	806.85	4,157.7	
3	300	155.11	784.4	
4	318	164.41	782.4	
5	331	585.56	2,677.4	
6	10,380	75.00	10.9	Upper Marker


Region table for sample 1 : NOVA1036-133 - F5 repeat SS Lib (1:4)

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	509	1,313.2	86	317	17.3	1,984.93	9,847.0	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...zer\2100 expert\data\2024-04-02\Nova1036_PippinSS_Pools.xad

Created: 4/2/2024 8:50:20 AM
 Modified: 4/2/2024 10:29:08 AM

Electropherogram Summary Continued ...

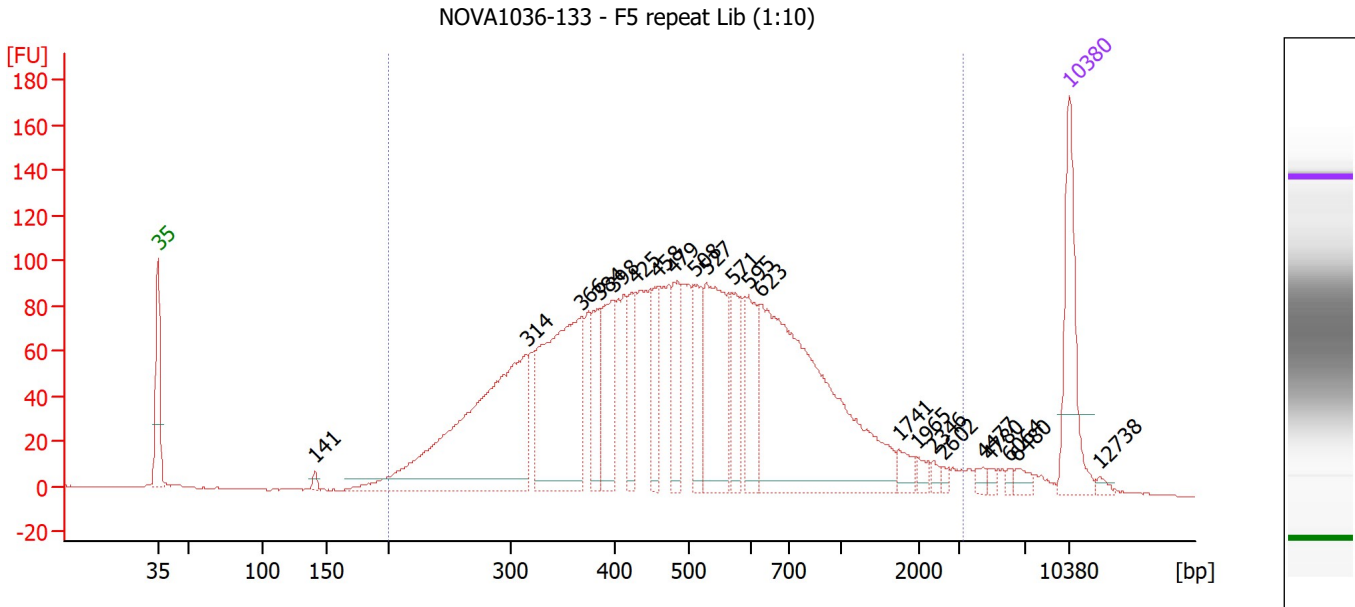

Overall Results for sample 2 : NOVA1036-133 - F5 repeat Lib (1:10)

Number of peaks found: 22 Corr. Area 1: 3,068.2
 Noise: 0.3

Peak table for sample 2 : NOVA1036-133 - F5 repeat Lib (1:10)

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	141	5.87	63.1	
3	314	387.38	1,866.5	
4	366	260.97	1,080.0	
5	384	55.30	218.1	
6	398	85.14	324.2	
7	425	49.61	176.8	
8	458	57.33	189.8	
9	479	61.64	195.0	
10	508	51.72	154.2	
11	527	145.12	416.9	
12	571	51.53	136.8	
13	595	60.32	153.6	
14	623	387.25	941.9	
15	1,741	13.68	11.9	
16	1,965	8.12	6.3	
17	2,346	5.22	3.4	
18	2,602	4.00	2.3	
19	4,477	5.15	1.7	
20	4,780	4.51	1.4	
21	6,064	3.38	0.8	
22	6,480	7.28	1.7	
23	10,380	75.00	10.9	Upper Marker
24	12,738	0.00	0.0	

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...zer\2100 expert\data\2024-04-02\Nova1036_PippinSS_Pools.xad

Created: 4/2/2024 8:50:20 AM
Modified: 4/2/2024 10:29:08 AM

Electropherogram Summary Continued ...

... Region table for sample 2 :


NOVA1036-133 - F5 repeat Lib (1:10)

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	3,241	3,068.2	96	579	67.7	2,134.94	7,605.7	■

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...zer\2100 expert\data\2024-04-02\Nova1036_PippinSS_Pools.xad

Created: 4/2/2024 8:50:20 AM
 Modified: 4/2/2024 10:29:08 AM

Electropherogram Summary Continued ...

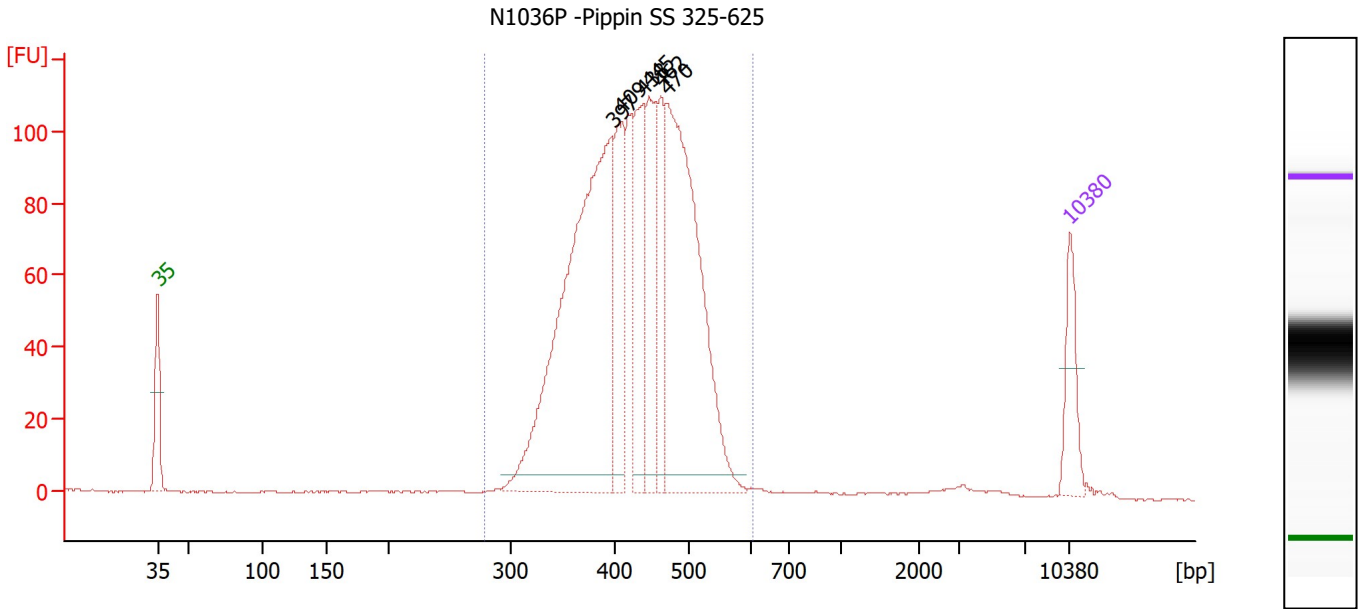

Overall Results for sample 3 : N1036P -Pippin SS 325-625

Number of peaks found: 6 Corr. Area 1: 1,533.2
 Noise: 0.2

Peak table for sample 3 : N1036P -Pippin SS 325-625

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	397	975.62	3,723.1	
3	409	207.55	769.2	
4	438	213.00	736.3	
5	445	228.37	777.2	
6	462	154.35	506.6	
7	470	725.34	2,336.6	
8	10,380	75.00	10.9	Upper Marker


Region table for sample 3 : N1036P -Pippin SS 325-625

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
278	602	1,533.2	97	428	13.7	2,740.50	9,924.1	Blue

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...zer\2100 expert\data\2024-04-02\Nova1036_PippinSS_Pools.xad

Created: 4/2/2024 8:50:20 AM
Modified: 4/2/2024 10:29:08 AM

Gel Image

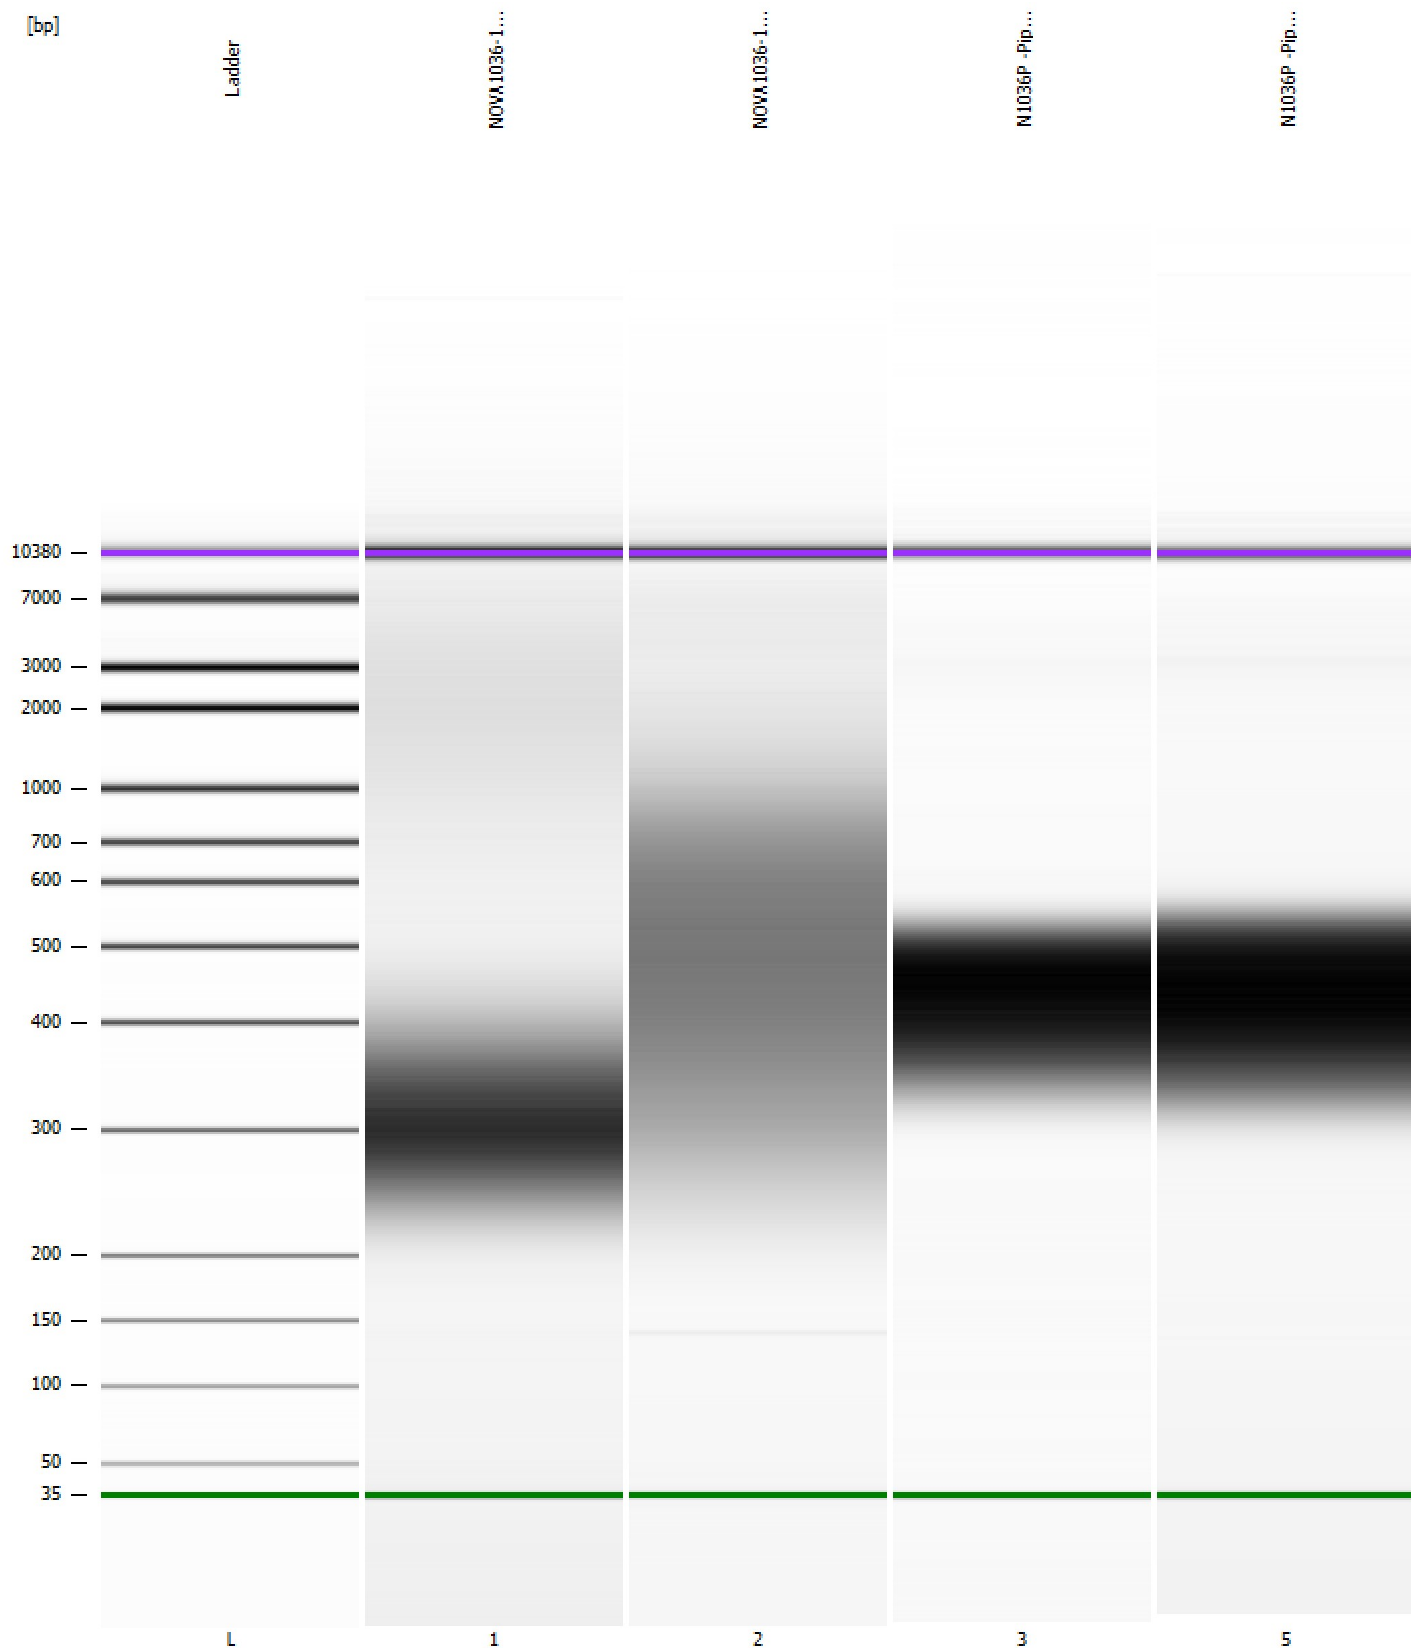

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...zer\2100 expert\data\2024-04-02\Nova1036_PippinSS_Pools.xad

Created: 4/2/2024 8:50:20 AM
 Modified: 4/2/2024 10:29:08 AM

Run Logbook

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 12)		Instrument	Run		4/2/2024 9:31:42 AM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Run started on port 1 (File: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\data\2024-04-02\Bioanalyzer1_High Sensitivity DNA Assay_DE34903152_2024-04-02_001.xad)		Instrument	Run		4/2/2024 8:50:26 AM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Product Number : G2938C		Instrument	Run		4/2/2024 8:50:26 AM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Name :		Instrument	Run		4/2/2024 8:50:26 AM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Vendor : Agilent Technologies		Instrument	Run		4/2/2024 8:50:26 AM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Serial# : DE34903152		Instrument	Run		4/2/2024 8:50:26 AM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Firmware : C.01.069		Instrument	Run		4/2/2024 8:50:26 AM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Cartridge : Electrode		Instrument	Run		4/2/2024 8:50:26 AM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB