


Assay Class: Eukaryote Total RNA Pico
Data Path: Z:\...02\Bioanalyzer1_Eukaryote Total RNA Pico_2020-06-02_002.xad

Created: 6/2/2020 3:31:28 PM
Modified: 6/2/2020 3:50:01 PM

Electrophoresis File Run Summary

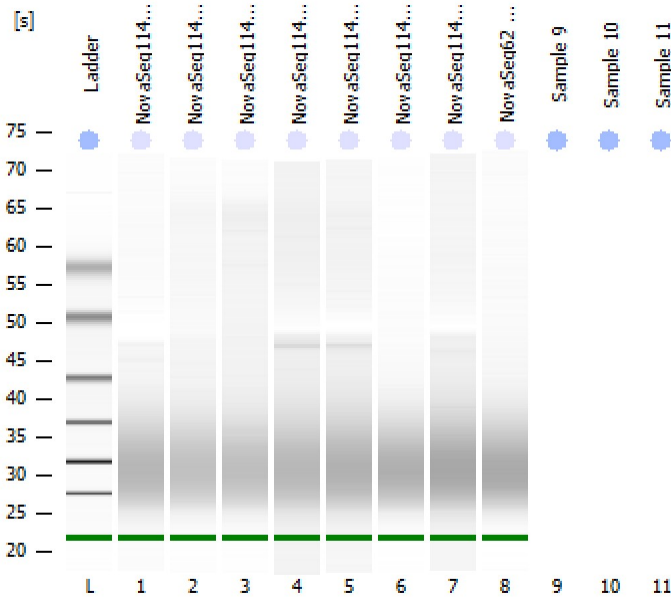

Instrument Information:

Instrument Name: DE34903152 Firmware: C.01.069
Serial#: DE34903152 Type: G2938C


Assay Information:

Assay Origin Path: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\assays\RNA\Eukaryote Total RNA Pico Series II.xsy
Assay Class: Eukaryote Total RNA Pico
Version: 2.6
Assay Comments: Total RNA Analysis pg sensitivity (Eukaryote)
© Copyright 2003 - 2009 Agilent Technologies, Inc.


Chip Information:

Chip Lot #:
Reagent Kit Lot #:
Chip Comments:


NovaSeq114 - 23 BC DNA 50ng input
RIN: 2.50

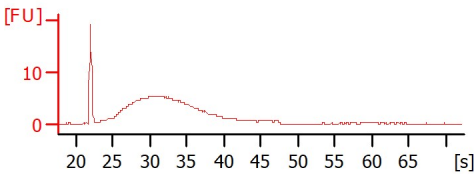


NovaSeq114 - 28 BC DNA 50ng input
RIN: 2.10

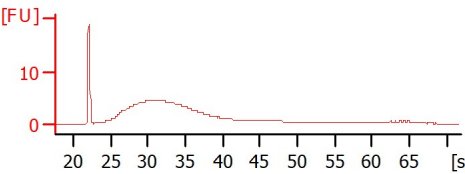


NovaSeq114 - 35 BC DNA 50ng input
RIN: 2.10

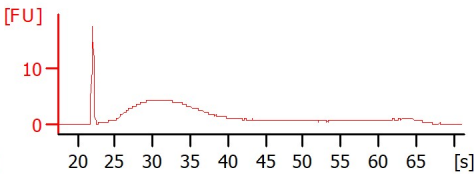


NovaSeq114 - 36 BC DNA 50ng input
RIN: 2.20

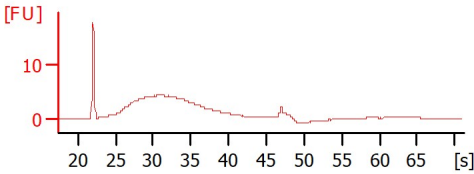


NovaSeq114 - 37 BC DNA 50ng input
RIN: 2.20

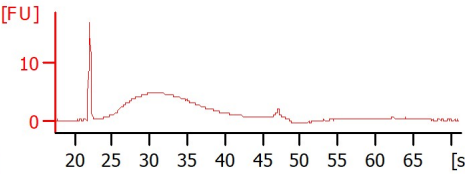


NovaSeq114 - 39 BC DNA 50ng input
RIN: 2.20

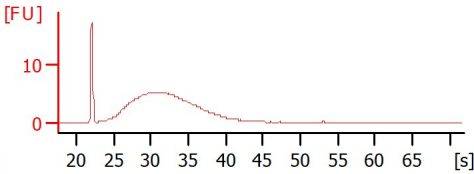

NovaSeq114 - 40 BC DNA 50ng input
RIN: 2.40

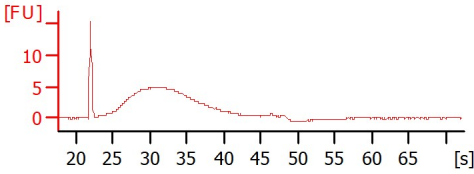



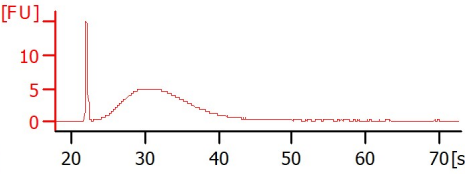









NovaSeq62 - 42 BC DNA 50ng input Posi...
RIN: 2.20



Assay Class: Eukaryote Total RNA Pico
 Data Path: Z:\...02\Bioanalyzer1_Eukaryote Total RNA Pico_2020-06-02_002.xad

Created: 6/2/2020 3:31:28 PM
 Modified: 6/2/2020 3:50:01 PM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Status	Result Label	Result Color
NovaSeq114 - 23 BC DNA 50ng input		✓	RIN: 2.50	
NovaSeq114 - 28 BC DNA 50ng input		✓	RIN: 2.10	
NovaSeq114 - 35 BC DNA 50ng input		✓	RIN: 2.10	
NovaSeq114 - 36 BC DNA 50ng input		✓	RIN: 2.20	
NovaSeq114 - 37 BC DNA 50ng input		✓	RIN: 2.20	
NovaSeq114 - 39 BC DNA 50ng input		✓	RIN: 2.20	
NovaSeq114 - 40 BC DNA 50ng input		✓	RIN: 2.40	
NovaSeq62 - 42 BC DNA 50ng input Positive ctrl		✓	RIN: 2.20	
Sample 9				
Sample 10				
Sample 11				
Ladder		✓	All Other Samples	

Chip Lot #

Reagent Kit Lot #

Chip Comments :

Assay Class: Eukaryote Total RNA Pico
 Data Path: Z:\...02\Bioanalyzer1_Eukaryote Total RNA Pico_2020-06-02_002.xad

Created: 6/2/2020 3:31:28 PM
 Modified: 6/2/2020 3:50:01 PM

Electrophoresis Assay Details

General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12
 Minimum Visible Range [s] : 17
 Maximum Visible Range [s] : 70
 Start Analysis Time Range [s] : 18
 End Analysis Time Range [s] : 69
 Ladder Concentration [pg/μl] : 1000
 Lower Marker Concentration [pg/μl] : 0
 Upper Marker Concentration [pg/μl] : 0
 Used Lower Marker for Quantitation
 Standard Curve Fit is Logarithmic
 Show Data Aligned to Lower Marker

Integrator Settings

Integration Start Time [s] : 18
 Integration End Time [s] : 69
 Slope Threshold : 0.6
 Height Threshold [FU] : 0.5
 Area Threshold : 0.2
 Width Threshold [s] : 0.3
 Baseline Plateau [s] : 6

Filter Settings

Filter Width [s] : 0.5
 Polynomial Order : 4


Ladder

Ladder Peak	Size
1	25
2	200
3	500
4	1000
5	2000
6	4000

Assay Class: Eukaryote Total RNA Pico
Data Path: Z:\...02\Bioanalyzer1_Eukaryote Total RNA Pico_2020-06-02_002.xad

Created: 6/2/2020 3:31:28 PM
Modified: 6/2/2020 3:50:01 PM

Electropherogram Summary

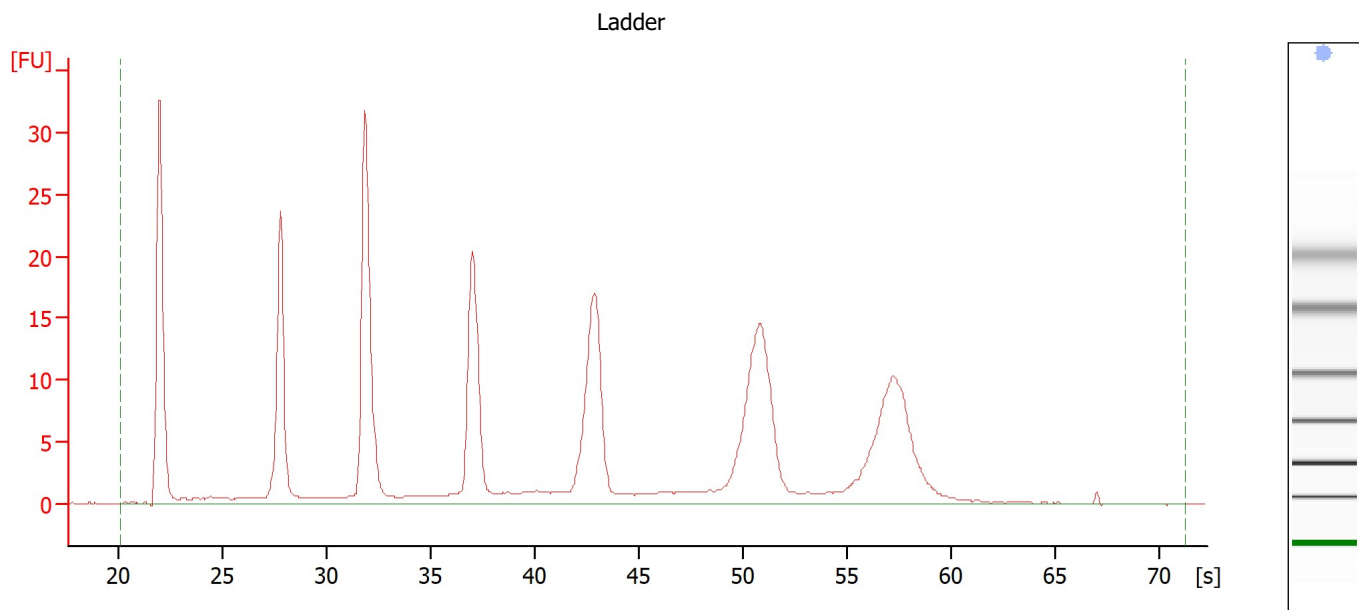

Overall Results for Ladder


RNA Area:	279.2	Result Flagging Color:	
RNA Concentration:	1,000 pg/μl	Result Flagging Label:	All Other Samples

Assay Class: Eukaryote Total RNA Pico
 Data Path: Z:\...02\Bioanalyzer1_Eukaryote Total RNA Pico_2020-06-02_002.xad

Created: 6/2/2020 3:31:28 PM
 Modified: 6/2/2020 3:50:01 PM

Electropherogram Summary Continued ...

NovaSeq114 - 23 BC DNA 50ng input

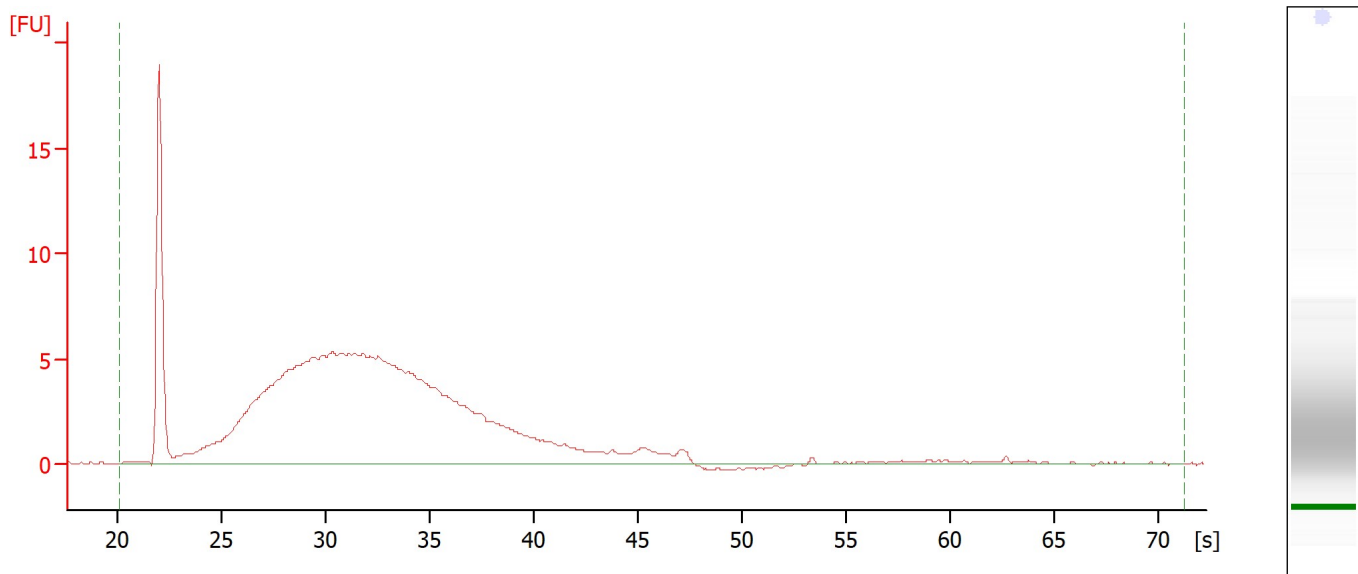

Overall Results for sample 1 : NovaSeq114 - 23 BC DNA 50ng input


RNA Area:	191.5	RNA Integrity Number (RIN):	2.5 (B.02.10)
RNA Concentration:	686 pg/μl	Result Flagging Color:	
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN: 2.50

Assay Class: Eukaryote Total RNA Pico
Data Path: Z:\...02\Bioanalyzer1_Eukaryote Total RNA Pico_2020-06-02_002.xad

Created: 6/2/2020 3:31:28 PM
Modified: 6/2/2020 3:50:01 PM

Electropherogram Summary Continued ...

NovaSeq114 - 28 BC DNA 50ng input

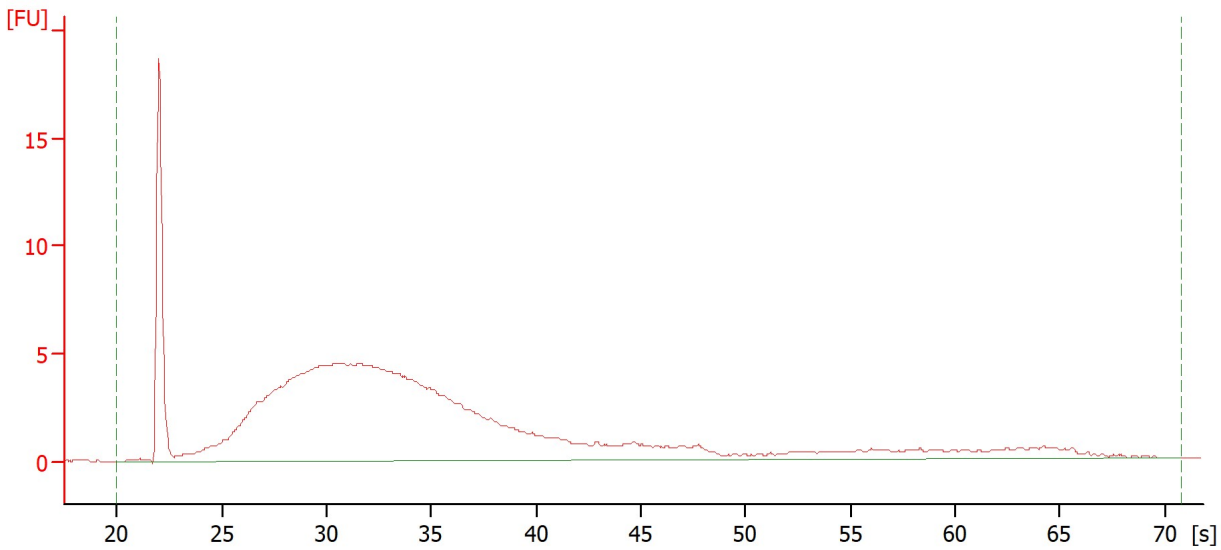

Overall Results for sample 2 : NovaSeq114 - 28 BC DNA 50ng input


RNA Area:	180.6	RNA Integrity Number (RIN):	2.1 (B.02.10)
RNA Concentration:	647 pg/μl	Result Flagging Color:	
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN: 2.10

Assay Class: Eukaryote Total RNA Pico
Data Path: Z:\...02\Bioanalyzer1_Eukaryote Total RNA Pico_2020-06-02_002.xad

Created: 6/2/2020 3:31:28 PM
Modified: 6/2/2020 3:50:01 PM

Electropherogram Summary Continued ...

NovaSeq114 - 35 BC DNA 50ng input

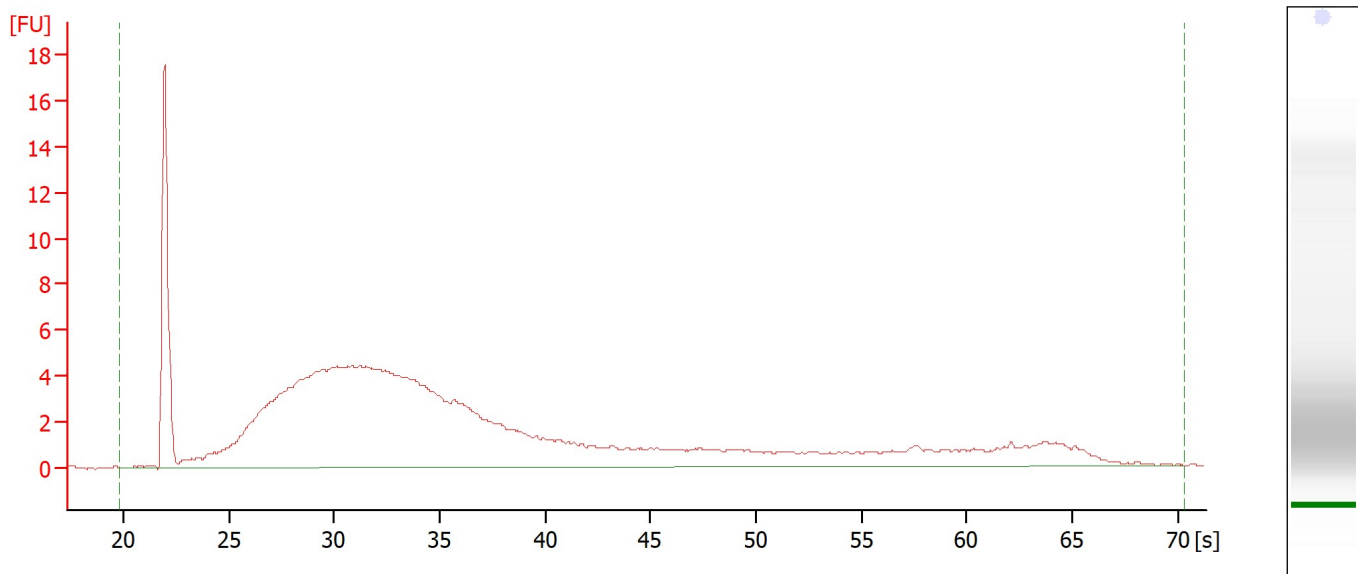

Overall Results for sample 3 : NovaSeq114 - 35 BC DNA 50ng input


RNA Area:	185.3	RNA Integrity Number (RIN):	2.1 (B.02.10)
RNA Concentration:	664 µg/µl	Result Flagging Color:	
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN: 2.10

Assay Class: Eukaryote Total RNA Pico
 Data Path: Z:\...02\Bioanalyzer1_Eukaryote Total RNA Pico_2020-06-02_002.xad

Created: 6/2/2020 3:31:28 PM
 Modified: 6/2/2020 3:50:01 PM

Electropherogram Summary Continued ...

NovaSeq114 - 36 BC DNA 50ng input

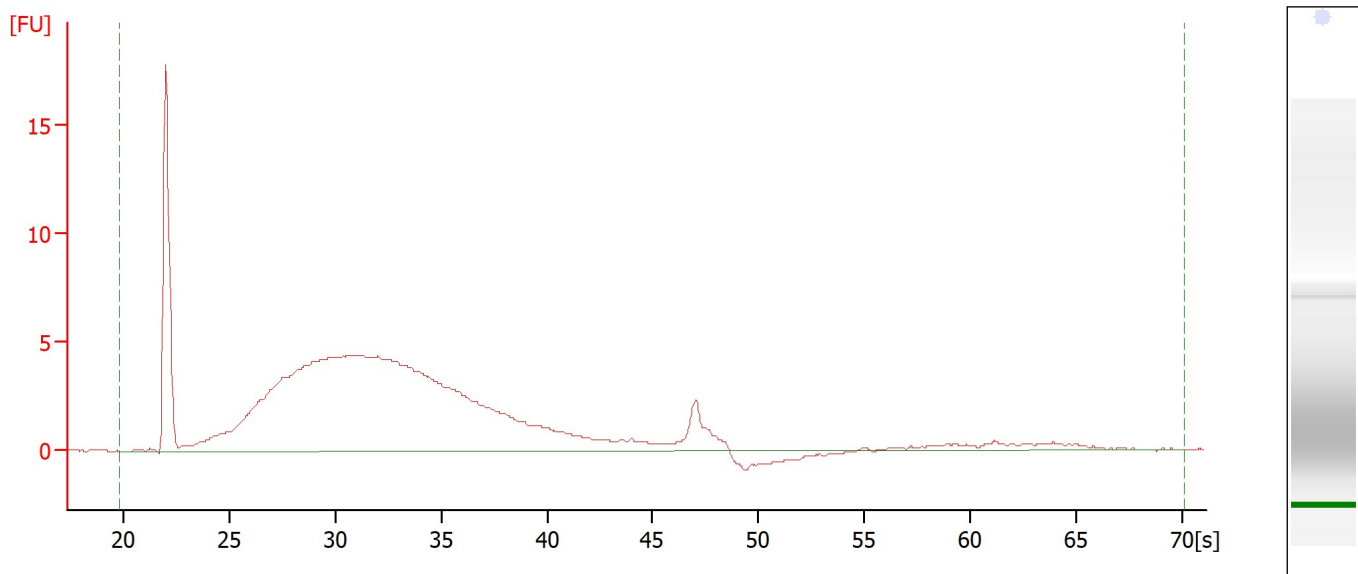

Overall Results for sample 4 : NovaSeq114 - 36 BC DNA 50ng input


RNA Area:	164.8	RNA Integrity Number (RIN):	2.2 (B.02.10)
RNA Concentration:	590 pg/μl	Result Flagging Color:	
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN: 2.20

Assay Class: Eukaryote Total RNA Pico
 Data Path: Z:\...02\Bioanalyzer1_Eukaryote Total RNA Pico_2020-06-02_002.xad

Created: 6/2/2020 3:31:28 PM
 Modified: 6/2/2020 3:50:01 PM

Electropherogram Summary Continued ...

NovaSeq114 - 37 BC DNA 50ng input

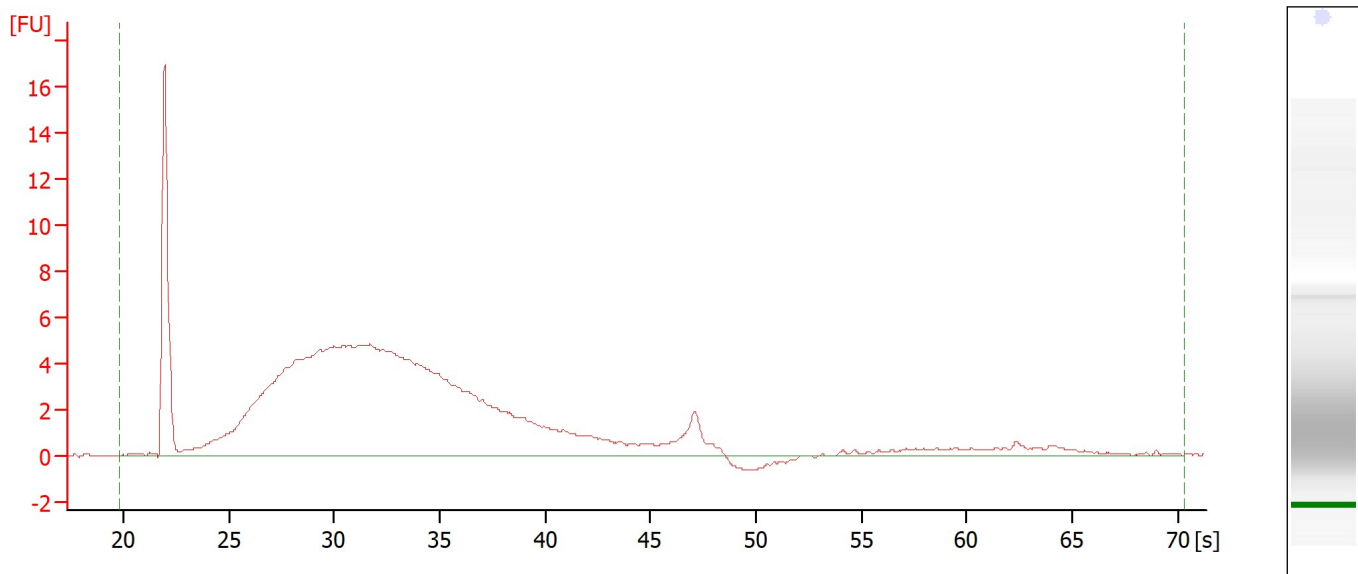

Overall Results for sample 5 : NovaSeq114 - 37 BC DNA 50ng input


RNA Area:	181.5	RNA Integrity Number (RIN):	2.2 (B.02.10)
RNA Concentration:	650 pg/μl	Result Flagging Color:	
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN: 2.20

Assay Class: Eukaryote Total RNA Pico
Data Path: Z:\...02\Bioanalyzer1_Eukaryote Total RNA Pico_2020-06-02_002.xad

Created: 6/2/2020 3:31:28 PM
Modified: 6/2/2020 3:50:01 PM

Electropherogram Summary Continued ...

NovaSeq114 - 39 BC DNA 50ng input

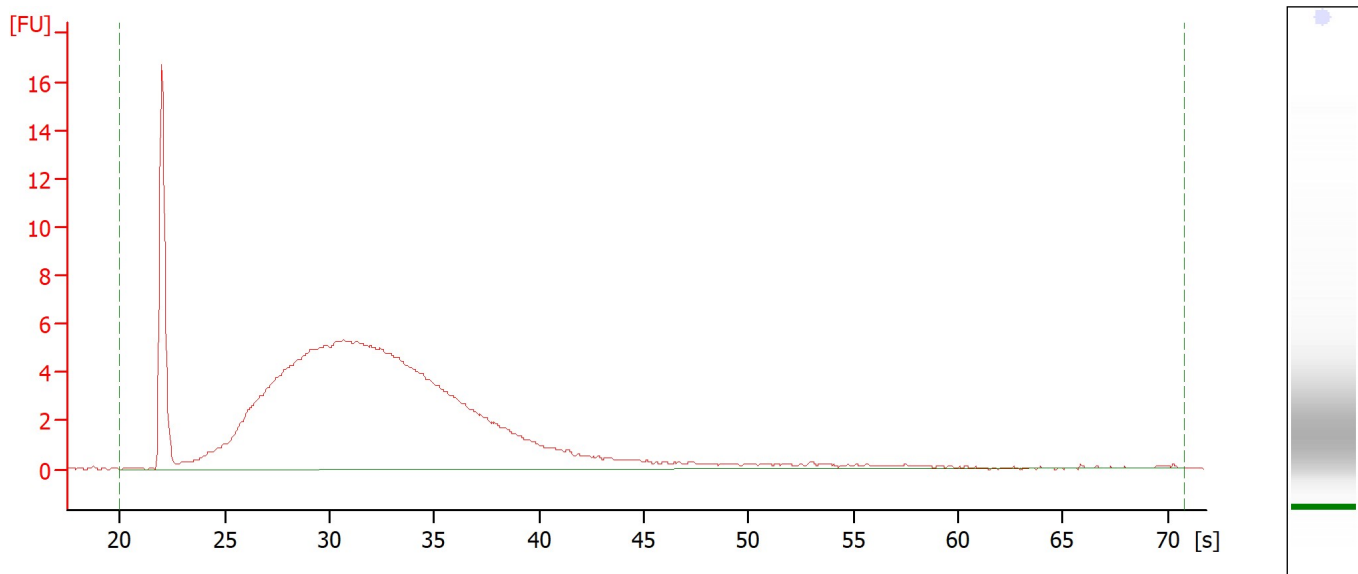

Overall Results for sample 6 : NovaSeq114 - 39 BC DNA 50ng input


RNA Area:	181.5	RNA Integrity Number (RIN):	2.2 (B.02.10)
RNA Concentration:	650 pg/μl	Result Flagging Color:	
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN: 2.20

Assay Class: Eukaryote Total RNA Pico
 Data Path: Z:\...02\Bioanalyzer1_Eukaryote Total RNA Pico_2020-06-02_002.xad

Created: 6/2/2020 3:31:28 PM
 Modified: 6/2/2020 3:50:01 PM

Electropherogram Summary Continued ...

NovaSeq114 - 40 BC DNA 50ng input

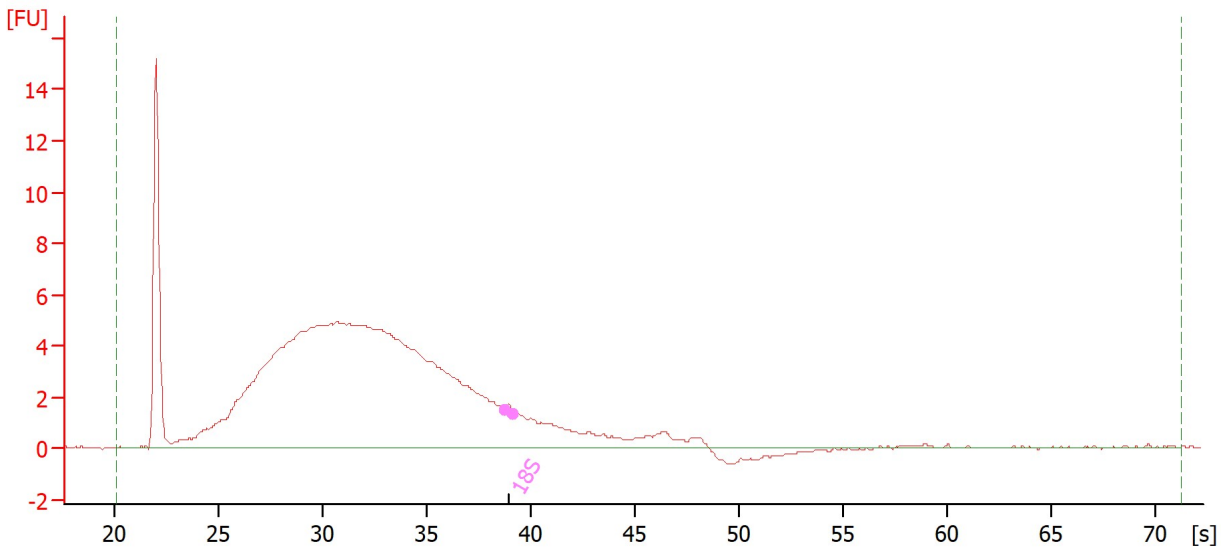

Overall Results for sample 7 : NovaSeq114 - 40 BC DNA 50ng input

RNA Area:	173.7	RNA Integrity Number (RIN):	2.4 (B.02.10)
RNA Concentration:	622 pg/μl	Result Flagging Color:	
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN: 2.40

Fragment table for sample 7 : NovaSeq114 - 40 BC DNA 50ng input


Name	Start Time [s]	End Time [s]	Area	% of total Area
18S	38.73	39.20	0.2	0.1

Assay Class: Eukaryote Total RNA Pico
Data Path: Z:\...02\Bioanalyzer1_Eukaryote Total RNA Pico_2020-06-02_002.xad

Created: 6/2/2020 3:31:28 PM
Modified: 6/2/2020 3:50:01 PM

Electropherogram Summary Continued ...

NovaSeq62 - 42 BC DNA 50ng input Positive ctrl

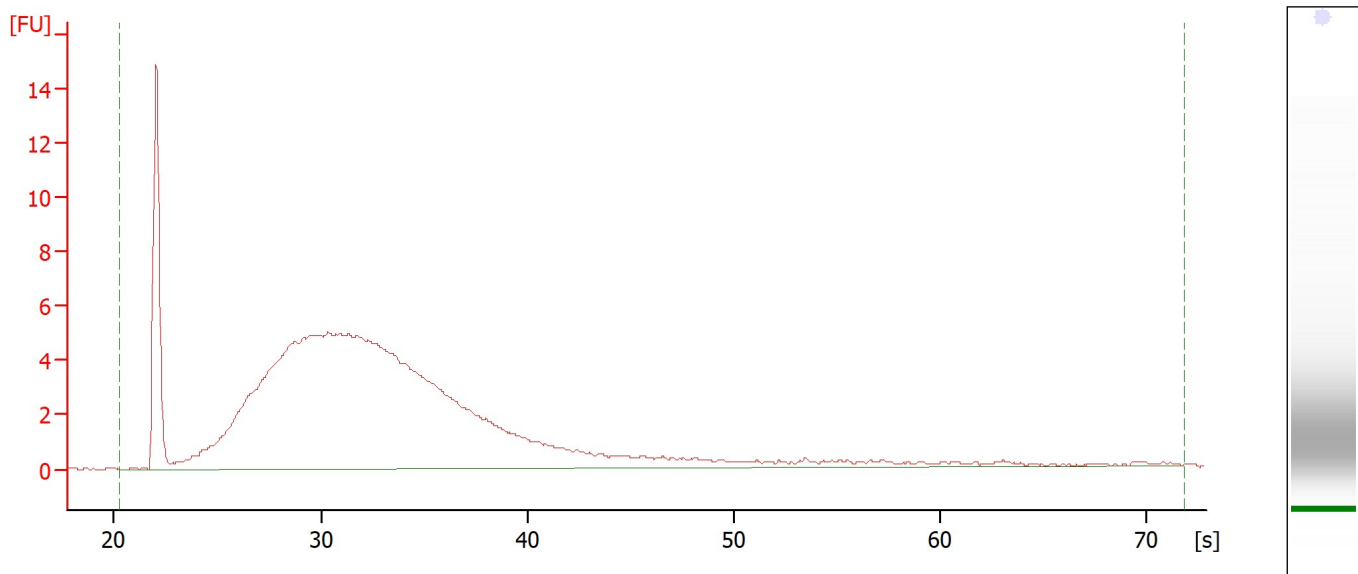


Overall Results for sample 8 : NovaSeq62 - 42 BC DNA 50ng input Positive ctrl

RNA Area:	177.5	RNA Integrity Number (RIN):	2.2 (B.02.10)
RNA Concentration:	636 µg/µl	Result Flagging Color:	
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN: 2.20

Assay Class: Eukaryote Total RNA Pico
Data Path: Z:\...02\Bioanalyzer1_Eukaryote Total RNA Pico_2020-06-02_002.xad

Created: 6/2/2020 3:31:28 PM
Modified: 6/2/2020 3:50:01 PM

Gel Image

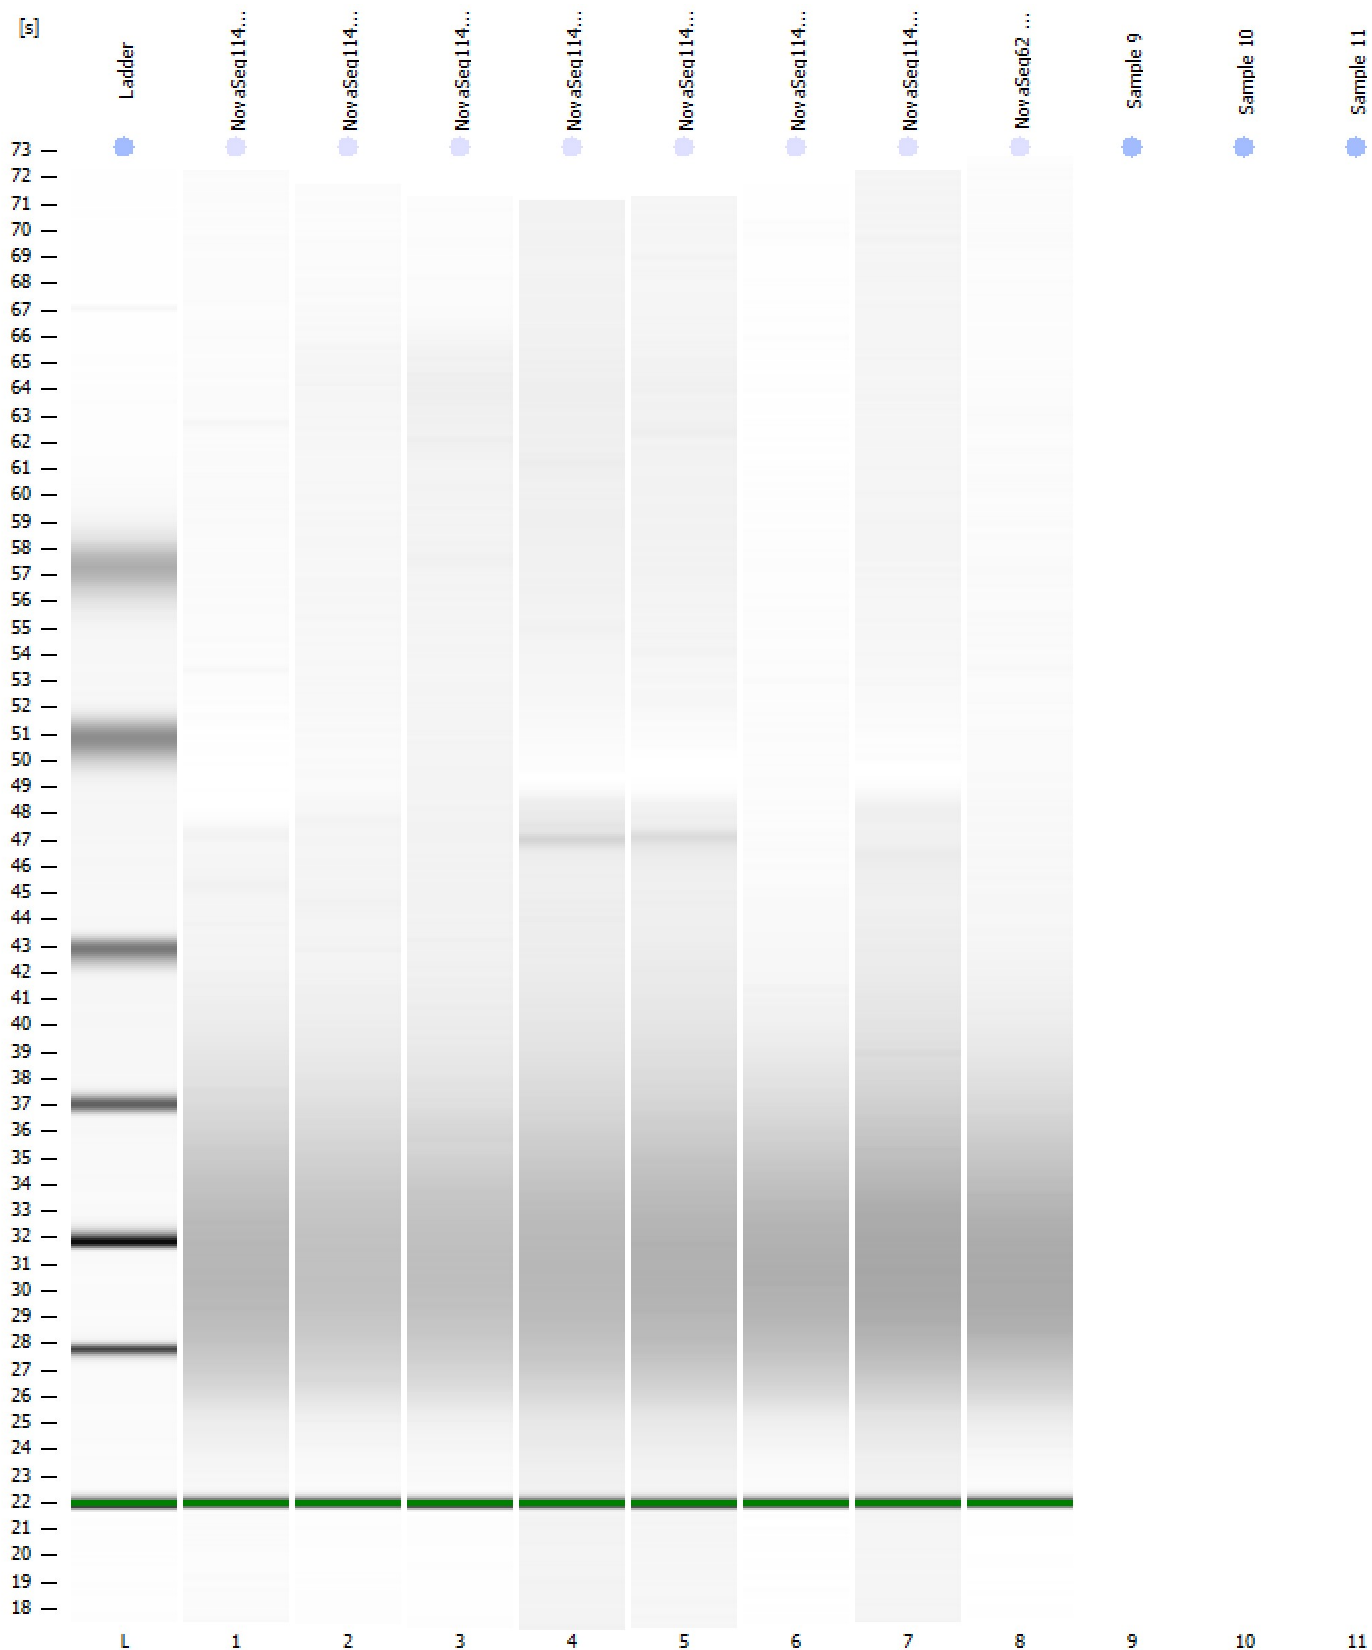

Assay Class: Eukaryote Total RNA Pico
Data Path: Z:\...02\Bioanalyzer1_Eukaryote Total RNA Pico_2020-06-02_002.xad

Created: 6/2/2020 3:31:28 PM
Modified: 6/2/2020 3:50:01 PM

Invalid Samples

Sample 9 has not been run, no results available.

Sample 10 has not been run, no results available.

Sample 11 has not been run, no results available.

Assay Class: Eukaryote Total RNA Pico
 Data Path: Z:\...02\Bioanalyzer1_Eukaryote Total RNA Pico_2020-06-02_002.xad
 Created: 6/2/2020 3:31:28 PM
 Modified: 6/2/2020 3:50:01 PM

Run Logbook

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 9)		Instrument	Run		6/2/2020 3:49:59 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Run started on port 1 (File: Z:\XADs\2020-06-02\Bioanalyze r1_Eukaryote Total RNA Pico_2020-06-02_002.xad)		Instrument	Run		6/2/2020 3:31:28 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Product Number : G2938C		Instrument	Run		6/2/2020 3:31:28 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Name :		Instrument	Run		6/2/2020 3:31:28 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Vendor : Agilent Technologies		Instrument	Run		6/2/2020 3:31:28 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Serial# : DE34903152		Instrument	Run		6/2/2020 3:31:28 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Firmware : C.01.069		Instrument	Run		6/2/2020 3:31:28 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Cartridge : Electrode		Instrument	Run		6/2/2020 3:31:28 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB