

Assay Class: Eukaryote Total RNA Pico  
Data Path: Z:\...28\Bioanalyzer1\_Eukaryote Total RNA Pico\_2020-09-28\_001.xad

Created: 9/28/2020 1:09:50 PM  
Modified: 9/28/2020 1:32:46 PM

**Electrophoresis File Run Summary**

Instrument Information:

Instrument Name: DE34903152      Firmware: C.01.069  
Serial#: DE34903152      Type: G2938C

Assay Information:

Assay Origin Path: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\assays\RNA\Eukaryote Total RNA Pico Series II.xsy

Assay Class: Eukaryote Total RNA Pico

Version: 2.6

Assay Comments: Total RNA Analysis pg sensitivity (Eukaryote)


© Copyright 2003 - 2009 Agilent Technologies, Inc.

Chip Information:

Chip Lot #:

Reagent Kit Lot #:

Chip Comments:

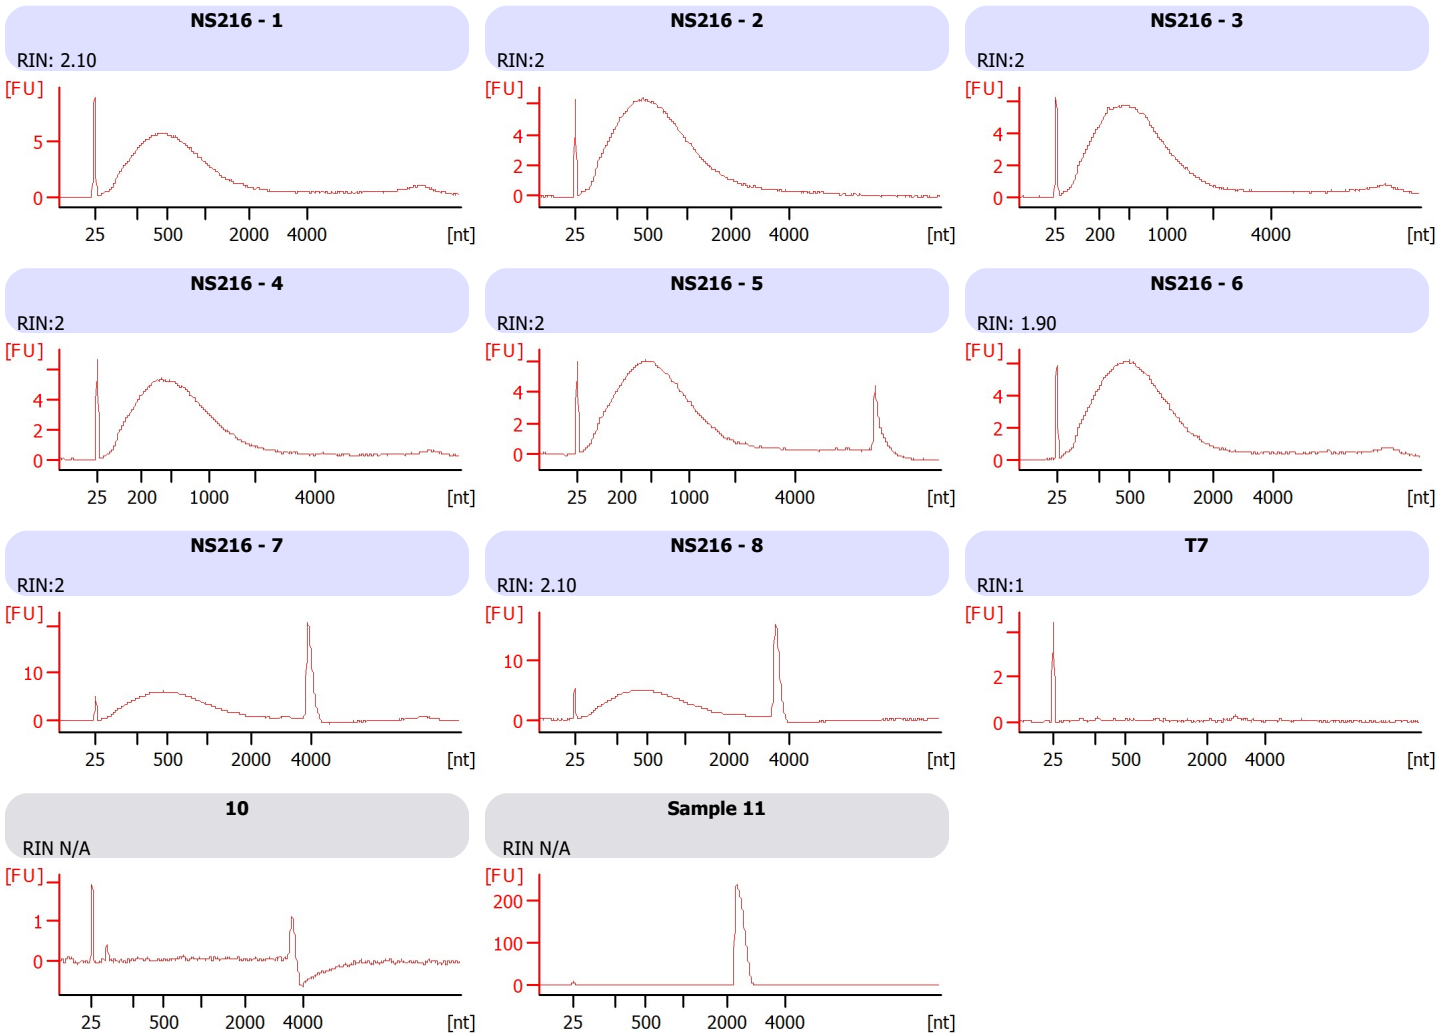

Assay Class: Eukaryote Total RNA Pico  
 Data Path: Z:\...28\Bioanalyzer1\_Eukaryote Total RNA Pico\_2020-09-28\_001.xad

Created: 9/28/2020 1:09:50 PM  
 Modified: 9/28/2020 1:32:46 PM

**Electrophoresis File Run Summary (Chip Summary)**

Sample Name	Sample Comment	Status	Result Label	Result Color
NS216 - 1		✓	RIN: 2.10	
NS216 - 2		✓	RIN:2	
NS216 - 3		✓	RIN:2	
NS216 - 4		✓	RIN:2	
NS216 - 5		✓	RIN:2	
NS216 - 6		✓	RIN: 1.90	
NS216 - 7		✓	RIN:2	
NS216 - 8		✓	RIN: 2.10	
T7		✓	RIN:1	
10		✓	RIN N/A	
Sample 11		✓	RIN N/A	
Ladder		✓	All Other Samples	

**Chip Lot #**

**Reagent Kit Lot #**

**Chip Comments :**

Assay Class: Eukaryote Total RNA Pico  
 Data Path: Z:\...28\Bioanalyzer1\_Eukaryote Total RNA Pico\_2020-09-28\_001.xad

Created: 9/28/2020 1:09:50 PM  
 Modified: 9/28/2020 1:32:46 PM

**Electrophoresis Assay Details**

**General Analysis Settings**

Number of Available Sample and Ladder Wells (Max.) : 12  
 Minimum Visible Range [s] : 17  
 Maximum Visible Range [s] : 70  
 Start Analysis Time Range [s] : 18  
 End Analysis Time Range [s] : 69  
 Ladder Concentration [pg/μl] : 1000  
 Lower Marker Concentration [pg/μl] : 0  
 Upper Marker Concentration [pg/μl] : 0  
 Used Lower Marker for Quantitation  
 Standard Curve Fit is Logarithmic  
 Show Data Aligned to Lower Marker

**Integrator Settings**

Integration Start Time [s] : 18  
 Integration End Time [s] : 69  
 Slope Threshold : 0.6  
 Height Threshold [FU] : 0.5  
 Area Threshold : 0.2  
 Width Threshold [s] : 0.3  
 Baseline Plateau [s] : 6

**Filter Settings**

Filter Width [s] : 0.5  
 Polynomial Order : 4


**Ladder**

Ladder Peak	Size
1	25
2	200
3	500
4	1000
5	2000
6	4000

Assay Class: Eukaryote Total RNA Pico  
Data Path: Z:\...28\Bioanalyzer1\_Eukaryote Total RNA Pico\_2020-09-28\_001.xad

Created: 9/28/2020 1:09:50 PM  
Modified: 9/28/2020 1:32:46 PM

**Electropherogram Summary**

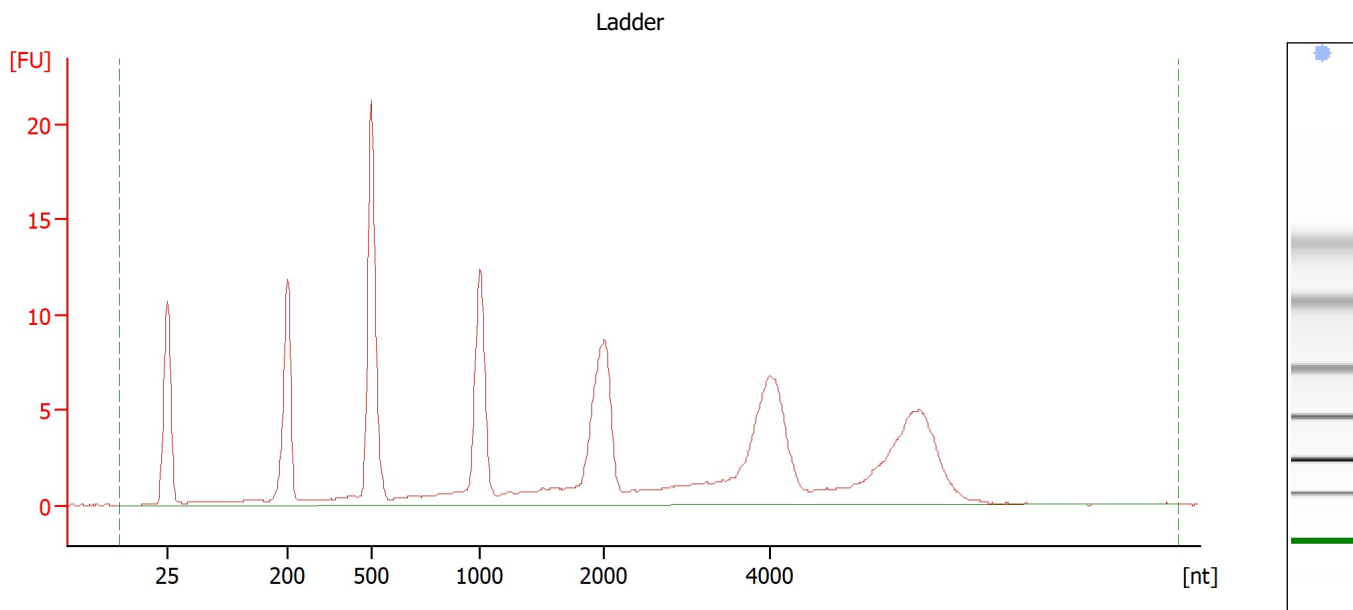


**Overall Results for Ladder**

RNA Area:	173.2	Result Flagging Color:	<span style="background-color: #add8e6; border: 1px solid black; display: inline-block; width: 20px; height: 10px;"></span>
RNA Concentration:	1,000 pg/μl	Result Flagging Label:	All Other Samples

Assay Class: Eukaryote Total RNA Pico  
 Data Path: Z:\...28\Bioanalyzer1\_Eukaryote Total RNA Pico\_2020-09-28\_001.xad

Created: 9/28/2020 1:09:50 PM  
 Modified: 9/28/2020 1:32:46 PM

**Electropherogram Summary Continued ...**

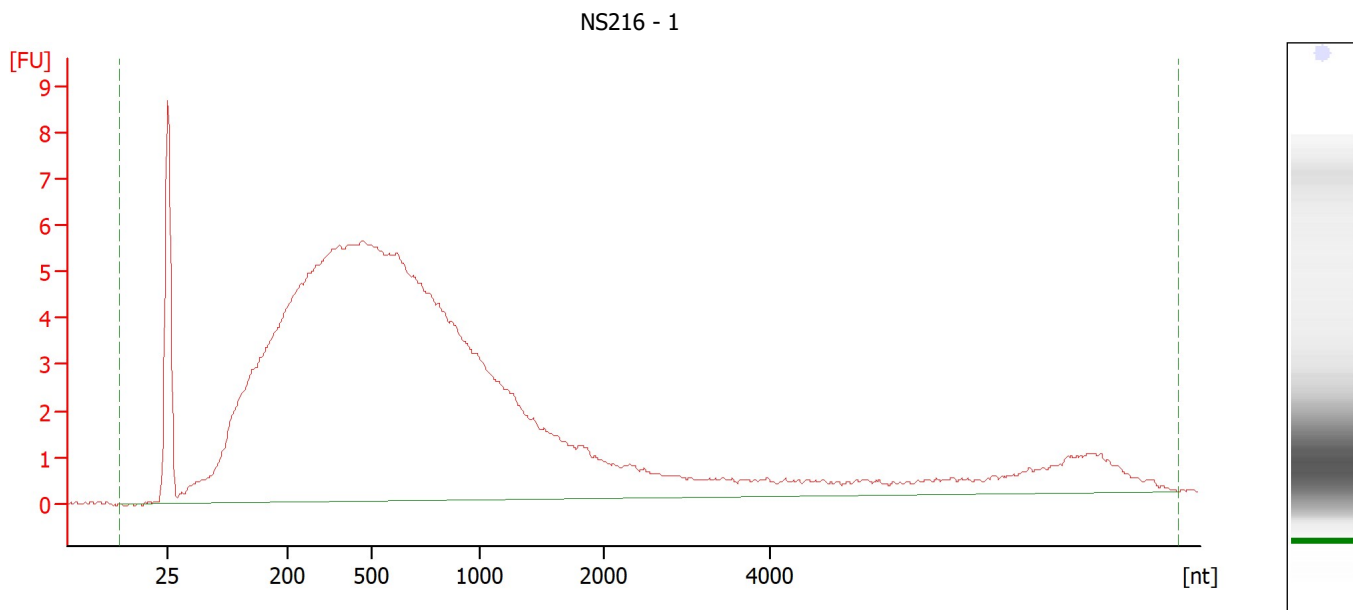


**Overall Results for sample 1 : NS216 - 1**

RNA Area:	219.0	RNA Integrity Number (RIN):	2.1 (B.02.10)
RNA Concentration:	1,264 pg/μl	Result Flagging Color:	<span style="background-color: #ccccff; border: 1px solid black; display: inline-block; width: 20px; height: 10px;"></span>
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN: 2.10

Assay Class: Eukaryote Total RNA Pico  
 Data Path: Z:\...28\Bioanalyzer1\_Eukaryote Total RNA Pico\_2020-09-28\_001.xad

Created: 9/28/2020 1:09:50 PM  
 Modified: 9/28/2020 1:32:46 PM

**Electropherogram Summary Continued ...**

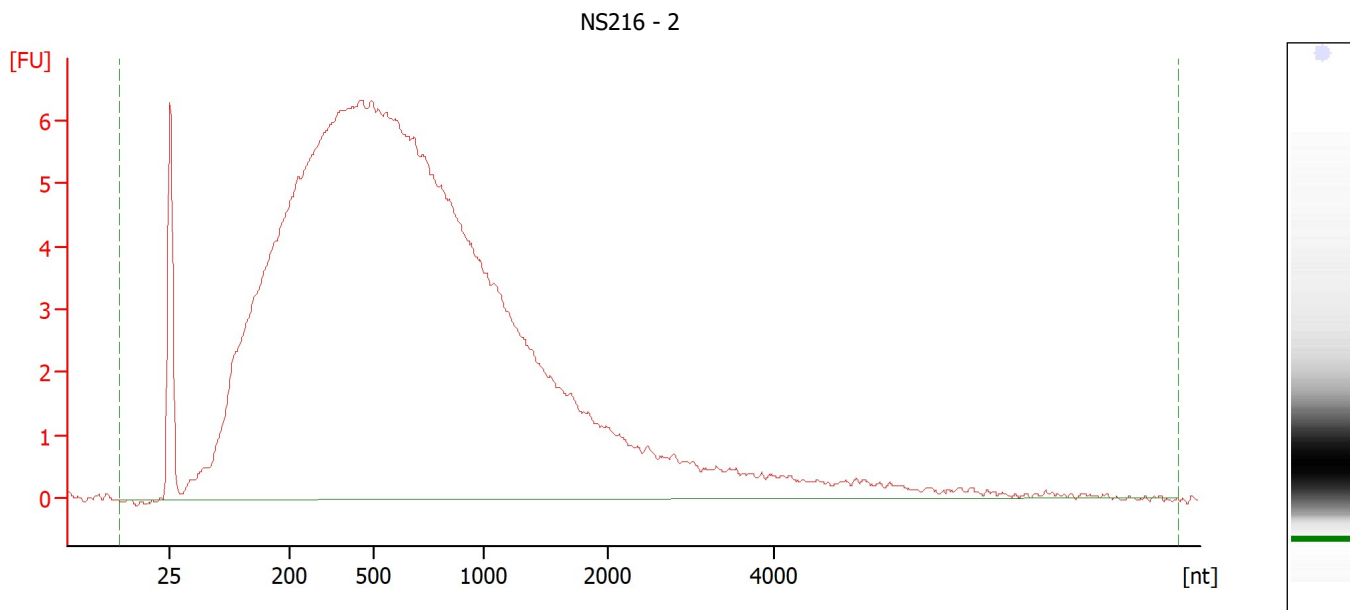


**Overall Results for sample 2 : NS216 - 2**

RNA Area:	246.8	RNA Integrity Number (RIN):	2 (B.02.10)
RNA Concentration:	1,425 pg/μl	Result Flagging Color:	<span style="background-color: #ccccff; border: 1px solid black; display: inline-block; width: 20px; height: 10px;"></span>
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN:2

Assay Class: Eukaryote Total RNA Pico  
Data Path: Z:\...28\Bioanalyzer1\_Eukaryote Total RNA Pico\_2020-09-28\_001.xad

Created: 9/28/2020 1:09:50 PM  
Modified: 9/28/2020 1:32:46 PM

**Electropherogram Summary Continued ...**

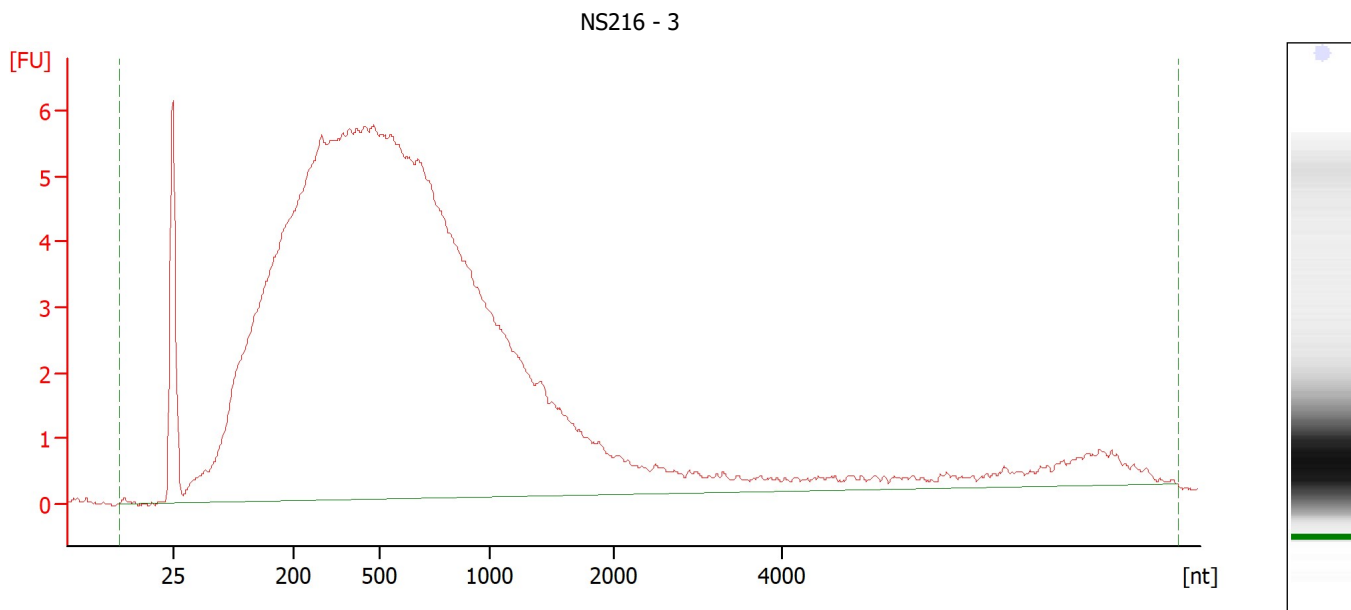


**Overall Results for sample 3 : NS216 - 3**

RNA Area:	216.5	RNA Integrity Number (RIN):	2 (B.02.10)
RNA Concentration:	1,250 pg/μl	Result Flagging Color:	<span style="background-color: #ccccff; border: 1px solid black; display: inline-block; width: 20px; height: 10px;"></span>
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN:2

Assay Class: Eukaryote Total RNA Pico  
 Data Path: Z:\...28\Bioanalyzer1\_Eukaryote Total RNA Pico\_2020-09-28\_001.xad

Created: 9/28/2020 1:09:50 PM  
 Modified: 9/28/2020 1:32:46 PM

**Electropherogram Summary Continued ...**

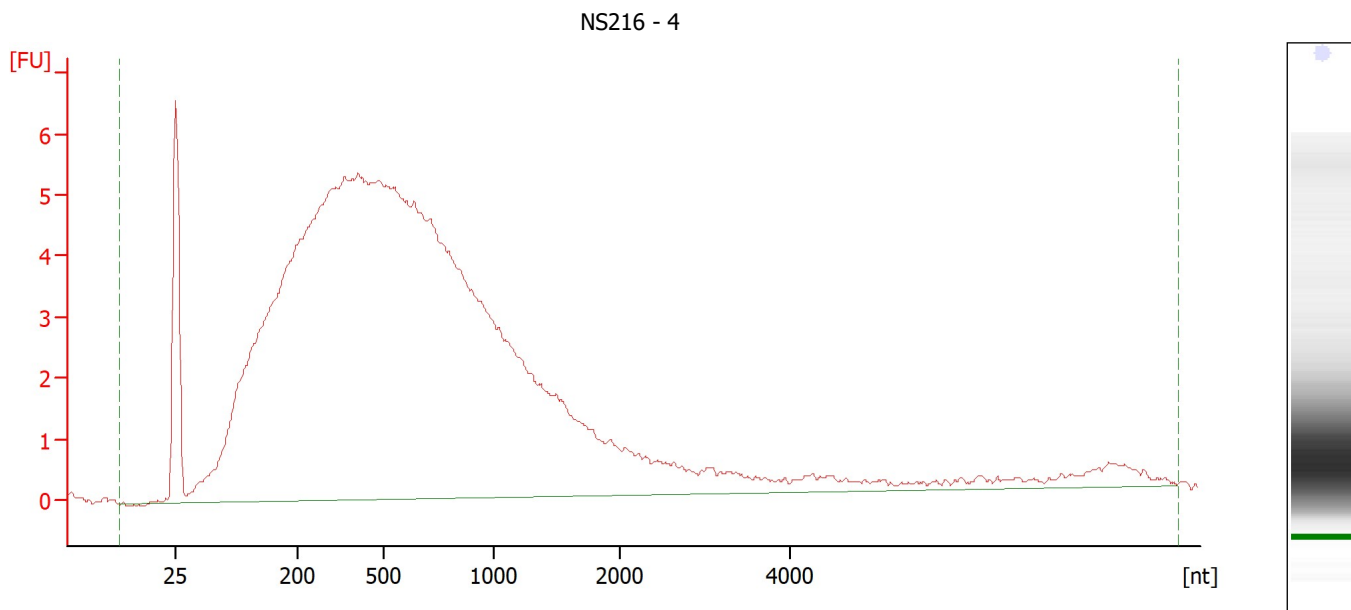

**Overall Results for sample 4 : NS216 - 4**


RNA Area:	206.8	RNA Integrity Number (RIN):	2 (B.02.10)
RNA Concentration:	1,194 pg/μl	Result Flagging Color:	<span style="background-color: #ccccff; border: 1px solid black; display: inline-block; width: 20px; height: 10px;"></span>
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN:2



Assay Class: Eukaryote Total RNA Pico  
 Data Path: Z:\...28\Bioanalyzer1\_Eukaryote Total RNA Pico\_2020-09-28\_001.xad

Created: 9/28/2020 1:09:50 PM  
 Modified: 9/28/2020 1:32:46 PM

**Electropherogram Summary Continued ...**

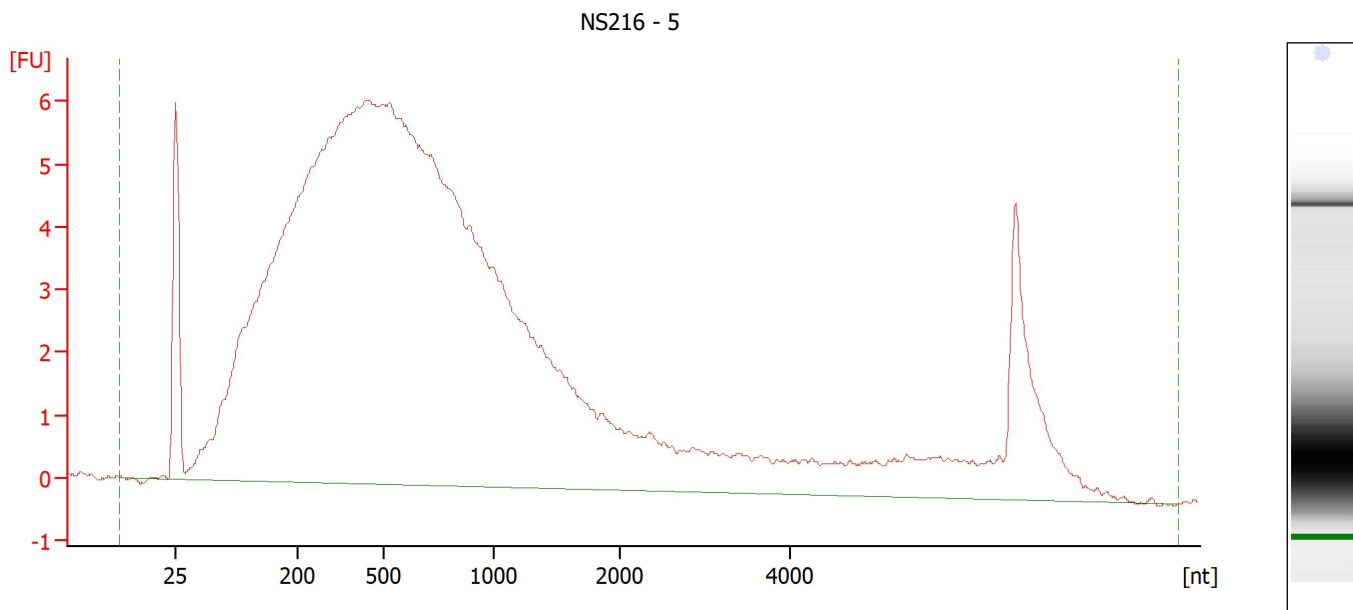


**Overall Results for sample 5 : NS216 - 5**

RNA Area:	254.0	RNA Integrity Number (RIN):	2 (B.02.10)
RNA Concentration:	1,466 pg/μl	Result Flagging Color:	<span style="background-color: #ccccff; border: 1px solid black; display: inline-block; width: 20px; height: 10px;"></span>
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN:2

Assay Class: Eukaryote Total RNA Pico  
Data Path: Z:\...28\Bioanalyzer1\_Eukaryote Total RNA Pico\_2020-09-28\_001.xad

Created: 9/28/2020 1:09:50 PM  
Modified: 9/28/2020 1:32:46 PM

**Electropherogram Summary Continued ...**

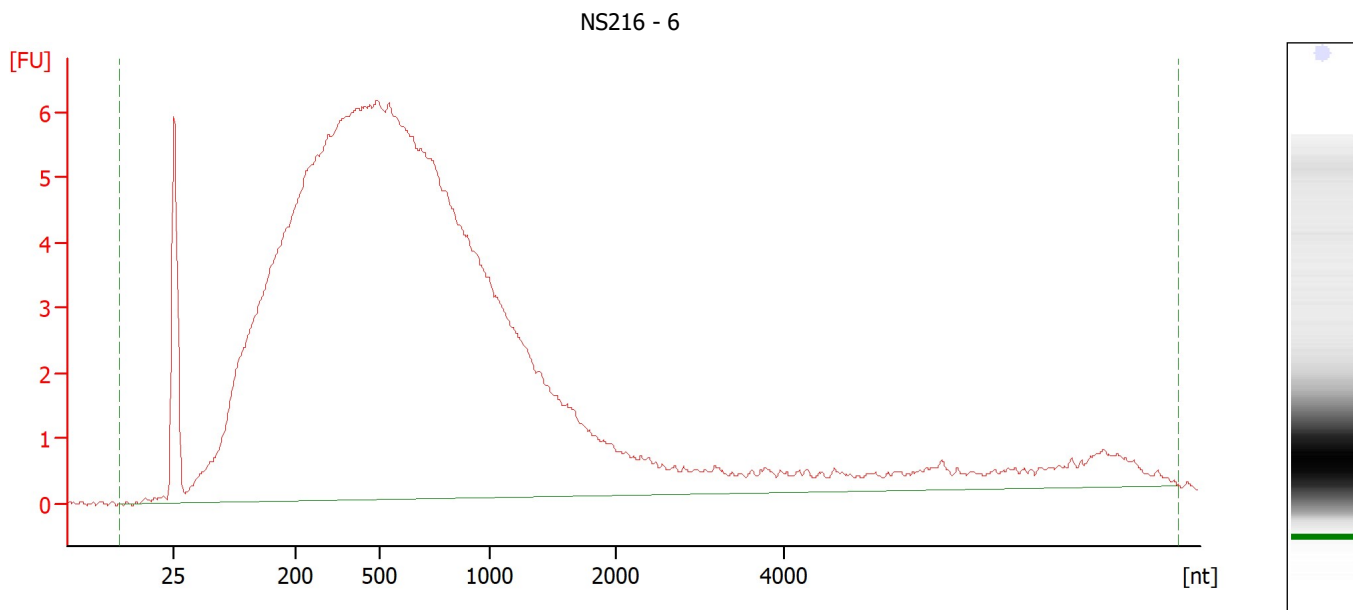


**Overall Results for sample 6 : NS216 - 6**

RNA Area:	233.1	RNA Integrity Number (RIN):	1.9 (B.02.10)
RNA Concentration:	1,346 pg/μl	Result Flagging Color:	<span style="background-color: #ccccff; border: 1px solid black; display: inline-block; width: 20px; height: 10px;"></span>
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN: 1.90

Assay Class: Eukaryote Total RNA Pico  
Data Path: Z:\...28\Bioanalyzer1\_Eukaryote Total RNA Pico\_2020-09-28\_001.xad

Created: 9/28/2020 1:09:50 PM  
Modified: 9/28/2020 1:32:46 PM

**Electropherogram Summary Continued ...**

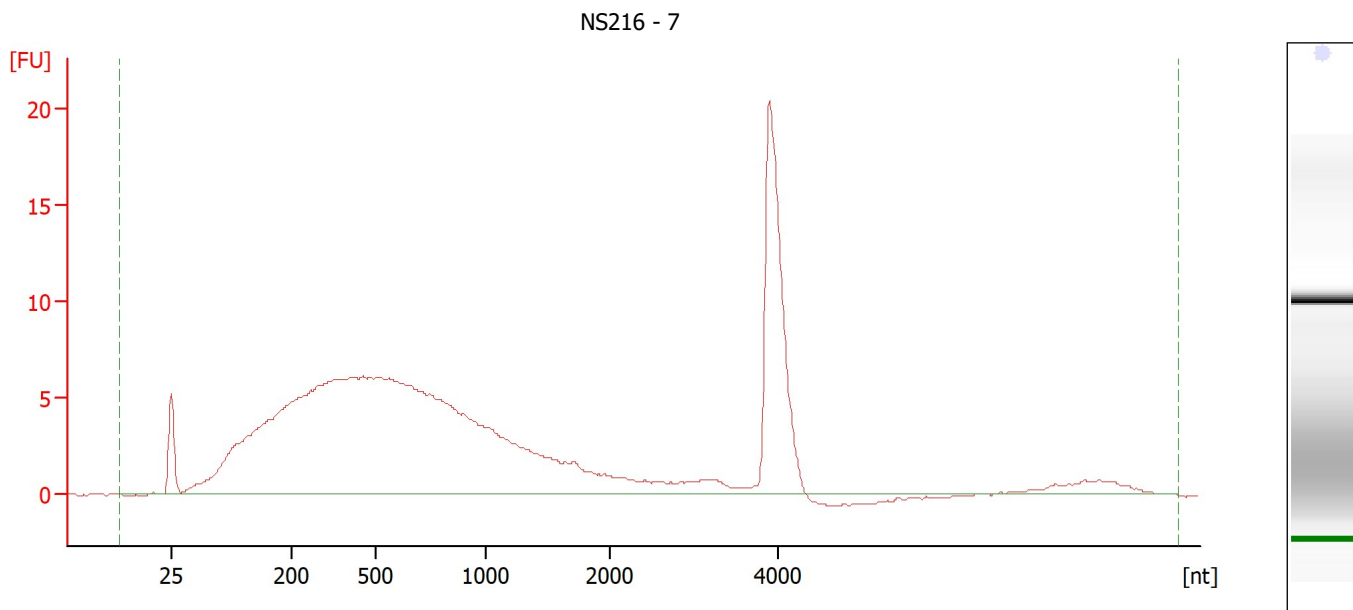


**Overall Results for sample 7 : NS216 - 7**

RNA Area:	281.2	RNA Integrity Number (RIN):	2 (B.02.10)
RNA Concentration:	1,623 pg/μl	Result Flagging Color:	<span style="background-color: #ccccff; border: 1px solid black; display: inline-block; width: 20px; height: 10px;"></span>
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN:2

Assay Class: Eukaryote Total RNA Pico  
 Data Path: Z:\...28\Bioanalyzer1\_Eukaryote Total RNA Pico\_2020-09-28\_001.xad

Created: 9/28/2020 1:09:50 PM  
 Modified: 9/28/2020 1:32:46 PM

**Electropherogram Summary Continued ...**

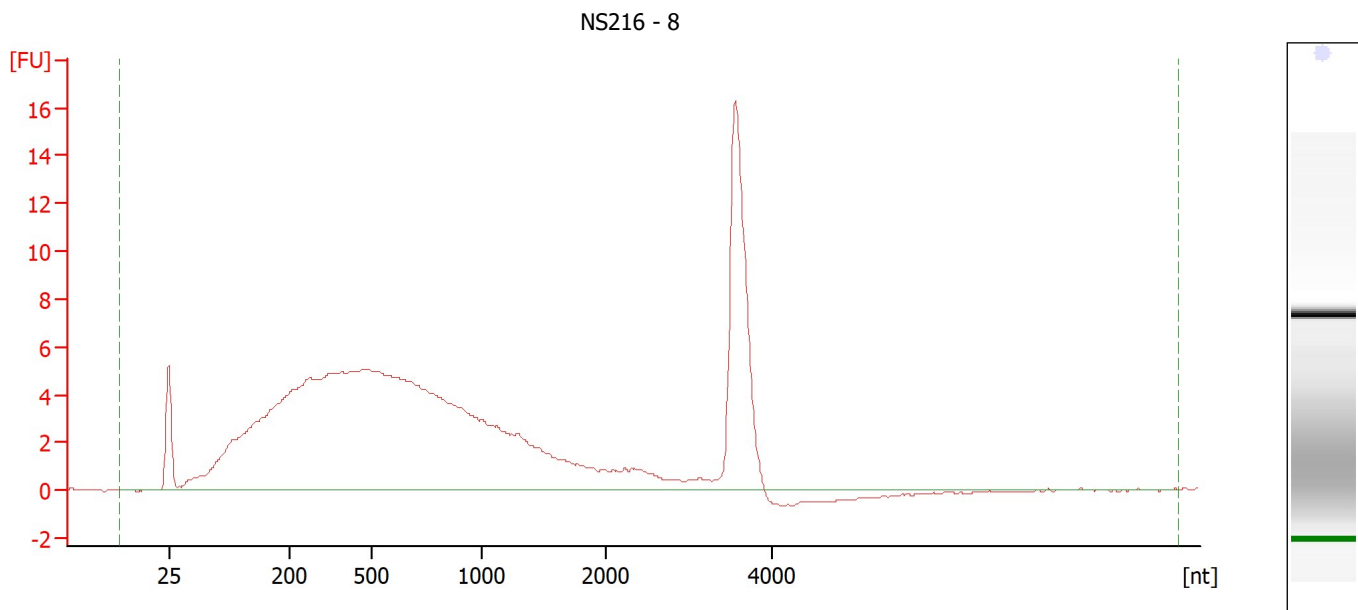


**Overall Results for sample 8 : NS216 - 8**

RNA Area:	225.2	RNA Integrity Number (RIN):	2.1 (B.02.10)
RNA Concentration:	1,300 pg/μl	Result Flagging Color:	<span style="background-color: #ccccff; border: 1px solid black; display: inline-block; width: 20px; height: 10px;"></span>
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN: 2.10

Assay Class: Eukaryote Total RNA Pico  
Data Path: Z:\...28\Bioanalyzer1\_Eukaryote Total RNA Pico\_2020-09-28\_001.xad

Created: 9/28/2020 1:09:50 PM  
Modified: 9/28/2020 1:32:46 PM

**Electropherogram Summary Continued ...**

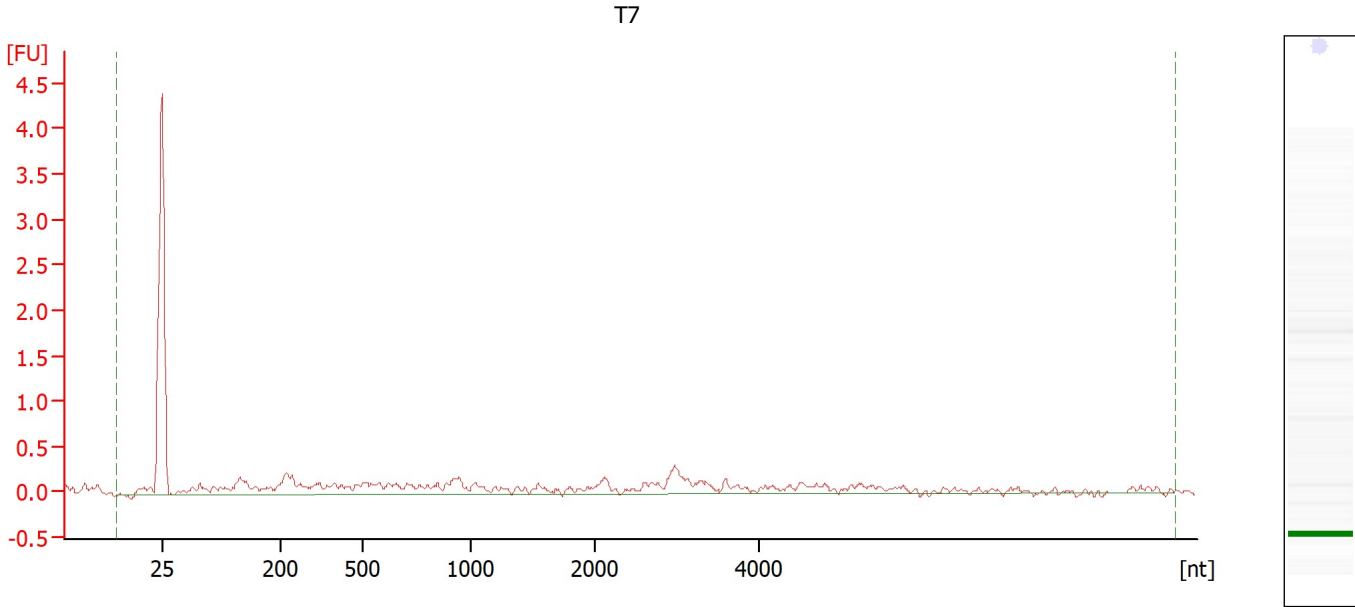


**Overall Results for sample 9 : T7**

RNA Area:	8.7	RNA Integrity Number (RIN):	1 (B.02.10)
RNA Concentration:	50 pg/μl	Result Flagging Color:	<span style="background-color: #ccccff; border: 1px solid black; display: inline-block; width: 20px; height: 10px;"></span>
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN:1

Assay Class: Eukaryote Total RNA Pico  
Data Path: Z:\...28\Bioanalyzer1\_Eukaryote Total RNA Pico\_2020-09-28\_001.xad

Created: 9/28/2020 1:09:50 PM  
Modified: 9/28/2020 1:32:46 PM

**Electropherogram Summary Continued ...**

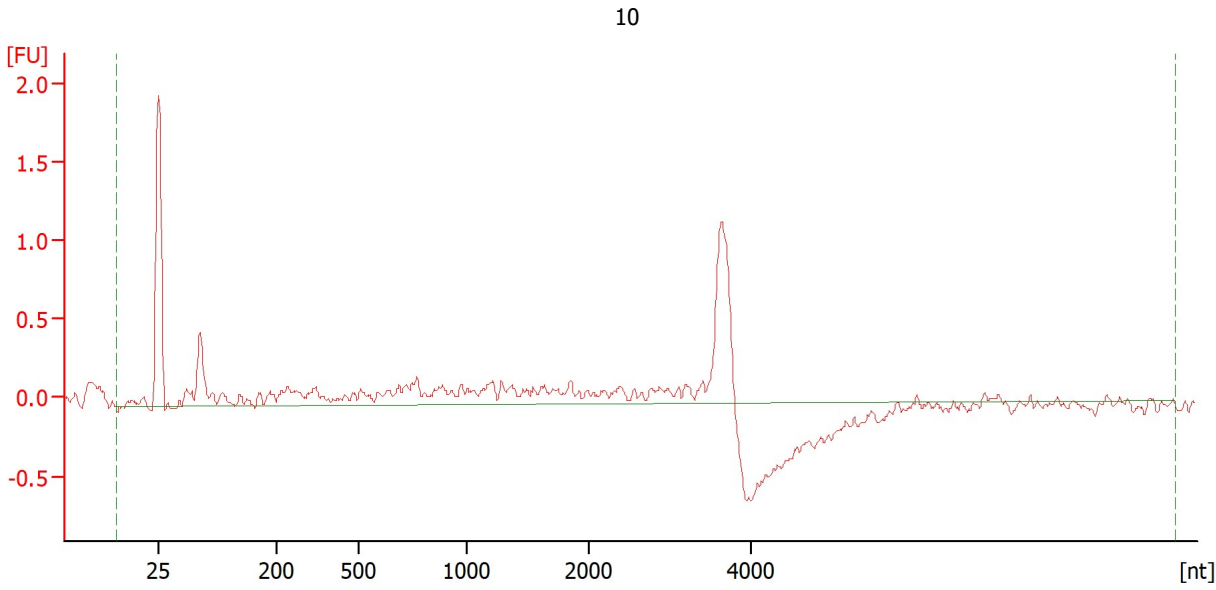


**Overall Results for sample 10 : 10**

RNA Area:	7.7	RNA Integrity Number (RIN):	N/A (B.02.10)
RNA Concentration:	44 pg/μl	Result Flagging Color:	<span style="background-color: #cccccc; border: 1px solid black; display: inline-block; width: 20px; height: 10px;"></span>
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN N/A

Assay Class: Eukaryote Total RNA Pico  
 Data Path: Z:\...28\Bioanalyzer1\_Eukaryote Total RNA Pico\_2020-09-28\_001.xad

Created: 9/28/2020 1:09:50 PM  
 Modified: 9/28/2020 1:32:46 PM

**Electropherogram Summary Continued ...**

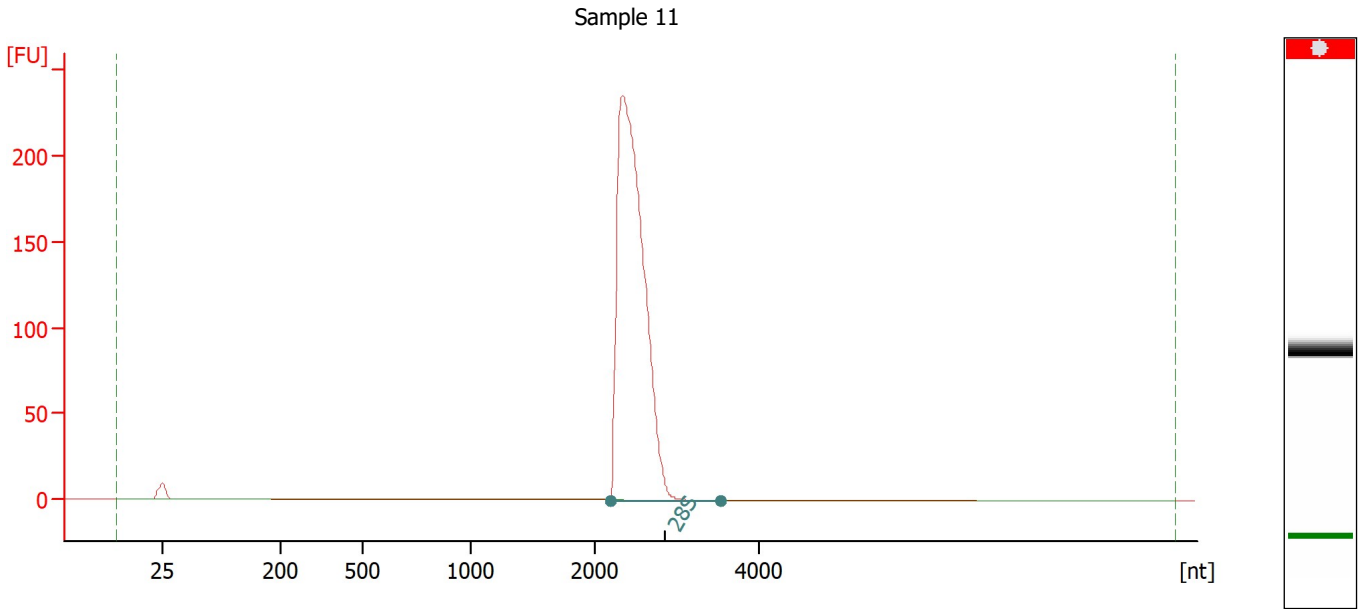

**Overall Results for sample 11 : Sample 11**

RNA Area:	789.8	RNA Integrity Number (RIN):	N/A (B.02.10)
RNA Concentration:	4,560 pg/μl	Result Flagging Color:	<span style="background-color: #cccccc; border: 1px solid black; display: inline-block; width: 20px; height: 10px;"></span>
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN N/A

**Fragment table for sample 11 : Sample 11**

Name	Start Size [nt]	End Size [nt]	Area	% of total Area
28S	2,192	3,543	780.0	98.8

---

Assay Class: Eukaryote Total RNA Pico  
Data Path: Z:\...28\Bioanalyzer1\_Eukaryote Total RNA Pico\_2020-09-28\_001.xad

Created: 9/28/2020 1:09:50 PM  
Modified: 9/28/2020 1:32:46 PM

**Gel Image**



Assay Class: Eukaryote Total RNA Pico Created: 9/28/2020 1:09:50 PM  
 Data Path: Z:\...28\Bioanalyzer1\_Eukaryote Total RNA Pico\_2020-09-28\_001.xad Modified: 9/28/2020 1:32:46 PM

**Run Logbook**

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 12)		Instrument	Run		9/28/2020 1:32:45 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Run started on port 1 (File: Z:\XADs\2020-09-28\Bioanalyze r1_Eukaryote Total RNA Pico_2020-09-28_001.xad)		Instrument	Run		9/28/2020 1:09:56 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Product Number : G2938C		Instrument	Run		9/28/2020 1:09:56 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Name :		Instrument	Run		9/28/2020 1:09:56 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Vendor : Agilent Technologies		Instrument	Run		9/28/2020 1:09:56 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Serial# : DE34903152		Instrument	Run		9/28/2020 1:09:56 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Firmware : C.01.069		Instrument	Run		9/28/2020 1:09:56 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Cartridge : Electrode		Instrument	Run		9/28/2020 1:09:56 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB