


Assay Class: Eukaryote Total RNA Pico
Data Path: C:\...\2100 bioanalyzer\2100 expert\data\2025-08-15\QC2262-12.xad

Created: 8/15/2025 1:32:51 PM
Modified: 8/15/2025 3:07:52 PM

Electrophoresis File Run Summary

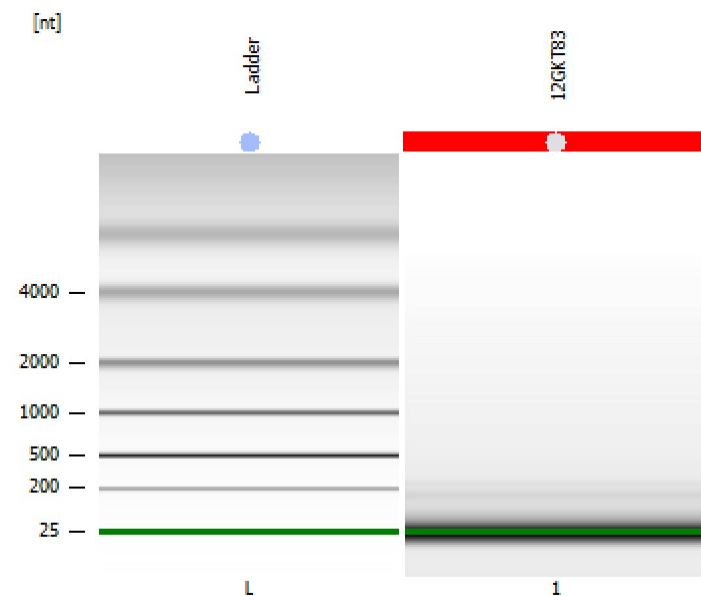

Instrument Information:


Instrument Name: DE34903152 Firmware: C.01.069
Serial#: DE34903152 Type: G2938C

Assay Information:

Assay Origin Path: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\assays\RNA\Eukaryote Total RNA Pico Series II.xsy
Assay Class: Eukaryote Total RNA Pico
Version: 2.6
Assay Comments: Total RNA Analysis pg sensitivity (Eukaryote)
© Copyright 2003 - 2009 Agilent Technologies, Inc.

Chip Information:

Chip Lot #:
Reagent Kit Lot #:
Chip Comments:

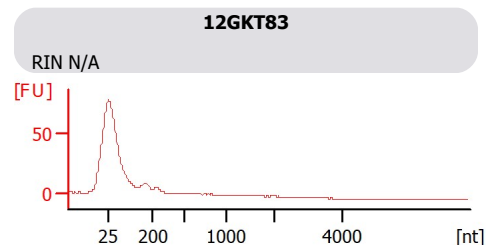

Assay Class: Eukaryote Total RNA Pico
Data Path: C:\...\2100 bioanalyzer\2100 expert\data\2025-08-15\QC2262-12.xad

Created: 8/15/2025 1:32:51 PM
Modified: 8/15/2025 3:07:52 PM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Status	Result Label	Result Color
12GKT83		✓	RIN N/A	
Ladder		✓	All Other Samples	

Chip Lot #**Reagent Kit Lot #****Chip Comments :**

Assay Class: Eukaryote Total RNA Pico
Data Path: C:\...\2100 bioanalyzer\2100 expert\data\2025-08-15\QC2262-12.xad

Created: 8/15/2025 1:32:51 PM
Modified: 8/15/2025 3:07:52 PM

Electrophoresis Assay Details

General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12

Minimum Visible Range [s] : 17

Maximum Visible Range [s] : 70

Start Analysis Time Range [s] : 18

End Analysis Time Range [s] : 69

Ladder Concentration [pg/μl] : 1000

Lower Marker Concentration [pg/μl] : 0

Upper Marker Concentration [pg/μl] : 0

Used Lower Marker for Quantitation

Standard Curve Fit is Logarithmic

Show Data Aligned to Lower Marker

Integrator Settings

Integration Start Time [s] : 18

Integration End Time [s] : 69

Slope Threshold : 0.6

Height Threshold [FU] : 0.5

Area Threshold : 0.2

Width Threshold [s] : 0.3

Baseline Plateau [s] : 6

Filter Settings

Filter Width [s] : 0.5

Polynomial Order : 4


Ladder

Ladder Peak	Size
1	25
2	200
3	500
4	1000
5	2000
6	4000

Assay Class: Eukaryote Total RNA Pico
Data Path: C:\...\2100 bioanalyzer\2100 expert\data\2025-08-15\QC2262-12.xad

Created: 8/15/2025 1:32:51 PM
Modified: 8/15/2025 3:07:52 PM

Electropherogram Summary

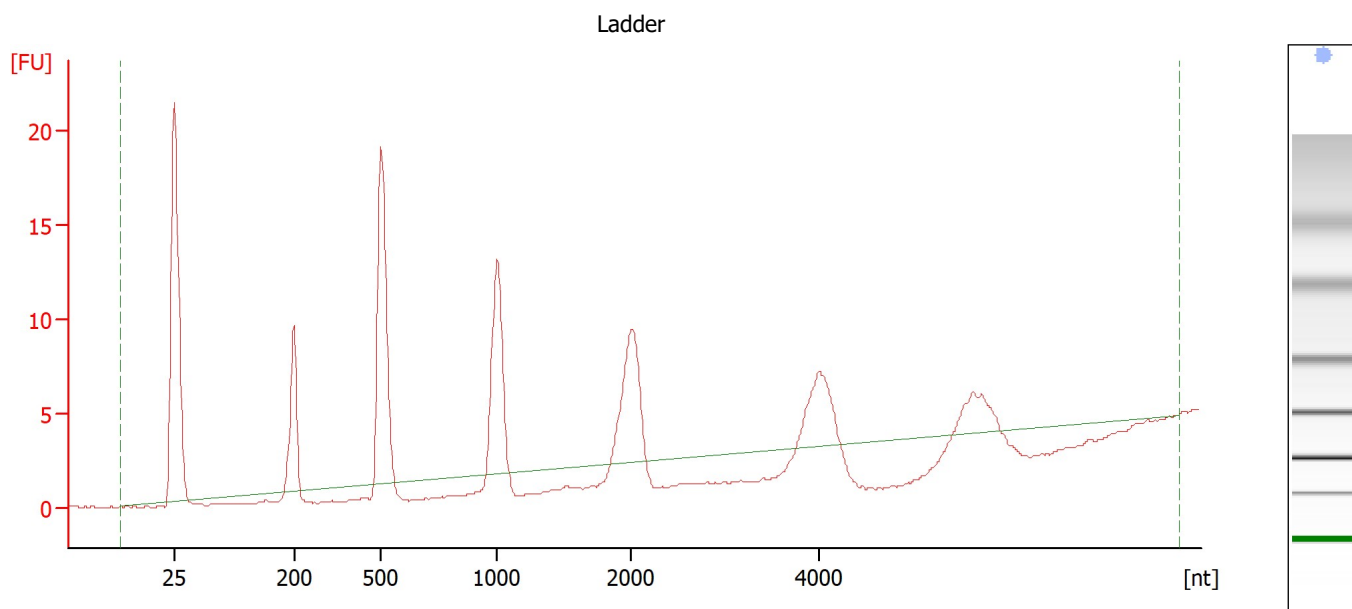

Overall Results for Ladder

RNA Area: 82.5

Result Flagging Color:




RNA Concentration: 1,000 pg/μl

Result Flagging Label:

All Other Samples

Assay Class: Eukaryote Total RNA Pico
Data Path: C:\...\2100 bioanalyzer\2100 expert\data\2025-08-15\QC2262-12.xad


Created: 8/15/2025 1:32:51 PM
Modified: 8/15/2025 3:07:52 PM

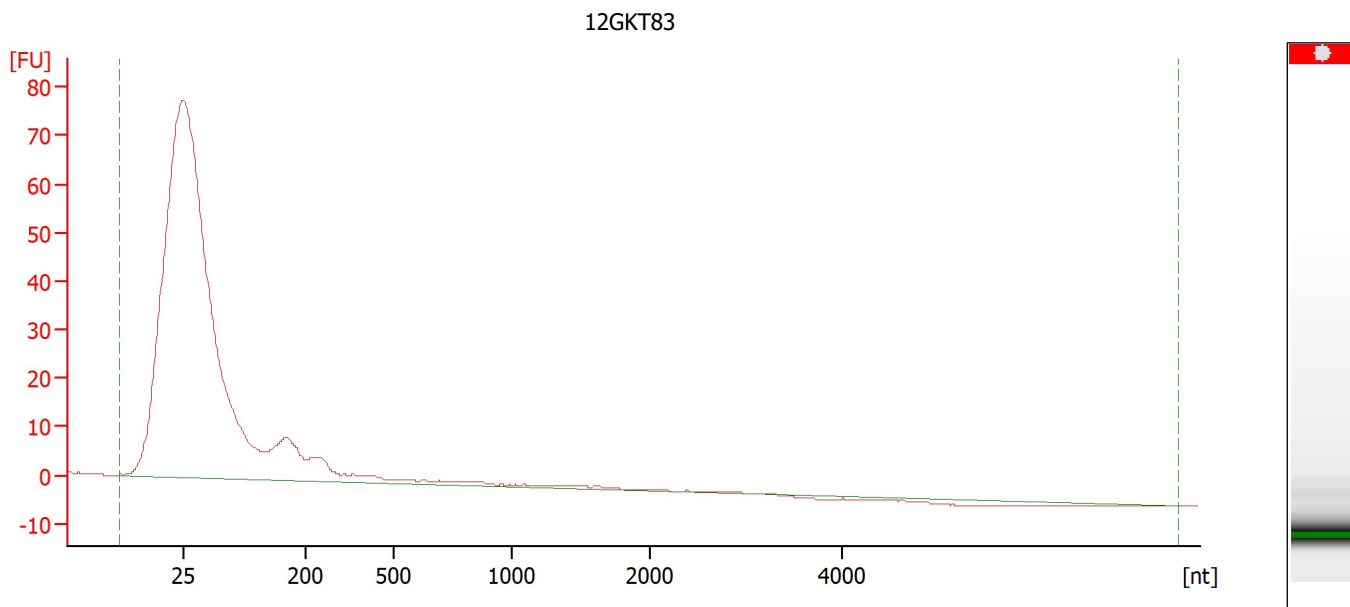Electropherogram Summary Continued ...**Overall Results for sample 1 : 12GKT83**

RNA Area:	93.4	RNA Integrity Number (RIN):	N/A (B.02.10)
RNA Concentration:	1,132 pg/μl	Result Flagging Color:	
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN N/A

Assay Class: Eukaryote Total RNA Pico
Data Path: C:\...\2100 bioanalyzer\2100 expert\data\2025-08-15\QC2262-12.xad

Created: 8/15/2025 1:32:51 PM
Modified: 8/15/2025 3:07:52 PM

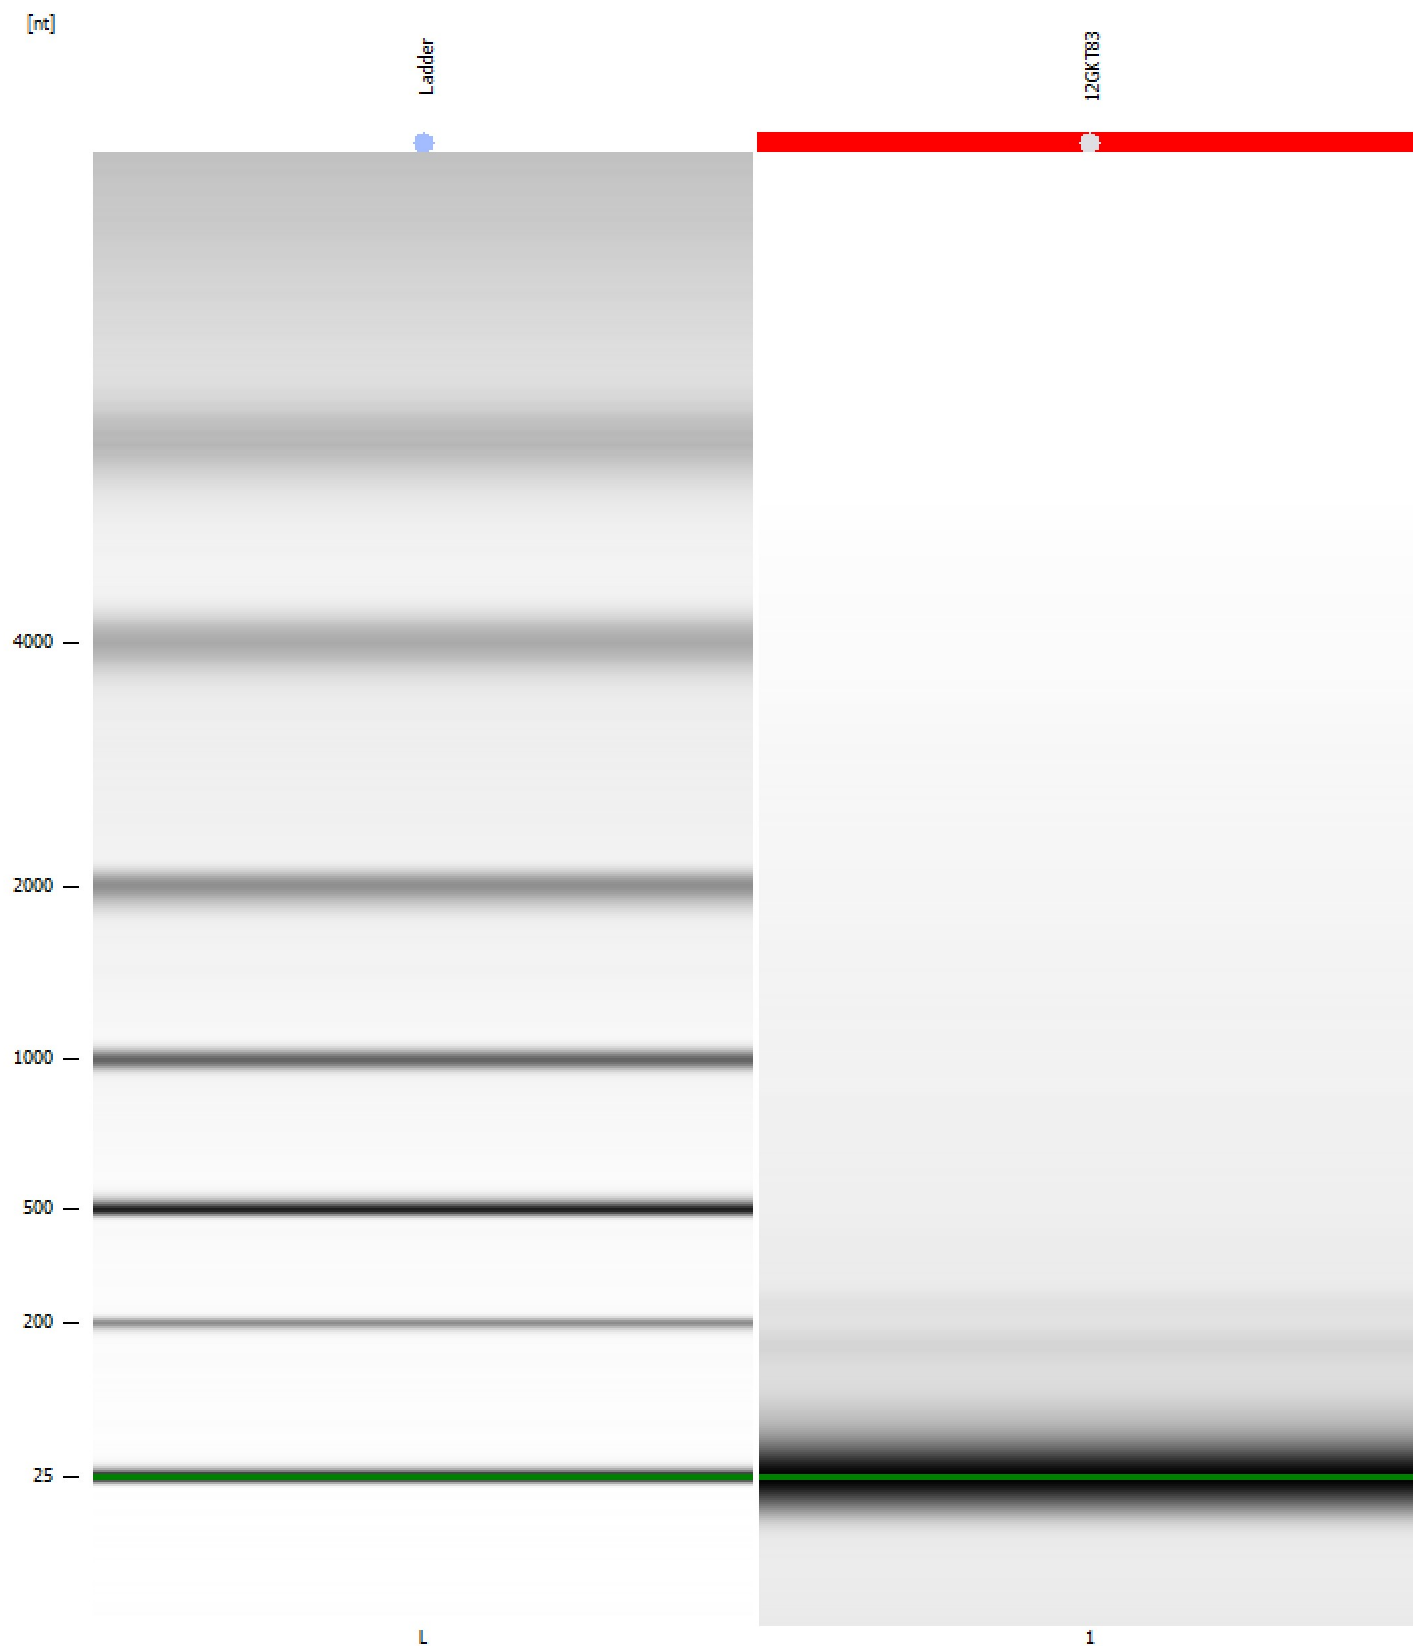Gel Image

Assay Class: Eukaryote Total RNA Pico
 Data Path: C:\...\2100 bioanalyzer\2100 expert\data\2025-08-15\QC2262-12.xad

Created: 8/15/2025 1:32:51 PM
 Modified: 8/15/2025 3:07:52 PM

Run Logbook

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 12)		Instrument	Run		8/15/2025 1:54:54 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Run started on port 1 (File: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\data\2025-08-15\Bioanalyzer1_Eukaryote Total RNA Pico_DE34903152_2025-08-15_002.xad)		Instrument	Run		8/15/2025 1:32:57 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Product Number : G2938C		Instrument	Run		8/15/2025 1:32:57 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Name :		Instrument	Run		8/15/2025 1:32:57 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Vendor : Agilent Technologies		Instrument	Run		8/15/2025 1:32:57 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Serial# : DE34903152		Instrument	Run		8/15/2025 1:32:57 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Firmware : C.01.069		Instrument	Run		8/15/2025 1:32:57 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Cartridge : Electrode		Instrument	Run		8/15/2025 1:32:57 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB