

Assay Class: Eukaryote Total RNA Nano
Data Path: C:\...analyzer\2100 expert\data\2025-12-15\QC2381_RNA_Nano_QC.xad

Created: 12/15/2025 3:30:33 PM
Modified: 12/15/2025 4:06:11 PM

Electrophoresis File Run Summary

Instrument Information:



Instrument Name: DE34903152 Firmware: C.01.069
Serial#: DE34903152 Type: G2938C

Assay Information:

Assay Origin Path: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\assays\RNA\Eukaryote Total RNA Nano Series II.xsy
Assay Class: Eukaryote Total RNA Nano
Version: 2.6
Assay Comments: Total RNA Analysis ng sensitivity (Eukaryote)
© Copyright 2003 - 2009 Agilent Technologies, Inc.

Chip Information:

Chip Lot #:
Reagent Kit Lot #:
Chip Comments:

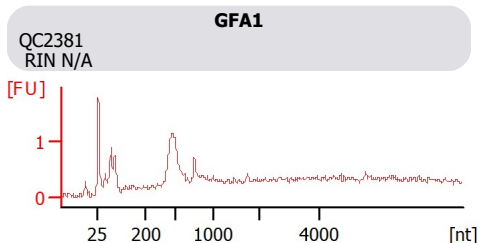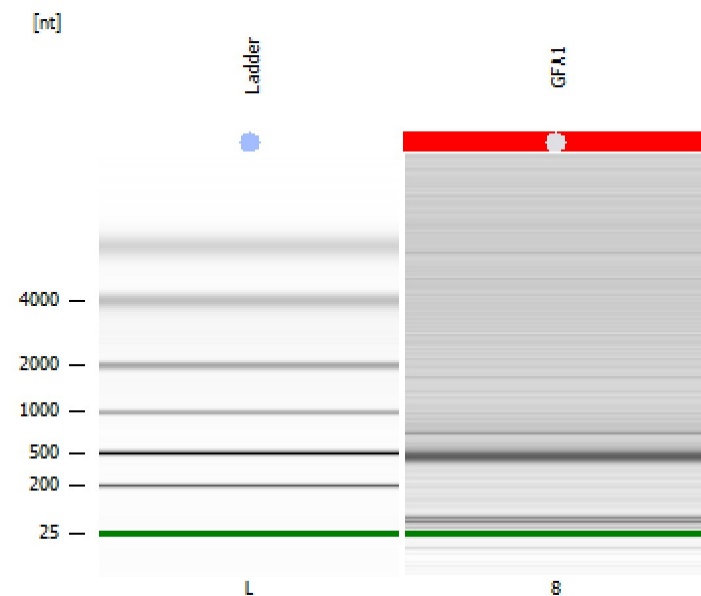

Assay Class: Eukaryote Total RNA Nano
Data Path: C:\...analyzer\2100 expert\data\2025-12-15\QC2381_RNA_Nano_QC.xad

Created: 12/15/2025 3:30:33 PM
Modified: 12/15/2025 4:06:11 PM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Status	Result Label	Result Color
GFA1	QC2381	✓	RIN N/A	
Ladder		✓	All Other Samples	

Chip Lot #**Reagent Kit Lot #****Chip Comments :**

Assay Class: Eukaryote Total RNA Nano
Data Path: C:\...analyzer\2100 expert\data\2025-12-15\QC2381_RNA_Nano_QC.xad

Created: 12/15/2025 3:30:33 PM
Modified: 12/15/2025 4:06:11 PM

Electrophoresis Assay Details

General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 13

Minimum Visible Range [s] : 17

Maximum Visible Range [s] : 70

Start Analysis Time Range [s] : 19

End Analysis Time Range [s] : 69

Ladder Concentration [ng/μl] : 150

Lower Marker Concentration [ng/μl] : 0

Upper Marker Concentration [ng/μl] : 0

Used Lower Marker for Quantitation

Standard Curve Fit is Logarithmic

Show Data Aligned to Lower Marker

Integrator Settings

Integration Start Time [s] : 19

Integration End Time [s] : 69

Slope Threshold : 0.6

Height Threshold [FU] : 0.5

Area Threshold : 0.2

Width Threshold [s] : 0.5

Baseline Plateau [s] : 6

Filter Settings

Filter Width [s] : 0.5

Polynomial Order : 4


Ladder

Ladder Peak	Size
1	25
2	200
3	500
4	1000
5	2000
6	4000

Assay Class: Eukaryote Total RNA Nano
Data Path: C:\...analyzer\2100 expert\data\2025-12-15\QC2381_RNA_Nano_QC.xad

Created: 12/15/2025 3:30:33 PM
Modified: 12/15/2025 4:06:11 PM

Electropherogram Summary

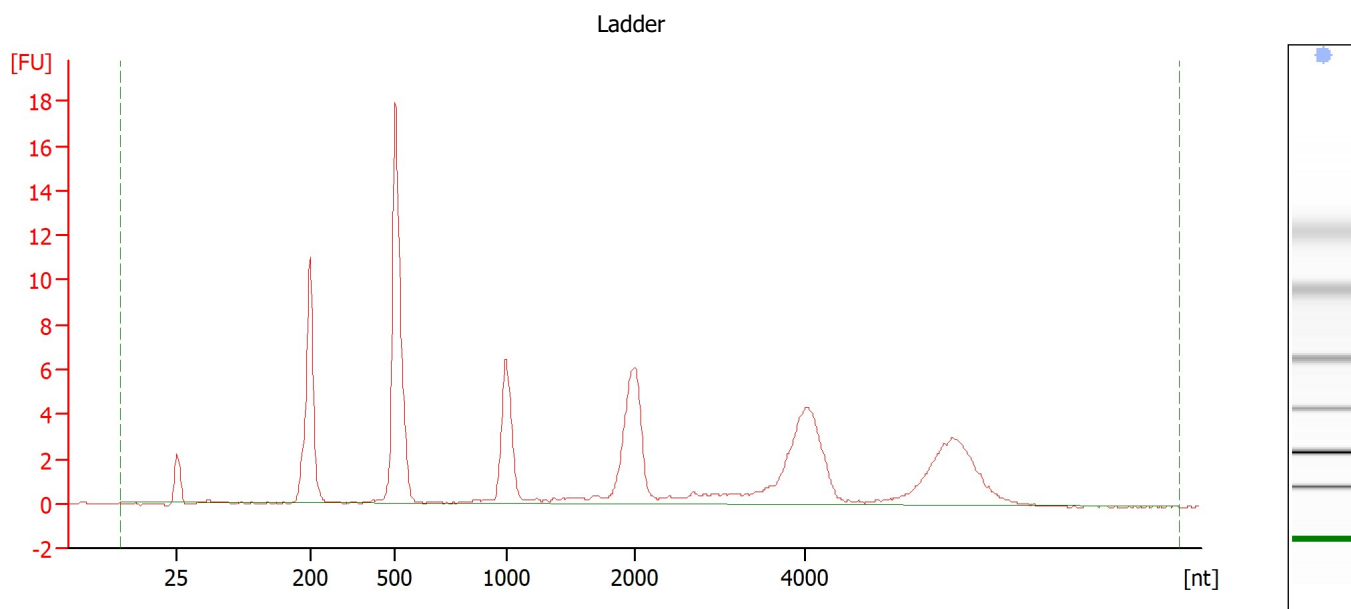

Overall Results for Ladder

RNA Area: 102.7

Result Flagging Color:




RNA Concentration: 150 ng/μl

Result Flagging Label:

All Other Samples

Assay Class: Eukaryote Total RNA Nano
Data Path: C:\...analyzer\2100 expert\data\2025-12-15\QC2381_RNA_Nano_QC.xad


Created: 12/15/2025 3:30:33 PM
Modified: 12/15/2025 4:06:11 PM

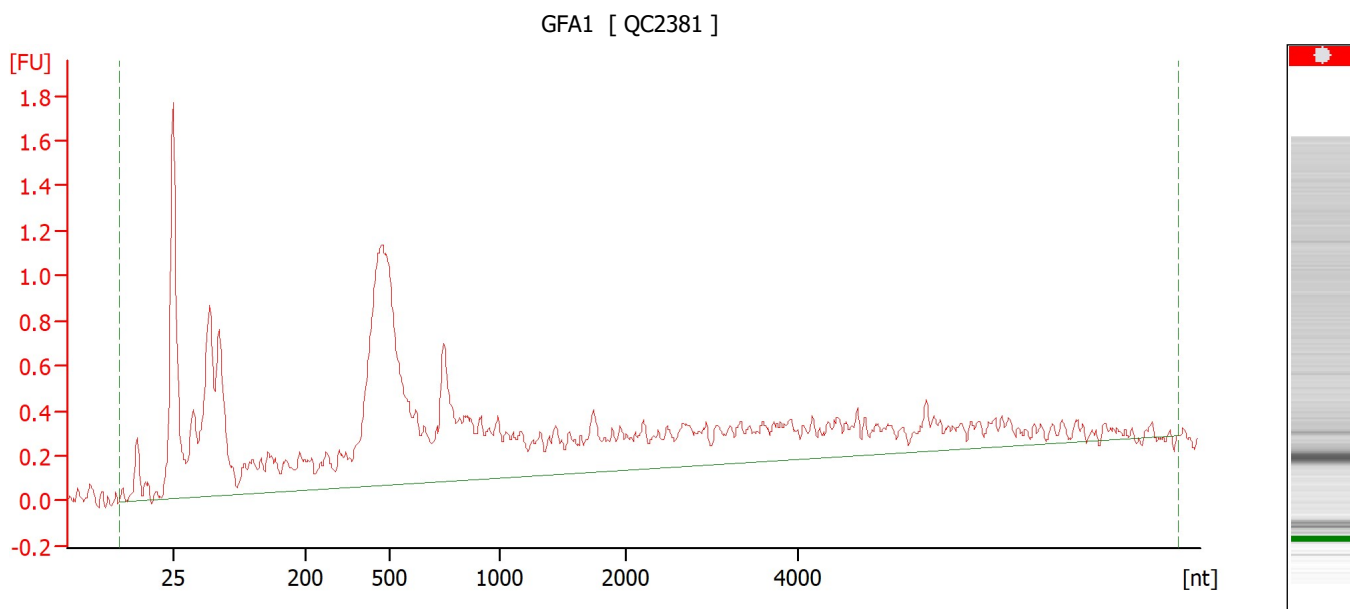Electropherogram Summary Continued ...**Overall Results for sample 8 : GFA1**

RNA Area:	23.6	RNA Integrity Number (RIN):	N/A (B.02.10)
RNA Concentration:	34 ng/μl	Result Flagging Color:	
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN N/A

Assay Class: Eukaryote Total RNA Nano
Data Path: C:\...analyzer\2100 expert\data\2025-12-15\QC2381_RNA_Nano_QC.xad

Created: 12/15/2025 3:30:33 PM
Modified: 12/15/2025 4:06:11 PM

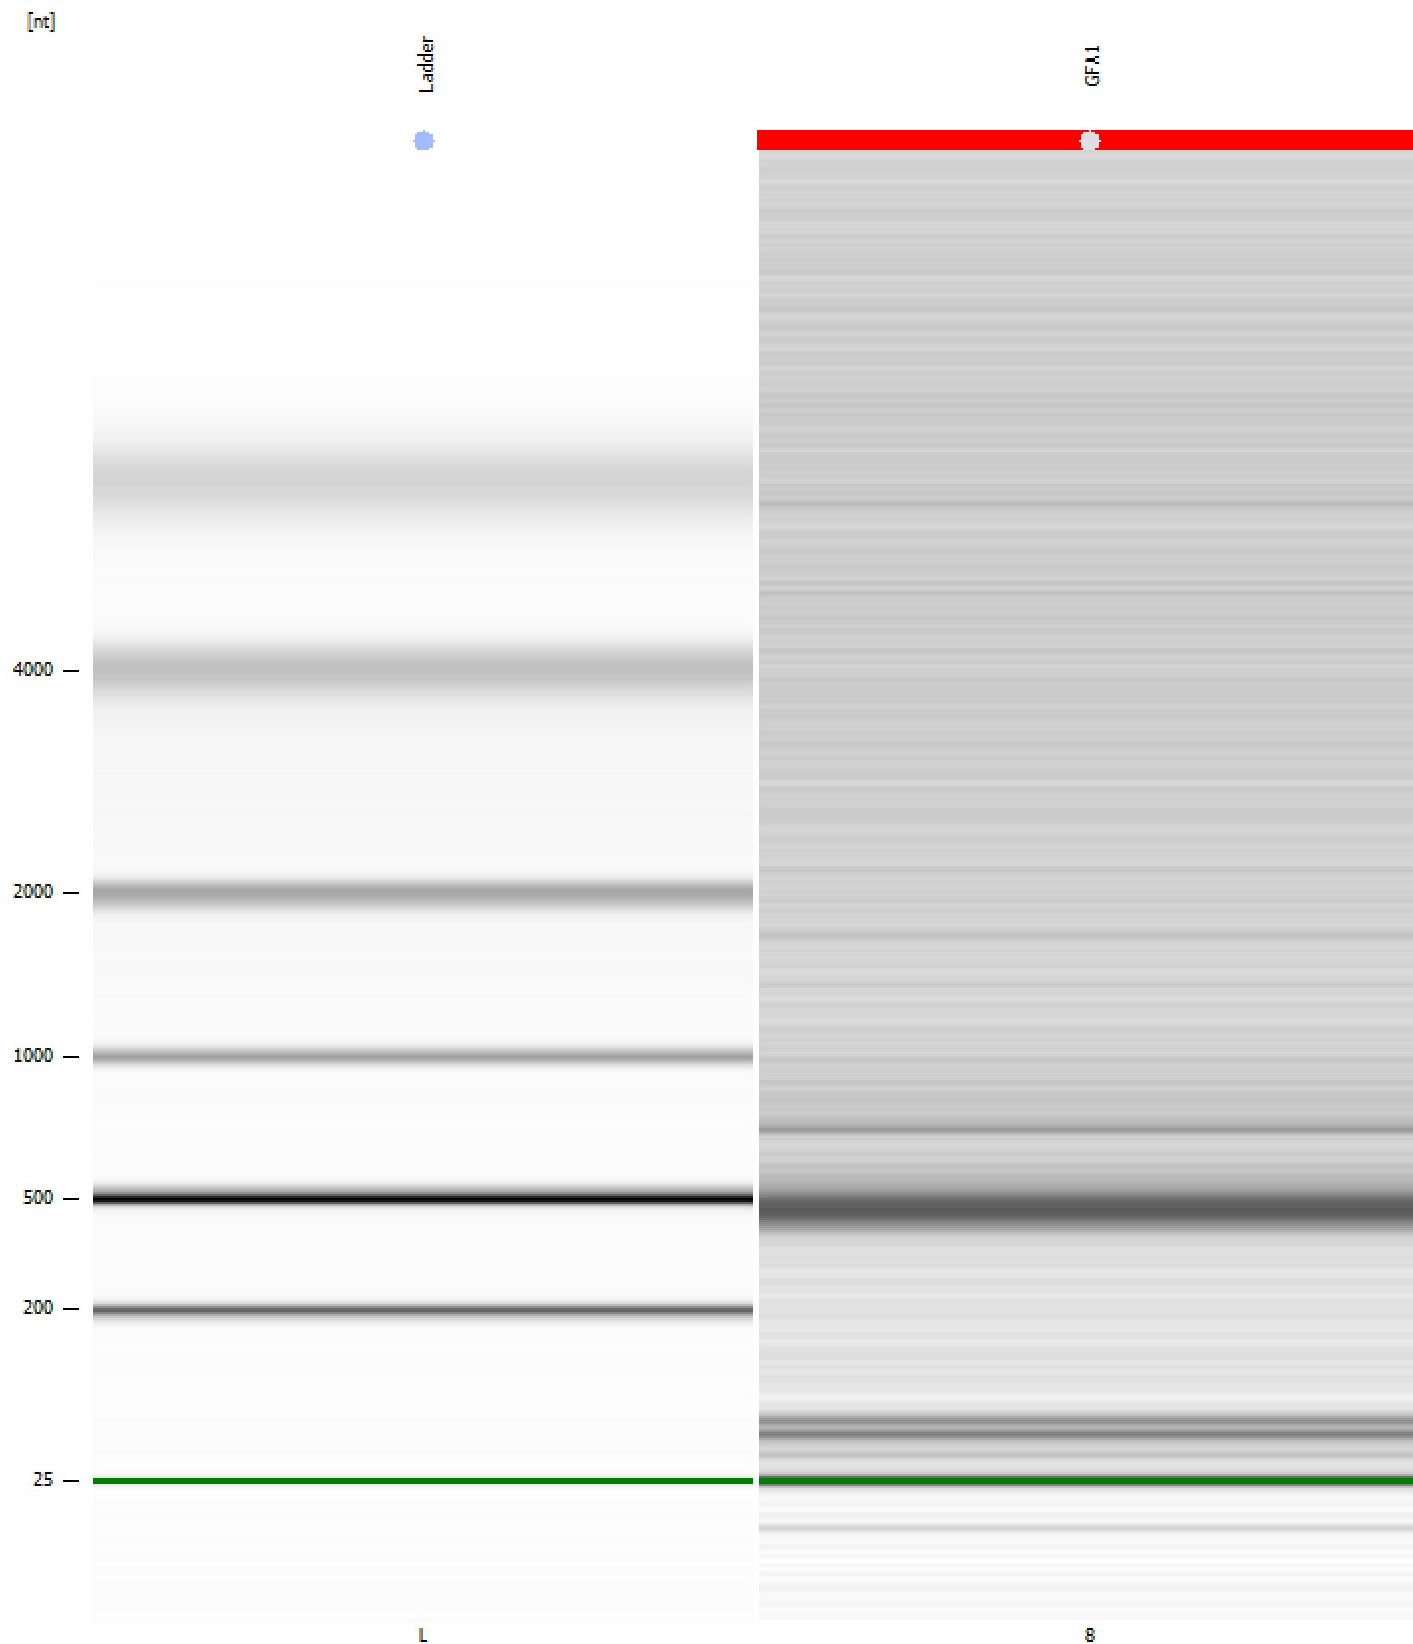Gel Image

Assay Class: Eukaryote Total RNA Nano
 Data Path: C:\...analyzer\2100 expert\data\2025-12-15\QC2381_RNA_Nano_QC.xad

Created: 12/15/2025 3:30:33 PM
 Modified: 12/15/2025 4:06:11 PM

Run Logbook

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 13)		Instrument	Run		12/15/2025 3:54:23 PM	(GMT --08:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Run started on port 1 (File: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\data\2025-12-15\Bioanalyzer1_Eukaryote Total RNA Nano_DE34903152_2025-12-15_001.xad)		Instrument	Run		12/15/2025 3:30:40 PM	(GMT --08:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Product Number : G2938C		Instrument	Run		12/15/2025 3:30:40 PM	(GMT --08:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Name :		Instrument	Run		12/15/2025 3:30:40 PM	(GMT --08:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Vendor : Agilent Technologies		Instrument	Run		12/15/2025 3:30:40 PM	(GMT --08:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Serial# : DE34903152		Instrument	Run		12/15/2025 3:30:40 PM	(GMT --08:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Firmware : C.01.069		Instrument	Run		12/15/2025 3:30:40 PM	(GMT --08:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Cartridge : Electrode		Instrument	Run		12/15/2025 3:30:40 PM	(GMT --08:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB