


Assay Class: Plant RNA Nano
Data Path: C:\...00 bioanalyzer\2100 expert\data\2025-09-24\SKA1_STITCH3.xad

Created: 9/24/2025 12:04:17 PM
Modified: 9/24/2025 12:43:31 PM

Electrophoresis File Run Summary

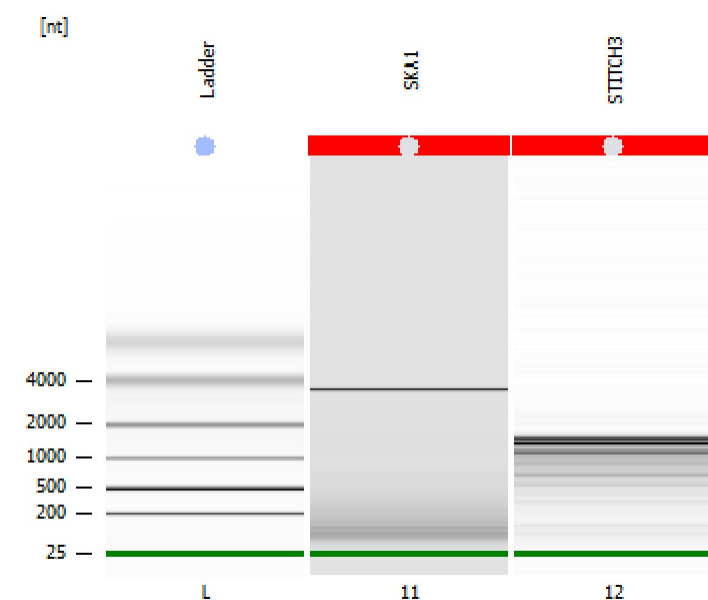

Instrument Information:

Instrument Name: DE34903152 Firmware: C.01.069
Serial#: DE34903152 Type: G2938C

Assay Information:

Assay Origin Path: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\assays\RNA\Plant RNA Nano.xsy

Assay Class: Plant RNA Nano

Version: 1.3

Assay Comments: Total RNA Analysis ng sensitivity (Plant)


© Copyright 2003 - 2009 Agilent Technologies, Inc.

Chip Information:

Chip Lot #:

Reagent Kit Lot #:

Chip Comments:

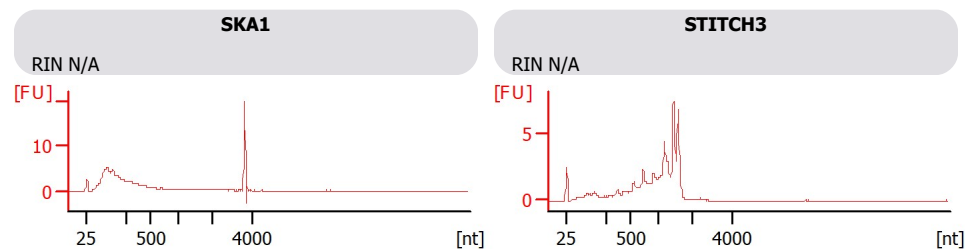

Assay Class: Plant RNA Nano
Data Path: C:\...00 bioanalyzer\2100 expert\data\2025-09-24\SKA1_STITCH3.xad

Created: 9/24/2025 12:04:17 PM
Modified: 9/24/2025 12:43:31 PM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Status	Result Label	Result Color
SKA1		✓	RIN N/A	
STITCH3		✓	RIN N/A	
Ladder		✓	All Other Samples	

Chip Lot #**Reagent Kit Lot #****Chip Comments :**

Assay Class: Plant RNA Nano
Data Path: C:\...00 bioanalyzer\2100 expert\data\2025-09-24\SKA1_STITCH3.xad

Created: 9/24/2025 12:04:17 PM
Modified: 9/24/2025 12:43:31 PM

Electrophoresis Assay Details

General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 13

Minimum Visible Range [s] : 17

Maximum Visible Range [s] : 70

Start Analysis Time Range [s] : 19

End Analysis Time Range [s] : 69

Ladder Concentration [ng/μl] : 150

Lower Marker Concentration [ng/μl] : 0

Upper Marker Concentration [ng/μl] : 0

Used Lower Marker for Quantitation

Standard Curve Fit is Logarithmic

Show Data Aligned to Lower Marker

Integrator Settings

Integration Start Time [s] : 19

Integration End Time [s] : 69

Slope Threshold : 0.6

Height Threshold [FU] : 0.2

Area Threshold : 0.1

Width Threshold [s] : 0.2

Baseline Plateau [s] : 6

Filter Settings

Filter Width [s] : 0.5

Polynomial Order : 4


Ladder

Ladder Peak	Size
1	25
2	200
3	500
4	1000
5	2000
6	4000

Assay Class: Plant RNA Nano
Data Path: C:\...00 bioanalyzer\2100 expert\data\2025-09-24\SKA1_STITCH3.xad

Created: 9/24/2025 12:04:17 PM
Modified: 9/24/2025 12:43:31 PM

Electropherogram Summary

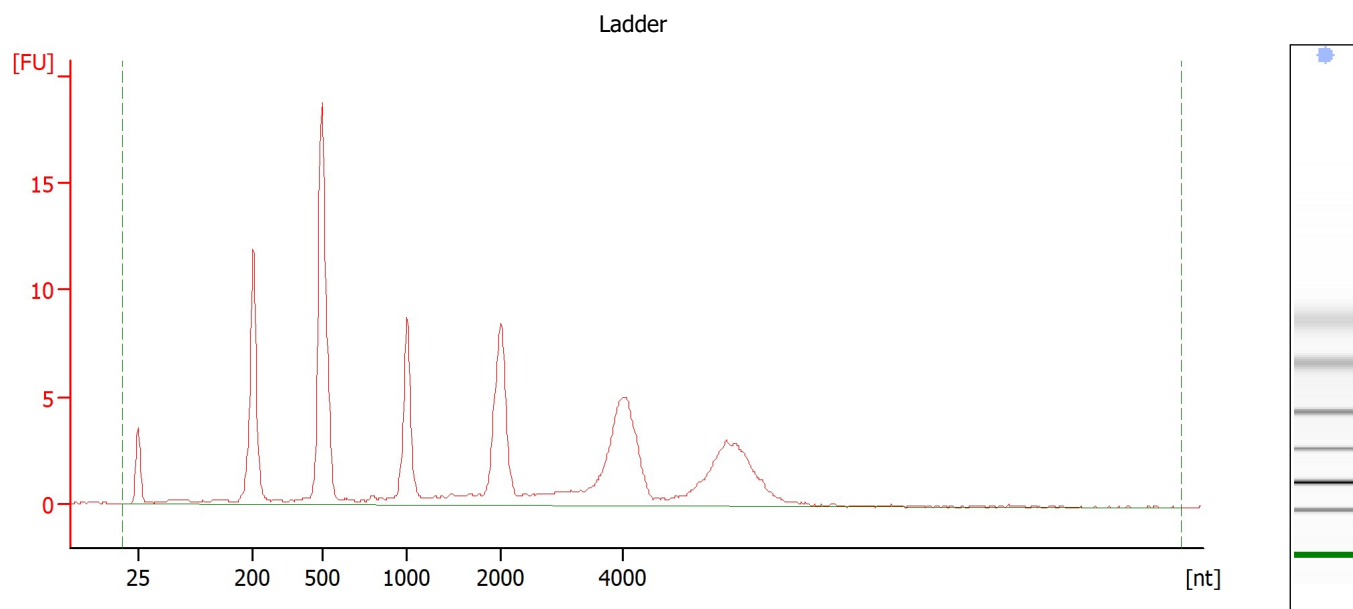

Overall Results for Ladder

RNA Area: 119.5

Result Flagging Color:




RNA Concentration: 150 ng/μl

Result Flagging Label:

All Other Samples

Assay Class: Plant RNA Nano
Data Path: C:\...00 bioanalyzer\2100 expert\data\2025-09-24\SKA1_STITCH3.xad

Created: 9/24/2025 12:04:17 PM
Modified: 9/24/2025 12:43:31 PM

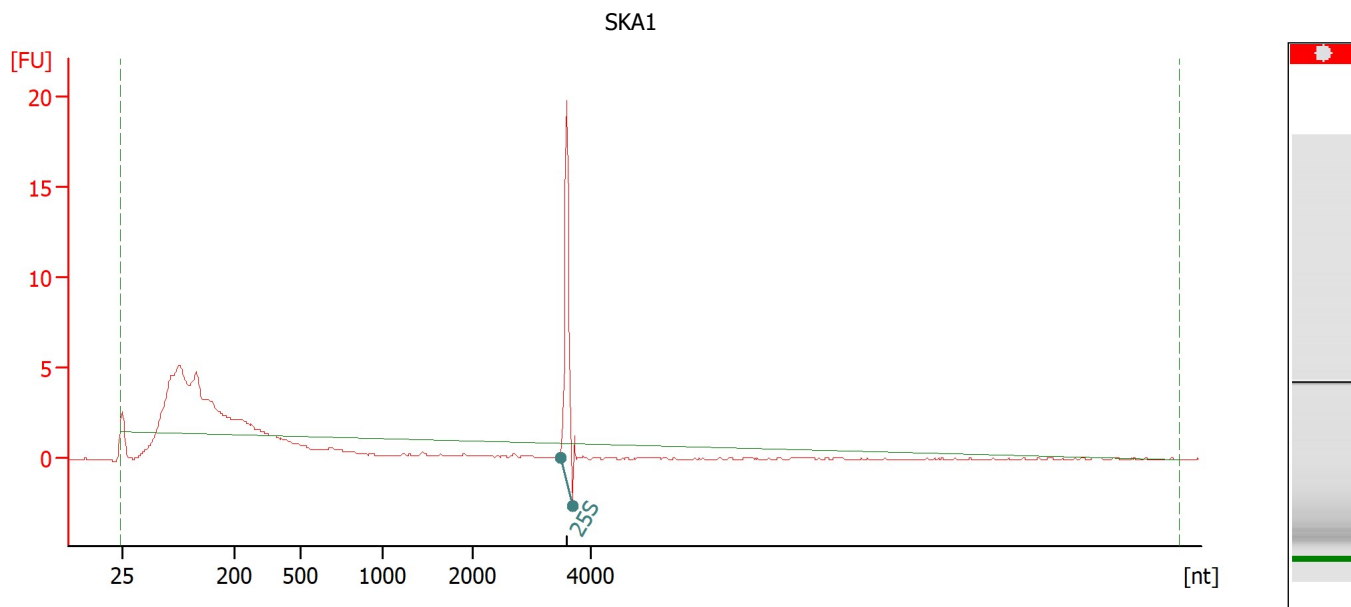Electropherogram Summary Continued ...**Overall Results for sample 11 : SKA1**


RNA Area:	46.4	RNA Integrity Number (RIN):	N/A (B.02.10)
RNA Concentration:	58 ng/μl	Result Flagging Color:	
rRNA Ratio [25s / 18s]:	0.0	Result Flagging Label:	RIN N/A

Fragment table for sample 11 : SKA1

Name	Start Size [nt]	End Size [nt]	Area	% of total Area
25S	3,480	3,681	12.5	26.9

Assay Class: Plant RNA Nano
Data Path: C:\...00 bioanalyzer\2100 expert\data\2025-09-24\SKA1_STITCH3.xad


Created: 9/24/2025 12:04:17 PM
Modified: 9/24/2025 12:43:31 PM

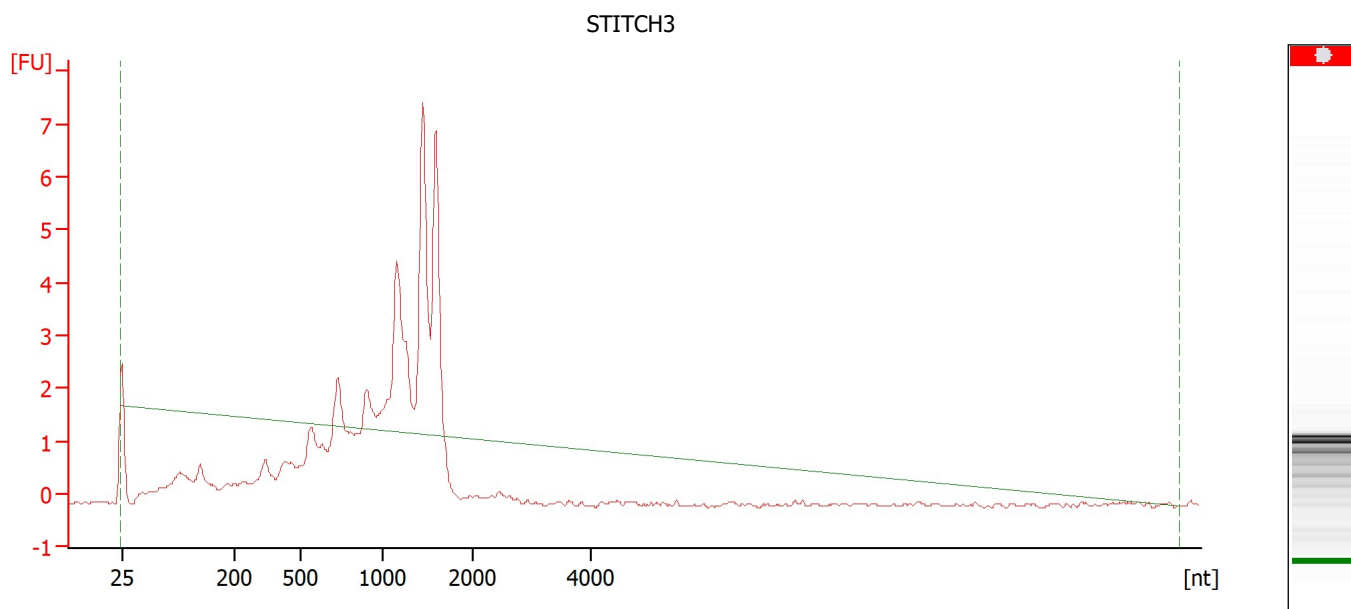Electropherogram Summary Continued ...**Overall Results for sample 12 : STITCH3**

RNA Area:	21.1	RNA Integrity Number (RIN):	N/A (B.02.10)
RNA Concentration:	27 ng/μl	Result Flagging Color:	
rRNA Ratio [25s / 18s]:	0.0	Result Flagging Label:	RIN N/A

Assay Class: Plant RNA Nano
Data Path: C:\...00 bioanalyzer\2100 expert\data\2025-09-24\SKA1_STITCH3.xad

Created: 9/24/2025 12:04:17 PM
Modified: 9/24/2025 12:43:31 PM

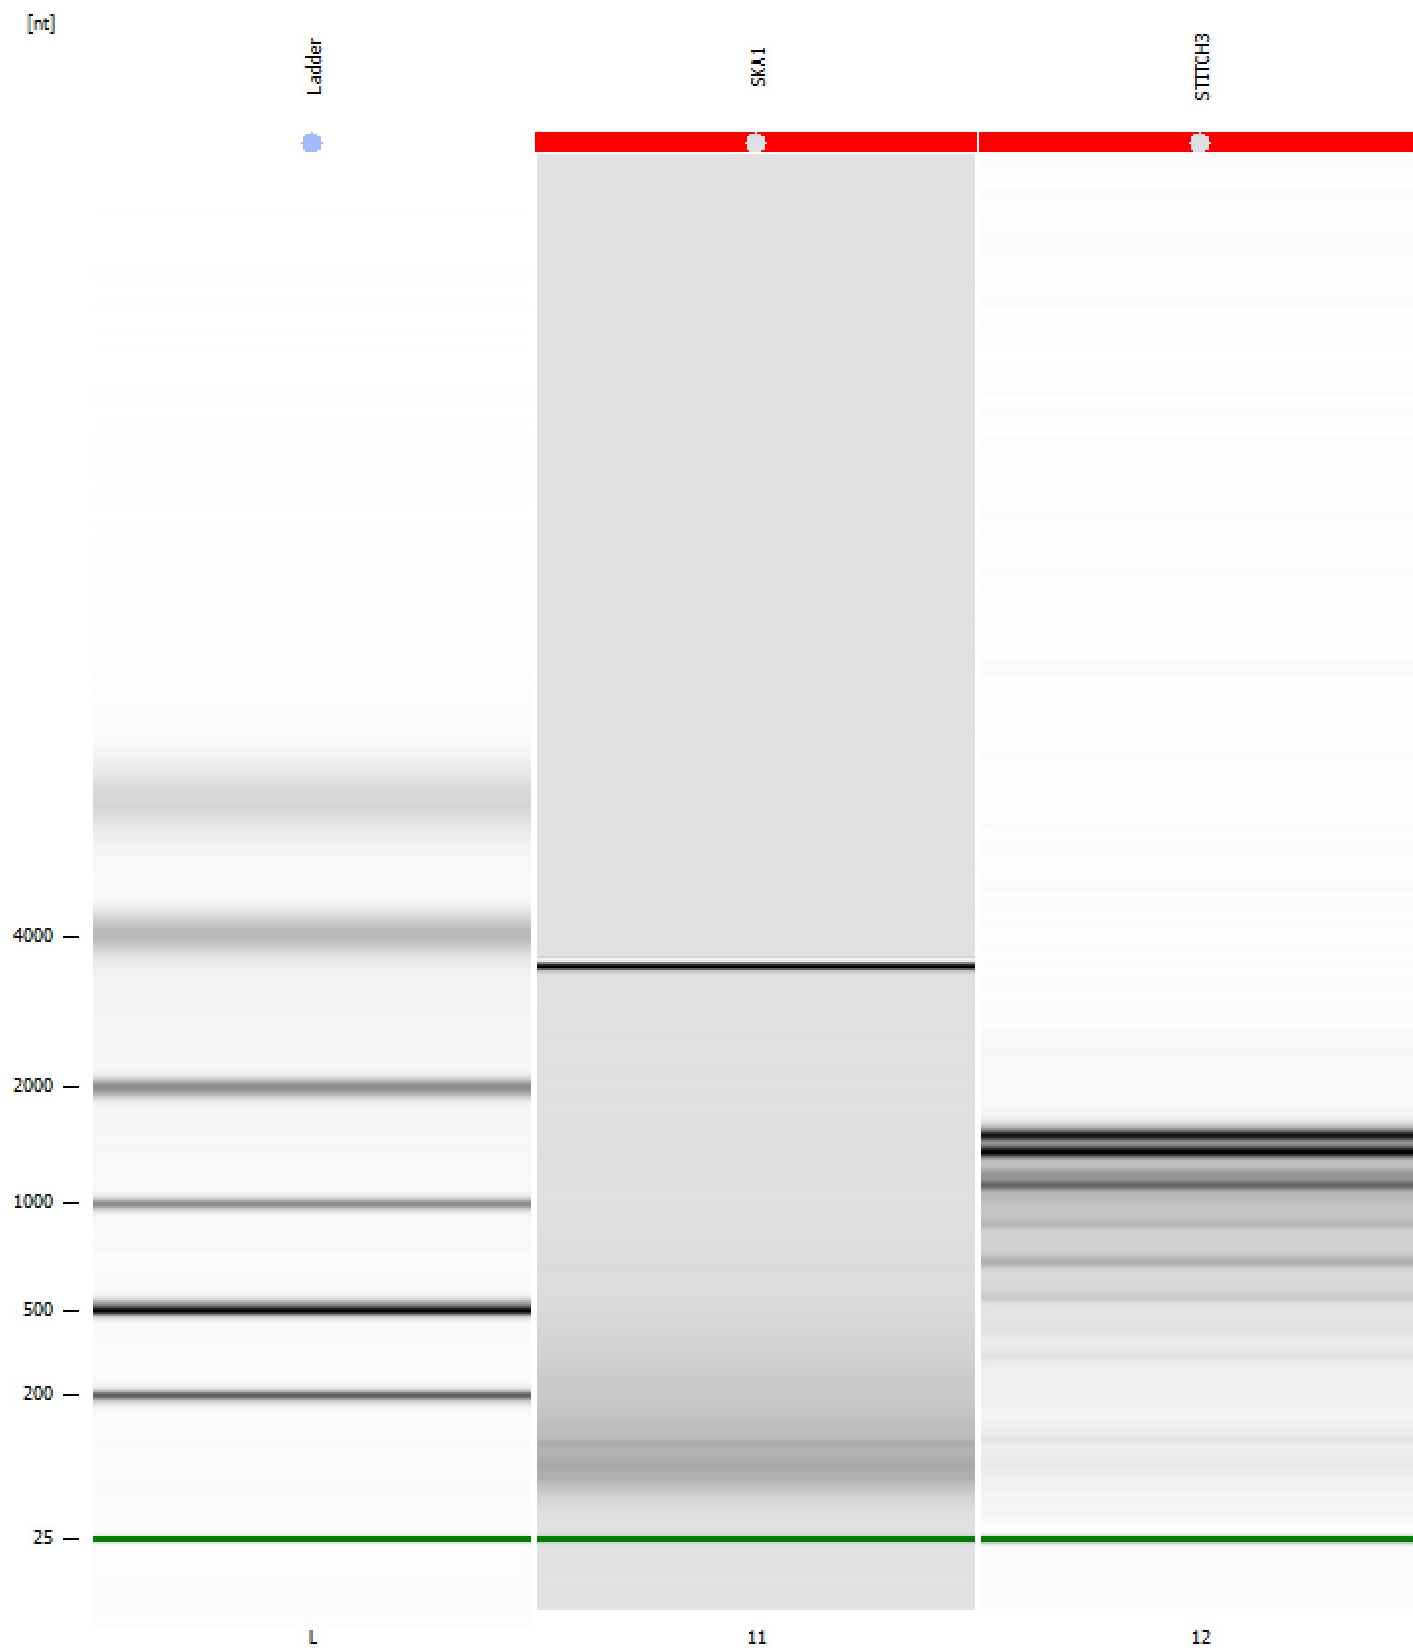Gel Image

Assay Class: Plant RNA Nano
 Data Path: C:\...00 bioanalyzer\2100 expert\data\2025-09-24\SKA1_STITCH3.xad

Created: 9/24/2025 12:04:17 PM
 Modified: 9/24/2025 12:43:31 PM

Run Logbook

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 13)		Instrument	Run		9/24/2025 12:28:10 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Run started on port 1 (File: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\data\2025-09-24\Bioanalyzer1_Plant RNA Nano_DE34903152_2025-09-24 Product Number : G2938C		Instrument	Run		9/24/2025 12:04:24 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Name :		Instrument	Run		9/24/2025 12:04:24 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Vendor : Agilent Technologies		Instrument	Run		9/24/2025 12:04:24 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Serial# : DE34903152		Instrument	Run		9/24/2025 12:04:24 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Firmware : C.01.069		Instrument	Run		9/24/2025 12:04:24 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB
Cartridge : Electrode		Instrument	Run		9/24/2025 12:04:24 PM	(GMT --07:00) Pacific Standard Time	sbsuser	DESKTOP-4UNV VOB