


Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...bioanalyzer\2100 expert\data\2025-04-03\TAG0302\_305\_306.xad

Created: 4/3/2025 11:16:18 AM  
Modified: 4/3/2025 12:24:31 PM

### Electrophoresis File Run Summary

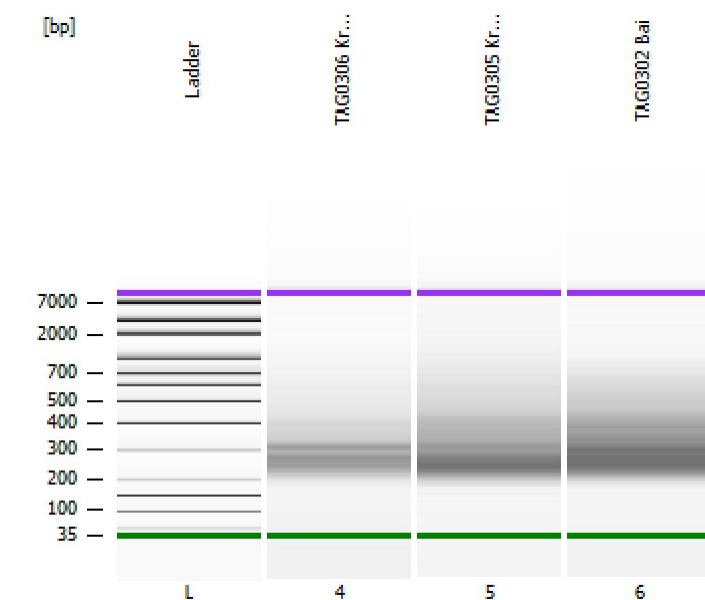

#### Instrument Information:

Instrument Name: DE34903152 Firmware: C.01.069  
Serial#: DE34903152 Type: G2938C


#### Assay Information:

Assay Origin Path: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy  
Assay Class: High Sensitivity DNA Assay  
Version: 1.03  
Assay Comments: Copyright © 2003-2010 Agilent Technologies


#### Chip Information:

Chip Lot #:  
Reagent Kit Lot #:  
Chip Comments:


TAG0306 Kramer

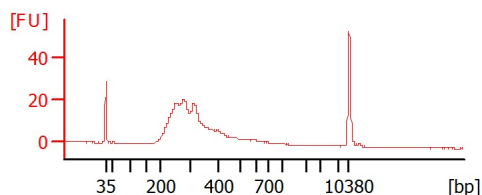

TAG0305 Kramer

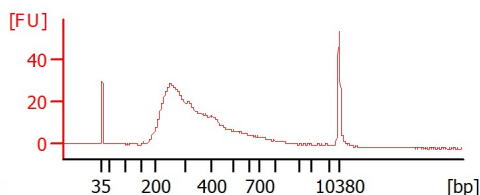

TAG0302 Bai

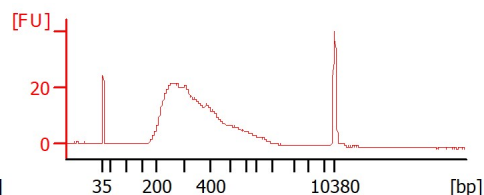

Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...bioanalyzer\2100 expert\data\2025-04-03\TAG0302\_305\_306.xad

Created: 4/3/2025 11:16:18 AM  
Modified: 4/3/2025 12:24:31 PM

**Electrophoresis File Run Summary (Chip Summary)**

| Sample Name    | Sample<br>Comment | Rest.<br>Digest          | Status | Observation | Result Label | Result Color |
|----------------|-------------------|--------------------------|--------|-------------|--------------|--------------|
| TAG0306 Kramer |                   | <input type="checkbox"/> | ✓      |             |              |              |
| TAG0305 Kramer |                   | <input type="checkbox"/> | ✓      |             |              |              |
| TAG0302 Bai    |                   | <input type="checkbox"/> | ✓      |             |              |              |
| Ladder         |                   | <input type="checkbox"/> | ✓      |             |              |              |

**Chip Lot #****Reagent Kit Lot #****Chip Comments :**

Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...bioanalyzer\2100 expert\data\2025-04-03\TAG0302\_305\_306.xad

Created: 4/3/2025 11:16:18 AM  
Modified: 4/3/2025 12:24:31 PM

## Electrophoresis Assay Details

### General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12  
Minimum Visible Range [s] : 32  
Maximum Visible Range [s] : 138  
Start Analysis Time Range [s] : 33  
End Analysis Time Range [s] : 137.5  
Ladder Concentration [pg/μl] : 1950  
Uses Standard Area for Ladder Fragments  
Lower Marker Concentration [pg/μl] : 125  
Upper Marker Concentration [pg/μl] : 75  
Used Upper Marker for Quantitation  
Standard Curve Fit is Point to Point  
Show Data Aligned to Lower and Upper Marker

### Integrator Settings

Integration Start Time [s] : 33.05  
Integration End Time [s] : 137  
Slope Threshold : 0.8  
Height Threshold [FU] : 5  
Area Threshold : 0.1  
Width Threshold [s] : 0.6  
Baseline Plateau [s] : 0.5

### Filter Settings

Filter Width [s] : 0.5  
Polynomial Order : 4


### Ladder

| Ladder Peak | Size  | Area |
|-------------|-------|------|
| 1           | 35    | 160  |
| 2           | 50    | 210  |
| 3           | 100   | 208  |
| 4           | 150   | 221  |
| 5           | 200   | 242  |
| 6           | 300   | 270  |
| 7           | 400   | 305  |
| 8           | 500   | 306  |
| 9           | 600   | 336  |
| 10          | 700   | 321  |
| 11          | 1000  | 366  |
| 12          | 2000  | 413  |
| 13          | 3000  | 411  |
| 14          | 7000  | 400  |
| 15          | 10380 | 214  |

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...bioanalyzer\2100 expert\data\2025-04-03\TAG0302\_305\_306.xad

Created: 4/3/2025 11:16:18 AM  
 Modified: 4/3/2025 12:24:31 PM

### Electropherogram Summary

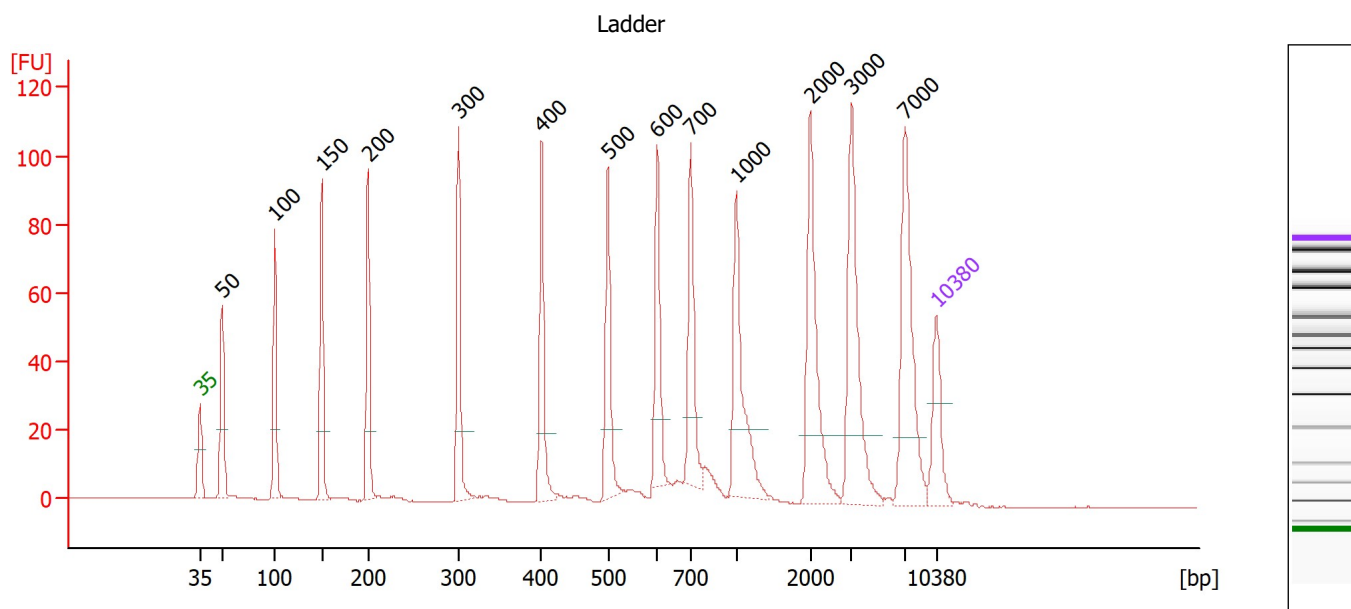

### Overall Results for Ladder

Noise: 0.1


### Peak table for Ladder

| Peak | Size [bp] | Conc. [pg/μl] | Molarity [pmol/l] | Observations |
|------|-----------|---------------|-------------------|--------------|
| 1    | 35        | 125.00        | 5,411.3           | Lower Marker |
| 2    | 50        | 150.00        | 4,545.5           | Ladder Peak  |
| 3    | 100       | 150.00        | 2,272.7           | Ladder Peak  |
| 4    | 150       | 150.00        | 1,515.2           | Ladder Peak  |
| 5    | 200       | 150.00        | 1,136.4           | Ladder Peak  |
| 6    | 300       | 150.00        | 757.6             | Ladder Peak  |
| 7    | 400       | 150.00        | 568.2             | Ladder Peak  |
| 8    | 500       | 150.00        | 454.5             | Ladder Peak  |
| 9    | 600       | 150.00        | 378.8             | Ladder Peak  |
| 10   | 700       | 150.00        | 324.7             | Ladder Peak  |
| 11   | 1,000     | 150.00        | 227.3             | Ladder Peak  |
| 12   | 2,000     | 150.00        | 113.6             | Ladder Peak  |
| 13   | 3,000     | 150.00        | 75.8              | Ladder Peak  |
| 14   | 7,000     | 150.00        | 32.5              | Ladder Peak  |
| 15   | 10,380    | 75.00         | 10.9              | Upper Marker |

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...bioanalyzer\2100 expert\data\2025-04-03\TAG0302\_305\_306.xad

Created: 4/3/2025 11:16:18 AM  
 Modified: 4/3/2025 12:24:31 PM

### Electropherogram Summary Continued ...

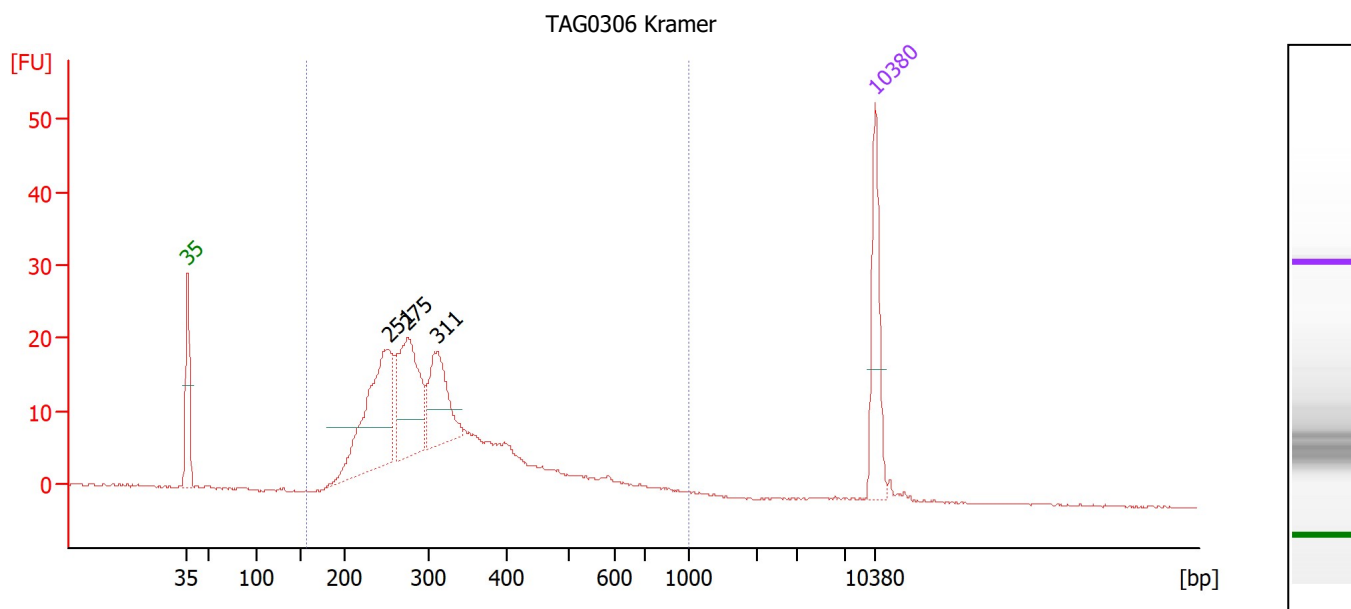

### Overall Results for sample 4 : TAG0306 Kramer

Number of peaks found: 3      Corr. Area 1: 352.6  
 Noise: 0.1

### Peak table for sample 4 : TAG0306 Kramer

| Peak | Size [bp] | Conc. [pg/μl] | Molarity [pmol/l] | Observations |
|------|-----------|---------------|-------------------|--------------|
| 1    | 35        | 125.00        | 5,411.3           | Lower Marker |
| 2    | 251       | 220.97        | 1,331.3           |              |
| 3    | 275       | 170.68        | 941.1             |              |
| 4    | 311       | 111.69        | 544.1             |              |
| 5    | 10,380    | 75.00         | 10.9              | Upper Marker |


### Region table for sample 4 : TAG0306 Kramer

| From [bp] | To [bp] | Corr. Area | % of Total | Average Size [bp] | Size distribution in CV [%] | Conc. [pg/μl] | Molarity [pmol/l] | Color |
|-----------|---------|------------|------------|-------------------|-----------------------------|---------------|-------------------|-------|
| 158       | 1,000   | 352.6      | 98         | 330               | 34.4                        | 989.22        | 5,067.1           | Blue  |

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...bioanalyzer\2100 expert\data\2025-04-03\TAG0302\_305\_306.xad

Created: 4/3/2025 11:16:18 AM  
 Modified: 4/3/2025 12:24:31 PM

### Electropherogram Summary Continued ...

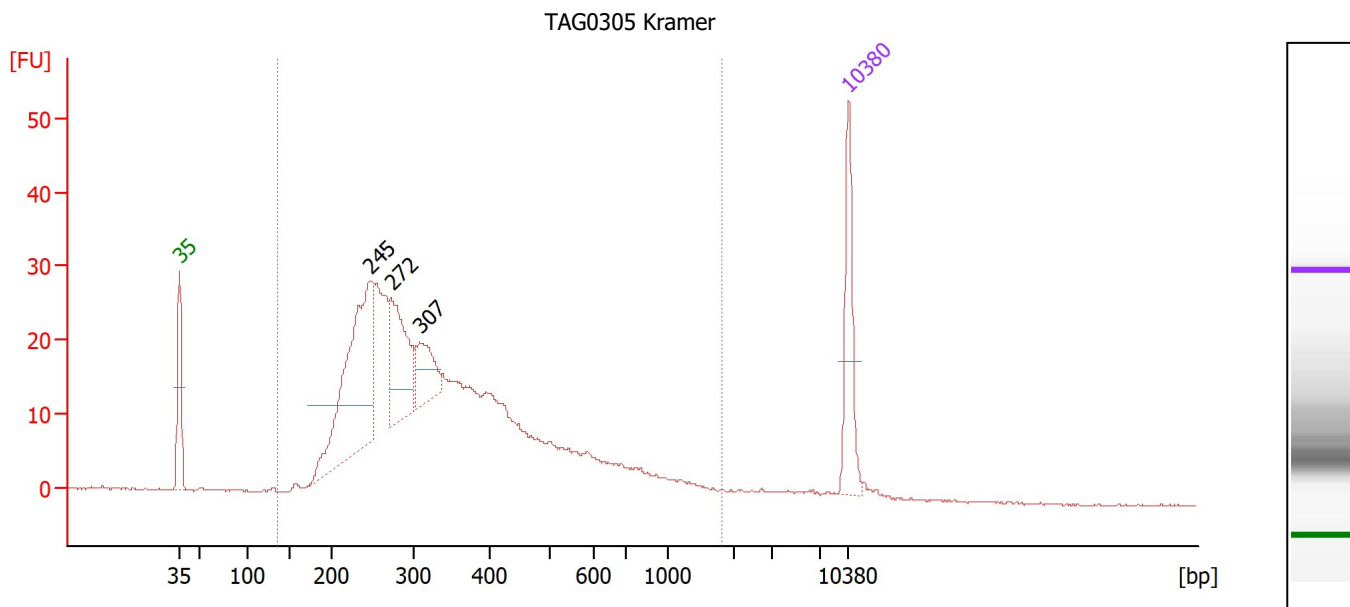

### Overall Results for sample 5 : TAG0305 Kramer

Number of peaks found: 3      Corr. Area 1: 619.3  
 Noise: 0.1

### Peak table for sample 5 : TAG0305 Kramer

| Peak | Size [bp] | Conc. [pg/μl] | Molarity [pmol/l] | Observations |
|------|-----------|---------------|-------------------|--------------|
| 1    | 35        | 125.00        | 5,411.3           | Lower Marker |
| 2    | 245       | 331.70        | 2,050.2           |              |
| 3    | 272       | 141.41        | 788.7             |              |
| 4    | 307       | 65.56         | 323.3             |              |
| 5    | 10,380    | 75.00         | 10.9              | Upper Marker |


### Region table for sample 5 : TAG0305 Kramer

| From [bp] | To [bp] | Corr. Area | % of Total | Average Size [bp] | Size distribution in CV [%] | Conc. [pg/μl] | Molarity [pmol/l] | Color |
|-----------|---------|------------|------------|-------------------|-----------------------------|---------------|-------------------|-------|
| 135       | 1,837   | 619.3      | 97         | 376               | 54.9                        | 1,760.20      | 8,787.3           | Blue  |

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...bioanalyzer\2100 expert\data\2025-04-03\TAG0302\_305\_306.xad

Created: 4/3/2025 11:16:18 AM  
 Modified: 4/3/2025 12:24:31 PM

### Electropherogram Summary Continued ...

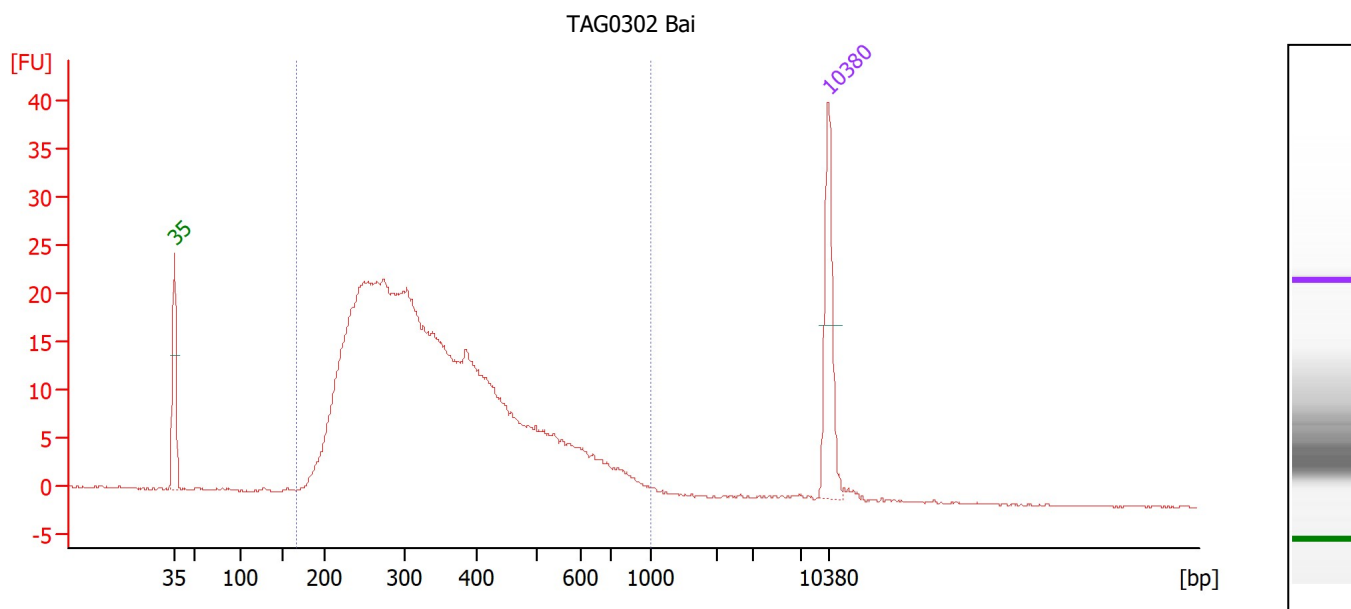

### Overall Results for sample 6 : TAG0302 Bai

Number of peaks found: 0      Corr. Area 1: 525.4  
 Noise: 0.1

### Peak table for sample 6 : TAG0302 Bai


| Peak | Size [bp] | Conc. [pg/μl] | Molarity [pmol/l] | Observations |
|------|-----------|---------------|-------------------|--------------|
| 1    | 35        | 125.00        | 5,411.3           | Lower Marker |
| 2    | 10,380    | 75.00         | 10.9              | Upper Marker |

### Region table for sample 6 : TAG0302 Bai

| From [bp] | To [bp] | Corr. Area | % of Total | Average Size [bp] | Size distribution in CV [%] | Conc. [pg/μl] | Molarity [pmol/l] | Color |
|-----------|---------|------------|------------|-------------------|-----------------------------|---------------|-------------------|-------|
| 166       | 1,000   | 525.4      | 98         | 358               | 36.1                        | 1,772.73      | 8,632.6           | Blue  |

Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...bioanalyzer\2100 expert\data\2025-04-03\TAG0302\_305\_306.xad

Created: 4/3/2025 11:16:18 AM  
Modified: 4/3/2025 12:24:31 PM

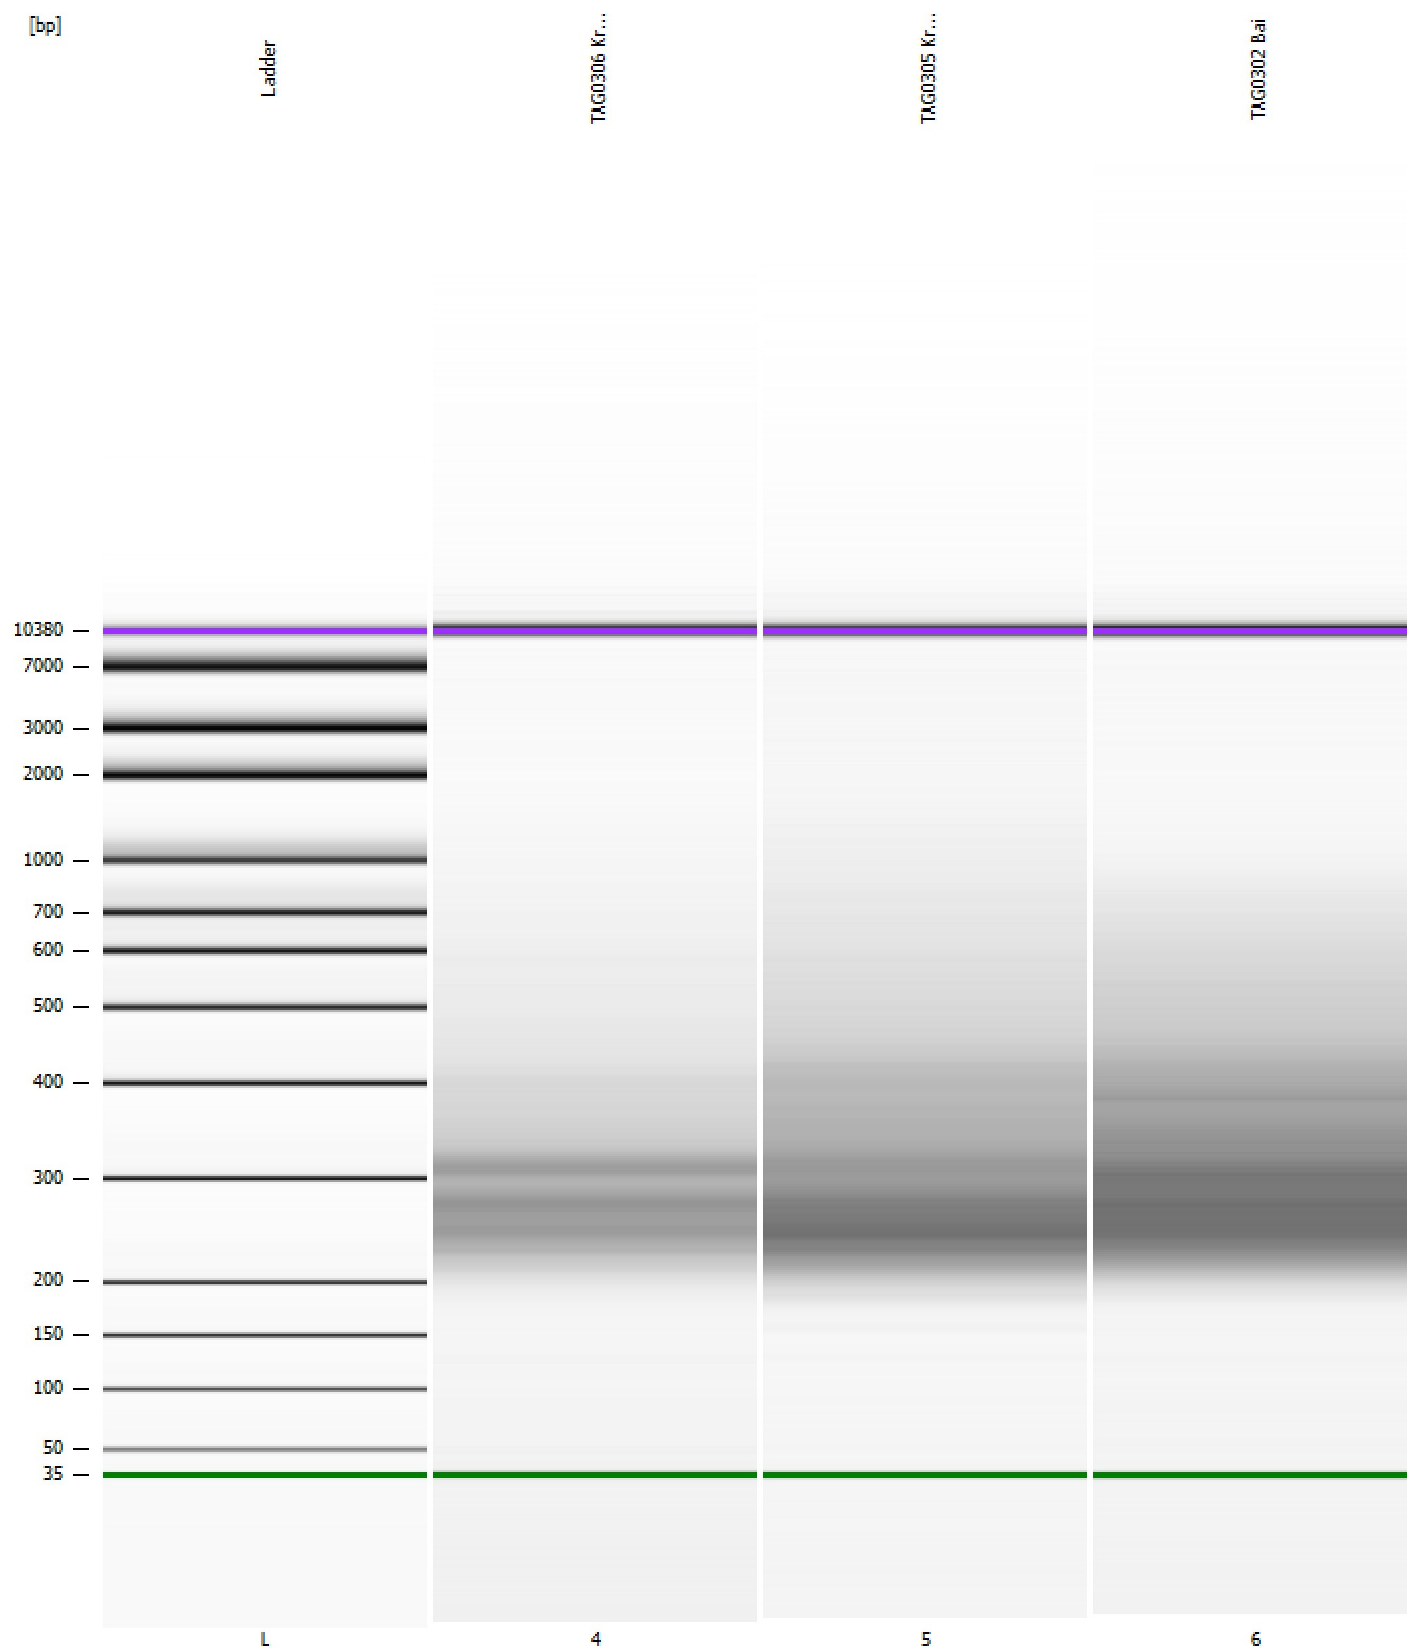**Gel Image**

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...bioanalyzer\2100 expert\data\2025-04-03\TAG0302\_305\_306.xad

Created: 4/3/2025 11:16:18 AM  
 Modified: 4/3/2025 12:24:31 PM

### Run Logbook

| Description                                                                                                                                                                     | Number | Source     | Category | Sub Category | Time                 | Time Zone                           | User    | Host             |
|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|------------|----------|--------------|----------------------|-------------------------------------|---------|------------------|
| Run ended on port 1 (Number of wells acquired: 12)                                                                                                                              |        | Instrument | Run      |              | 4/3/2025 11:57:39 AM | (GMT --07:00) Pacific Standard Time | sbsuser | DESKTOP-4UNV VOB |
| Run started on port 1 (File: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\data\2025-04-03\Bioanalyzer1_High Sensitivity DNA Assay_DE34903152_2025-04-03_001.xad) |        | Instrument | Run      |              | 4/3/2025 11:16:25 AM | (GMT --07:00) Pacific Standard Time | sbsuser | DESKTOP-4UNV VOB |
| Product Number : G2938C                                                                                                                                                         |        | Instrument | Run      |              | 4/3/2025 11:16:25 AM | (GMT --07:00) Pacific Standard Time | sbsuser | DESKTOP-4UNV VOB |
| Name :                                                                                                                                                                          |        | Instrument | Run      |              | 4/3/2025 11:16:25 AM | (GMT --07:00) Pacific Standard Time | sbsuser | DESKTOP-4UNV VOB |
| Vendor : Agilent Technologies                                                                                                                                                   |        | Instrument | Run      |              | 4/3/2025 11:16:25 AM | (GMT --07:00) Pacific Standard Time | sbsuser | DESKTOP-4UNV VOB |
| Serial# : DE34903152                                                                                                                                                            |        | Instrument | Run      |              | 4/3/2025 11:16:25 AM | (GMT --07:00) Pacific Standard Time | sbsuser | DESKTOP-4UNV VOB |
| Firmware : C.01.069                                                                                                                                                             |        | Instrument | Run      |              | 4/3/2025 11:16:25 AM | (GMT --07:00) Pacific Standard Time | sbsuser | DESKTOP-4UNV VOB |
| Cartridge : Electrode                                                                                                                                                           |        | Instrument | Run      |              | 4/3/2025 11:16:25 AM | (GMT --07:00) Pacific Standard Time | sbsuser | DESKTOP-4UNV VOB |