


Assay Class: High Sensitivity DNA Assay
Data Path: C:\...ents and Settings\Bioanalyzer\2015-06-12\2015-06-12_002.xad

Created: 6/12/2015 9:35:39 AM
Modified: 6/12/2015 10:22:33 AM

Electrophoresis File Run Summary

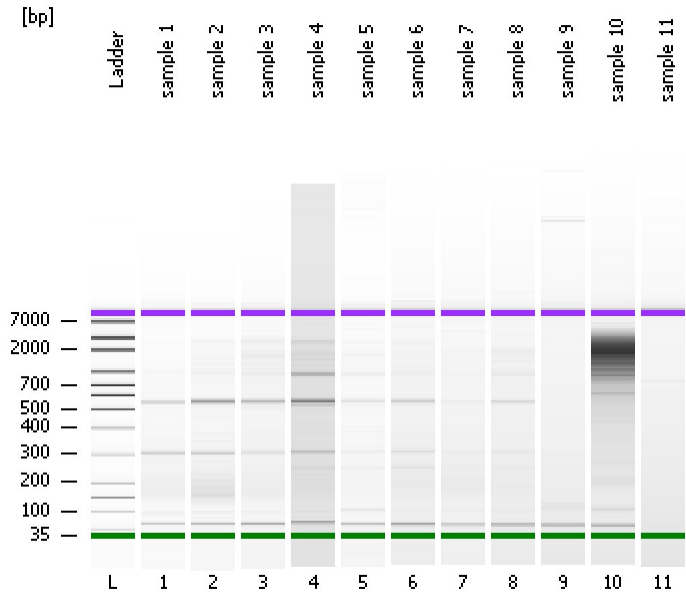

Instrument Information:


Instrument Name: DE13701086 Firmware: C.01.069
Serial#: DE13701086 Type: G2938B

Assay Information:

Assay Origin Path: C:\Program Files\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy
Assay Class: High Sensitivity DNA Assay
Version: 1.03
Assay Comments: Copyright © 2003-2010 Agilent Technologies

Chip Information:

Chip Lot #:
Reagent Kit Lot #:
Chip Comments:

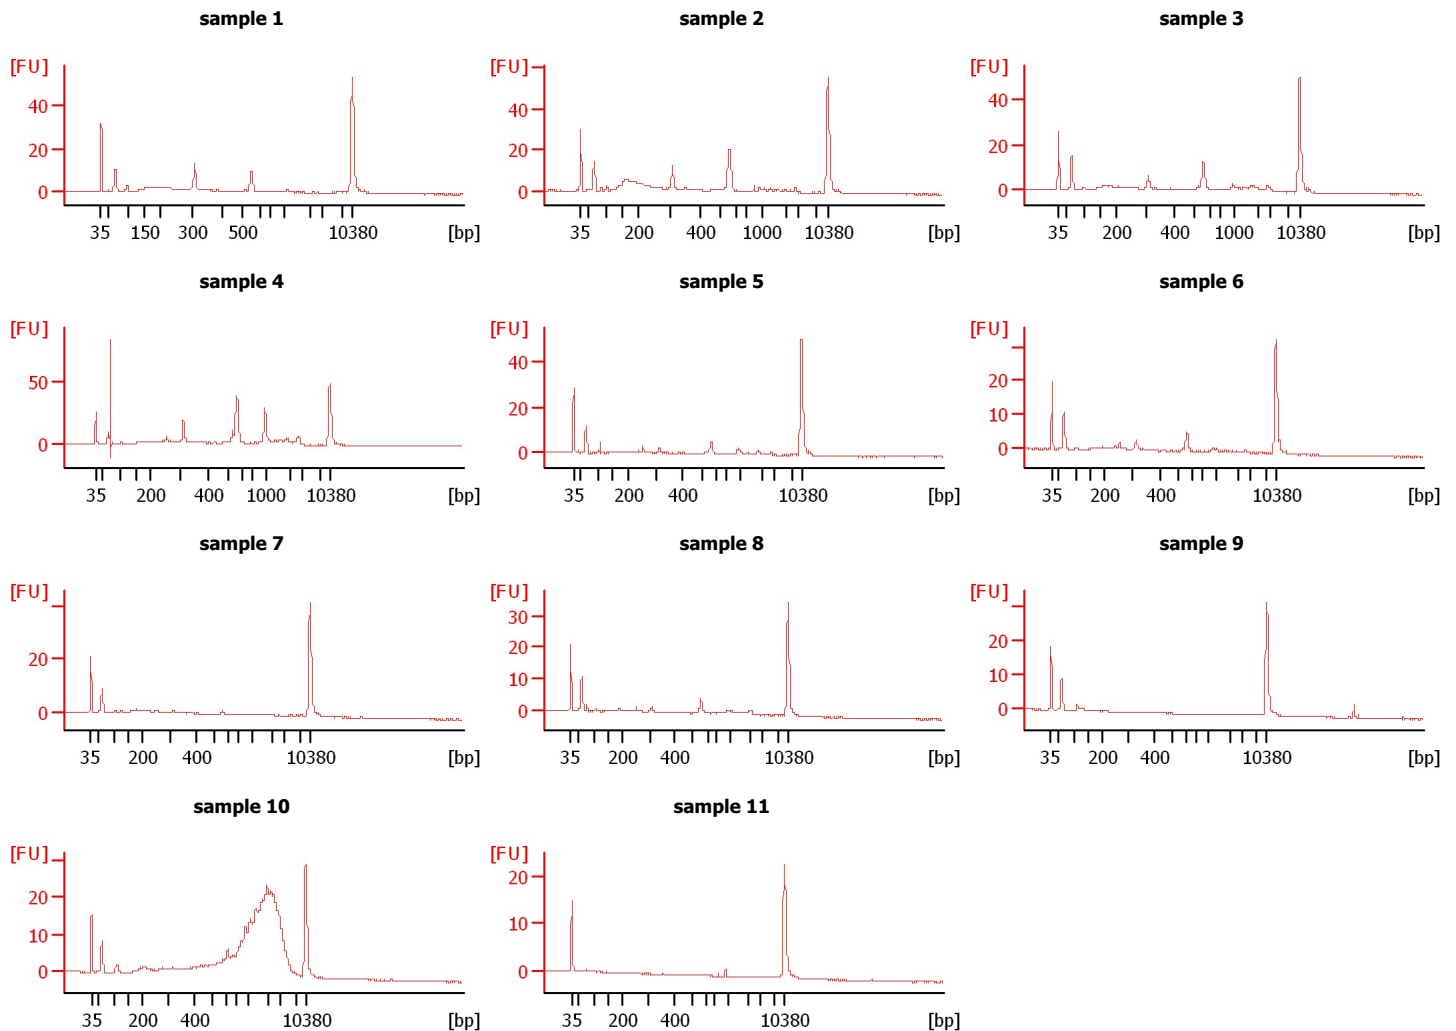

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2015-06-12\2015-06-12_002.xad

Created: 6/12/2015 9:35:39 AM
 Modified: 6/12/2015 10:22:33 AM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
sample 1		<input type="checkbox"/>	✓			
sample 2		<input type="checkbox"/>	✓			
sample 3		<input type="checkbox"/>	✓			
sample 4		<input type="checkbox"/>	✓			
sample 5		<input type="checkbox"/>	✓			
sample 6		<input type="checkbox"/>	✓			
sample 7		<input type="checkbox"/>	✓			
sample 8		<input type="checkbox"/>	✓			
sample 9		<input type="checkbox"/>	✓			
sample 10		<input type="checkbox"/>	✓			
sample 11		<input type="checkbox"/>	✓			
Ladder		<input type="checkbox"/>	✓			

Chip Lot #

Reagent Kit Lot #

Chip Comments :

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...ents and Settings\Bioanalyzer\2015-06-12\2015-06-12_002.xad

Created: 6/12/2015 9:35:39 AM
Modified: 6/12/2015 10:22:33 AM

Electrophoresis Assay Details

General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12
Minimum Visible Range [s] : 32
Maximum Visible Range [s] : 138
Start Analysis Time Range [s] : 33
End Analysis Time Range [s] : 137.5
Ladder Concentration [pg/μl] : 1950
Uses Standard Area for Ladder Fragments
Lower Marker Concentration [pg/μl] : 125
Upper Marker Concentration [pg/μl] : 75
Used Upper Marker for Quantitation
Standard Curve Fit is Point to Point
Show Data Aligned to Lower and Upper Marker

Integrator Settings

Integration Start Time [s] : 33.05
Integration End Time [s] : 137
Slope Threshold : 0.8
Height Threshold [FU] : 5
Area Threshold : 0.1
Width Threshold [s] : 0.6
Baseline Plateau [s] : 0.5

Filter Settings

Filter Width [s] : 0.5
Polynomial Order : 4


Ladder

Ladder Peak	Size	Area
1	35	160
2	50	210
3	100	208
4	150	221
5	200	242
6	300	270
7	400	305
8	500	306
9	600	336
10	700	321
11	1000	366
12	2000	413
13	3000	411
14	7000	400
15	10380	214

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2015-06-12\2015-06-12_002.xad

Created: 6/12/2015 9:35:39 AM
 Modified: 6/12/2015 10:22:33 AM

Electropherogram Summary

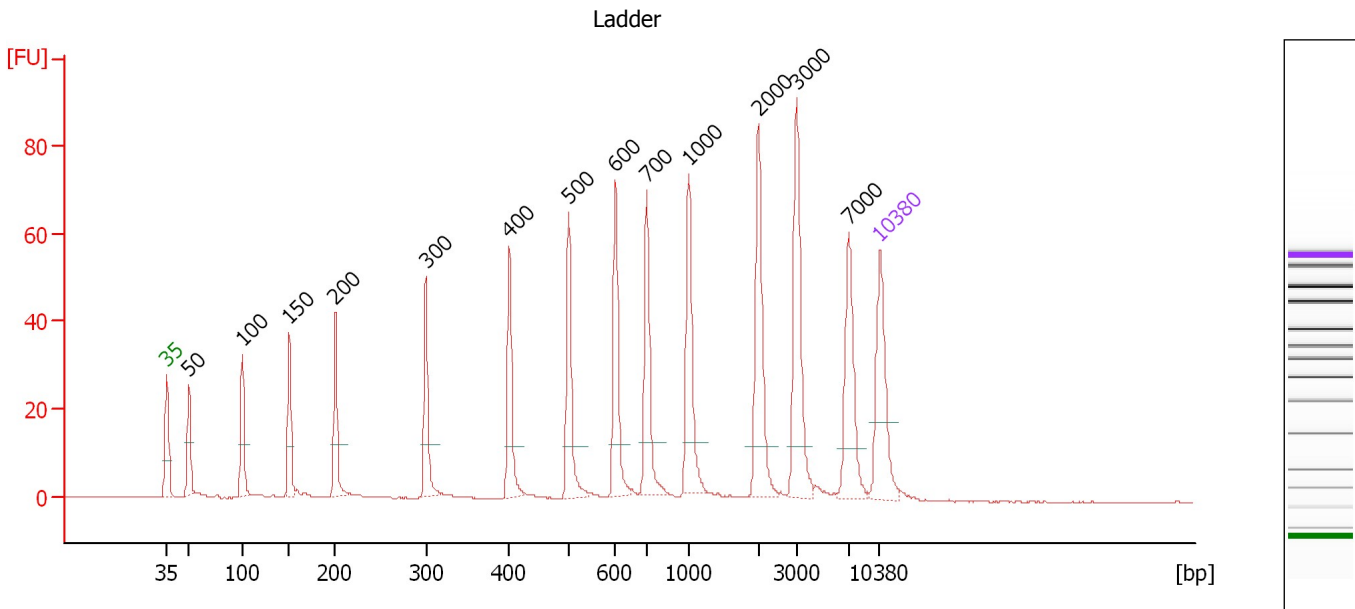

Overall Results for Ladder

Noise: 0.1


Peak table for Ladder

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	50	150.00	4,545.5	Ladder Peak	45.15
3	100	150.00	2,272.7	Ladder Peak	50.43
4	150	150.00	1,515.2	Ladder Peak	55.04
5	200	150.00	1,136.4	Ladder Peak	59.54
6	300	150.00	757.6	Ladder Peak	68.45
7	400	150.00	568.2	Ladder Peak	76.66
8	500	150.00	454.5	Ladder Peak	82.48
9	600	150.00	378.8	Ladder Peak	87.08
10	700	150.00	324.7	Ladder Peak	90.12
11	1,000	150.00	227.3	Ladder Peak	94.26
12	2,000	150.00	113.6	Ladder Peak	101.12
13	3,000	150.00	75.8	Ladder Peak	104.83
14	7,000	150.00	32.5	Ladder Peak	109.96
15	10,380	75.00	10.9	Upper Marker	113.00

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2015-06-12\2015-06-12_002.xad

Created: 6/12/2015 9:35:39 AM
 Modified: 6/12/2015 10:22:33 AM

Electropherogram Summary Continued ...

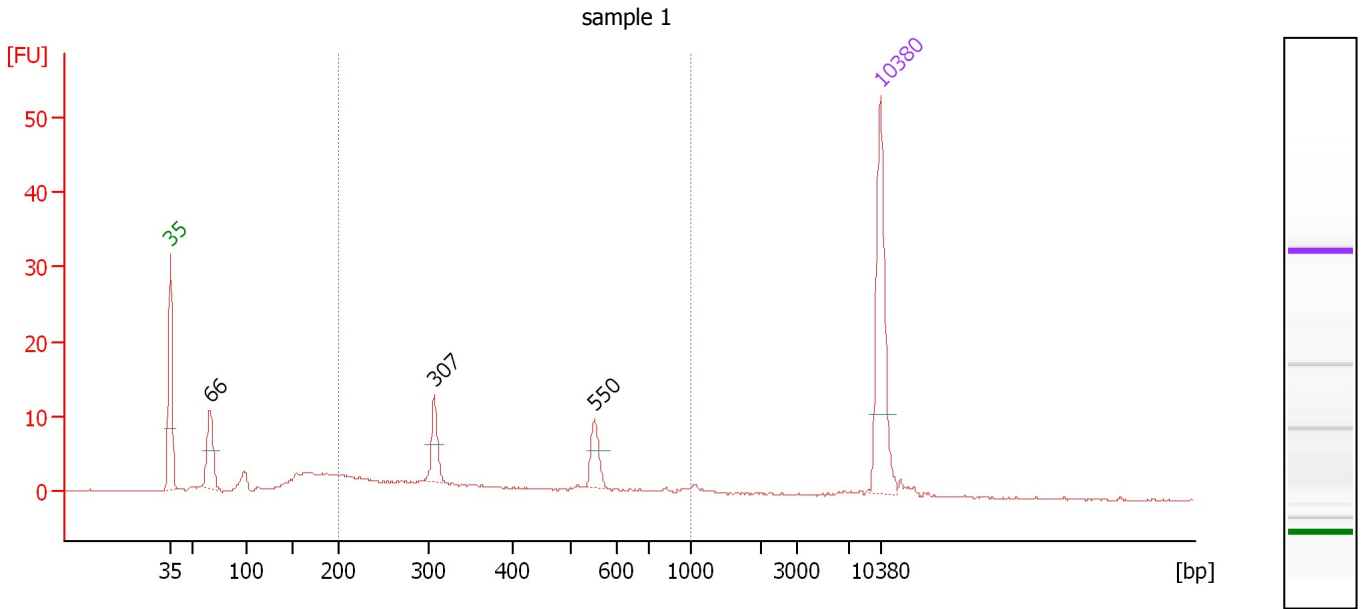

Overall Results for sample 1 : sample 1

Number of peaks found: 3 Corr. Area 1: 72.5
 Noise: 0.1

Peak table for sample 1 : sample 1

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	66	51.57	1,175.4		46.89
3	307	28.69	141.6		69.01
4	550	21.59	59.5		84.78
5	10,380	75.00	10.9	Upper Marker	113.00


Region table for sample 1 : sample 1

From [bp]	Average Size [bp]	To [bp]	Corr. Area	Molarity [pmol/l]	Co % of lor Total	Size distribution in CV [%]	Conc. [pg/μl]
200	405	1,000	72.5	823.5	55	41.3	178.77

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2015-06-12\2015-06-12_002.xad

Created: 6/12/2015 9:35:39 AM
 Modified: 6/12/2015 10:22:33 AM

Electropherogram Summary Continued ...

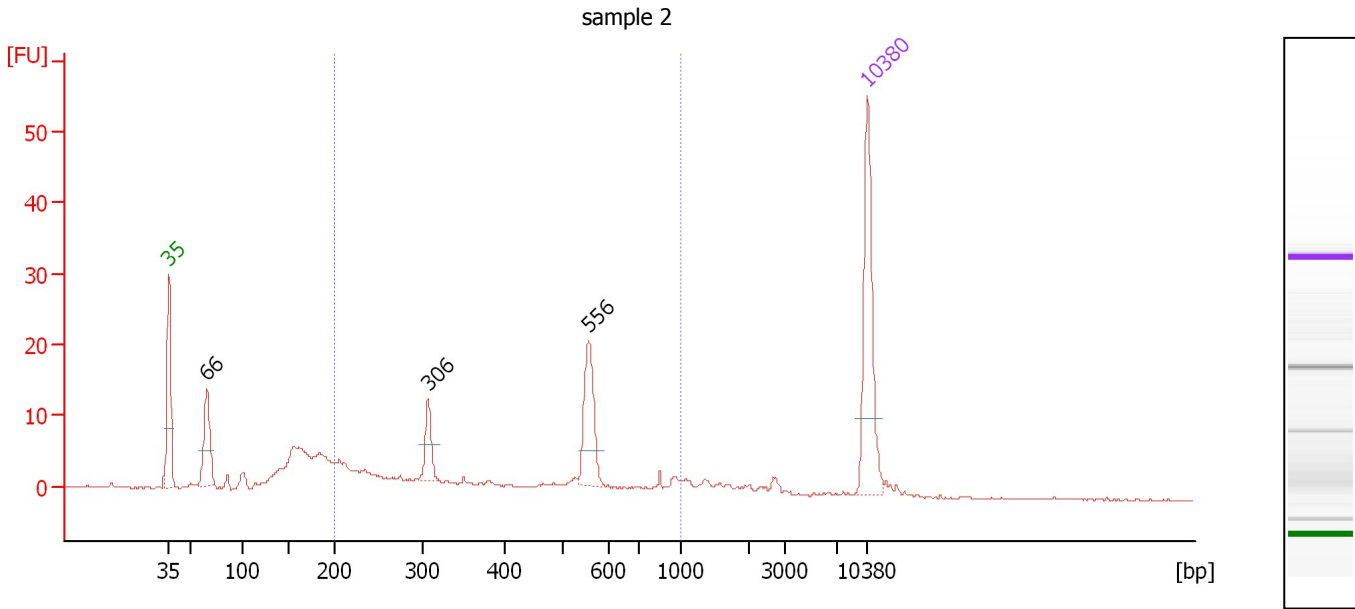

Overall Results for sample 2 : sample 2

Number of peaks found: 3 Corr. Area 1: 105.4
 Noise: 0.1

Peak table for sample 2 : sample 2

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	66	65.16	1,505.6		46.79
3	306	28.00	138.5		68.97
4	556	56.64	154.4		85.05
5	10,380	75.00	10.9	Upper Marker	113.00


Region table for sample 2 : sample 2

From [bp]	Average Size [bp]	To [bp]	Corr. Area	Molarity [pmol/l]	Co % of lor Total	Size distribution in CV [%]	Conc. [pg/μl]
200	443	1,000	105.4	1,078.3	52	41.0	245.74

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2015-06-12\2015-06-12_002.xad

Created: 6/12/2015 9:35:39 AM
 Modified: 6/12/2015 10:22:33 AM

Electropherogram Summary Continued ...

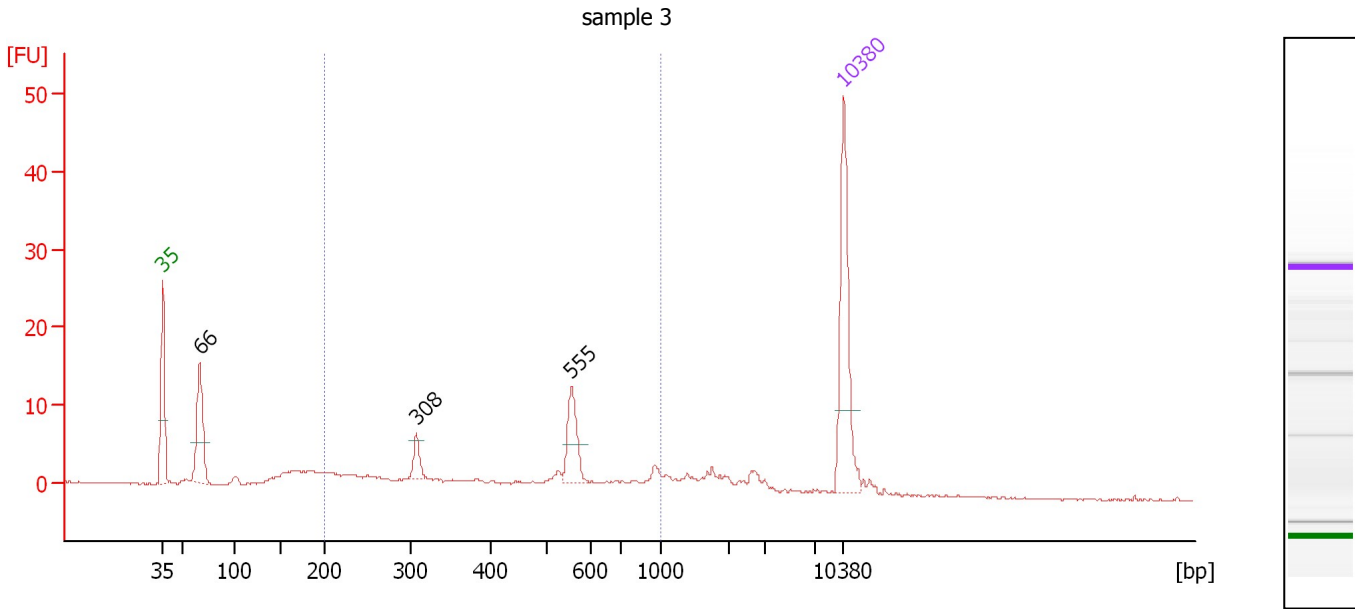

Overall Results for sample 3 : sample 3

Number of peaks found: 3 Corr. Area 1: 76.2
 Noise: 0.1

Peak table for sample 3 : sample 3

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	66	80.95	1,859.7		46.83
3	308	16.16	79.6		69.07
4	555	35.93	98.1		85.01
5	10,380	75.00	10.9	Upper Marker	113.00


Region table for sample 3 : sample 3

From [bp]	Average Size [bp]	To [bp]	Corr. Area	Molarity [pmol/l]	Co % of Ior Total	Size distribution in CV [%]	Conc. [pg/μl]
200	479	1,000	76.2	784.3	52	41.0	192.48

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2015-06-12\2015-06-12_002.xad

Created: 6/12/2015 9:35:39 AM
 Modified: 6/12/2015 10:22:33 AM

Electropherogram Summary Continued ...

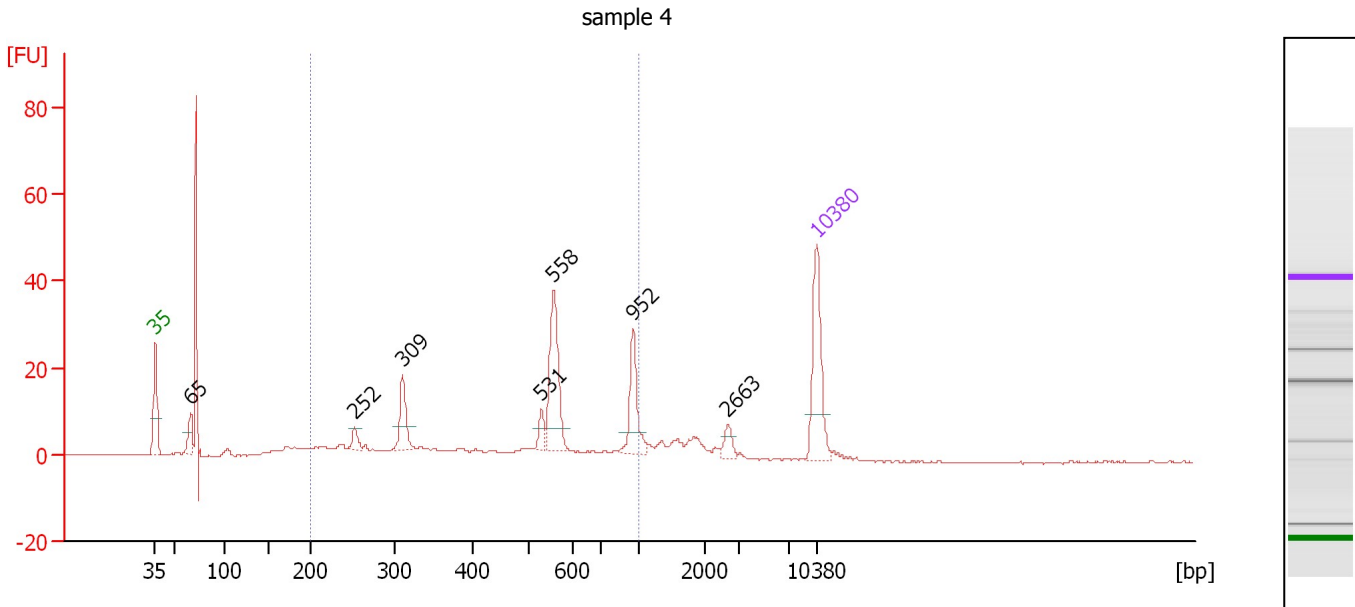

Overall Results for sample 4 : sample 4

Number of peaks found: 7 Corr. Area 1: 175.4
 Noise: 0.1

Peak table for sample 4 : sample 4

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	65	30.96	716.9		46.78
3	252	14.38	86.5		64.15
4	309	44.28	217.2		69.17
5	531	15.15	43.2		83.89
6	558	98.40	267.3		85.14
7	952	53.06	84.4		93.60
8	2,663	12.04	6.9		103.58
9	10,380	75.00	10.9	Upper Marker	113.00


Region table for sample 4 : sample 4

From [bp]	Average Size [bp]	To [bp]	Corr. Area	Molarity [pmol/l]	Co % of Ior Total	Size distribution in CV [%]	Conc. [pg/μl]
200	540	1,000	175.4	1,516.1	61	42.3	407.76

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2015-06-12\2015-06-12_002.xad

Created: 6/12/2015 9:35:39 AM
 Modified: 6/12/2015 10:22:33 AM

Electropherogram Summary Continued ...

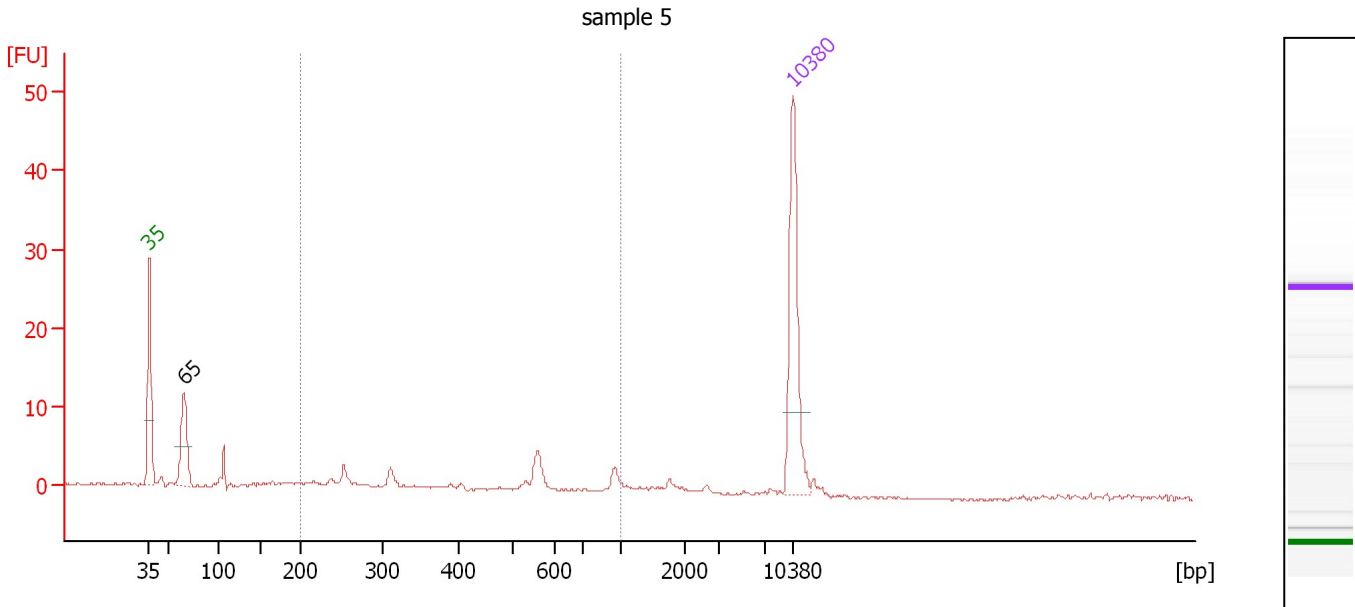

Overall Results for sample 5 : sample 5

Number of peaks found: 1 Corr. Area 1: 22.1
 Noise: 0.2

Peak table for sample 5 : sample 5

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	65	60.07	1,393.5		46.77
3	10,380	75.00	10.9	Upper Marker	113.00


Region table for sample 5 : sample 5

From [bp]	Average Size [bp]	To [bp]	Corr. Area	Molarity [pmol/l]	Co % of lor Total	Size distribution in CV [%]	Conc. [pg/μl]
200	473	1,000	22.1	232.5	40	49.2	52.75

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2015-06-12\2015-06-12_002.xad

Created: 6/12/2015 9:35:39 AM
 Modified: 6/12/2015 10:22:33 AM

Electropherogram Summary Continued ...

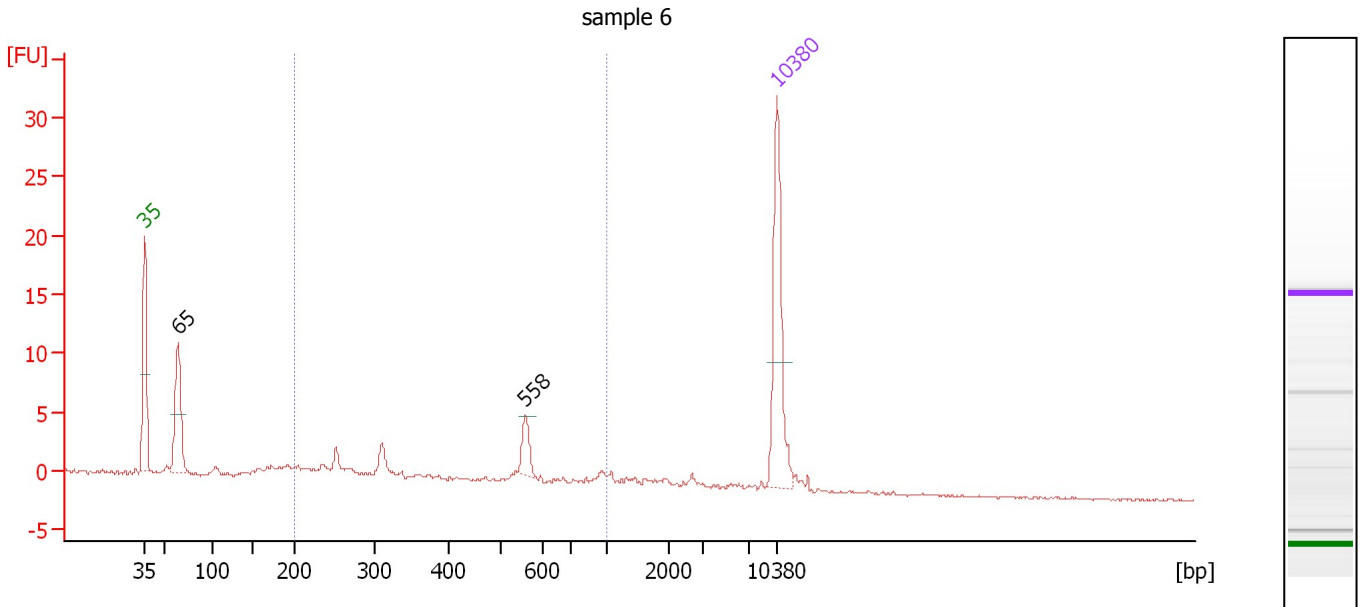

Overall Results for sample 6 : sample 6

Number of peaks found: 2 Corr. Area 1: 26.0
 Noise: 0.1

Peak table for sample 6 : sample 6

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	65	86.75	2,026.5		46.72
3	558	17.84	48.5		85.14
4	10,380	75.00	10.9	Upper Marker	113.00


Region table for sample 6 : sample 6

From [bp]	Average Size [bp]	To [bp]	Corr. Area	Molarity [pmol/l]	Co % of lor Total	Size distribution in CV [%]	Conc. [pg/μl]
200	442	1,000	26.0	442.7	47	44.6	98.92

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2015-06-12\2015-06-12_002.xad

Created: 6/12/2015 9:35:39 AM
 Modified: 6/12/2015 10:22:33 AM

Electropherogram Summary Continued ...

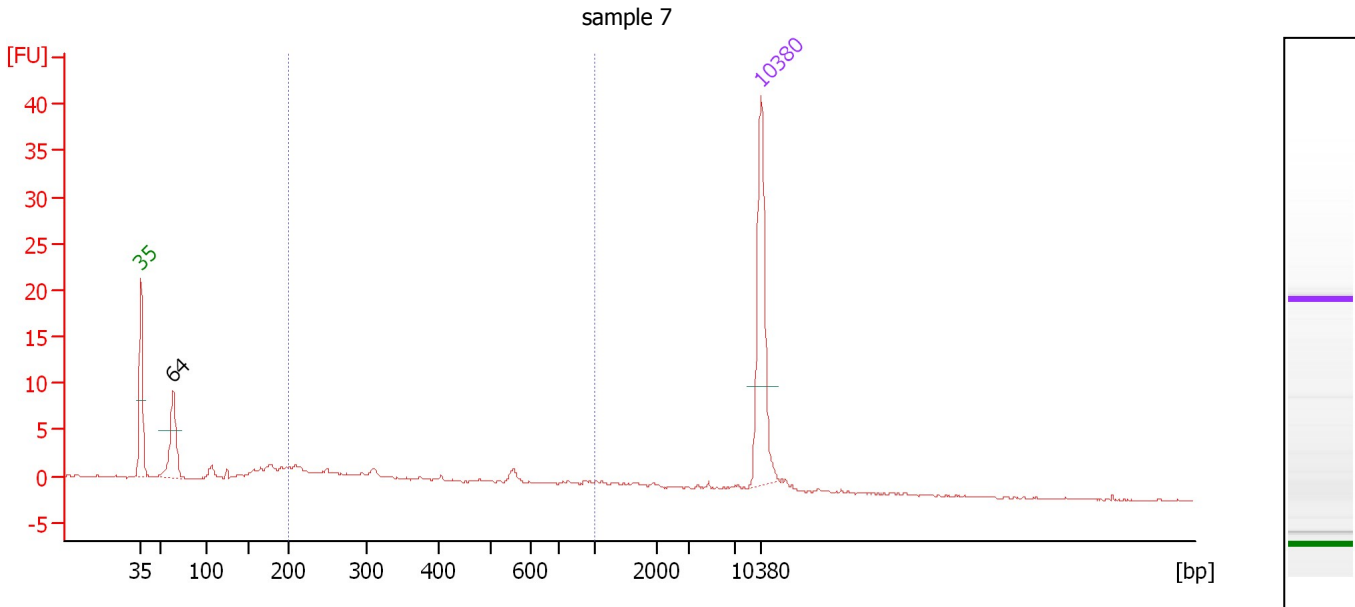

Overall Results for sample 7 : sample 7

Number of peaks found: 1 Corr. Area 1: 31.4
 Noise: 0.1

Peak table for sample 7 : sample 7

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	64	62.01	1,471.6		46.61
3	10,380	75.00	10.9	Upper Marker	113.00


Region table for sample 7 : sample 7

From [bp]	Average Size [bp]	To [bp]	Corr. Area	Molarity [pmol/l]	Co % of Ior Total	Size distribution in CV [%]	Conc. [pg/μl]
200	406	1,000	31.4	468.6	45	47.7	97.56

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2015-06-12\2015-06-12_002.xad

Created: 6/12/2015 9:35:39 AM
 Modified: 6/12/2015 10:22:33 AM

Electropherogram Summary Continued ...

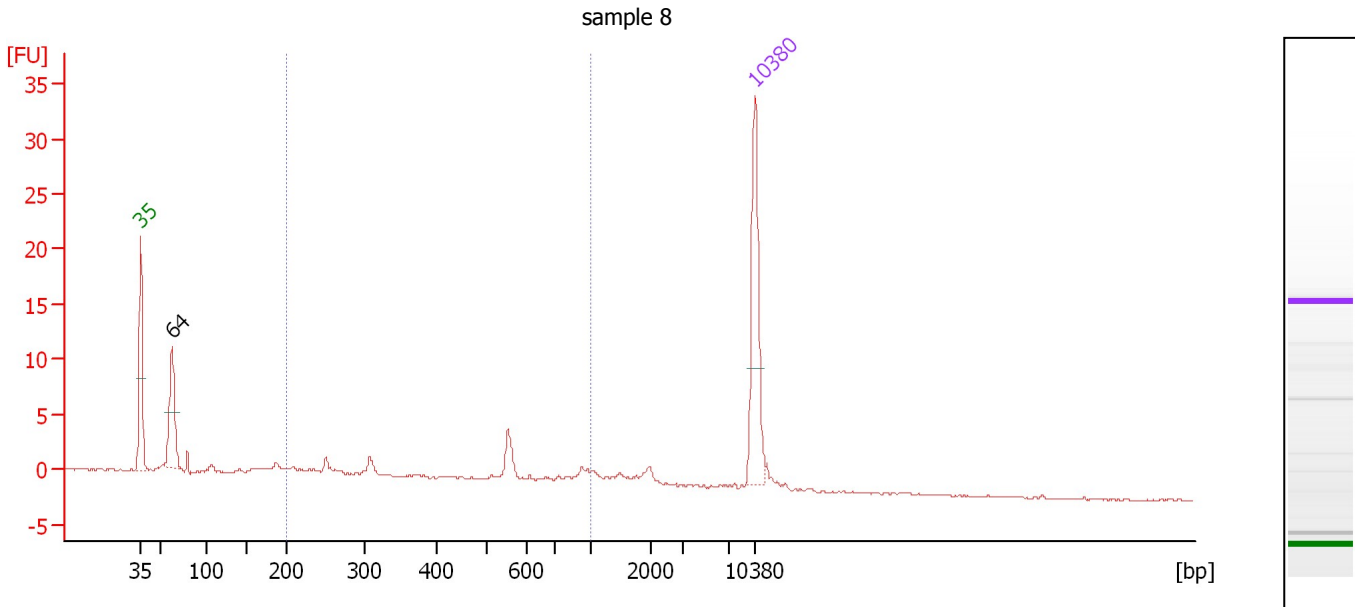

Overall Results for sample 8 : sample 8

Number of peaks found: 1 Corr. Area 1: 24.8
 Noise: 0.1

Peak table for sample 8 : sample 8

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	64	82.29	1,960.3		46.59
3	10,380	75.00	10.9	Upper Marker	113.00


Region table for sample 8 : sample 8

From [bp]	Average Size [bp]	To [bp]	Corr. Area	Molarity [pmol/l]	Co % of Ior Total	Size distribution in CV [%]	Conc. [pg/μl]
200	483	1,000	24.8	406.3	39	45.8	95.80

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2015-06-12\2015-06-12_002.xad

Created: 6/12/2015 9:35:39 AM
 Modified: 6/12/2015 10:22:33 AM

Electropherogram Summary Continued ...

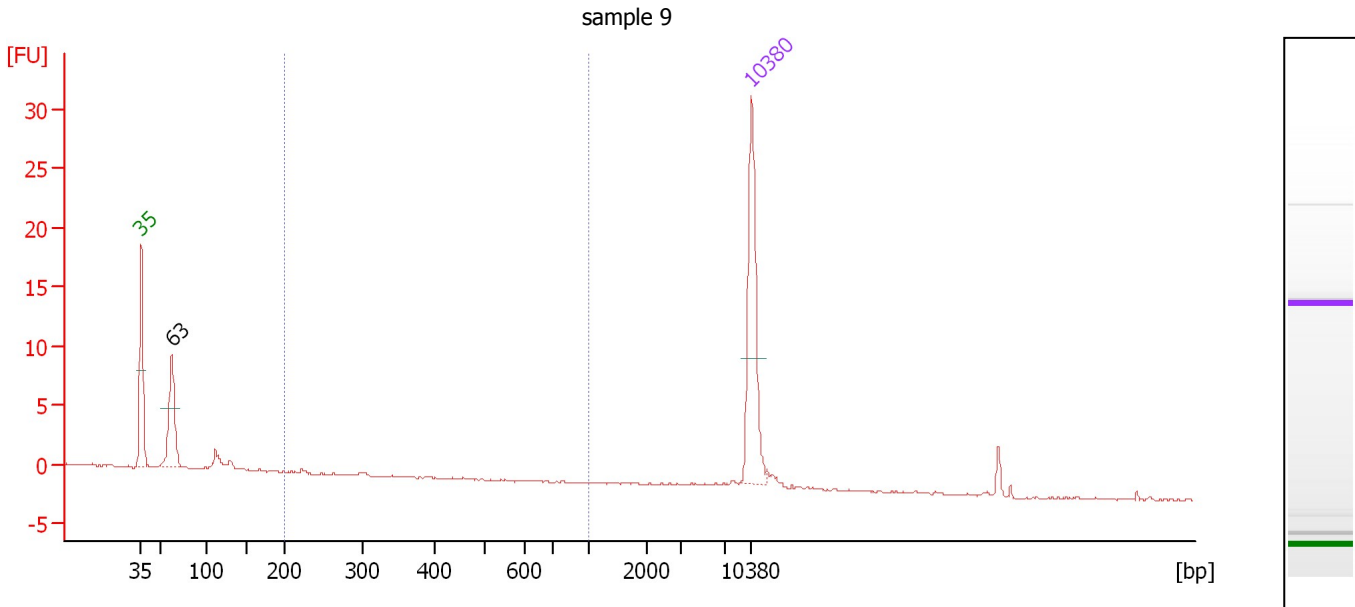

Overall Results for sample 9 : sample 9

Number of peaks found: 1 Corr. Area 1: 0.1
 Noise: 0.1

Peak table for sample 9 : sample 9

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	63	74.70	1,805.7		46.49
3	10,380	75.00	10.9	Upper Marker	113.00


Region table for sample 9 : sample 9

From [bp]	Average Size [bp]	To [bp]	Corr. Area	Molarity [pmol/l]	Co % of lor Total	Size distribution in CV [%]	Conc. [pg/μl]
200	224	1,000	0.1	2.8	0	5.8	0.41

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2015-06-12\2015-06-12_002.xad

Created: 6/12/2015 9:35:39 AM
 Modified: 6/12/2015 10:22:33 AM

Electropherogram Summary Continued ...

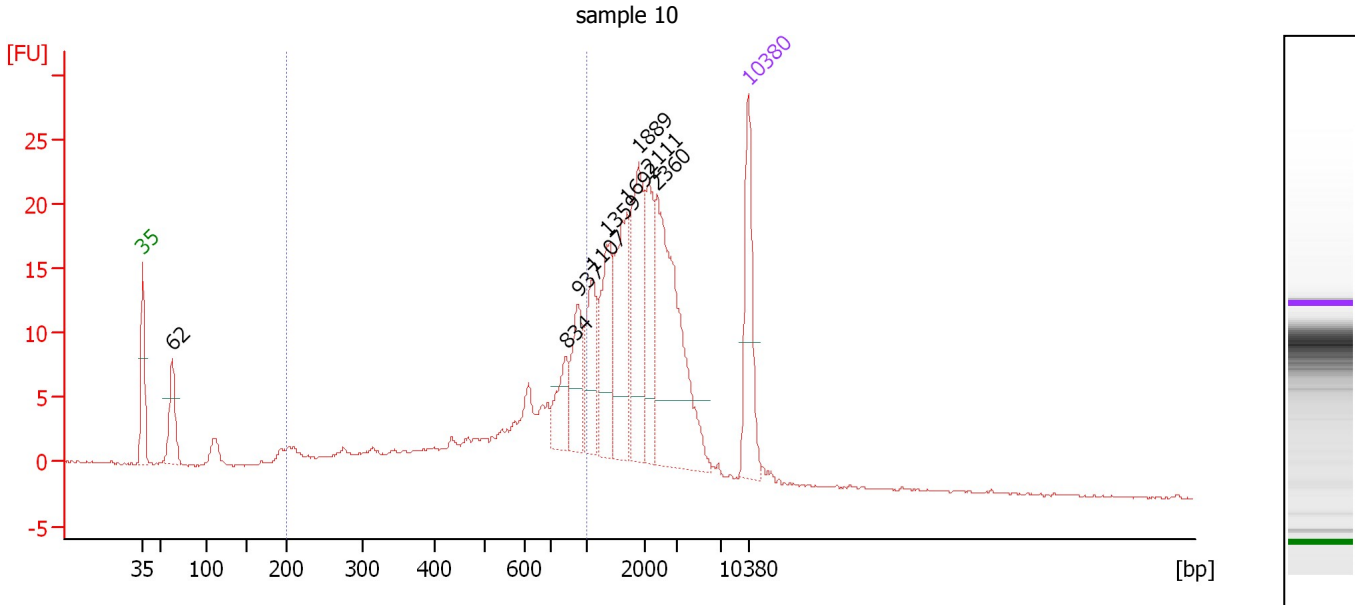

Overall Results for sample 10 : sample 10

Number of peaks found: 9 Corr. Area 1: 125.7
 Noise: 0.1

Peak table for sample 10 : sample 10

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	62	73.02	1,791.0		46.39
3	834	39.05	70.9		91.97
4	937	53.71	86.9		93.39
5	1,107	61.75	84.5		94.99
6	1,359	75.05	83.7		96.72
7	1,692	95.59	85.6		99.00
8	1,889	104.40	83.7		100.36
9	2,111	61.35	44.0		101.53
10	2,360	186.74	119.9		102.45
11	10,380	75.00	10.9	Upper Marker	113.00


Region table for sample 10 : sample 10

From [bp]	Average Size [bp]	To [bp]	Corr. Area	Molarity [pmol/l]	Co % of lor Total	Size distribution in CV [%]	Conc. [pg/μl]
200	610	1,000	125.7	1,605.2	34	37.3	493.70

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2015-06-12\2015-06-12_002.xad

Created: 6/12/2015 9:35:39 AM
 Modified: 6/12/2015 10:22:33 AM

Electropherogram Summary Continued ...

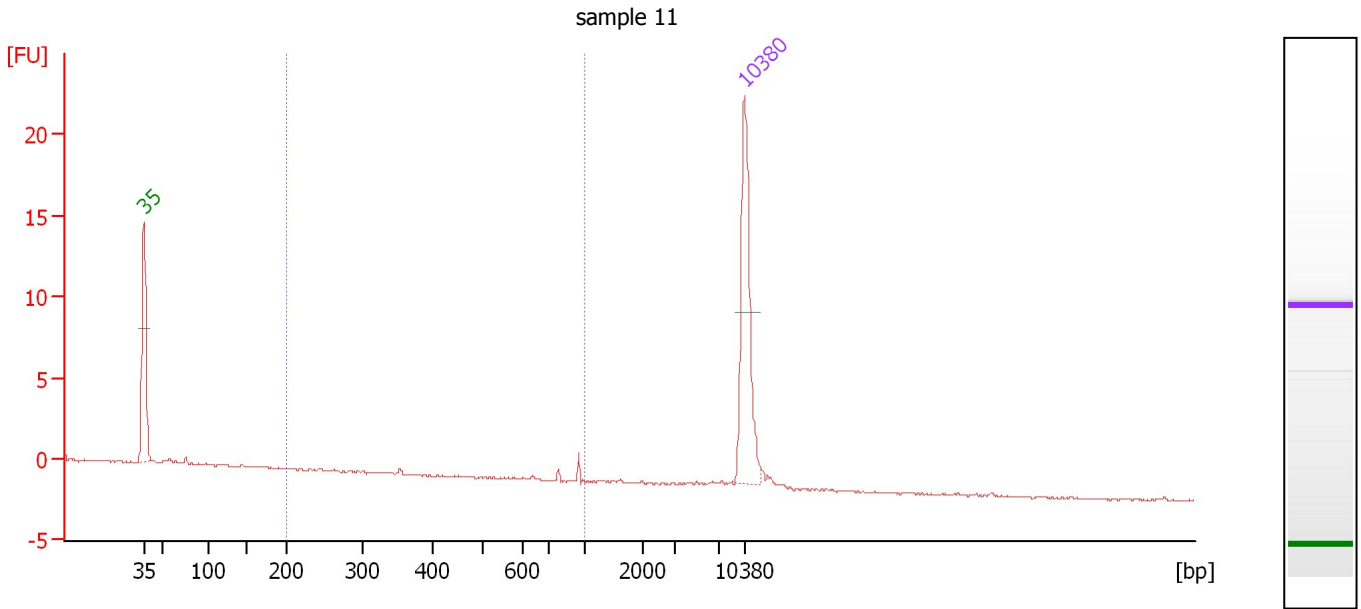

Overall Results for sample 11 : sample 11

Number of peaks found: 0 Corr. Area 1: 0.5
 Noise: 0.1

Peak table for sample 11 : sample 11

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	10,380	75.00	10.9	Upper Marker	113.00

Region table for sample 11 : sample 11

From [bp]	Average Size [bp]	To [bp]	Corr. Area	Molarity [pmol/l]	Co % of Ior Total	Size distribution in CV [%]	Conc. [pg/μl]
200	859	1,000	0.5	4.1	21	21.5	1.99

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...ents and Settings\Bioanalyzer\2015-06-12\2015-06-12_002.xad

Created: 6/12/2015 9:35:39 AM
Modified: 6/12/2015 10:22:33 AM

Gel Image

