

Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...alyzer\2016-01-14\2016-01-14\_003\_KDMJ001\_KDMJ002\_QC\_061.xad

Created: 1/14/2016 3:08:47 PM  
Modified: 1/14/2016 4:54:25 PM

**Electrophoresis File Run Summary**

Instrument Information:



Instrument Name: DE13701086                      Firmware: C.01.069  
Serial#: DE13701086                              Type: G2938B

Assay Information:

Assay Origin Path: C:\Program Files\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy  
Assay Class: High Sensitivity DNA Assay  
Version: 1.03  
Assay Comments: Copyright © 2003-2010 Agilent Technologies

Chip Information:

Chip Lot #:  
Reagent Kit Lot #:  
Chip Comments:

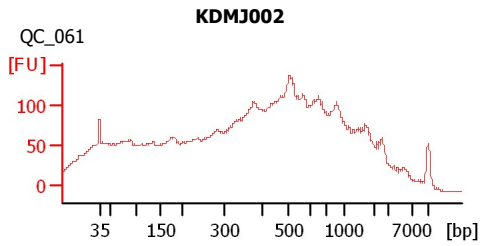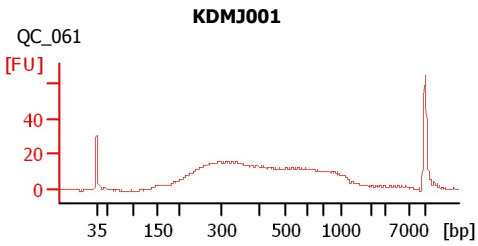

Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...alyzer\2016-01-14\2016-01-14\_003\_KDMJ001\_KDMJ002\_QC\_061.xad

Created: 1/14/2016 3:08:47 PM  
Modified: 1/14/2016 4:54:25 PM

**Electrophoresis File Run Summary (Chip Summary)**

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
KDMJ001	QC_061	<input type="checkbox"/>	✓			
KDMJ002	QC_061	<input type="checkbox"/>	✓			
Ladder		<input type="checkbox"/>	✓			

**Chip Lot #** **Reagent Kit Lot #**

**Chip Comments :**

Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...alyzer\2016-01-14\2016-01-14\_003\_KDMJ001\_KDMJ002\_QC\_061.xad

Created: 1/14/2016 3:08:47 PM  
Modified: 1/14/2016 4:54:25 PM

**Electrophoresis Assay Details**

**General Analysis Settings**

Number of Available Sample and Ladder Wells (Max.) : 12  
Minimum Visible Range [s] : 32  
Maximum Visible Range [s] : 138  
Start Analysis Time Range [s] : 33  
End Analysis Time Range [s] : 137.5  
Ladder Concentration [pg/μl] : 1950  
Uses Standard Area for Ladder Fragments  
Lower Marker Concentration [pg/μl] : 125  
Upper Marker Concentration [pg/μl] : 75  
Used Upper Marker for Quantitation  
Standard Curve Fit is Point to Point  
Show Data Aligned to Lower and Upper Marker

**Integrator Settings**

Integration Start Time [s] : 33.05  
Integration End Time [s] : 137  
Slope Threshold : 0.8  
Height Threshold [FU] : 5  
Area Threshold : 0.1  
Width Threshold [s] : 0.6  
Baseline Plateau [s] : 0.5

**Filter Settings**

Filter Width [s] : 0.5  
Polynomial Order : 4


**Ladder**

Ladder Peak	Size	Area
1	35	160
2	50	210
3	100	208
4	150	221
5	200	242
6	300	270
7	400	305
8	500	306
9	600	336
10	700	321
11	1000	366
12	2000	413
13	3000	411
14	7000	400
15	10380	214

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...alyzer\2016-01-14\2016-01-14\_003\_KDMJ001\_KDMJ002\_QC\_061.xad

Created: 1/14/2016 3:08:47 PM  
 Modified: 1/14/2016 4:54:25 PM

**Electropherogram Summary**

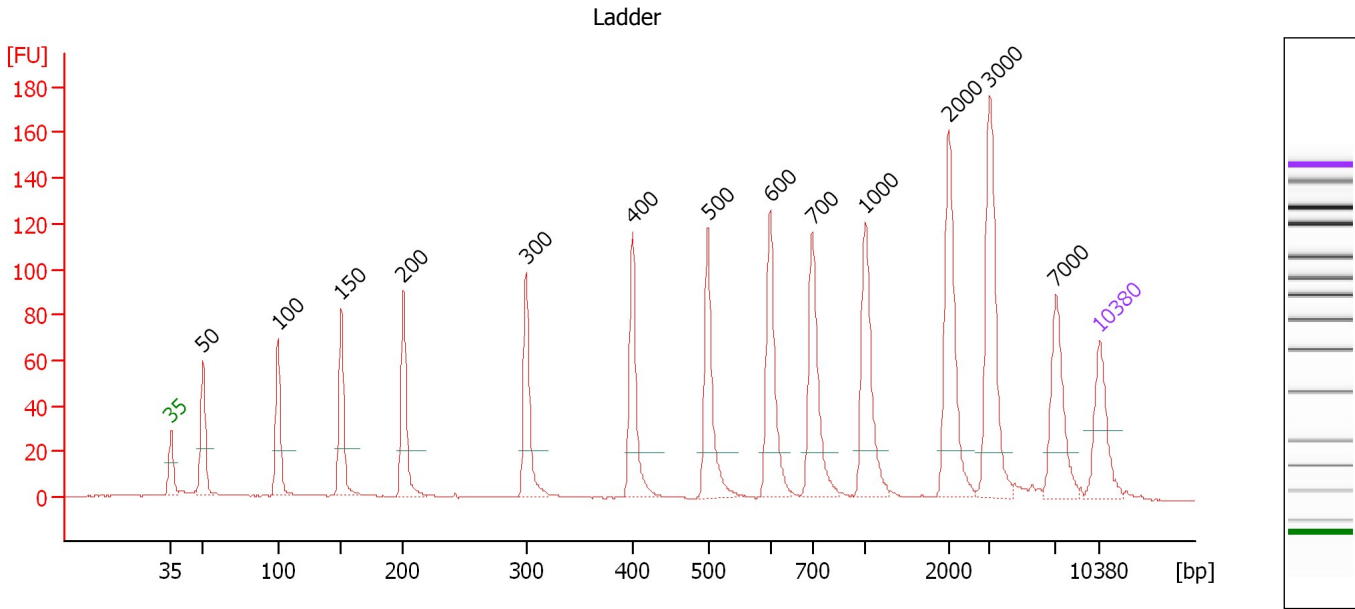

**Overall Results for Ladder**

Noise: 0.3


**Peak table for Ladder**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	50	150.00	4,545.5	Ladder Peak	45.43
3	100	150.00	2,272.7	Ladder Peak	51.06
4	150	150.00	1,515.2	Ladder Peak	55.84
5	200	150.00	1,136.4	Ladder Peak	60.51
6	300	150.00	757.6	Ladder Peak	69.77
7	400	150.00	568.2	Ladder Peak	77.79
8	500	150.00	454.5	Ladder Peak	83.46
9	600	150.00	378.8	Ladder Peak	88.14
10	700	150.00	324.7	Ladder Peak	91.34
11	1,000	150.00	227.3	Ladder Peak	95.34
12	2,000	150.00	113.6	Ladder Peak	101.60
13	3,000	150.00	75.8	Ladder Peak	104.70
14	7,000	150.00	32.5	Ladder Peak	109.66
15	10,380	75.00	10.9	Upper Marker	113.00

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...alyzer\2016-01-14\2016-01-14\_003\_KDMJ001\_KDMJ002\_QC\_061.xad

Created: 1/14/2016 3:08:47 PM  
 Modified: 1/14/2016 4:54:25 PM

**Electropherogram Summary Continued ...**

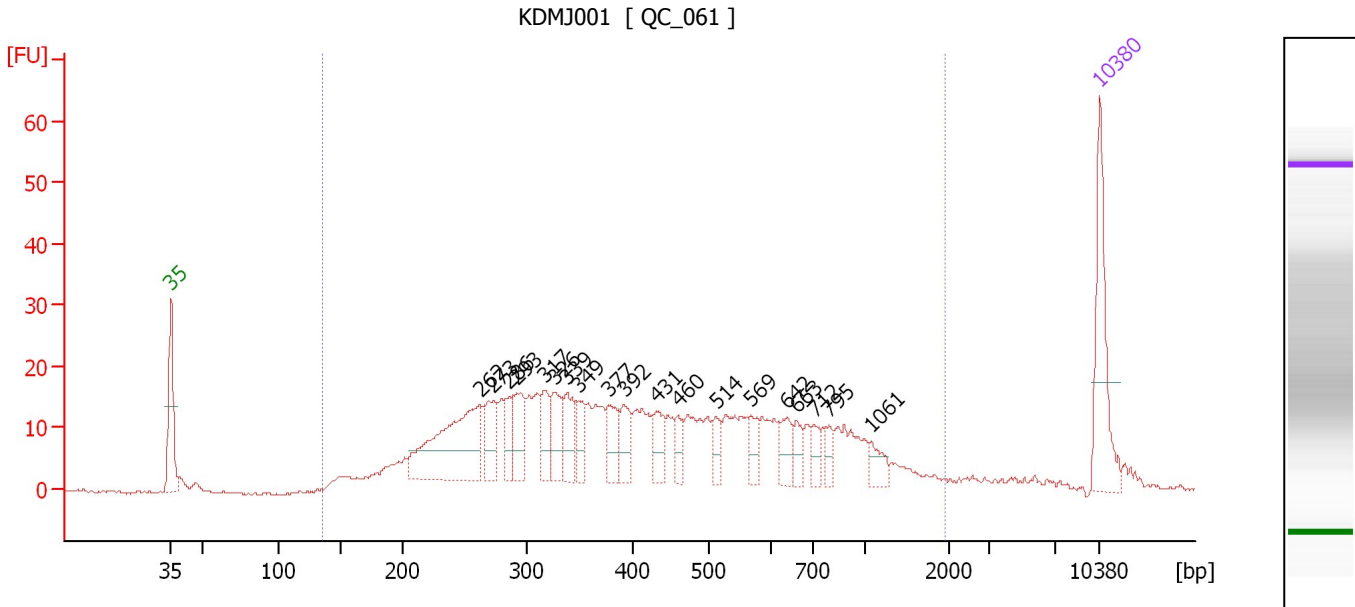

**Overall Results for sample 1 : KDMJ001**

Number of peaks found: 19                      Corr. Area 1: 625.2  
 Noise: 0.2

**Peak table for sample 1 : KDMJ001**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	262	176.62	1,020.0		66.29
3	273	45.27	251.0		67.30
4	286	32.22	170.5		68.50
5	293	47.75	247.3		69.08
6	317	38.88	185.7		71.14
7	326	44.27	205.6		71.87
8	339	41.96	187.7		72.88
9	349	26.60	115.5		73.69
10	377	36.01	144.7		75.96
11	392	30.91	119.4		77.16
12	431	32.42	113.9		79.56
13	460	20.02	65.9		81.20
14	514	17.67	52.1		84.13
15	569	20.60	54.9		86.68
16	642	25.00	59.0		89.47
17	663	16.91	38.7		90.15
18	712	17.36	36.9		91.49
19	795	13.27	25.3		92.60
20	1,061	17.31	24.7		95.73
21	10,380	75.00	10.9	Upper Marker	113.00


**Region table for sample 1 : KDMJ001**

From [bp]	To [bp]	Average Size [bp]	Corr. Area	Molarity [pmol/l]	Co Conc. [pg/μl]	% of Total	Size distribution in CV [%]
136	1,949	485	625.2	6,419.2	1,466.89	94	59.5

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...alyzer\2016-01-14\2016-01-14\_003\_KDMJ001\_KDMJ002\_QC\_061.xad

Created: 1/14/2016 3:08:47 PM  
 Modified: 1/14/2016 4:54:25 PM

**Electropherogram Summary Continued ...**

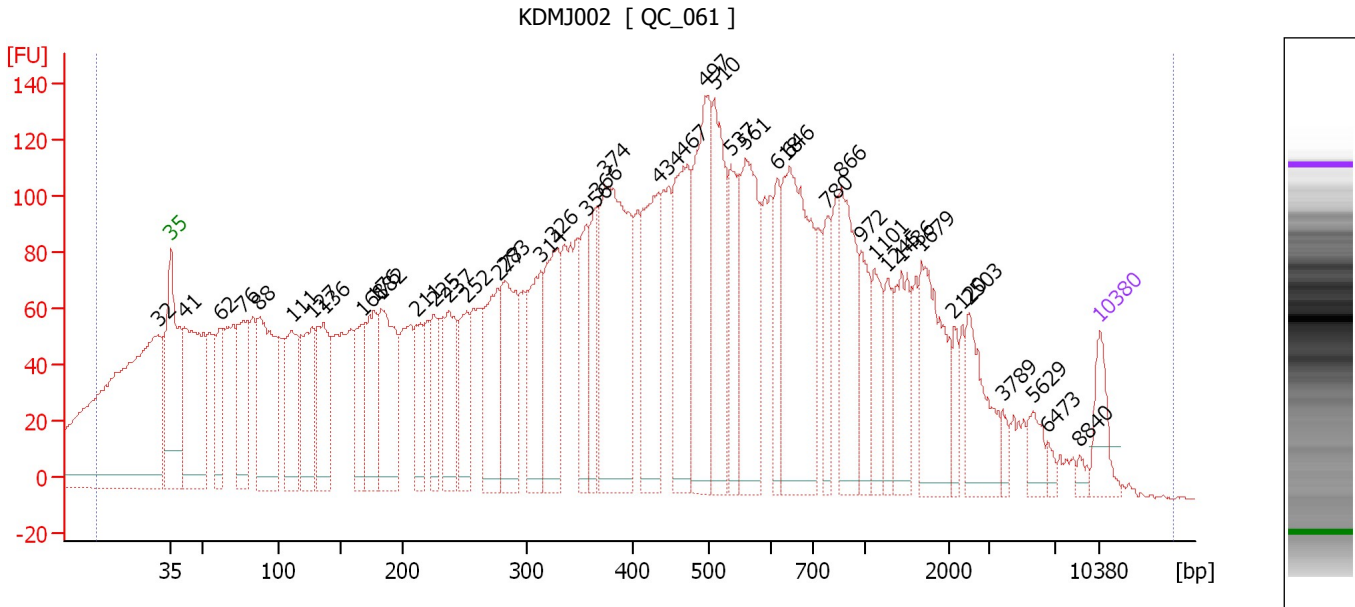

**Overall Results for sample 2 : KDMJ002**

Number of peaks found: 43                      Corr. Area 1: 7,017.2  
 Noise: 0.7

**Peak table for sample 2 : KDMJ002**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	32	0.00	0.0		42.00
2	35	125.00	5,411.3	Lower Marker	43.00
3	41	613.41	22,423.3		44.05
4	62	194.78	4,746.7		46.80
5	76	260.67	5,189.5		48.37
6	88	489.87	8,481.6		49.66
7	111	300.56	4,096.2		52.13
8	127	291.80	3,478.0		53.65
9	136	302.11	3,363.6		54.51
10	168	196.54	1,774.3		57.50
11	176	238.04	2,043.6		58.31
12	182	387.83	3,227.3		58.84
13	211	163.42	1,175.4		61.50
14	225	132.92	894.9		62.83
15	237	221.00	1,410.7		63.97
16	252	175.44	1,055.8		65.30
17	277	261.63	1,431.4		67.63
18	283	312.64	1,673.3		68.20
19	314	250.90	1,211.8		70.87
20	326	292.27	1,360.2		71.82
21	356	179.52	763.2		74.29
22	366	163.02	674.0		75.10
23	374	663.13	2,685.0		75.72
24	434	353.21	1,233.3		79.71
25	467	355.75	1,155.2		81.57

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...alyzer\2016-01-14\2016-01-14\_003\_KDMJ001\_KDMJ002\_QC\_061.xad

Created: 1/14/2016 3:08:47 PM  
 Modified: 1/14/2016 4:54:25 PM

**Electropherogram Summary Continued ...**

**... Peak table for sample 2 : KDMJ002**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
26	497	423.29	1,291.1		83.28
27	510	320.30	951.1		83.94
28	537	175.76	496.2		85.18
29	561	367.61	992.6		86.32
30	618	134.14	329.1		88.70
31	646	513.73	1,205.3		89.60
32	780	106.62	207.0		92.41
33	866	262.50	459.4		93.55
34	972	112.11	174.7		94.98
35	1,101	107.01	147.3		95.98
36	1,245	84.89	103.3		96.88
37	1,436	144.11	152.1		98.07
38	1,679	231.36	208.8		99.59
39	2,120	45.80	32.7		101.97
40	2,503	152.45	92.3		103.16
41	3,789	21.75	8.7		105.68
42	5,629	48.07	12.9		107.96
43	6,473	15.57	3.6		109.01
44	8,840	14.37	2.5		111.48
45	10,380	75.00	10.9	Upper Marker	113.00

**Region table for sample 2 : KDMJ002**

From [bp]	To [bp]	Average Size [bp]	Corr. Area	Molarity [pmol/l]	Co Conc. lor [pg/μl]	% of Total	Size distribution in CV [%]
0	15,980	816	7,017.2	226,728.7	14,280.57	97	100.0

Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...alyzer\2016-01-14\2016-01-14\_003\_KDMJ001\_KDMJ002\_QC\_061.xad

Created: 1/14/2016 3:08:47 PM  
Modified: 1/14/2016 4:54:25 PM

**Gel Image**



Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...alyzer\2016-01-14\2016-01-14\_003\_KDMJ001\_KDMJ002\_QC\_061.xad

Created: 1/14/2016 3:08:47 PM  
 Modified: 1/14/2016 4:54:25 PM

**Run Logbook**

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 12)		Instrument	Run		1/14/2016 3:50:04 PM	(GMT --08:00) Pacific Standard Time	UC Davis	D8XSMGH1
Run started on port 1 (File: C:\Documents and Settings\Bioanalyser\2016-01-14\2016-01-14_003.xad)		Instrument	Run		1/14/2016 3:08:52 PM	(GMT --08:00) Pacific Standard Time	UC Davis	D8XSMGH1
Product Number : G2938B		Instrument	Run		1/14/2016 3:08:52 PM	(GMT --08:00) Pacific Standard Time	UC Davis	D8XSMGH1
Name :		Instrument	Run		1/14/2016 3:08:52 PM	(GMT --08:00) Pacific Standard Time	UC Davis	D8XSMGH1
Vendor : Agilent Technologies		Instrument	Run		1/14/2016 3:08:52 PM	(GMT --08:00) Pacific Standard Time	UC Davis	D8XSMGH1
Serial# : DE13701086		Instrument	Run		1/14/2016 3:08:52 PM	(GMT --08:00) Pacific Standard Time	UC Davis	D8XSMGH1
Firmware : C.01.069		Instrument	Run		1/14/2016 3:08:52 PM	(GMT --08:00) Pacific Standard Time	UC Davis	D8XSMGH1
Cartridge : Electrode		Instrument	Run		1/14/2016 3:08:52 PM	(GMT --08:00) Pacific Standard Time	UC Davis	D8XSMGH1