


Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...0 expert\data\2016-06-23\2016-06-23\_001\_Bird\_Pines\_RTHA.xad

Created: 6/23/2016 9:31:46 AM  
Modified: 6/23/2016 10:13:56 AM

**Electrophoresis File Run Summary**

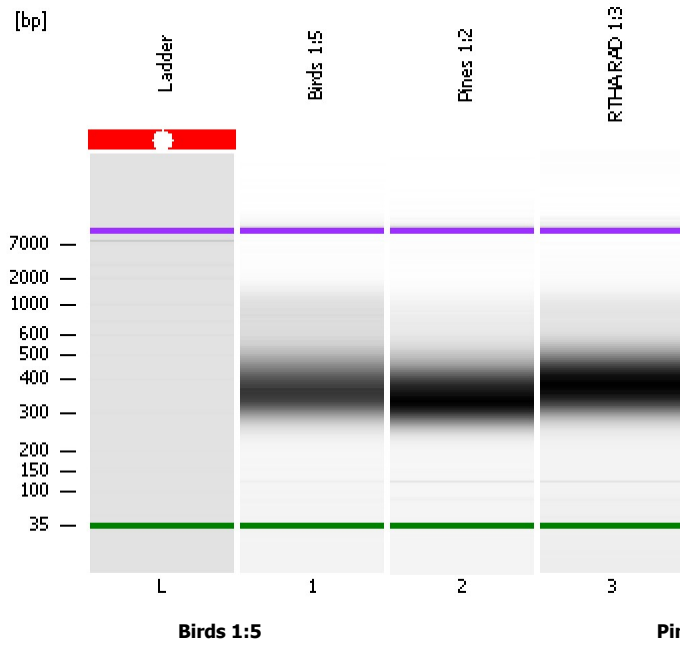

Instrument Information:

Instrument Name: DE13701086      Firmware: C.01.069  
Serial#: DE13701086      Type: G2938B

Assay Information:

Assay Origin Path: C:\Program Files\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy  
Assay Class: High Sensitivity DNA Assay  
Version: 1.03  
Assay Comments: Copyright © 2003-2010 Agilent Technologies

Chip Information:

Chip Lot #:  
Reagent Kit Lot #:  
Chip Comments:

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...0 expert\data\2016-06-23\2016-06-23\_001\_Bird\_Pines\_RTHA.xad

Created: 6/23/2016 9:31:46 AM  
 Modified: 6/23/2016 10:13:56 AM

**Electrophoresis File Run Summary (Chip Summary)**

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
Birds 1:5		<input type="checkbox"/>				
Pines 1:2		<input type="checkbox"/>				
RTHA RAD 1:3		<input type="checkbox"/>				
Ladder		<input type="checkbox"/>				

**Chip Lot #** **Reagent Kit Lot #**

**Chip Comments :**

Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...0 expert\data\2016-06-23\2016-06-23\_001\_Bird\_Pines\_RTHA.xad

Created: 6/23/2016 9:31:46 AM  
Modified: 6/23/2016 10:13:56 AM

**Electrophoresis Assay Details**

**General Analysis Settings**

Number of Available Sample and Ladder Wells (Max.) : 12  
Minimum Visible Range [s] : 32  
Maximum Visible Range [s] : 138  
Start Analysis Time Range [s] : 33  
End Analysis Time Range [s] : 137.5  
Ladder Concentration [pg/μl] : 1950  
Uses Standard Area for Ladder Fragments  
Lower Marker Concentration [pg/μl] : 125  
Upper Marker Concentration [pg/μl] : 75  
Used Upper Marker for Quantitation  
Standard Curve Fit is Point to Point  
Show Data Aligned to Lower and Upper Marker

**Integrator Settings**

Integration Start Time [s] : 33.05  
Integration End Time [s] : 137  
Slope Threshold : 0.8  
Height Threshold [FU] : 5  
Area Threshold : 0.1  
Width Threshold [s] : 0.6  
Baseline Plateau [s] : 0.5

**Filter Settings**

Filter Width [s] : 0.5  
Polynomial Order : 4

**Ladder**

Ladder Peak	Size	Area
1	35	160
2	50	210
3	100	208
4	150	221
5	200	242
6	300	270
7	400	305
8	500	306
9	600	336
10	700	321
11	1000	366
12	2000	413
13	3000	411
14	7000	400
15	10380	214

Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...0 expert\data\2016-06-23\2016-06-23\_001\_Bird\_Pines\_RTHA.xad

Created: 6/23/2016 9:31:46 AM  
Modified: 6/23/2016 10:13:56 AM

**Electropherogram Summary**

Ladder



Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...0 expert\data\2016-06-23\2016-06-23\_001\_Bird\_Pines\_RTHA.xad

Created: 6/23/2016 9:31:46 AM  
Modified: 6/23/2016 10:13:56 AM

**Electropherogram Summary Continued ...**

Birds 1:5



Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...0 expert\data\2016-06-23\2016-06-23\_001\_Bird\_Pines\_RTHA.xad

Created: 6/23/2016 9:31:46 AM  
Modified: 6/23/2016 10:13:56 AM

**Electropherogram Summary Continued ...**

Pines 1:2



Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...0 expert\data\2016-06-23\2016-06-23\_001\_Bird\_Pines\_RTHA.xad

Created: 6/23/2016 9:31:46 AM  
Modified: 6/23/2016 10:13:56 AM

**Electropherogram Summary Continued ...**


RTHA RAD 1:3



Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...0 expert\data\2016-06-23\2016-06-23\_001\_Bird\_Pines\_RTHA.xad

Created: 6/23/2016 9:31:46 AM  
Modified: 6/23/2016 10:13:56 AM

**Gel Image**

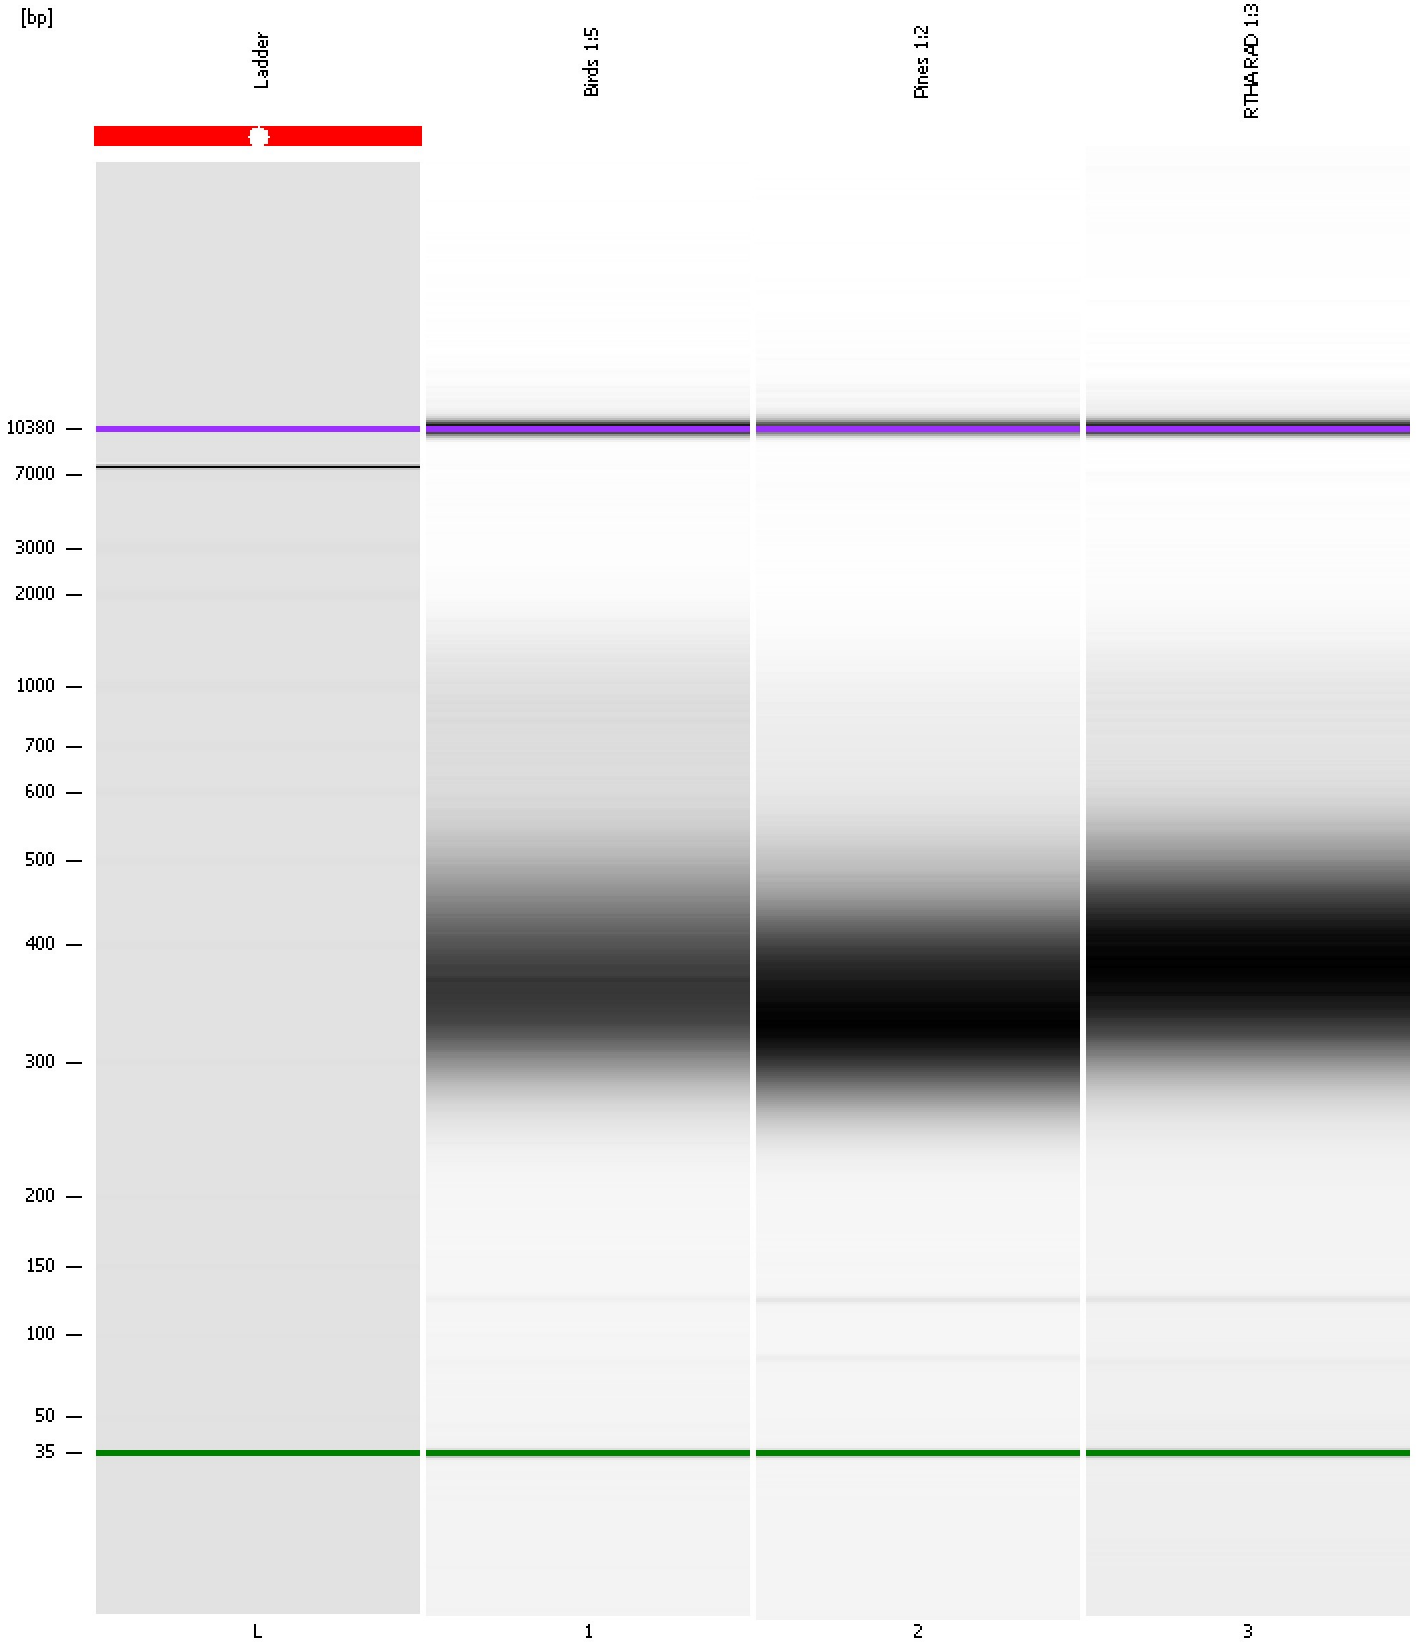



Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...0 expert\data\2016-06-23\2016-06-23\_001\_Bird\_Pines\_RTHA.xad

Created: 6/23/2016 9:31:46 AM  
 Modified: 6/23/2016 10:13:56 AM

**Run Logbook**

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 12)		Instrument	Run		6/23/2016 10:13:03 AM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Instrument error occurred on port 1, Optical signal too high (1605h)	559	Instrument	Run	Ladder	6/23/2016 9:41:44 AM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Run started on port 1 (File: C:\Program Files\Agilent\2100 bioanalyzer\2100 expert\data\2016-06-23\2016-06-23_001.xad)		Instrument	Run		6/23/2016 9:31:51 AM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Product Number : G2938B		Instrument	Run		6/23/2016 9:31:51 AM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Name :		Instrument	Run		6/23/2016 9:31:51 AM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Vendor : Agilent Technologies		Instrument	Run		6/23/2016 9:31:51 AM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Serial# : DE13701086		Instrument	Run		6/23/2016 9:31:51 AM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Firmware : C.01.069		Instrument	Run		6/23/2016 9:31:51 AM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Cartridge : Electrode		Instrument	Run		6/23/2016 9:31:51 AM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1