

Assay Class: Eukaryote Total RNA Pico
Data Path: C:\... bioanalyzer\2100 expert\data\2016-11-29\2016-11-29_003.xad

Created: 11/29/2016 3:32:51 PM
Modified: 11/29/2016 3:44:18 PM

Electrophoresis File Run Summary

Instrument Information:

Instrument Name: DE13701086 Firmware: C.01.069
Serial#: DE13701086 Type: G2938B

Assay Information:




Assay Origin Path: C:\Program Files\Agilent\2100 bioanalyzer\2100 expert\assays\RNA\Eukaryote Total RNA Pico Series II.xsy

Assay Class: Eukaryote Total RNA Pico
Version: 2.6
Assay Comments: Total RNA Analysis pg sensitivity (Eukaryote)

© Copyright 2003 - 2009 Agilent Technologies, Inc.

Chip Information:

Chip Lot #:
Reagent Kit Lot #:
Chip Comments:

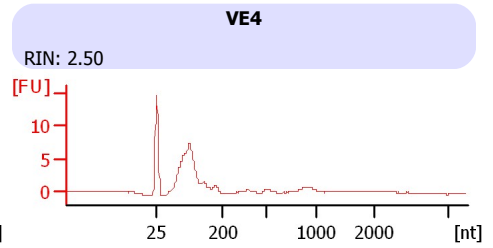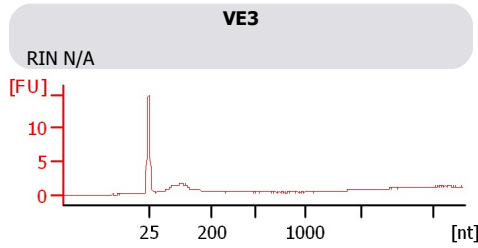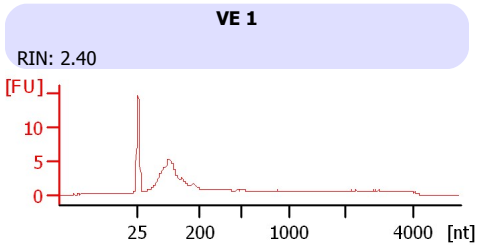

Assay Class: Eukaryote Total RNA Pico
 Data Path: C:\... bioanalyzer\2100 expert\data\2016-11-29\2016-11-29_003.xad

Created: 11/29/2016 3:32:51 PM
 Modified: 11/29/2016 3:44:18 PM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Status	Result Label	Result Color
VE 1		✓	RIN: 2.40	
VE3		✓	RIN N/A	
VE4		✓	RIN: 2.50	
Sample 4				
Sample 5				
Sample 6				
Sample 7				
Sample 8				
Sample 9				
Sample 10				
Sample 11				
Ladder		✓	All Other Samples	

Chip Lot #

Reagent Kit Lot #

Chip Comments :

Assay Class: Eukaryote Total RNA Pico
Data Path: C:\... bioanalyzer\2100 expert\data\2016-11-29\2016-11-29_003.xad

Created: 11/29/2016 3:32:51 PM
Modified: 11/29/2016 3:44:18 PM

Electrophoresis Assay Details

General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12

Minimum Visible Range [s] : 17

Maximum Visible Range [s] : 70

Start Analysis Time Range [s] : 18

End Analysis Time Range [s] : 69

Ladder Concentration [pg/ μ l] : 1000

Lower Marker Concentration [pg/ μ l] : 0

Upper Marker Concentration [pg/ μ l] : 0

Used Lower Marker for Quantitation

Standard Curve Fit is Logarithmic

Show Data Aligned to Lower Marker

Integrator Settings

Integration Start Time [s] : 18

Integration End Time [s] : 69

Slope Threshold : 0.6

Height Threshold [FU] : 0.5

Area Threshold : 0.2

Width Threshold [s] : 0.3

Baseline Plateau [s] : 6

Filter Settings

Filter Width [s] : 0.5

Polynomial Order : 4


Ladder

Ladder Peak	Size
1	25
2	200
3	500
4	1000
5	2000
6	4000

Assay Class: Eukaryote Total RNA Pico
Data Path: C:\... bioanalyzer\2100 expert\data\2016-11-29\2016-11-29_003.xad

Created: 11/29/2016 3:32:51 PM
Modified: 11/29/2016 3:44:18 PM

Electropherogram Summary

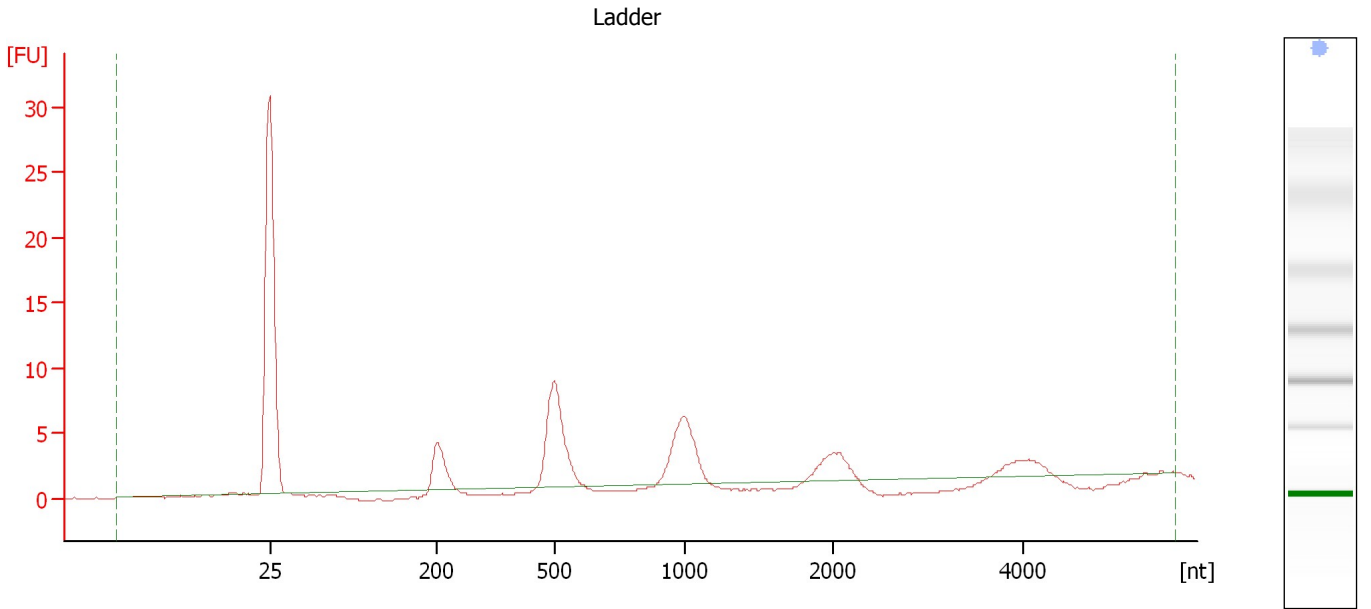


Overall Results for Ladder

RNA Area:	48.3	Result Flagging Color:	
RNA Concentration:	1,000 pg/μl	Result Flagging Label:	All Other Samples

Assay Class: Eukaryote Total RNA Pico
Data Path: C:\... bioanalyzer\2100 expert\data\2016-11-29\2016-11-29_003.xad

Created: 11/29/2016 3:32:51 PM
Modified: 11/29/2016 3:44:18 PM

Electropherogram Summary Continued ...

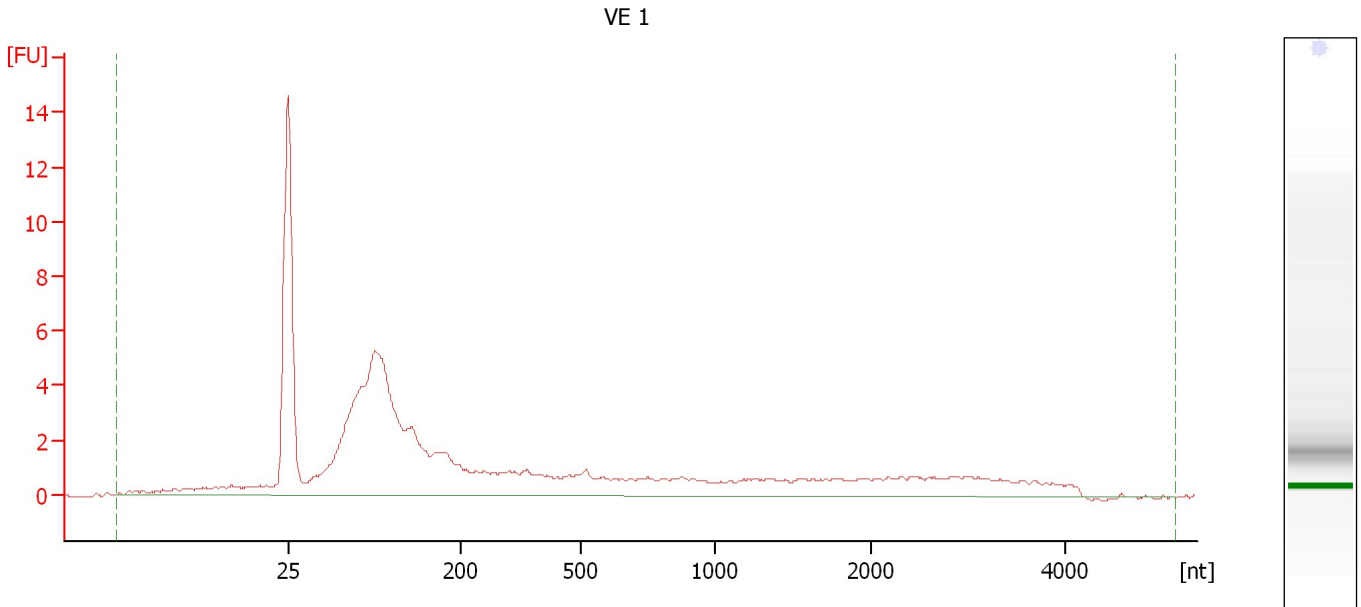


Overall Results for sample 1 : VE 1

RNA Area:	102.0	RNA Integrity Number (RIN):	2.4 (B.02.08)
RNA Concentration:	2,111 pg/μl	Result Flagging Color:	
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN: 2.40


Assay Class: Eukaryote Total RNA Pico
Data Path: C:\... bioanalyzer\2100 expert\data\2016-11-29\2016-11-29_003.xad

Created: 11/29/2016 3:32:51 PM
Modified: 11/29/2016 3:44:18 PM

Electropherogram Summary Continued ...

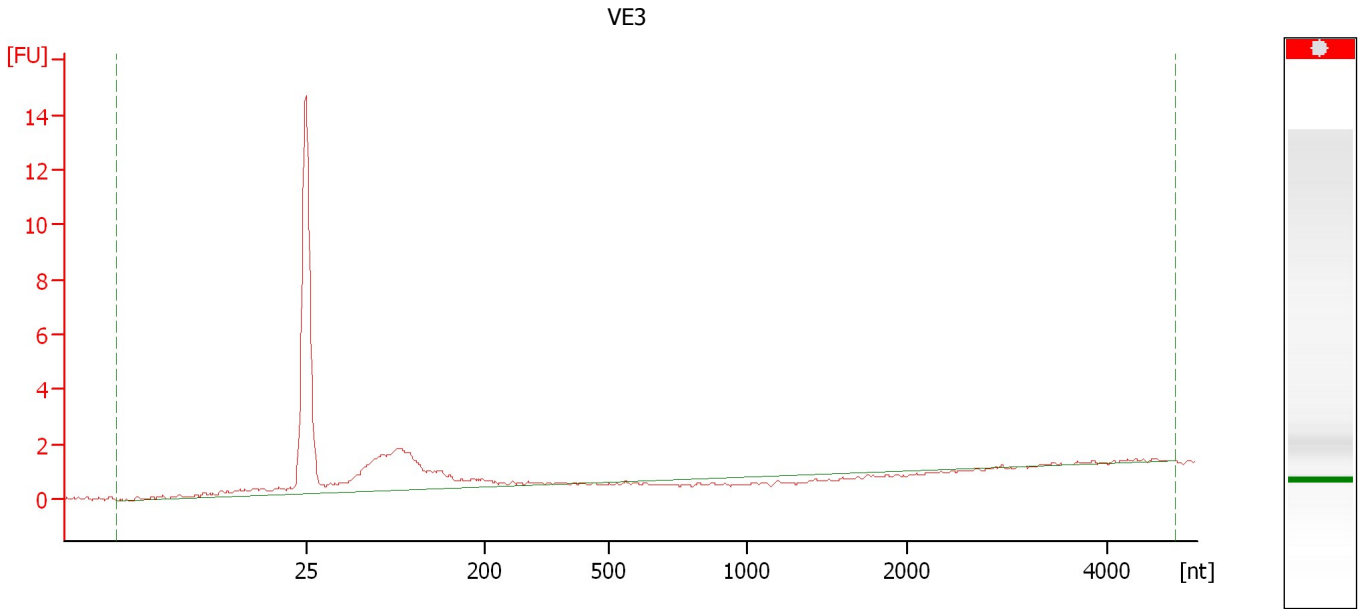


Overall Results for sample 2 : VE3

RNA Area:	21.6	RNA Integrity Number (RIN):	N/A (B.02.08)
RNA Concentration:	446 µg/µl	Result Flagging Color:	
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN N/A

Assay Class: Eukaryote Total RNA Pico
Data Path: C:\... bioanalyzer\2100 expert\data\2016-11-29\2016-11-29_003.xad

Created: 11/29/2016 3:32:51 PM
Modified: 11/29/2016 3:44:18 PM

Electropherogram Summary Continued ...

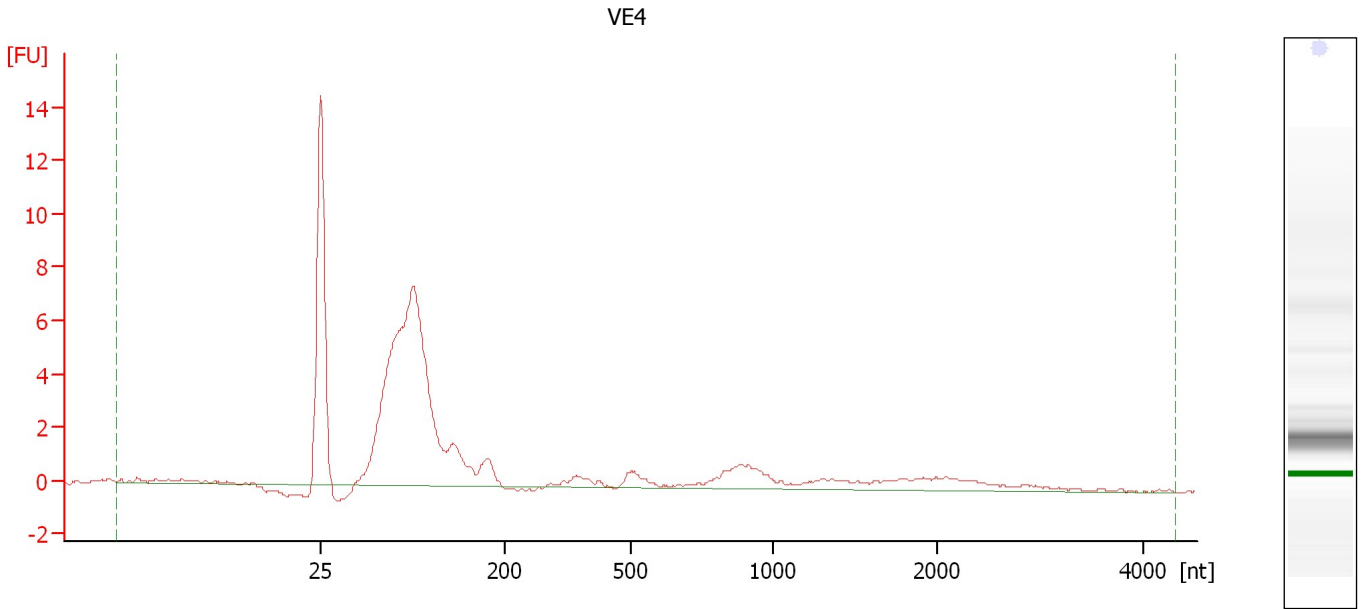

Overall Results for sample 3 : VE4

RNA Area:	67.5	RNA Integrity Number (RIN):	2.5 (B.02.08)
RNA Concentration:	1,397 pg/μl	Result Flagging Color:	
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN: 2.50

Assay Class: Eukaryote Total RNA Pico
Data Path: C:\... bioanalyzer\2100 expert\data\2016-11-29\2016-11-29_003.xad

Created: 11/29/2016 3:32:51 PM
Modified: 11/29/2016 3:44:18 PM

Gel Image

Assay Class: Eukaryote Total RNA Pico
Data Path: C:\... bioanalyzer\2100 expert\data\2016-11-29\2016-11-29_003.xad

Created: 11/29/2016 3:32:51 PM
Modified: 11/29/2016 3:44:18 PM

Invalid Samples

Sample 4 has not been run, no results available.

Sample 5 has not been run, no results available.

Sample 6 has not been run, no results available.

Sample 7 has not been run, no results available.

Sample 8 has not been run, no results available.

Sample 9 has not been run, no results available.

Sample 10 has not been run, no results available.

Sample 11 has not been run, no results available.

Assay Class: Eukaryote Total RNA Pico
 Data Path: C:\... bioanalyzer\2100 expert\data\2016-11-29\2016-11-29_003.xad

Created: 11/29/2016 3:32:51 PM
 Modified: 11/29/2016 3:44:18 PM

Run Logbook

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 4)		Instrument	Run		11/29/2016 3:44:18 PM	(GMT --08:00) Pacific Standard Time	UC Davis	D8XSMGH1
Run started on port 1 (File: C:\Program Files\Agilent\2100 bioanalyzer\2100 expert\data\2016-11-29\2016-11-29_003.xad)		Instrument	Run		11/29/2016 3:32:57 PM	(GMT --08:00) Pacific Standard Time	UC Davis	D8XSMGH1
Product Number : G2938B		Instrument	Run		11/29/2016 3:32:57 PM	(GMT --08:00) Pacific Standard Time	UC Davis	D8XSMGH1
Name :		Instrument	Run		11/29/2016 3:32:57 PM	(GMT --08:00) Pacific Standard Time	UC Davis	D8XSMGH1
Vendor : Agilent Technologies		Instrument	Run		11/29/2016 3:32:57 PM	(GMT --08:00) Pacific Standard Time	UC Davis	D8XSMGH1
Serial# : DE13701086		Instrument	Run		11/29/2016 3:32:57 PM	(GMT --08:00) Pacific Standard Time	UC Davis	D8XSMGH1
Firmware : C.01.069		Instrument	Run		11/29/2016 3:32:57 PM	(GMT --08:00) Pacific Standard Time	UC Davis	D8XSMGH1
Cartridge : Electrode		Instrument	Run		11/29/2016 3:32:57 PM	(GMT --08:00) Pacific Standard Time	UC Davis	D8XSMGH1