

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...\2100 expert\data\2017-06-28\2017-06-28_001_H973P-5-4-3.xad

Created: 6/28/2017 8:09:12 AM
Modified: 6/28/2017 3:09:53 PM

Electrophoresis File Run Summary

Instrument Information:

Instrument Name: DE13701086 Firmware: C.01.069
Serial#: DE13701086 Type: G2938B


Assay Information:

Assay Origin Path: C:\Program Files\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy
Assay Class: High Sensitivity DNA Assay
Version: 1.03
Assay Comments: Copyright © 2003-2010 Agilent Technologies


Chip Information:

Chip Lot #:
Reagent Kit Lot #:
Chip Comments:


H973P-5

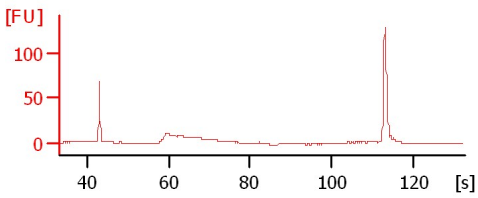

H973P-4

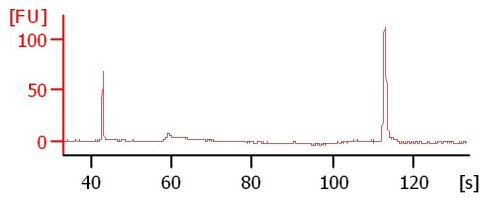

H973P-3

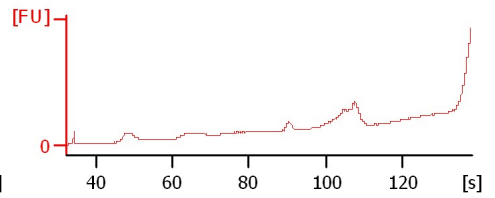

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...\2100 expert\data\2017-06-28\2017-06-28_001_H973P-5-4-3.xad

Created: 6/28/2017 8:09:12 AM
 Modified: 6/28/2017 3:09:53 PM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
H973P-5		<input type="checkbox"/>	✓			
H973P-4		<input type="checkbox"/>	✓			
H973P-3		<input type="checkbox"/>	✓			
Ladder		<input type="checkbox"/>	✓			


Chip Lot # **Reagent Kit Lot #**

Chip Comments :

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...\2100 expert\data\2017-06-28\2017-06-28_001_H973P-5-4-3.xad

Created: 6/28/2017 8:09:12 AM
 Modified: 6/28/2017 3:09:53 PM

Electropherogram Summary

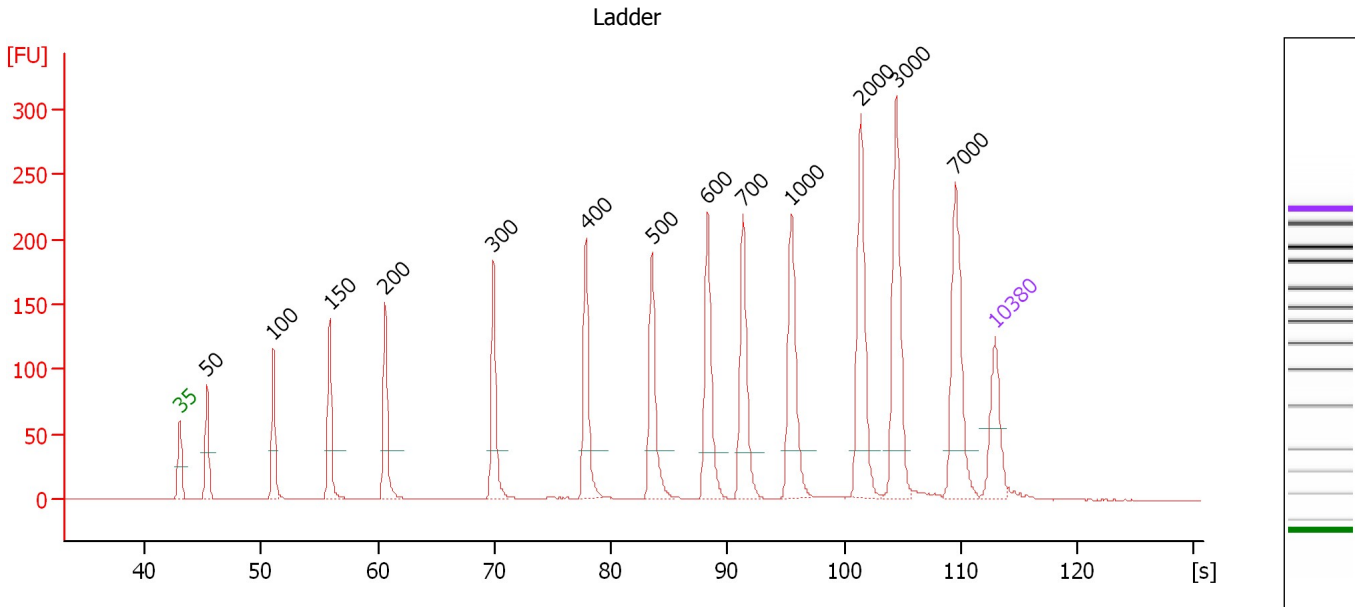

Overall Results for Ladder

Noise: 0.2


Peak table for Ladder

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	50	150.00	4,545.5	Ladder Peak	45.35
3	100	150.00	2,272.7	Ladder Peak	51.02
4	150	150.00	1,515.2	Ladder Peak	55.86
5	200	150.00	1,136.4	Ladder Peak	60.60
6	300	150.00	757.6	Ladder Peak	69.91
7	400	150.00	568.2	Ladder Peak	77.84
8	500	150.00	454.5	Ladder Peak	83.51
9	600	150.00	378.8	Ladder Peak	88.30
10	700	150.00	324.7	Ladder Peak	91.34
11	1,000	150.00	227.3	Ladder Peak	95.49
12	2,000	150.00	113.6	Ladder Peak	101.43
13	3,000	150.00	75.8	Ladder Peak	104.47
14	7,000	150.00	32.5	Ladder Peak	109.54
15	10,380	75.00	10.9	Upper Marker	113.00

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...\2100 expert\data\2017-06-28\2017-06-28_001_H973P-5-4-3.xad

Created: 6/28/2017 8:09:12 AM
 Modified: 6/28/2017 3:09:53 PM

Electropherogram Summary Continued ...

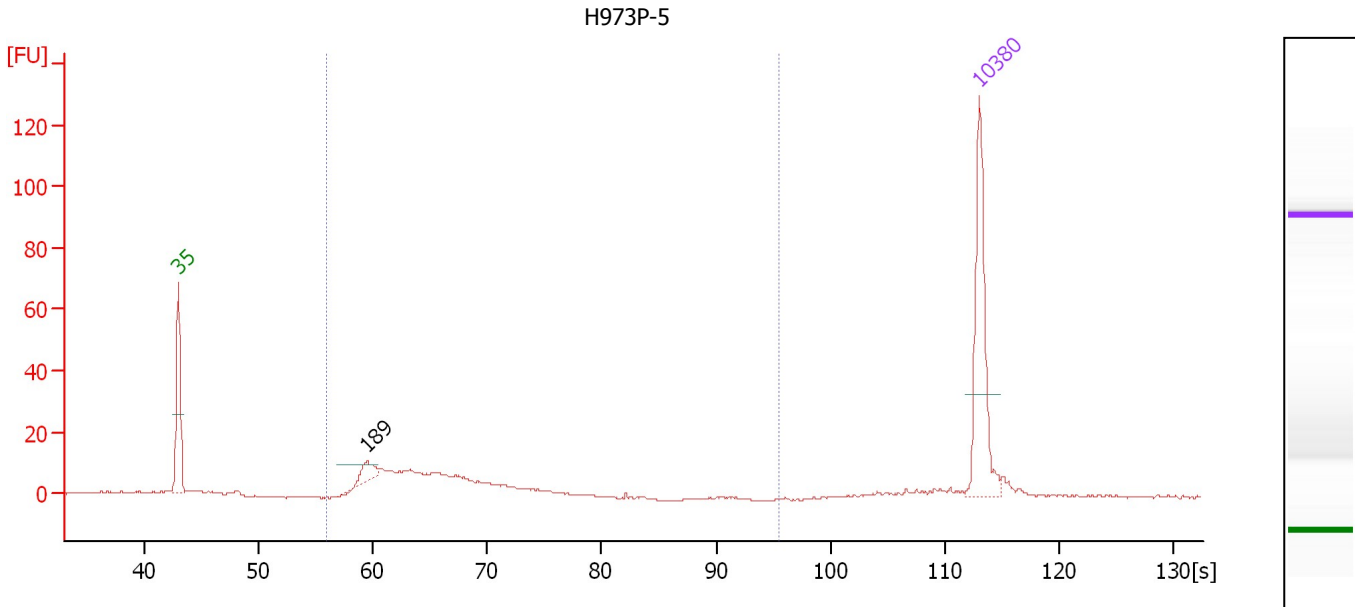

Overall Results for sample 1 : H973P-5

Number of peaks found: 1 Corr. Area 1: 156.6
 Noise: 0.2

Peak table for sample 1 : H973P-5

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	189	17.93	144.1		59.51
3	10,380	75.00	10.9	Upper Marker	113.00


Region table for sample 1 : H973P-5

From [bp]	To [bp]	Average Size [bp]	Corr. Area	Molarity [pmol/l]	Co Conc. lor [pg/μl]	% of Total	Size distribution in CV [%]
151	1,000	249	156.6	1,148.5	179.47	78	20.8

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...\2100 expert\data\2017-06-28\2017-06-28_001_H973P-5-4-3.xad

Created: 6/28/2017 8:09:12 AM
 Modified: 6/28/2017 3:09:53 PM

Electropherogram Summary Continued ...

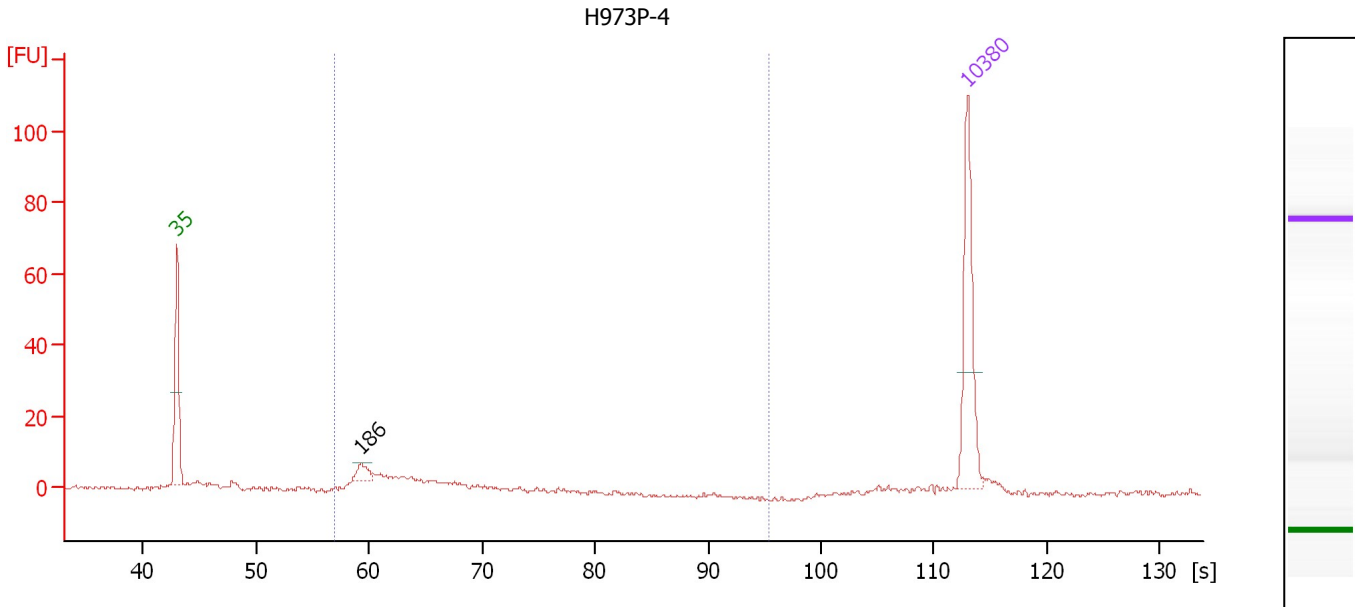

Overall Results for sample 2 : H973P-4

Number of peaks found: 1 Corr. Area 1: 55.2
 Noise: 0.7

Peak table for sample 2 : H973P-4

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	186	16.55	134.9		59.26
3	10,380	75.00	10.9	Upper Marker	113.00


Region table for sample 2 : H973P-4

From [bp]	To [bp]	Average Size [bp]	Corr. Area	Molarity [pmol/l]	Co Conc. lor [pg/μl]	% of Total	Size distribution in CV [%]
162	1,000	223	55.2	576.7	82.66	71	16.8

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...\2100 expert\data\2017-06-28\2017-06-28_001_H973P-5-4-3.xad

Created: 6/28/2017 8:09:12 AM
 Modified: 6/28/2017 3:09:53 PM

Electropherogram Summary Continued ...

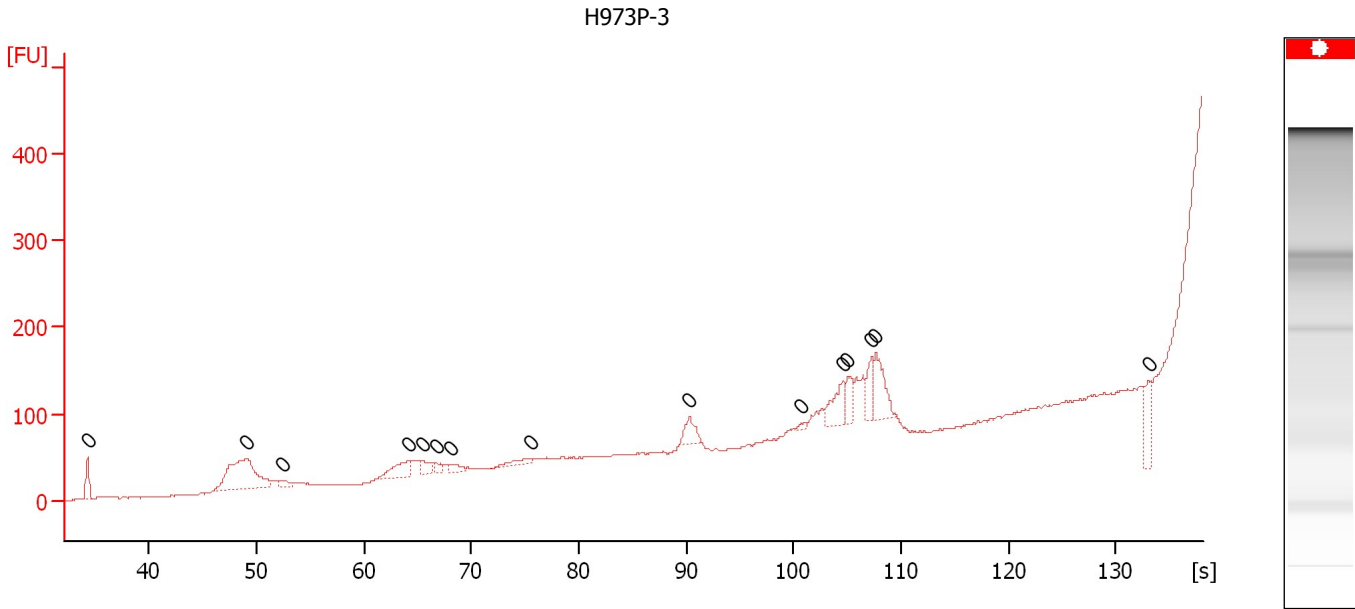

Overall Results for sample 3 : H973P-3

Number of peaks found: 0 Noise: 0.5

Peak table for sample 3 : H973P-3

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	0	0.00	0.0		34.25
2	0	0.00	0.0		49.05
3	0	0.00	0.0		52.40
4	0	0.00	0.0		64.10
5	0	0.00	0.0		65.50
6	0	0.00	0.0		66.70
7	0	0.00	0.0		68.15
8	0	0.00	0.0		75.45
9	0	0.00	0.0		90.30
10	0	0.00	0.0		100.70
11	0	0.00	0.0		104.55
12	0	0.00	0.0		105.05
13	0	0.00	0.0		107.25
14	0	0.00	0.0		107.65
15	0	0.00	0.0		133.05

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...\2100 expert\data\2017-06-28\2017-06-28_001_H973P-5-4-3.xad

Created: 6/28/2017 8:09:12 AM
Modified: 6/28/2017 3:09:53 PM

Gel Image