


Assay Class: mRNA Pico
Data Path: C:\... bioanalyzer\2100 expert\data\2017-07-25\2017-07-25_001.xad

Created: 7/25/2017 8:04:35 AM
Modified: 7/25/2017 8:13:41 AM

Electrophoresis File Run Summary

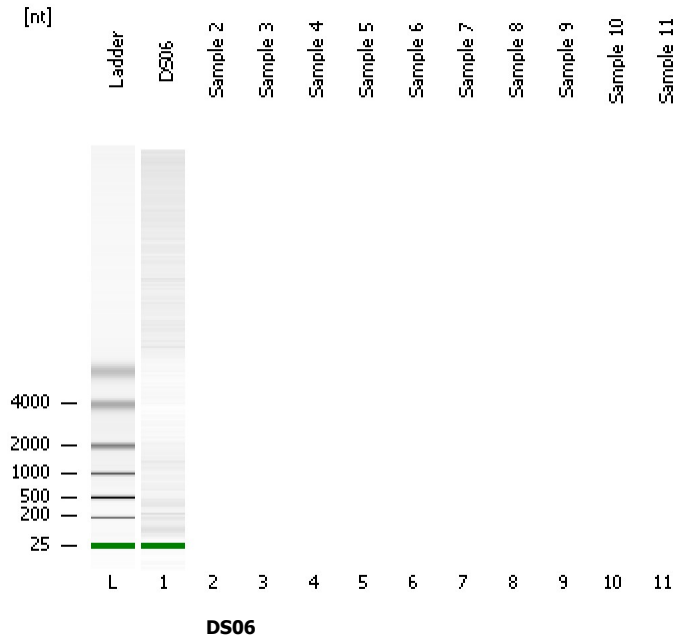

Instrument Information:

Instrument Name: DE13701086 Firmware: C.01.069
Serial#: DE13701086 Type: G2938B

Assay Information:

Assay Origin Path: C:\Program Files\Agilent\2100 bioanalyzer\2100 expert\assays\RNA\mRNA Pico Series II.xsy

Assay Class: mRNA Pico

Version: 2.6

Assay Comments: mRNA Analysis pg sensitivity


© Copyright 2003 - 2009 Agilent Technologies, Inc.

Chip Information:

Chip Lot #:

Reagent Kit Lot #:

Chip Comments:

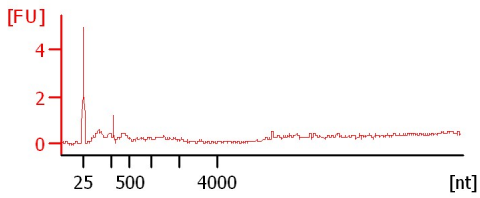

Assay Class: mRNA Pico
Data Path: C:\... bioanalyzer\2100 expert\data\2017-07-25\2017-07-25_001.xad

Created: 7/25/2017 8:04:35 AM
Modified: 7/25/2017 8:13:41 AM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Status	Result Label	Result Color
DS06		✓		
Sample 2				
Sample 3				
Sample 4				
Sample 5				
Sample 6				
Sample 7				
Sample 8				
Sample 9				
Sample 10				
Sample 11				
Ladder		✓		

Chip Lot #


Reagent Kit Lot #

Chip Comments :

Assay Class: mRNA Pico
Data Path: C:\... bioanalyzer\2100 expert\data\2017-07-25\2017-07-25_001.xad

Created: 7/25/2017 8:04:35 AM
Modified: 7/25/2017 8:13:41 AM

Electropherogram Summary

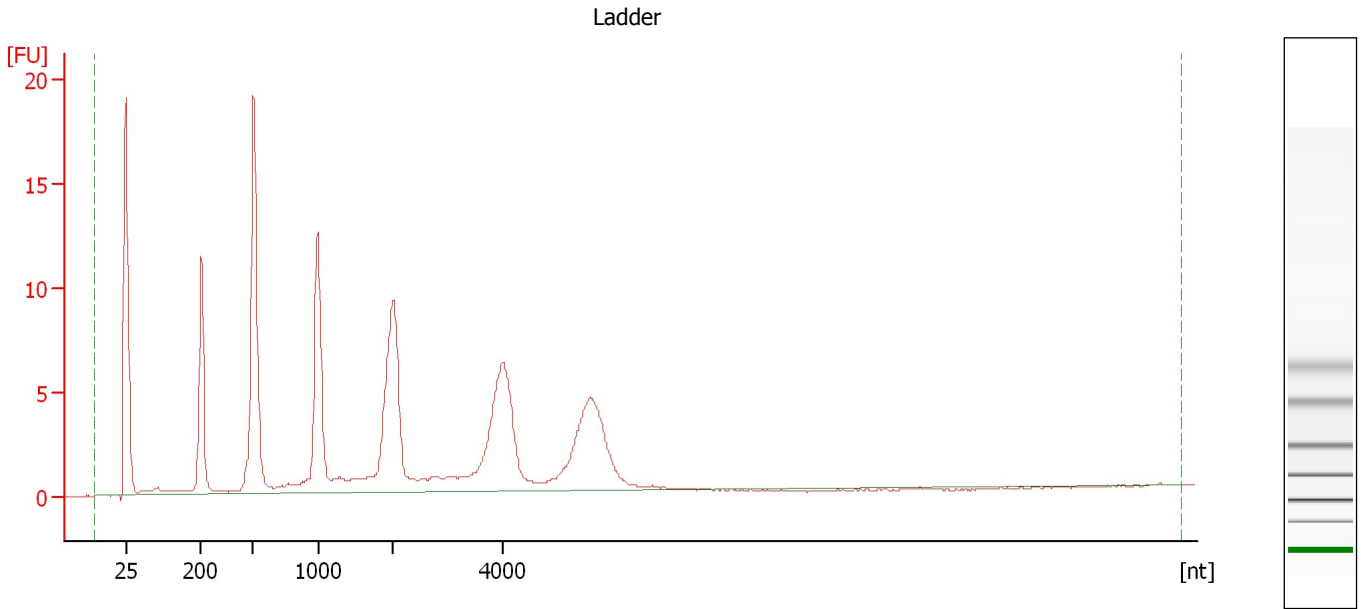

Overall Results for Ladder


RNA Area: 167.8 RNA Concentration: 1,000 pg/μl

Assay Class: mRNA Pico
Data Path: C:\... bioanalyzer\2100 expert\data\2017-07-25\2017-07-25_001.xad

Created: 7/25/2017 8:04:35 AM
Modified: 7/25/2017 8:13:41 AM

Electropherogram Summary Continued ...

DS06

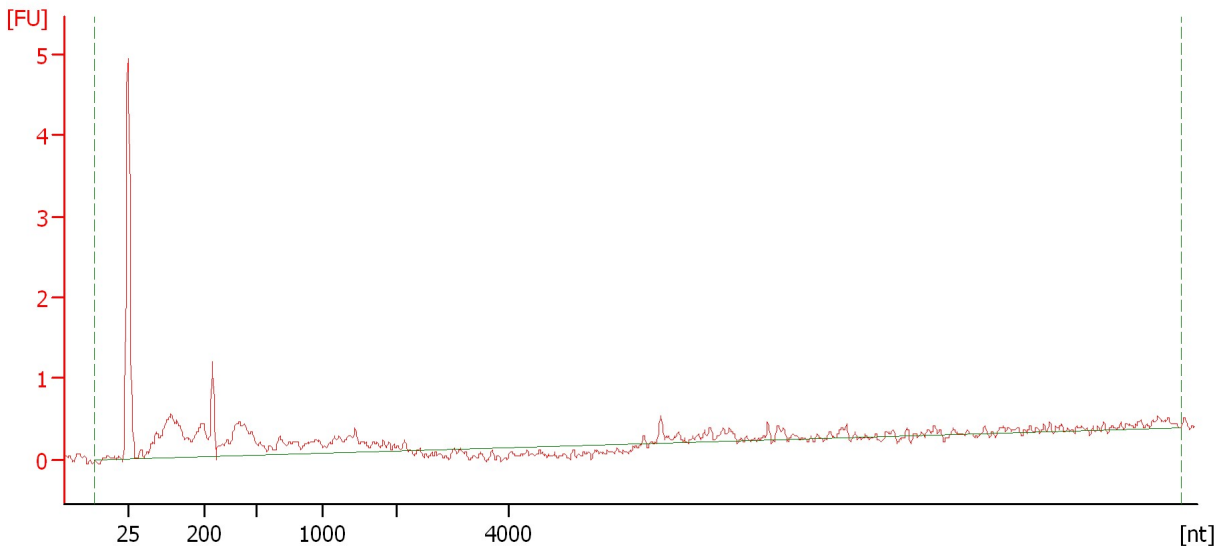


Overall Results for sample 1 : DS06

RNA Area:	15.9	rRNA Contamination:	0.0 %
RNA Concentration:	95 pg/μl		

Assay Class: mRNA Pico
Data Path: C:\... bioanalyzer\2100 expert\data\2017-07-25\2017-07-25_001.xad

Created: 7/25/2017 8:04:35 AM
Modified: 7/25/2017 8:13:41 AM

Gel Image

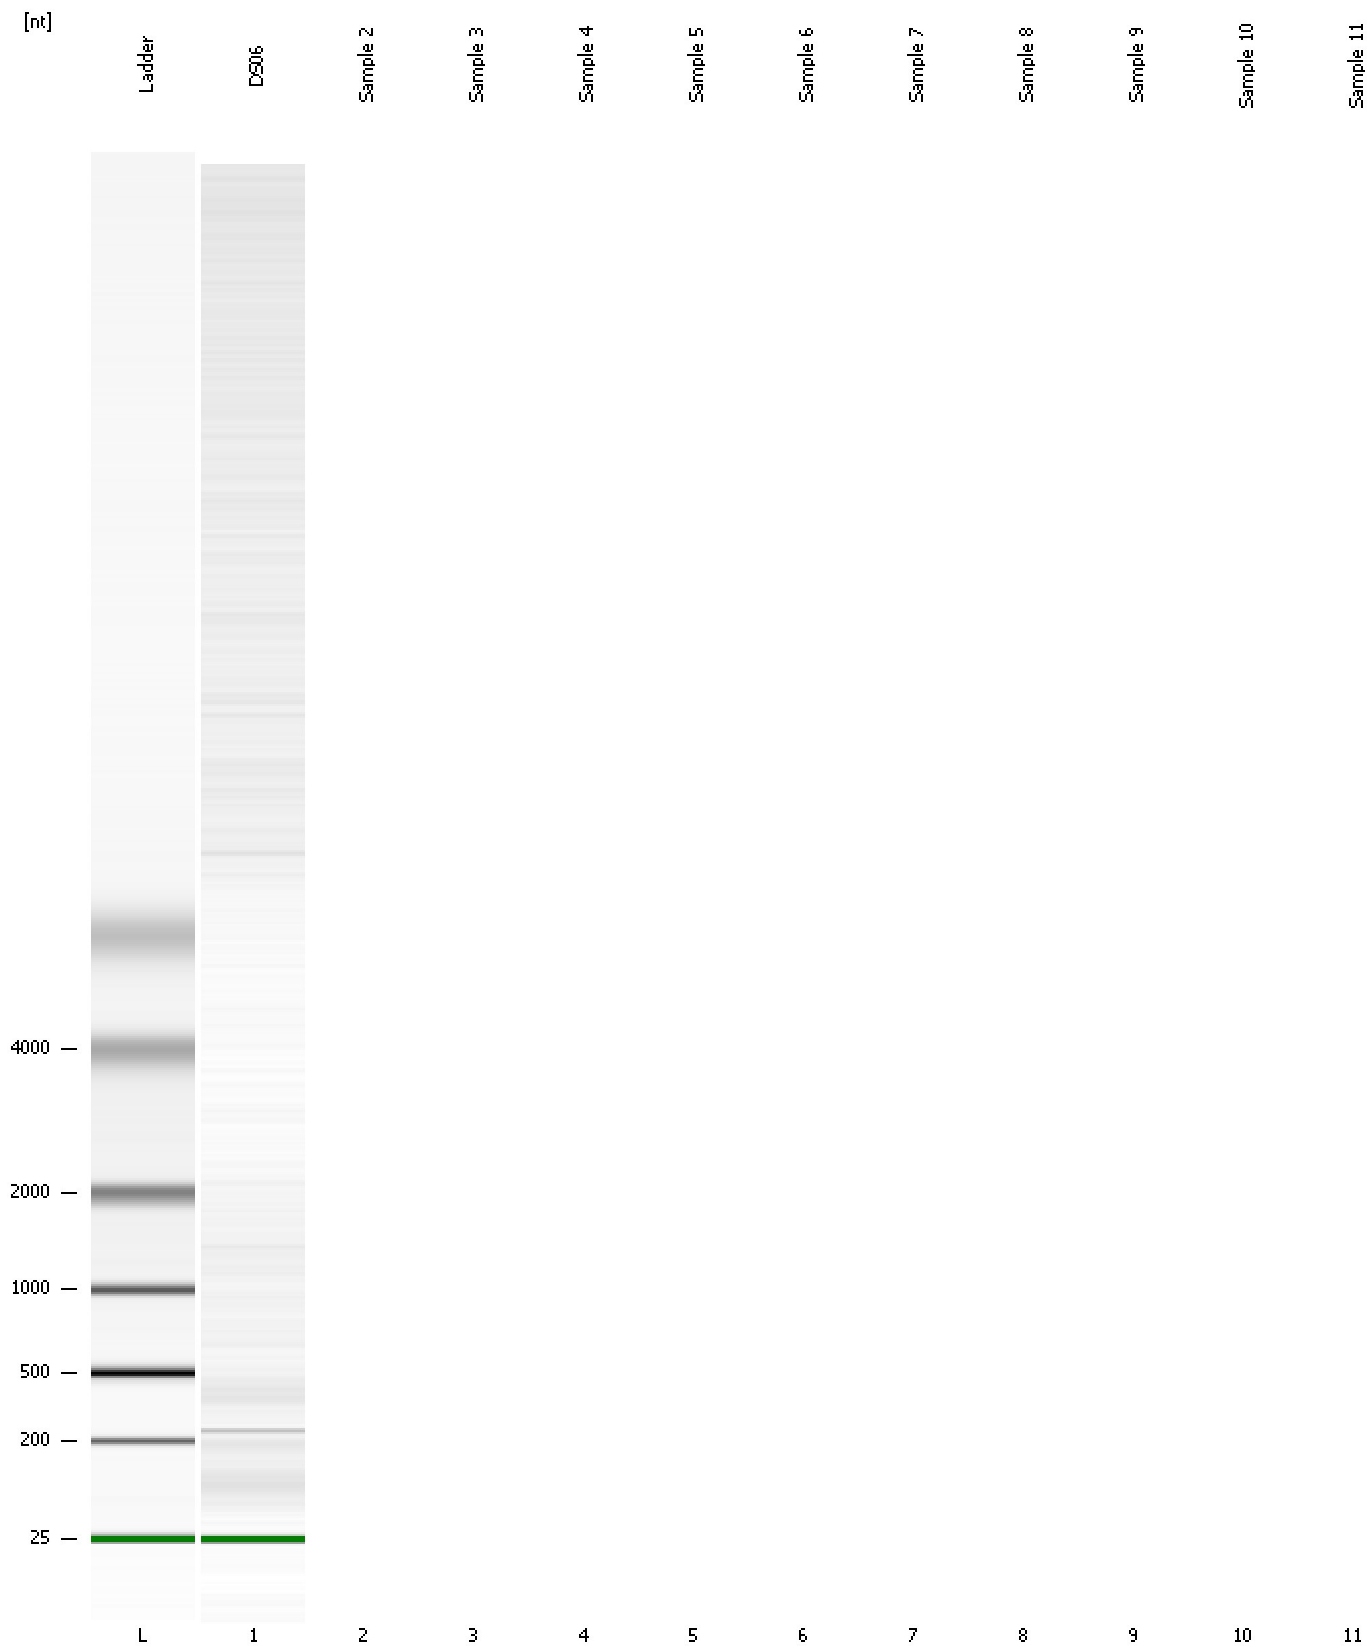


Assay Class: mRNA Pico
Data Path: C:\... bioanalyzer\2100 expert\data\2017-07-25\2017-07-25_001.xad

Created: 7/25/2017 8:04:35 AM
Modified: 7/25/2017 8:13:41 AM

Curves

Standard Curve

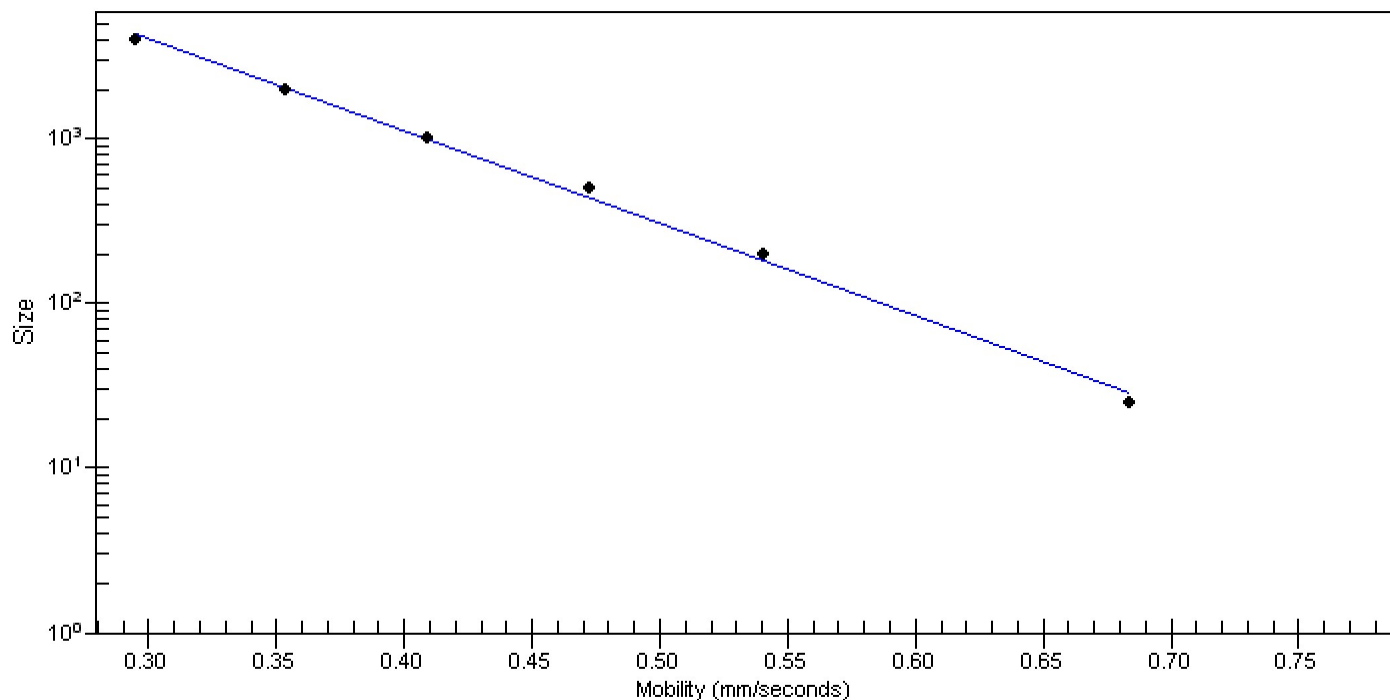

Assay Class: mRNA Pico
Data Path: C:\... bioanalyzer\2100 expert\data\2017-07-25\2017-07-25_001.xad

Created: 7/25/2017 8:04:35 AM
Modified: 7/25/2017 8:13:41 AM

Invalid Samples

Sample 2 has not been run, no results available.

Sample 3 has not been run, no results available.

Sample 4 has not been run, no results available.

Sample 5 has not been run, no results available.

Sample 6 has not been run, no results available.

Sample 7 has not been run, no results available.

Sample 8 has not been run, no results available.

Sample 9 has not been run, no results available.

Sample 10 has not been run, no results available.

Sample 11 has not been run, no results available.