

Assay Class: High Sensitivity DNA Assay
Data Path: C:\... bioanalyzer\2100 expert\data\2018-01-19\2018-01-19_004.xad

Created: 1/19/2018 12:58:53 PM
Modified: 1/19/2018 1:23:53 PM

Electrophoresis File Run Summary

Instrument Information:

Instrument Name: DE13701086 Firmware: C.01.069
Serial#: DE13701086 Type: G2938B


Assay Information:

Assay Origin Path: C:\Program Files\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy
Assay Class: High Sensitivity DNA Assay
Version: 1.03
Assay Comments: Copyright © 2003-2010 Agilent Technologies


Chip Information:

Chip Lot #:
Reagent Kit Lot #:
Chip Comments:


ATAC_1

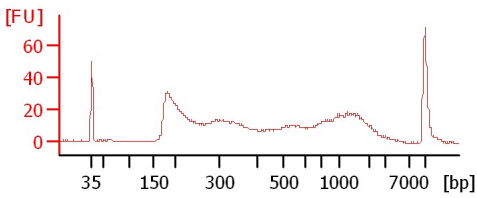


ATAC_2

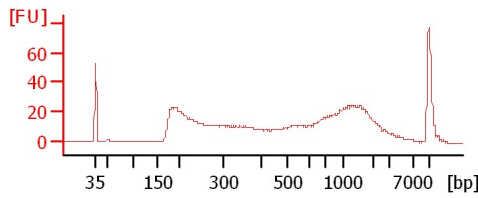


ATAC_3

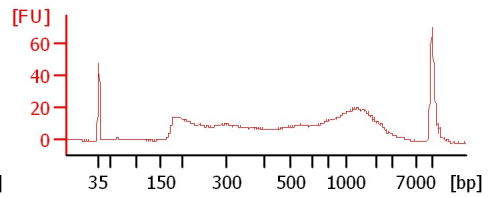

H1269P_SanzA

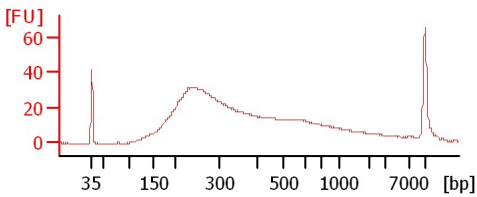

H1269P_SanzB

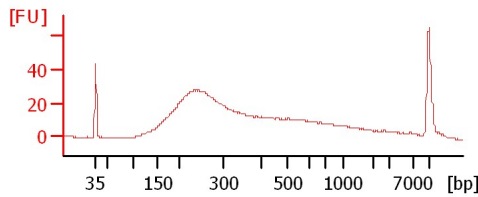

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\... bioanalyzer\2100 expert\data\2018-01-19\2018-01-19_004.xad

Created: 1/19/2018 12:58:53 PM
 Modified: 1/19/2018 1:23:53 PM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
ATAC_1		<input type="checkbox"/>	✓			
ATAC_2		<input type="checkbox"/>	✓			
ATAC_3		<input type="checkbox"/>	✓			
H1269P_SanzA		<input type="checkbox"/>	✓			
H1269P_SanzB		<input type="checkbox"/>	✓			
sample 6		<input type="checkbox"/>				
sample 7		<input type="checkbox"/>				
sample 8		<input type="checkbox"/>				
sample 9		<input type="checkbox"/>				
sample 10		<input type="checkbox"/>				
sample 11		<input type="checkbox"/>				
Ladder		<input type="checkbox"/>	✓			

Chip Lot #


Reagent Kit Lot #

Chip Comments :

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\... bioanalyzer\2100 expert\data\2018-01-19\2018-01-19_004.xad

Created: 1/19/2018 12:58:53 PM
 Modified: 1/19/2018 1:23:53 PM

Electropherogram Summary

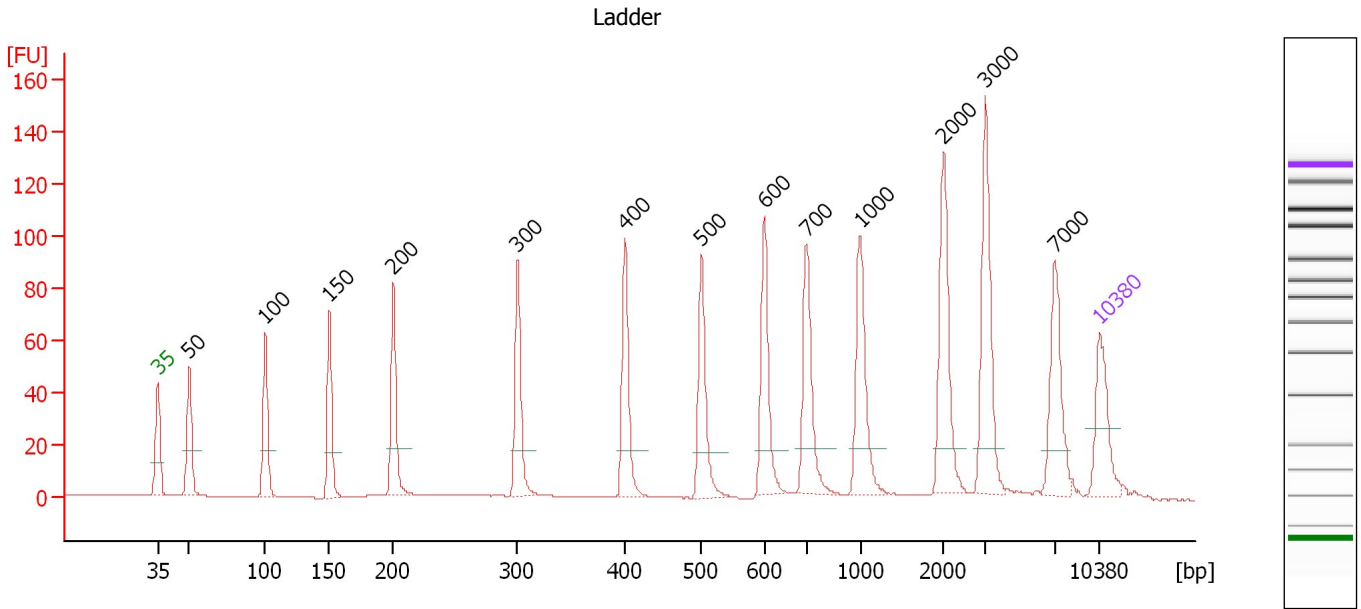

Overall Results for Ladder

Noise: 0.2


Peak table for Ladder

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	50	150.00	4,545.5	Ladder Peak	45.34
3	100	150.00	2,272.7	Ladder Peak	50.98
4	150	150.00	1,515.2	Ladder Peak	55.77
5	200	150.00	1,136.4	Ladder Peak	60.50
6	300	150.00	757.6	Ladder Peak	69.73
7	400	150.00	568.2	Ladder Peak	77.71
8	500	150.00	454.5	Ladder Peak	83.40
9	600	150.00	378.8	Ladder Peak	88.04
10	700	150.00	324.7	Ladder Peak	91.20
11	1,000	150.00	227.3	Ladder Peak	95.21
12	2,000	150.00	113.6	Ladder Peak	101.38
13	3,000	150.00	75.8	Ladder Peak	104.49
14	7,000	150.00	32.5	Ladder Peak	109.65
15	10,380	75.00	10.9	Upper Marker	113.00

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\... bioanalyzer\2100 expert\data\2018-01-19\2018-01-19_004.xad

Created: 1/19/2018 12:58:53 PM
 Modified: 1/19/2018 1:23:53 PM

Electropherogram Summary Continued ...

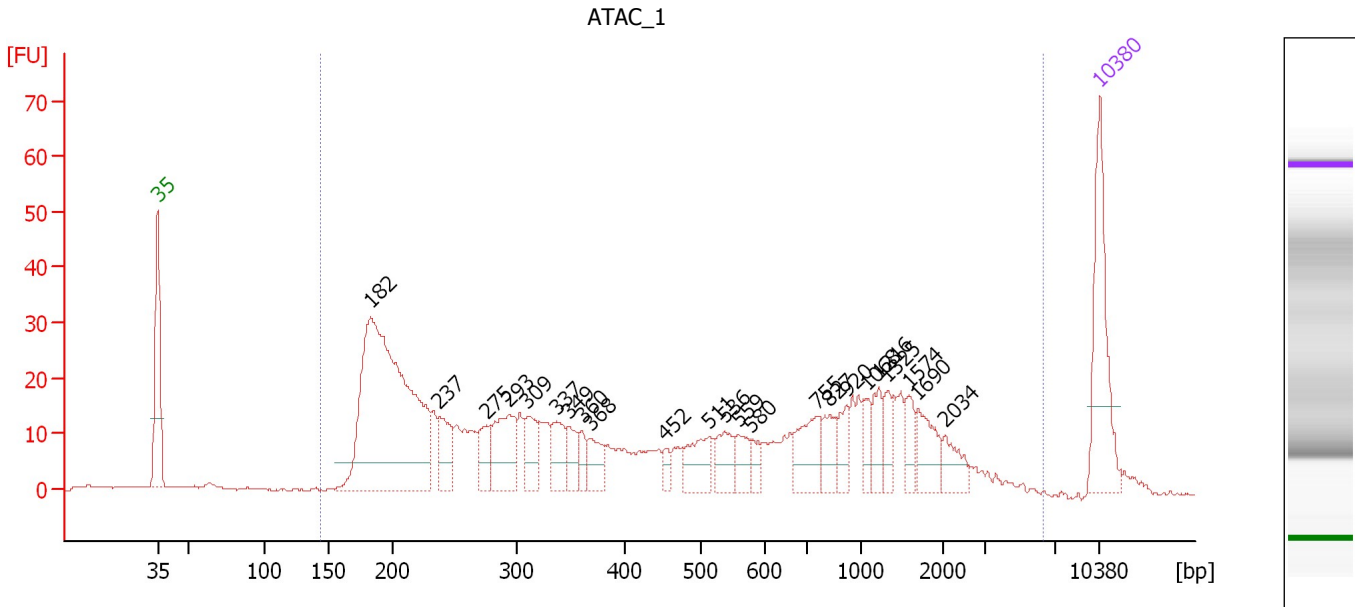

Overall Results for sample 1 : ATAC 1

Number of peaks found: 23 Corr. Area 1: 820.7
 Noise: 0.2

Peak table for sample 1 : ATAC 1

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	182	458.17	3,806.1		58.83
3	237	42.96	274.6		63.92
4	275	29.59	163.0		67.42
5	293	64.19	331.7		69.10
6	309	36.05	176.8		70.44
7	337	33.95	152.5		72.70
8	349	24.12	104.8		73.61
9	360	14.71	61.9		74.52
10	368	25.42	104.7		75.15
11	452	9.59	32.2		80.66
12	511	37.15	110.1		83.93
13	536	27.42	77.5		85.08
14	559	20.48	55.5		86.13
15	580	12.09	31.6		87.09
16	755	42.18	84.6		91.94
17	827	23.68	43.4		92.90
18	920	18.96	31.2		94.14
19	1,068	14.73	20.9		95.63
20	1,216	20.82	25.9		96.54
21	1,325	16.05	18.4		97.22
22	1,574	17.37	16.7		98.75
23	1,690	29.37	26.3		99.47
24	2,034	18.79	14.0		101.49
25	10,380	75.00	10.9	Upper Marker	113.00


Assay Class: High Sensitivity DNA Assay
Data Path: C:\... bioanalyzer\2100 expert\data\2018-01-19\2018-01-19_004.xad

Created: 1/19/2018 12:58:53 PM
Modified: 1/19/2018 1:23:53 PM

Electropherogram Summary Continued ...

... Region table for sample 1 :


ATAC 1

From [bp]	To [bp]	Average Size [bp]	Corr. Area	Conc. [pg/μl]	Molarity [pmol/l]	Co % of lor Total	Size distribution in CV [%]
142	6,275	713	820.7	1,380.61	6,643.6	 97	100.0

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\... bioanalyzer\2100 expert\data\2018-01-19\2018-01-19_004.xad

Created: 1/19/2018 12:58:53 PM
 Modified: 1/19/2018 1:23:53 PM

Electropherogram Summary Continued ...

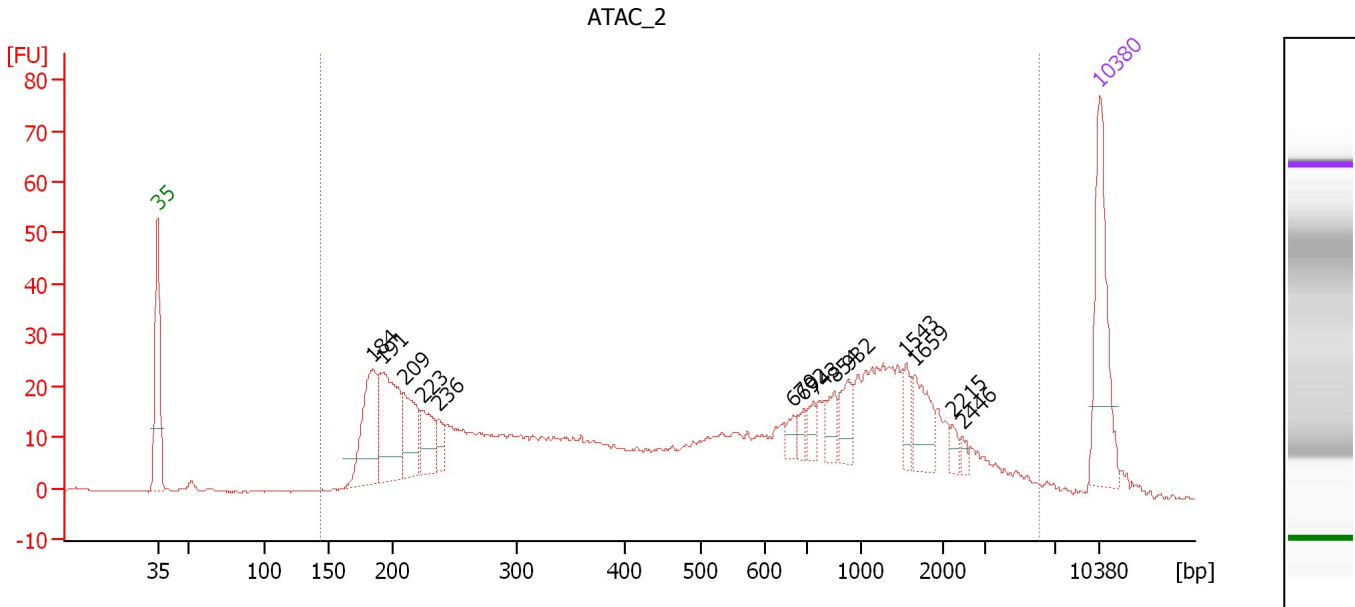

Overall Results for sample 2 : ATAC_2

Number of peaks found: 14 Corr. Area 1: 864.5
 Noise: 0.1

Peak table for sample 2 : ATAC_2

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	184	97.92	807.1		58.97
3	191	113.14	895.6		59.69
4	209	57.47	417.0		61.31
5	223	37.94	257.4		62.65
6	236	17.45	111.9		63.85
7	670	10.09	22.8		90.24
8	692	9.22	20.2		90.96
9	743	11.22	22.9		91.77
10	854	15.91	28.2		93.25
11	932	22.91	37.2		94.30
12	1,543	15.53	15.3		98.56
13	1,659	31.66	28.9		99.28
14	2,215	6.25	4.3		102.05
15	2,446	4.43	2.7		102.77
16	10,380	75.00	10.9	Upper Marker	113.00


Region table for sample 2 : ATAC_2

From [bp]	To [bp]	Average Size [bp]	Corr. Area	Conc. [pg/μl]	Molarity [pmol/l]	Co % of Ior Total	Size distribution in CV [%]
143	6,139	850	864.5	1,310.74	5,665.4	99	98.9

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\... bioanalyzer\2100 expert\data\2018-01-19\2018-01-19_004.xad

Created: 1/19/2018 12:58:53 PM
 Modified: 1/19/2018 1:23:53 PM

Electropherogram Summary Continued ...

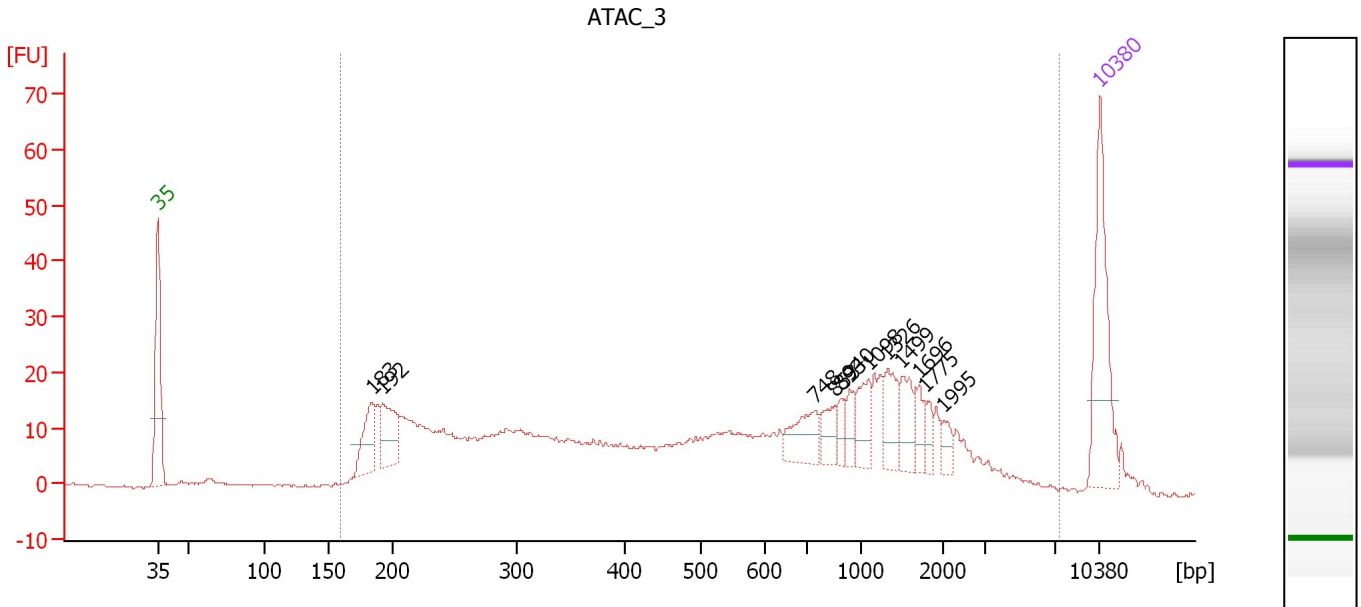

Overall Results for sample 3 : ATAC 3

Number of peaks found: 12 Corr. Area 1: 680.9
 Noise: 0.2

Peak table for sample 3 : ATAC 3

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	183	44.33	366.4		58.92
3	192	52.05	411.7		59.70
4	748	34.62	70.1		91.83
5	853	18.53	32.9		93.24
6	893	12.33	20.9		93.78
7	940	12.70	20.5		94.41
8	1,098	25.01	34.5		95.82
9	1,326	25.31	28.9		97.22
10	1,499	25.26	25.5		98.29
11	1,696	12.75	11.4		99.50
12	1,775	10.64	9.1		99.99
13	1,995	9.16	7.0		101.35
14	10,380	75.00	10.9	Upper Marker	113.00

Region table for sample 3 : ATAC 3

From [bp]	To [bp]	Average Size [bp]	Corr. Area	Conc. [pg/μl]	Molarity [pmol/l]	Co % of lor Total	Size distribution in CV [%]
159	7,279	857	680.9	1,137.96	4,678.1	98	97.6

Assay Class: High Sensitivity DNA Assay
Data Path: C:\... bioanalyzer\2100 expert\data\2018-01-19\2018-01-19_004.xad

Created: 1/19/2018 12:58:53 PM
Modified: 1/19/2018 1:23:53 PM

Gel Image