


Assay Class: High Sensitivity DNA Assay
 Data Path: C:\... bioanalyzer\2100 expert\data\2018-02-06\2018-02-06_001.xad

Created: 2/6/2018 10:26:32 AM
 Modified: 2/6/2018 10:50:37 AM

Electrophoresis File Run Summary

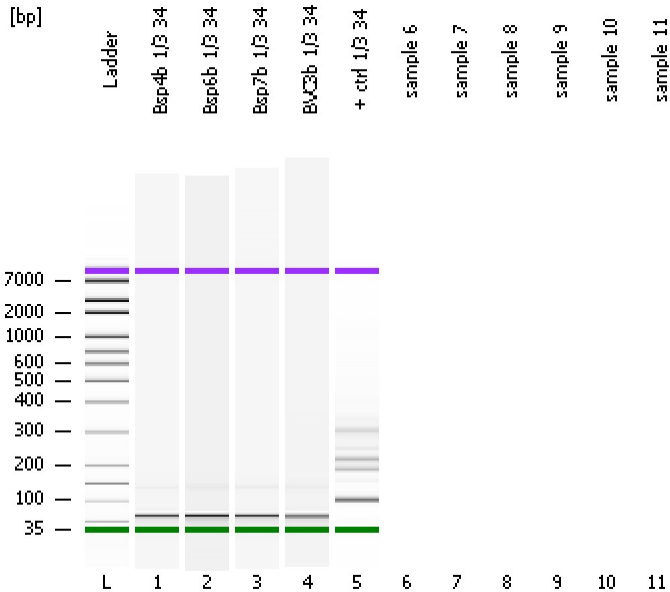

Instrument Information:

Instrument Name: DE34903152 Firmware: C.01.069
 Serial#: DE34903152 Type: G2938C

Assay Information:

Assay Origin Path: C:\Program Files\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy
 Assay Class: High Sensitivity DNA Assay
 Version: 1.03
 Assay Comments: Copyright © 2003-2010 Agilent Technologies




Chip Information:

Chip Lot #:
 Reagent Kit Lot #:
 Chip Comments:

Bsp4b 1/3 34



Bsp6b 1/3 34

Bsp7b 1/3 34

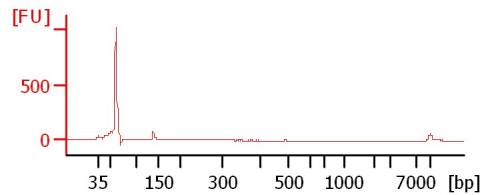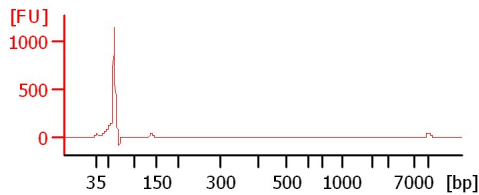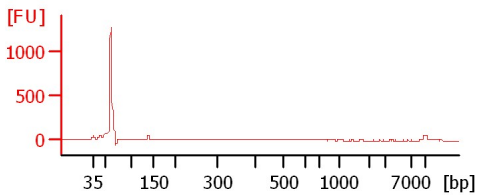

BVC3b 1/3 34

+ ctrl 1/3 34

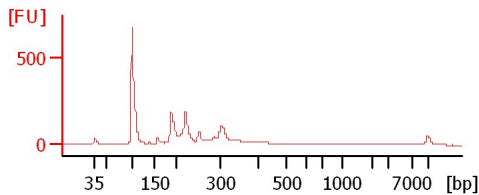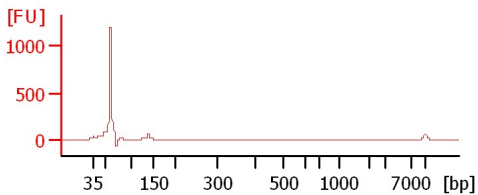

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\... bioanalyzer\2100 expert\data\2018-02-06\2018-02-06_001.xad

Created: 2/6/2018 10:26:32 AM
 Modified: 2/6/2018 10:50:37 AM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
Bsp4b 1/3 34		<input type="checkbox"/>	✓			
Bsp6b 1/3 34		<input type="checkbox"/>	✓			
Bsp7b 1/3 34		<input type="checkbox"/>	✓			
BVC3b 1/3 34		<input type="checkbox"/>	✓			
+ ctrl 1/3 34		<input type="checkbox"/>	✓			
sample 6		<input type="checkbox"/>				
sample 7		<input type="checkbox"/>				
sample 8		<input type="checkbox"/>				
sample 9		<input type="checkbox"/>				
sample 10		<input type="checkbox"/>				
sample 11		<input type="checkbox"/>				
Ladder		<input type="checkbox"/>	✓			

Chip Lot #


Reagent Kit Lot #

Chip Comments :

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\... bioanalyzer\2100 expert\data\2018-02-06\2018-02-06_001.xad

Created: 2/6/2018 10:26:32 AM
 Modified: 2/6/2018 10:50:37 AM

Electropherogram Summary

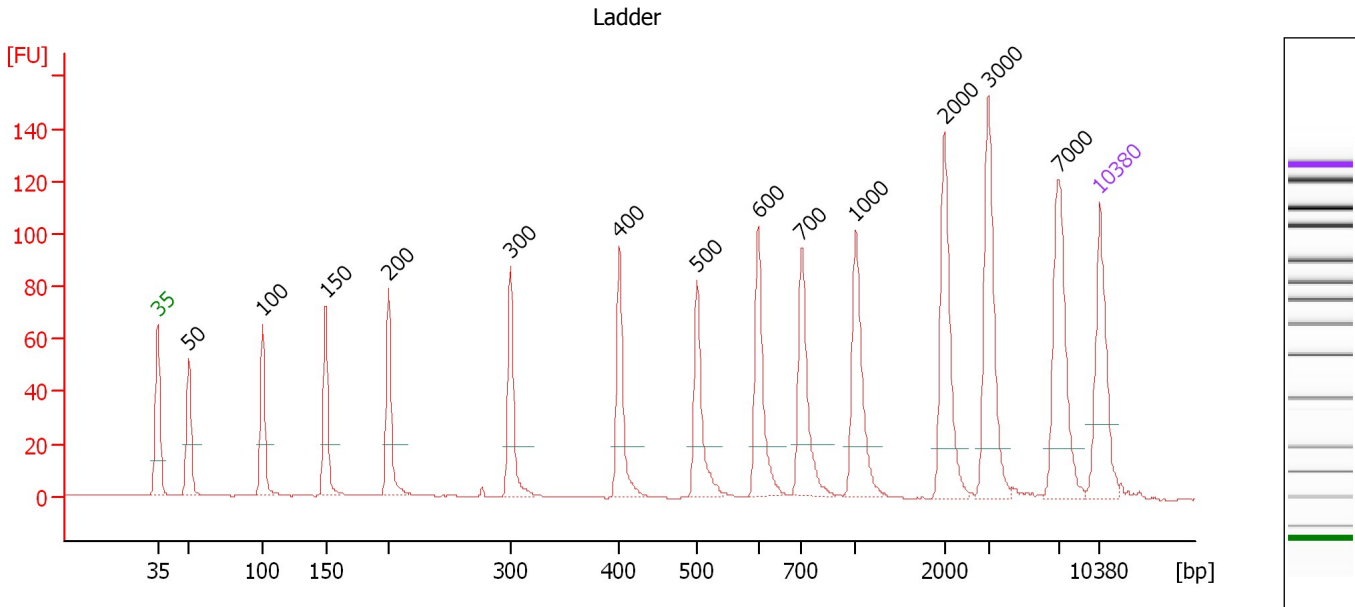

Overall Results for Ladder

Noise: 0.2

Peak table for Ladder


Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	50	150.00	4,545.5	Ladder Peak	45.33
3	100	150.00	2,272.7	Ladder Peak	50.80
4	150	150.00	1,515.2	Ladder Peak	55.52
5	200	150.00	1,136.4	Ladder Peak	60.14
6	300	150.00	757.6	Ladder Peak	69.23
7	400	150.00	568.2	Ladder Peak	77.33
8	500	150.00	454.5	Ladder Peak	83.04
9	600	150.00	378.8	Ladder Peak	87.61
10	700	150.00	324.7	Ladder Peak	90.84
11	1,000	150.00	227.3	Ladder Peak	94.87
12	2,000	150.00	113.6	Ladder Peak	101.42
13	3,000	150.00	75.8	Ladder Peak	104.70
14	7,000	150.00	32.5	Ladder Peak	109.92
15	10,380	75.00	10.9	Upper Marker	113.00

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\... bioanalyzer\2100 expert\data\2018-02-06\2018-02-06_001.xad

Created: 2/6/2018 10:26:32 AM
 Modified: 2/6/2018 10:50:37 AM

Electropherogram Summary Continued ...

Bsp4b 1/3 34

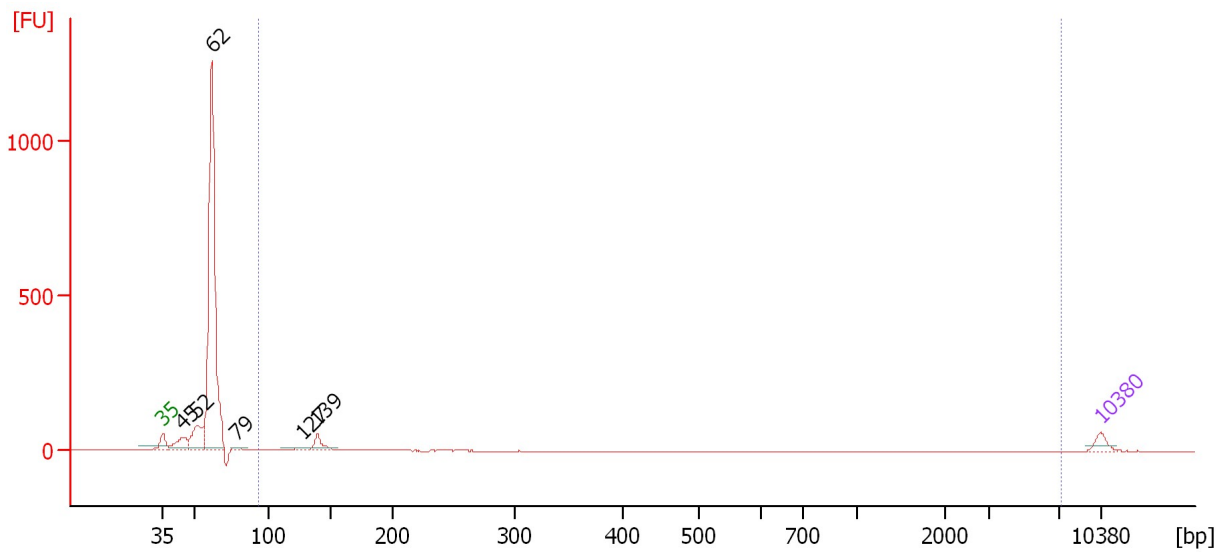

Overall Results for sample 1 : Bsp4b 1/3 34

Number of peaks found: 6 Corr. Area 1: 131.7
 Noise: 0.2

Peak table for sample 1 : Bsp4b 1/3 34

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	45	287.56	9,759.7		44.50
3	52	470.42	13,711.1		45.55
4	62	4,268.68	104,224.6		46.65
5	79	34.29	661.6		48.45
6	127	55.54	662.1		53.36
7	139	179.02	1,947.4		54.51
8	10,380	75.00	10.9	Upper Marker	113.00


Region table for sample 1 : Bsp4b 1/3 34

From [bp]	To [bp]	Average Size [bp]	Corr. Area	Conc. [pg/μl]	Molarity [pmol/l]	Co % of Ior Total	Size distribution in CV [%]
93	7,093	275	131.7	354.44	3,823.5	7	100.0

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\... bioanalyzer\2100 expert\data\2018-02-06\2018-02-06_001.xad

Created: 2/6/2018 10:26:32 AM
 Modified: 2/6/2018 10:50:37 AM

Electropherogram Summary Continued ...

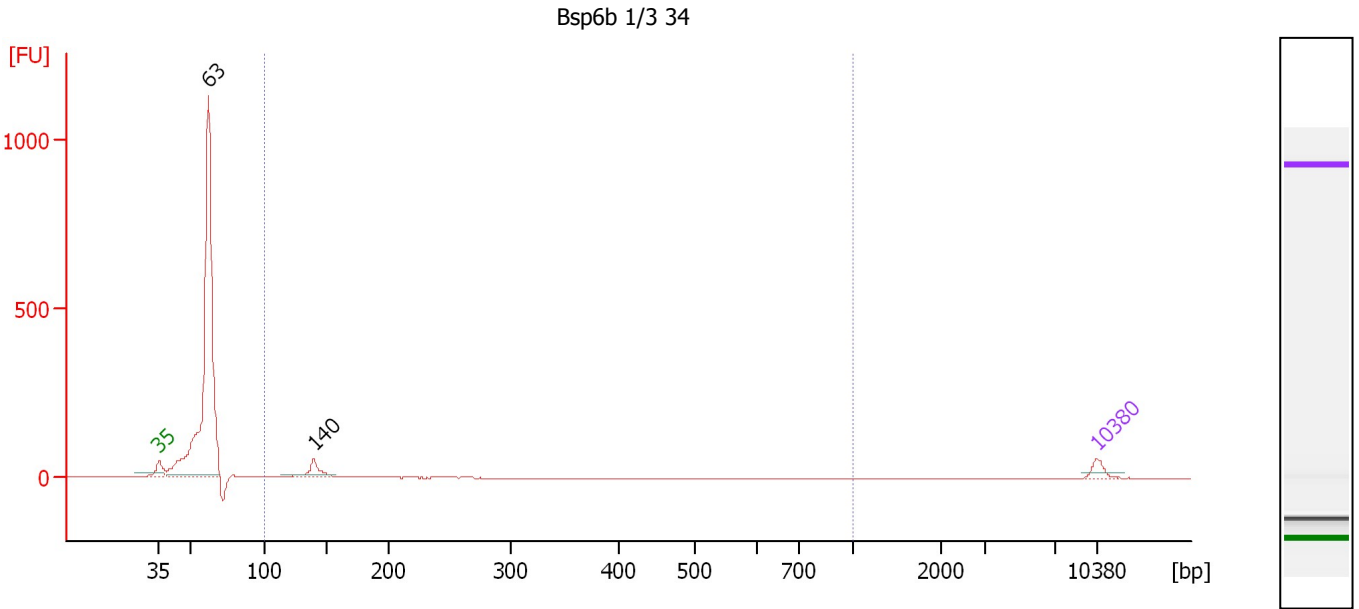

Overall Results for sample 2 : Bsp6b 1/3 34

Number of peaks found: 2 Corr. Area 1: 142.4
 Noise: 0.2

Peak table for sample 2 : Bsp6b 1/3 34

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	63	5,005.08	121,262.7		46.71
3	140	244.09	2,643.5		54.57
4	10,380	75.00	10.9	Upper Marker	113.00


Region table for sample 2 : Bsp6b 1/3 34

From [bp]	To [bp]	Average Size [bp]	Corr. Area	Conc. [pg/μl]	Molarity [pmol/l]	Co % of lor Total	Size distribution in CV [%]
101	1,000	151	142.4	371.60	3,957.5	7	38.7

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\... bioanalyzer\2100 expert\data\2018-02-06\2018-02-06_001.xad

Created: 2/6/2018 10:26:32 AM
 Modified: 2/6/2018 10:50:37 AM

Electropherogram Summary Continued ...

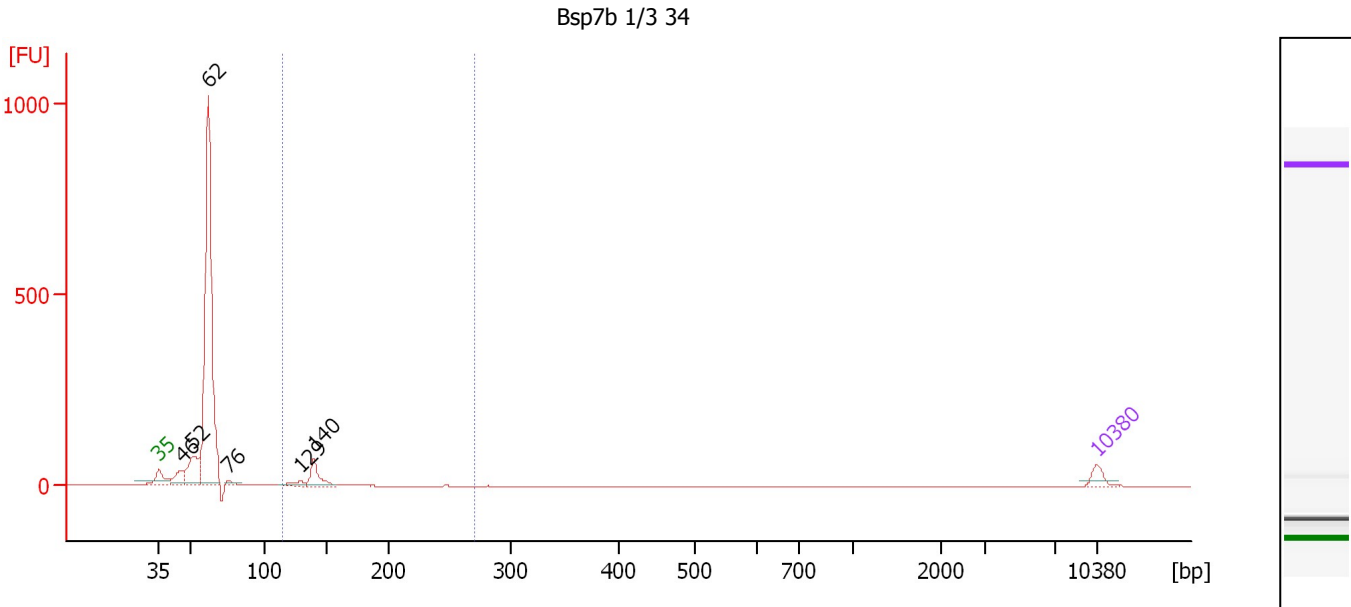

Overall Results for sample 3 : Bsp7b 1/3 34

Number of peaks found: 6 Corr. Area 1: 132.8
 Noise: 0.2

Peak table for sample 3 : Bsp7b 1/3 34

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	46	221.08	7,210.5		44.78
3	52	469.07	13,682.6		45.55
4	62	3,419.50	83,300.3		46.67
5	76	52.74	1,055.3		48.15
6	129	72.79	854.3		53.55
7	140	247.67	2,682.6		54.56
8	10,380	75.00	10.9	Upper Marker	113.00


Region table for sample 3 : Bsp7b 1/3 34

From [bp]	To [bp]	Average Size [bp]	Corr. Area	Conc. [pg/μl]	Molarity [pmol/l]	Co % of Ior Total	Size distribution in CV [%]
114	271	143	132.8	354.16	3,799.3	8	13.4

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\... bioanalyzer\2100 expert\data\2018-02-06\2018-02-06_001.xad

Created: 2/6/2018 10:26:32 AM
 Modified: 2/6/2018 10:50:37 AM

Electropherogram Summary Continued ...

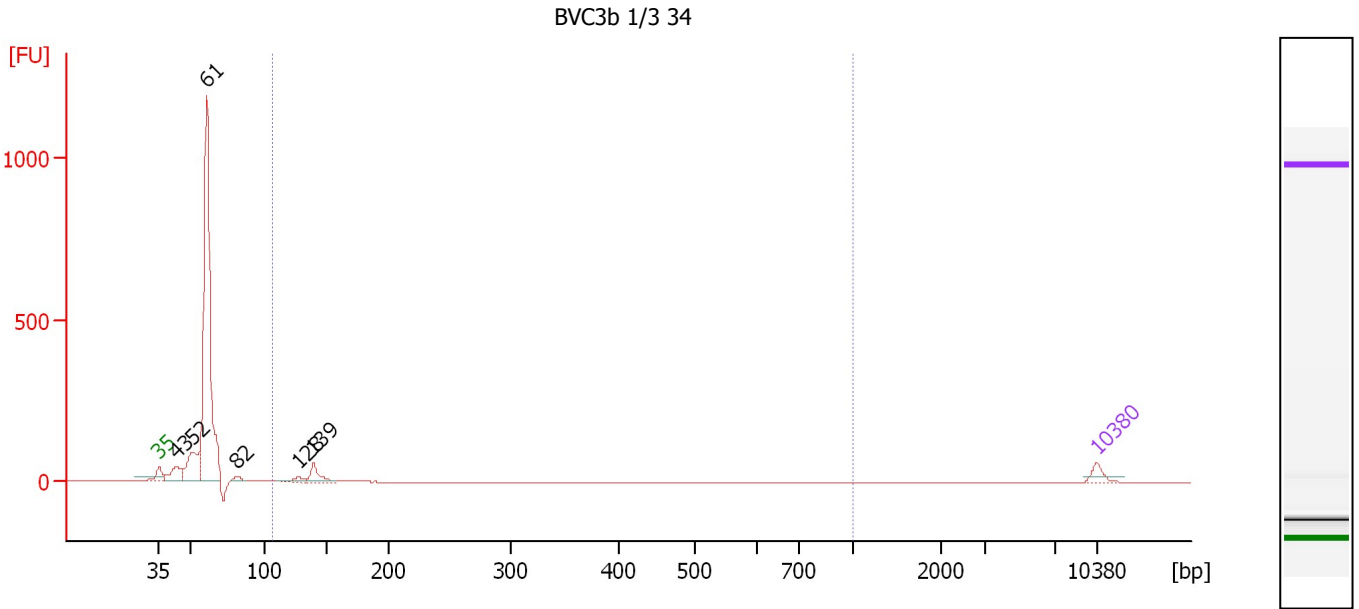

Overall Results for sample 4 : BVC3b 1/3 34

Number of peaks found: 6 Corr. Area 1: 123.2
 Noise: 0.2

Peak table for sample 4 : BVC3b 1/3 34

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	43	293.71	10,340.6		44.25
3	52	558.36	16,268.2		45.55
4	61	4,034.00	100,093.0		46.54
5	82	68.09	1,257.3		48.84
6	128	79.73	945.2		53.42
7	139	202.90	2,205.4		54.52
8	10,380	75.00	10.9	Upper Marker	113.00


Region table for sample 4 : BVC3b 1/3 34

From [bp]	To [bp]	Average Size [bp]	Corr. Area	Conc. [pg/μl]	Molarity [pmol/l]	Co % of Ior Total	Size distribution in CV [%]
108	1,000	143	123.2	329.46	3,550.0	6	14.4

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\... bioanalyzer\2100 expert\data\2018-02-06\2018-02-06_001.xad

Created: 2/6/2018 10:26:32 AM
 Modified: 2/6/2018 10:50:37 AM

Electropherogram Summary Continued ...

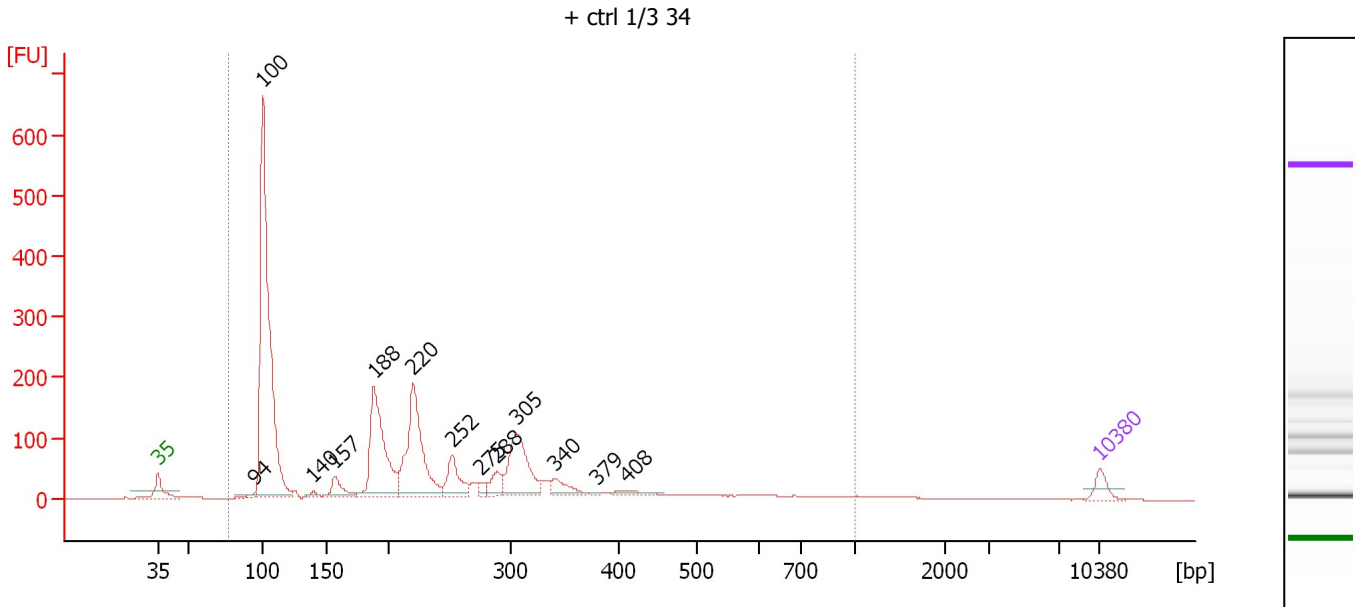

Overall Results for sample 5 : + ctrl 1/3 34

Number of peaks found: 13 Corr. Area 1: 2,677.1
 Noise: 0.2

Peak table for sample 5 : + ctrl 1/3 34

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	94	35.20	565.6		50.18
3	100	3,057.29	46,226.7		50.82
4	140	32.82	355.4		54.57
5	157	167.04	1,611.1		56.18
6	188	1,044.11	8,397.3		59.07
7	220	1,043.96	7,189.3		61.96
8	252	277.99	1,668.7		64.91
9	275	55.77	306.8		66.99
10	288	145.20	763.0		68.17
11	305	587.99	2,916.8		69.67
12	340	138.98	618.5		72.51
13	379	12.55	50.2		75.62
14	408	43.89	162.8		77.81
15	10,380	75.00	10.9	Upper Marker	113.00


Region table for sample 5 : + ctrl 1/3 34

From [bp]	To [bp]	Average Size [bp]	Corr. Area	Conc. [pg/μl]	Molarity [pmol/l]	Co % of lor Total	Size distribution in CV [%]
77	1,000	232	2,677.1	7,603.19	73,902.0	97	59.3

Assay Class: High Sensitivity DNA Assay
Data Path: C:\... bioanalyzer\2100 expert\data\2018-02-06\2018-02-06_001.xad

Created: 2/6/2018 10:26:32 AM
Modified: 2/6/2018 10:50:37 AM

Gel Image

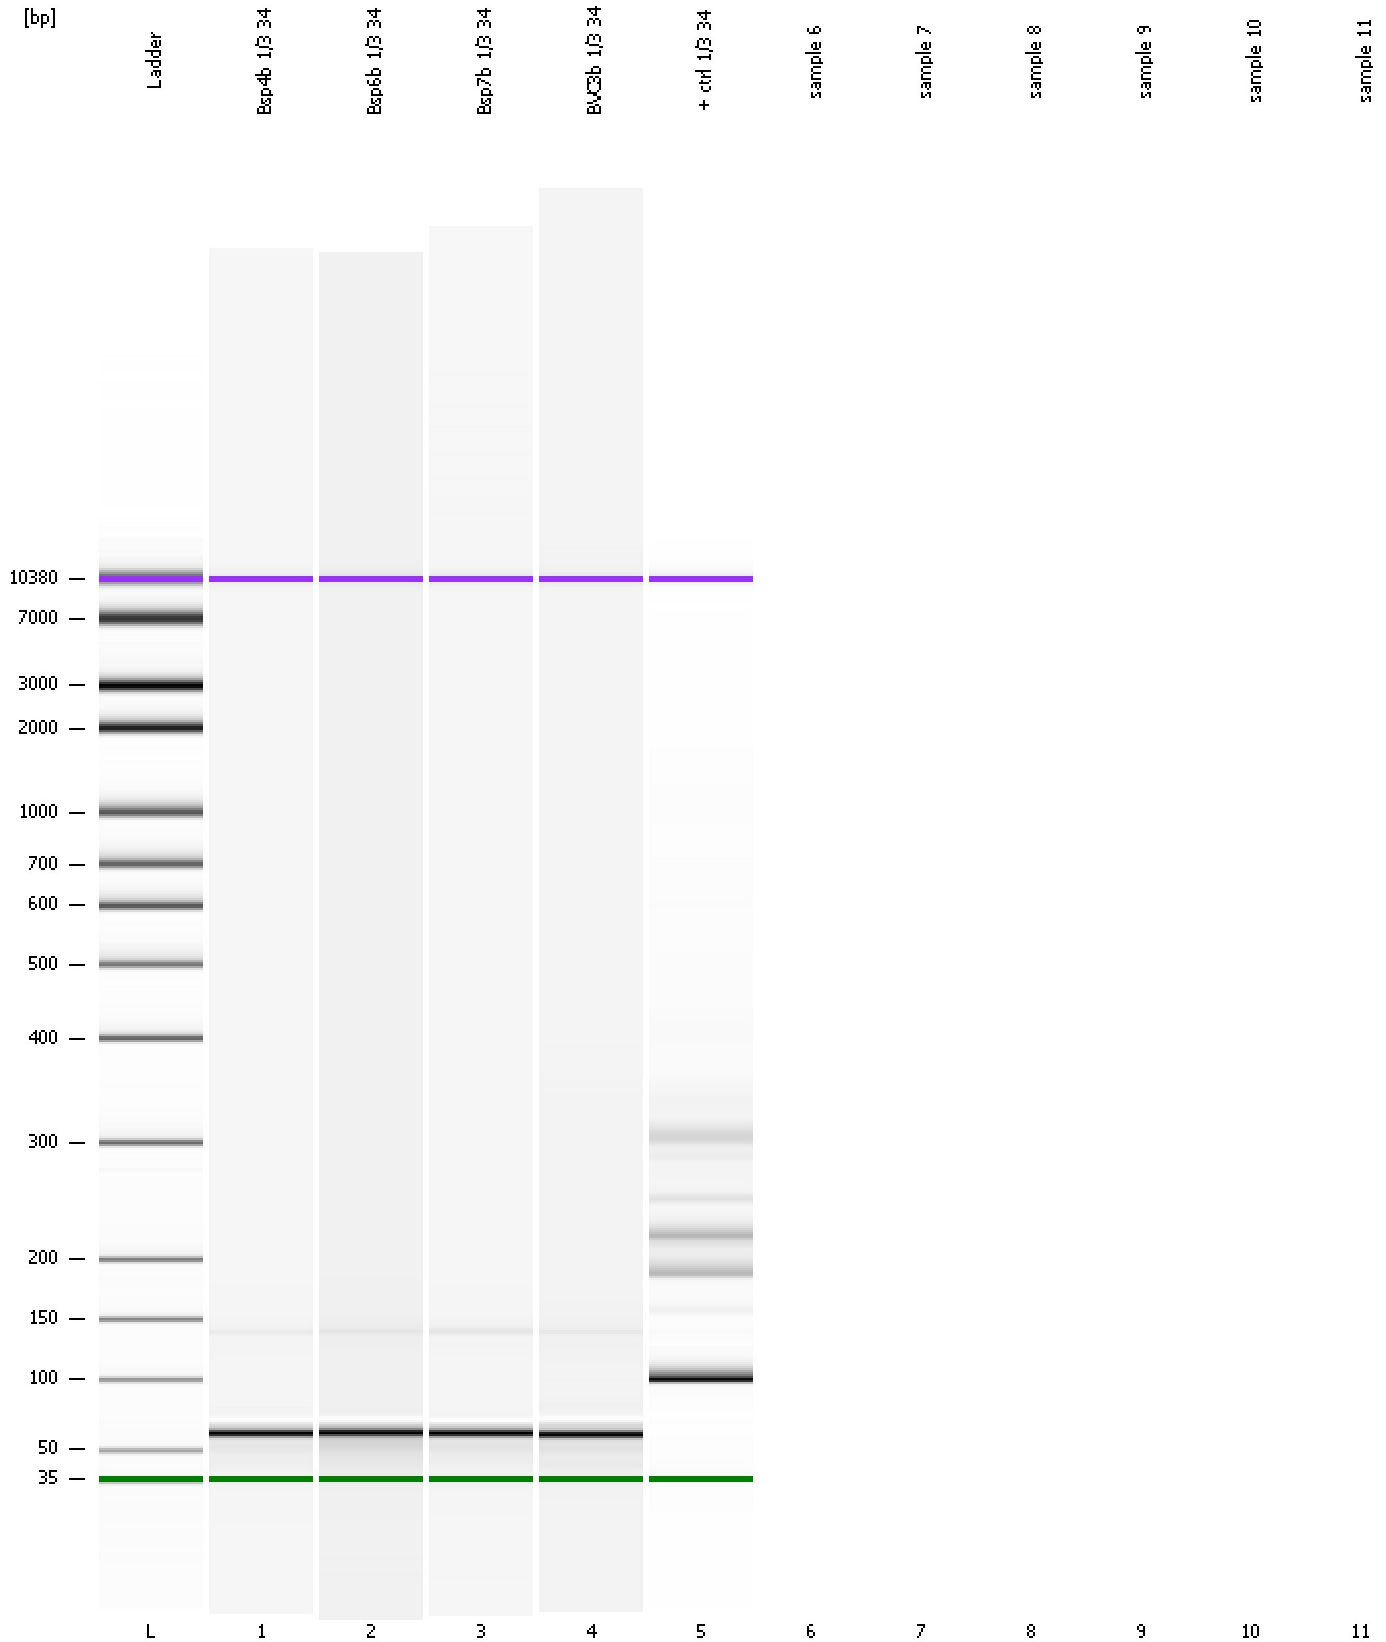

Assay Class: High Sensitivity DNA Assay
Data Path: C:\... bioanalyzer\2100 expert\data\2018-02-06\2018-02-06_001.xad

Created: 2/6/2018 10:26:32 AM
Modified: 2/6/2018 10:50:37 AM

Invalid Samples

Sample 6 has not been run, no results available.

Sample 7 has not been run, no results available.

Sample 8 has not been run, no results available.

Sample 9 has not been run, no results available.

Sample 10 has not been run, no results available.

Sample 11 has not been run, no results available.