


Assay Class: High Sensitivity DNA Assay
Data Path: C:\...lyzer\2100 expert\data\2018-07-04\2018-07-04_001_H1427P.xad

Created: 7/4/2018 3:02:09 PM
Modified: 7/4/2018 3:42:46 PM

Electrophoresis File Run Summary

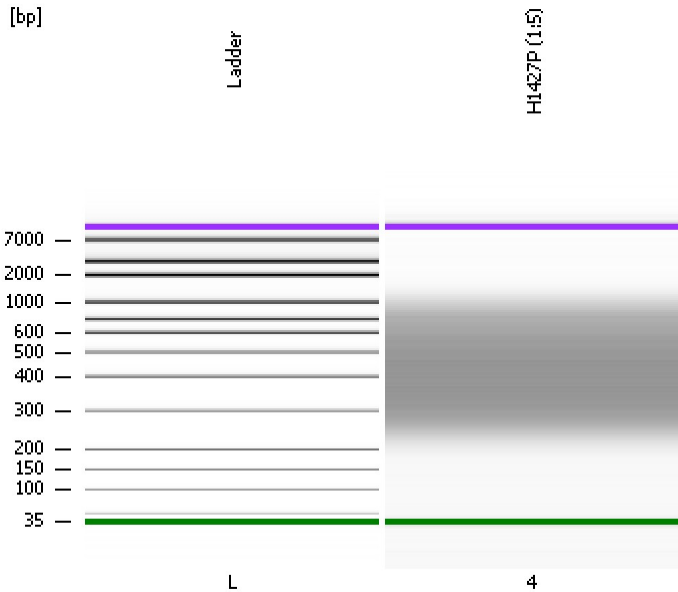

Instrument Information:

Instrument Name: DE34903152 Firmware: C.01.069
Serial#: DE34903152 Type: G2938C

Assay Information:


Assay Origin Path: C:\Program Files\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy

Assay Class: High Sensitivity DNA Assay
Version: 1.03
Assay Comments: Copyright © 2003-2010 Agilent Technologies

Chip Information:

Chip Lot #:
Reagent Kit Lot #:
Chip Comments:

H1427P (1:5)

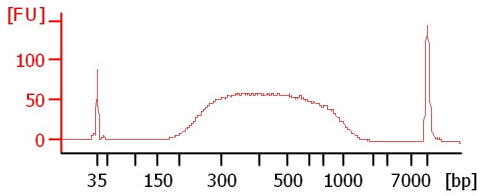

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...lyzer\2100 expert\data\2018-07-04\2018-07-04_001_H1427P.xad

Created: 7/4/2018 3:02:09 PM
 Modified: 7/4/2018 3:42:46 PM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
H1427P (1:5)		<input type="checkbox"/>				
Ladder		<input type="checkbox"/>				

Chip Lot # **Reagent Kit Lot #**

Chip Comments :

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...lyzer\2100 expert\data\2018-07-04\2018-07-04_001_H1427P.xad

Created: 7/4/2018 3:02:09 PM
Modified: 7/4/2018 3:42:46 PM

Electrophoresis Assay Details

General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12
Minimum Visible Range [s] : 32
Maximum Visible Range [s] : 138
Start Analysis Time Range [s] : 33
End Analysis Time Range [s] : 137.5
Ladder Concentration [pg/μl] : 1950
Uses Standard Area for Ladder Fragments
Lower Marker Concentration [pg/μl] : 125
Upper Marker Concentration [pg/μl] : 75
Used Upper Marker for Quantitation
Standard Curve Fit is Point to Point
Show Data Aligned to Lower and Upper Marker

Integrator Settings

Integration Start Time [s] : 33.05
Integration End Time [s] : 137
Slope Threshold : 0.8
Height Threshold [FU] : 5
Area Threshold : 0.1
Width Threshold [s] : 0.6
Baseline Plateau [s] : 0.5

Filter Settings

Filter Width [s] : 0.5
Polynomial Order : 4


Ladder

Ladder Peak	Size	Area
1	35	160
2	50	210
3	100	208
4	150	221
5	200	242
6	300	270
7	400	305
8	500	306
9	600	336
10	700	321
11	1000	366
12	2000	413
13	3000	411
14	7000	400
15	10380	214

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...lyzer\2100 expert\data\2018-07-04\2018-07-04_001_H1427P.xad

Created: 7/4/2018 3:02:09 PM
 Modified: 7/4/2018 3:42:46 PM

Electropherogram Summary

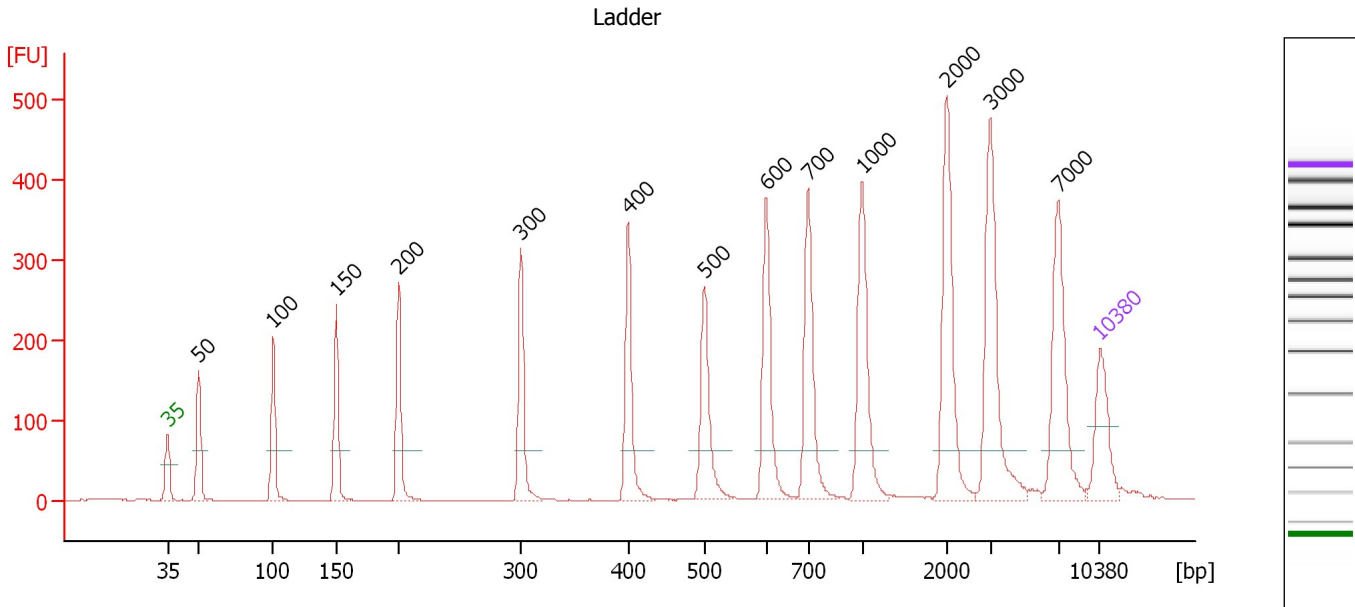

Overall Results for Ladder

Noise: 0.3


Peak table for Ladder

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	50	150.00	4,545.5	Ladder Peak	45.32
3	100	150.00	2,272.7	Ladder Peak	50.93
4	150	150.00	1,515.2	Ladder Peak	55.65
5	200	150.00	1,136.4	Ladder Peak	60.33
6	300	150.00	757.6	Ladder Peak	69.51
7	400	150.00	568.2	Ladder Peak	77.58
8	500	150.00	454.5	Ladder Peak	83.28
9	600	150.00	378.8	Ladder Peak	87.96
10	700	150.00	324.7	Ladder Peak	91.08
11	1,000	150.00	227.3	Ladder Peak	95.13
12	2,000	150.00	113.6	Ladder Peak	101.50
13	3,000	150.00	75.8	Ladder Peak	104.76
14	7,000	150.00	32.5	Ladder Peak	109.88
15	10,380	75.00	10.9	Upper Marker	113.00

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...lyzer\2100 expert\data\2018-07-04\2018-07-04_001_H1427P.xad

Created: 7/4/2018 3:02:09 PM
 Modified: 7/4/2018 3:42:46 PM

Electropherogram Summary Continued ...

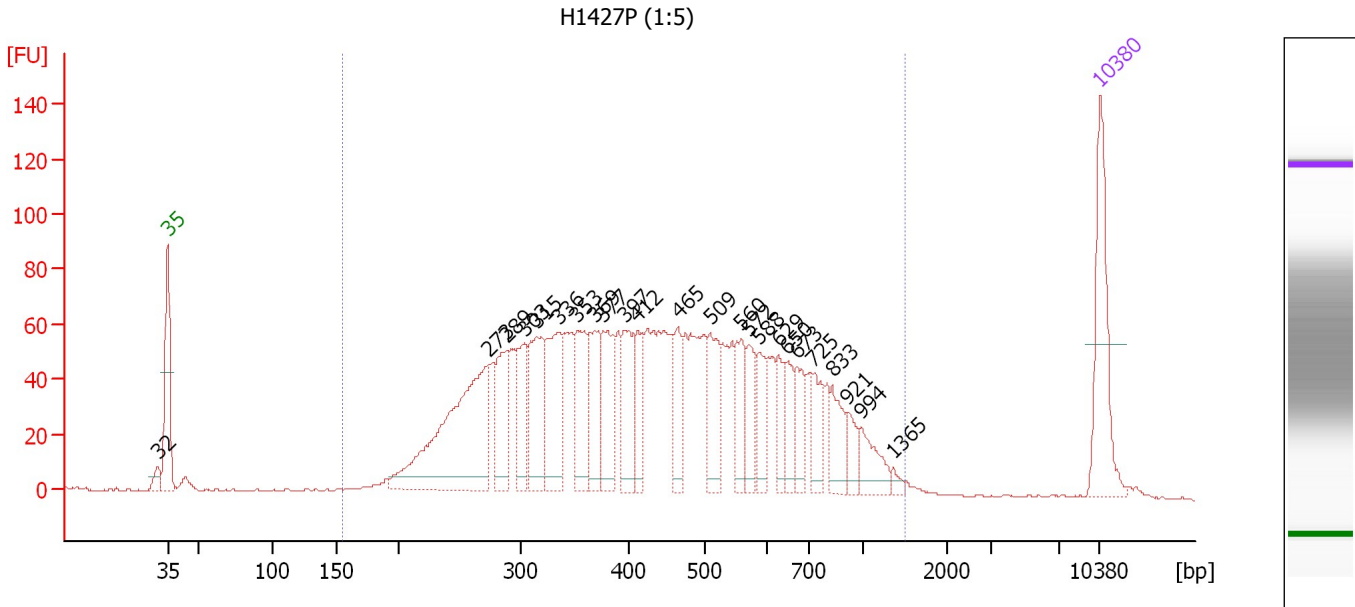

Overall Results for sample 4 : H1427P (1:5)

Number of peaks found: 24 Corr. Area 1: 2,232.5
 Noise: 0.3

Peak table for sample 4 : H1427P (1:5)

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	32	0.00	0.0		42.24
2	35	125.00	5,411.3	Lower Marker	43.00
3	273	252.08	1,398.6		67.04
4	289	75.52	396.6		68.46
5	303	60.86	304.0		69.78
6	315	89.33	429.6		70.73
7	336	93.82	422.9		72.43
8	353	72.71	312.5		73.75
9	369	66.78	274.3		75.07
10	377	65.30	262.7		75.69
11	397	62.82	239.7		77.34
12	412	37.89	139.2		78.28
13	465	39.81	129.6		81.31
14	509	55.06	163.8		83.72
15	560	42.48	115.0		86.08
16	572	35.73	94.7		86.64
17	588	31.31	80.7		87.40
18	629	25.83	62.2		88.86
19	650	32.61	76.0		89.52
20	673	31.24	70.3		90.23
21	725	32.14	67.2		91.41
22	833	34.69	63.1		92.88
23	921	17.59	28.9		94.06
24	994	29.48	44.9		95.05
25	1,365	4.95	5.5		97.46

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...lyzer\2100 expert\data\2018-07-04\2018-07-04_001_H1427P.xad

Created: 7/4/2018 3:02:09 PM
 Modified: 7/4/2018 3:42:46 PM

Electropherogram Summary Continued ...

... Peak table for sample 4 : H1427P (1:5)

Peak	Size [bp]	Conc. [pg/ μ l]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
26	10,380	75.00	10.9	Upper Marker	113.00

Region table for sample 4 : H1427P (1:5)

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/ μ l]	Corr. Area	Molarity [pmol/l]	Co % of lor Total	Size distribution in CV [%]
155	1,501	472	1,890.28	2,232.5	7,546.3	98	43.4

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...lyzer\2100 expert\data\2018-07-04\2018-07-04_001_H1427P.xad

Created: 7/4/2018 3:02:09 PM
Modified: 7/4/2018 3:42:46 PM

Gel Image

