


Assay Class: High Sensitivity DNA Assay
Data Path: C:\... bioanalyzer\2100 expert\data\2019-03-27\2019-03-27_001.xad

Created: 3/27/2019 10:20:55 AM
Modified: 3/27/2019 10:56:37 AM

Electrophoresis File Run Summary

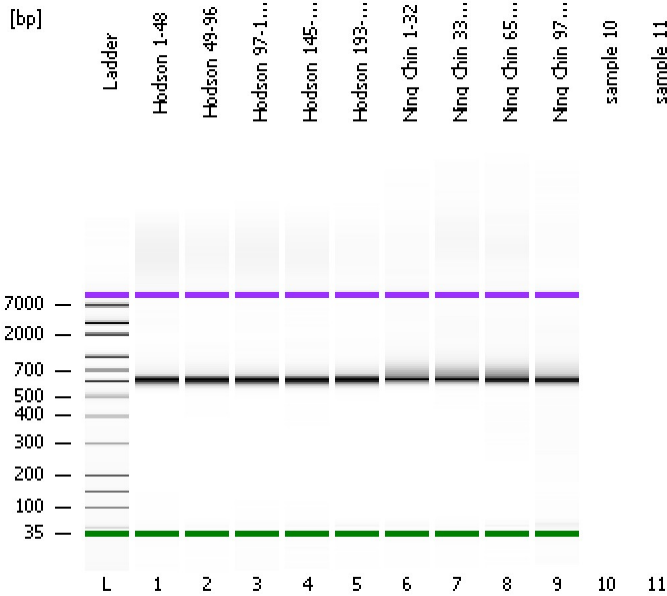

Instrument Information:

Instrument Name: DE34903152 Firmware: C.01.069
Serial#: DE34903152 Type: G2938C


Assay Information:

Assay Origin Path: C:\Program Files\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy
Assay Class: High Sensitivity DNA Assay
Version: 1.03
Assay Comments: Copyright © 2003-2010 Agilent Technologies


Chip Information:

Chip Lot #:
Reagent Kit Lot #:
Chip Comments:


Hodson 1-48

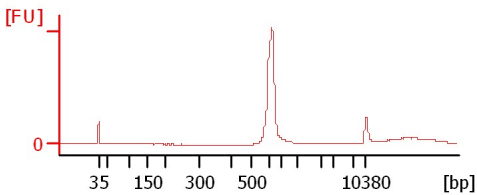


Hodson 49-96

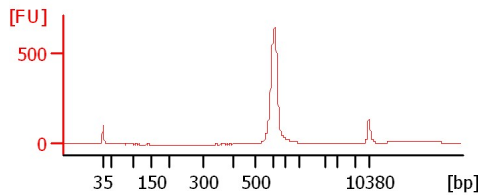


Hodson 97-144

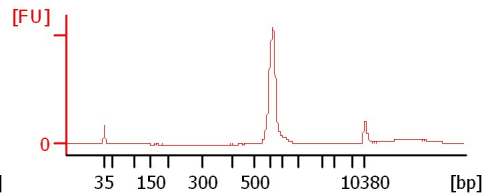


Hodson 145-192

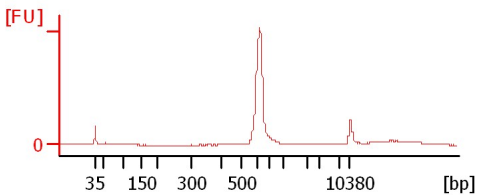


Hodson 193-216

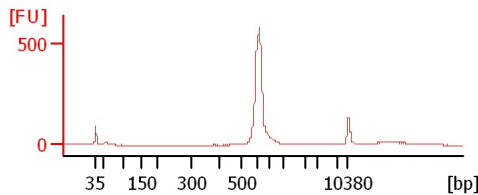


Ning Chin 1-32

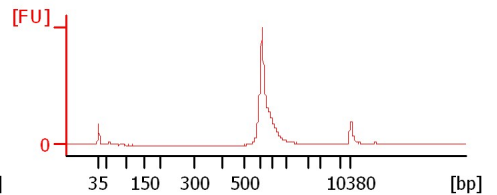


Ning Chin 33-64

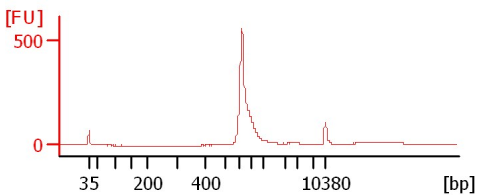

Ning Chin 65-96

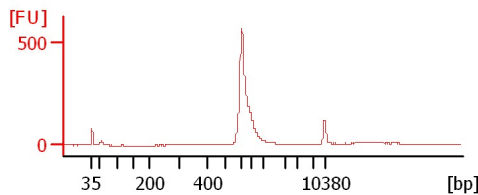

Ning Chin 97-111

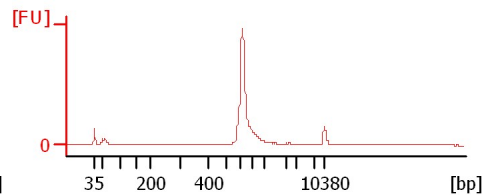

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\... bioanalyzer\2100 expert\data\2019-03-27\2019-03-27_001.xad

Created: 3/27/2019 10:20:55 AM
 Modified: 3/27/2019 10:56:37 AM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
Hodson 1-48		<input type="checkbox"/>	✓			
Hodson 49-96		<input type="checkbox"/>	✓			
Hodson 97-144		<input type="checkbox"/>	✓			
Hodson 145-192		<input type="checkbox"/>	✓			
Hodson 193-216		<input type="checkbox"/>	✓			
Ning Chin 1-32		<input type="checkbox"/>	✓			
Ning Chin 33-64		<input type="checkbox"/>	✓			
Ning Chin 65-96		<input type="checkbox"/>	✓			
Ning Chin 97-111		<input type="checkbox"/>	✓			
sample 10		<input type="checkbox"/>				
sample 11		<input type="checkbox"/>				
Ladder		<input type="checkbox"/>	✓			

Chip Lot #

Reagent Kit Lot #

Chip Comments :

Assay Class: High Sensitivity DNA Assay
Data Path: C:\... bioanalyzer\2100 expert\data\2019-03-27\2019-03-27_001.xad

Created: 3/27/2019 10:20:55 AM
Modified: 3/27/2019 10:56:37 AM

Electrophoresis Assay Details

General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12
Minimum Visible Range [s] : 32
Maximum Visible Range [s] : 138
Start Analysis Time Range [s] : 33
End Analysis Time Range [s] : 137.5
Ladder Concentration [pg/μl] : 1950
Uses Standard Area for Ladder Fragments
Lower Marker Concentration [pg/μl] : 125
Upper Marker Concentration [pg/μl] : 75
Used Upper Marker for Quantitation
Standard Curve Fit is Point to Point
Show Data Aligned to Lower and Upper Marker

Integrator Settings

Integration Start Time [s] : 33.05
Integration End Time [s] : 137
Slope Threshold : 0.8
Height Threshold [FU] : 5
Area Threshold : 0.1
Width Threshold [s] : 0.6
Baseline Plateau [s] : 0.5

Filter Settings

Filter Width [s] : 0.5
Polynomial Order : 4


Ladder

Ladder Peak	Size	Area
1	35	160
2	50	210
3	100	208
4	150	221
5	200	242
6	300	270
7	400	305
8	500	306
9	600	336
10	700	321
11	1000	366
12	2000	413
13	3000	411
14	7000	400
15	10380	214

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\... bioanalyzer\2100 expert\data\2019-03-27\2019-03-27_001.xad

Created: 3/27/2019 10:20:55 AM
 Modified: 3/27/2019 10:56:37 AM

Electropherogram Summary

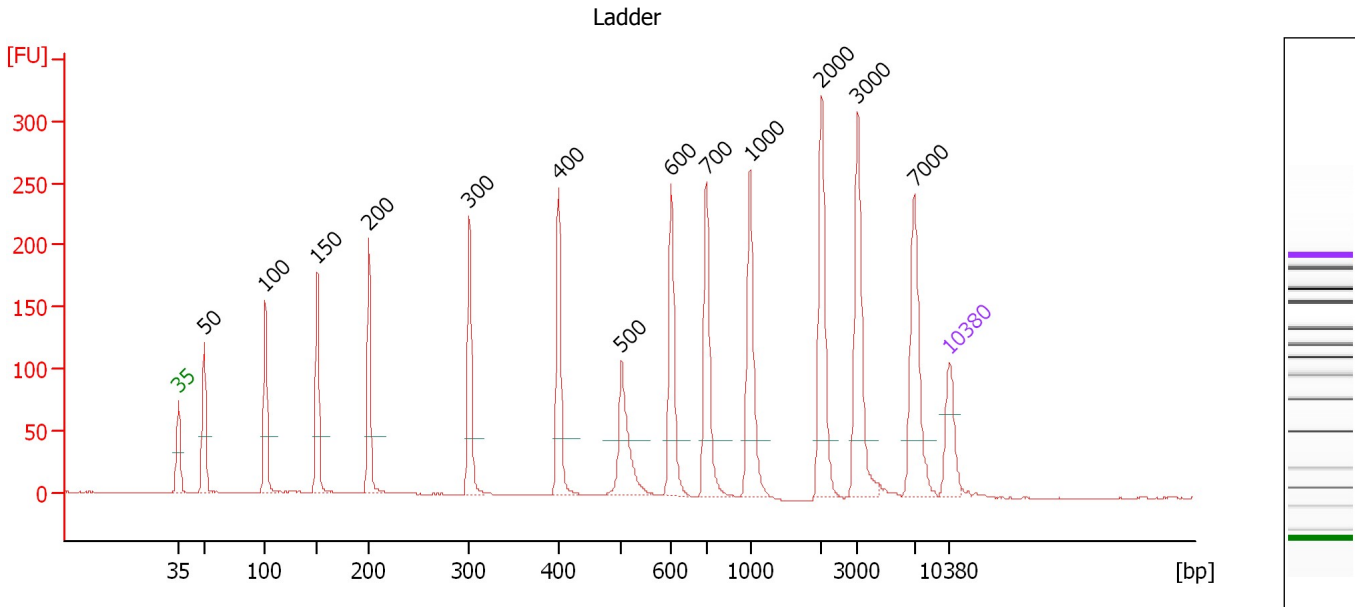

Overall Results for Ladder

Noise: 0.4


Peak table for Ladder

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	50	150.00	4,545.5	Ladder Peak	45.32
3	100	150.00	2,272.7	Ladder Peak	50.89
4	150	150.00	1,515.2	Ladder Peak	55.58
5	200	150.00	1,136.4	Ladder Peak	60.27
6	300	150.00	757.6	Ladder Peak	69.41
7	400	150.00	568.2	Ladder Peak	77.49
8	500	150.00	454.5	Ladder Peak	83.20
9	600	150.00	378.8	Ladder Peak	87.70
10	700	150.00	324.7	Ladder Peak	90.89
11	1,000	150.00	227.3	Ladder Peak	94.86
12	2,000	150.00	113.6	Ladder Peak	101.34
13	3,000	150.00	75.8	Ladder Peak	104.63
14	7,000	150.00	32.5	Ladder Peak	109.76
15	10,380	75.00	10.9	Upper Marker	113.00

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\... bioanalyzer\2100 expert\data\2019-03-27\2019-03-27_001.xad

Created: 3/27/2019 10:20:55 AM
 Modified: 3/27/2019 10:56:37 AM

Electropherogram Summary Continued ...

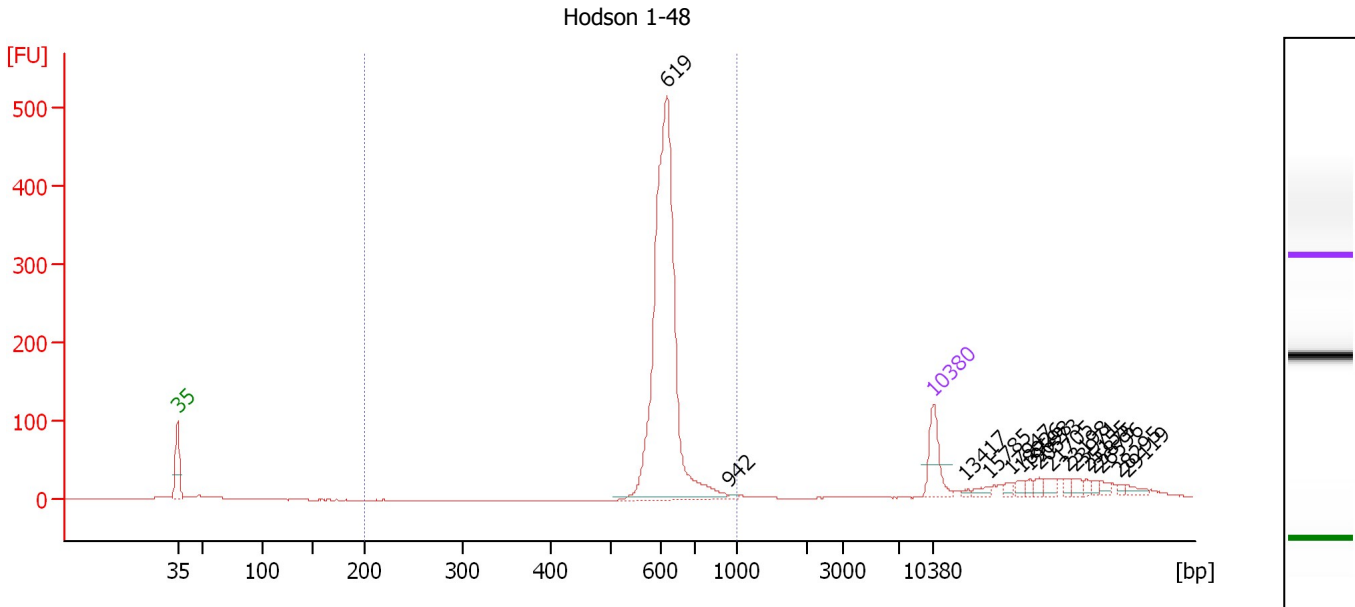

Overall Results for sample 1 : Hodson 1-48

Number of peaks found: 16 Corr. Area 1: 1,257.5
 Noise: 0.4

Peak table for sample 1 : Hodson 1-48

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	619	1,078.28	2,637.8		88.32
3	942	4.43	7.1		94.09
4	10,380	75.00	10.9	Upper Marker	113.00
5	13,417	0.00	0.0		115.91
6	15,785	0.00	0.0		118.18
7	17,947	0.00	0.0		120.26
8	18,926	0.00	0.0		121.19
9	19,698	0.00	0.0		121.94
10	20,573	0.00	0.0		122.77
11	21,705	0.00	0.0		123.86
12	23,198	0.00	0.0		125.29
13	23,971	0.00	0.0		126.03
14	25,155	0.00	0.0		127.17
15	25,875	0.00	0.0		127.86
16	26,596	0.00	0.0		128.55
17	28,295	0.00	0.0		130.18
18	29,119	0.00	0.0		130.97


Region table for sample 1 : Hodson 1-48

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/μl]	Corr. Area	Molarity [pmol/l]	Co % of lor Total	Size distribution in CV [%]
200	1,000	620	1,057.21	1,257.5	2,595.1	81	7.3

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\... bioanalyzer\2100 expert\data\2019-03-27\2019-03-27_001.xad

Created: 3/27/2019 10:20:55 AM
 Modified: 3/27/2019 10:56:37 AM

Electropherogram Summary Continued ...

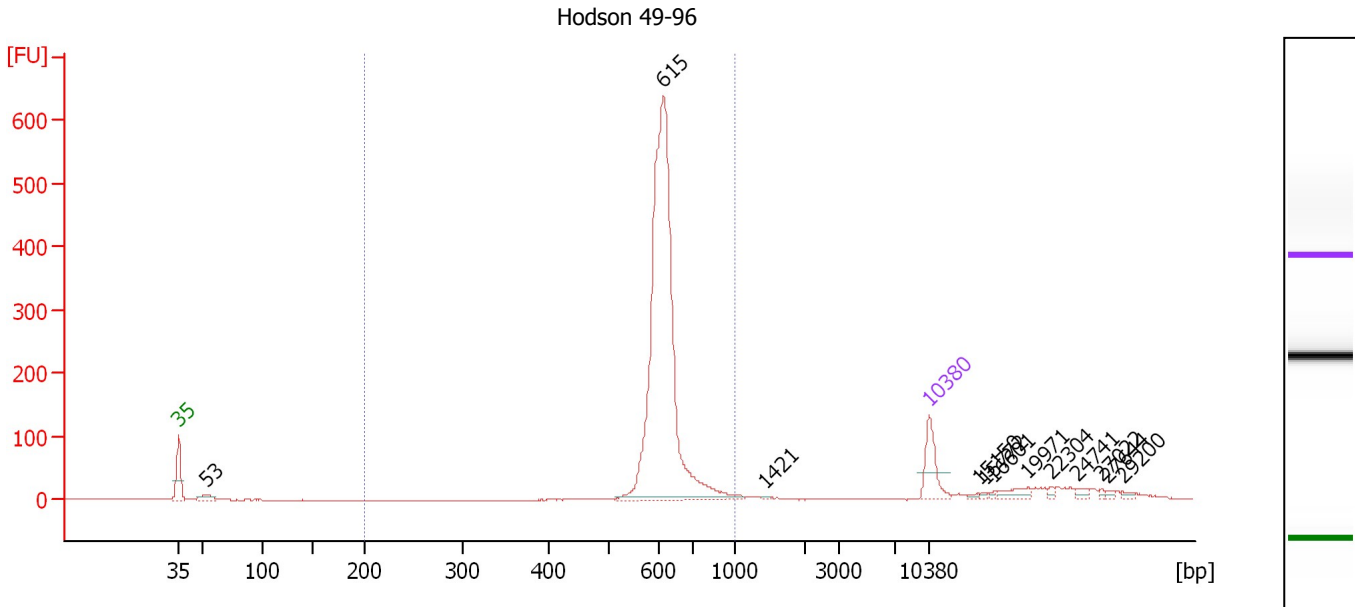

Overall Results for sample 2 : Hodson 49-96

Number of peaks found: 12 Corr. Area 1: 1,638.6
 Noise: 0.5

Peak table for sample 2 : Hodson 49-96

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	53	30.37	871.4		45.63
3	615	1,240.15	3,053.2		88.19
4	1,421	2.48	2.6		97.59
5	10,380	75.00	10.9	Upper Marker	113.00
6	15,150	0.00	0.0		117.57
7	15,772	0.00	0.0		118.17
8	16,601	0.00	0.0		118.97
9	19,971	0.00	0.0		122.20
10	22,304	0.00	0.0		124.43
11	24,741	0.00	0.0		126.77
12	27,022	0.00	0.0		128.96
13	27,644	0.00	0.0		129.56
14	29,200	0.00	0.0		131.05


Region table for sample 2 : Hodson 49-96

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/μl]	Corr. Area	Molarity [pmol/l]	Co % of lor Total	Size distribution in CV [%]
200	1,000	622	1,228.19	1,638.6	3,008.9	86	8.5

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\... bioanalyzer\2100 expert\data\2019-03-27\2019-03-27_001.xad

Created: 3/27/2019 10:20:55 AM
 Modified: 3/27/2019 10:56:37 AM

Electropherogram Summary Continued ...

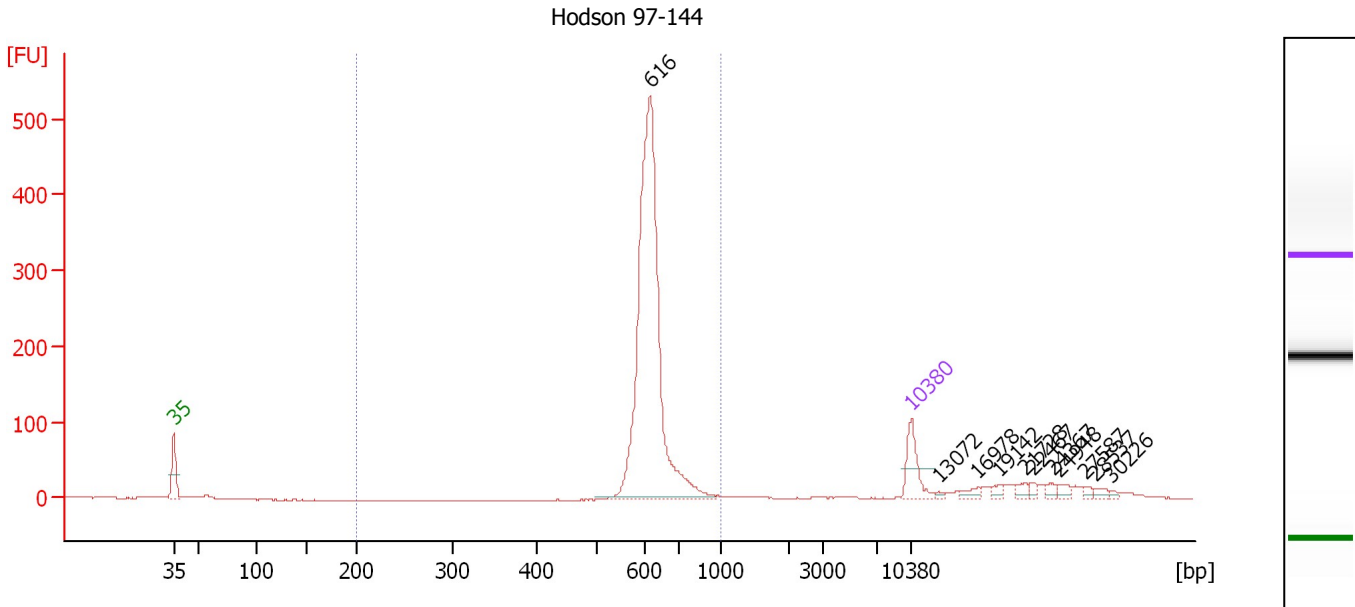

Overall Results for sample 3 : Hodson 97-144

Number of peaks found: 11 Corr. Area 1: 1,329.0
 Noise: 0.3

Peak table for sample 3 : Hodson 97-144

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	616	1,181.74	2,908.3		88.20
3	10,380	75.00	10.9	Upper Marker	113.00
4	13,072	0.00	0.0		115.58
5	16,978	0.00	0.0		119.33
6	19,142	0.00	0.0		121.40
7	21,728	0.00	0.0		123.88
8	22,467	0.00	0.0		124.59
9	24,367	0.00	0.0		126.41
10	24,948	0.00	0.0		126.97
11	27,587	0.00	0.0		129.50
12	28,537	0.00	0.0		130.41
13	30,226	0.00	0.0		132.03


Region table for sample 3 : Hodson 97-144

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/μl]	Corr. Area	Molarity [pmol/l]	Co % of lor Total	Size distribution in CV [%]
200	1,000	622	1,165.46	1,329.0	2,853.5	84	7.7

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\... bioanalyzer\2100 expert\data\2019-03-27\2019-03-27_001.xad

Created: 3/27/2019 10:20:55 AM
 Modified: 3/27/2019 10:56:37 AM

Electropherogram Summary Continued ...

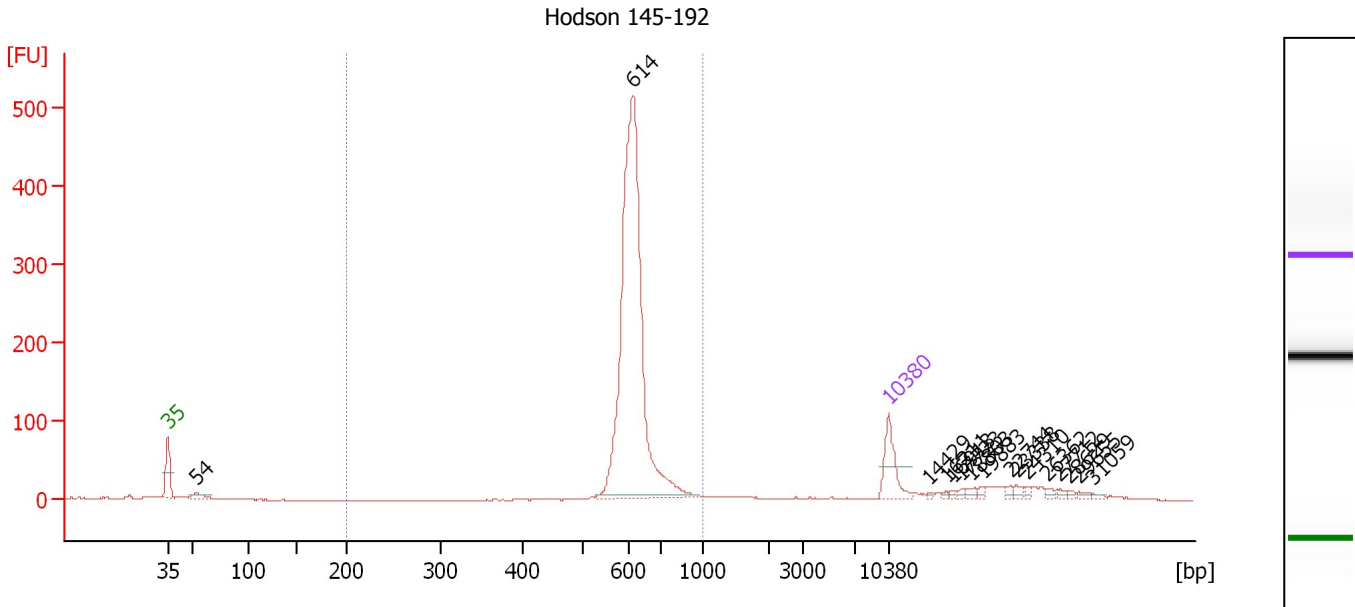

Overall Results for sample 4 : Hodson 145-192

Number of peaks found: 16 Corr. Area 1: 1,326.6
 Noise: 0.5

Peak table for sample 4 : Hodson 145-192

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	54	25.46	717.1		45.74
3	614	1,155.69	2,851.6		88.15
4	10,380	75.00	10.9	Upper Marker	113.00
5	14,429	0.00	0.0		116.88
6	16,211	0.00	0.0		118.59
7	16,913	0.00	0.0		119.26
8	17,723	0.00	0.0		120.04
9	18,803	0.00	0.0		121.08
10	19,883	0.00	0.0		122.11
11	22,744	0.00	0.0		124.86
12	23,338	0.00	0.0		125.43
13	24,310	0.00	0.0		126.36
14	26,362	0.00	0.0		128.33
15	27,712	0.00	0.0		129.62
16	28,629	0.00	0.0		130.50
17	29,655	0.00	0.0		131.48
18	31,059	0.00	0.0		132.83


Region table for sample 4 : Hodson 145-192

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/μl]	Corr. Area	Molarity [pmol/l]	Co % of lor Total	Size distribution in CV [%]
200	1,000	621	1,182.35	1,326.6	2,900.4	83	8.2

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\... bioanalyzer\2100 expert\data\2019-03-27\2019-03-27_001.xad

Created: 3/27/2019 10:20:55 AM
 Modified: 3/27/2019 10:56:37 AM

Electropherogram Summary Continued ...

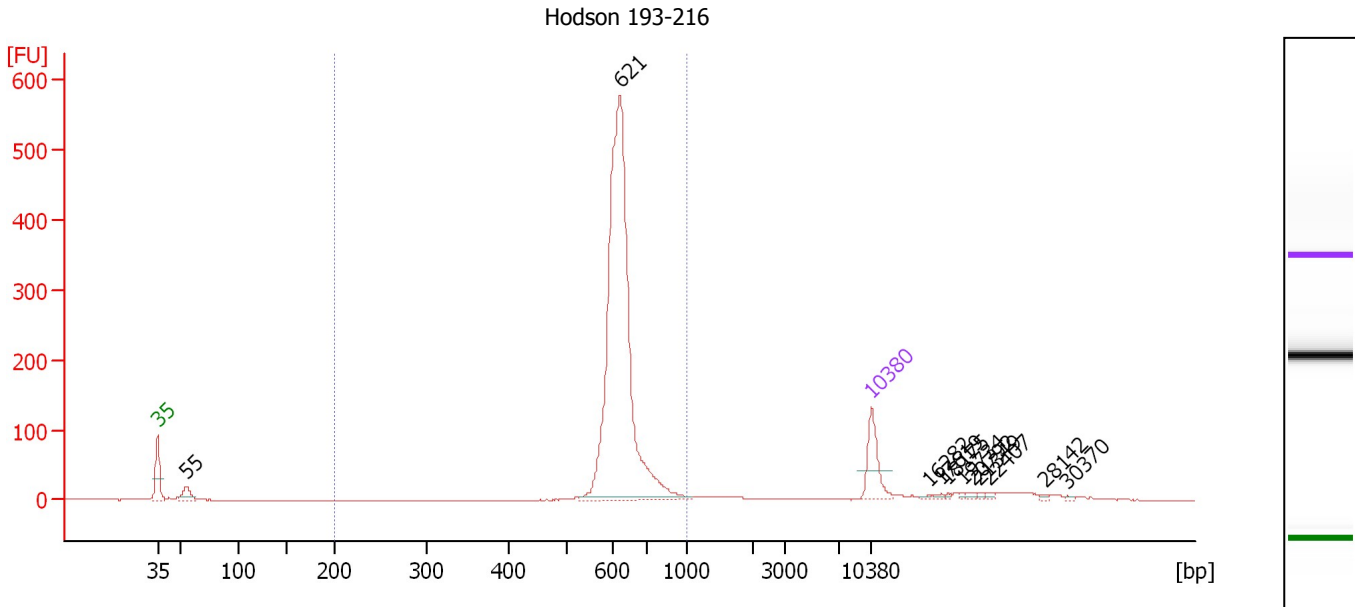

Overall Results for sample 5 : Hodson 193-216

Number of peaks found: 11 Corr. Area 1: 1,539.9
 Noise: 0.4

Peak table for sample 5 : Hodson 193-216

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	55	45.21	1,255.3		45.83
3	621	1,142.34	2,785.0		88.39
4	10,380	75.00	10.9	Upper Marker	113.00
5	16,282	0.00	0.0		118.66
6	17,619	0.00	0.0		119.94
7	18,175	0.00	0.0		120.48
8	19,734	0.00	0.0		121.97
9	20,792	0.00	0.0		122.98
10	21,349	0.00	0.0		123.52
11	22,407	0.00	0.0		124.53
12	28,142	0.00	0.0		130.03
13	30,370	0.00	0.0		132.17


Region table for sample 5 : Hodson 193-216

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/μl]	Corr. Area	Molarity [pmol/l]	Co % of lor Total	Size distribution in CV [%]
200	1,000	627	1,150.66	1,539.9	2,795.9	86	8.7

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\... bioanalyzer\2100 expert\data\2019-03-27\2019-03-27_001.xad

Created: 3/27/2019 10:20:55 AM
 Modified: 3/27/2019 10:56:37 AM

Electropherogram Summary Continued ...

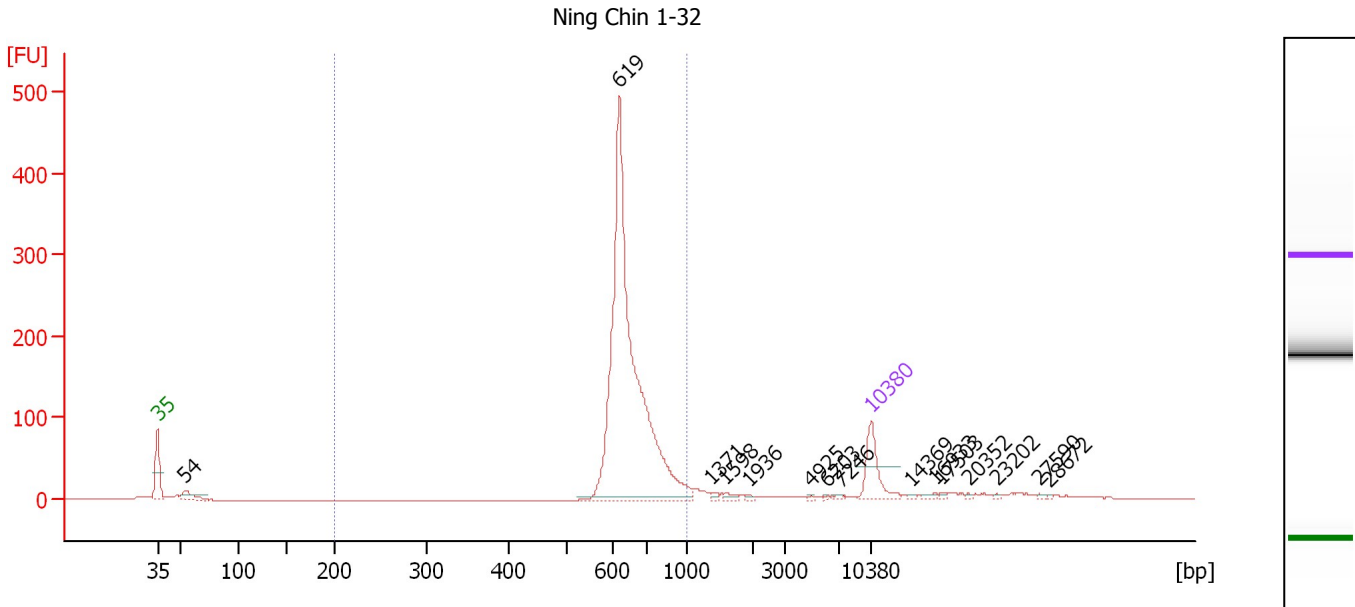

Overall Results for sample 6 : Ning Chin 1-32

Number of peaks found: 15 Corr. Area 1: 1,246.4
 Noise: 0.4

Peak table for sample 6 : Ning Chin 1-32

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	54	41.83	1,180.4		45.73
3	619	1,132.43	2,772.6		88.30
4	1,371	5.45	6.0		97.26
5	1,598	8.47	8.0		98.74
6	1,936	3.89	3.0		100.92
7	4,925	2.51	0.8		107.10
8	6,203	2.25	0.5		108.74
9	7,246	4.64	1.0		109.99
10	10,380	75.00	10.9	Upper Marker	113.00
11	14,369	0.00	0.0		116.83
12	16,933	0.00	0.0		119.28
13	17,503	0.00	0.0		119.83
14	20,352	0.00	0.0		122.56
15	23,202	0.00	0.0		125.30
16	27,590	0.00	0.0		129.50
17	28,672	0.00	0.0		130.54


Region table for sample 6 : Ning Chin 1-32

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/μl]	Corr. Area	Molarity [pmol/l]	Co % of Ior Total	Size distribution in CV [%]
200	1,000	660	1,089.21	1,246.4	2,528.2	87	11.8

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\... bioanalyzer\2100 expert\data\2019-03-27\2019-03-27_001.xad

Created: 3/27/2019 10:20:55 AM
 Modified: 3/27/2019 10:56:37 AM

Electropherogram Summary Continued ...

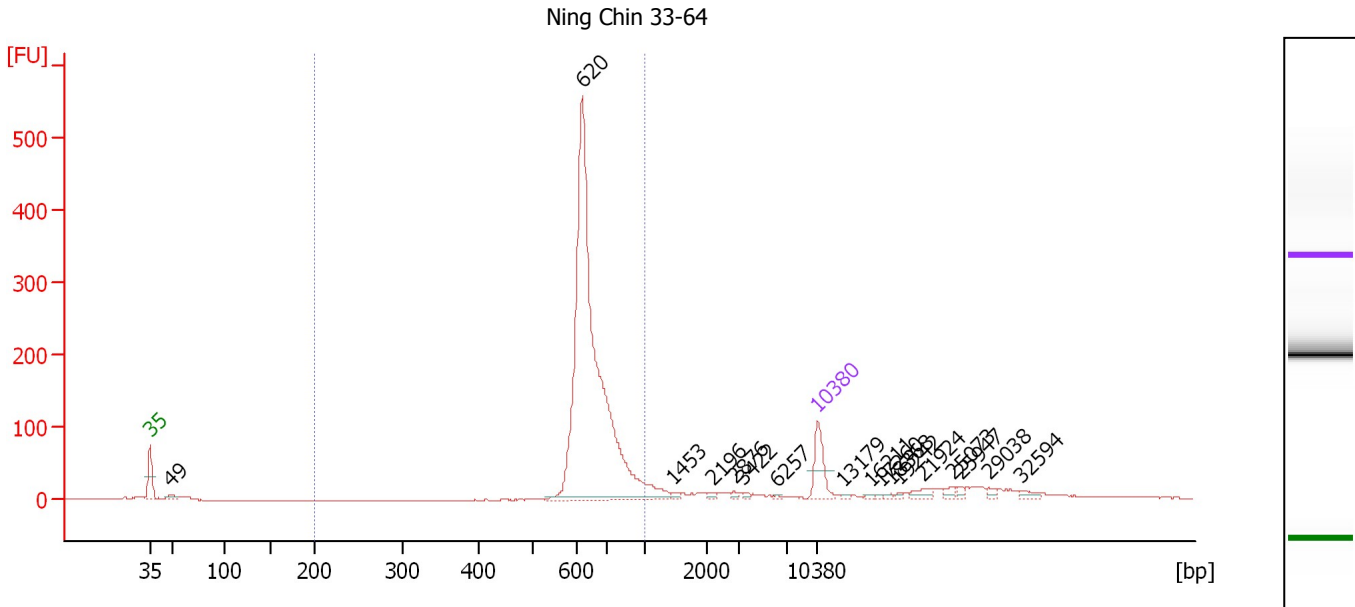

Overall Results for sample 7 : Ning Chin 33-64

Number of peaks found: 17 Corr. Area 1: 1,464.4
 Noise: 0.5

Peak table for sample 7 : Ning Chin 33-64

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	49	21.93	677.0		45.18
3	620	1,427.73	3,488.1		88.34
4	1,453	8.76	9.1		97.79
5	2,196	6.85	4.7		101.99
6	2,876	6.57	3.5		104.22
7	3,422	4.83	2.1		105.17
8	6,257	3.65	0.9		108.81
9	10,380	75.00	10.9	Upper Marker	113.00
10	13,179	0.00	0.0		115.68
11	16,211	0.00	0.0		118.59
12	17,260	0.00	0.0		119.60
13	18,368	0.00	0.0		120.66
14	19,242	0.00	0.0		121.50
15	21,924	0.00	0.0		124.07
16	25,073	0.00	0.0		127.09
17	25,947	0.00	0.0		127.93
18	29,038	0.00	0.0		130.89
19	32,594	0.00	0.0		134.30


Region table for sample 7 : Ning Chin 33-64

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/μl]	Corr. Area	Molarity [pmol/l]	Co % of Ior Total	Size distribution in CV [%]
200	1,000	660	1,356.34	1,464.4	3,146.2	81	11.8

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\... bioanalyzer\2100 expert\data\2019-03-27\2019-03-27_001.xad

Created: 3/27/2019 10:20:55 AM
 Modified: 3/27/2019 10:56:37 AM

Electropherogram Summary Continued ...

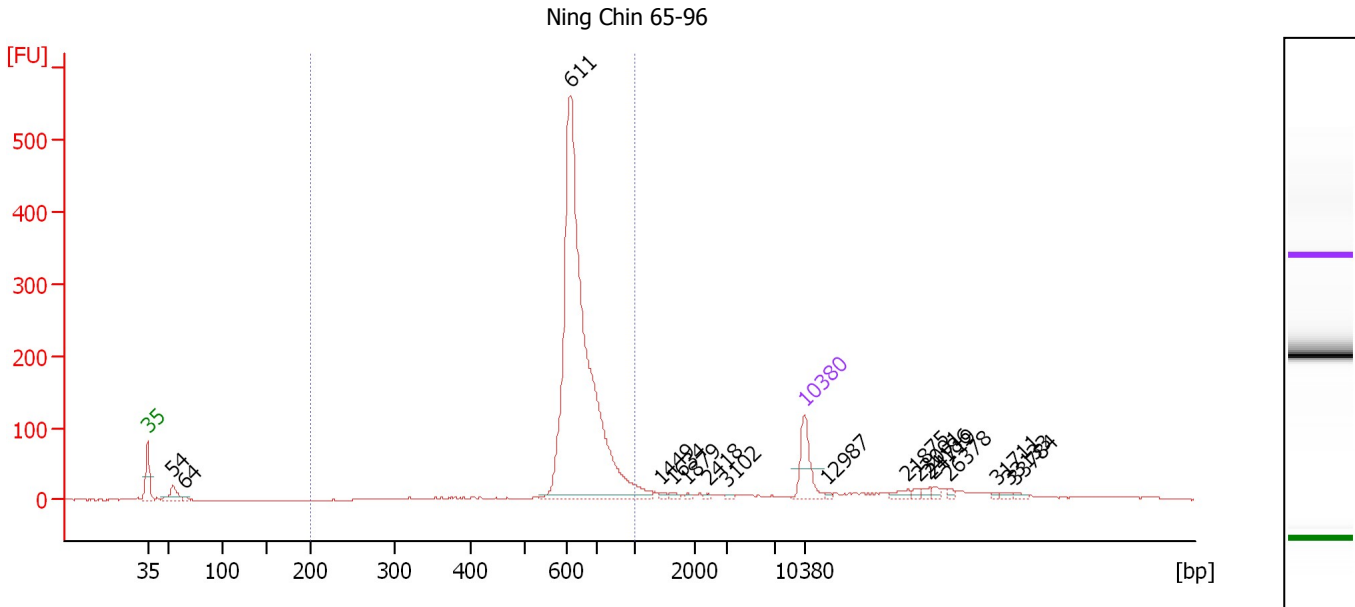

Overall Results for sample 8 : Ning Chin 65-96

Number of peaks found: 17 Corr. Area 1: 1,687.0
 Noise: 0.5

Peak table for sample 8 : Ning Chin 65-96

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	54	51.45	1,453.3		45.73
3	64	8.53	202.3		46.86
4	611	1,328.37	3,293.0		88.06
5	1,449	4.81	5.0		97.77
6	1,634	5.08	4.7		98.97
7	1,879	3.57	2.9		100.56
8	2,418	3.05	1.9		102.72
9	3,102	3.19	1.6		104.76
10	10,380	75.00	10.9	Upper Marker	113.00
11	12,987	0.00	0.0		115.50
12	21,875	0.00	0.0		124.02
13	23,001	0.00	0.0		125.10
14	24,186	0.00	0.0		126.24
15	24,719	0.00	0.0		126.75
16	26,378	0.00	0.0		128.34
17	31,711	0.00	0.0		133.45
18	33,133	0.00	0.0		134.82
19	33,784	0.00	0.0		135.44


Region table for sample 8 : Ning Chin 65-96

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/μl]	Corr. Area	Molarity [pmol/l]	Co % of Ior Total	Size distribution in CV [%]
200	1,000	648	1,365.91	1,687.0	3,271.3	81	13.3

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\... bioanalyzer\2100 expert\data\2019-03-27\2019-03-27_001.xad

Created: 3/27/2019 10:20:55 AM
 Modified: 3/27/2019 10:56:37 AM

Electropherogram Summary Continued ...

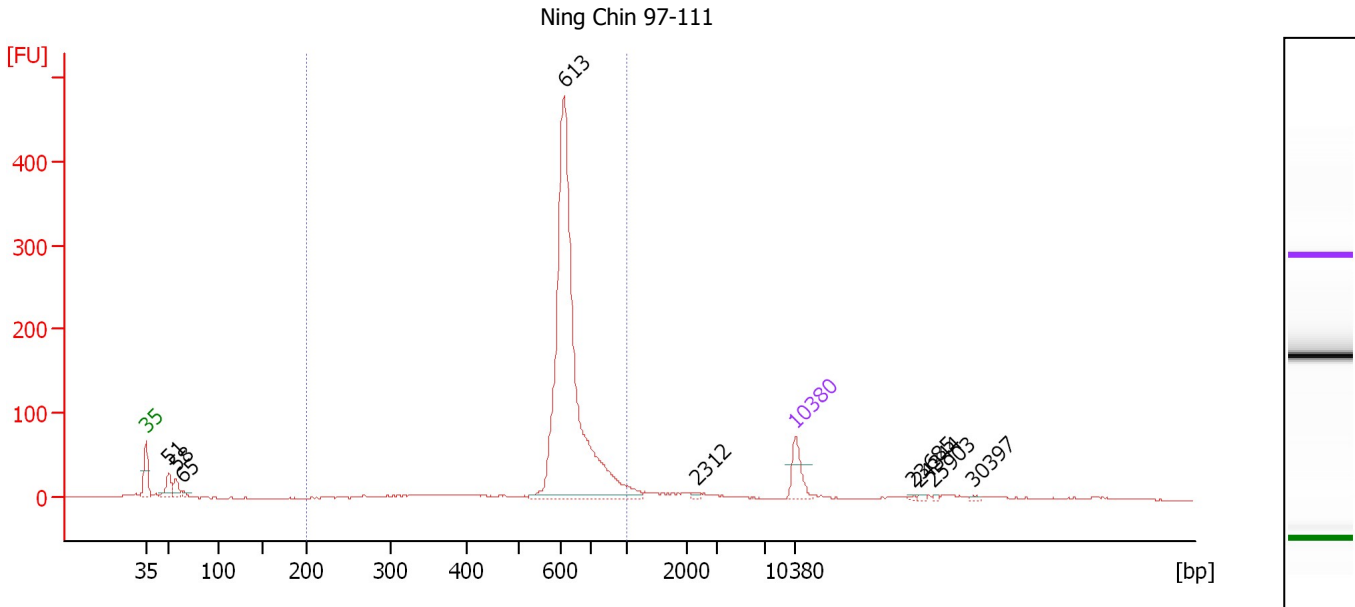

Overall Results for sample 9 : Ning Chin 97-111

Number of peaks found: 9 Corr. Area 1: 1,258.4
 Noise: 0.6

Peak table for sample 9 : Ning Chin 97-111

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	51	84.60	2,522.1		45.41
3	58	59.50	1,552.8		46.22
4	65	17.33	405.5		46.97
5	613	1,557.97	3,850.7		88.11
6	2,312	7.46	4.9		102.37
7	10,380	75.00	10.9	Upper Marker	113.00
8	23,685	0.00	0.0		125.76
9	24,344	0.00	0.0		126.39
10	25,903	0.00	0.0		127.89
11	30,397	0.00	0.0		132.20


Region table for sample 9 : Ning Chin 97-111

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/μl]	Corr. Area	Molarity [pmol/l]	Co % of lor Total	Size distribution in CV [%]
200	1,000	632	1,606.74	1,258.4	3,983.3	83	14.4

Assay Class: High Sensitivity DNA Assay
Data Path: C:\... bioanalyzer\2100 expert\data\2019-03-27\2019-03-27_001.xad

Created: 3/27/2019 10:20:55 AM
Modified: 3/27/2019 10:56:37 AM

Gel Image

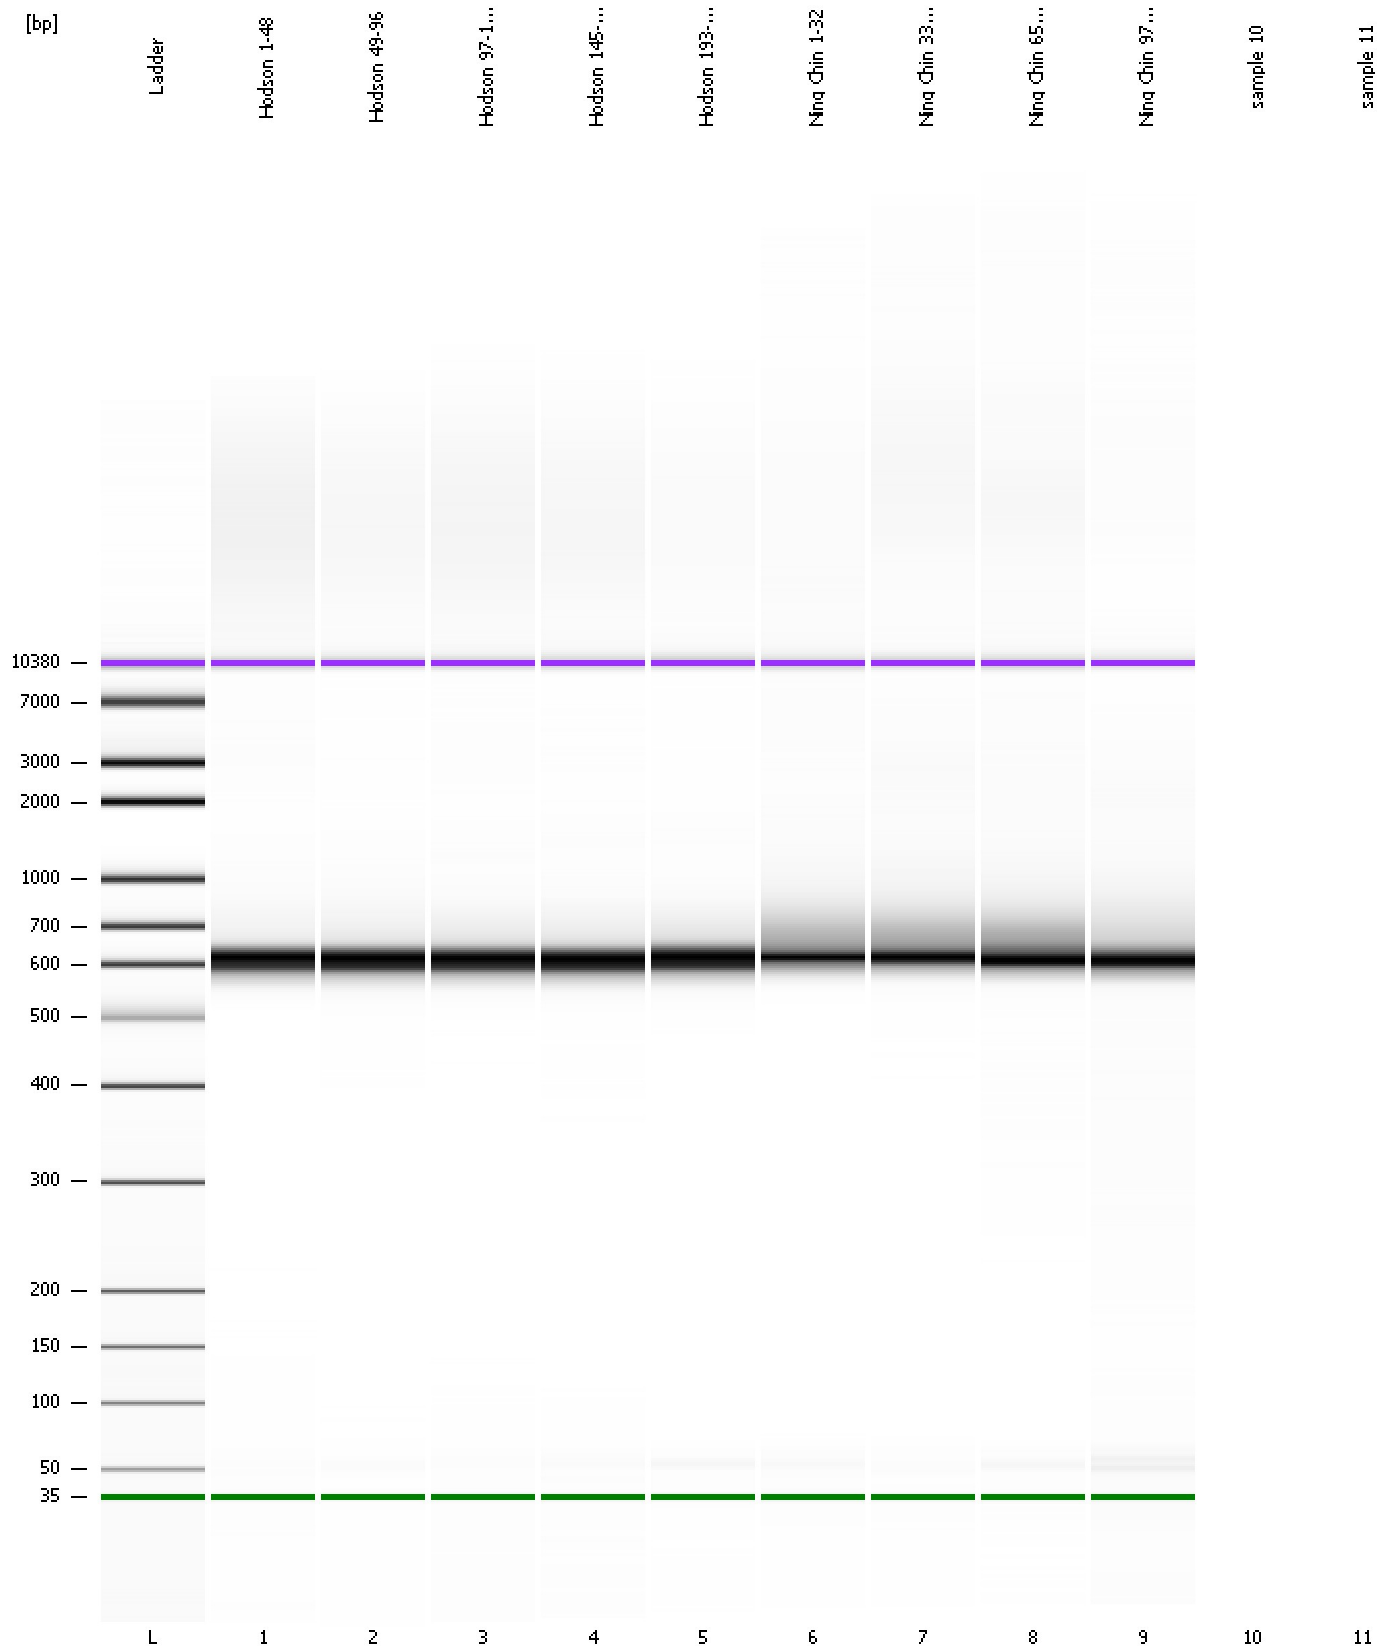


Assay Class: High Sensitivity DNA Assay
Data Path: C:\... bioanalyzer\2100 expert\data\2019-03-27\2019-03-27_001.xad

Created: 3/27/2019 10:20:55 AM
Modified: 3/27/2019 10:56:37 AM

Curves

Standard Curve

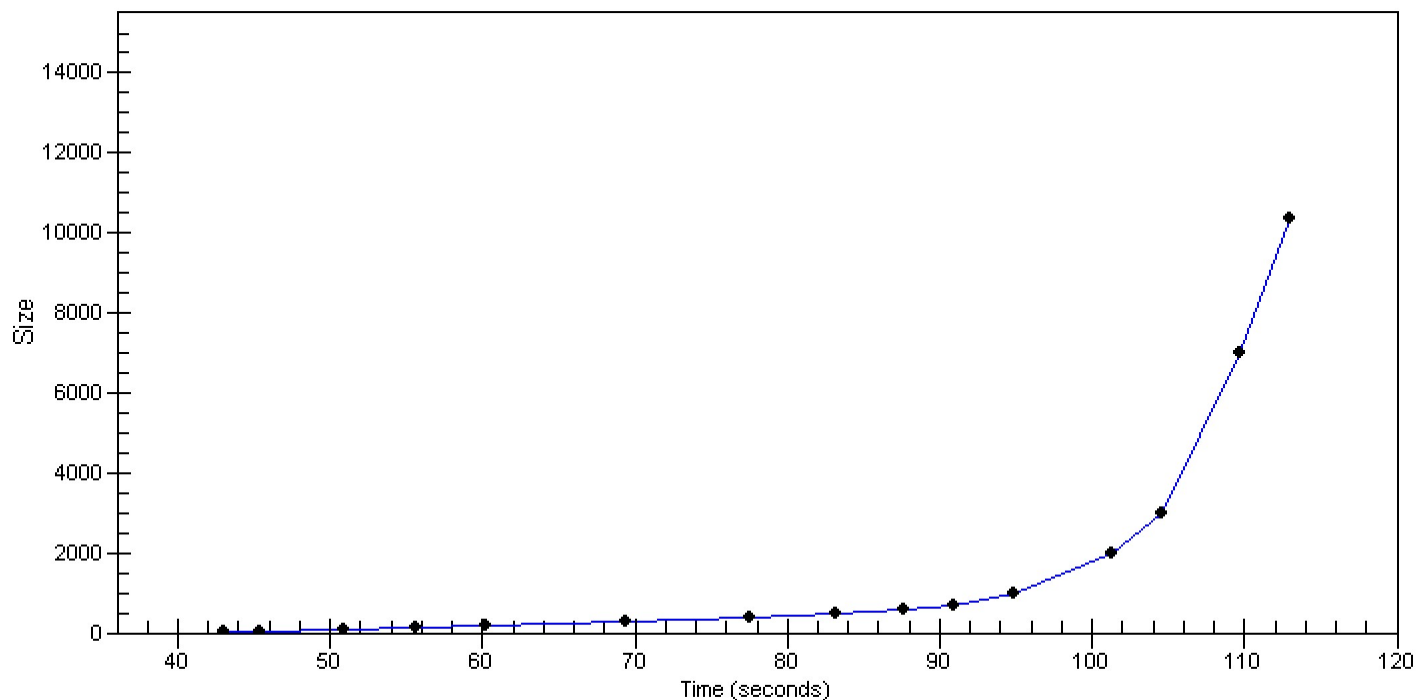

Assay Class: High Sensitivity DNA Assay
Data Path: C:\... bioanalyzer\2100 expert\data\2019-03-27\2019-03-27_001.xad

Created: 3/27/2019 10:20:55 AM
Modified: 3/27/2019 10:56:37 AM

Invalid Samples

Sample 10 has not been run, no results available.

Sample 11 has not been run, no results available.

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\... bioanalyzer\2100 expert\data\2019-03-27\2019-03-27_001.xad

Created: 3/27/2019 10:20:55 AM
 Modified: 3/27/2019 10:56:37 AM

Run Logbook

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 10)		Instrument	Run		3/27/2019 10:56:29 AM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Run started on port 1 (File: C:\Program Files\Agilent\2100 bioanalyzer\2100 expert\data\2019-03-27\2019-03-27_001.xad)		Instrument	Run		3/27/2019 10:21:00 AM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Product Number : G2938C		Instrument	Run		3/27/2019 10:21:00 AM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Name :		Instrument	Run		3/27/2019 10:21:00 AM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Vendor : Agilent Technologies		Instrument	Run		3/27/2019 10:21:00 AM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Serial# : DE34903152		Instrument	Run		3/27/2019 10:21:00 AM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Firmware : C.01.069		Instrument	Run		3/27/2019 10:21:00 AM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Cartridge : Electrode		Instrument	Run		3/27/2019 10:21:00 AM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1