


Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...a\2019-09-24\2019-09-24\_001\_AmpliconQC\_MiSeq901\_903\_904.xad

Created: 9/24/2019 9:53:07 AM  
Modified: 9/26/2019 9:44:14 AM

**Electrophoresis File Run Summary**

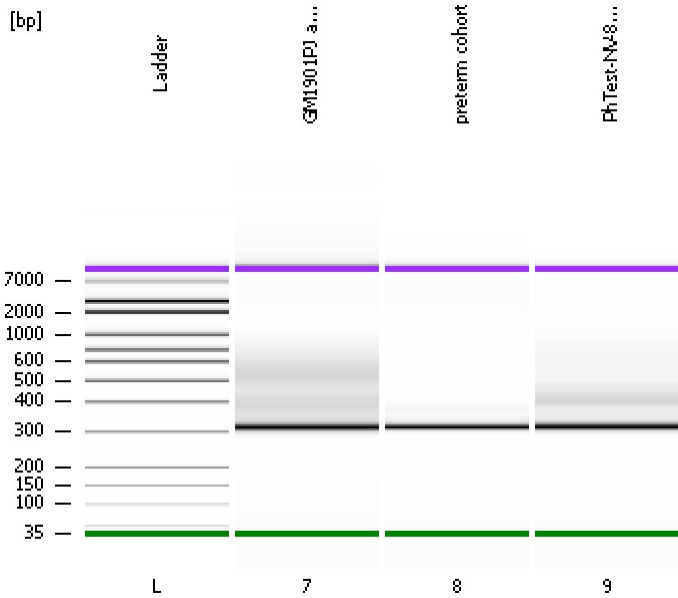

Instrument Information:




Instrument Name: DE34903152      Firmware: C.01.069  
Serial#: DE34903152      Type: G2938C

Assay Information:

Assay Origin Path: C:\Program Files\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy  
Assay Class: High Sensitivity DNA Assay  
Version: 1.03  
Assay Comments: Copyright © 2003-2010 Agilent Technologies

Chip Information:

Chip Lot #:  
Reagent Kit Lot #:  
Chip Comments:

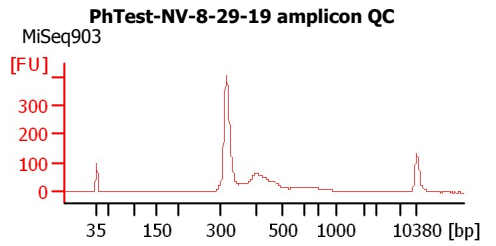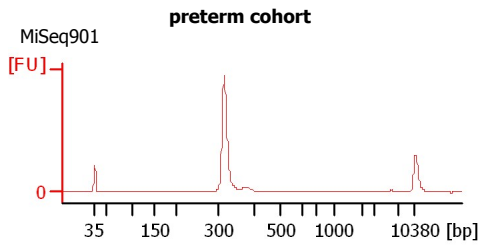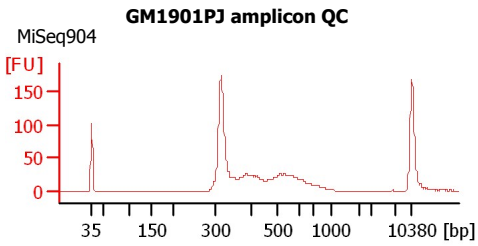

Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...a\2019-09-24\2019-09-24\_001\_AmpliconQC\_MiSeq901\_903\_904.xad

Created: 9/24/2019 9:53:07 AM  
Modified: 9/26/2019 9:44:14 AM

**Electrophoresis File Run Summary (Chip Summary)**

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
GM1901PJ amplicon QC	MiSeq904	<input type="checkbox"/>	✓			
preterm cohort	MiSeq901	<input type="checkbox"/>	✓			
PhTest-NV-8-29-19 amplicon QC	MiSeq903	<input type="checkbox"/>	✓			
Ladder		<input type="checkbox"/>	✓			

**Chip Lot #****Reagent Kit Lot #****Chip Comments :**

Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...a\2019-09-24\2019-09-24\_001\_AmpliconQC\_MiSeq901\_903\_904.xad

Created: 9/24/2019 9:53:07 AM  
Modified: 9/26/2019 9:44:14 AM

**Electrophoresis Assay Details**

**General Analysis Settings**

Number of Available Sample and Ladder Wells (Max.) : 12  
Minimum Visible Range [s] : 32  
Maximum Visible Range [s] : 138  
Start Analysis Time Range [s] : 33  
End Analysis Time Range [s] : 137.5  
Ladder Concentration [pg/μl] : 1950  
Uses Standard Area for Ladder Fragments  
Lower Marker Concentration [pg/μl] : 125  
Upper Marker Concentration [pg/μl] : 75  
Used Upper Marker for Quantitation  
Standard Curve Fit is Point to Point  
Show Data Aligned to Lower and Upper Marker

**Integrator Settings**

Integration Start Time [s] : 33.05  
Integration End Time [s] : 137  
Slope Threshold : 0.8  
Height Threshold [FU] : 5  
Area Threshold : 0.1  
Width Threshold [s] : 0.6  
Baseline Plateau [s] : 0.5

**Filter Settings**

Filter Width [s] : 0.5  
Polynomial Order : 4


**Ladder**

Ladder Peak	Size	Area
1	35	160
2	50	210
3	100	208
4	150	221
5	200	242
6	300	270
7	400	305
8	500	306
9	600	336
10	700	321
11	1000	366
12	2000	413
13	3000	411
14	7000	400
15	10380	214

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...a\2019-09-24\2019-09-24\_001\_AmpliconQC\_MiSeq901\_903\_904.xad

Created: 9/24/2019 9:53:07 AM  
 Modified: 9/26/2019 9:44:14 AM

**Electropherogram Summary**

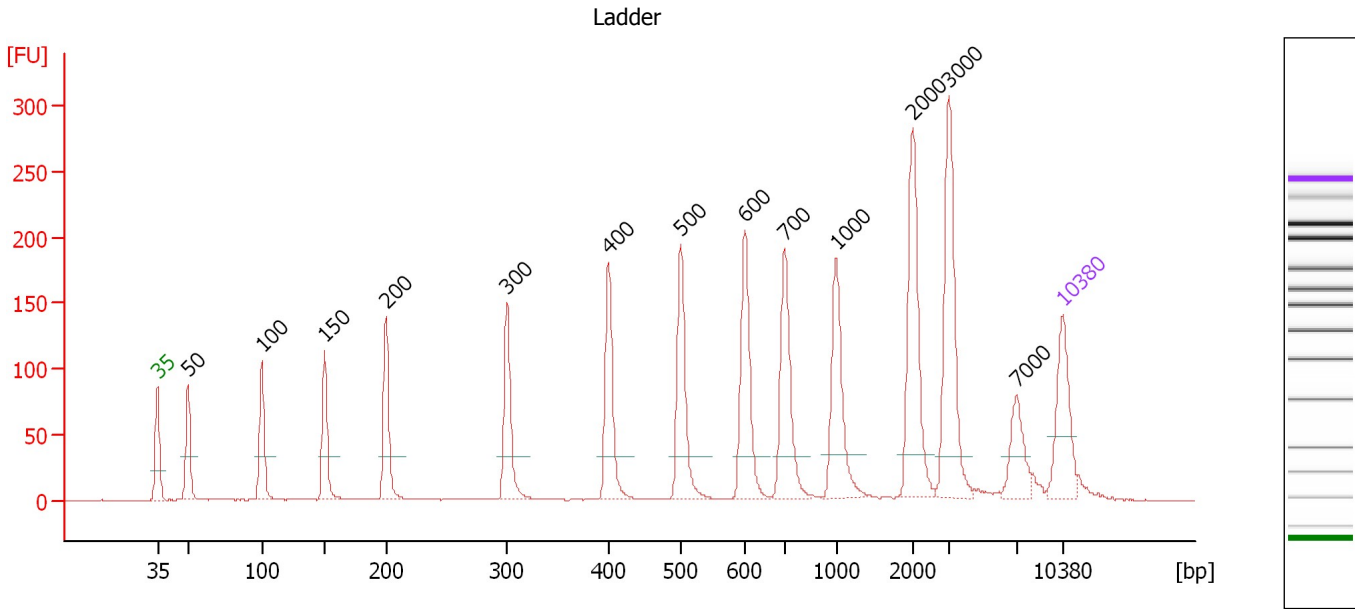

**Overall Results for Ladder**

Noise: 0.2


**Peak table for Ladder**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	50	150.00	4,545.5	Ladder Peak	45.33
3	100	150.00	2,272.7	Ladder Peak	51.04
4	150	150.00	1,515.2	Ladder Peak	55.93
5	200	150.00	1,136.4	Ladder Peak	60.65
6	300	150.00	757.6	Ladder Peak	70.03
7	400	150.00	568.2	Ladder Peak	77.84
8	500	150.00	454.5	Ladder Peak	83.46
9	600	150.00	378.8	Ladder Peak	88.39
10	700	150.00	324.7	Ladder Peak	91.49
11	1,000	150.00	227.3	Ladder Peak	95.44
12	2,000	150.00	113.6	Ladder Peak	101.37
13	3,000	150.00	75.8	Ladder Peak	104.15
14	7,000	150.00	32.5	Ladder Peak	109.41
15	10,380	75.00	10.9	Upper Marker	113.00

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...a\2019-09-24\2019-09-24\_001\_AmpliconQC\_MiSeq901\_903\_904.xad

Created: 9/24/2019 9:53:07 AM  
 Modified: 9/26/2019 9:44:14 AM

**Electropherogram Summary Continued ...**

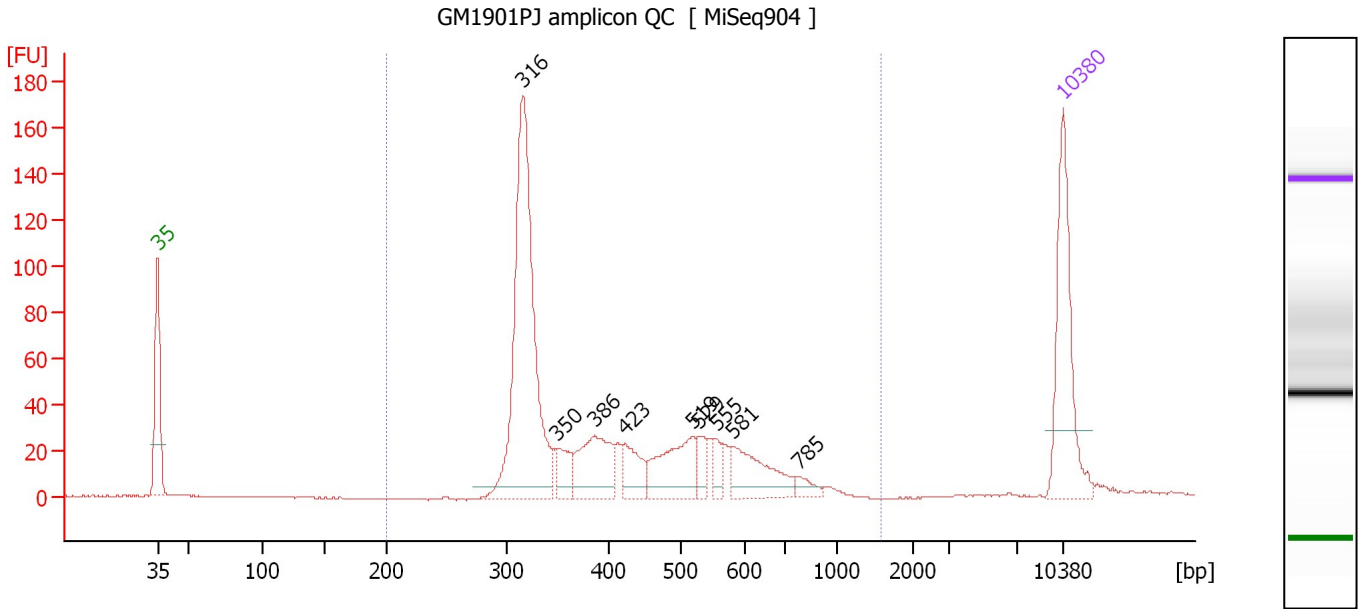

**Overall Results for sample 7 : GM1901PJ amplicon QC**

Number of peaks found: 9                      Corr. Area 1: 924.9  
 Noise: 0.3

**Peak table for sample 7 : GM1901PJ amplicon QC**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	316	278.64	1,336.4		71.27
3	350	22.76	98.6		73.90
4	386	60.06	235.5		76.79
5	423	29.18	104.6		79.11
6	519	55.58	162.4		84.37
7	529	15.45	44.3		84.88
8	555	11.59	31.6		86.19
9	581	47.17	123.0		87.46
10	785	8.33	16.1		92.62
11	10,380	75.00	10.9	Upper Marker	113.00


**Region table for sample 7 : GM1901PJ amplicon QC**

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/μl]	Corr. Area	Molarity [pmol/l]	Co % of Ior Total	Size distribution in CV [%]
200	1,597	432	560.28	924.9	2,205.8	94	33.6

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...a\2019-09-24\2019-09-24\_001\_AmpliconQC\_MiSeq901\_903\_904.xad

Created: 9/24/2019 9:53:07 AM  
 Modified: 9/26/2019 9:44:14 AM

**Electropherogram Summary Continued ...**

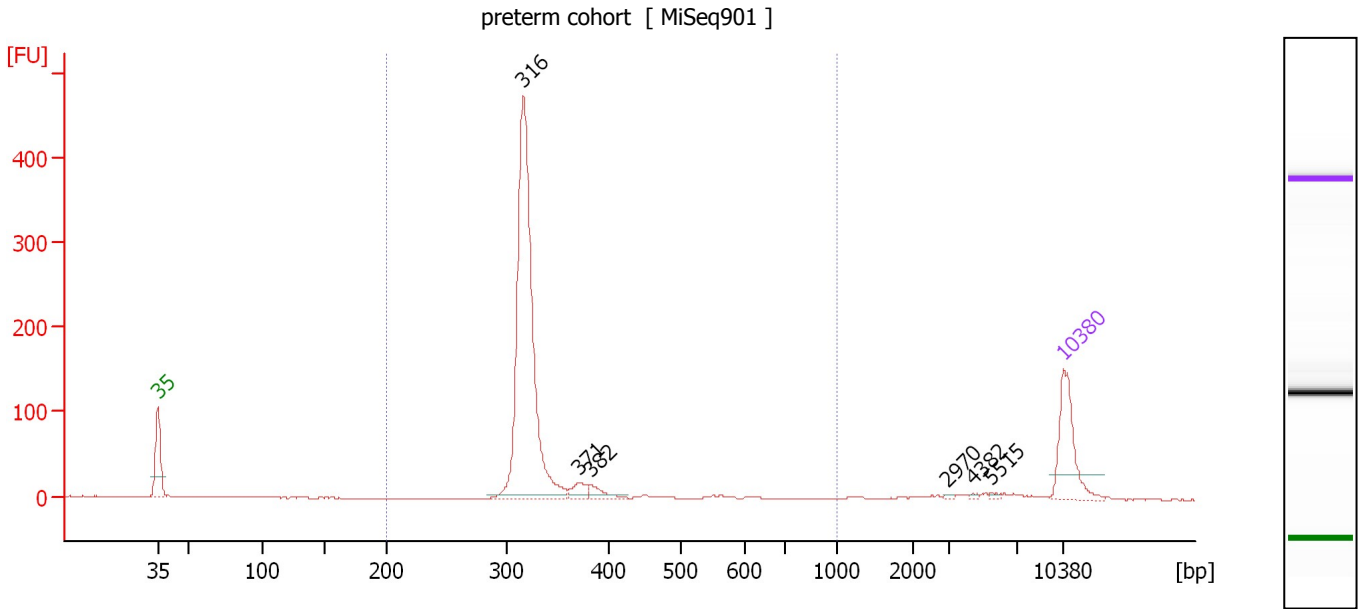

**Overall Results for sample 8 : preterm cohort**

Number of peaks found: 6                      Corr. Area 1: 978.5  
 Noise: 0.3

**Peak table for sample 8 : preterm cohort**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	316	589.53	2,827.0		71.28
3	371	19.01	77.6		75.59
4	382	17.26	68.4		76.46
5	2,970	1.80	0.9		104.07
6	4,382	1.88	0.6		105.97
7	5,515	2.79	0.8		107.46
8	10,380	75.00	10.9	Upper Marker	113.00


**Region table for sample 8 : preterm cohort**

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/μl]	Corr. Area	Molarity [pmol/l]	Co % of Ior Total	Size distribution in CV [%]
200	1,000	327	623.54	978.5	2,909.8	94	11.1

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...a\2019-09-24\2019-09-24\_001\_AmpliconQC\_MiSeq901\_903\_904.xad

Created: 9/24/2019 9:53:07 AM  
 Modified: 9/26/2019 9:44:14 AM

**Electropherogram Summary Continued ...**

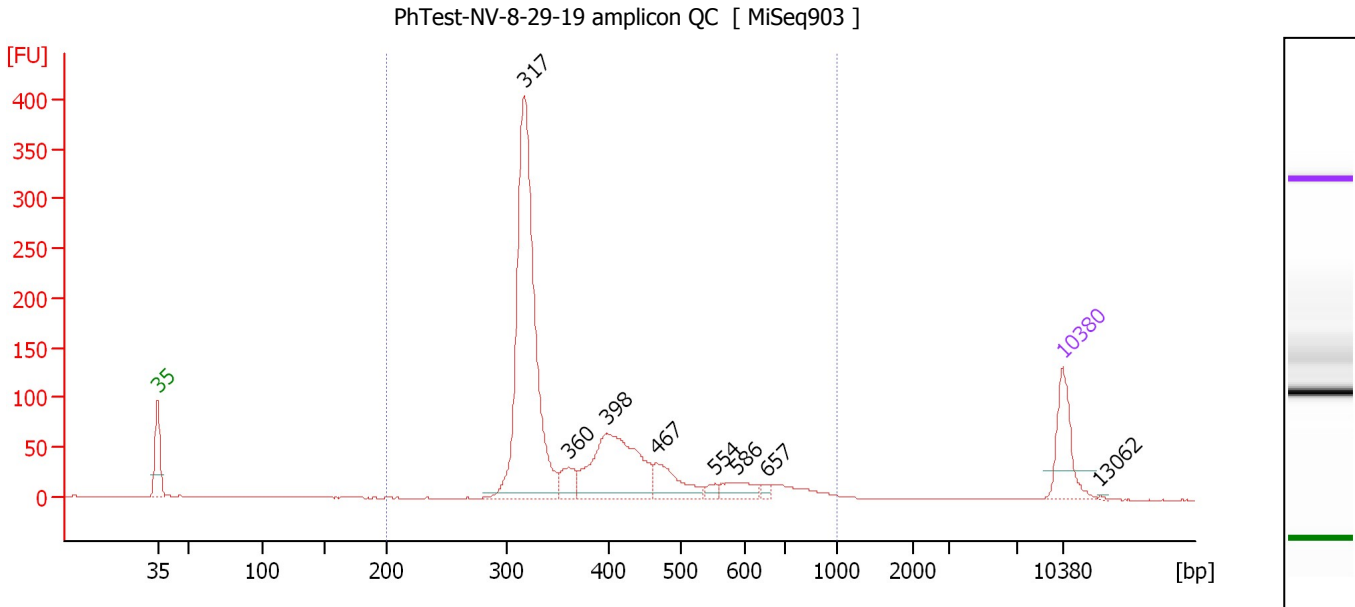

**Overall Results for sample 9 : PhTest-NV-8-29-19 amplicon QC**

Number of peaks found: 8                      Corr. Area 1: 1,578.1  
 Noise: 0.2

**Peak table for sample 9 : PhTest-NV-8-29-19 amplicon QC**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations	Aligned Migration Time [s]
1	35	125.00	5,411.3	Lower Marker	43.00
2	317	719.18	3,432.5		71.39
3	360	42.50	178.9		74.71
4	398	258.49	984.8		77.66
5	467	72.61	235.6		81.60
6	554	11.27	30.9		86.11
7	586	35.60	92.0		87.72
8	657	8.45	19.5		90.15
9	10,380	75.00	10.9	Upper Marker	113.00
10	13,062	0.00	0.0		115.85


**Region table for sample 9 : PhTest-NV-8-29-19 amplicon QC**

From [bp]	To [bp]	Average Size [bp]	Conc. [pg/μl]	Corr. Area	Molarity [pmol/l]	Co % of lor Total	Size distribution in CV [%]
200	1,000	392	1,175.01	1,578.1	4,907.8	99	29.1

Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...a\2019-09-24\2019-09-24\_001\_AmpliconQC\_MiSeq901\_903\_904.xad

Created: 9/24/2019 9:53:07 AM  
Modified: 9/26/2019 9:44:14 AM

**Gel Image**

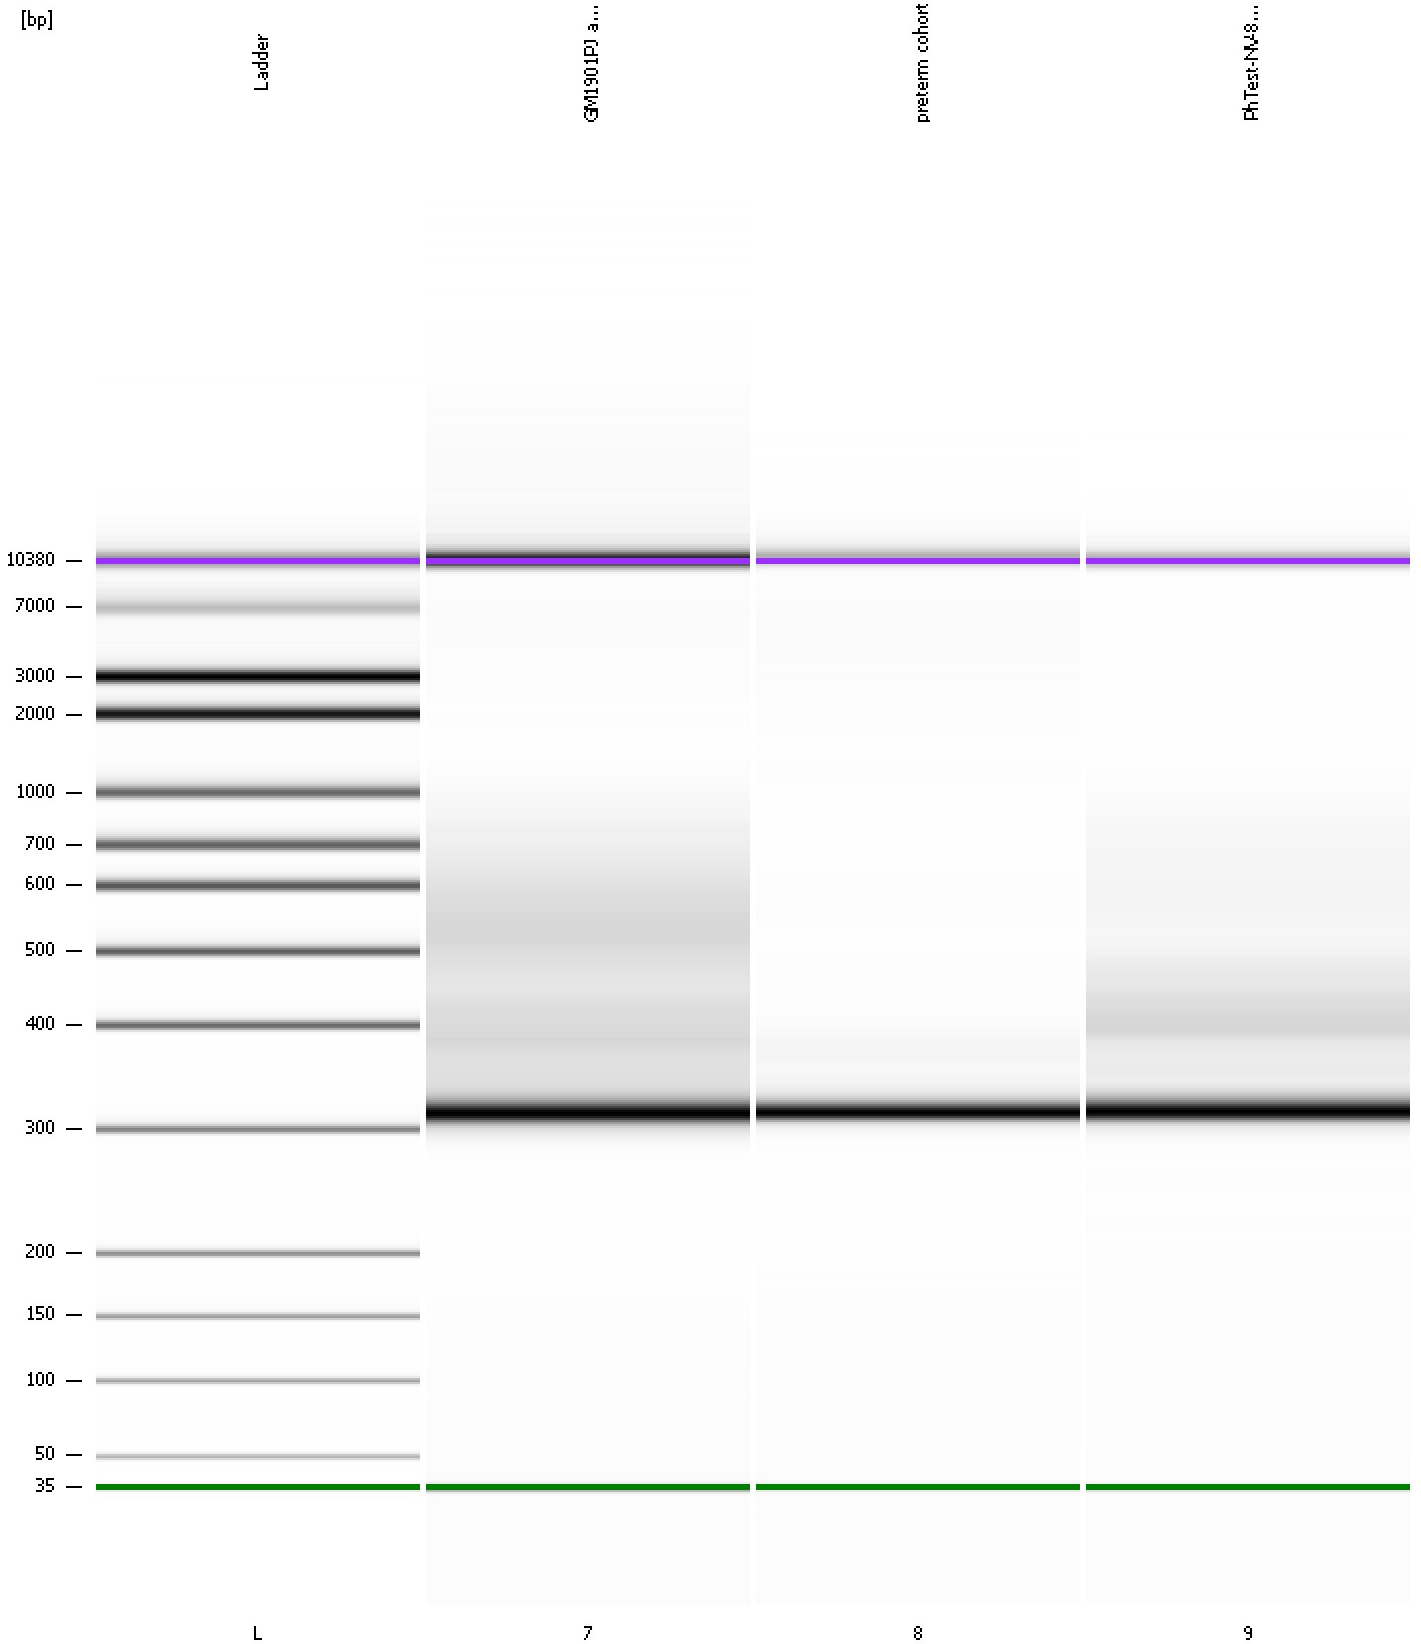




Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...a\2019-09-24\2019-09-24\_001\_AmpliconQC\_MiSeq901\_903\_904.xad

Created: 9/24/2019 9:53:07 AM  
Modified: 9/26/2019 9:44:14 AM

### Curves

#### Standard Curve

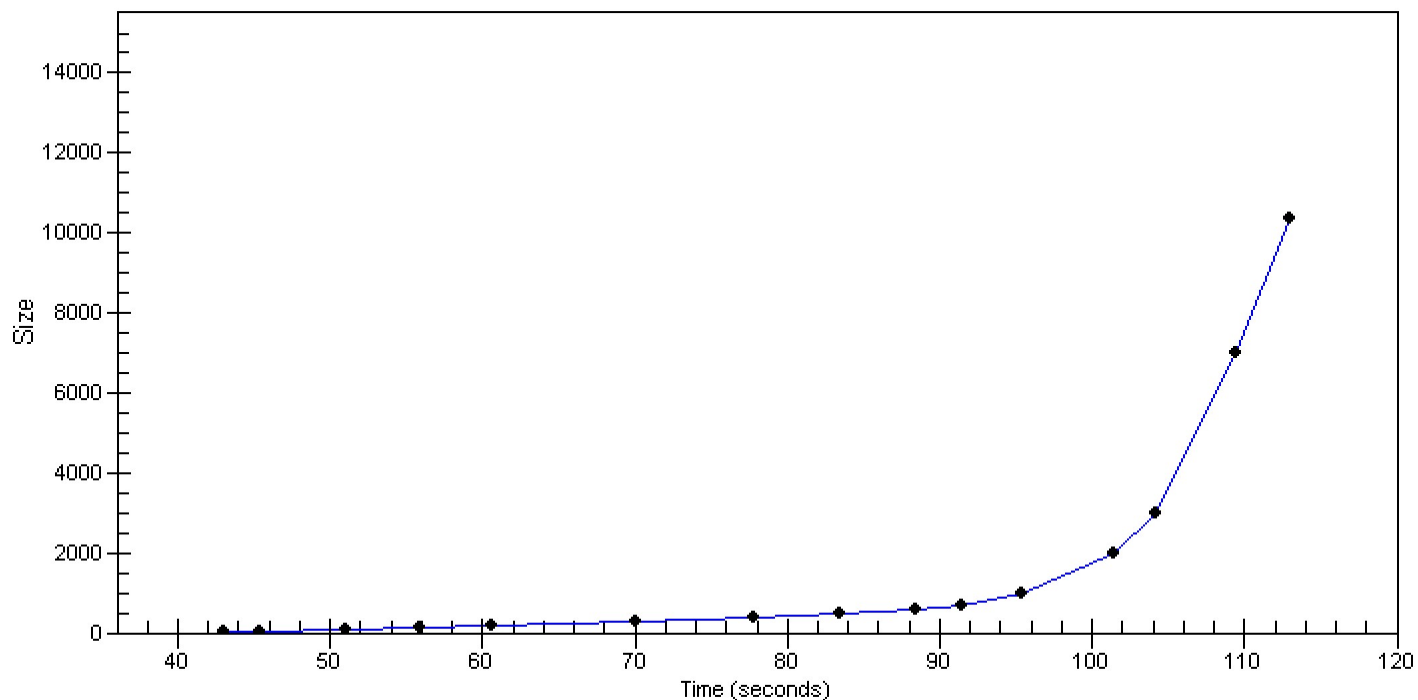

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...a\2019-09-24\2019-09-24\_001\_AmpliconQC\_MiSeq901\_903\_904.xad

Created: 9/24/2019 9:53:07 AM  
 Modified: 9/26/2019 9:44:14 AM

**Run Logbook**

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 12)		Instrument	Run		9/24/2019 10:34:23 AM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Run started on port 1 (File: C:\Program Files\Agilent\2100 bioanalyzer\2100 expert\data\2019-09-24\2019-09-24_001.xad)		Instrument	Run		9/24/2019 9:53:12 AM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Product Number : G2938C		Instrument	Run		9/24/2019 9:53:12 AM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Name :		Instrument	Run		9/24/2019 9:53:12 AM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Vendor : Agilent Technologies		Instrument	Run		9/24/2019 9:53:12 AM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Serial# : DE34903152		Instrument	Run		9/24/2019 9:53:12 AM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Firmware : C.01.069		Instrument	Run		9/24/2019 9:53:12 AM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Cartridge : Electrode		Instrument	Run		9/24/2019 9:53:12 AM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1