


Assay Class: High Sensitivity DNA Assay
Data Path: C:\...ents and Settings\Bioanalyzer\2013-07-26\2013-07-26_003.xad

Created: 7/26/2013 4:30:49 PM
Modified: 7/26/2013 5:12:08 PM

Electrophoresis File Run Summary

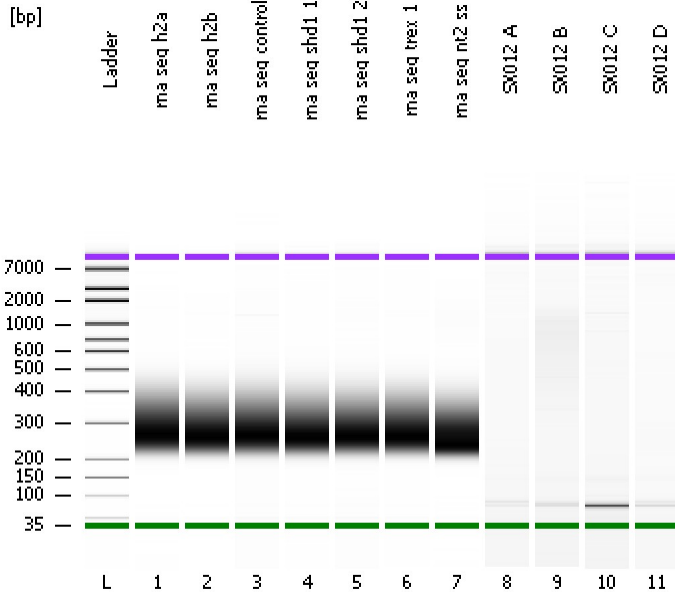

Instrument Information:


Instrument Name: DE13701086 Firmware: C.01.069
Serial#: DE13701086 Type: G2938B

Assay Information:

Assay Origin Path: C:\Program Files\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy
Assay Class: High Sensitivity DNA Assay
Version: 1.03
Assay Comments: Copyright © 2003-2010 Agilent Technologies

Chip Information:

Chip Lot #:
Reagent Kit Lot #:
Chip Comments:

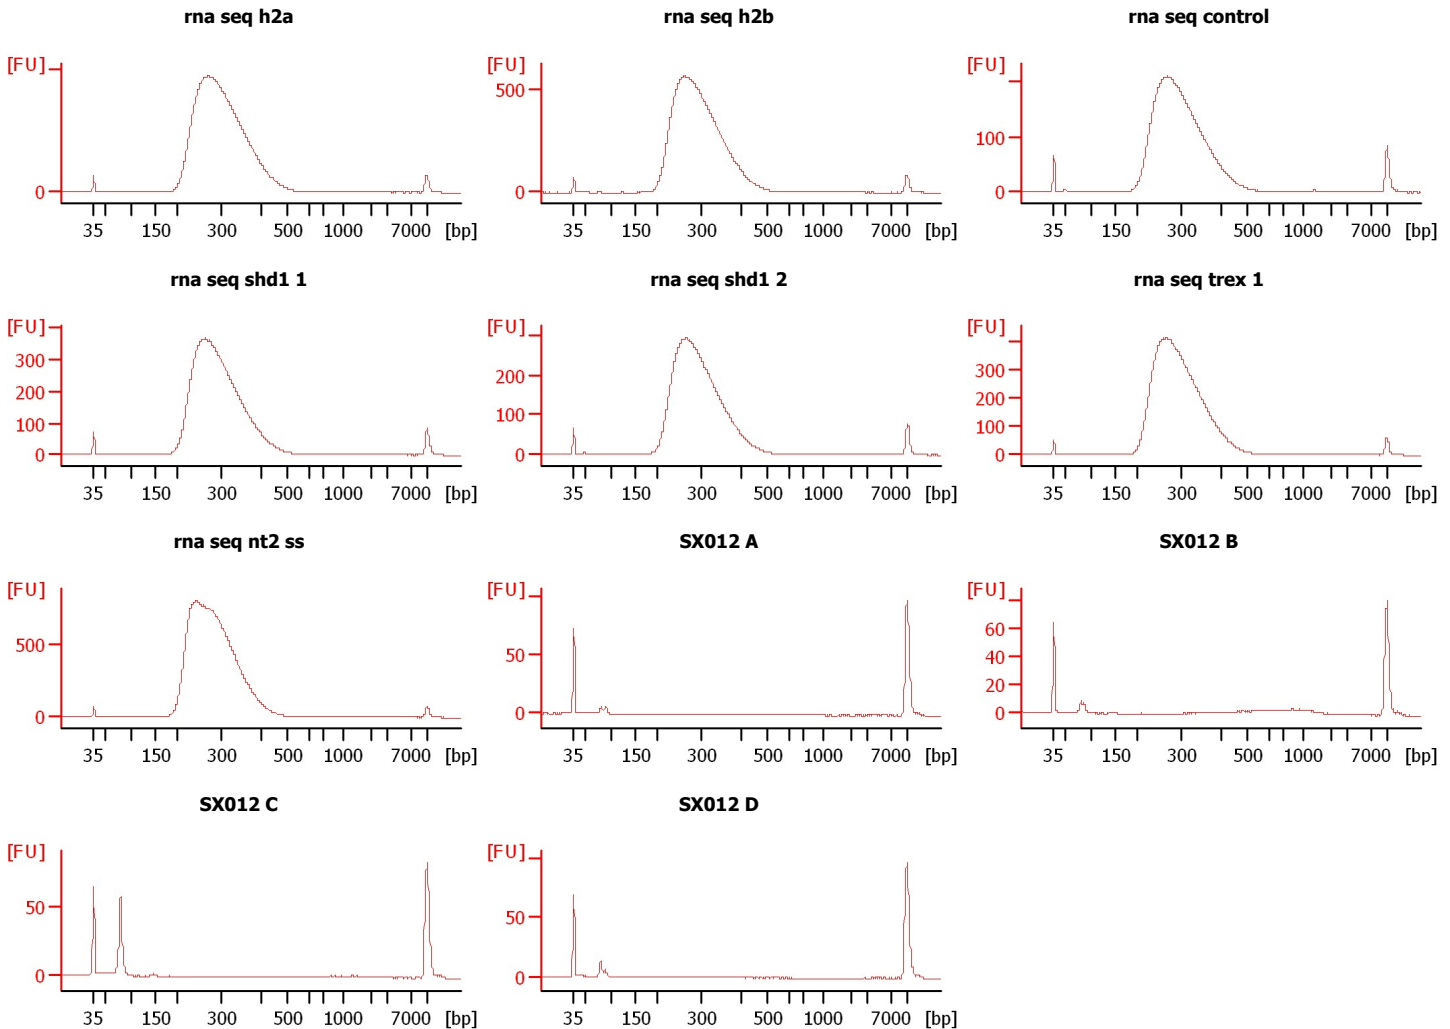

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...ents and Settings\Bioanalyzer\2013-07-26\2013-07-26_003.xad

Created: 7/26/2013 4:30:49 PM
Modified: 7/26/2013 5:12:08 PM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
rna seq h2a		<input type="checkbox"/>	✓			
rna seq h2b		<input type="checkbox"/>	✓			
rna seq control		<input type="checkbox"/>	✓			
rna seq shd1 1		<input type="checkbox"/>	✓			
rna seq shd1 2		<input type="checkbox"/>	✓			
rna seq trex 1		<input type="checkbox"/>	✓			
rna seq nt2 ss		<input type="checkbox"/>	✓			
SX012 A		<input type="checkbox"/>	✓			
SX012 B		<input type="checkbox"/>	✓			
SX012 C		<input type="checkbox"/>	✓			
SX012 D		<input type="checkbox"/>	✓			
Ladder		<input type="checkbox"/>	✓			

Chip Lot #

Reagent Kit Lot #

Chip Comments :

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...ents and Settings\Bioanalyzer\2013-07-26\2013-07-26_003.xad

Created: 7/26/2013 4:30:49 PM
Modified: 7/26/2013 5:12:08 PM

Electrophoresis Assay Details

General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12
Minimum Visible Range [s] : 32
Maximum Visible Range [s] : 138
Start Analysis Time Range [s] : 33
End Analysis Time Range [s] : 137.5
Ladder Concentration [pg/μl] : 1950
Uses Standard Area for Ladder Fragments
Lower Marker Concentration [pg/μl] : 125
Upper Marker Concentration [pg/μl] : 75
Used Upper Marker for Quantitation
Standard Curve Fit is Point to Point
Show Data Aligned to Lower and Upper Marker

Integrator Settings

Integration Start Time [s] : 33.05
Integration End Time [s] : 137
Slope Threshold : 0.8
Height Threshold [FU] : 5
Area Threshold : 0.1
Width Threshold [s] : 0.6
Baseline Plateau [s] : 0.5

Filter Settings

Filter Width [s] : 0.5
Polynomial Order : 4


Ladder

Ladder Peak	Size	Area
1	35	160
2	50	210
3	100	208
4	150	221
5	200	242
6	300	270
7	400	305
8	500	306
9	600	336
10	700	321
11	1000	366
12	2000	413
13	3000	411
14	7000	400
15	10380	214

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2013-07-26\2013-07-26_003.xad

Created: 7/26/2013 4:30:49 PM
 Modified: 7/26/2013 5:12:08 PM

Electropherogram Summary

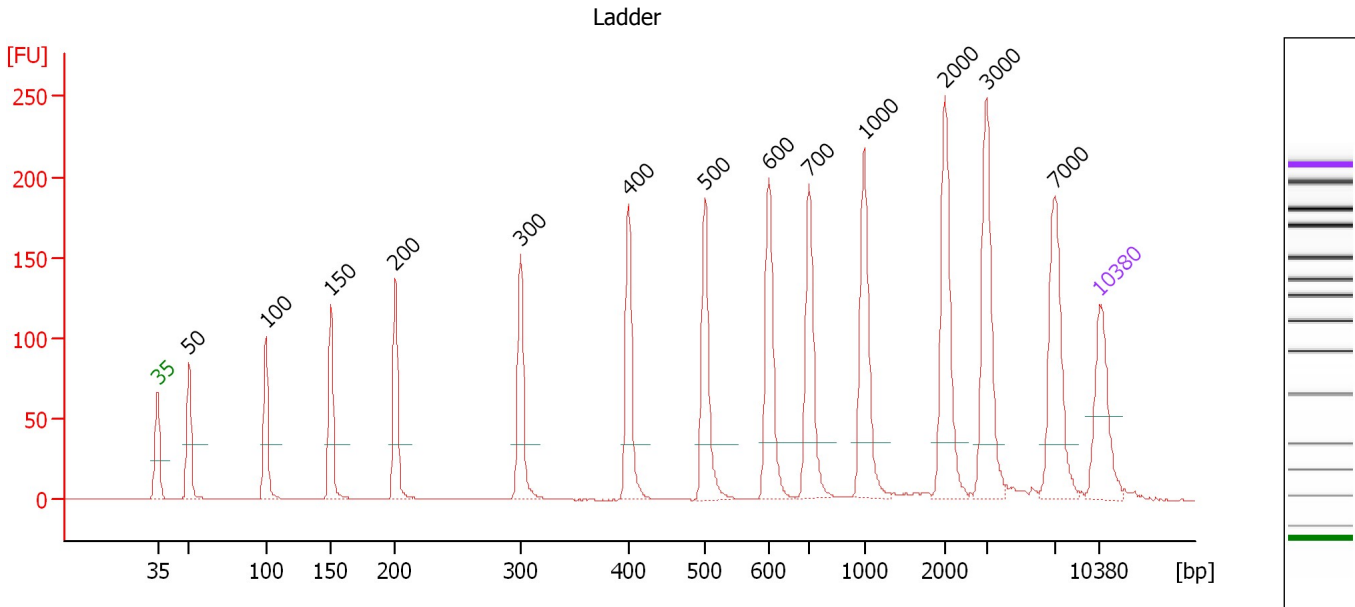

Overall Results for Ladder

Noise: 0.1


Peak table for Ladder

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	50	150.00	4,545.5	Ladder Peak
3	100	150.00	2,272.7	Ladder Peak
4	150	150.00	1,515.2	Ladder Peak
5	200	150.00	1,136.4	Ladder Peak
6	300	150.00	757.6	Ladder Peak
7	400	150.00	568.2	Ladder Peak
8	500	150.00	454.5	Ladder Peak
9	600	150.00	378.8	Ladder Peak
10	700	150.00	324.7	Ladder Peak
11	1,000	150.00	227.3	Ladder Peak
12	2,000	150.00	113.6	Ladder Peak
13	3,000	150.00	75.8	Ladder Peak
14	7,000	150.00	32.5	Ladder Peak
15	10,380	75.00	10.9	Upper Marker

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2013-07-26\2013-07-26_003.xad

Created: 7/26/2013 4:30:49 PM
 Modified: 7/26/2013 5:12:08 PM

Electropherogram Summary Continued ...

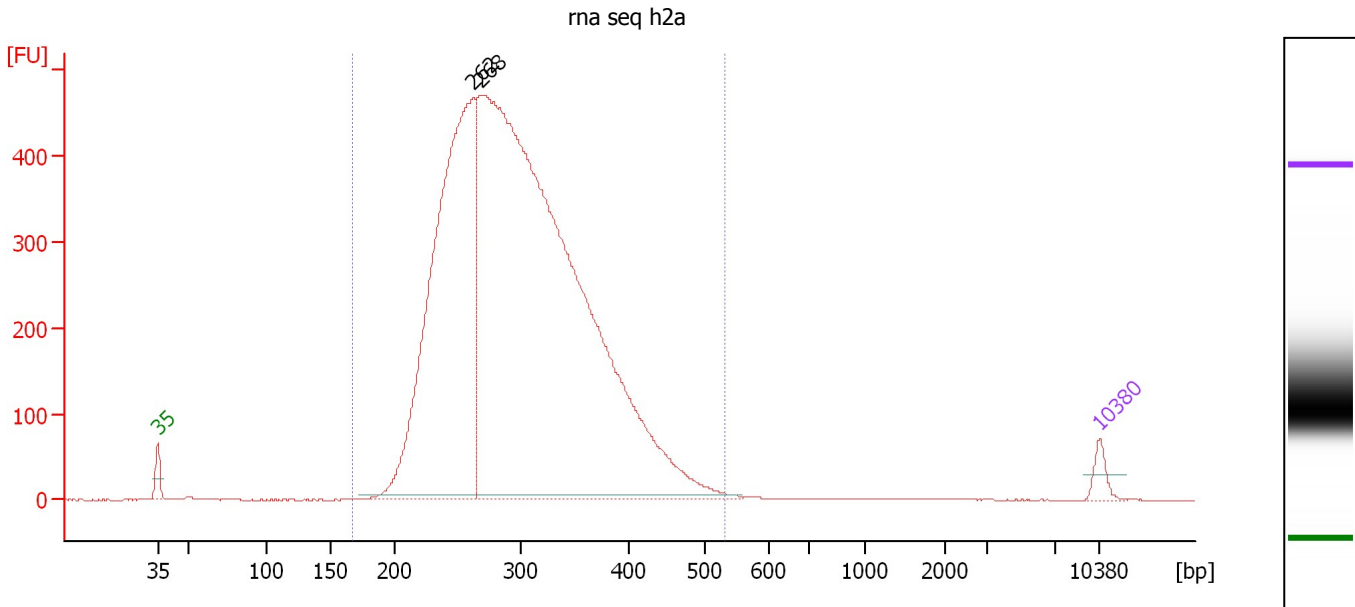

Overall Results for sample 1 : rna seq h2a

Number of peaks found: 2 Corr. Area 1: 8,454.5
 Noise: 0.1

Peak table for sample 1 : rna seq h2a

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	262	4,938.15	28,511.4	
3	268	11,319.46	63,890.9	
4	10,380	75.00	10.9	Upper Marker


Region table for sample 1 : rna seq h2a

From [bp]	To [bp]	Average Size [bp]	Molarity [pmol/l]	Conc. [pg/μl]	Corr. Area	% of Total	Size distribution in CV [%]	Color
166	531	301	79,926.7	15,214.83	8,454.5	99	19.2	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2013-07-26\2013-07-26_003.xad

Created: 7/26/2013 4:30:49 PM
 Modified: 7/26/2013 5:12:08 PM

Electropherogram Summary Continued ...

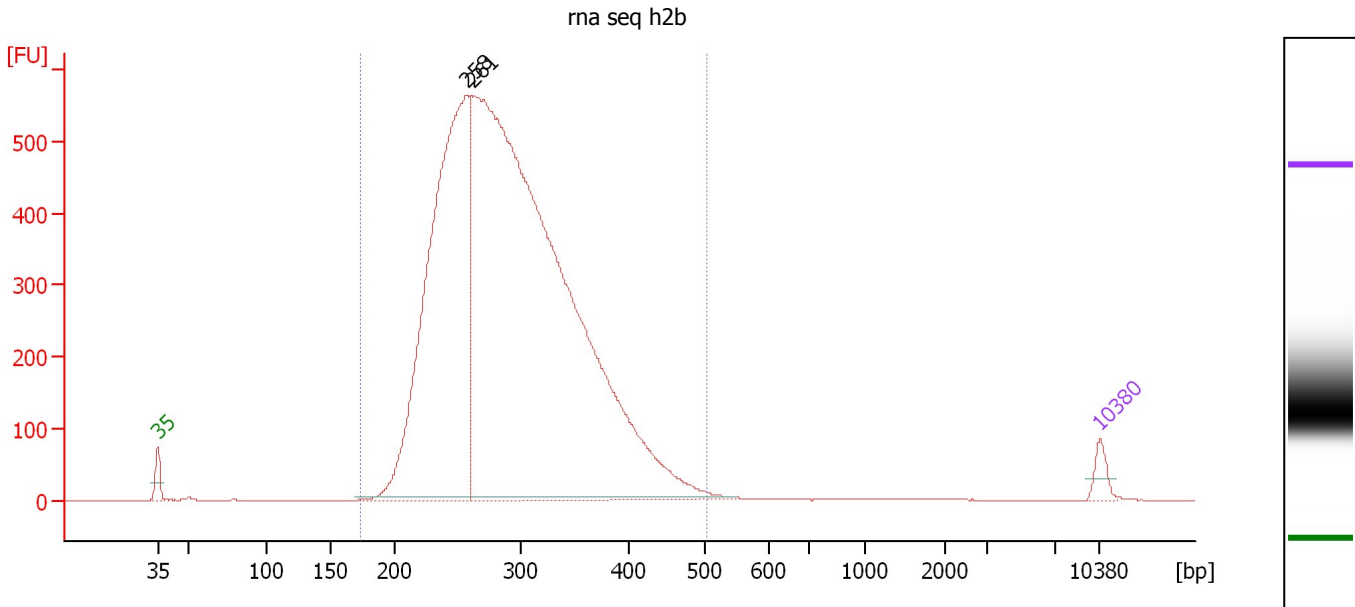

Overall Results for sample 2 : rna seq h2b

Number of peaks found: 2 Corr. Area 1: 9,650.2
 Noise: 0.2

Peak table for sample 2 : rna seq h2b

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	258	4,891.89	28,780.3	
3	261	10,910.44	63,315.4	
4	10,380	75.00	10.9	Upper Marker


Region table for sample 2 : rna seq h2b

From [bp]	To [bp]	Average Size [bp]	Molarity [pmol/l]	Conc. [pg/μl]	Corr. Area	% of Total	Size distribution in CV [%]	Color
173	502	294	78,889.4	14,721.60	9,650.2	99	18.6	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2013-07-26\2013-07-26_003.xad

Created: 7/26/2013 4:30:49 PM
 Modified: 7/26/2013 5:12:08 PM

Electropherogram Summary Continued ...

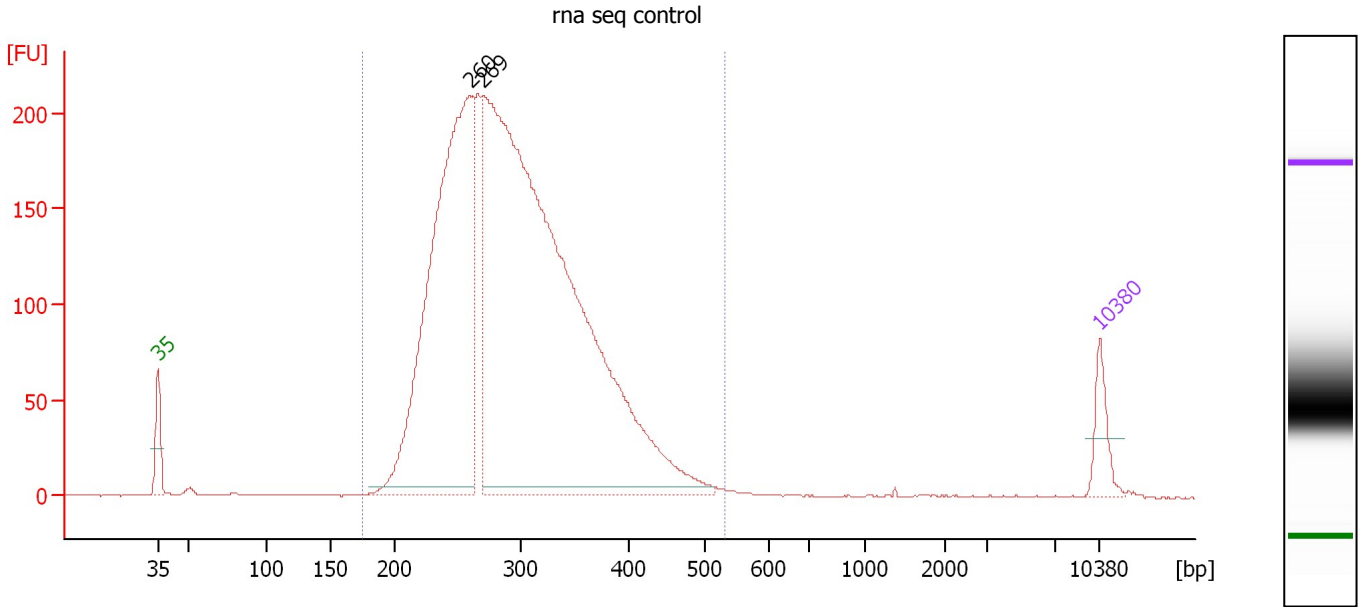

Overall Results for sample 3 : rna seq control

Number of peaks found: 2 Corr. Area 1: 3,644.9
 Noise: 0.2

Peak table for sample 3 : rna seq control

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	260	1,955.17	11,405.9	
3	269	3,939.20	22,148.8	
4	10,380	75.00	10.9	Upper Marker


Region table for sample 3 : rna seq control

From [bp]	To [bp]	Average Size [bp]	Molarity [pmol/l]	Conc. [pg/μl]	Corr. Area	% of Total	Size distribution in CV [%]	Color
175	531	298	31,086.1	5,857.22	3,644.9	99	19.2	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2013-07-26\2013-07-26_003.xad

Created: 7/26/2013 4:30:49 PM
 Modified: 7/26/2013 5:12:08 PM

Electropherogram Summary Continued ...

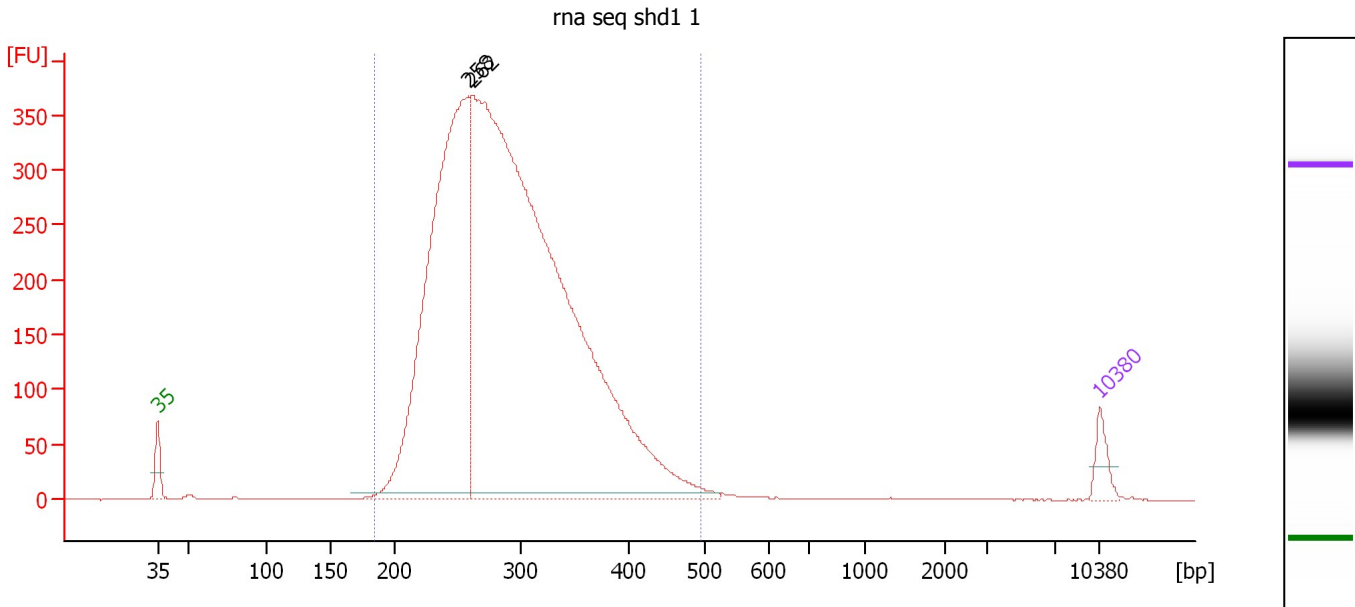

Overall Results for sample 4 : rna seq shd1 1

Number of peaks found: 2 Corr. Area 1: 6,119.7
 Noise: 0.2

Peak table for sample 4 : rna seq shd1 1

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	258	3,327.45	19,504.6	
3	262	7,342.77	42,525.7	
4	10,380	75.00	10.9	Upper Marker


Region table for sample 4 : rna seq shd1 1

From [bp]	To [bp]	Average Size [bp]	Molarity [pmol/l]	Conc. [pg/μl]	Corr. Area	% of Total	Size distribution in CV [%]	Color
183	494	293	53,728.4	9,996.60	6,119.7	99	18.6	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2013-07-26\2013-07-26_003.xad

Created: 7/26/2013 4:30:49 PM
 Modified: 7/26/2013 5:12:08 PM

Electropherogram Summary Continued ...

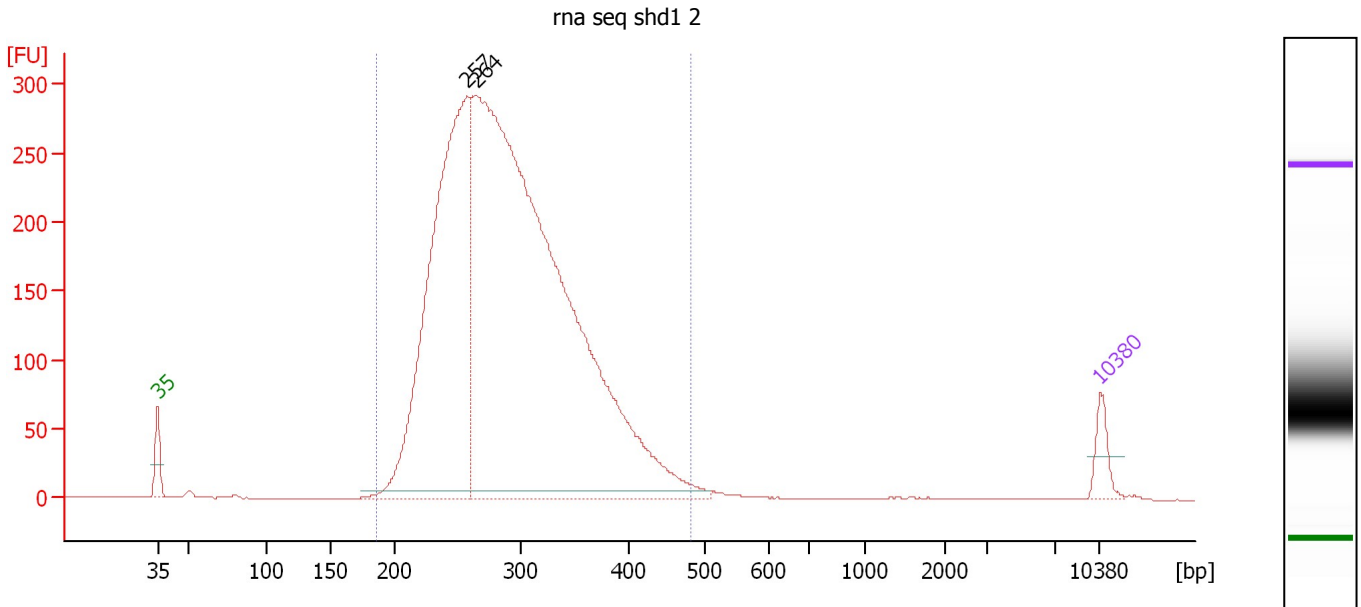

Overall Results for sample 5 : rna seq shd1 2

Number of peaks found: 2 Corr. Area 1: 4,786.7
 Noise: 0.1

Peak table for sample 5 : rna seq shd1 2

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	257	2,663.78	15,680.0	
3	264	5,929.79	33,998.4	
4	10,380	75.00	10.9	Upper Marker


Region table for sample 5 : rna seq shd1 2

From [bp]	To [bp]	Average Size [bp]	Molarity [pmol/l]	Conc. [pg/μl]	Corr. Area	% of Total	Size distribution in CV [%]	Color
185	482	293	43,335.8	8,084.37	4,786.7	98	18.1	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2013-07-26\2013-07-26_003.xad

Created: 7/26/2013 4:30:49 PM
 Modified: 7/26/2013 5:12:08 PM

Electropherogram Summary Continued ...

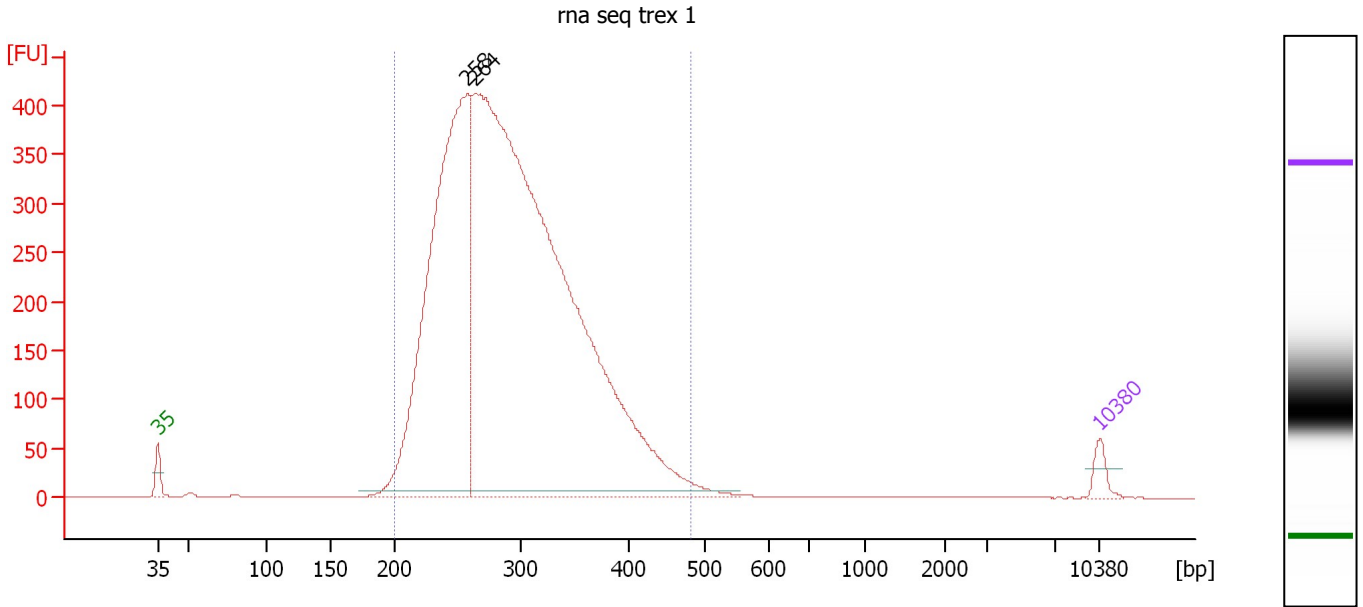

Overall Results for sample 6 : rna seq trex 1

Number of peaks found: 2 Corr. Area 1: 6,872.1
 Noise: 0.2

Peak table for sample 6 : rna seq trex 1

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	258	4,844.83	28,502.3	
3	264	10,802.38	62,011.5	
4	10,380	75.00	10.9	Upper Marker


Region table for sample 6 : rna seq trex 1

From [bp]	To [bp]	Average Size [bp]	Molarity [pmol/l]	Conc. [pg/μl]	Corr. Area	% of Total	Size distribution in CV [%]	Color
200	480	295	77,594.8	14,541.65	6,872.1	98	18.1	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2013-07-26\2013-07-26_003.xad

Created: 7/26/2013 4:30:49 PM
 Modified: 7/26/2013 5:12:08 PM

Electropherogram Summary Continued ...

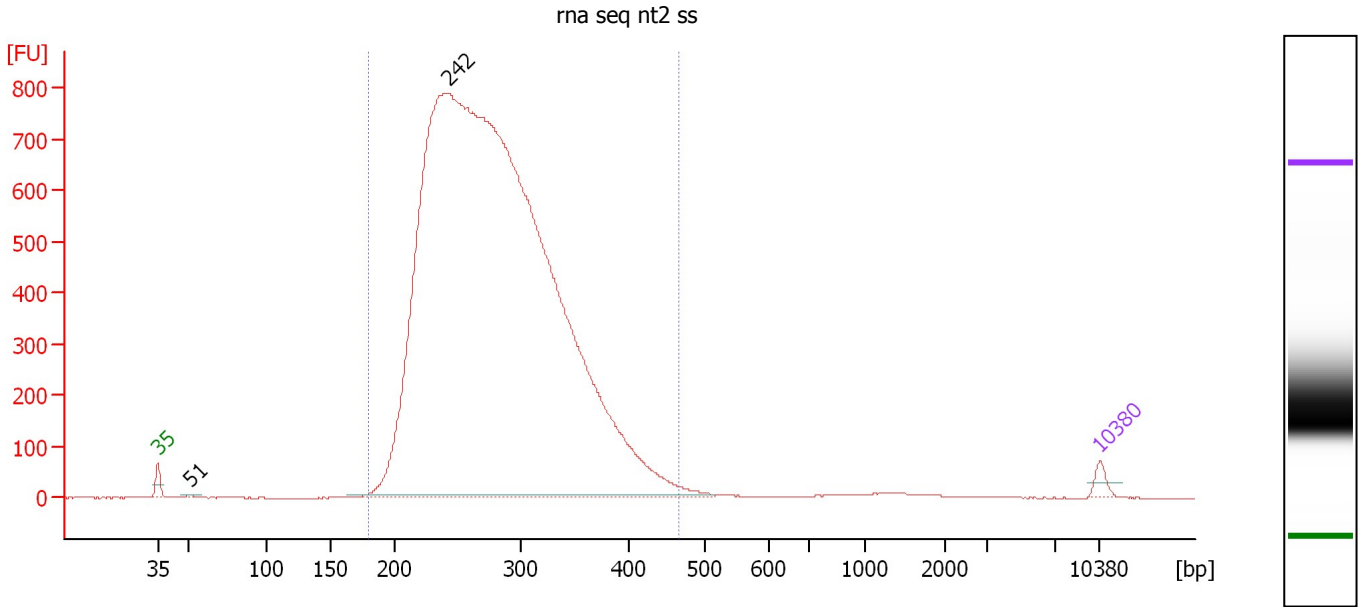

Overall Results for sample 7 : rna seq nt2 ss

Number of peaks found: 2 Corr. Area 1: 13,356.4
 Noise: 0.1

Peak table for sample 7 : rna seq nt2 ss

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	51	18.63	556.8	
3	242	28,398.64	177,544.4	
4	10,380	75.00	10.9	Upper Marker


Region table for sample 7 : rna seq nt2 ss

From [bp]	To [bp]	Average Size [bp]	Molarity [pmol/l]	Conc. [pg/μl]	Corr. Area	% of Total	Size distribution in CV [%]	Color
179	465	282	144,721.2	26,013.96	13,356.4	98	18.0	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2013-07-26\2013-07-26_003.xad

Created: 7/26/2013 4:30:49 PM
 Modified: 7/26/2013 5:12:08 PM

Electropherogram Summary Continued ...

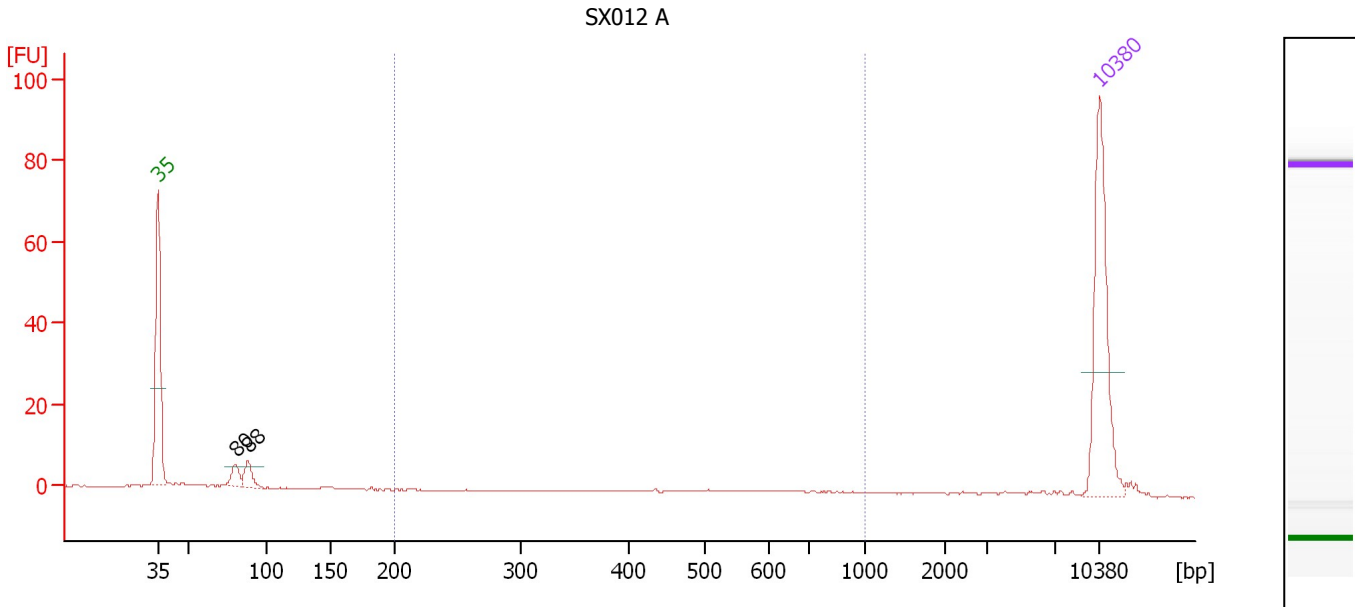

Overall Results for sample 8 : SX012 A

Number of peaks found: 2 Corr. Area 1: 15.9
 Noise: 0.2

Peak table for sample 8 : SX012 A

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	80	11.94	225.2	
3	88	14.78	253.6	
4	10,380	75.00	10.9	Upper Marker


Region table for sample 8 : SX012 A

From [bp]	To [bp]	Average Size [bp]	Molarity [pmol/l]	Conc. [pg/μl]	Corr. Area	% of Total	Size distribution in CV [%]	Color
200	1,000	549	57.9	17.75	15.9	24	32.5	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2013-07-26\2013-07-26_003.xad

Created: 7/26/2013 4:30:49 PM
 Modified: 7/26/2013 5:12:08 PM

Electropherogram Summary Continued ...

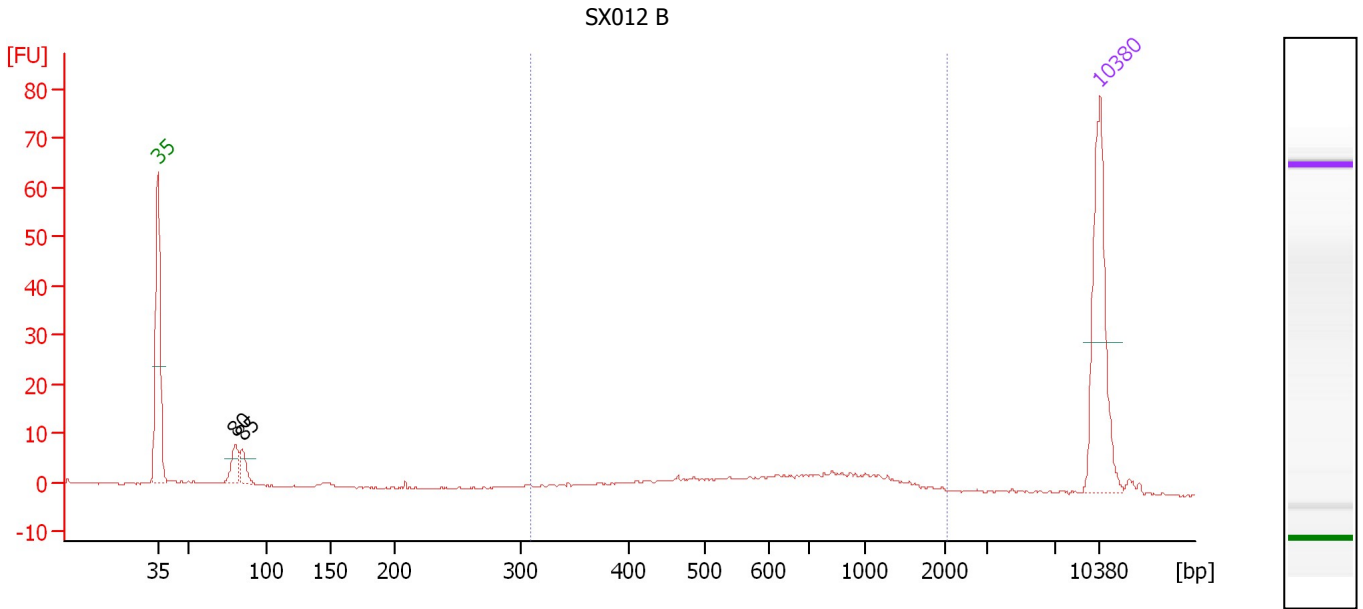

Overall Results for sample 9 : SX012 B

Number of peaks found: 2 Corr. Area 1: 80.5
 Noise: 0.2

Peak table for sample 9 : SX012 B

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	80	20.01	378.5	
3	85	15.68	281.0	
4	10,380	75.00	10.9	Upper Marker


Region table for sample 9 : SX012 B

From [bp]	To [bp]	Average Size [bp]	Molarity [pmol/l]	Conc. [pg/μl]	Corr. Area	% of Total	Size distribution in CV [%]	Color
308	2,050	763	261.9	102.53	80.5	66	49.1	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2013-07-26\2013-07-26_003.xad

Created: 7/26/2013 4:30:49 PM
 Modified: 7/26/2013 5:12:08 PM

Electropherogram Summary Continued ...

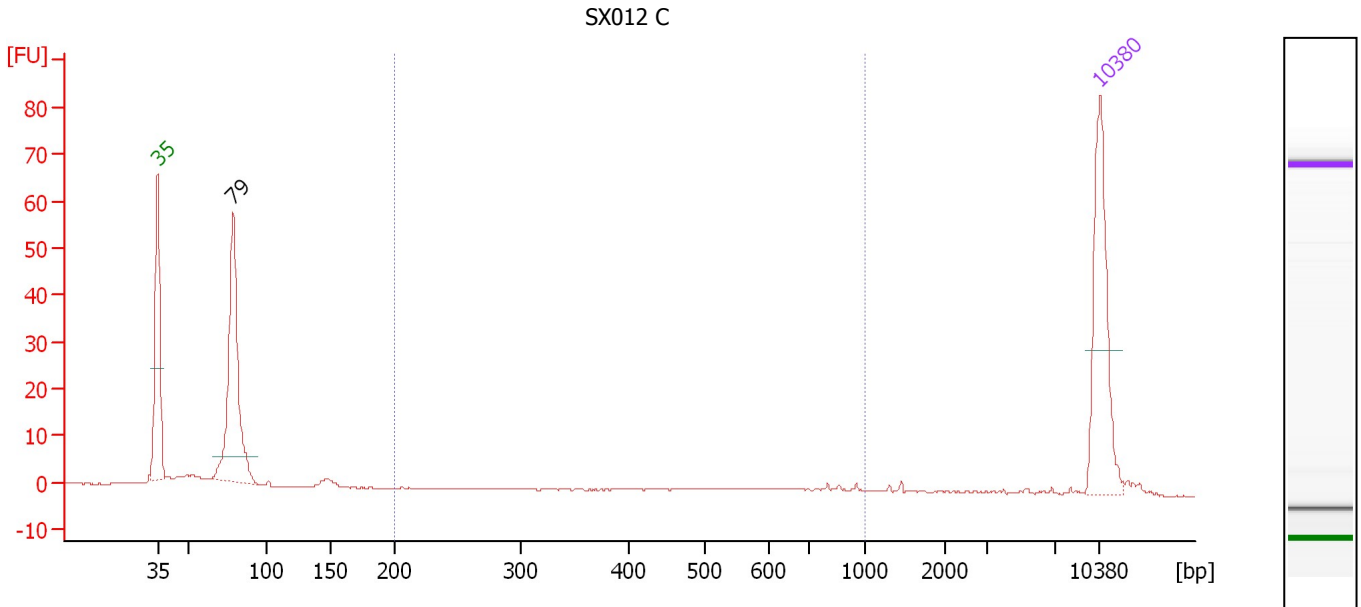

Overall Results for sample 10 : SX012 C

Number of peaks found: 1 Corr. Area 1: 10.7
 Noise: 0.1

Peak table for sample 10 : SX012 C

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	79	174.88	3,360.9	
3	10,380	75.00	10.9	Upper Marker


Region table for sample 10 : SX012 C

From [bp]	To [bp]	Average Size [bp]	Molarity [pmol/l]	Conc. [pg/μl]	Corr. Area	% of Total	Size distribution in CV [%]	Color
200	1,000	658	31.0	12.41	10.7	7	25.4	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2013-07-26\2013-07-26_003.xad

Created: 7/26/2013 4:30:49 PM
 Modified: 7/26/2013 5:12:08 PM

Electropherogram Summary Continued ...

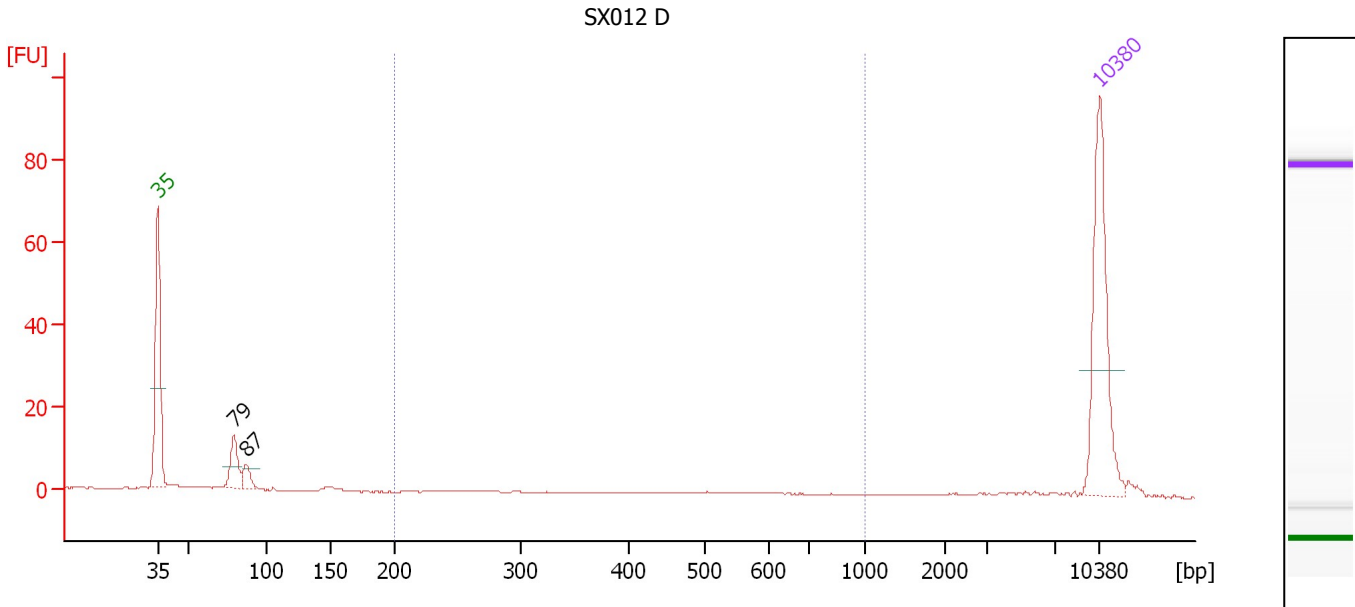

Overall Results for sample 11 : SX012 D

Number of peaks found: 2 Corr. Area 1: 7.7
 Noise: 0.1

Peak table for sample 11 : SX012 D

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	79	26.15	500.1	
3	87	12.51	216.8	
4	10,380	75.00	10.9	Upper Marker


Region table for sample 11 : SX012 D

From [bp]	To [bp]	Average Size [bp]	Molarity [pmol/l]	Conc. [pg/μl]	Corr. Area	% of Total	Size distribution in CV [%]	Color
200	1,000	524	29.8	8.36	7.7	12	36.1	Blue

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...ents and Settings\Bioanalyzer\2013-07-26\2013-07-26_003.xad

Created: 7/26/2013 4:30:49 PM
Modified: 7/26/2013 5:12:08 PM

Gel Image

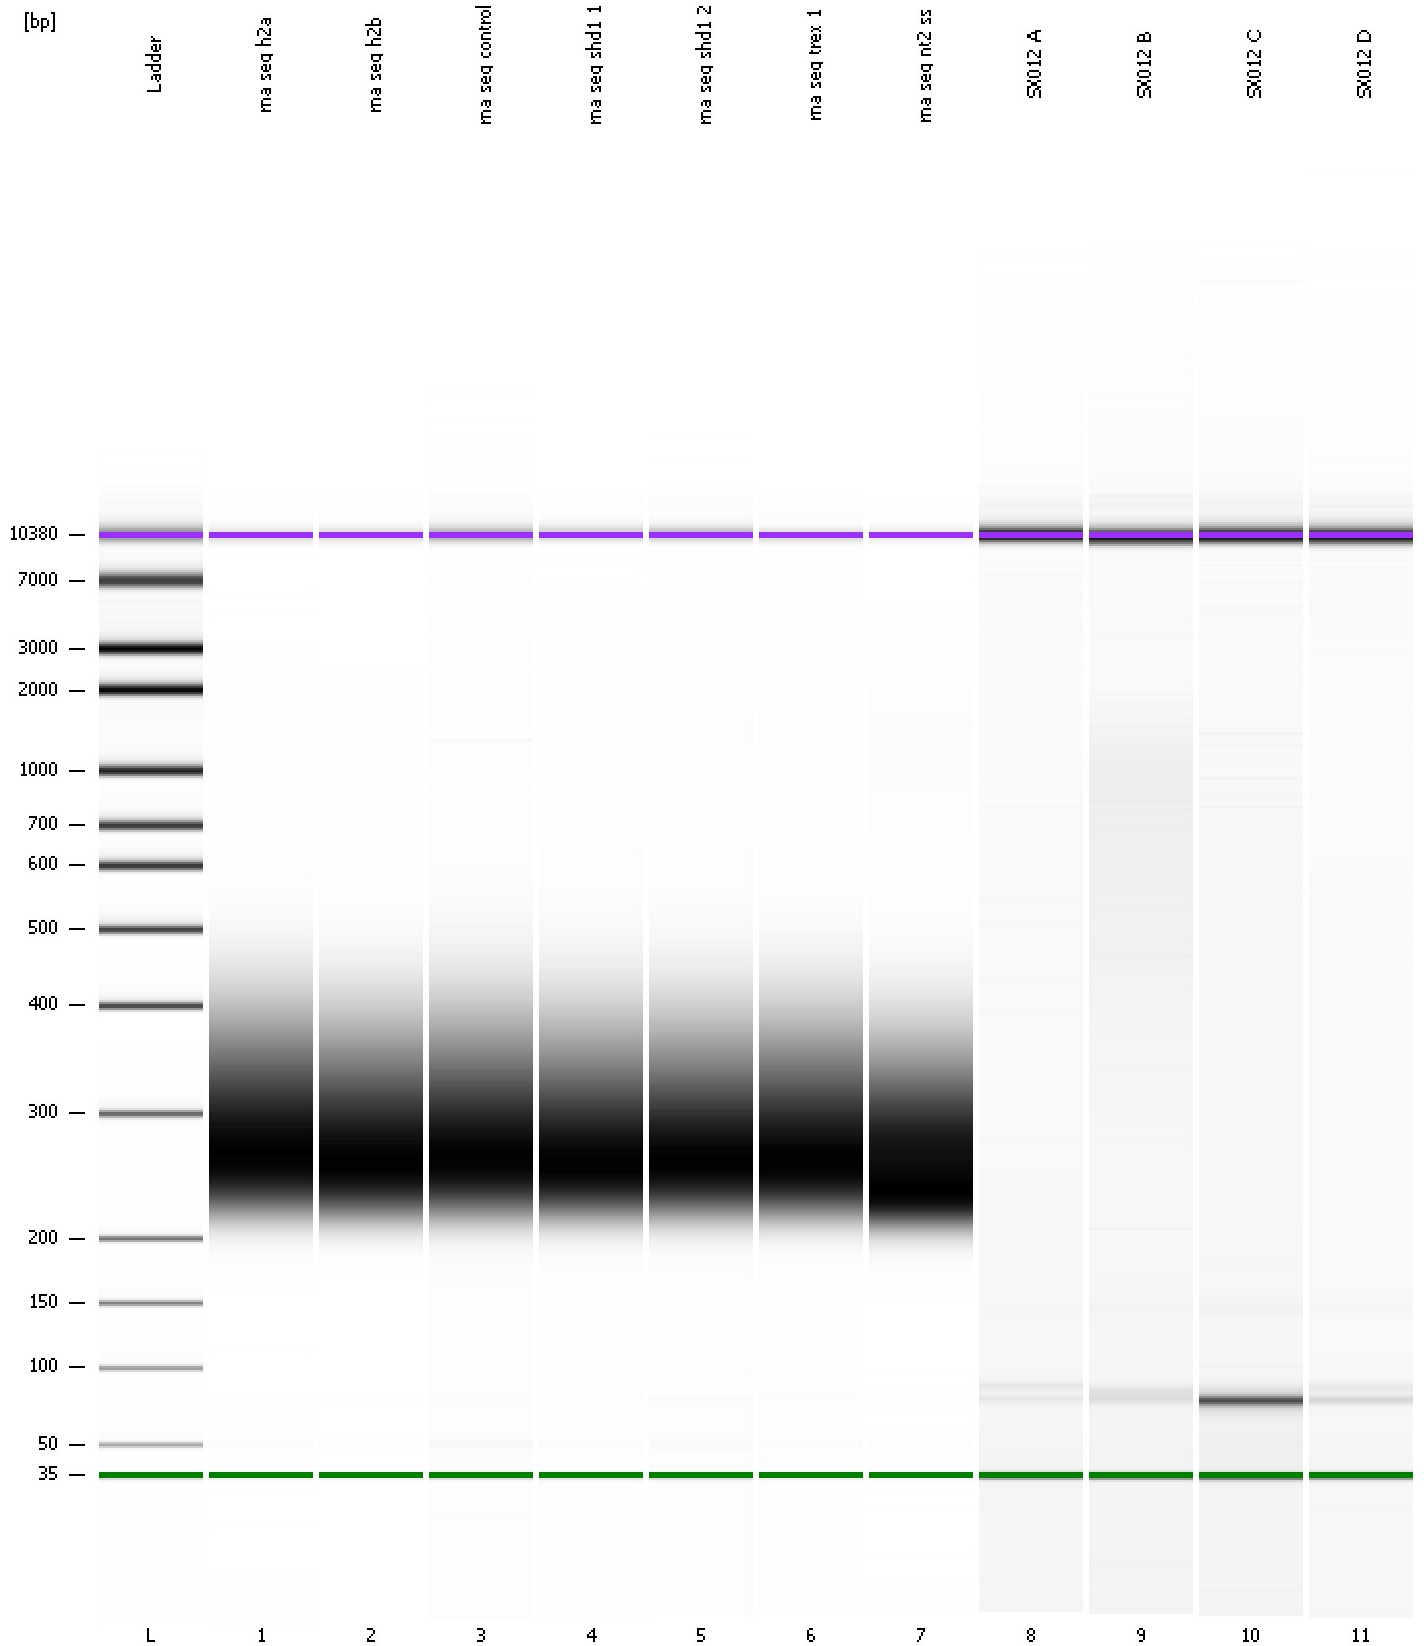

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2013-07-26\2013-07-26_003.xad

Created: 7/26/2013 4:30:49 PM
 Modified: 7/26/2013 5:12:08 PM

Run Logbook

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 12)		Instrument	Run		7/26/2013 5:12:05 PM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Run started on port 1 (File: C:\Documents and Settings\Bioanalyzer\2013-07-26\2013-07-26_003.xad)		Instrument	Run		7/26/2013 4:30:54 PM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Product Number : G2938B		Instrument	Run		7/26/2013 4:30:54 PM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Name :		Instrument	Run		7/26/2013 4:30:54 PM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Vendor : Agilent Technologies		Instrument	Run		7/26/2013 4:30:54 PM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Serial# : DE13701086		Instrument	Run		7/26/2013 4:30:54 PM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Firmware : C.01.069		Instrument	Run		7/26/2013 4:30:54 PM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Cartridge : Electrode		Instrument	Run		7/26/2013 4:30:54 PM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1