


Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...ents and Settings\Bioanalyzer\2013-10-18\2013-10-18\_003.xad

Created: 10/18/2013 11:36:20 AM  
Modified: 10/18/2013 12:18:28 PM

**Electrophoresis File Run Summary**

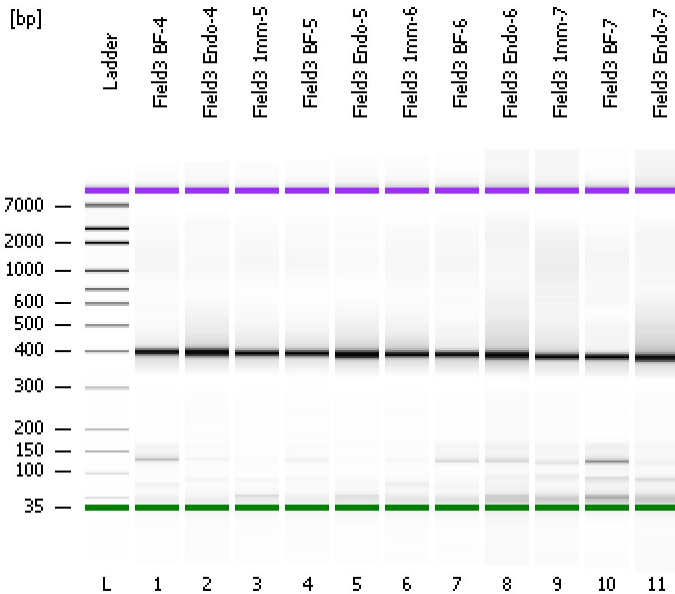

Instrument Information:

Instrument Name: DE13701086      Firmware: C.01.069  
Serial#: DE13701086      Type: G2938B

Assay Information:

Assay Origin Path: C:\Program Files\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy  
Assay Class: High Sensitivity DNA Assay  
Version: 1.03  
Assay Comments: Copyright © 2003-2010 Agilent Technologies




Chip Information:

Chip Lot #:   
Reagent Kit Lot #:   
Chip Comments:

**Field3 BF-4**

**Field3 Endo-4**




**Field3 1mm-5**

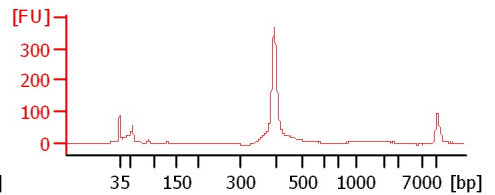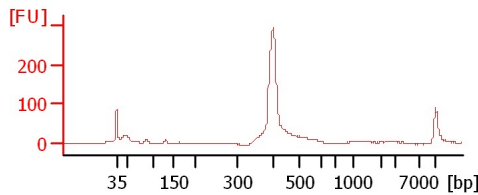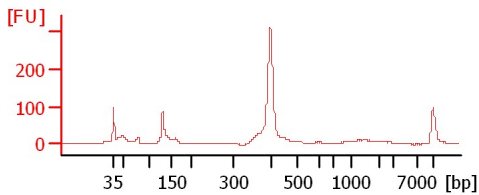

**Field3 BF-5**

**Field3 Endo-5**




**Field3 1mm-6**

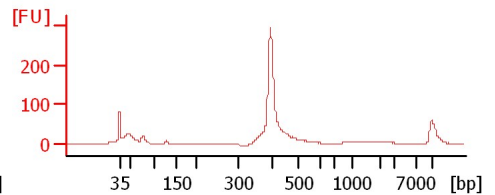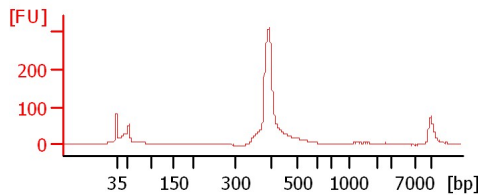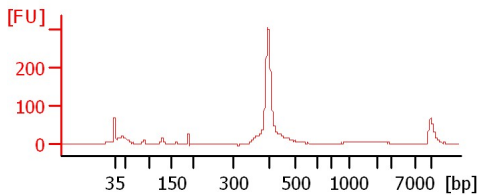

**Field3 BF-6**



**Field3 Endo-6**

**Field3 1mm-7**

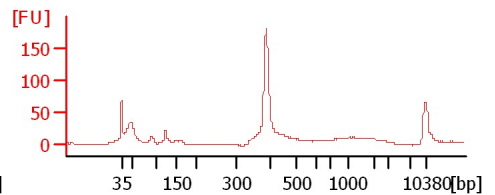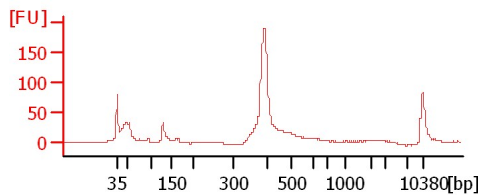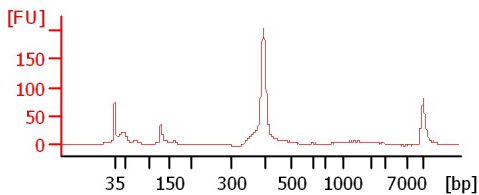

**Field3 BF-7**

**Field3 Endo-7**

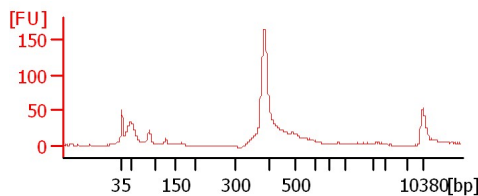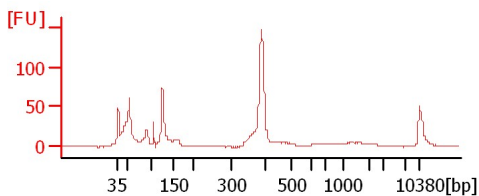

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...ents and Settings\Bioanalyzer\2013-10-18\2013-10-18\_003.xad

Created: 10/18/2013 11:36:20 AM  
 Modified: 10/18/2013 12:18:28 PM

**Electrophoresis File Run Summary (Chip Summary)**

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
Field3 BF-4		<input type="checkbox"/>	✓			
Field3 Endo-4		<input type="checkbox"/>	✓			
Field3 1mm-5		<input type="checkbox"/>	✓			
Field3 BF-5		<input type="checkbox"/>	✓			
Field3 Endo-5		<input type="checkbox"/>	✓			
Field3 1mm-6		<input type="checkbox"/>	✓			
Field3 BF-6		<input type="checkbox"/>	✓			
Field3 Endo-6		<input type="checkbox"/>	✓			
Field3 1mm-7		<input type="checkbox"/>	✓			
Field3 BF-7		<input type="checkbox"/>	✓			
Field3 Endo-7		<input type="checkbox"/>	✓			
Ladder		<input type="checkbox"/>	✓			

**Chip Lot #**

**Reagent Kit Lot #**

**Chip Comments :**

Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...ents and Settings\Bioanalyzer\2013-10-18\2013-10-18\_003.xad

Created: 10/18/2013 11:36:20 AM  
Modified: 10/18/2013 12:18:28 PM

**Electrophoresis Assay Details**

**General Analysis Settings**

Number of Available Sample and Ladder Wells (Max.) : 12  
Minimum Visible Range [s] : 32  
Maximum Visible Range [s] : 138  
Start Analysis Time Range [s] : 33  
End Analysis Time Range [s] : 137.5  
Ladder Concentration [pg/μl] : 1950  
Uses Standard Area for Ladder Fragments  
Lower Marker Concentration [pg/μl] : 125  
Upper Marker Concentration [pg/μl] : 75  
Used Upper Marker for Quantitation  
Standard Curve Fit is Point to Point  
Show Data Aligned to Lower and Upper Marker

**Integrator Settings**

Integration Start Time [s] : 33.05  
Integration End Time [s] : 137  
Slope Threshold : 0.8  
Height Threshold [FU] : 5  
Area Threshold : 0.1  
Width Threshold [s] : 0.6  
Baseline Plateau [s] : 0.5

**Filter Settings**

Filter Width [s] : 0.5  
Polynomial Order : 4


**Ladder**

Ladder Peak	Size	Area
1	35	160
2	50	210
3	100	208
4	150	221
5	200	242
6	300	270
7	400	305
8	500	306
9	600	336
10	700	321
11	1000	366
12	2000	413
13	3000	411
14	7000	400
15	10380	214

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...ents and Settings\Bioanalyzer\2013-10-18\2013-10-18\_003.xad

Created: 10/18/2013 11:36:20 AM  
 Modified: 10/18/2013 12:18:28 PM

**Electropherogram Summary**

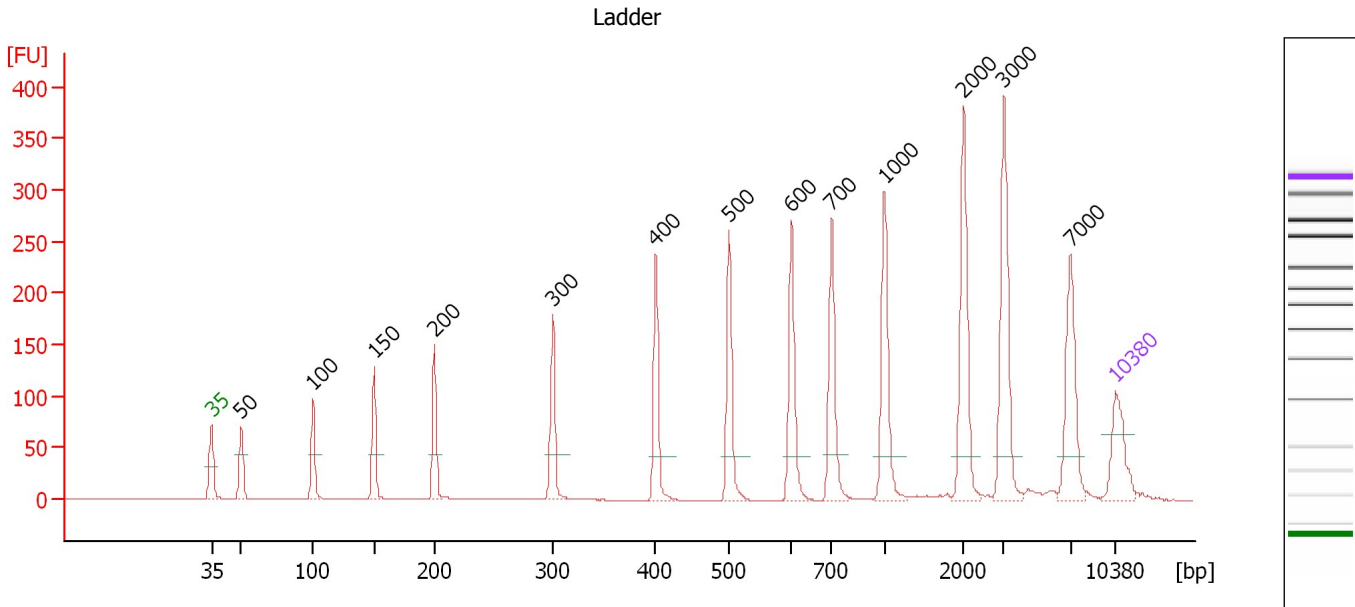

**Overall Results for Ladder**

Noise: 0.2


**Peak table for Ladder**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	50	150.00	4,545.5	Ladder Peak
3	100	150.00	2,272.7	Ladder Peak
4	150	150.00	1,515.2	Ladder Peak
5	200	150.00	1,136.4	Ladder Peak
6	300	150.00	757.6	Ladder Peak
7	400	150.00	568.2	Ladder Peak
8	500	150.00	454.5	Ladder Peak
9	600	150.00	378.8	Ladder Peak
10	700	150.00	324.7	Ladder Peak
11	1,000	150.00	227.3	Ladder Peak
12	2,000	150.00	113.6	Ladder Peak
13	3,000	150.00	75.8	Ladder Peak
14	7,000	150.00	32.5	Ladder Peak
15	10,380	75.00	10.9	Upper Marker

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...ents and Settings\Bioanalyzer\2013-10-18\2013-10-18\_003.xad

Created: 10/18/2013 11:36:20 AM  
 Modified: 10/18/2013 12:18:28 PM

**Electropherogram Summary Continued ...**

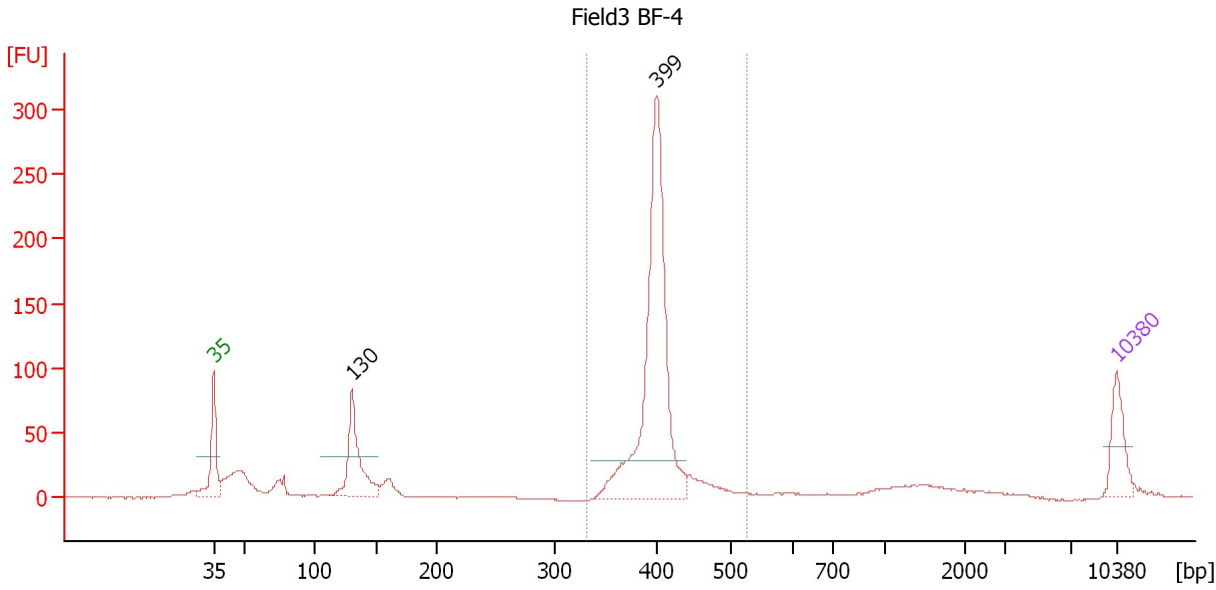

**Setpoint Deviations for sample 1 : Field3 BF-4**

Height Threshold [FU] : 30

**Overall Results for sample 1 : Field3 BF-4**

Number of peaks found: 2                      Corr. Area 1: 774.0  
 Noise: 0.2

**Peak table for sample 1 : Field3 BF-4**

Peak	Size [bp]	Conc. [pg/µl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	130	258.18	3,006.0	
3	399	816.11	3,095.4	
4	10,380	75.00	10.9	Upper Marker


**Region table for sample 1 : Field3 BF-4**

From [bp]	To [bp]	Average Size [bp]	Molarity [pmol/l]	Conc. [pg/µl]	Corr. Area	% of Total	Size distribution in CV [%]	Color
332	525	402	3,233.1	856.08	774.0	62	5.9	Blue

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...ents and Settings\Bioanalyzer\2013-10-18\2013-10-18\_003.xad

Created: 10/18/2013 11:36:20 AM  
 Modified: 10/18/2013 12:18:28 PM

**Electropherogram Summary Continued ...**

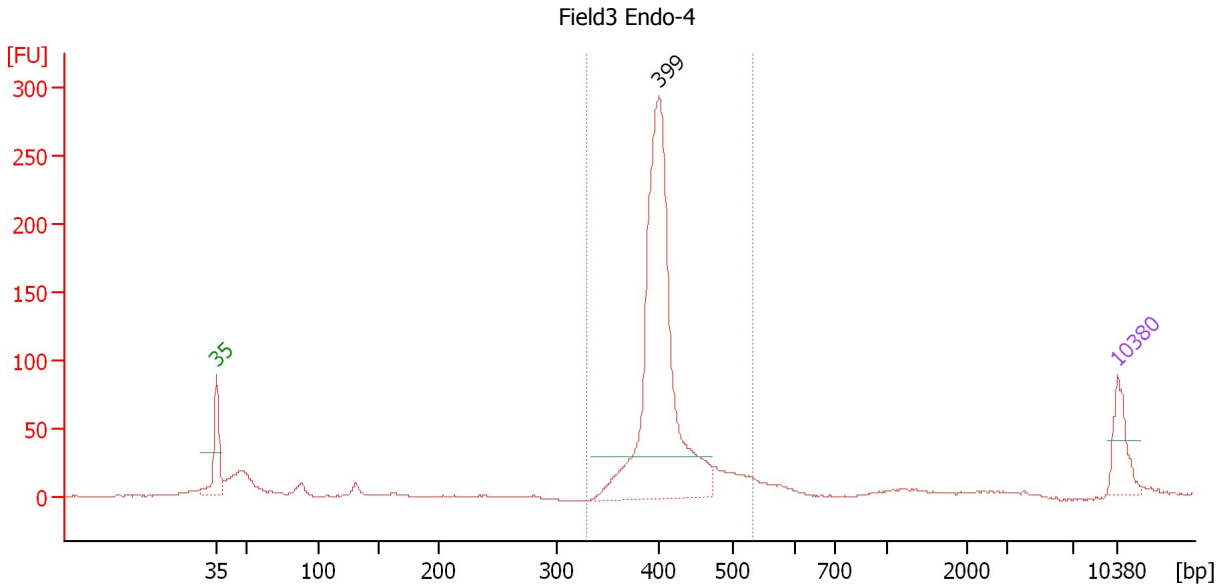

**Setpoint Deviations for sample 2 : Field3 Endo-4**

Height Threshold [FU] : 30

**Overall Results for sample 2 : Field3 Endo-4**

Number of peaks found: 1                      Corr. Area 1: 980.6  
 Noise: 0.4

**Peak table for sample 2 : Field3 Endo-4**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	399	1,115.72	4,232.0	
3	10,380	75.00	10.9	Upper Marker


**Region table for sample 2 : Field3 Endo-4**

From [bp]	To [bp]	Average Size [bp]	Molarity [pmol/l]	Conc. [pg/μl]	Corr. Area	% of Total	Size distribution in CV [%]	Color
330	532	409	4,298.9	1,155.20	980.6	82	7.8	Blue

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...ents and Settings\Bioanalyzer\2013-10-18\2013-10-18\_003.xad

Created: 10/18/2013 11:36:20 AM  
 Modified: 10/18/2013 12:18:28 PM

**Electropherogram Summary Continued ...**

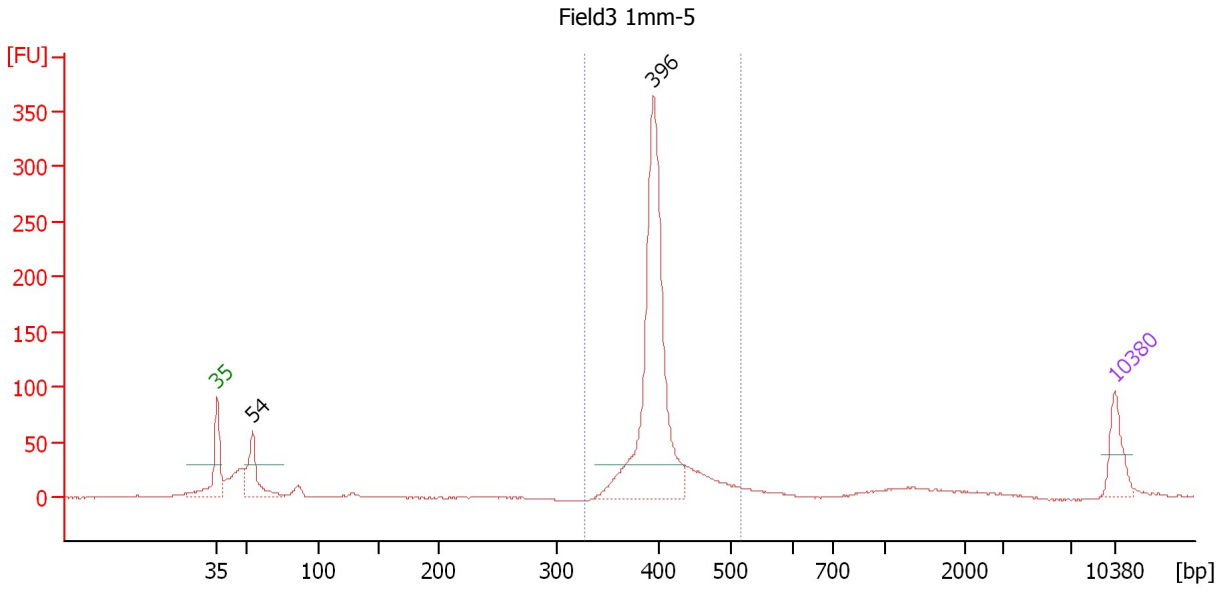

**Setpoint Deviations for sample 3 : Field3 1mm-5**

Height Threshold [FU] : 30

**Overall Results for sample 3 : Field3 1mm-5**

Number of peaks found: 2                      Corr. Area 1: 921.0  
 Noise: 0.6

**Peak table for sample 3 : Field3 1mm-5**

Peak	Size [bp]	Conc. [pg/µl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	54	199.04	5,557.0	
3	396	934.79	3,581.0	
4	10,380	75.00	10.9	Upper Marker


**Region table for sample 3 : Field3 1mm-5**

From [bp]	To [bp]	Average Size [bp]	Molarity [pmol/l]	Conc. [pg/µl]	Corr. Area	% of Total	Size distribution in CV [%]	Color
328	515	403	3,877.8	1,028.16	921.0	73	6.7	Blue

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...ents and Settings\Bioanalyzer\2013-10-18\2013-10-18\_003.xad

Created: 10/18/2013 11:36:20 AM  
 Modified: 10/18/2013 12:18:28 PM

**Electropherogram Summary Continued ...**

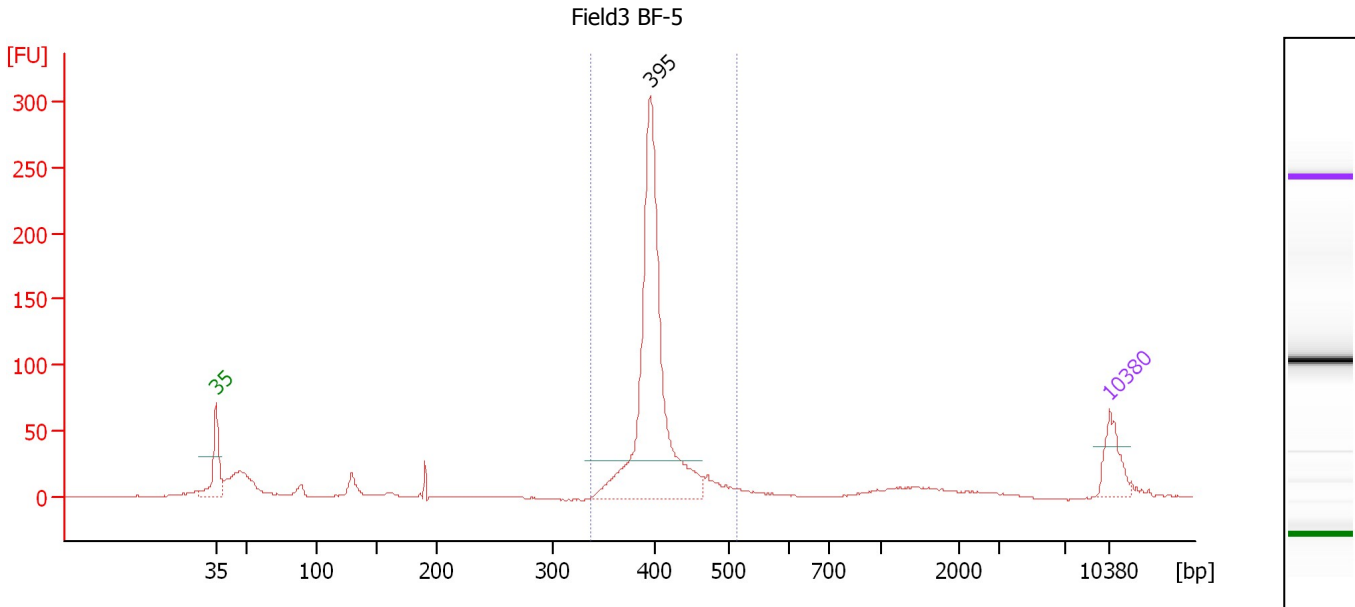

**Setpoint Deviations for sample 4 : Field3 BF-5**

Height Threshold [FU] : 30

**Overall Results for sample 4 : Field3 BF-5**

Number of peaks found: 1                      Corr. Area 1: 772.4  
 Noise: 0.4

**Peak table for sample 4 : Field3 BF-5**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	395	1,010.81	3,875.4	
3	10,380	75.00	10.9	Upper Marker

**Region table for sample 4 : Field3 BF-5**


From [bp]	To [bp]	Average Size [bp]	Molarity [pmol/l]	Conc. [pg/μl]	Corr. Area	% of Total	Size distribution in CV [%]	Color
336	516	403	3,874.4	1,026.97	772.4	73	6.6	Blue



Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...ents and Settings\Bioanalyzer\2013-10-18\2013-10-18\_003.xad

Created: 10/18/2013 11:36:20 AM  
 Modified: 10/18/2013 12:18:28 PM

**Electropherogram Summary Continued ...**

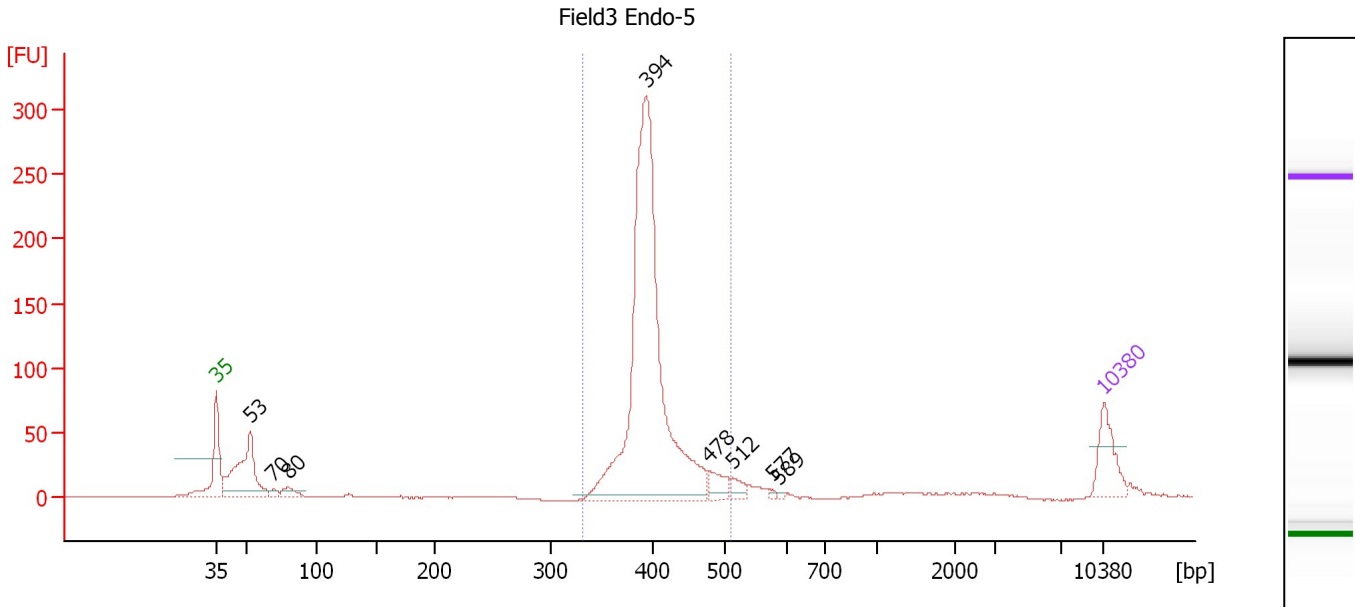

**Overall Results for sample 5 : Field3 Endo-5**

Number of peaks found: 8                      Corr. Area 1: 1,074.2  
 Noise: 0.3

**Peak table for sample 5 : Field3 Endo-5**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	53	305.29	8,659.7	
3	70	15.73	341.7	
4	80	34.51	650.4	
5	394	1,233.73	4,750.0	
6	478	48.85	154.8	
7	512	25.32	74.9	
8	577	4.72	12.4	
9	589	3.69	9.5	
10	10,380	75.00	10.9	Upper Marker


**Region table for sample 5 : Field3 Endo-5**

From [bp]	To [bp]	Average Size [bp]	Molarity [pmol/l]	Conc. [pg/μl]	Corr. Area	% of Total	Size distribution in CV [%]	Color
331	511	402	4,666.4	1,232.10	1,074.2	78	7.2	Blue

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...ents and Settings\Bioanalyzer\2013-10-18\2013-10-18\_003.xad

Created: 10/18/2013 11:36:20 AM  
 Modified: 10/18/2013 12:18:28 PM

**Electropherogram Summary Continued ...**

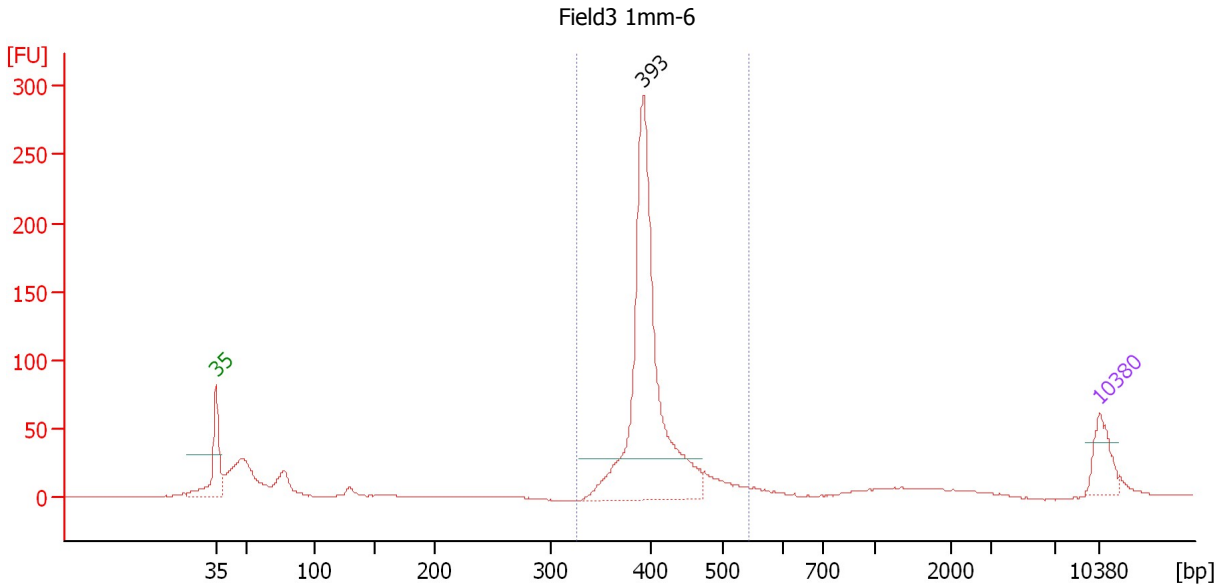

**Setpoint Deviations for sample 6 : Field3 1mm-6**

Height Threshold [FU] : 30

**Overall Results for sample 6 : Field3 1mm-6**

Number of peaks found: 1                      Corr. Area 1: 842.0  
 Noise: 0.4

**Peak table for sample 6 : Field3 1mm-6**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	393	1,085.29	4,184.8	
3	10,380	75.00	10.9	Upper Marker


**Region table for sample 6 : Field3 1mm-6**

From [bp]	To [bp]	Average Size [bp]	Molarity [pmol/l]	Conc. [pg/μl]	Corr. Area	% of Total	Size distribution in CV [%]	Color
326	544	406	4,081.2	1,085.87	842.0	73	8.1	Blue

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...ents and Settings\Bioanalyzer\2013-10-18\2013-10-18\_003.xad

Created: 10/18/2013 11:36:20 AM  
 Modified: 10/18/2013 12:18:28 PM

**Electropherogram Summary Continued ...**

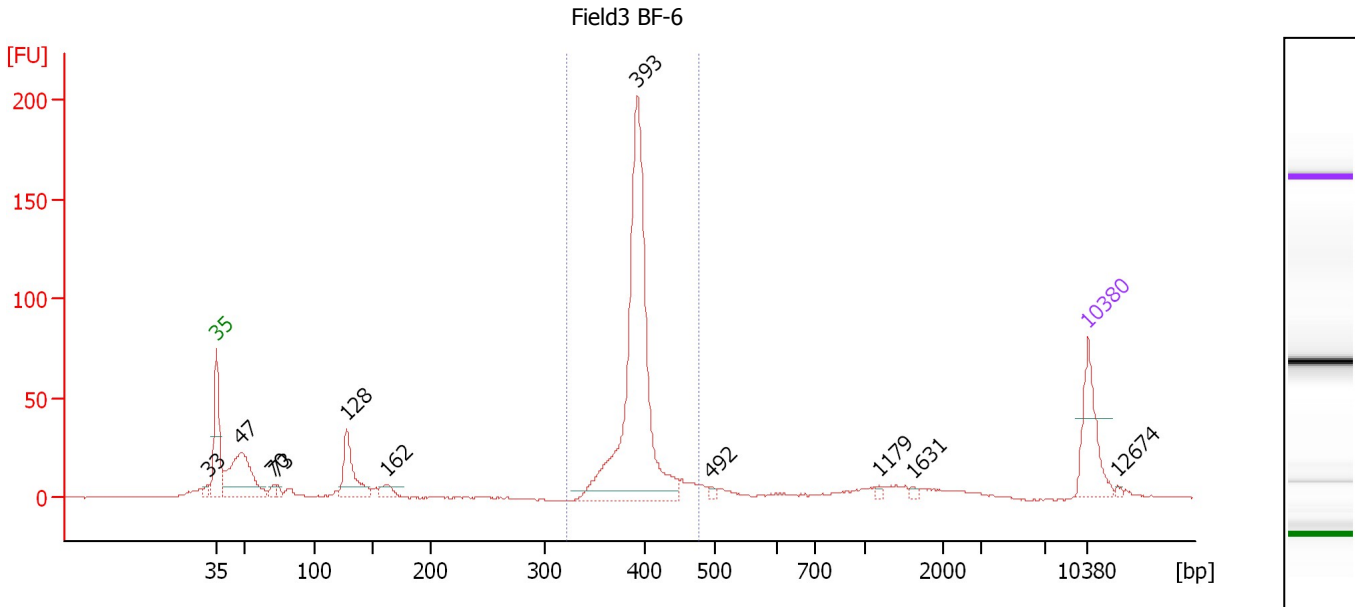

**Overall Results for sample 7 : Field3 BF-6**

Number of peaks found: 11                      Corr. Area 1: 482.8  
 Noise: 0.3

**Peak table for sample 7 : Field3 BF-6**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	33	0.00	0.0	
2	35	125.00	5,411.3	Lower Marker
3	47	208.11	6,638.8	
4	70	12.22	262.6	
5	73	9.80	202.9	
6	128	111.57	1,322.5	
7	162	23.46	219.6	
8	393	609.58	2,351.7	
9	492	7.04	21.7	
10	1,179	4.15	5.3	
11	1,631	3.79	3.5	
12	10,380	75.00	10.9	Upper Marker
13	12,674	0.00	0.0	


**Region table for sample 7 : Field3 BF-6**

From [bp]	To [bp]	Average Size [bp]	Molarity [pmol/l]	Conc. [pg/μl]	Corr. Area	% of Total	Size distribution in CV [%]	Color
322	477	394	2,342.6	607.78	482.8	60	5.2	Blue

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...ents and Settings\Bioanalyzer\2013-10-18\2013-10-18\_003.xad

Created: 10/18/2013 11:36:20 AM  
 Modified: 10/18/2013 12:18:28 PM

**Electropherogram Summary Continued ...**

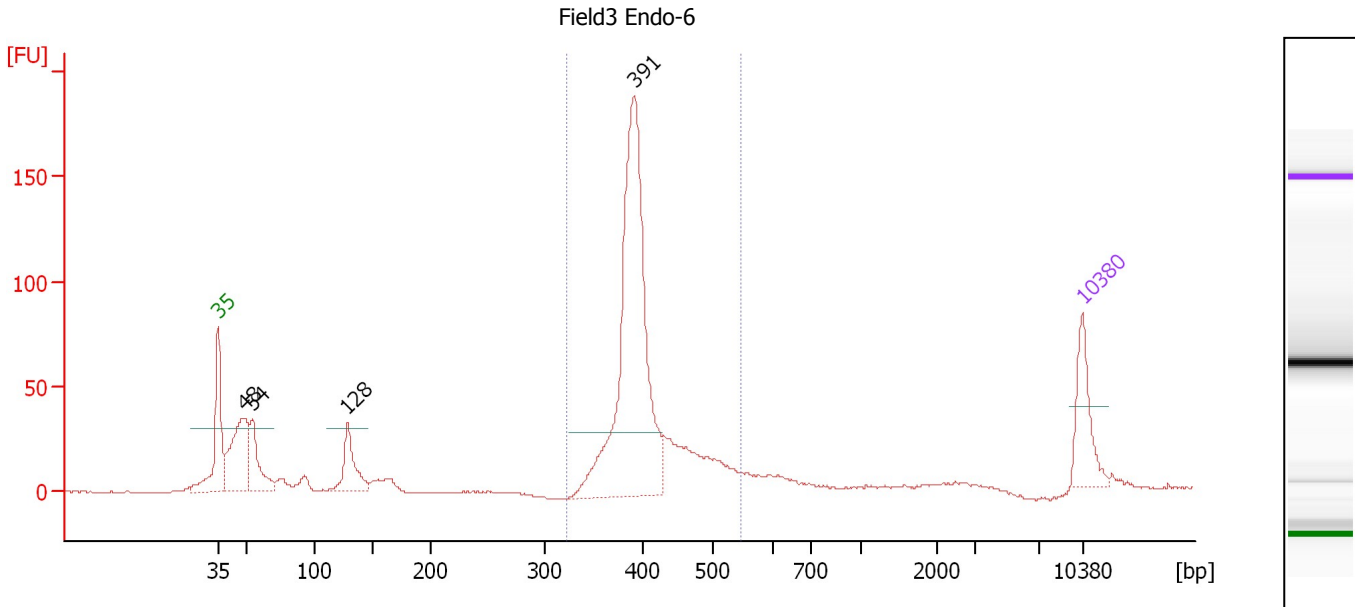

**Setpoint Deviations for sample 8 : Field3 Endo-6**

Height Threshold [FU] : 30

**Overall Results for sample 8 : Field3 Endo-6**

Number of peaks found: 4                      Corr. Area 1: 687.0  
 Noise: 0.3

**Peak table for sample 8 : Field3 Endo-6**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	48	226.51	7,084.3	
3	54	112.85	3,139.3	
4	128	101.94	1,208.0	
5	391	685.65	2,657.0	
6	10,380	75.00	10.9	Upper Marker


**Region table for sample 8 : Field3 Endo-6**

From [bp]	To [bp]	Average Size [bp]	Molarity [pmol/l]	Conc. [pg/μl]	Corr. Area	% of Total	Size distribution in CV [%]	Color
323	546	406	3,023.3	803.62	687.0	65	9.6	Blue

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...ents and Settings\Bioanalyzer\2013-10-18\2013-10-18\_003.xad

Created: 10/18/2013 11:36:20 AM  
 Modified: 10/18/2013 12:18:28 PM

**Electropherogram Summary Continued ...**

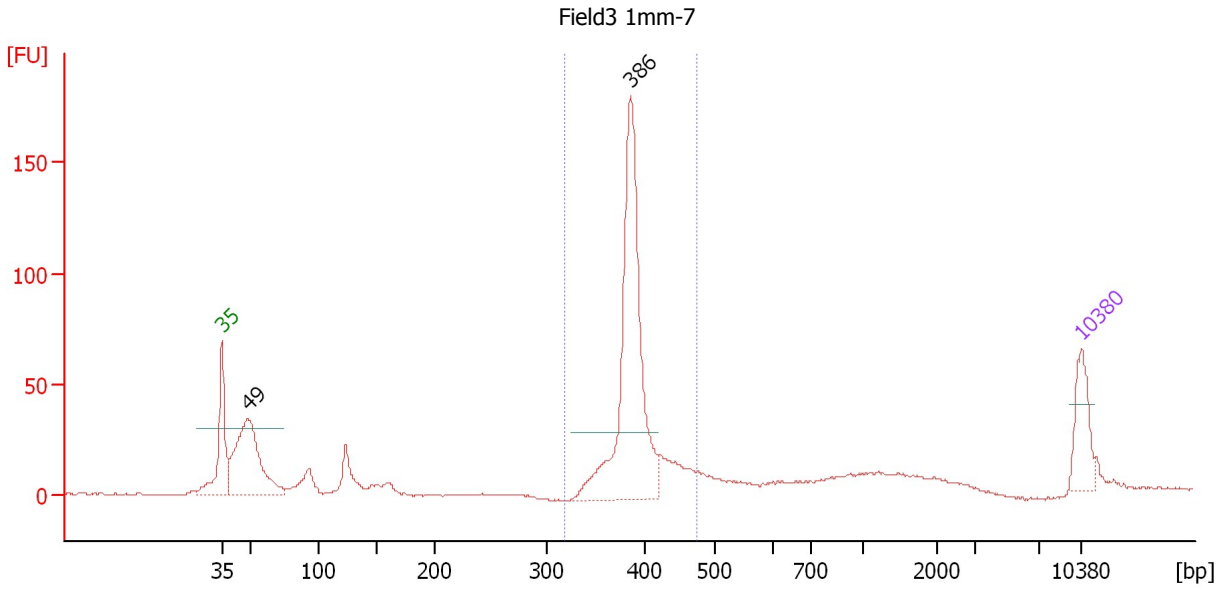

**Setpoint Deviations for sample 9 : Field3 1mm-7**

Height Threshold [FU] : 30

**Overall Results for sample 9 : Field3 1mm-7**

Number of peaks found: 2                      Corr. Area 1: 447.5  
 Noise: 0.4

**Peak table for sample 9 : Field3 1mm-7**

Peak	Size [bp]	Conc. [pg/µl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	49	394.19	12,240.9	
3	386	635.24	2,493.4	
4	10,380	75.00	10.9	Upper Marker


**Region table for sample 9 : Field3 1mm-7**

From [bp]	To [bp]	Average Size [bp]	Molarity [pmol/l]	Conc. [pg/µl]	Corr. Area	% of Total	Size distribution in CV [%]	Color
318	475	393	2,570.9	663.96	447.5	52	5.9	Blue

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...ents and Settings\Bioanalyzer\2013-10-18\2013-10-18\_003.xad

Created: 10/18/2013 11:36:20 AM  
 Modified: 10/18/2013 12:18:28 PM

**Electropherogram Summary Continued ...**

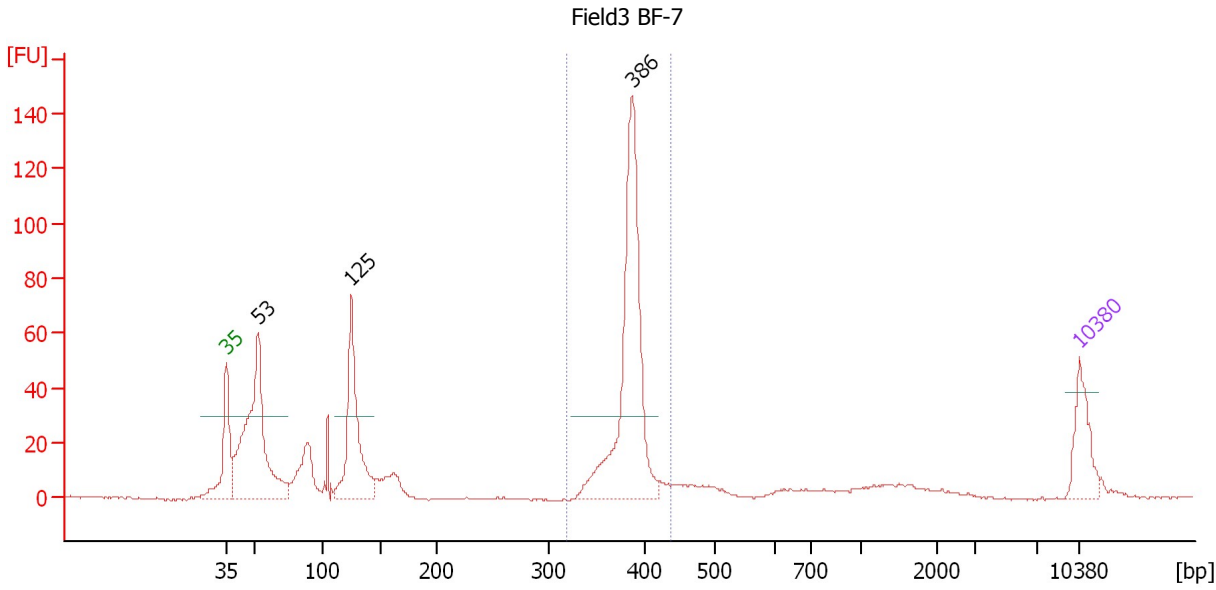

**Setpoint Deviations for sample 10 : Field3 BF-7**

Height Threshold [FU] : 30

**Overall Results for sample 10 : Field3 BF-7**

Number of peaks found: 3                      Corr. Area 1: 319.3  
 Noise: 0.3

**Peak table for sample 10 : Field3 BF-7**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	53	580.81	16,660.1	
3	125	344.99	4,176.0	
4	386	583.84	2,291.1	
5	10,380	75.00	10.9	Upper Marker


**Region table for sample 10 : Field3 BF-7**

From [bp]	To [bp]	Average Size [bp]	Molarity [pmol/l]	Conc. [pg/μl]	Corr. Area	% of Total	Size distribution in CV [%]	Color
319	435	383	2,317.1	585.87	319.3	38	3.8	Blue

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...ents and Settings\Bioanalyzer\2013-10-18\2013-10-18\_003.xad

Created: 10/18/2013 11:36:20 AM  
 Modified: 10/18/2013 12:18:28 PM

**Electropherogram Summary Continued ...**

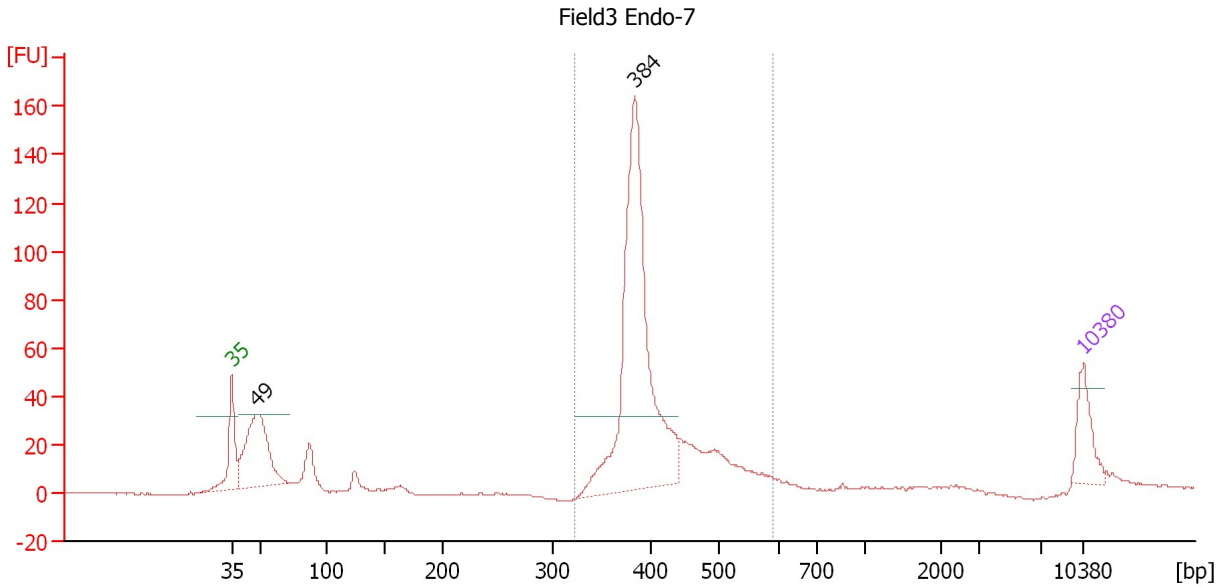

**Setpoint Deviations for sample 11 : Field3 Endo-7**

Height Threshold [FU] : 30

**Overall Results for sample 11 : Field3 Endo-7**

Number of peaks found: 2                      Corr. Area 1: 605.0  
 Noise: 0.1

**Peak table for sample 11 : Field3 Endo-7**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	49	394.71	12,293.9	
3	384	910.49	3,596.3	
4	10,380	75.00	10.9	Upper Marker

**Region table for sample 11 : Field3 Endo-7**

From [bp]	To [bp]	Average Size [bp]	Molarity [pmol/l]	Conc. [pg/μl]	Corr. Area	% of Total	Size distribution in CV [%]	Color
321	590	410	4,168.6	1,110.59	605.0	70	12.1	Blue

Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...ents and Settings\Bioanalyzer\2013-10-18\2013-10-18\_003.xad

Created: 10/18/2013 11:36:20 AM  
Modified: 10/18/2013 12:18:28 PM

**Gel Image**

