

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...ents and Settings\Bioanalyzer\2014-09-04\2014-09-04_008.xad

Created: 9/4/2014 4:11:57 PM
Modified: 9/4/2014 4:53:34 PM

Electrophoresis File Run Summary

Instrument Information:



Instrument Name: DE13701086 Firmware: C.01.069
Serial#: DE13701086 Type: G2938B

Assay Information:

Assay Origin Path: C:\Program Files\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy
Assay Class: High Sensitivity DNA Assay
Version: 1.03
Assay Comments: Copyright © 2003-2010 Agilent Technologies

Chip Information:

Chip Lot #:
Reagent Kit Lot #:
Chip Comments:

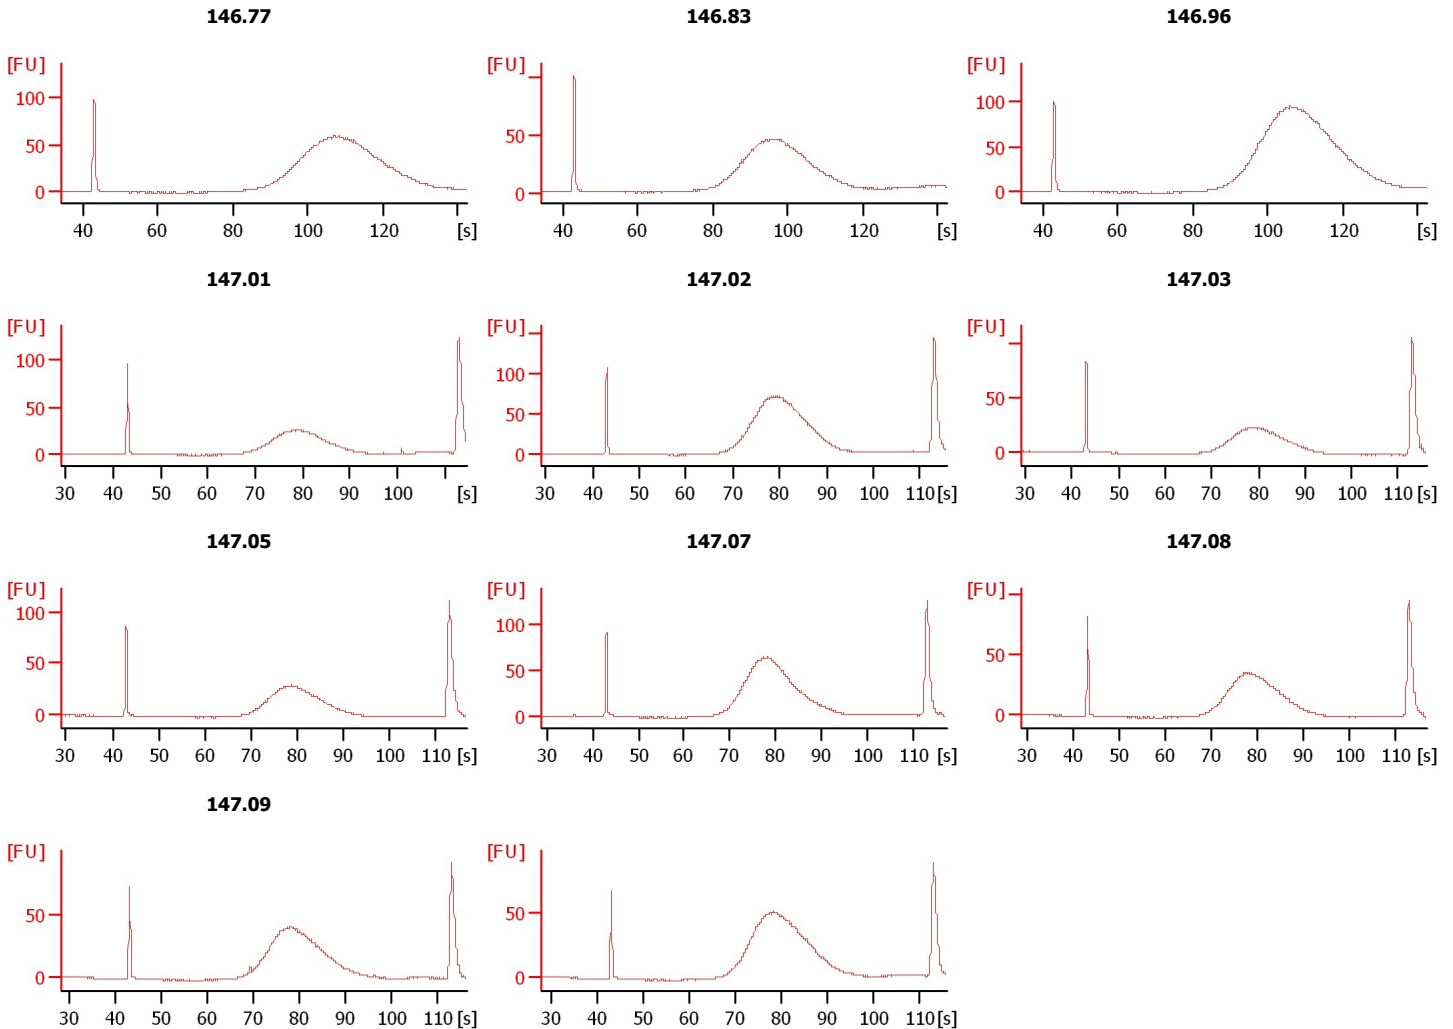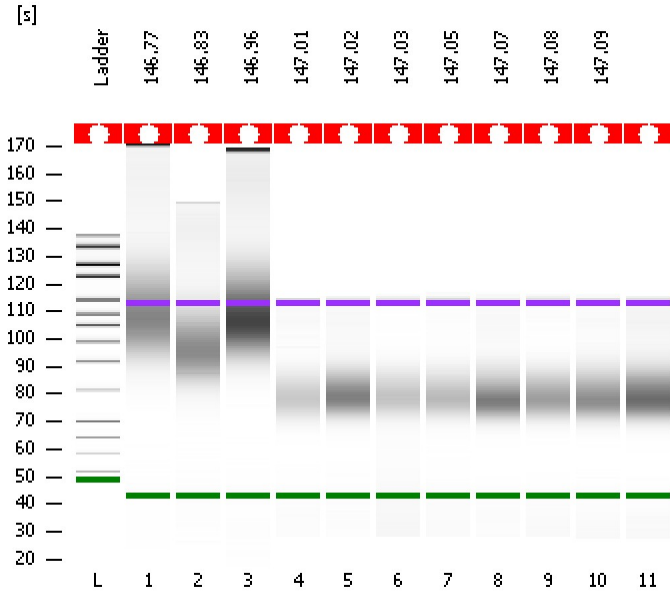

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-09-04\2014-09-04_008.xad

Created: 9/4/2014 4:11:57 PM
 Modified: 9/4/2014 4:53:34 PM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
146.77		<input type="checkbox"/>	✓			
146.83		<input type="checkbox"/>	✓			
146.96		<input type="checkbox"/>	✓			
147.01		<input type="checkbox"/>	✓			
147.02		<input type="checkbox"/>	✓			
147.03		<input type="checkbox"/>	✓			
147.05		<input type="checkbox"/>	✓			
147.07		<input type="checkbox"/>	✓			
147.08		<input type="checkbox"/>	✓			
147.09		<input type="checkbox"/>	✓			
Ladder		<input type="checkbox"/>	✓			

Chip Lot #

Reagent Kit Lot #

Chip Comments :

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-09-04\2014-09-04_008.xad

Created: 9/4/2014 4:11:57 PM
 Modified: 9/4/2014 4:53:34 PM

Electrophoresis Assay Details

General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12
 Minimum Visible Range [s] : 32
 Maximum Visible Range [s] : 138
 Start Analysis Time Range [s] : 33
 End Analysis Time Range [s] : 137.5
 Ladder Concentration [pg/μl] : 1950
 Uses Standard Area for Ladder Fragments
 Lower Marker Concentration [pg/μl] : 125
 Upper Marker Concentration [pg/μl] : 75
 Used Upper Marker for Quantitation
 Standard Curve Fit is Point to Point
 Show Data Aligned to Lower and Upper Marker

Integrator Settings

Integration Start Time [s] : 33.05
 Integration End Time [s] : 137
 Slope Threshold : 0.8
 Height Threshold [FU] : 5
 Area Threshold : 0.1
 Width Threshold [s] : 0.6
 Baseline Plateau [s] : 0.5

Filter Settings

Filter Width [s] : 0.5
 Polynomial Order : 4


Ladder

Ladder Peak	Size	Area
1	35	160
2	50	210
3	100	208
4	150	221
5	200	242
6	300	270
7	400	305
8	500	306
9	600	336
10	700	321
11	1000	366
12	2000	413
13	3000	411
14	7000	400
15	10380	214

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-09-04\2014-09-04_008.xad

Created: 9/4/2014 4:11:57 PM
 Modified: 9/4/2014 4:53:34 PM

Electropherogram Summary

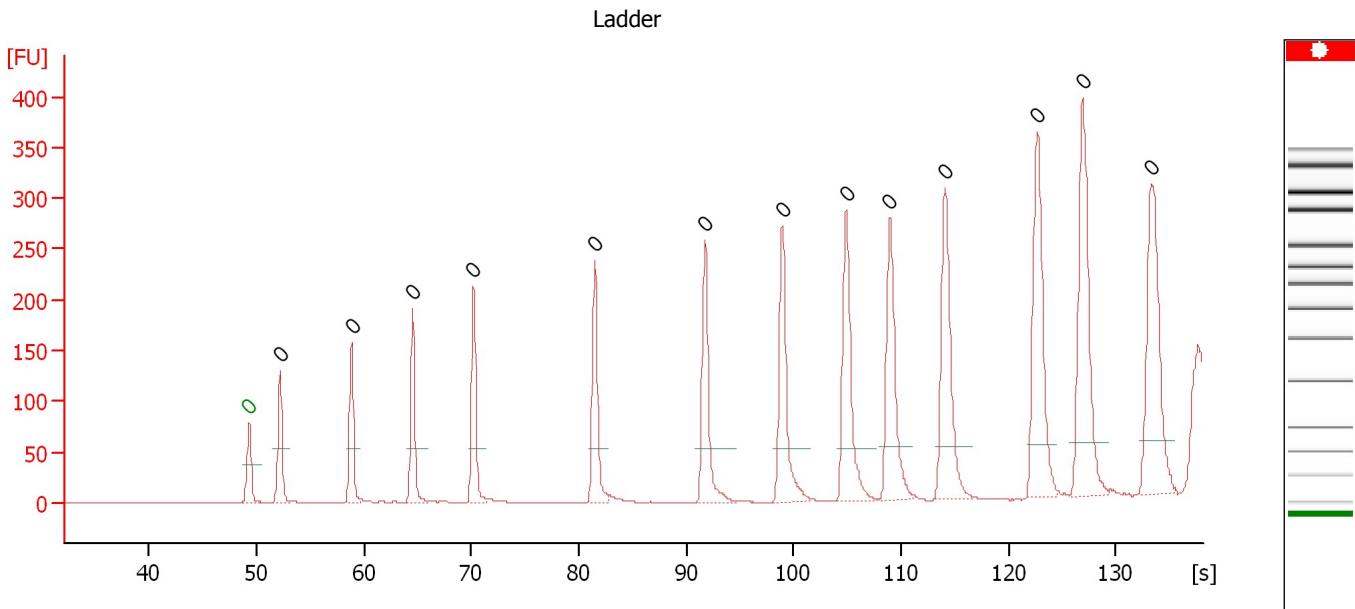

Overall Results for Ladder

Noise: 0.2


Peak table for Ladder

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	0	0.00	0.0	Lower Marker
2	0	0.00	0.0	Ladder Peak
3	0	0.00	0.0	Ladder Peak
4	0	0.00	0.0	Ladder Peak
5	0	0.00	0.0	Ladder Peak
6	0	0.00	0.0	Ladder Peak
7	0	0.00	0.0	Ladder Peak
8	0	0.00	0.0	Ladder Peak
9	0	0.00	0.0	Ladder Peak
10	0	0.00	0.0	Ladder Peak
11	0	0.00	0.0	Ladder Peak
12	0	0.00	0.0	Ladder Peak
13	0	0.00	0.0	Ladder Peak
14	0	0.00	0.0	Ladder Peak

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-09-04\2014-09-04_008.xad

Created: 9/4/2014 4:11:57 PM
 Modified: 9/4/2014 4:53:34 PM

Electropherogram Summary Continued ...

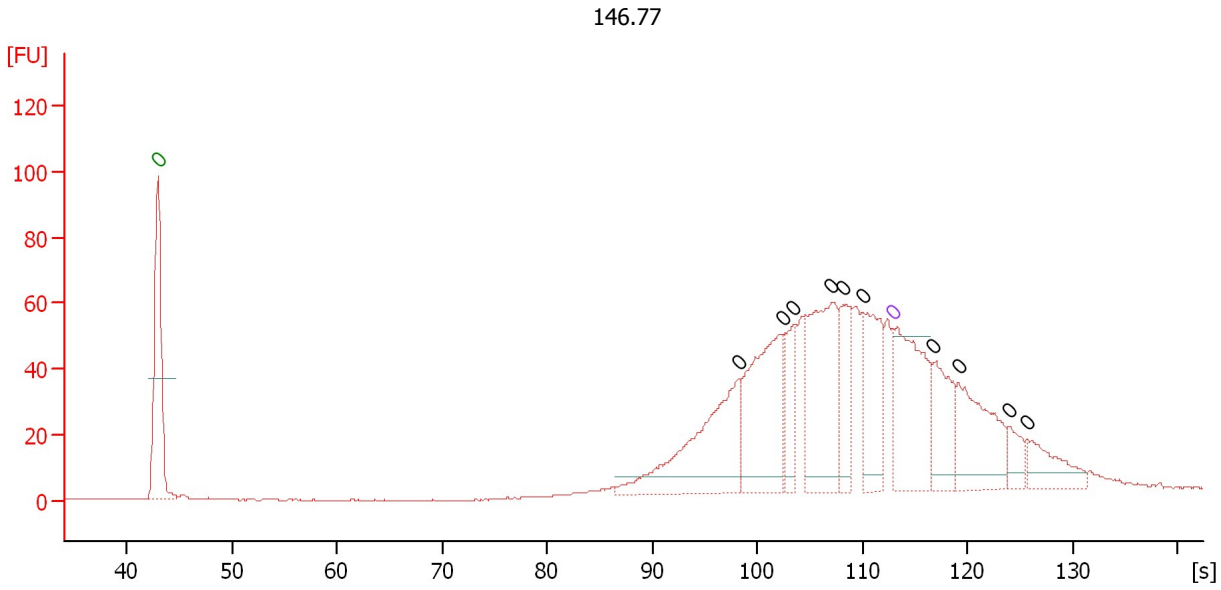

Overall Results for sample 1 : 146.77

Number of peaks found: 10 Noise: 0.2


Peak table for sample 1 : 146.77

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	0	0.00	0.0	Lower Marker
2	0	0.00	0.0	
3	0	0.00	0.0	
4	0	0.00	0.0	
5	0	0.00	0.0	
6	0	0.00	0.0	
7	0	0.00	0.0	
8	0	0.00	0.0	Upper Marker
9	0	0.00	0.0	
10	0	0.00	0.0	
11	0	0.00	0.0	
12	0	0.00	0.0	

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-09-04\2014-09-04_008.xad

Created: 9/4/2014 4:11:57 PM
 Modified: 9/4/2014 4:53:34 PM

Electropherogram Summary Continued ...

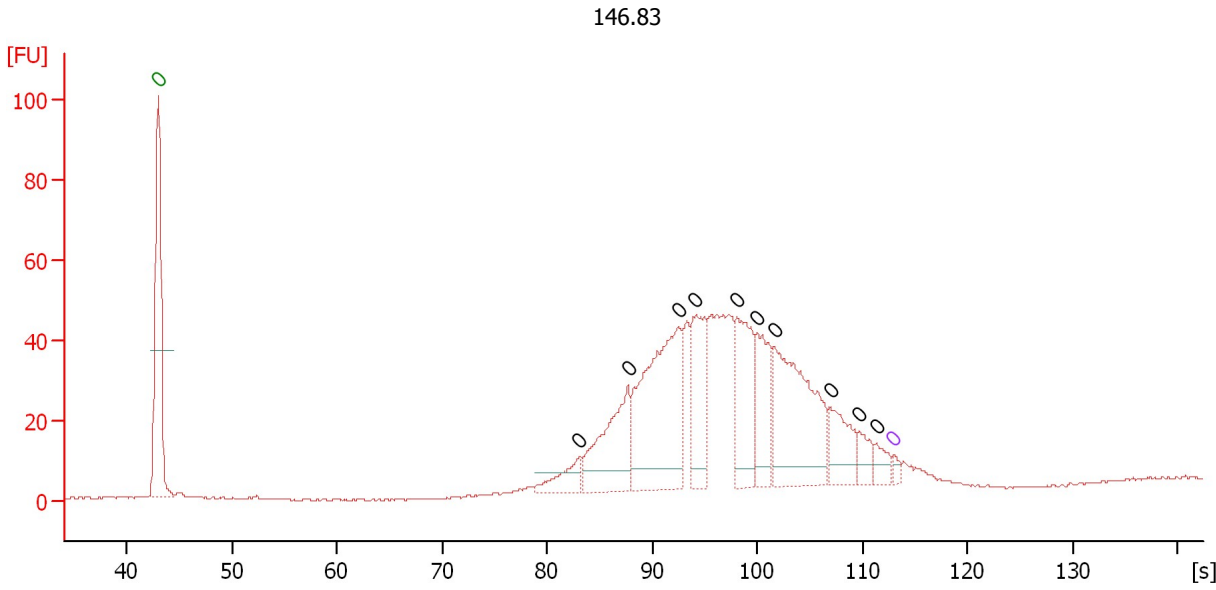

Overall Results for sample 2 : 146.83

Number of peaks found: 10 Noise: 0.2


Peak table for sample 2 : 146.83

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	0	0.00	0.0	Lower Marker
2	0	0.00	0.0	
3	0	0.00	0.0	
4	0	0.00	0.0	
5	0	0.00	0.0	
6	0	0.00	0.0	
7	0	0.00	0.0	
8	0	0.00	0.0	
9	0	0.00	0.0	
10	0	0.00	0.0	
11	0	0.00	0.0	
12	0	0.00	0.0	Upper Marker

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-09-04\2014-09-04_008.xad

Created: 9/4/2014 4:11:57 PM
 Modified: 9/4/2014 4:53:34 PM

Electropherogram Summary Continued ...

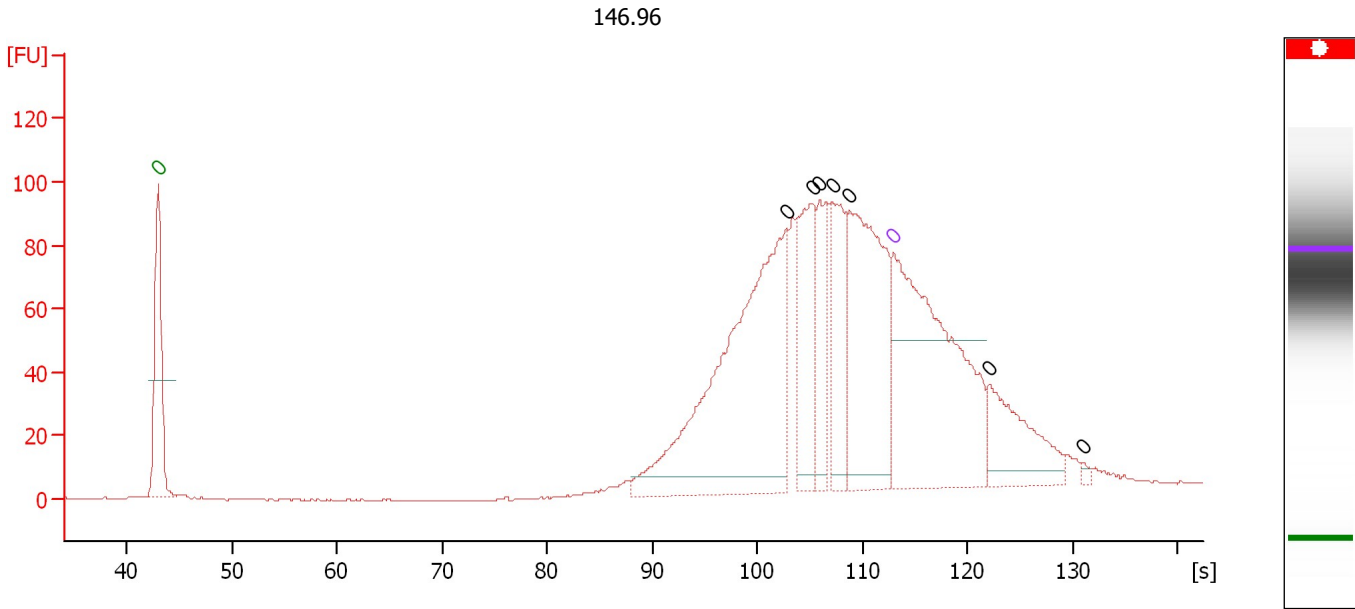

Overall Results for sample 3 : 146.96

Number of peaks found: 7 Noise: 0.2


Peak table for sample 3 : 146.96

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	0	0.00	0.0	Lower Marker
2	0	0.00	0.0	
3	0	0.00	0.0	
4	0	0.00	0.0	
5	0	0.00	0.0	
6	0	0.00	0.0	
7	0	0.00	0.0	Upper Marker
8	0	0.00	0.0	
9	0	0.00	0.0	

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-09-04\2014-09-04_008.xad

Created: 9/4/2014 4:11:57 PM
 Modified: 9/4/2014 4:53:34 PM

Electropherogram Summary Continued ...

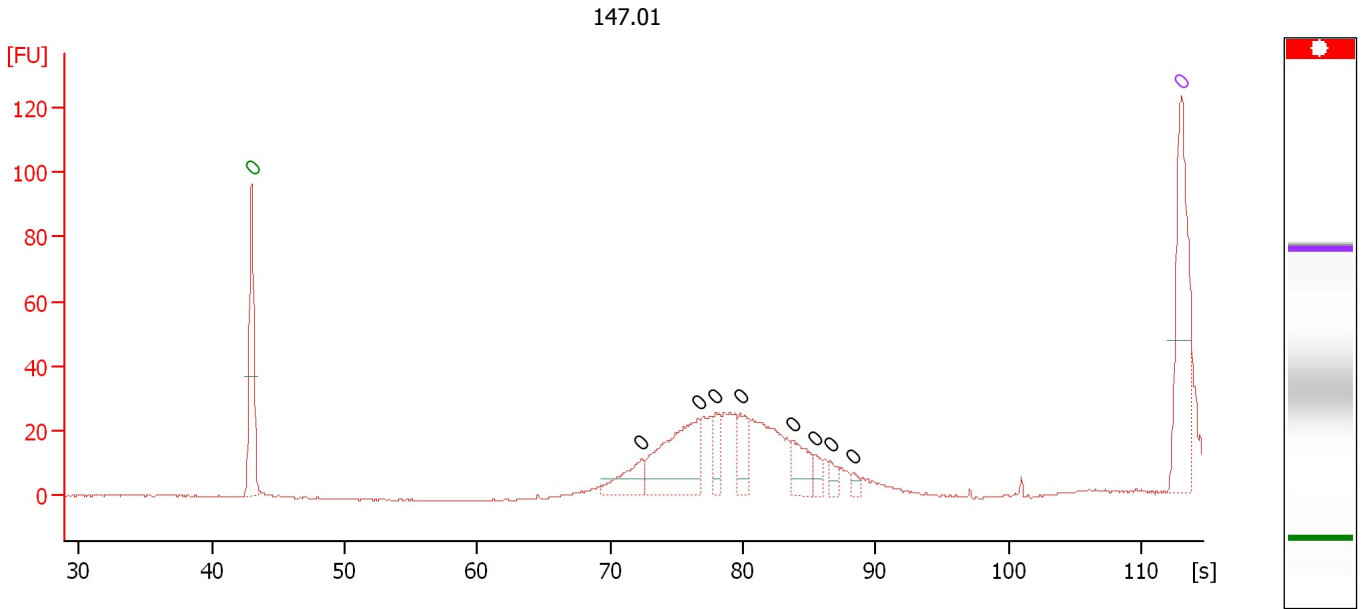

Overall Results for sample 4 : 147.01

Number of peaks found: 8 Noise: 0.2


Peak table for sample 4 : 147.01

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	0	0.00	0.0	Lower Marker
2	0	0.00	0.0	
3	0	0.00	0.0	
4	0	0.00	0.0	
5	0	0.00	0.0	
6	0	0.00	0.0	
7	0	0.00	0.0	
8	0	0.00	0.0	
9	0	0.00	0.0	
10	0	0.00	0.0	Upper Marker

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-09-04\2014-09-04_008.xad

Created: 9/4/2014 4:11:57 PM
 Modified: 9/4/2014 4:53:34 PM

Electropherogram Summary Continued ...

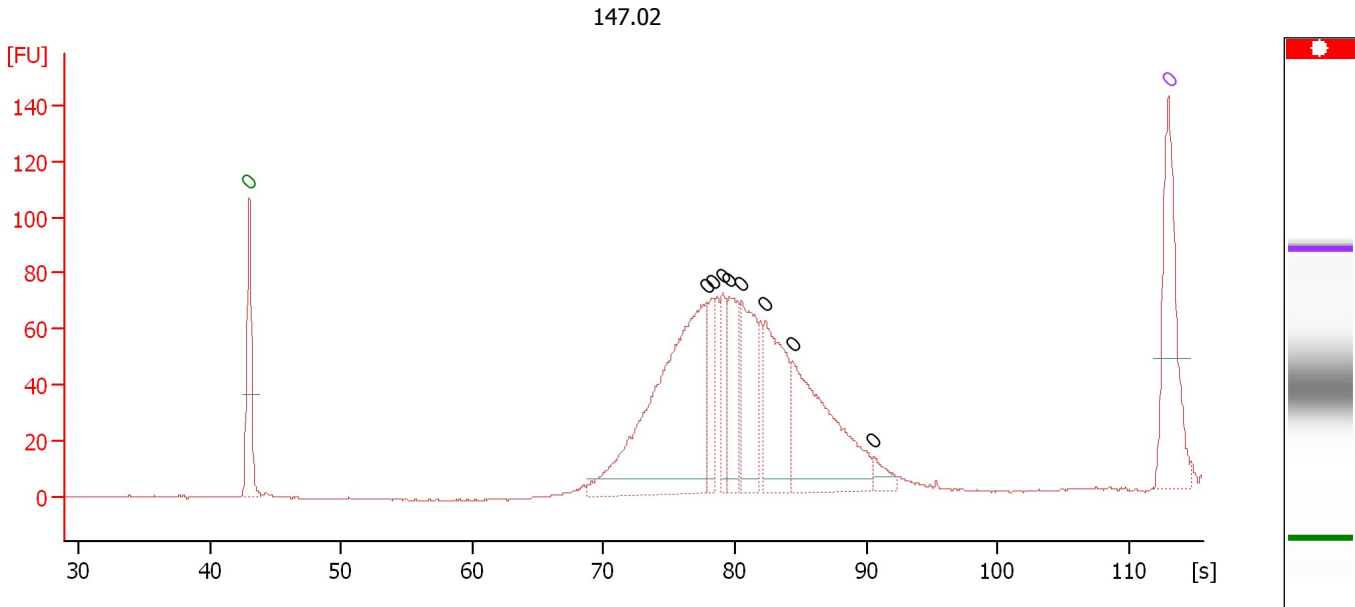

Overall Results for sample 5 : 147.02

Number of peaks found: 8 Noise: 0.2


Peak table for sample 5 : 147.02

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	0	0.00	0.0	Lower Marker
2	0	0.00	0.0	
3	0	0.00	0.0	
4	0	0.00	0.0	
5	0	0.00	0.0	
6	0	0.00	0.0	
7	0	0.00	0.0	
8	0	0.00	0.0	
9	0	0.00	0.0	
10	0	0.00	0.0	Upper Marker

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-09-04\2014-09-04_008.xad

Created: 9/4/2014 4:11:57 PM
 Modified: 9/4/2014 4:53:34 PM

Electropherogram Summary Continued ...

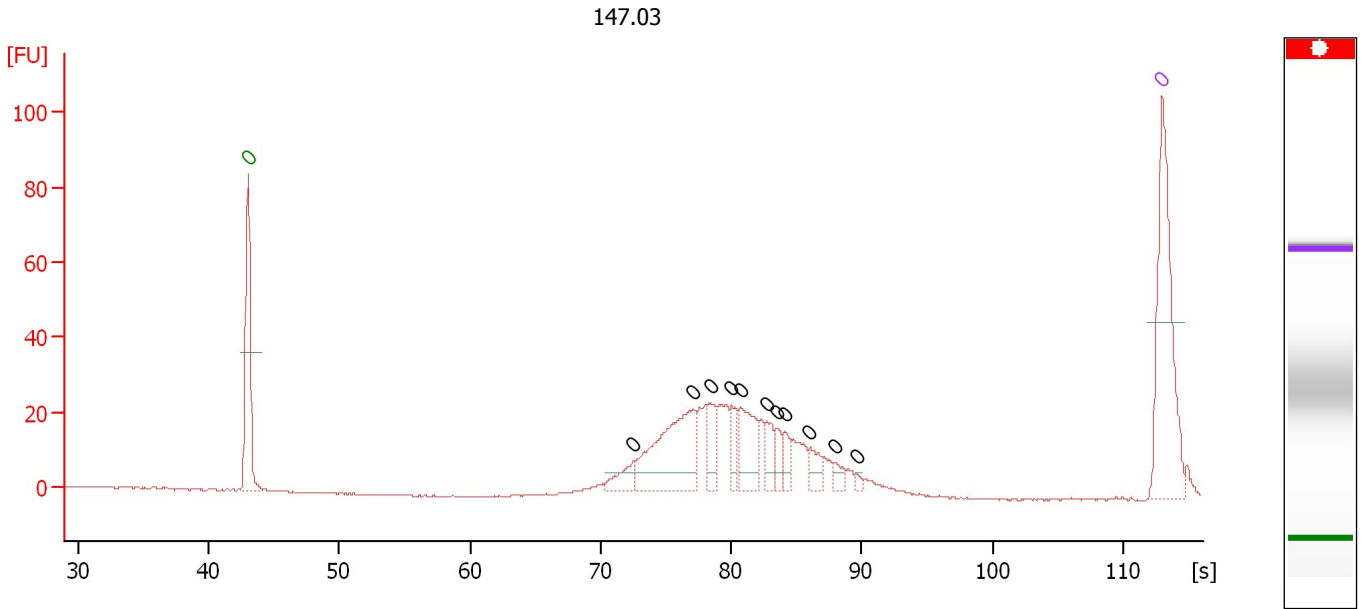

Overall Results for sample 6 : 147.03

Number of peaks found: 11 Noise: 0.2


Peak table for sample 6 : 147.03

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	0	0.00	0.0	Lower Marker
2	0	0.00	0.0	
3	0	0.00	0.0	
4	0	0.00	0.0	
5	0	0.00	0.0	
6	0	0.00	0.0	
7	0	0.00	0.0	
8	0	0.00	0.0	
9	0	0.00	0.0	
10	0	0.00	0.0	
11	0	0.00	0.0	
12	0	0.00	0.0	
13	0	0.00	0.0	Upper Marker

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-09-04\2014-09-04_008.xad

Created: 9/4/2014 4:11:57 PM
 Modified: 9/4/2014 4:53:34 PM

Electropherogram Summary Continued ...

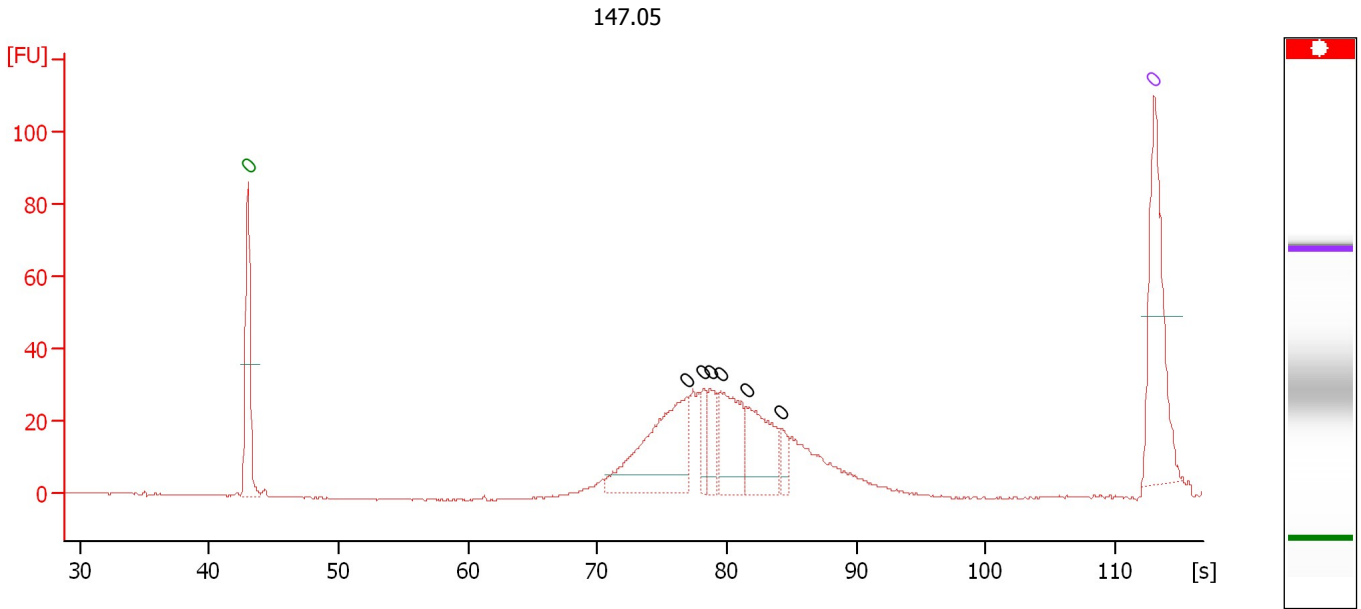

Overall Results for sample 7 : 147.05

Number of peaks found: 6 Noise: 0.2


Peak table for sample 7 : 147.05

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	0	0.00	0.0	Lower Marker
2	0	0.00	0.0	
3	0	0.00	0.0	
4	0	0.00	0.0	
5	0	0.00	0.0	
6	0	0.00	0.0	
7	0	0.00	0.0	
8	0	0.00	0.0	Upper Marker

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-09-04\2014-09-04_008.xad

Created: 9/4/2014 4:11:57 PM
 Modified: 9/4/2014 4:53:34 PM

Electropherogram Summary Continued ...

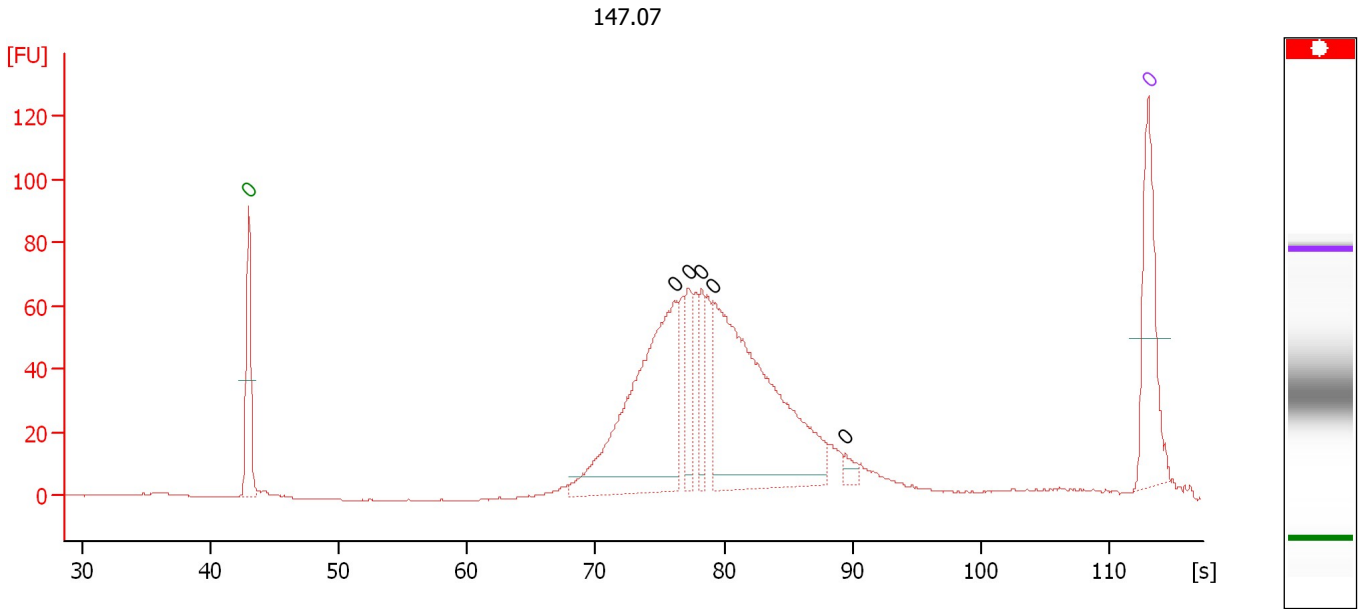

Overall Results for sample 8 : 147.07

Number of peaks found: 5 Noise: 0.2


Peak table for sample 8 : 147.07

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	0	0.00	0.0	Lower Marker
2	0	0.00	0.0	
3	0	0.00	0.0	
4	0	0.00	0.0	
5	0	0.00	0.0	
6	0	0.00	0.0	
7	0	0.00	0.0	Upper Marker

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-09-04\2014-09-04_008.xad

Created: 9/4/2014 4:11:57 PM
 Modified: 9/4/2014 4:53:34 PM

Electropherogram Summary Continued ...

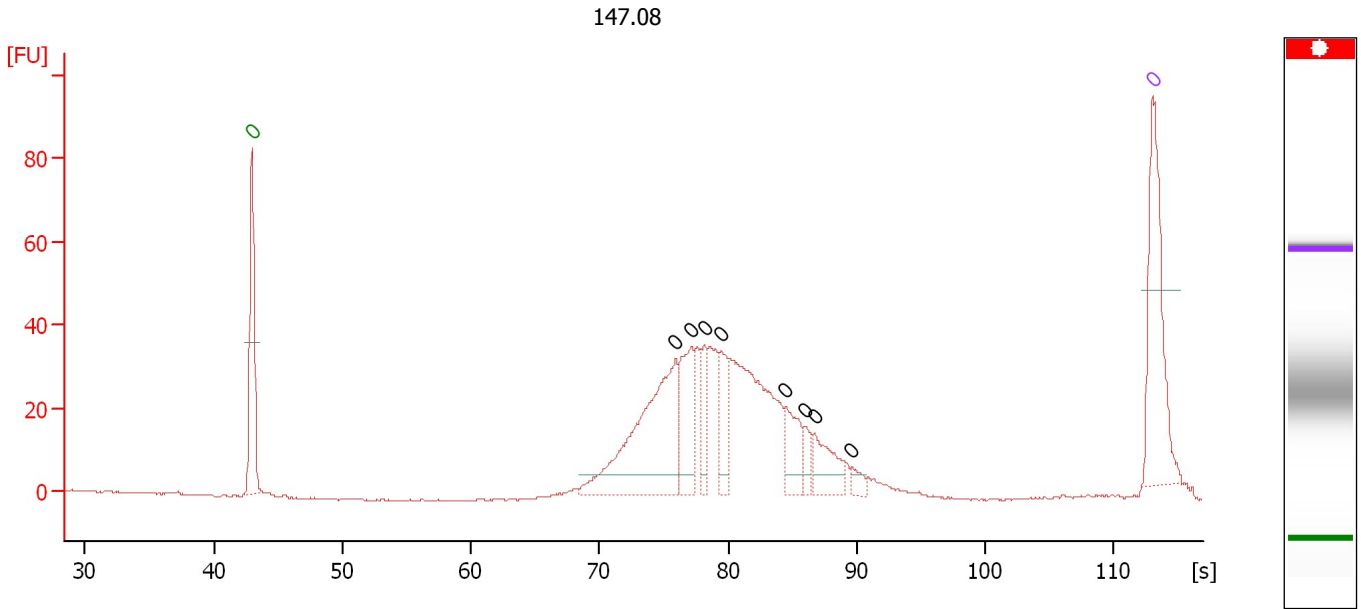

Overall Results for sample 9 : 147.08

Number of peaks found: 8 Noise: 0.2


Peak table for sample 9 : 147.08

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	0	0.00	0.0	Lower Marker
2	0	0.00	0.0	
3	0	0.00	0.0	
4	0	0.00	0.0	
5	0	0.00	0.0	
6	0	0.00	0.0	
7	0	0.00	0.0	
8	0	0.00	0.0	
9	0	0.00	0.0	
10	0	0.00	0.0	Upper Marker

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-09-04\2014-09-04_008.xad

Created: 9/4/2014 4:11:57 PM
 Modified: 9/4/2014 4:53:34 PM

Electropherogram Summary Continued ...

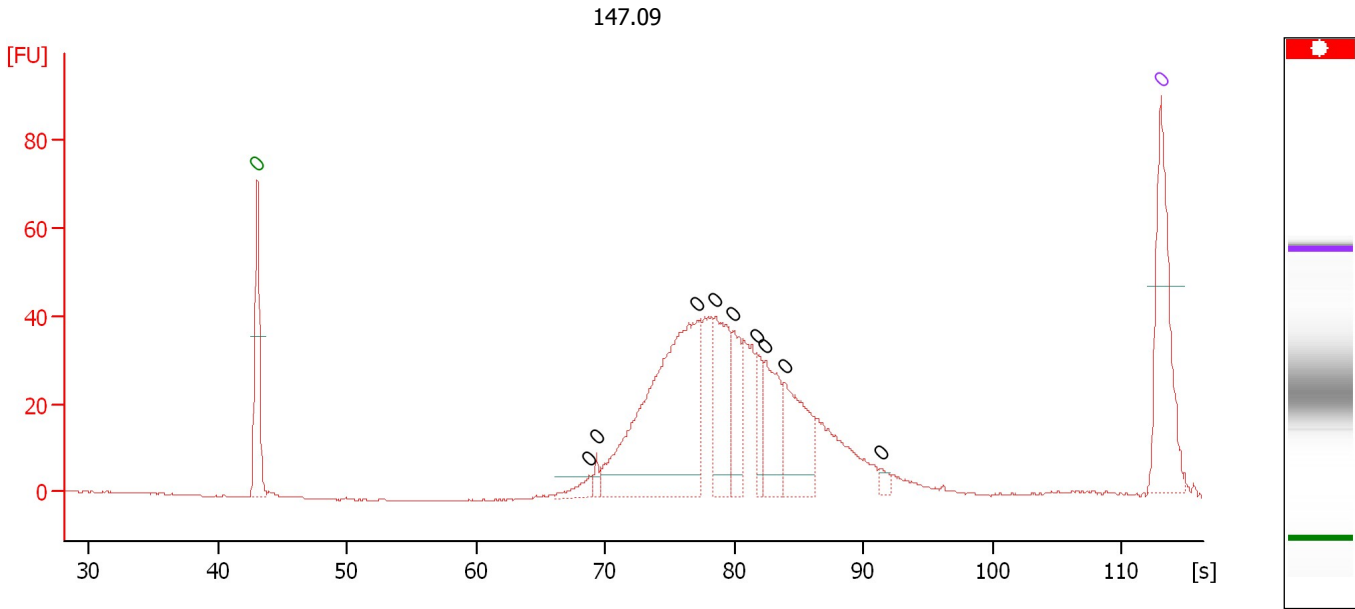

Overall Results for sample 10 : 147.09

Number of peaks found: 9 Noise: 0.2


Peak table for sample 10 : 147.09

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	0	0.00	0.0	Lower Marker
2	0	0.00	0.0	
3	0	0.00	0.0	
4	0	0.00	0.0	
5	0	0.00	0.0	
6	0	0.00	0.0	
7	0	0.00	0.0	
8	0	0.00	0.0	
9	0	0.00	0.0	
10	0	0.00	0.0	
11	0	0.00	0.0	Upper Marker

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...ents and Settings\Bioanalyzer\2014-09-04\2014-09-04_008.xad

Created: 9/4/2014 4:11:57 PM
Modified: 9/4/2014 4:53:34 PM

Electropherogram Summary Continued ...

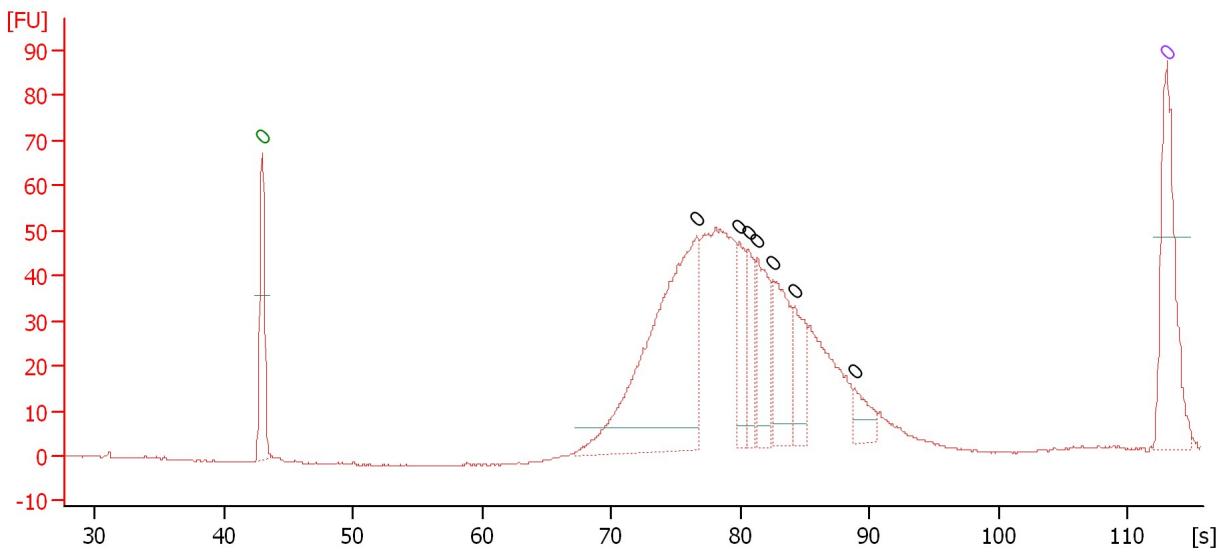

Overall Results for sample 11 :

Number of peaks found: 7 Noise: 0.1


Peak table for sample 11 :

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	0	0.00	0.0	Lower Marker
2	0	0.00	0.0	
3	0	0.00	0.0	
4	0	0.00	0.0	
5	0	0.00	0.0	
6	0	0.00	0.0	
7	0	0.00	0.0	
8	0	0.00	0.0	
9	0	0.00	0.0	Upper Marker

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...ents and Settings\Bioanalyzer\2014-09-04\2014-09-04_008.xad

Created: 9/4/2014 4:11:57 PM
Modified: 9/4/2014 4:53:34 PM

Gel Image

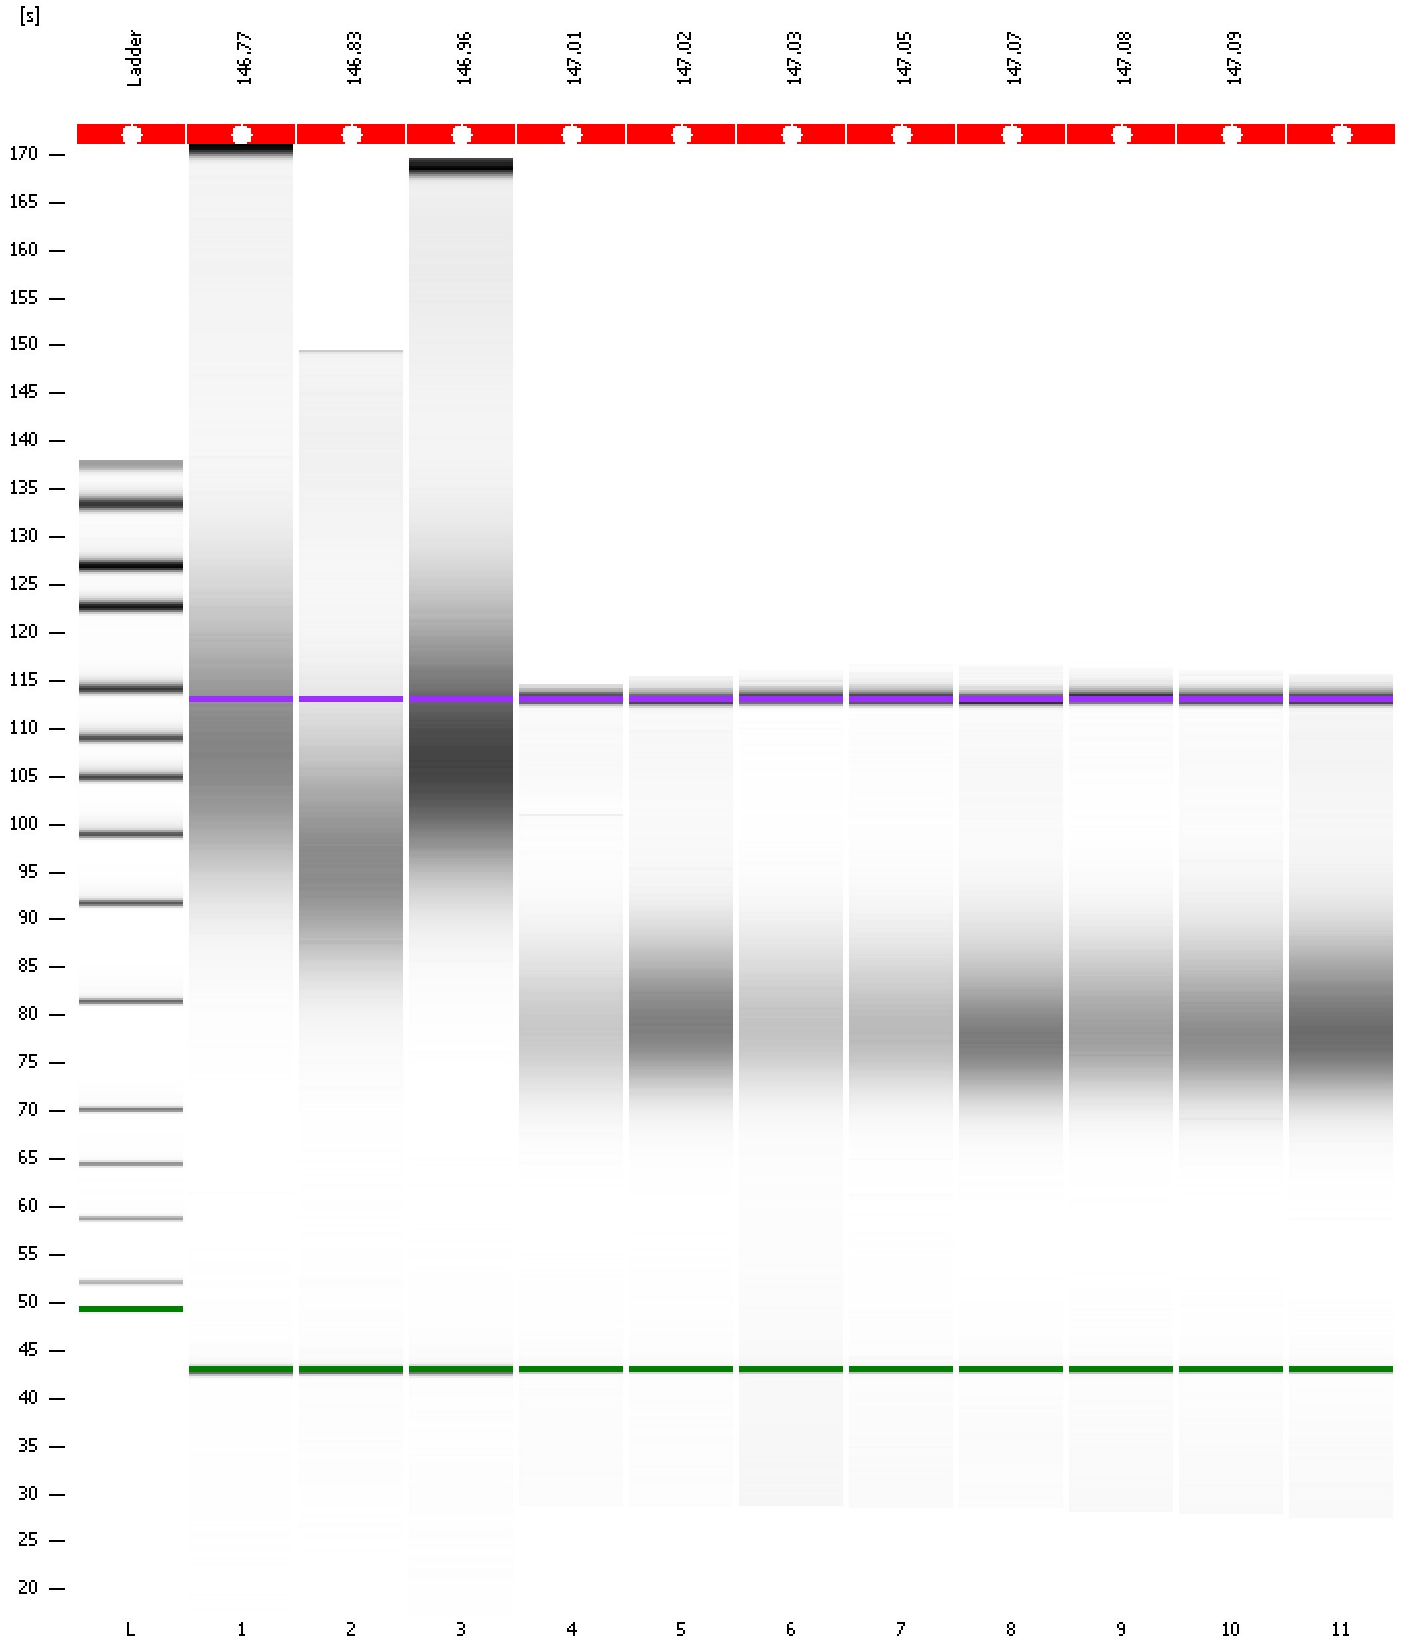

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-09-04\2014-09-04_008.xad

Created: 9/4/2014 4:11:57 PM
 Modified: 9/4/2014 4:53:34 PM

Run Logbook

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 12)		Instrument	Run		9/4/2014 4:52:25 PM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Run started on port 1 (File: C:\Documents and Settings\Bioanalyzer\2014-09-04\2014-09-04_008.xad)		Instrument	Run		9/4/2014 4:12:03 PM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Product Number : G2938B		Instrument	Run		9/4/2014 4:12:03 PM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Name :		Instrument	Run		9/4/2014 4:12:03 PM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Vendor : Agilent Technologies		Instrument	Run		9/4/2014 4:12:03 PM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Serial# : DE13701086		Instrument	Run		9/4/2014 4:12:03 PM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Firmware : C.01.069		Instrument	Run		9/4/2014 4:12:03 PM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Cartridge : Electrode		Instrument	Run		9/4/2014 4:12:03 PM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1