


Assay Class: High Sensitivity DNA Assay
Data Path: C:\...ents and Settings\Bioanalyzer\2014-10-28\2014-10-28_002.xad

Created: 10/28/2014 2:22:26 PM
Modified: 10/28/2014 3:03:27 PM

Electrophoresis File Run Summary

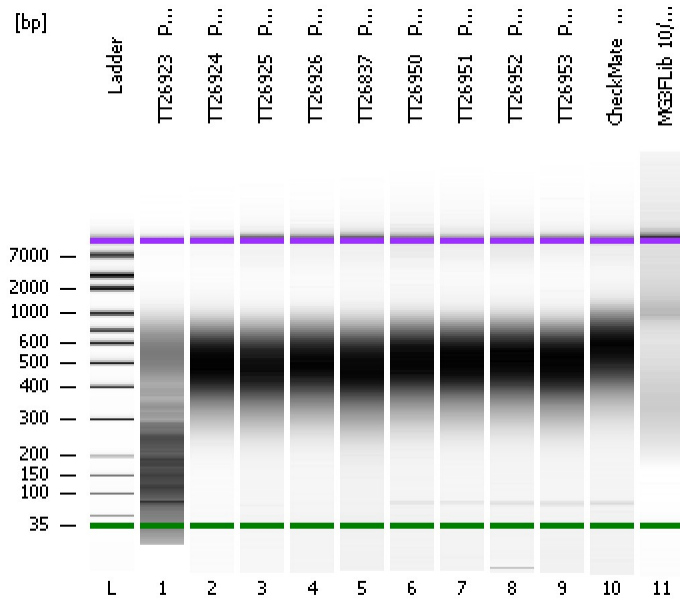

Instrument Information:

Instrument Name: DE13701086 Firmware: C.01.069
Serial#: DE13701086 Type: G2938B


Assay Information:

Assay Origin Path: C:\Program Files\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy
Assay Class: High Sensitivity DNA Assay
Version: 1.03
Assay Comments: Copyright © 2003-2010 Agilent Technologies


Chip Information:

Chip Lot #:
Reagent Kit Lot #:
Chip Comments:


TT26923 PCR Free Library

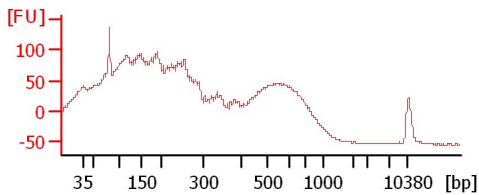


TT26924 PCR Free Library

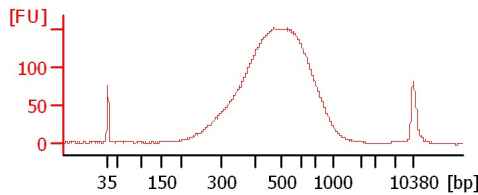


TT26925 PCR Free Library

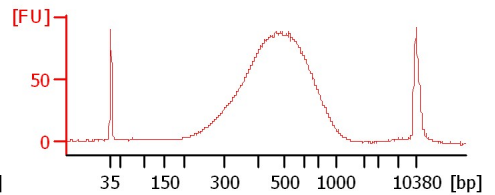


TT26926 PCR Free Library

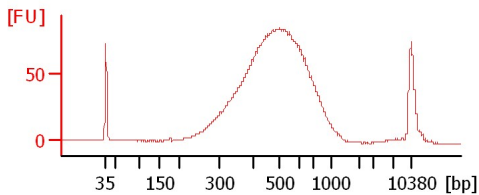


TT26837 PCR Free Library

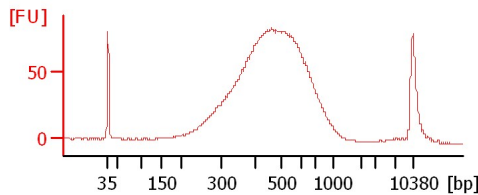


TT26950 PCR Free Library

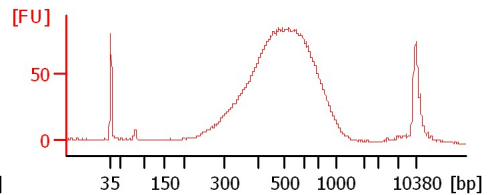


TT26951 PCR Free Library

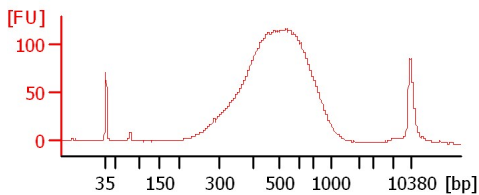


TT26952 PCR Free Library

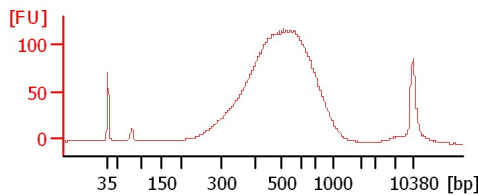


TT26953 PCR Free Library

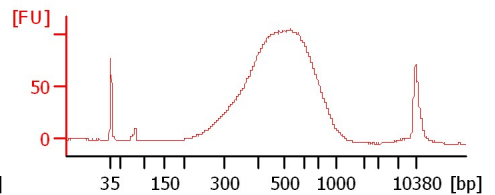

CheckMate PCR Free Library

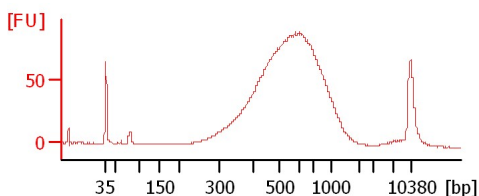

MG3FLib 10/24/14 (1:5)

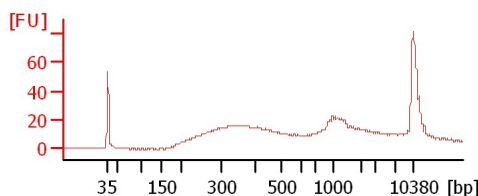

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...ents and Settings\Bioanalyzer\2014-10-28\2014-10-28_002.xad

Created: 10/28/2014 2:22:26 PM
Modified: 10/28/2014 3:03:27 PM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
TT26923	PCR Free Library	<input type="checkbox"/>	✓			
TT26924	PCR Free Library	<input type="checkbox"/>	✓			
TT26925	PCR Free Library	<input type="checkbox"/>	✓			
TT26926	PCR Free Library	<input type="checkbox"/>	✓			
TT26837	PCR Free Library	<input type="checkbox"/>	✓			
TT26950	PCR Free Library	<input type="checkbox"/>	✓			
TT26951	PCR Free Library	<input type="checkbox"/>	✓			
TT26952	PCR Free Library	<input type="checkbox"/>	✓			
TT26953	PCR Free Library	<input type="checkbox"/>	✓			
CheckMate	PCR Free Library	<input type="checkbox"/>	✓			
MG3FLib	10/24/14 (1:5)	<input type="checkbox"/>	✓			
Ladder		<input type="checkbox"/>	✓			

Chip Lot #

Reagent Kit Lot #

Chip Comments :

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...ents and Settings\Bioanalyzer\2014-10-28\2014-10-28_002.xad

Created: 10/28/2014 2:22:26 PM
Modified: 10/28/2014 3:03:27 PM

Electrophoresis Assay Details

General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12
Minimum Visible Range [s] : 32
Maximum Visible Range [s] : 138
Start Analysis Time Range [s] : 33
End Analysis Time Range [s] : 137.5
Ladder Concentration [pg/μl] : 1950
Uses Standard Area for Ladder Fragments
Lower Marker Concentration [pg/μl] : 125
Upper Marker Concentration [pg/μl] : 75
Used Upper Marker for Quantitation
Standard Curve Fit is Point to Point
Show Data Aligned to Lower and Upper Marker

Integrator Settings

Integration Start Time [s] : 33.05
Integration End Time [s] : 137
Slope Threshold : 0.8
Height Threshold [FU] : 5
Area Threshold : 0.1
Width Threshold [s] : 0.6
Baseline Plateau [s] : 0.5

Filter Settings

Filter Width [s] : 0.5
Polynomial Order : 4


Ladder

Ladder Peak	Size	Area
1	35	160
2	50	210
3	100	208
4	150	221
5	200	242
6	300	270
7	400	305
8	500	306
9	600	336
10	700	321
11	1000	366
12	2000	413
13	3000	411
14	7000	400
15	10380	214

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-10-28\2014-10-28_002.xad

Created: 10/28/2014 2:22:26 PM
 Modified: 10/28/2014 3:03:27 PM

Electropherogram Summary

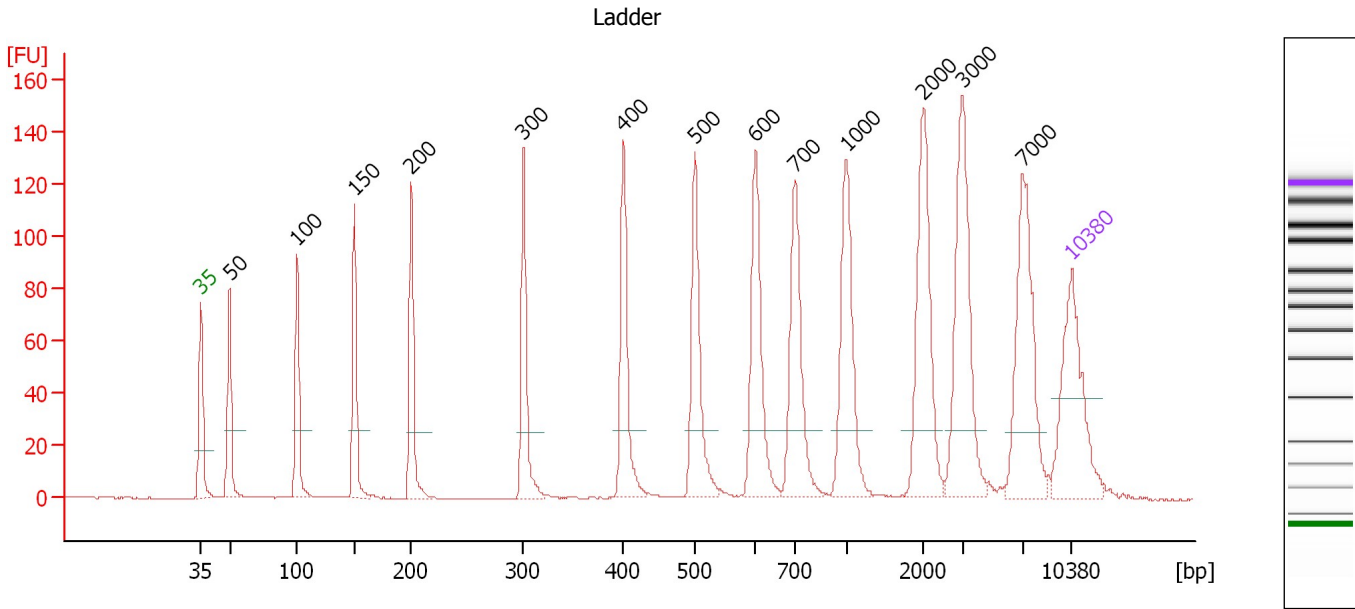

Overall Results for Ladder

Noise: 0.2


Peak table for Ladder

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	50	150.00	4,545.5	Ladder Peak
3	100	150.00	2,272.7	Ladder Peak
4	150	150.00	1,515.2	Ladder Peak
5	200	150.00	1,136.4	Ladder Peak
6	300	150.00	757.6	Ladder Peak
7	400	150.00	568.2	Ladder Peak
8	500	150.00	454.5	Ladder Peak
9	600	150.00	378.8	Ladder Peak
10	700	150.00	324.7	Ladder Peak
11	1,000	150.00	227.3	Ladder Peak
12	2,000	150.00	113.6	Ladder Peak
13	3,000	150.00	75.8	Ladder Peak
14	7,000	150.00	32.5	Ladder Peak
15	10,380	75.00	10.9	Upper Marker

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-10-28\2014-10-28_002.xad

Created: 10/28/2014 2:22:26 PM
 Modified: 10/28/2014 3:03:27 PM

Electropherogram Summary Continued ...

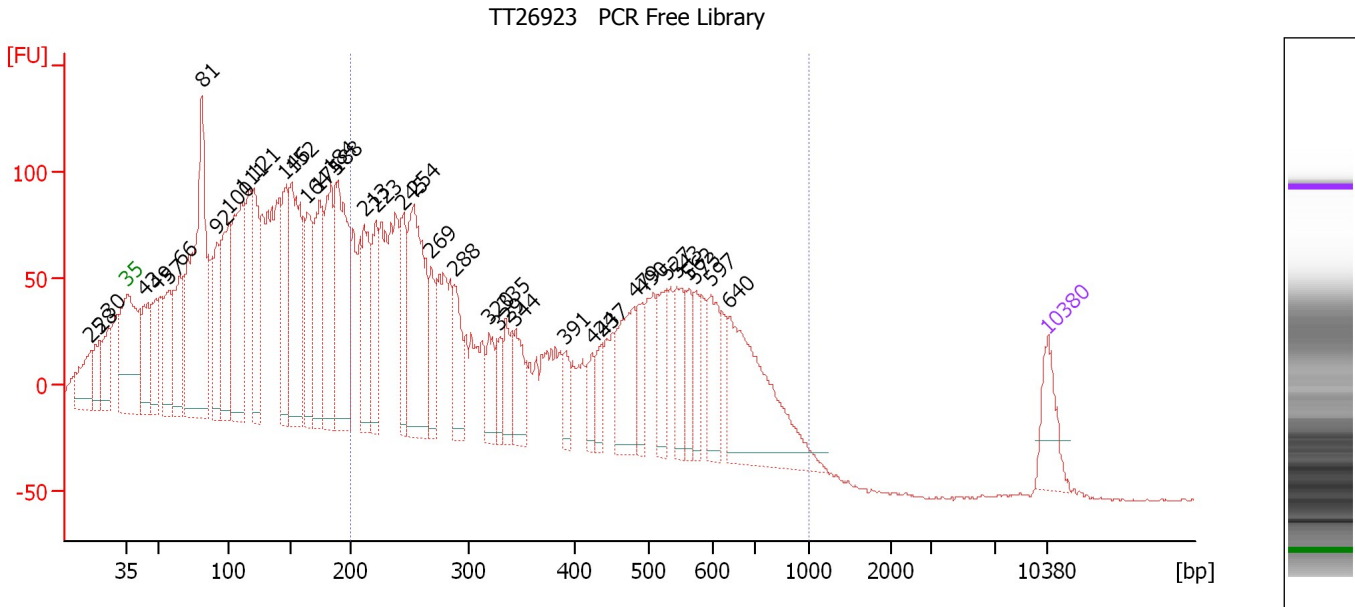

Overall Results for sample 1 : TT26923 PCR Free Library

Number of peaks found: 39 Corr. Area 1: 3,028.7
 Noise: 0.7

Peak table for sample 1 : TT26923 PCR Free Library

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	25	0.00	0.0	
2	28	0.00	0.0	
3	30	0.00	0.0	
4	35	125.00	5,411.3	Lower Marker
5	43	190.38	6,644.0	
6	49	178.73	5,504.0	
7	57	199.04	5,279.6	
8	66	235.34	5,422.2	
9	81	797.55	14,888.5	
10	92	192.37	3,166.2	
11	100	335.69	5,088.9	
12	111	461.28	6,302.5	
13	121	242.60	3,049.4	
14	146	284.80	2,947.6	
15	152	432.55	4,321.1	
16	164	254.51	2,344.2	
17	175	268.23	2,326.7	
18	184	288.15	2,367.6	
19	188	441.27	3,549.0	
20	213	200.28	1,428.0	
21	223	167.09	1,135.9	
22	245	154.08	953.0	
23	254	414.14	2,470.6	
24	269	102.56	578.0	
25	288	115.47	606.9	
26	320	81.06	384.3	

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-10-28\2014-10-28_002.xad

Created: 10/28/2014 2:22:26 PM
 Modified: 10/28/2014 3:03:27 PM

Electropherogram Summary Continued ...

... Peak table for sample 1 : TT26923 PCR Free Library

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
27	329	55.93	257.4	
28	335	83.79	378.7	
29	344	97.01	427.6	
30	391	52.13	202.0	
31	424	52.53	187.6	
32	437	51.80	179.6	
33	479	175.13	553.5	
34	490	67.22	207.9	
35	527	99.80	287.1	
36	543	109.72	306.4	
37	562	62.35	168.2	
38	573	65.66	173.7	
39	597	116.18	294.9	
40	640	359.74	851.4	
41	▶ 10,380	75.00	10.9	Upper Marker


Region table for sample 1 : TT26923 PCR Free Library

From [bp]	Average Size [bp]	To [bp]	Corr. Area	% of Total	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	417	1,000	3,028.7	49	40.9	3,825.27	17,814.1	■

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-10-28\2014-10-28_002.xad

Created: 10/28/2014 2:22:26 PM
 Modified: 10/28/2014 3:03:27 PM

Electropherogram Summary Continued ...

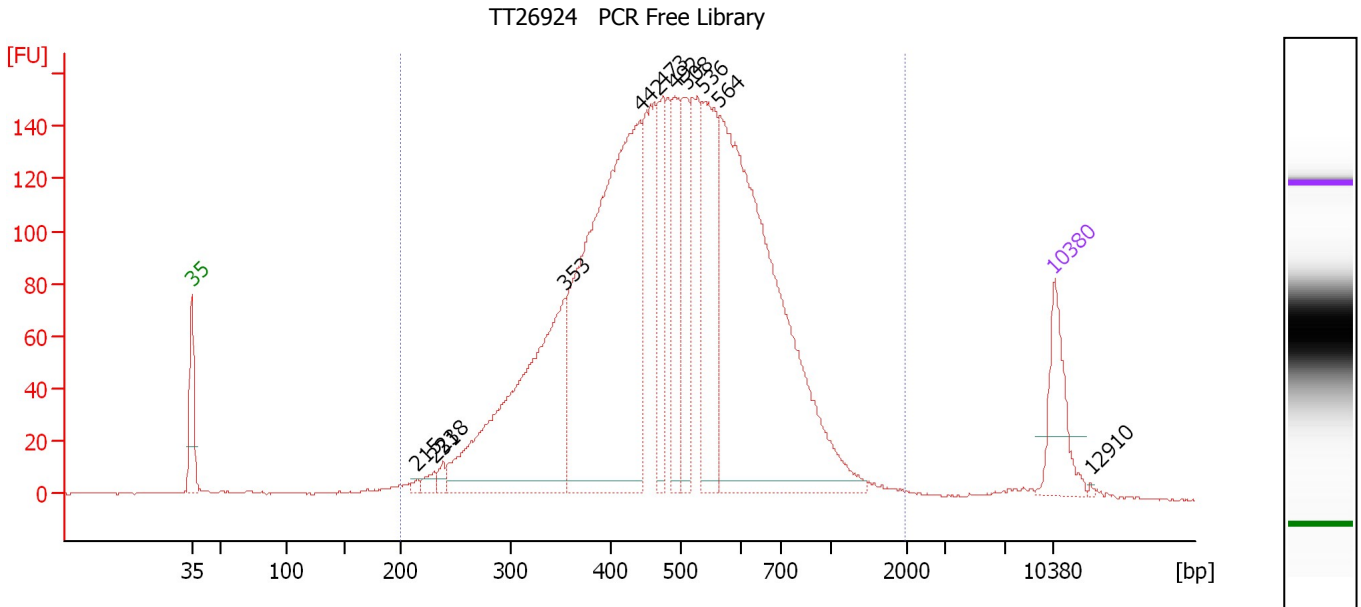

Overall Results for sample 2 : TT26924 PCR Free Library

Number of peaks found: 11 Corr. Area 1: 3,693.9
 Noise: 0.3

Peak table for sample 2 : TT26924 PCR Free Library

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	215	7.46	52.6	
3	231	15.10	99.1	
4	238	14.95	95.0	
5	353	526.88	2,262.5	
6	442	866.91	2,971.3	
7	473	130.91	419.2	
8	492	121.47	374.1	
9	508	135.05	402.8	
10	536	231.07	653.6	
11	564	863.23	2,317.9	
12	10,380	75.00	10.9	Upper Marker
13	12,910	0.00	0.0	


Region table for sample 2 : TT26924 PCR Free Library

From [bp]	Average Size [bp]	To [bp]	Corr. Area	% of Total	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	509	1,972	3,693.9	97	35.3	3,529.18	12,048.7	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-10-28\2014-10-28_002.xad

Created: 10/28/2014 2:22:26 PM
 Modified: 10/28/2014 3:03:27 PM

Electropherogram Summary Continued ...

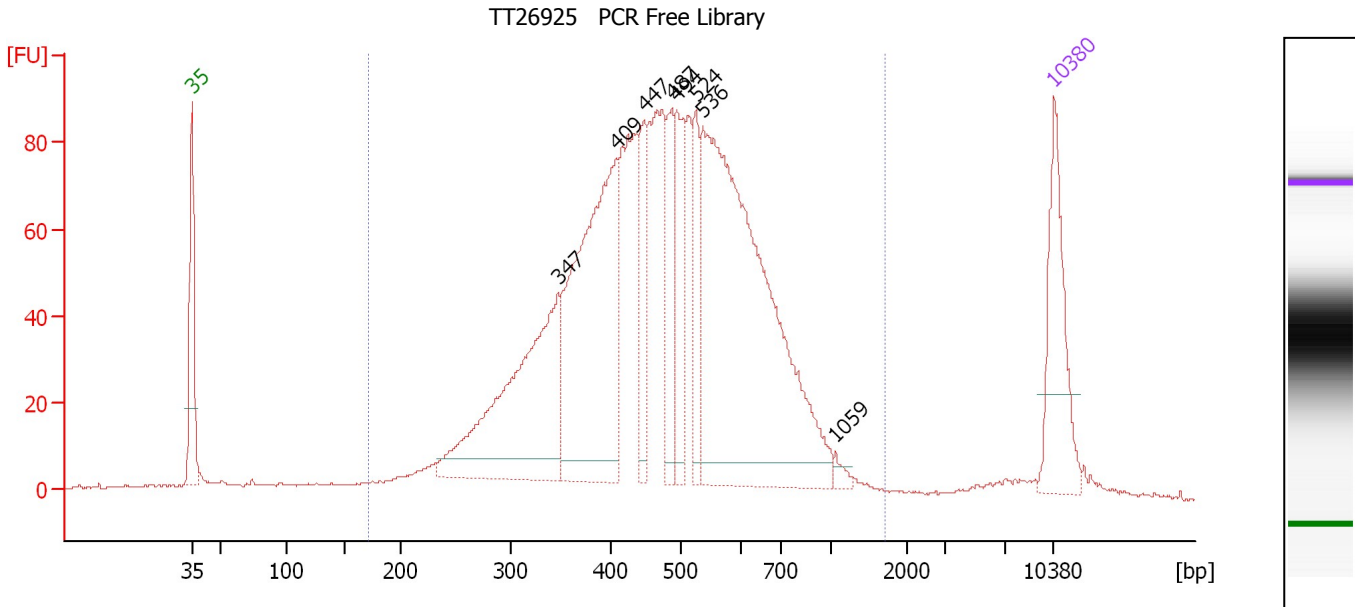

Overall Results for sample 3 : TT26925 PCR Free Library

Number of peaks found: 8 Corr. Area 1: 2,149.6
 Noise: 0.2

Peak table for sample 3 : TT26925 PCR Free Library

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	347	267.14	1,166.4	
3	409	322.22	1,192.9	
4	447	71.02	240.7	
5	487	67.38	209.8	
6	494	70.68	216.9	
7	524	55.04	159.1	
8	536	513.83	1,453.8	
9	1,059	5.85	8.4	
10	10,380	75.00	10.9	Upper Marker


Region table for sample 3 : TT26925 PCR Free Library

From [bp]	Average Size [bp]	To [bp]	Corr. Area	% of Total	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
171	490	1,696	2,149.6	96	32.6	1,865.02	6,608.7	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-10-28\2014-10-28_002.xad

Created: 10/28/2014 2:22:26 PM
 Modified: 10/28/2014 3:03:27 PM

Electropherogram Summary Continued ...

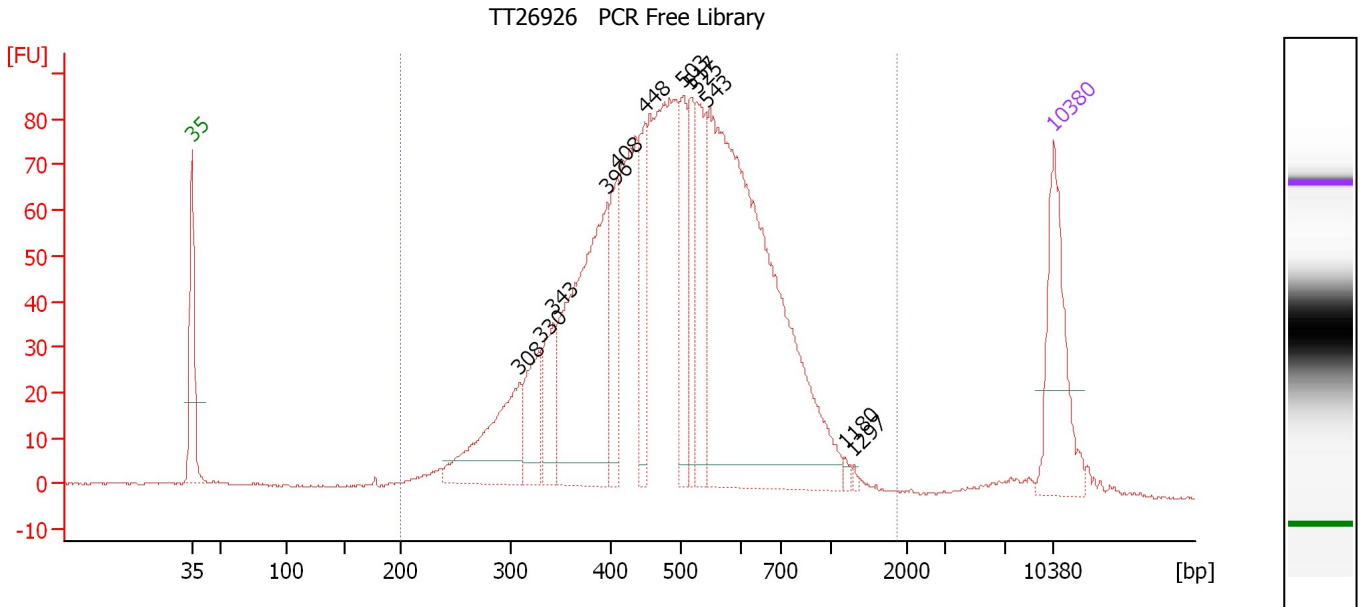

Overall Results for sample 4 : TT26926 PCR Free Library

Number of peaks found: 12 Corr. Area 1: 1,984.8
 Noise: 0.2

Peak table for sample 4 : TT26926 PCR Free Library

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	308	114.28	562.5	
3	330	57.70	265.3	
4	343	55.67	246.2	
5	396	251.50	961.7	
6	408	66.34	246.2	
7	448	59.80	202.1	
8	503	66.56	200.4	
9	517	56.41	165.5	
10	525	75.75	218.6	
11	543	546.18	1,523.7	
12	1,180	2.97	3.8	
13	1,297	1.91	2.2	
14	10,380	75.00	10.9	Upper Marker


Region table for sample 4 : TT26926 PCR Free Library

From [bp]	Average Size [bp]	To [bp]	Corr. Area	% of Total	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	510	1,849	1,984.8	97	32.7	1,820.45	6,143.5	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-10-28\2014-10-28_002.xad

Created: 10/28/2014 2:22:26 PM
 Modified: 10/28/2014 3:03:27 PM

Electropherogram Summary Continued ...

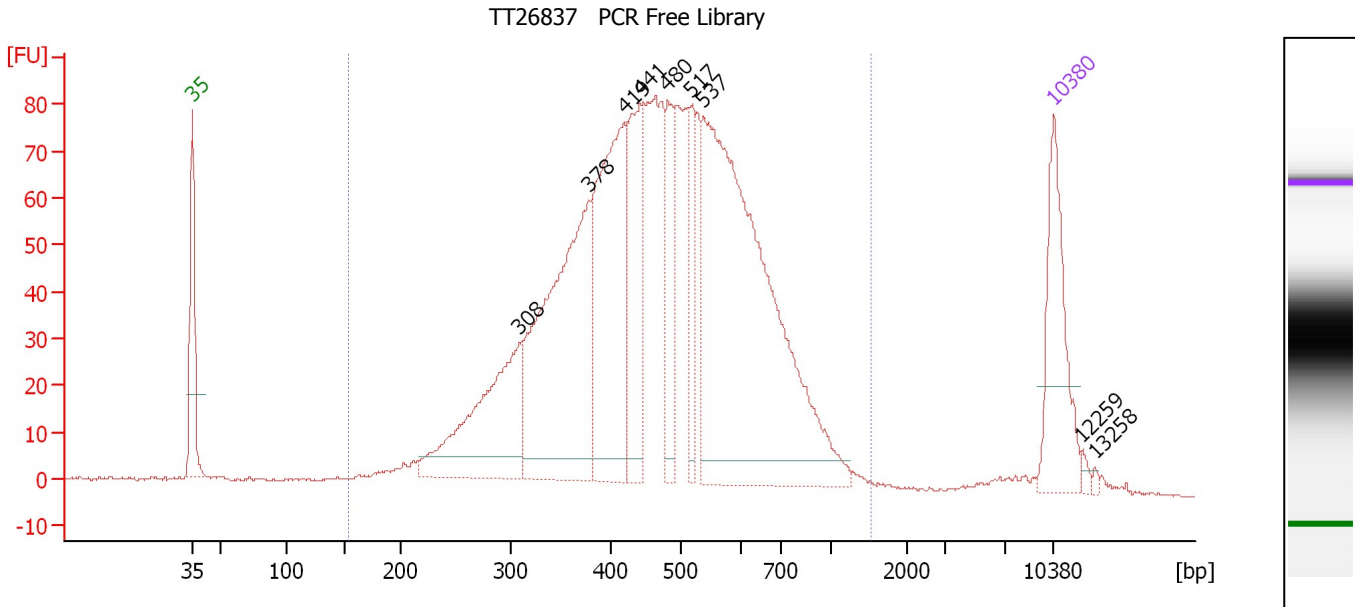

Overall Results for sample 5 : TT26837 PCR Free Library

Number of peaks found: 9 Corr. Area 1: 2,080.6
 Noise: 0.2

Peak table for sample 5 : TT26837 PCR Free Library

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	308	183.20	901.1	
3	378	307.61	1,232.8	
4	419	233.69	845.5	
5	441	110.20	378.2	
6	480	67.38	212.5	
7	517	52.03	152.4	
8	537	504.72	1,422.8	
9	10,380	75.00	10.9	Upper Marker
10	12,259	0.00	0.0	
11	13,258	0.00	0.0	


Region table for sample 5 : TT26837 PCR Free Library

From [bp]	Average Size [bp]	To [bp]	Corr. Area	% of Total	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
153	484	1,519	2,080.6	97	32.6	1,871.82	6,754.1	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-10-28\2014-10-28_002.xad

Created: 10/28/2014 2:22:26 PM
 Modified: 10/28/2014 3:03:27 PM

Electropherogram Summary Continued ...

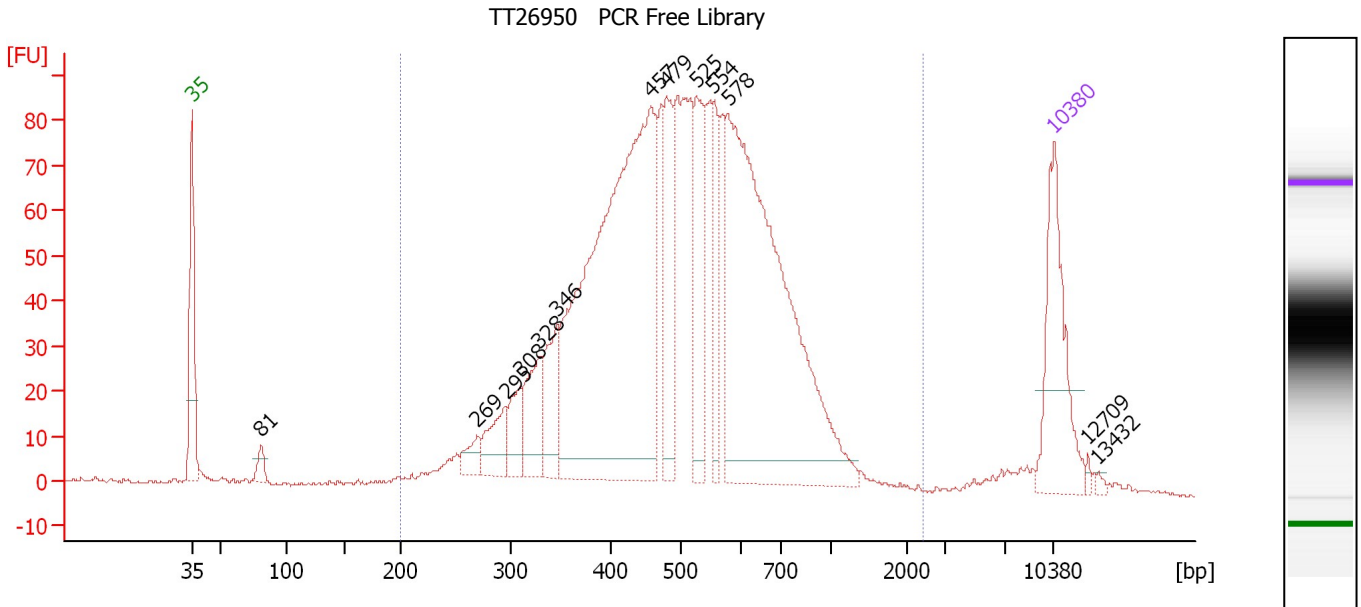

Overall Results for sample 6 : TT26950 PCR Free Library

Number of peaks found: 13 Corr. Area 1: 2,038.1
 Noise: 0.4

Peak table for sample 6 : TT26950 PCR Free Library

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	81	13.49	253.4	
3	269	18.42	103.7	
4	295	37.77	193.9	
5	308	32.41	159.2	
6	328	51.13	236.4	
7	346	53.21	232.9	
8	457	525.84	1,744.6	
9	479	78.51	248.5	
10	525	82.79	238.9	
11	554	50.68	138.6	
12	578	428.24	1,122.1	
13	10,380	75.00	10.9	Upper Marker
14	12,709	0.00	0.0	
15	13,432	0.00	0.0	


Region table for sample 6 : TT26950 PCR Free Library

From [bp]	Average Size [bp]	To [bp]	Corr. Area	% of Total	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	524	2,406	2,038.1	96	36.4	1,778.74	5,907.7	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-10-28\2014-10-28_002.xad

Created: 10/28/2014 2:22:26 PM
 Modified: 10/28/2014 3:03:27 PM

Electropherogram Summary Continued ...

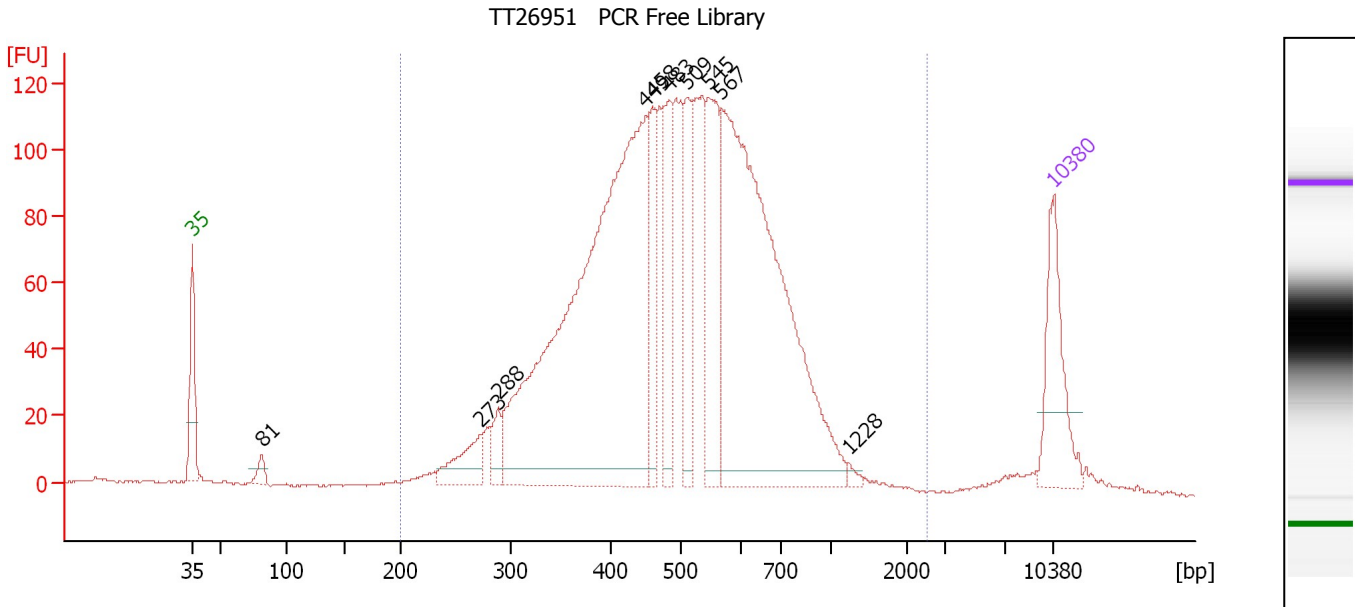

Overall Results for sample 7 : TT26951 PCR Free Library

Number of peaks found: 10 Corr. Area 1: 2,753.0
 Noise: 0.3

Peak table for sample 7 : TT26951 PCR Free Library

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	81	16.47	306.9	
3	273	54.55	302.9	
4	288	28.14	147.9	
5	449	838.48	2,827.3	
6	458	83.58	276.2	
7	483	107.16	336.0	
8	509	93.78	279.4	
9	545	137.79	383.2	
10	567	602.61	1,609.5	
11	1,228	4.83	6.0	
12	10,380	75.00	10.9	Upper Marker


Region table for sample 7 : TT26951 PCR Free Library

From [bp]	Average Size [bp]	To [bp]	Corr. Area	% of Total	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	519	2,514	2,753.0	97	35.3	2,384.88	7,938.3	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-10-28\2014-10-28_002.xad

Created: 10/28/2014 2:22:26 PM
 Modified: 10/28/2014 3:03:27 PM

Electropherogram Summary Continued ...

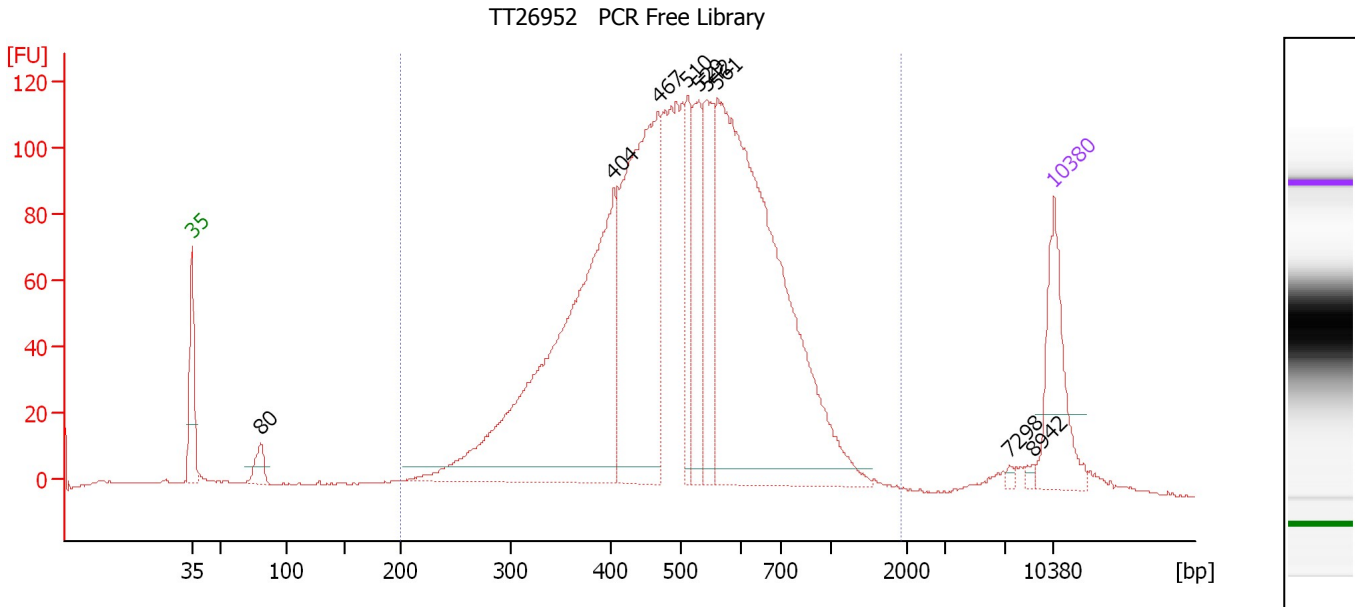

Overall Results for sample 8 : TT26952 PCR Free Library

Number of peaks found: 9 Corr. Area 1: 2,266.6
 Noise: 0.2

Peak table for sample 8 : TT26952 PCR Free Library

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	80	25.55	483.5	
3	404	551.41	2,067.0	
4	467	386.06	1,253.1	
5	510	72.90	216.5	
6	529	97.61	279.6	
7	542	101.41	283.6	
8	561	670.38	1,811.9	
9	7,298	2.89	0.6	
10	8,942	3.42	0.6	
11	10,380	75.00	10.9	Upper Marker


Region table for sample 8 : TT26952 PCR Free Library

From [bp]	Average Size [bp]	To [bp]	Corr. Area	% of Total	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	525	1,905	2,266.6	99	27.0	1,868.89	5,901.5	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-10-28\2014-10-28_002.xad

Created: 10/28/2014 2:22:26 PM
 Modified: 10/28/2014 3:03:27 PM

Electropherogram Summary Continued ...

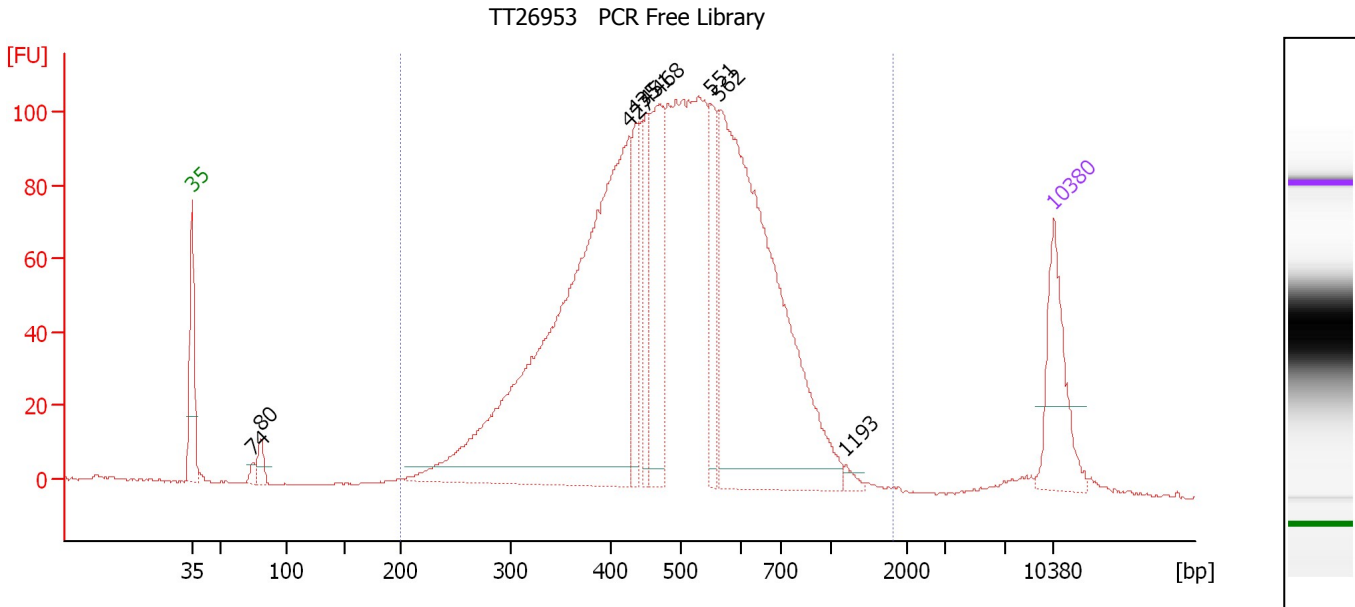

Overall Results for sample 9 : TT26953 PCR Free Library

Number of peaks found: 9 Corr. Area 1: 2,459.9
 Noise: 0.1

Peak table for sample 9 : TT26953 PCR Free Library

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	74	8.69	177.6	
3	80	22.02	415.3	
4	427	819.39	2,909.1	
5	435	77.64	270.3	
6	451	79.07	265.6	
7	468	153.61	497.4	
8	551	83.78	230.6	
9	562	608.55	1,639.3	
10	1,193	6.49	8.2	
11	10,380	75.00	10.9	Upper Marker


Region table for sample 9 : TT26953 PCR Free Library

From [bp]	Average Size [bp]	To [bp]	Corr. Area	% of Total	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	505	1,807	2,459.9	97	31.7	2,431.51	8,245.3	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-10-28\2014-10-28_002.xad

Created: 10/28/2014 2:22:26 PM
 Modified: 10/28/2014 3:03:27 PM

Electropherogram Summary Continued ...

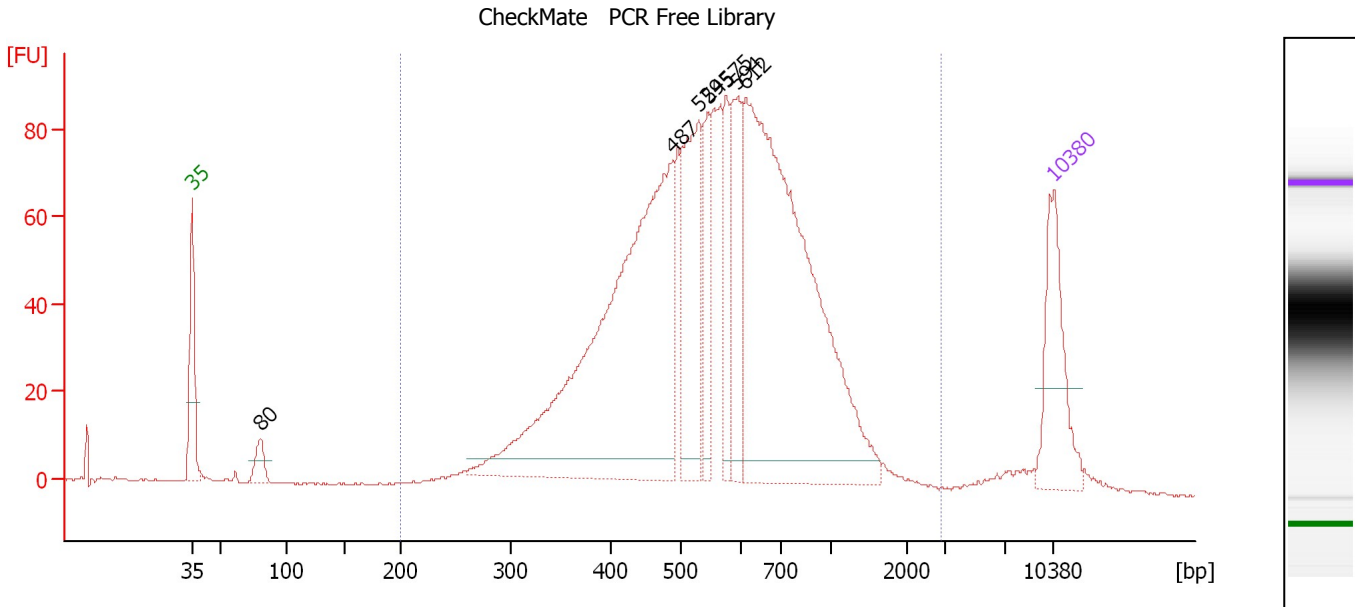

Overall Results for sample 10 : CheckMate PCR Free Library

Number of peaks found: 7 Corr. Area 1: 1,884.0
 Noise: 0.2

Peak table for sample 10 : CheckMate PCR Free Library

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	80	25.29	479.3	
3	487	596.73	1,857.2	
4	529	159.34	456.2	
5	545	59.30	164.8	
6	575	59.13	155.8	
7	594	89.12	227.3	
8	612	569.10	1,408.9	
9	10,380	75.00	10.9	Upper Marker

Region table for sample 10 : CheckMate PCR Free Library


From [bp]	Average Size [bp]	To [bp]	Corr. Area	% of Total	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	608	2,867	1,884.0	96	42.7	1,825.03	5,374.7	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-10-28\2014-10-28_002.xad

Created: 10/28/2014 2:22:26 PM
 Modified: 10/28/2014 3:03:27 PM

Electropherogram Summary Continued ...

MG3FLib 10/24/14 (1:5)

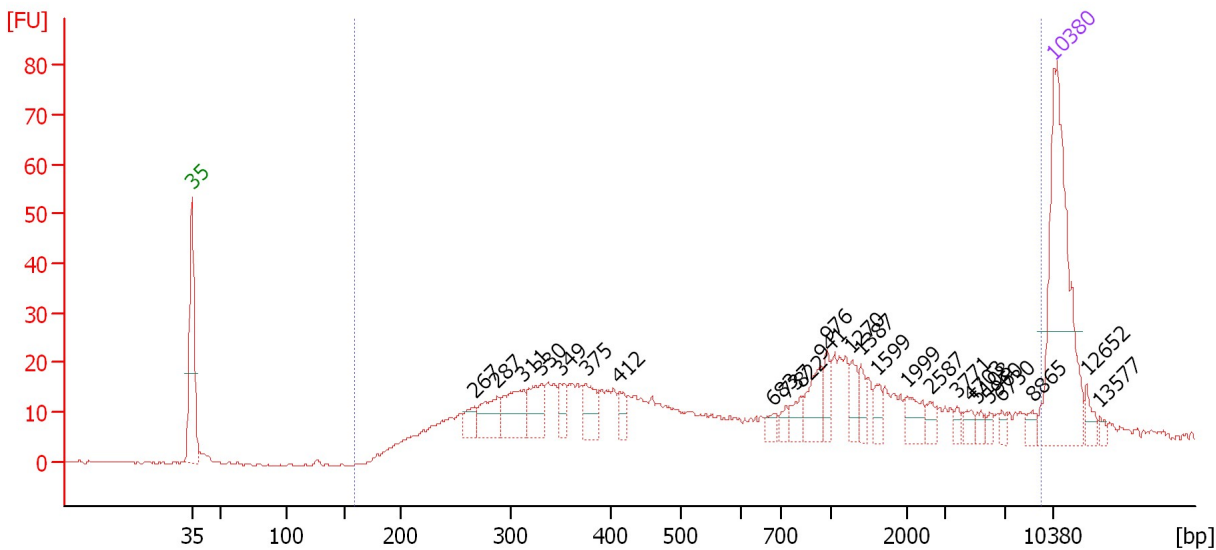

Overall Results for sample 11 : MG3FLib 10/24/14 (1:5)

Number of peaks found: 25 Corr. Area 1: 642.1
 Noise: 0.2

Peak table for sample 11 : MG3FLib 10/24/14 (1:5)

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	267	8.85	50.3	
3	287	20.38	107.5	
4	311	24.48	119.1	
5	330	20.07	92.1	
6	349	10.14	44.0	
7	375	15.68	63.3	
8	412	7.49	27.5	
9	683	4.87	10.8	
10	737	4.62	9.5	
11	822	7.38	13.6	
12	941	15.52	25.0	
13	976	8.86	13.8	
14	1,270	8.40	10.0	
15	1,387	6.55	7.1	
16	1,599	5.73	5.4	
17	1,999	9.47	7.2	
18	2,587	4.15	2.4	
19	3,771	2.74	1.1	
20	4,703	3.76	1.2	
21	5,108	3.19	0.9	
22	5,960	2.38	0.6	
23	6,730	2.51	0.6	
24	8,865	3.45	0.6	
25	10,380	75.00	10.9	Upper Marker
26	12,652	0.00	0.0	


Assay Class: High Sensitivity DNA Assay
Data Path: C:\...ents and Settings\Bioanalyzer\2014-10-28\2014-10-28_002.xad

Created: 10/28/2014 2:22:26 PM
Modified: 10/28/2014 3:03:27 PM

Electropherogram Summary Continued ...**... Peak table for sample 11 : MG3FLib 10/24/14 (1:5)**

Peak	Size [bp]	Conc. [pg/ μ l]	Molarity [pmol/l]	Observations
27	13,577	0.00	0.0	


Region table for sample 11 : MG3FLib 10/24/14 (1:5)

From [bp]	Average Size [bp]	To [bp]	Corr. Area	% of Total	Size distribution in CV [%]	Conc. [pg/ μ l]	Molarity [pmol/l]	Color
159	1,342	9,444	642.1	94	100.0	545.76	1,864.6	

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...ents and Settings\Bioanalyzer\2014-10-28\2014-10-28_002.xad

Created: 10/28/2014 2:22:26 PM
Modified: 10/28/2014 3:03:27 PM

Gel Image

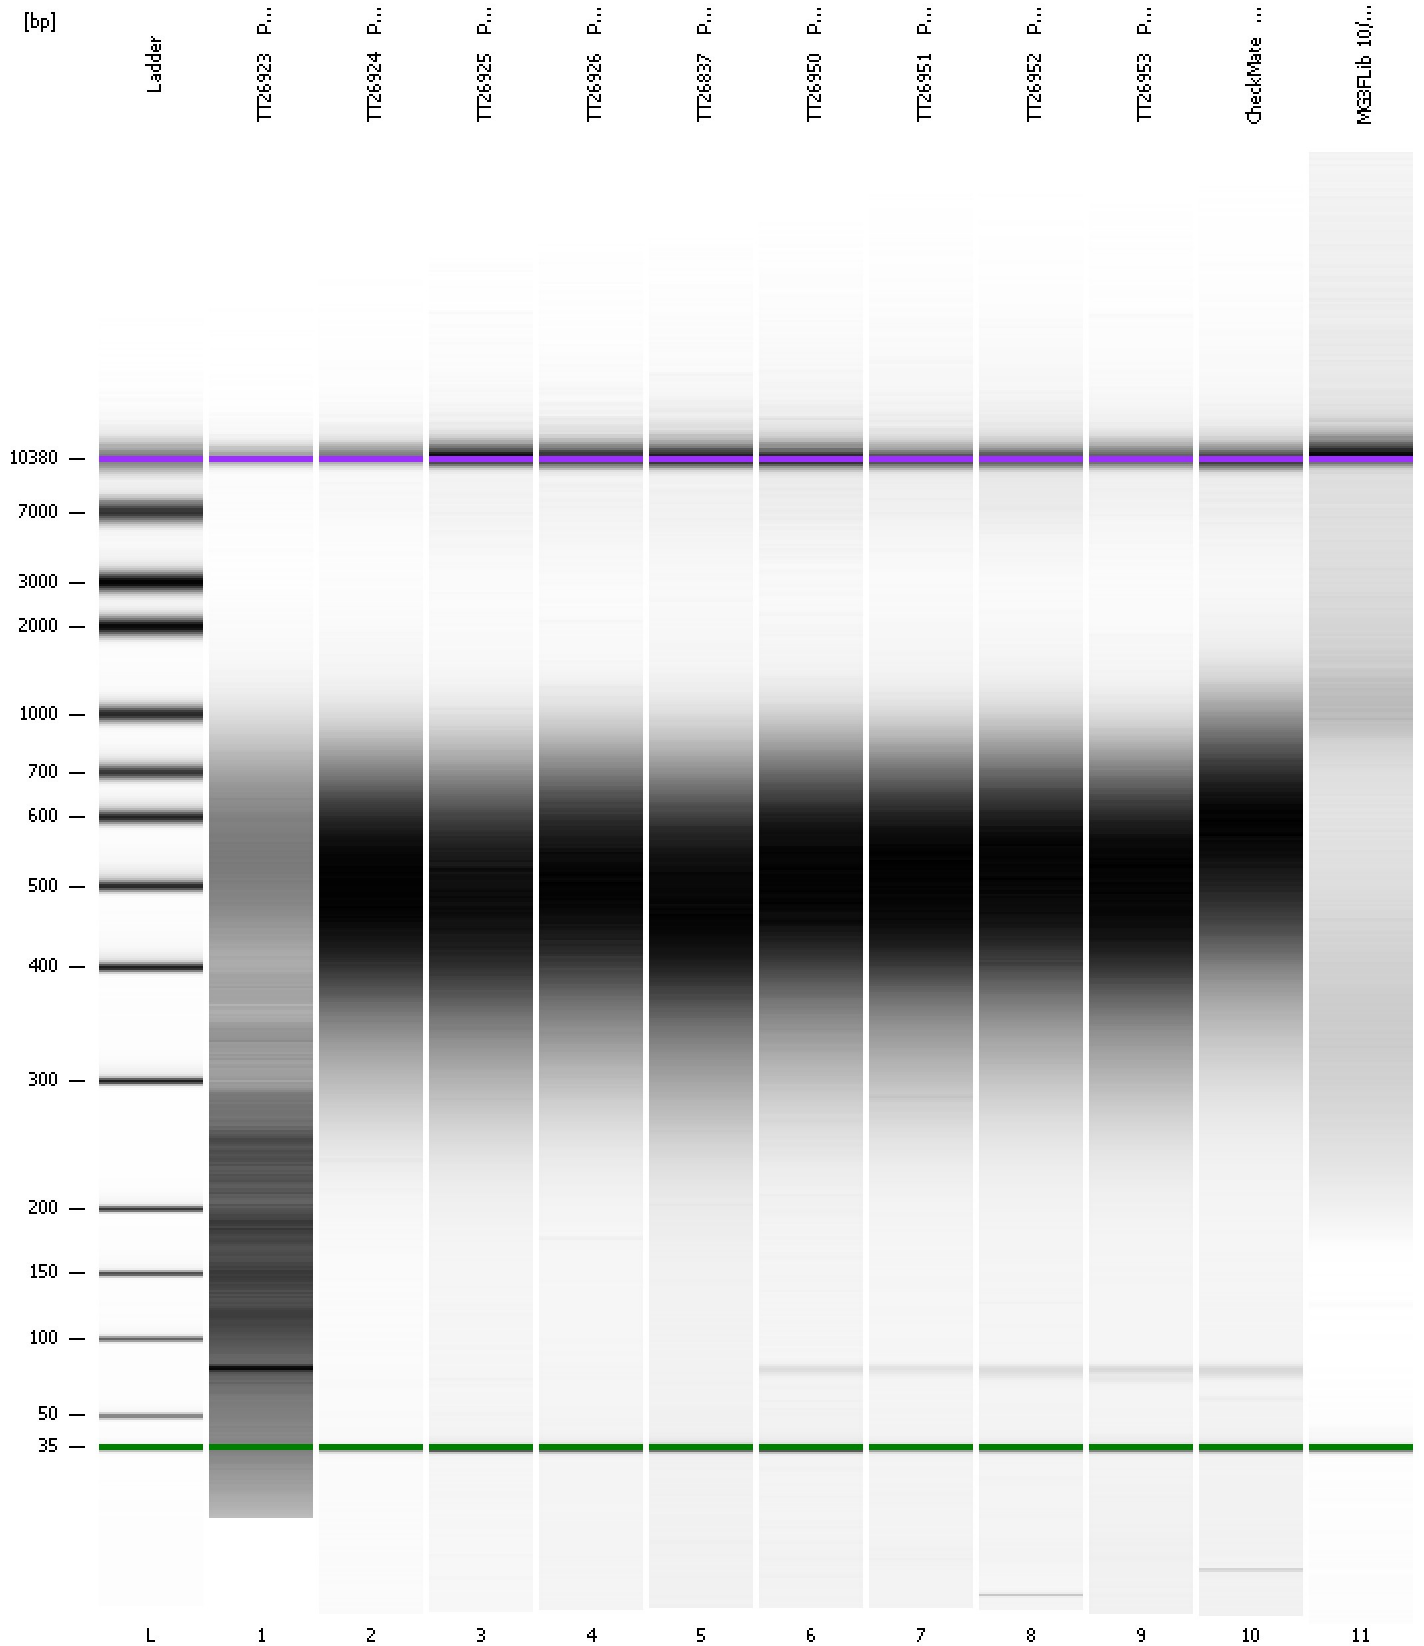

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...ents and Settings\Bioanalyzer\2014-10-28\2014-10-28_002.xad

Created: 10/28/2014 2:22:26 PM
 Modified: 10/28/2014 3:03:27 PM

Run Logbook

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 12)		Instrument	Run		10/28/2014 3:02:53 PM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Run started on port 1 (File: C:\Documents and Settings\Bioanalyzer\2014-10-28\2014-10-28_002.xad)		Instrument	Run		10/28/2014 2:22:32 PM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Product Number : G2938B		Instrument	Run		10/28/2014 2:22:32 PM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Name :		Instrument	Run		10/28/2014 2:22:32 PM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Vendor : Agilent Technologies		Instrument	Run		10/28/2014 2:22:32 PM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Serial# : DE13701086		Instrument	Run		10/28/2014 2:22:32 PM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Firmware : C.01.069		Instrument	Run		10/28/2014 2:22:32 PM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1
Cartridge : Electrode		Instrument	Run		10/28/2014 2:22:32 PM	(GMT --07:00) Pacific Standard Time	UC Davis	D8XSMGH1